

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 22:02
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 08:03:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.344	3.594	32263292	58243537	22.696	22.746
2)	SA Decachlor...	10.091	8.567	32121060	27610336	26.187	24.494
Target Compounds							
8)	L2 AR-1221-1	4.561	3.806	797610	908434	46.788	27.065 #
9)	L2 AR-1221-2	4.649	3.891	772582	1489286	60.433	58.015
10)	L2 AR-1221-3	4.721	3.965	1183485	1947372	29.906	26.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 22:02
Operator : YP\AJ
Sample : N3214-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 08:03:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

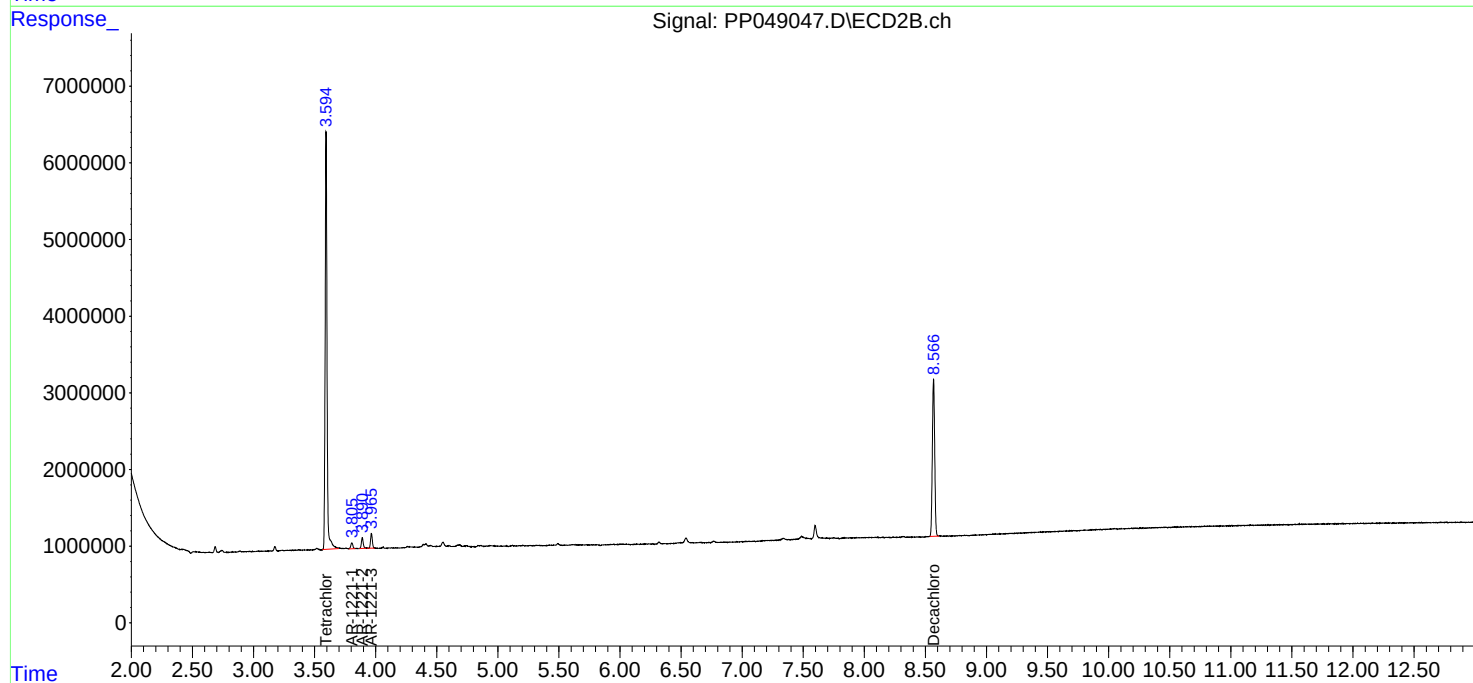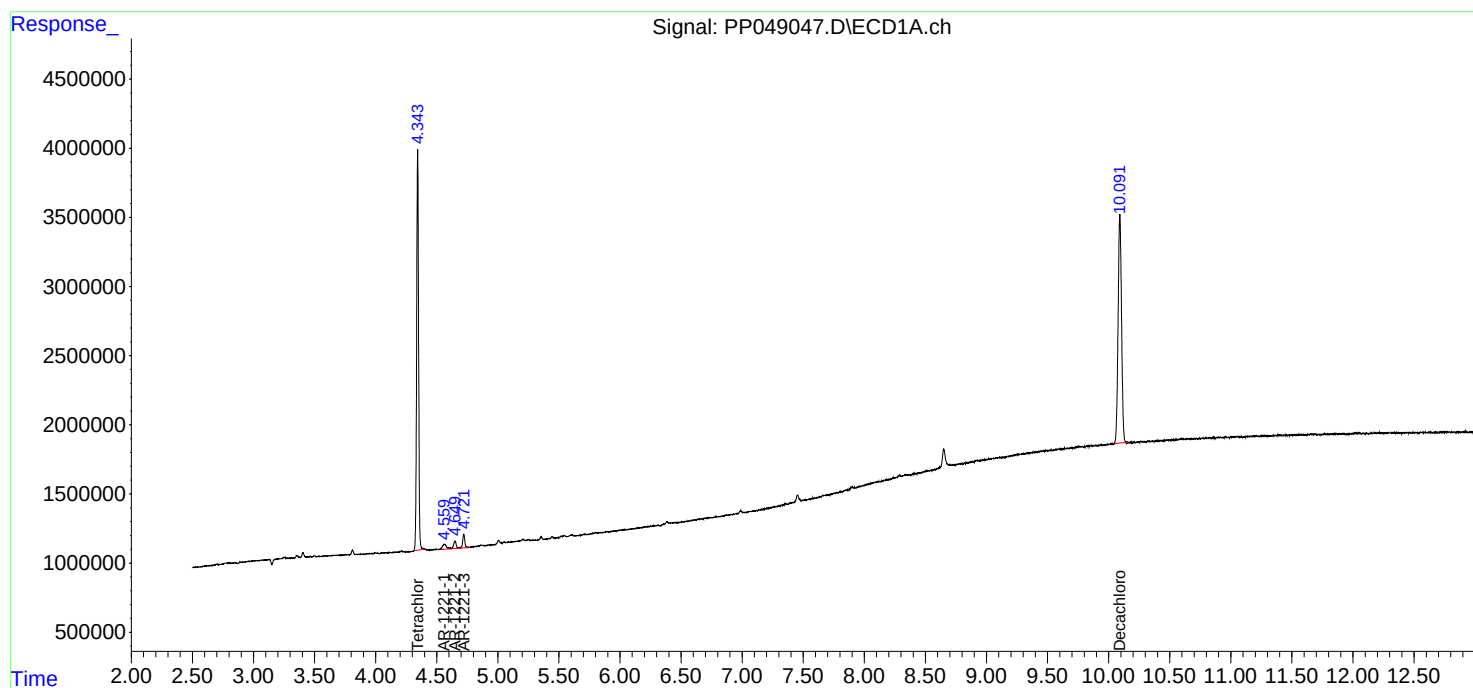


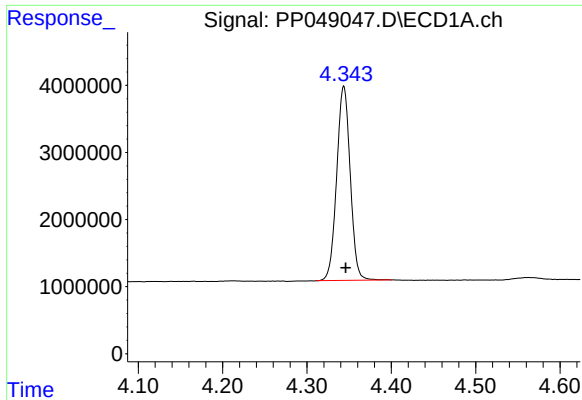

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 32263292
Conc: 22.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

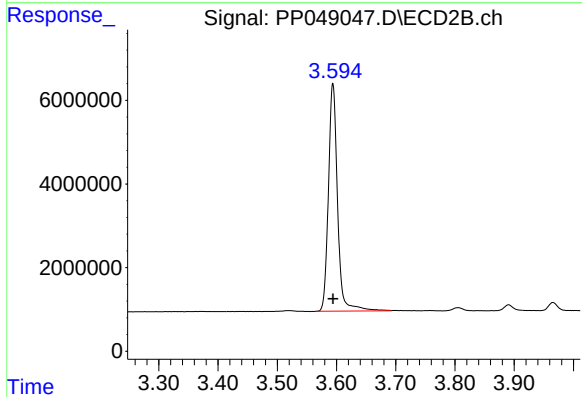


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 58243537
Conc: 22.75 ng/ml

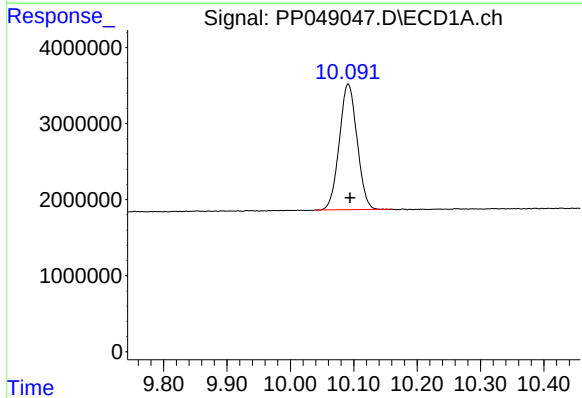


#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: -0.003 min
Response: 32121060
Conc: 26.19 ng/ml

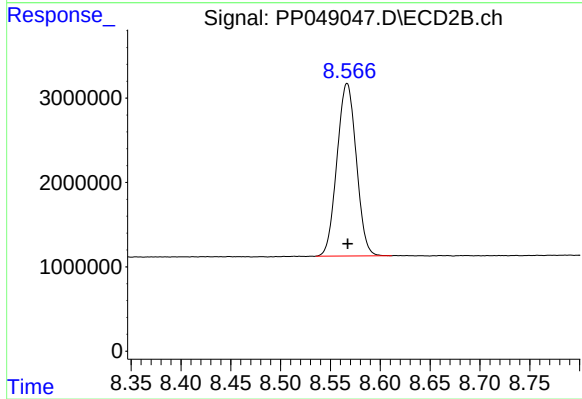

#2 Decachlorobiphenyl


R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 27610336
Conc: 24.49 ng/ml

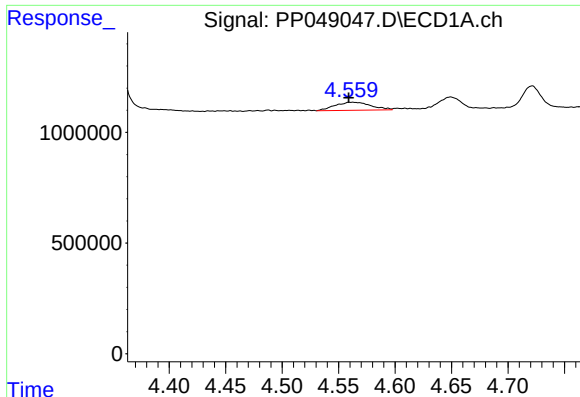

#8 AR-1221-1


R.T.: 4.561 min
Delta R.T.: 0.002 min
Response: 797610
Conc: 46.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

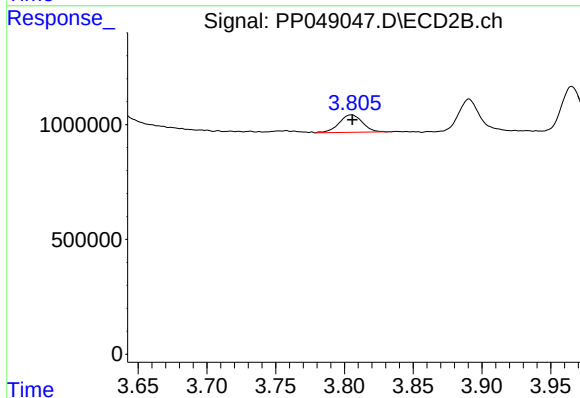


#8 AR-1221-1

R.T.: 3.806 min
Delta R.T.: 0.000 min
Response: 908434
Conc: 27.06 ng/ml

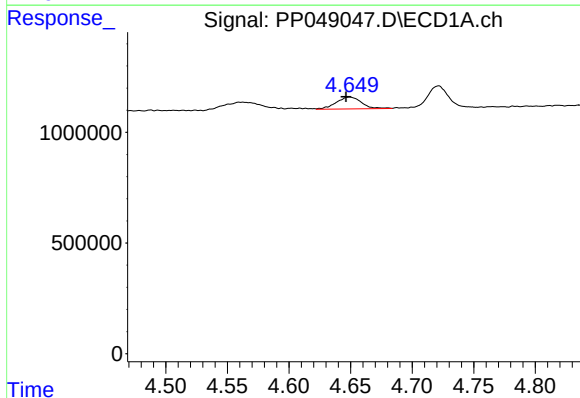


#9 AR-1221-2

R.T.: 4.649 min
Delta R.T.: 0.003 min
Response: 772582
Conc: 60.43 ng/ml

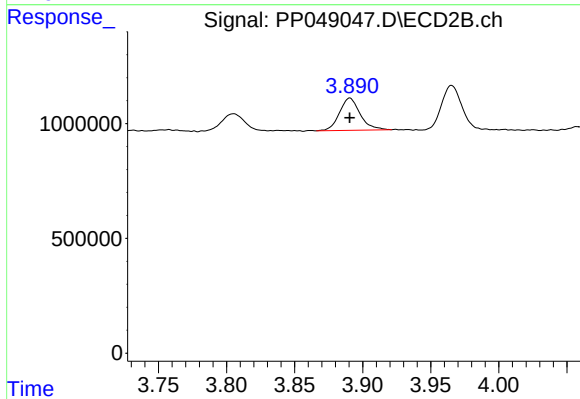

#9 AR-1221-2


R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 1489286
Conc: 58.01 ng/ml

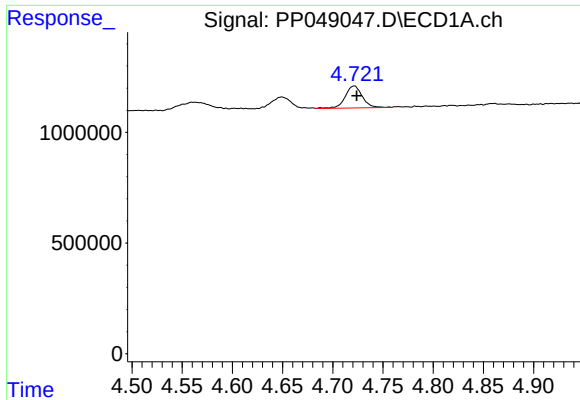

#10 AR-1221-3

R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 1183485
Conc: 29.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

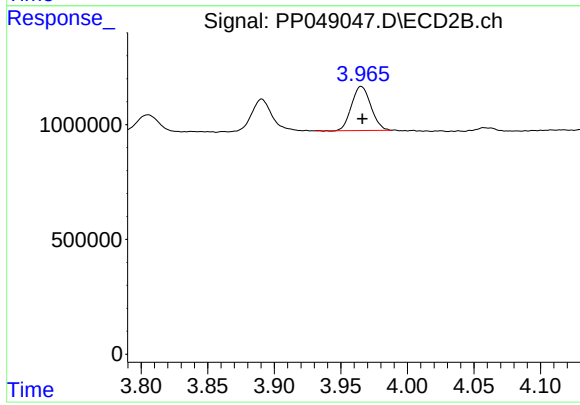

#10 AR-1221-3

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 1947372
Conc: 26.48 ng/ml