

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 22:19
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 08:05:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.594	29017414	52518101	20.412	20.510
2) SA Decachlor...	10.092	8.566	29124912	24999304	23.744	22.178
Target Compounds						
11) L3 AR-1232-1	4.722	3.965	1312222	2382343	34.512	34.292
12) L3 AR-1232-2	5.251	4.688	756922	2188095	40.044	34.057
13) L3 AR-1232-3	5.544	4.863	1219828	1114448	33.003	31.655
14) L3 AR-1232-4	5.707	4.945	559052	1113051	29.247	35.172
15) L3 AR-1232-5	5.794	5.116	625739	1282134	40.124	35.813



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 22:19
Operator : YP\AJ
Sample : N3214-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 08:05:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

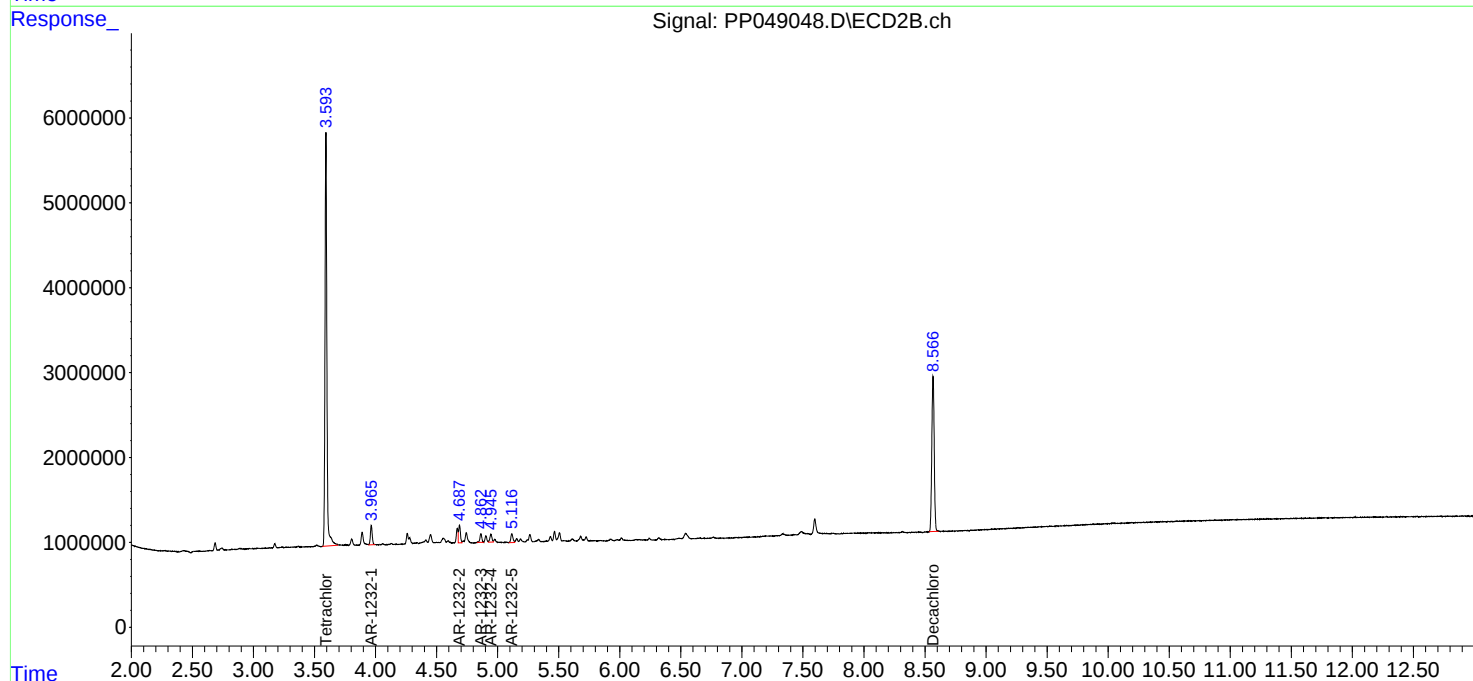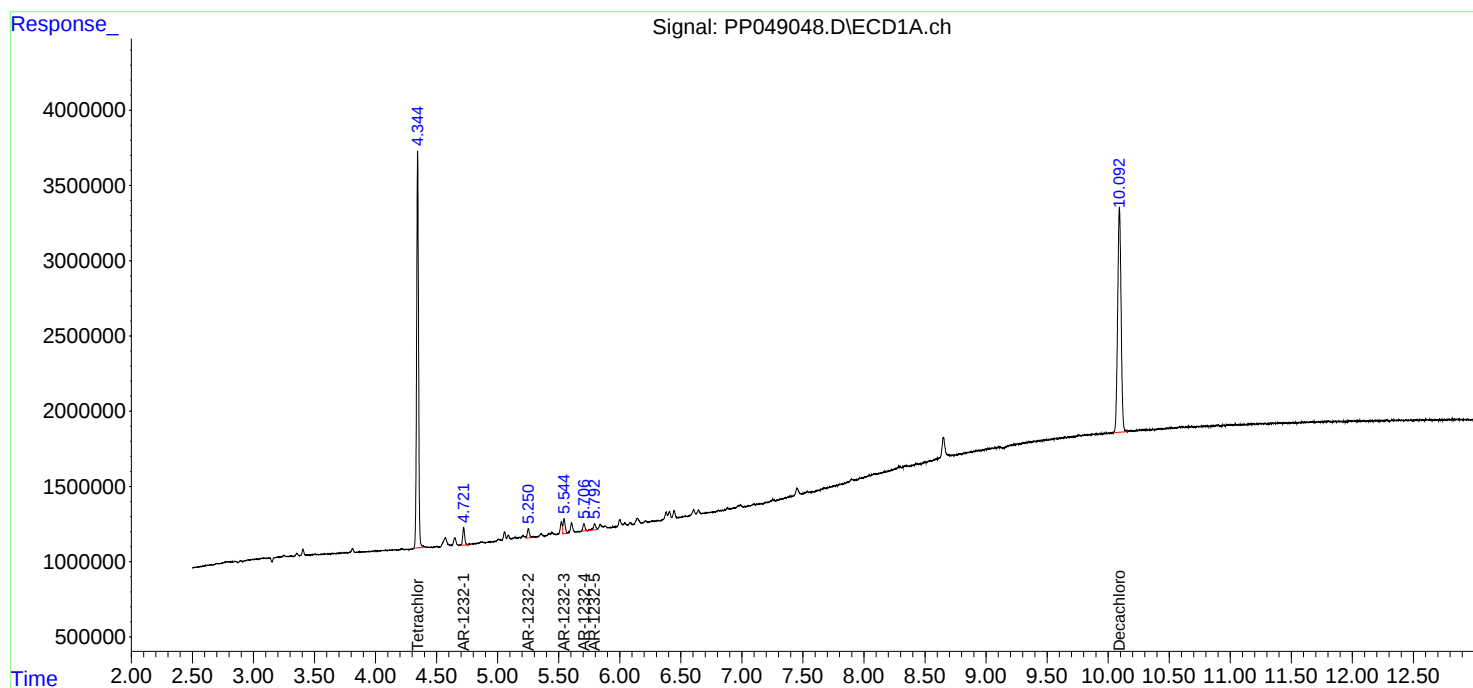


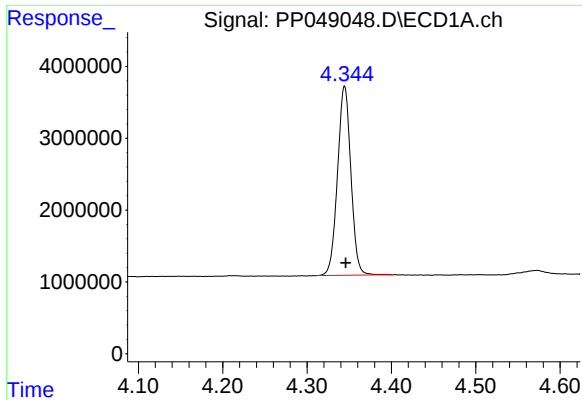

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: -0.001 min
Response: 29017414
Conc: 20.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

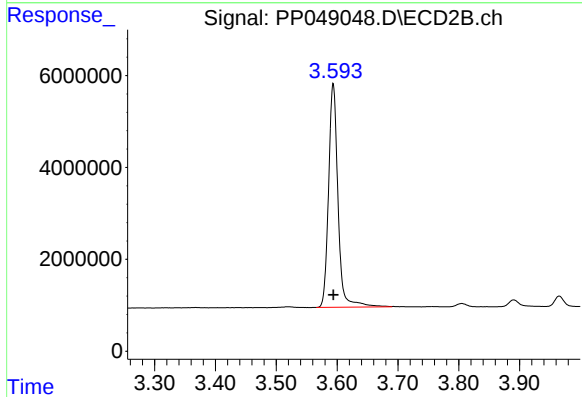


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 52518101
Conc: 20.51 ng/ml

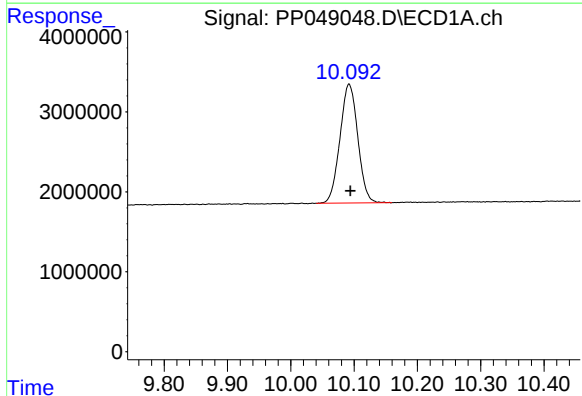


#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 29124912
Conc: 23.74 ng/ml

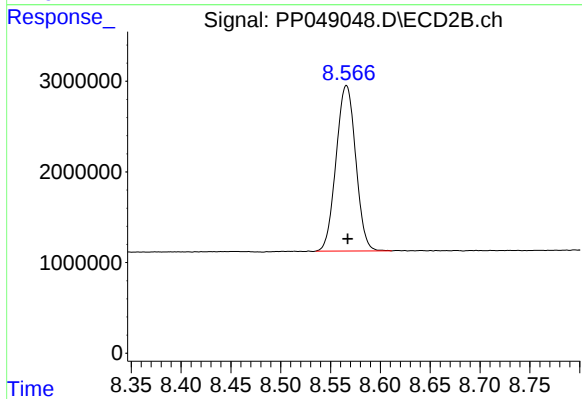

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.001 min
Response: 24999304
Conc: 22.18 ng/ml

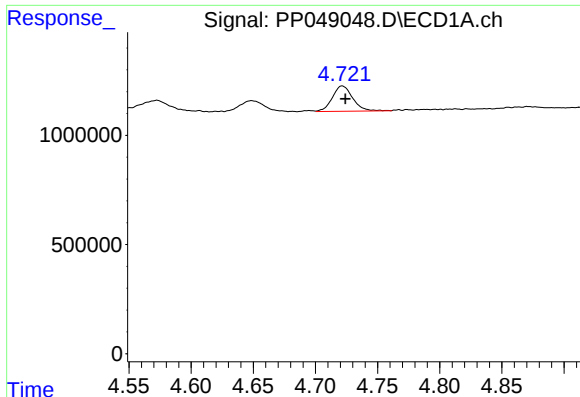

#11 AR-1232-1


R.T.: 4.722 min
Delta R.T.: -0.002 min
Response: 1312222
Conc: 34.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

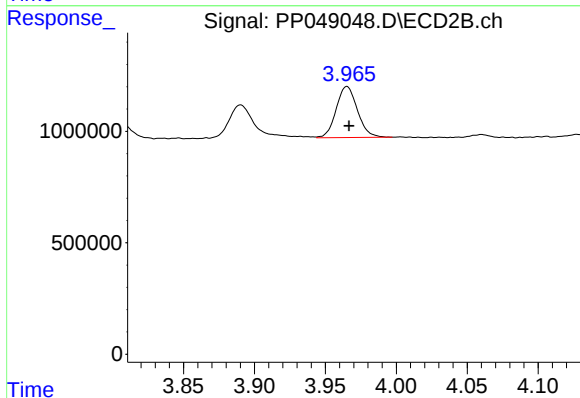


#11 AR-1232-1

R.T.: 3.965 min
Delta R.T.: -0.001 min
Response: 2382343
Conc: 34.29 ng/ml

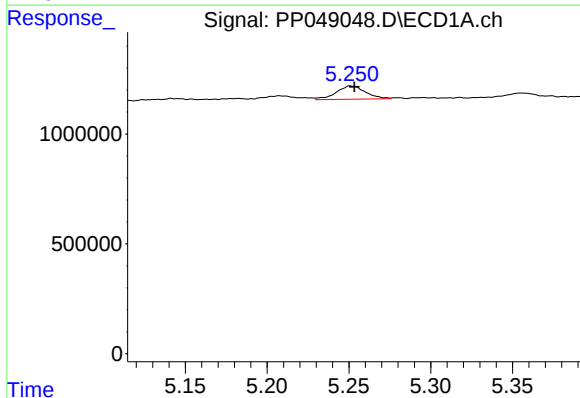


#12 AR-1232-2

R.T.: 5.251 min
Delta R.T.: -0.002 min
Response: 756922
Conc: 40.04 ng/ml

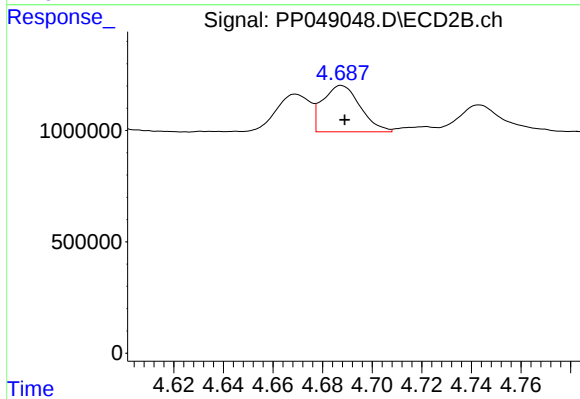

#12 AR-1232-2


R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 2188095
Conc: 34.06 ng/ml

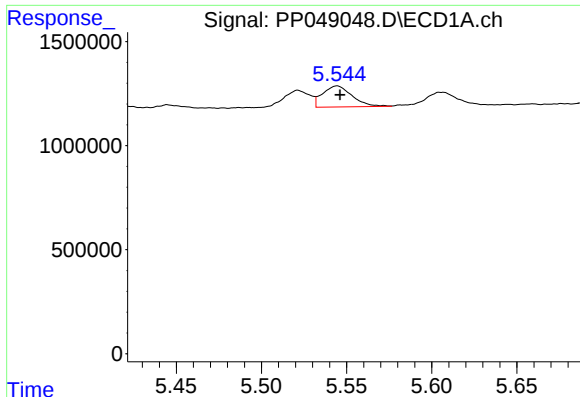

#13 AR-1232-3


R.T.: 5.544 min
Delta R.T.: -0.002 min
Response: 1219828
Conc: 33.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

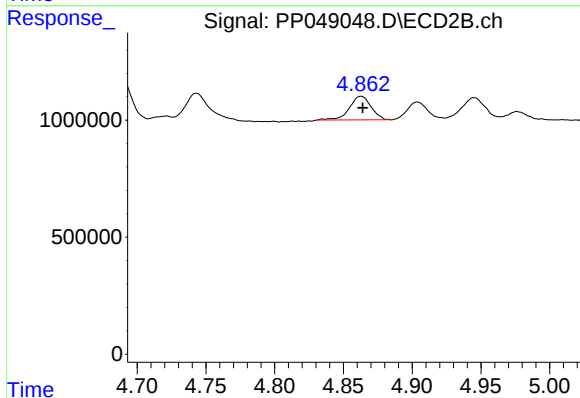


#13 AR-1232-3

R.T.: 4.863 min
Delta R.T.: -0.001 min
Response: 1114448
Conc: 31.66 ng/ml

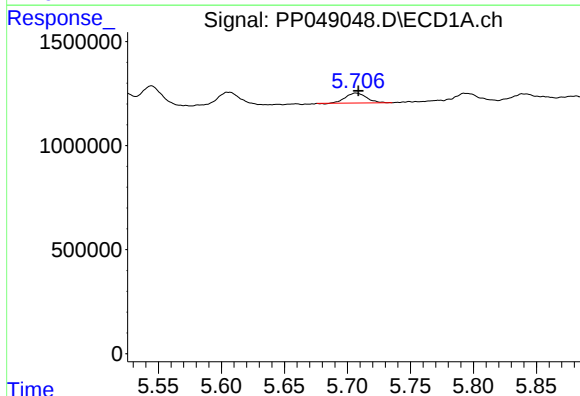


#14 AR-1232-4

R.T.: 5.707 min
Delta R.T.: -0.002 min
Response: 559052
Conc: 29.25 ng/ml

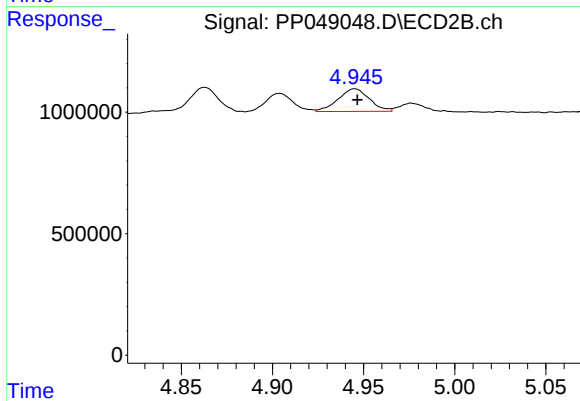

#14 AR-1232-4


R.T.: 4.945 min
Delta R.T.: -0.002 min
Response: 1113051
Conc: 35.17 ng/ml

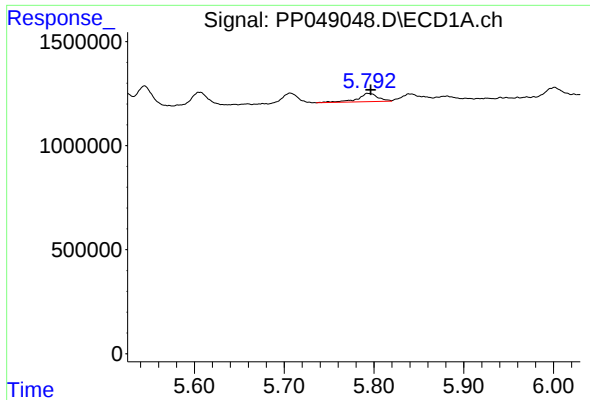

#15 AR-1232-5

R.T.: 5.794 min
Delta R.T.: -0.003 min
Response: 625739
Conc: 40.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

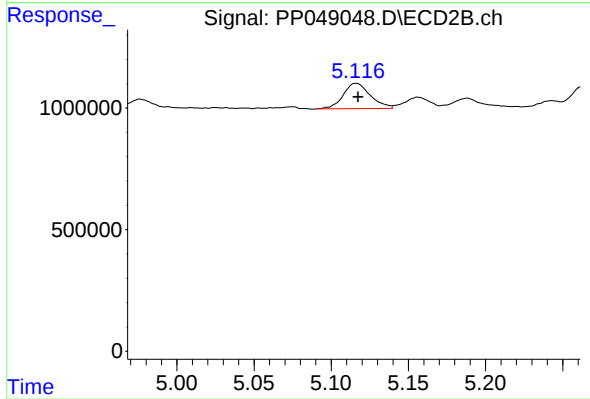

#15 AR-1232-5

R.T.: 5.116 min
Delta R.T.: -0.001 min
Response: 1282134
Conc: 35.81 ng/ml