

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 23:08
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 08:09:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.594	28124304	49217288	19.784	19.221
2) SA Decachlor...	10.092	8.566	27871473	23930361	22.723	21.230
Target Compounds						
26) L6 AR-1254-1	6.379	5.466	2388573	5376391	35.434	36.622
27) L6 AR-1254-2	6.597	5.612	3777451	4804062	40.276	38.507
28) L6 AR-1254-3	6.967	6.015	3919533	7107631	38.628	39.475
29) L6 AR-1254-4	7.255	6.243	2995740	4183380	39.930	38.667
30) L6 AR-1254-5	7.674	6.659	3183328	5518991	37.731	38.025



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 23:08
Operator : YP\AJ
Sample : N3214-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 08:09:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

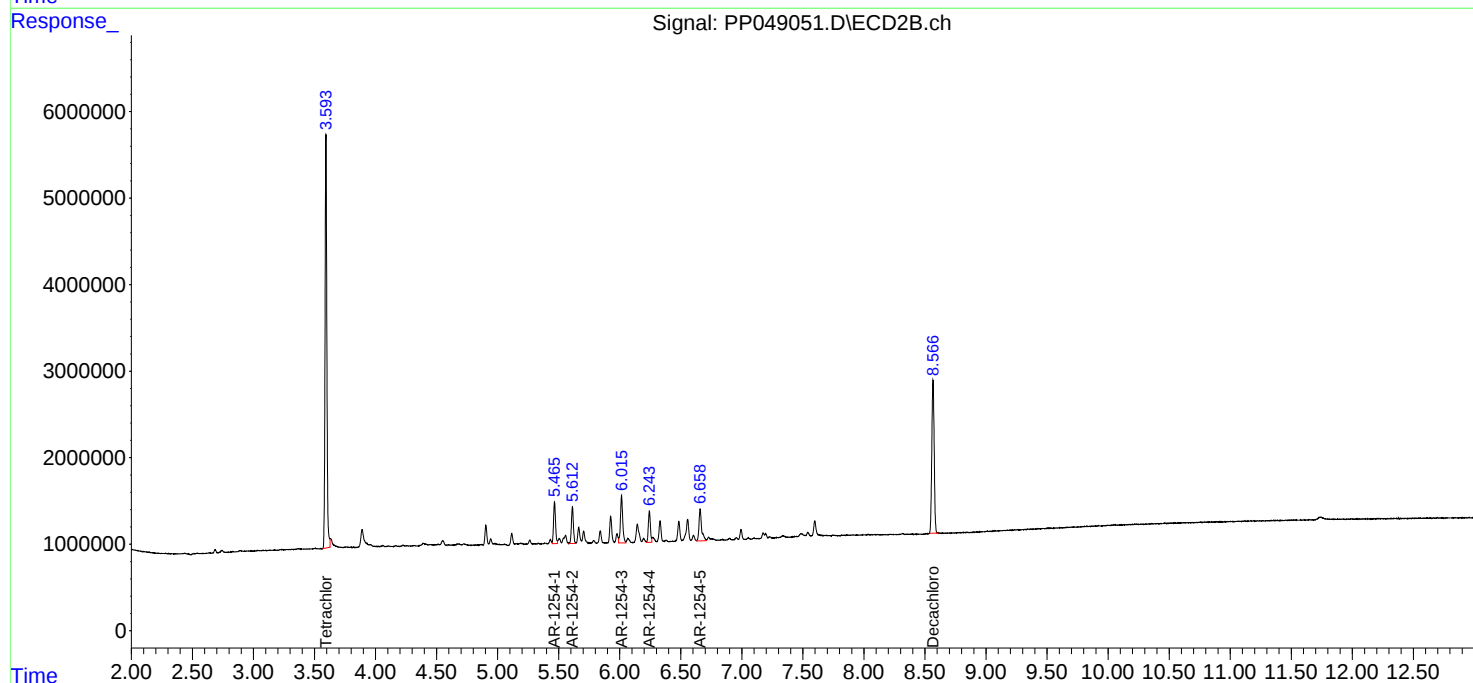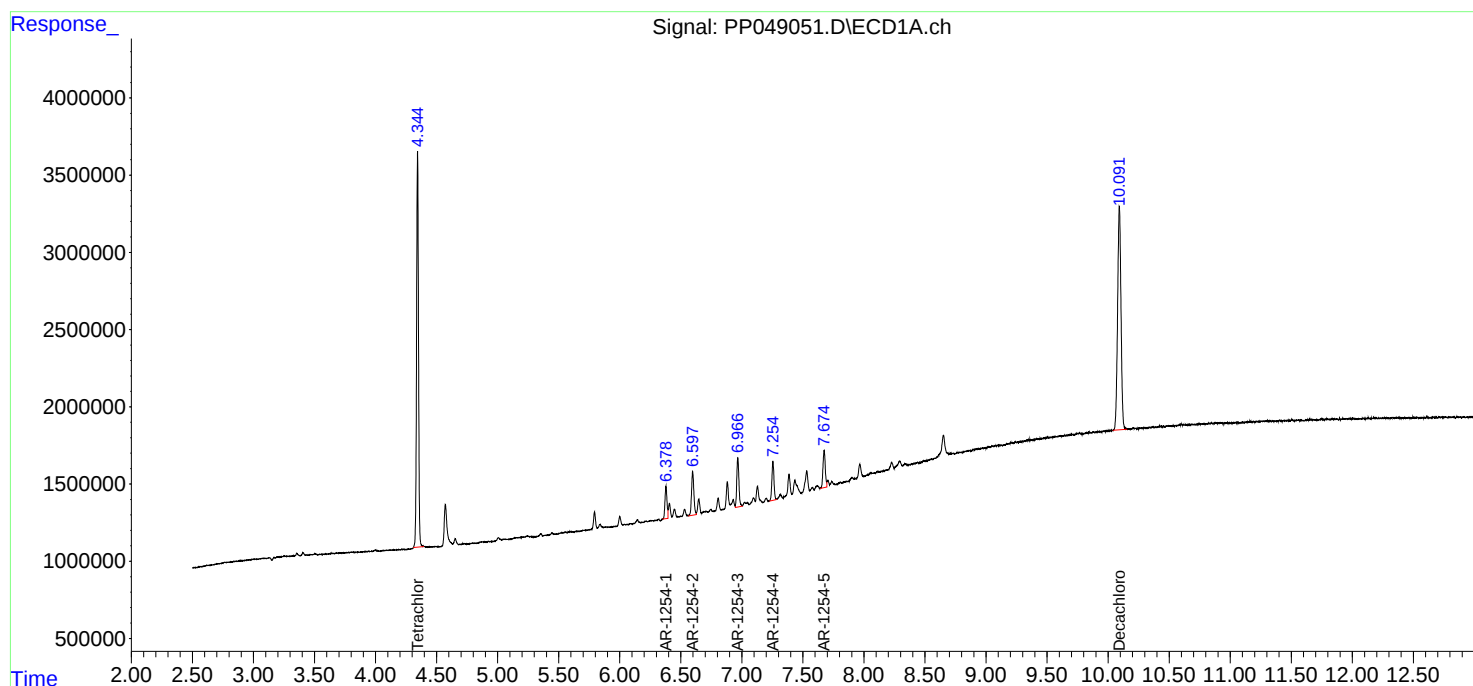


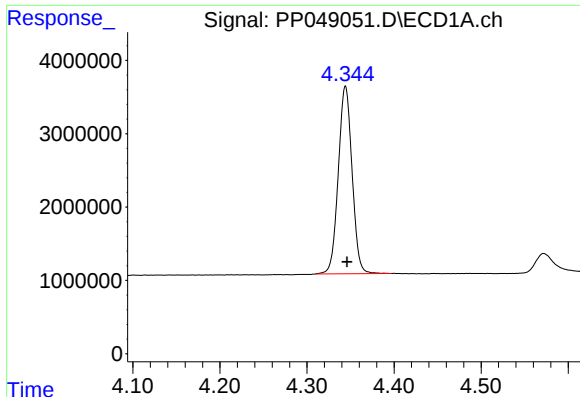

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 28124304
Conc: 19.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

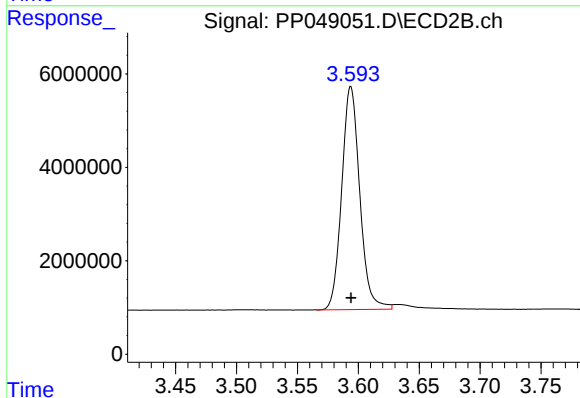


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 49217288
Conc: 19.22 ng/ml

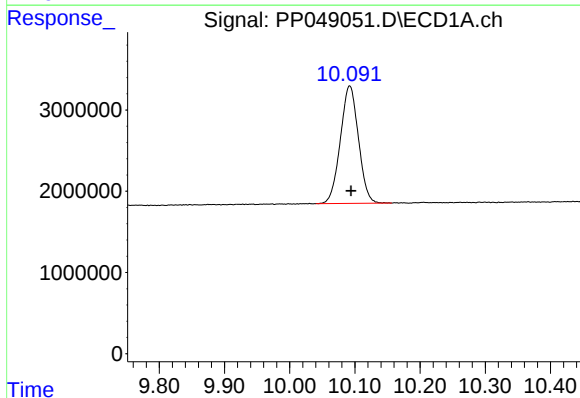


#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 27871473
Conc: 22.72 ng/ml

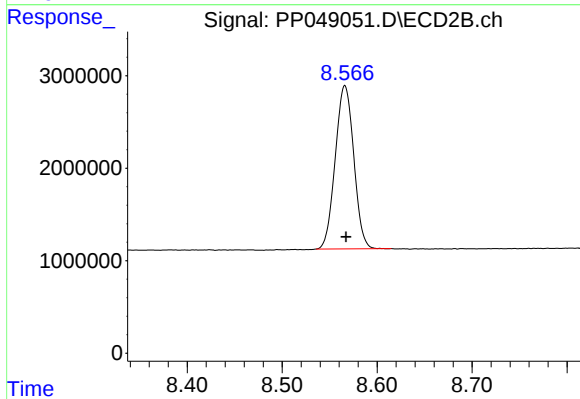

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.001 min
Response: 23930361
Conc: 21.23 ng/ml

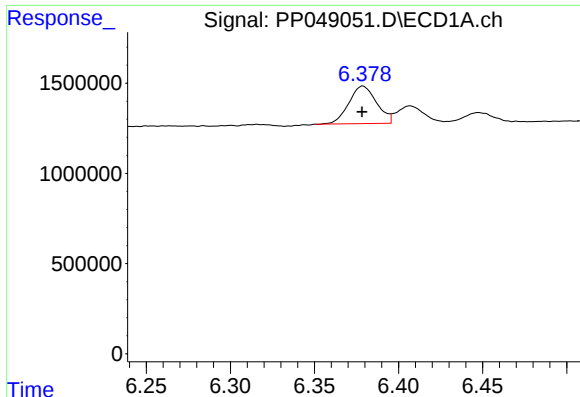

#26 AR-1254-1


R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 2388573
Conc: 35.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

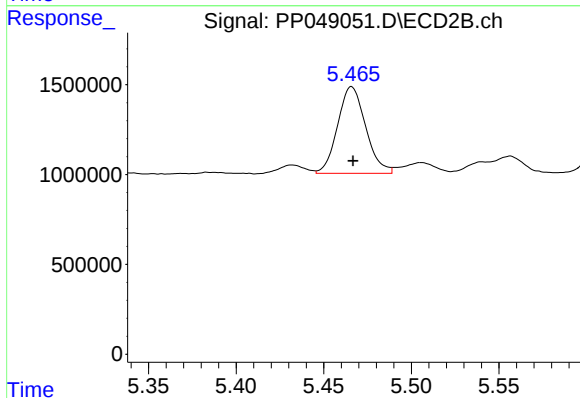


#26 AR-1254-1

R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 5376391
Conc: 36.62 ng/ml

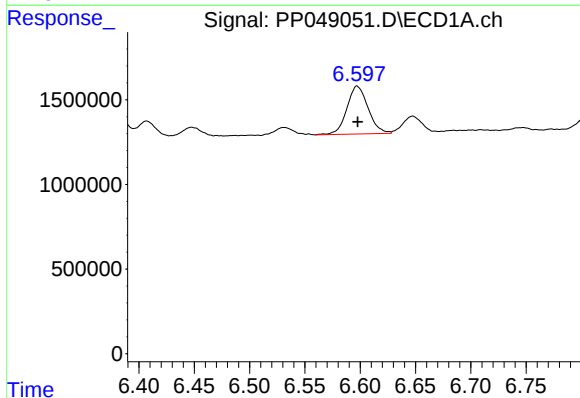


#27 AR-1254-2

R.T.: 6.597 min
Delta R.T.: 0.000 min
Response: 3777451
Conc: 40.28 ng/ml

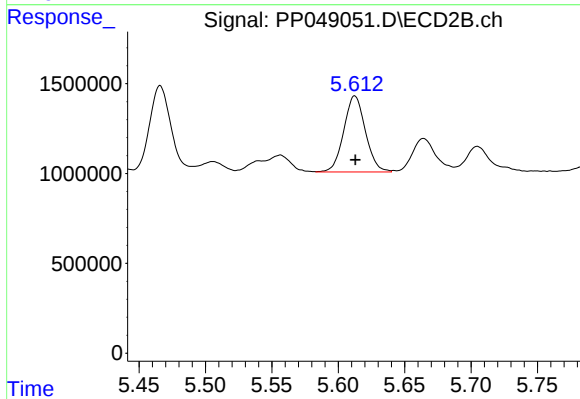

#27 AR-1254-2


R.T.: 5.612 min
Delta R.T.: 0.000 min
Response: 4804062
Conc: 38.51 ng/ml

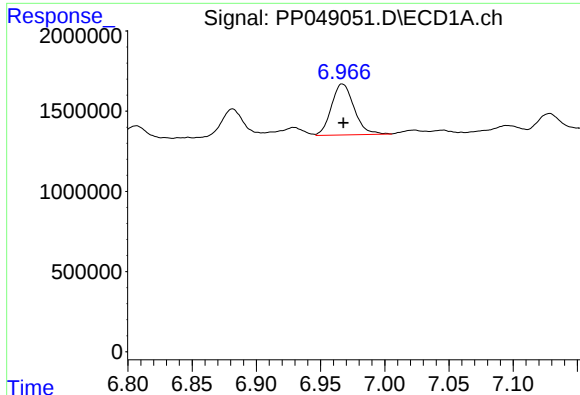

#28 AR-1254-3


R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 3919533
Conc: 38.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

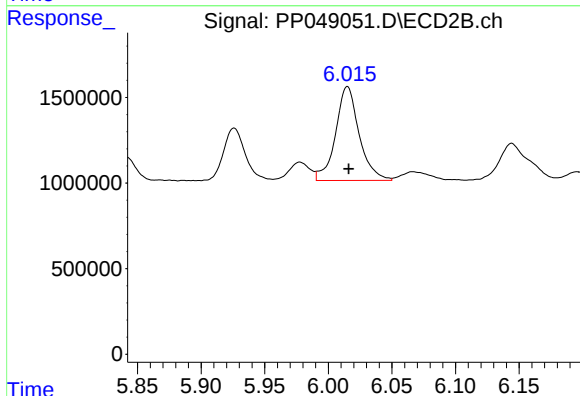


#28 AR-1254-3

R.T.: 6.015 min
Delta R.T.: 0.000 min
Response: 7107631
Conc: 39.47 ng/ml

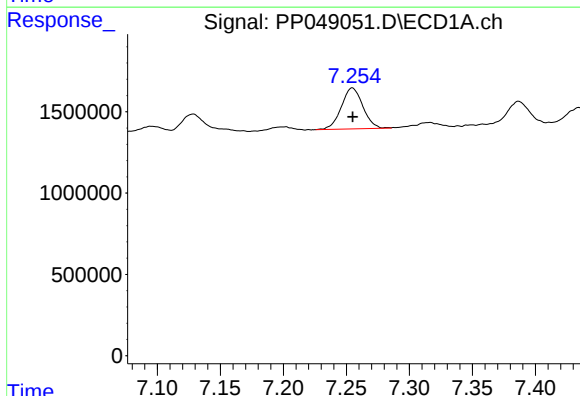


#29 AR-1254-4

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 2995740
Conc: 39.93 ng/ml

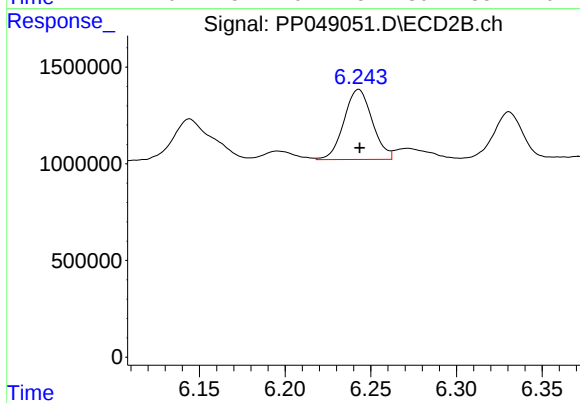

#29 AR-1254-4


R.T.: 6.243 min
Delta R.T.: 0.000 min
Response: 4183380
Conc: 38.67 ng/ml

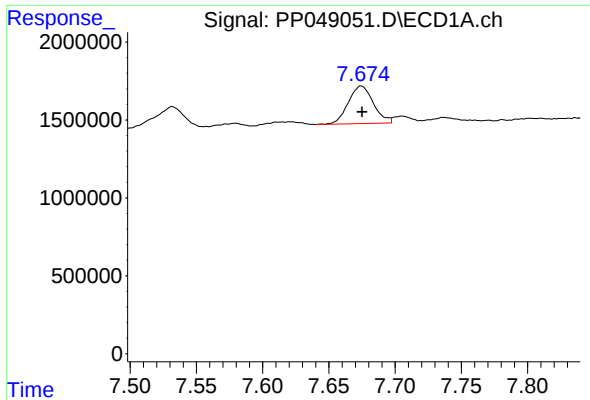

#30 AR-1254-5

R.T.: 7.674 min
Delta R.T.: 0.000 min
Response: 3183328
Conc: 37.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

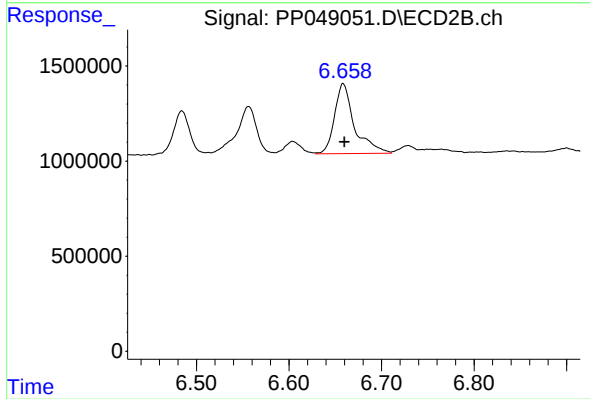

#30 AR-1254-5

R.T.: 6.659 min
Delta R.T.: -0.001 min
Response: 5518991
Conc: 38.03 ng/ml