

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 23:24
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 08:10:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.594	28567026	51331967	20.095	20.046
2) SA Decachlor...	10.092	8.566	28541228	24544538	23.269	21.775
Target Compounds						
36) L8 AR-1262-1	7.745	6.696	4093684	5976780	43.675	44.930
37) L8 AR-1262-2	8.294	6.955	7367314	5042811	43.052	44.501
38) L8 AR-1262-3	8.599	7.478	3200835	4249917	42.773	52.160
39) L8 AR-1262-4	8.689	7.542	2058420	6638286	43.855	45.540
40) L8 AR-1262-5	9.351	8.034	2822619	2629713	46.685	43.599



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 23:24
Operator : YP\AJ
Sample : N3214-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 08:10:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

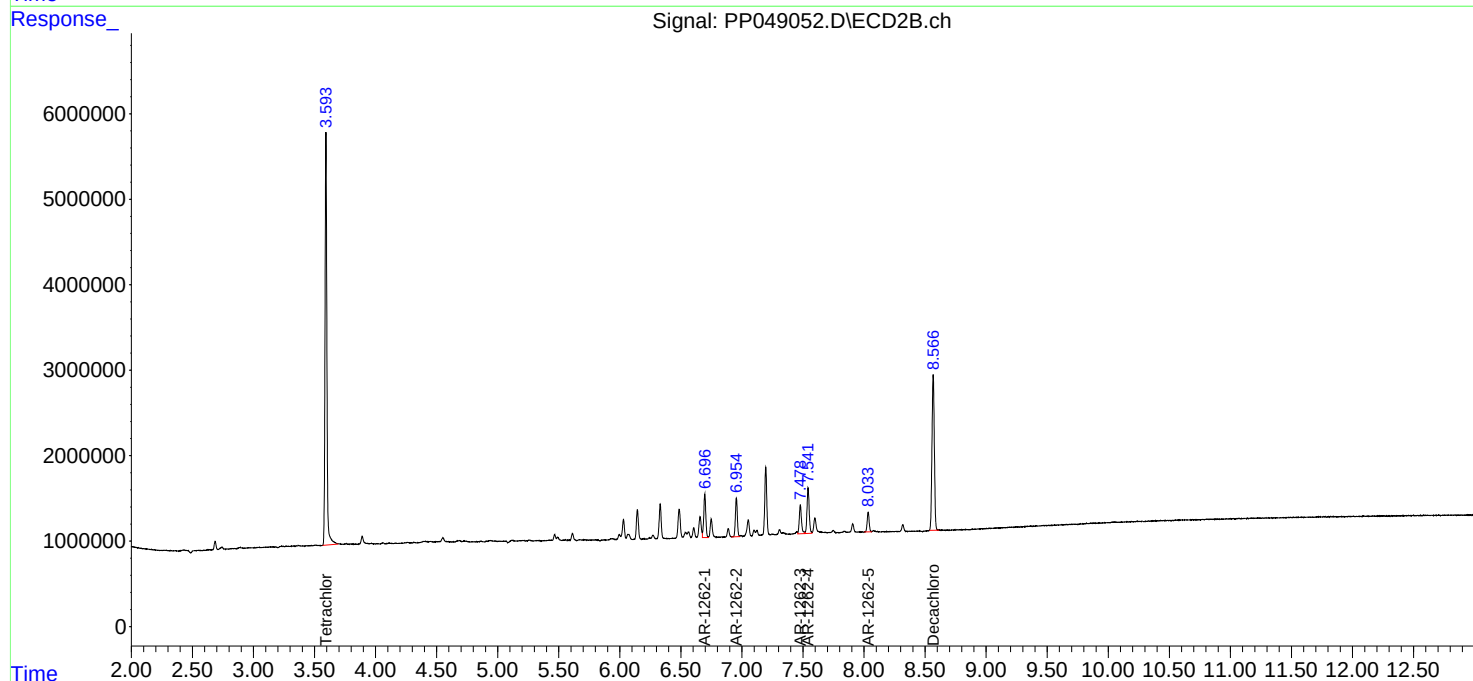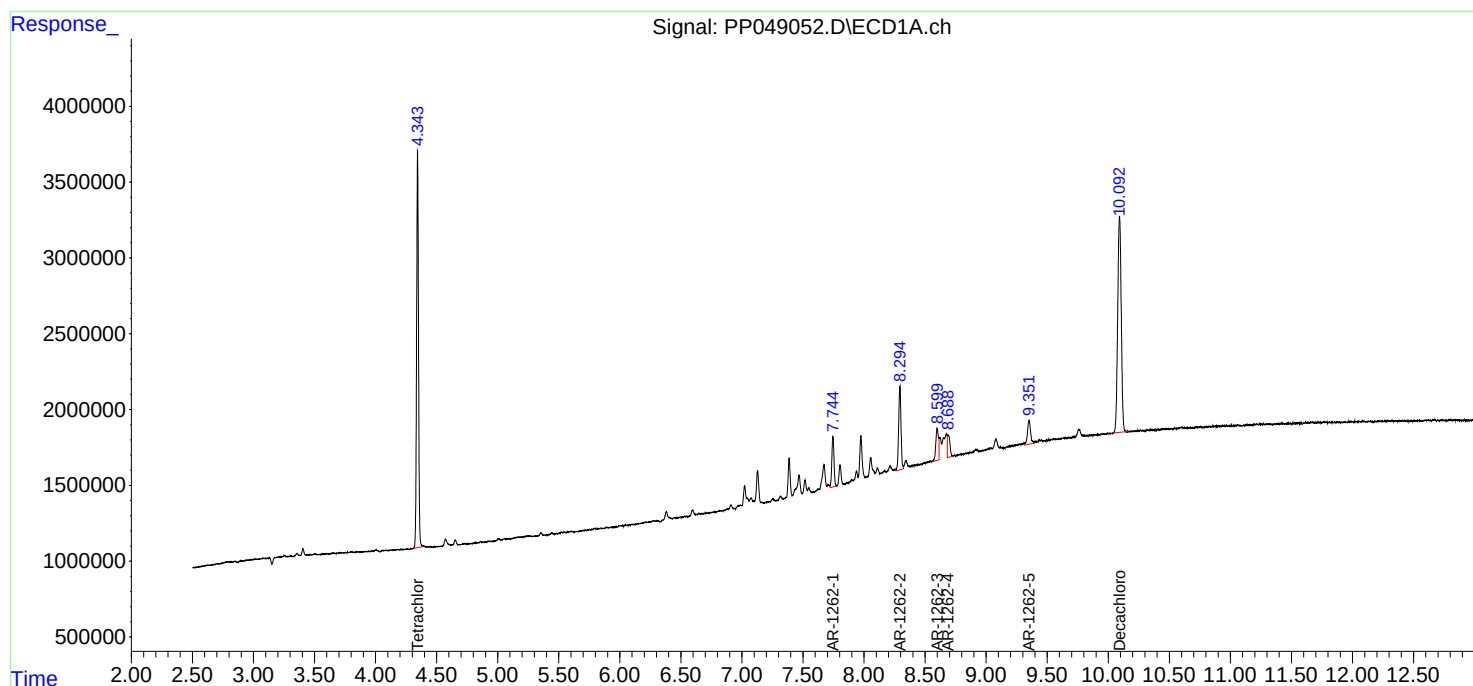


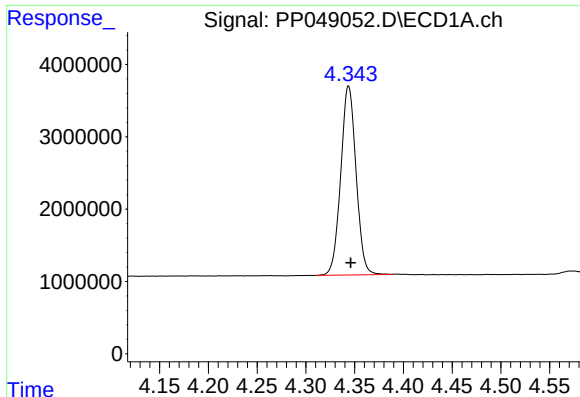

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 28567026
Conc: 20.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

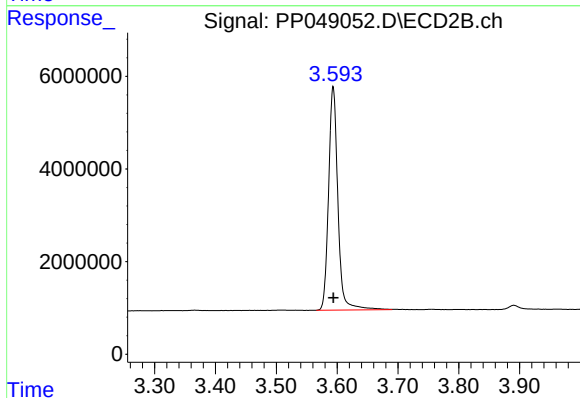


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 51331967
Conc: 20.05 ng/ml

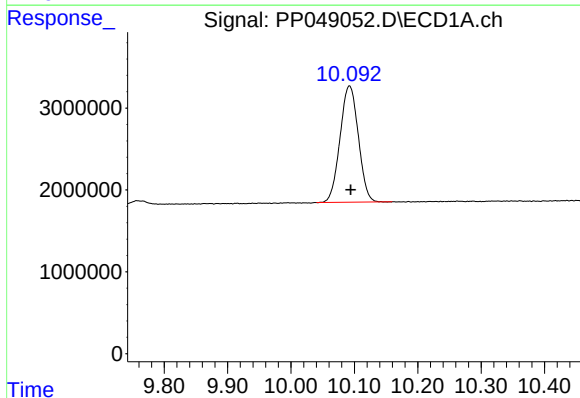


#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 28541228
Conc: 23.27 ng/ml

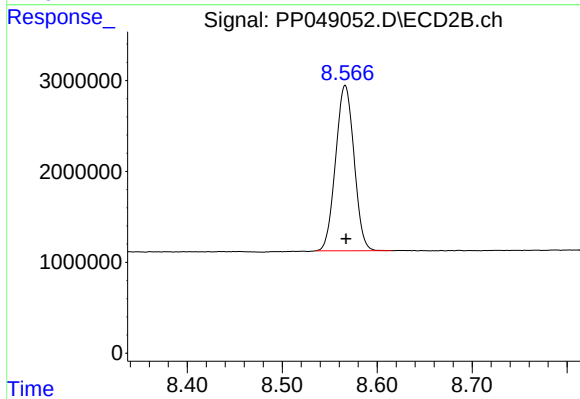

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.001 min
Response: 24544538
Conc: 21.77 ng/ml

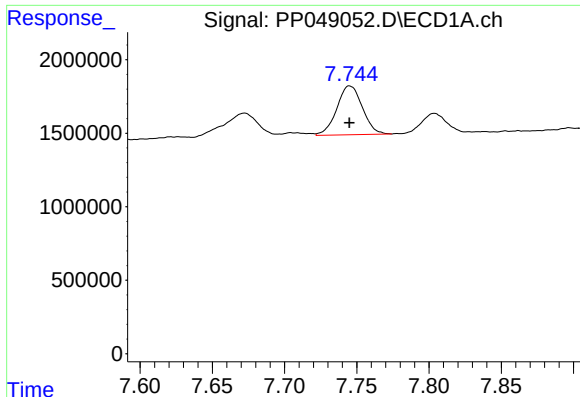

#36 AR-1262-1


R.T.: 7.745 min
Delta R.T.: 0.000 min
Response: 4093684
Conc: 43.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

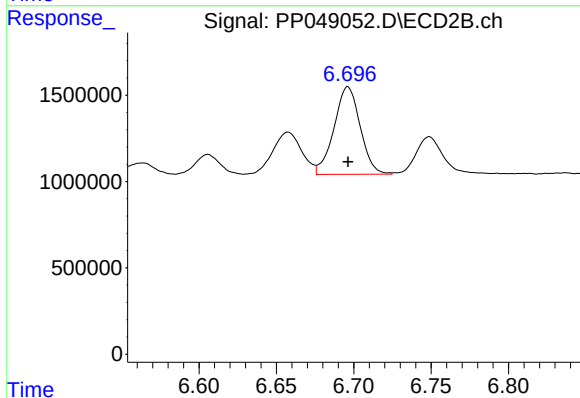


#36 AR-1262-1

R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 5976780
Conc: 44.93 ng/ml

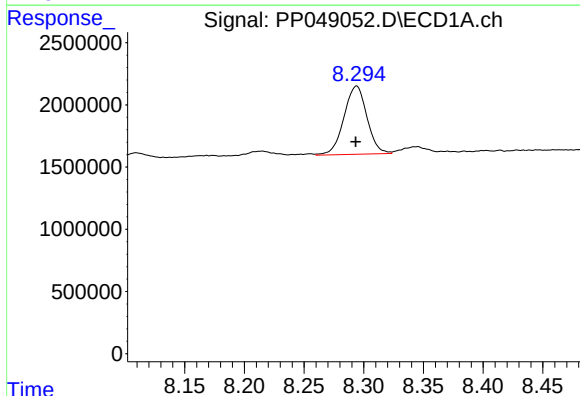


#37 AR-1262-2

R.T.: 8.294 min
Delta R.T.: 0.000 min
Response: 7367314
Conc: 43.05 ng/ml

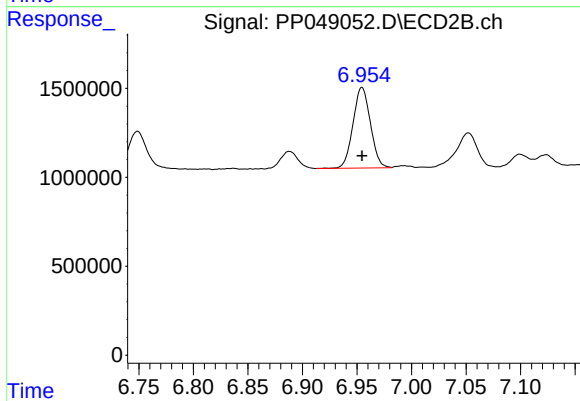

#37 AR-1262-2


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 5042811
Conc: 44.50 ng/ml

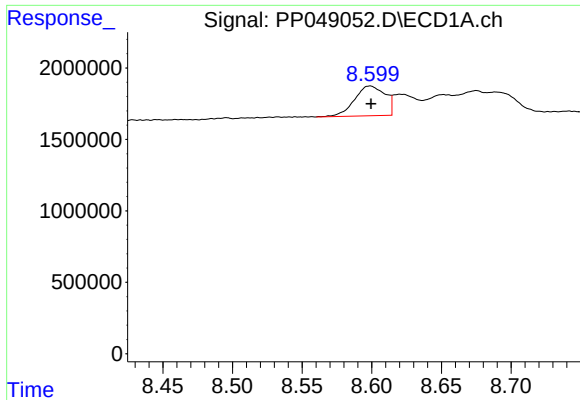

#38 AR-1262-3


R.T.: 8.599 min
Delta R.T.: 0.000 min
Response: 3200835
Conc: 42.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

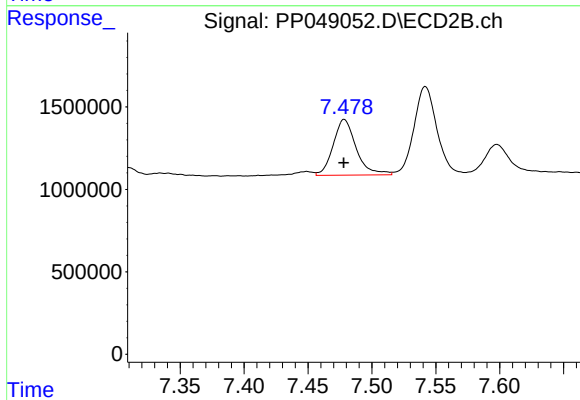


#38 AR-1262-3

R.T.: 7.478 min
Delta R.T.: 0.000 min
Response: 4249917
Conc: 52.16 ng/ml

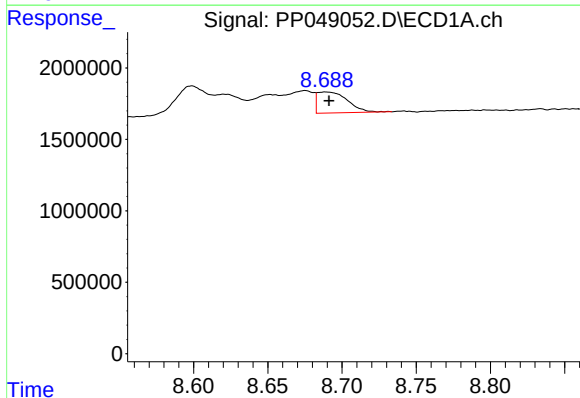


#39 AR-1262-4

R.T.: 8.689 min
Delta R.T.: -0.002 min
Response: 2058420
Conc: 43.86 ng/ml

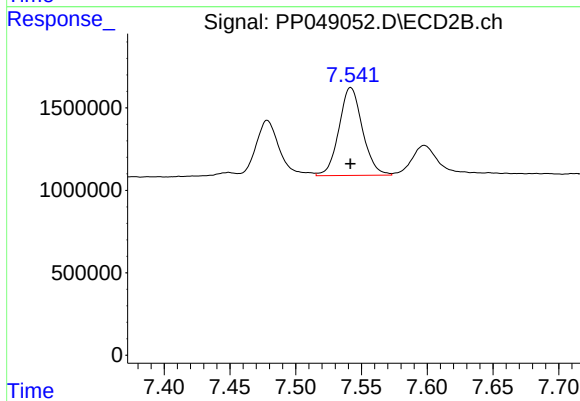

#39 AR-1262-4


R.T.: 7.542 min
Delta R.T.: 0.000 min
Response: 6638286
Conc: 45.54 ng/ml

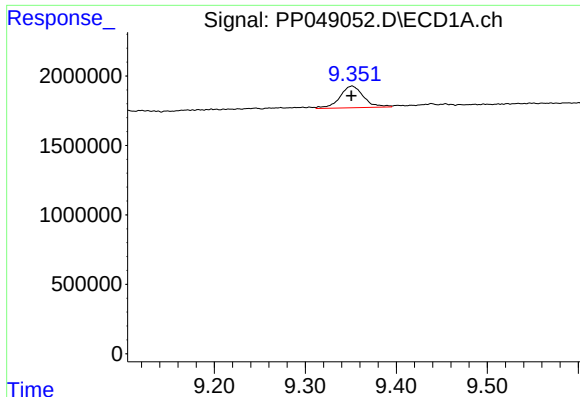

#40 AR-1262-5

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 2822619
Conc: 46.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

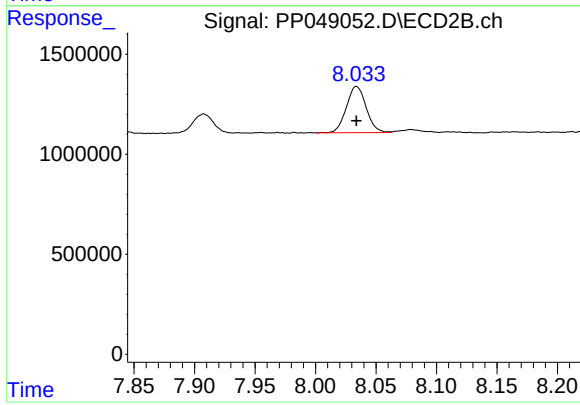

#40 AR-1262-5

R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 2629713
Conc: 43.60 ng/ml