

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
 Data File : PP049053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 23:41
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1268 LOD 40 PPB
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 08:12:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.593	27486763	49730812	19.336	19.421
2) SA Decachlor...	10.092	8.565	30735092	26305154	25.057	23.336
Target Compounds						
41) L9 AR-1268-1	8.598	7.477	7696647	9848338	40.984	45.780
42) L9 AR-1268-2	8.695	7.542	7048258	8337649	40.285	43.587
43) L9 AR-1268-3	8.917	7.748	5995346	6789982	41.852	44.581
44) L9 AR-1268-4	9.351	8.034	2831099	2685852	44.194	42.143
45) L9 AR-1268-5	9.760	8.317	18283871	16488168	39.642	41.323



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062922\
Data File : PP049053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 23:41
Operator : YP\AJ
Sample : N3214-07
Misc : AR1268 LOD 40 PPB
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 08:12:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

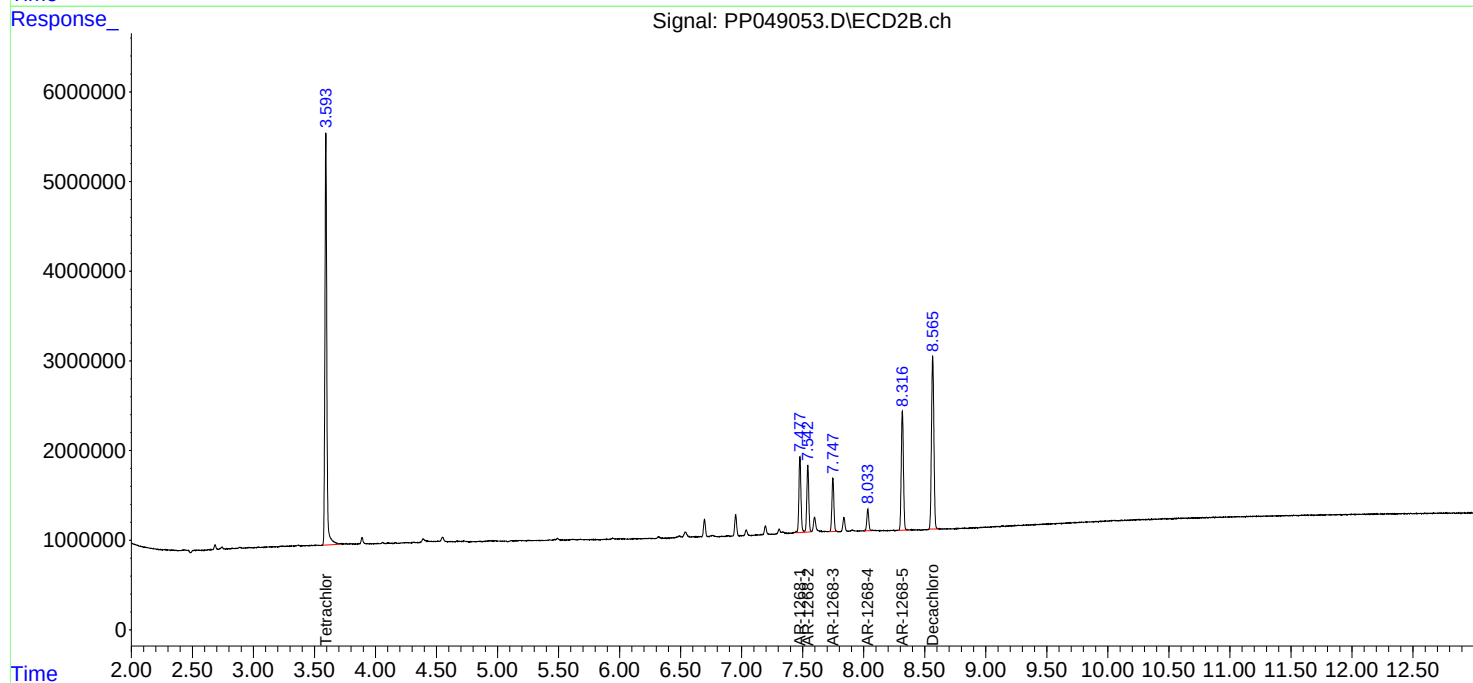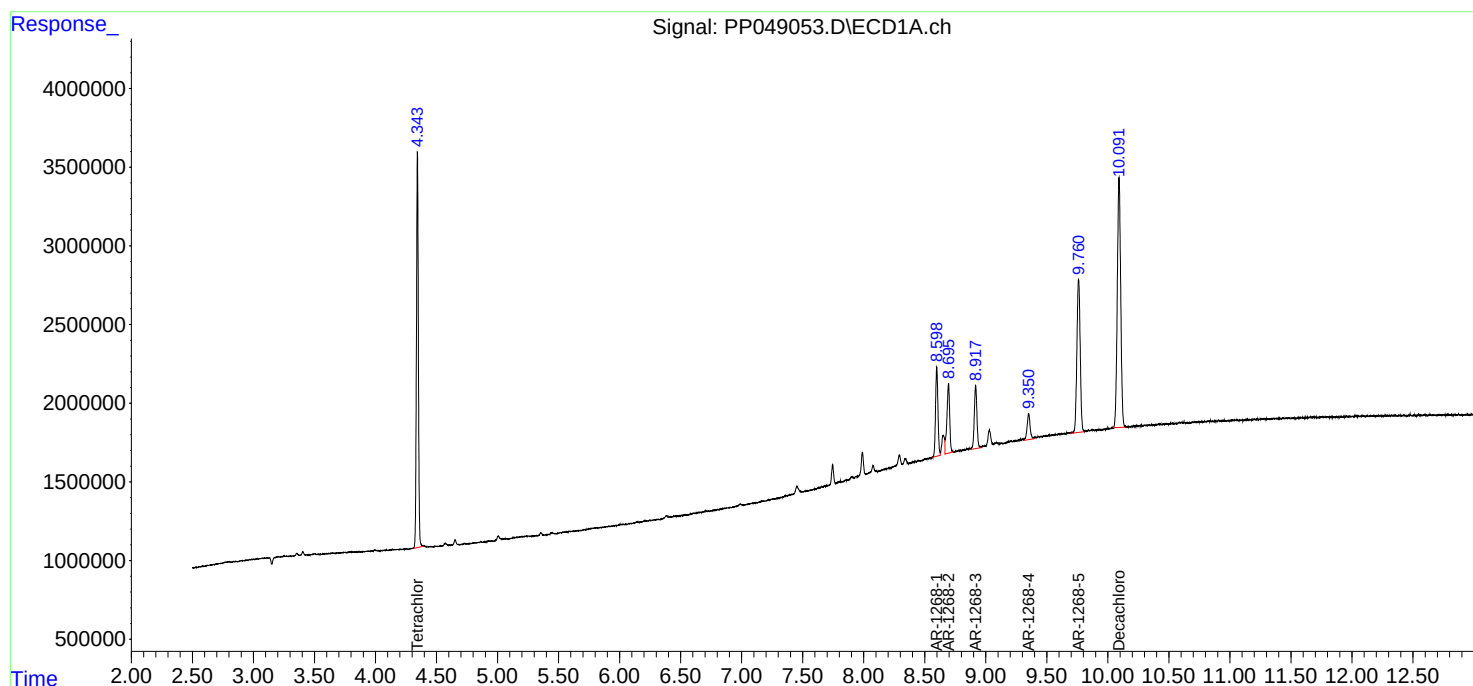


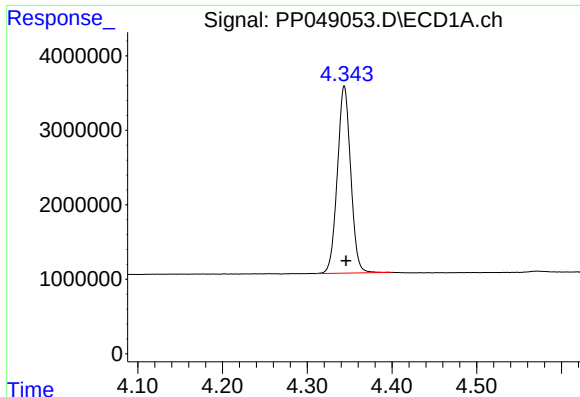

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 27486763
Conc: 19.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

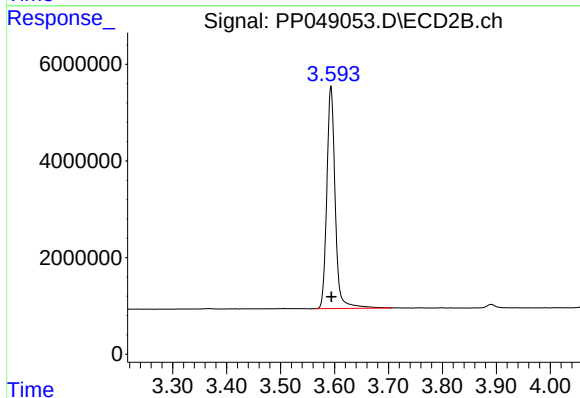


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 49730812
Conc: 19.42 ng/ml

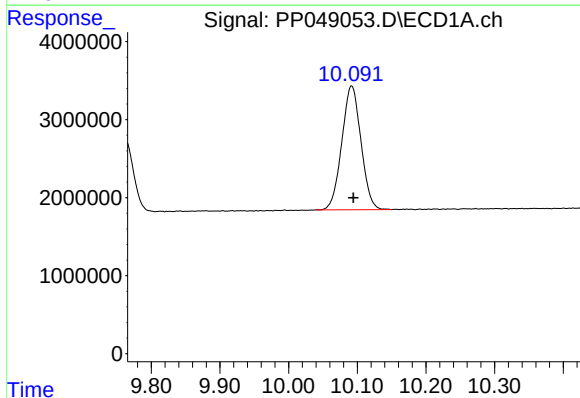


#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 30735092
Conc: 25.06 ng/ml

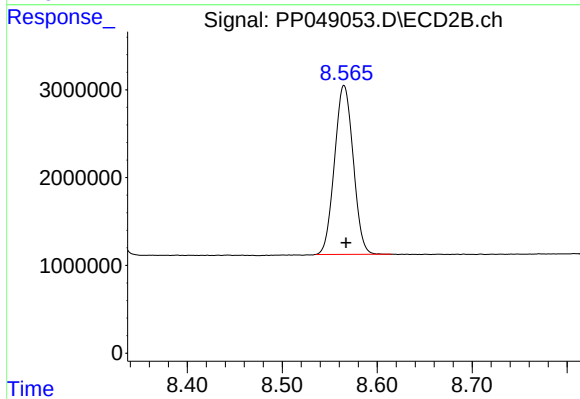

#2 Decachlorobiphenyl


R.T.: 8.565 min
Delta R.T.: -0.002 min
Response: 26305154
Conc: 23.34 ng/ml

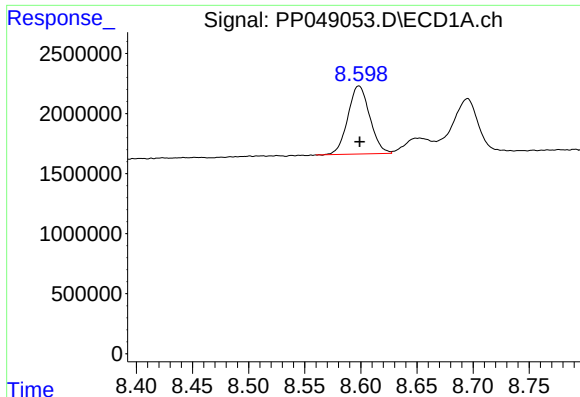

#41 AR-1268-1


R.T.: 8.598 min
Delta R.T.: 0.000 min
Response: 7696647
Conc: 40.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

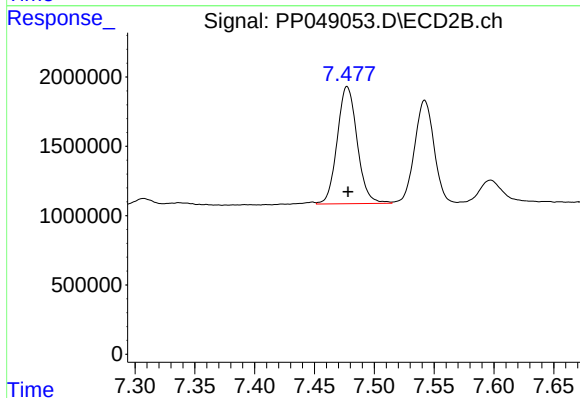


#41 AR-1268-1

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 9848338
Conc: 45.78 ng/ml

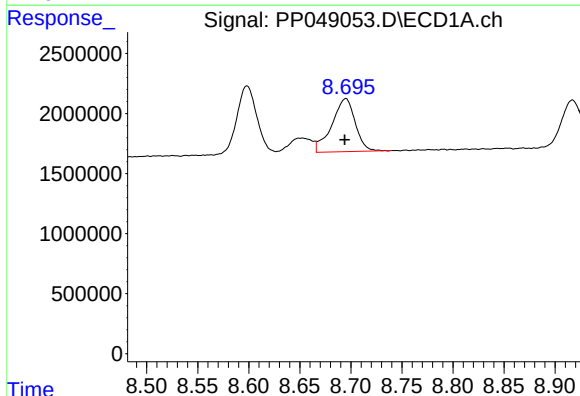


#42 AR-1268-2

R.T.: 8.695 min
Delta R.T.: 0.001 min
Response: 7048258
Conc: 40.28 ng/ml

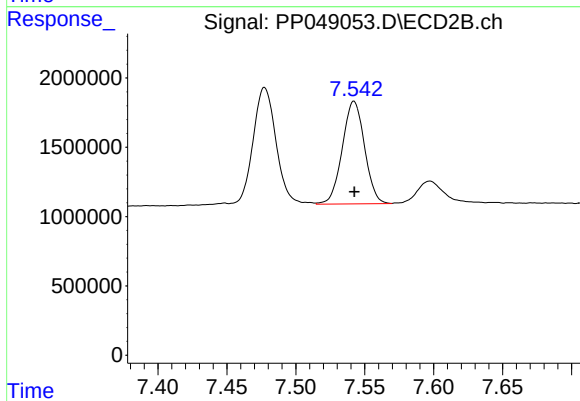

#42 AR-1268-2


R.T.: 7.542 min
Delta R.T.: 0.000 min
Response: 8337649
Conc: 43.59 ng/ml

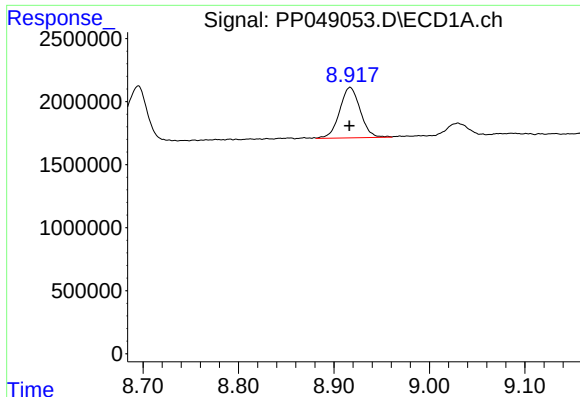

#43 AR-1268-3


R.T.: 8.917 min
Delta R.T.: 0.000 min
Response: 5995346
Conc: 41.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

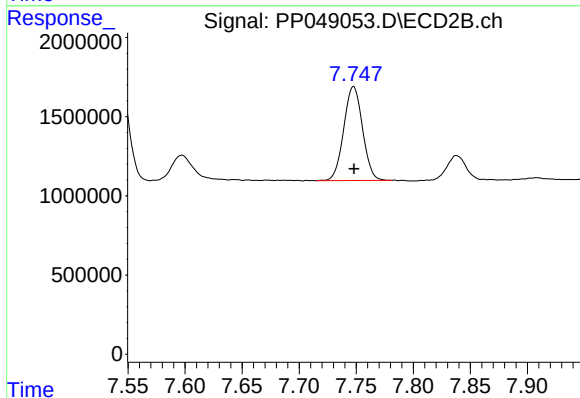


#43 AR-1268-3

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 6789982
Conc: 44.58 ng/ml

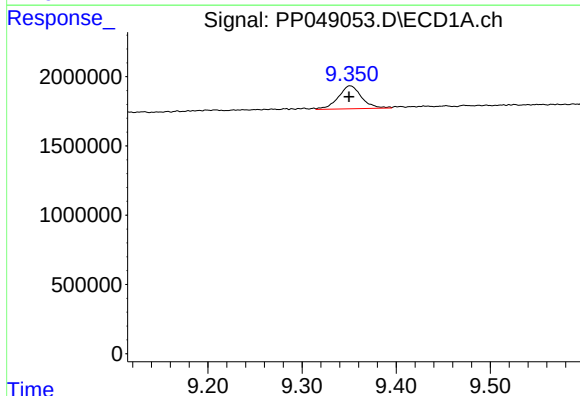


#44 AR-1268-4

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 2831099
Conc: 44.19 ng/ml

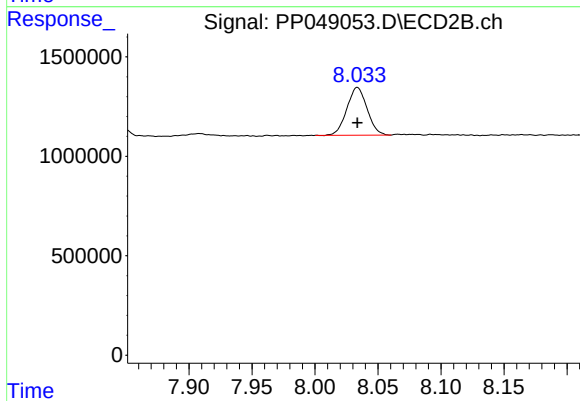

#44 AR-1268-4


R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 2685852
Conc: 42.14 ng/ml

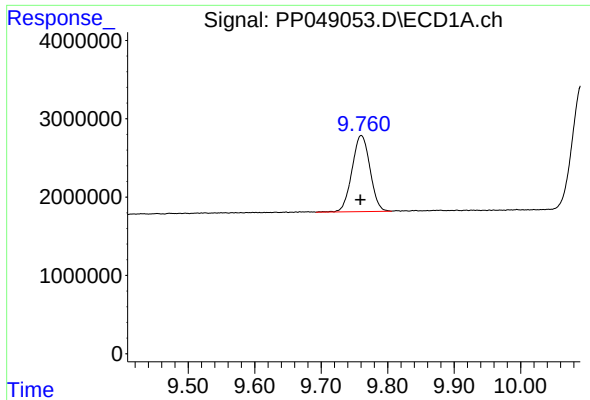

#45 AR-1268-5

R.T.: 9.760 min
Delta R.T.: 0.001 min
Response: 18283871
Conc: 39.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

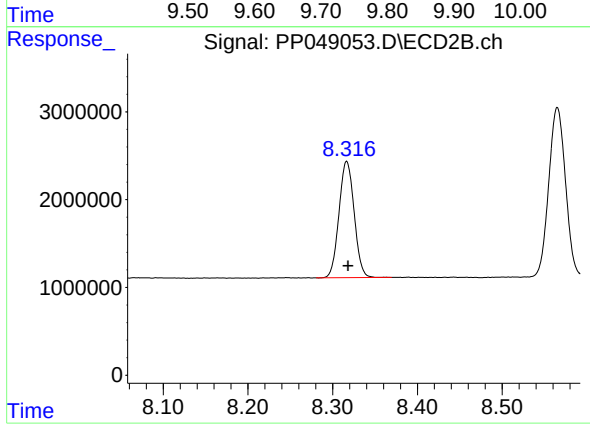

#45 AR-1268-5

R.T.: 8.317 min
Delta R.T.: -0.002 min
Response: 16488168
Conc: 41.32 ng/ml