

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063021\
 Data File : PP036928.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2021 17:47
 Operator : DD\AJ
 Sample : M2894-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAT-TP

Manual Integrations
 APPROVED

mohammad
 7/1/2021 12:07:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 00:54:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.955	652793	412996	14.770	13.334
2) SA Decachlor...	10.998	9.252	682949	397318	15.921	12.424
Target Compounds						
26) L6 AR-1254-1	7.193	6.076	351953	262503	200.126	154.927m
27) L6 AR-1254-2	7.422	6.237	592293	307736	218.904	206.895m
28) L6 AR-1254-3	7.804	6.656	748559	593996	252.717	244.325m
29) L6 AR-1254-4	8.100	6.897	523824	291640	238.280	188.462
30) L6 AR-1254-5	8.529	7.327	850112	672277	357.469	312.645

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063021\
Data File : PP036928.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2021 17:47
Operator : DD\AJ
Sample : M2894-02
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
PAT-TP


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 00:54:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

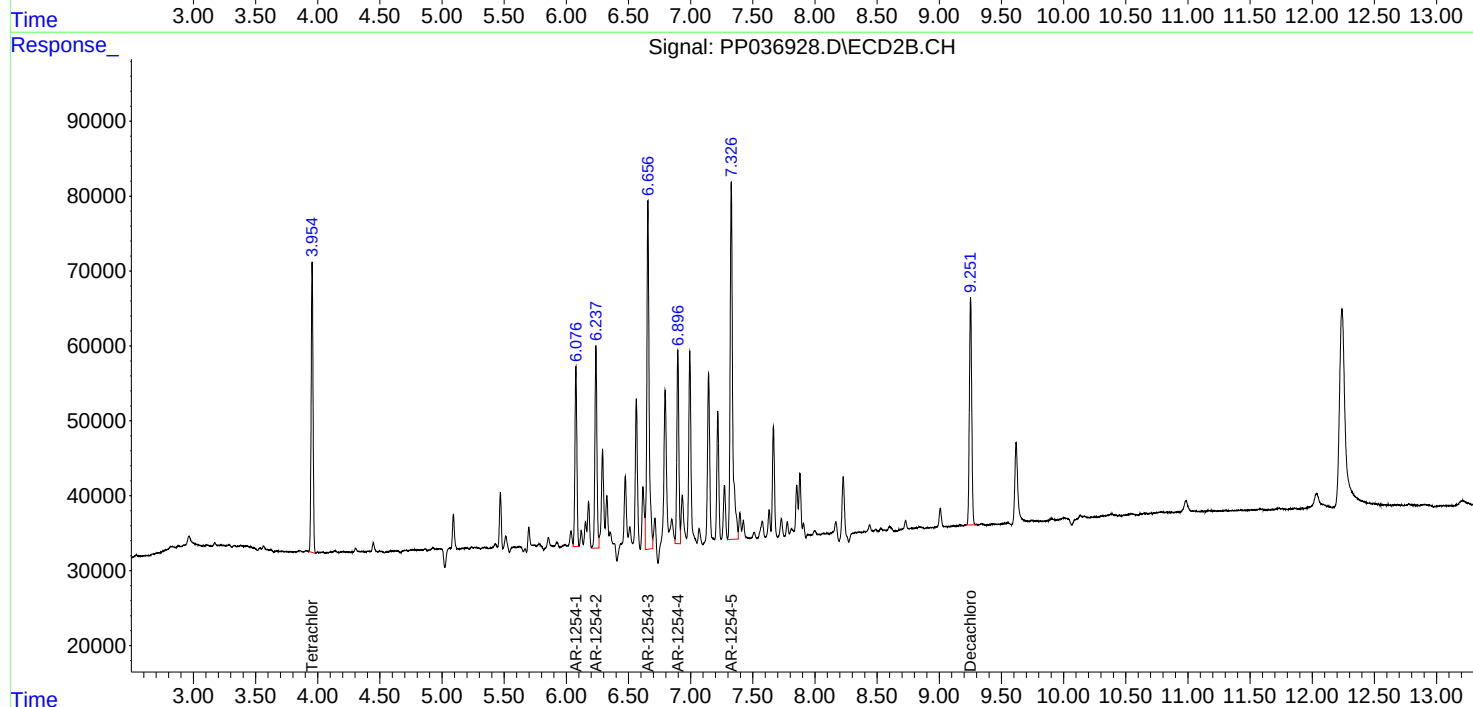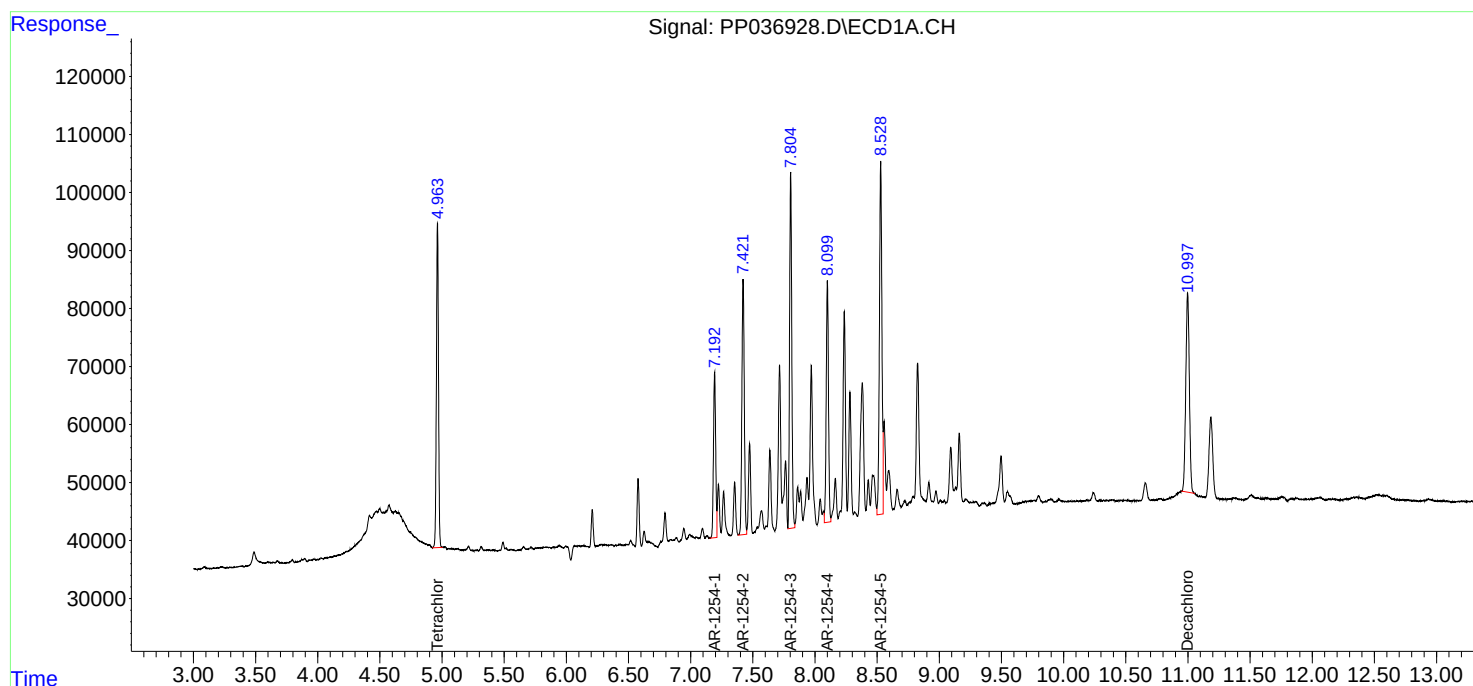

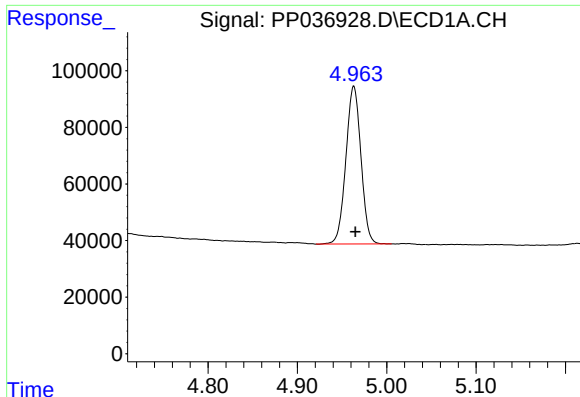


#1 Tetrachloro-m-xylene

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 652793
Conc: 14.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-TP


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:12 PM

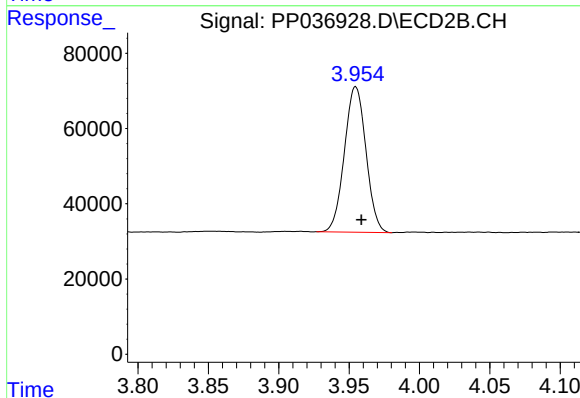


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.004 min
Response: 412996
Conc: 13.33 ng/ml

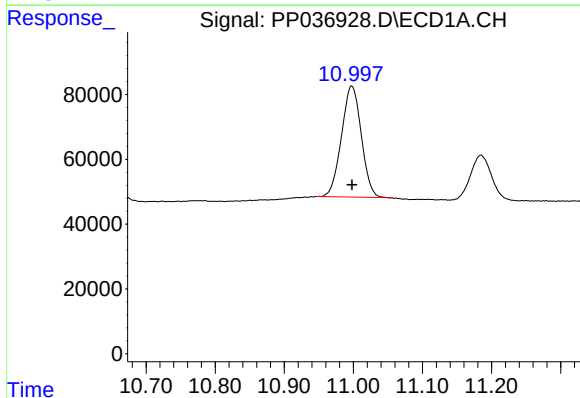


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 682949
Conc: 15.92 ng/ml

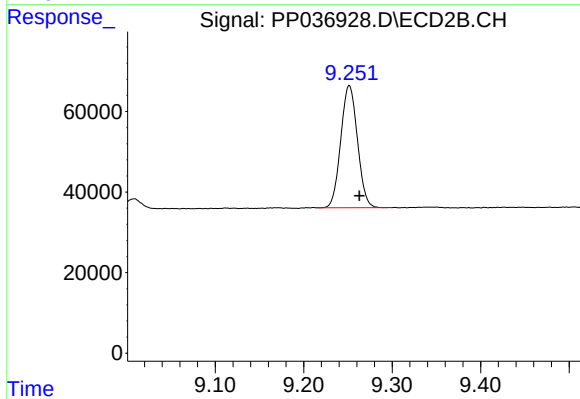

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.011 min
Response: 397318
Conc: 12.42 ng/ml

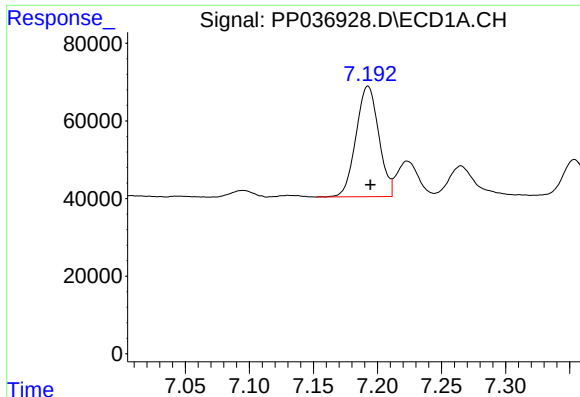


#26 AR-1254-1

R.T.: 7.193 min
Delta R.T.: -0.002 min
Response: 351953
Conc: 200.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-TP


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:12 PM

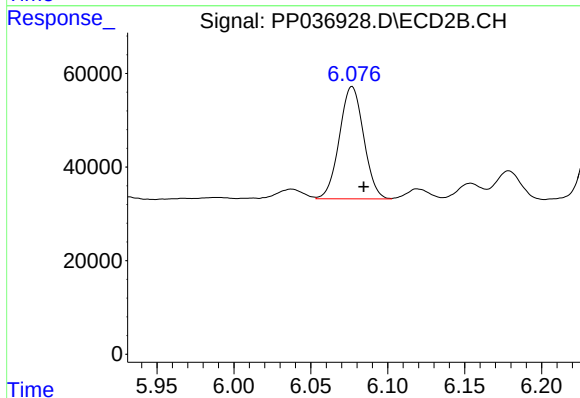


#26 AR-1254-1

R.T.: 6.076 min
Delta R.T.: -0.008 min
Response: 262503
Conc: 154.93 ng/ml m

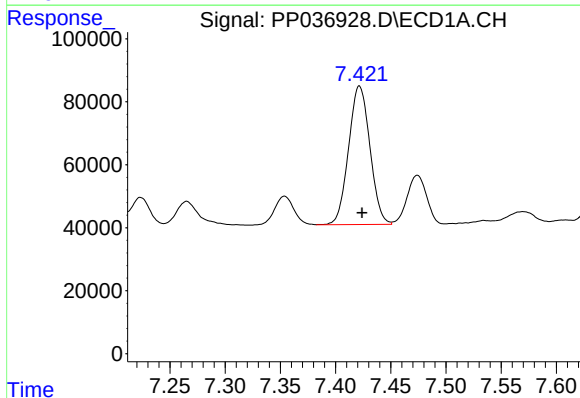


#27 AR-1254-2

R.T.: 7.422 min
Delta R.T.: -0.002 min
Response: 592293
Conc: 218.90 ng/ml

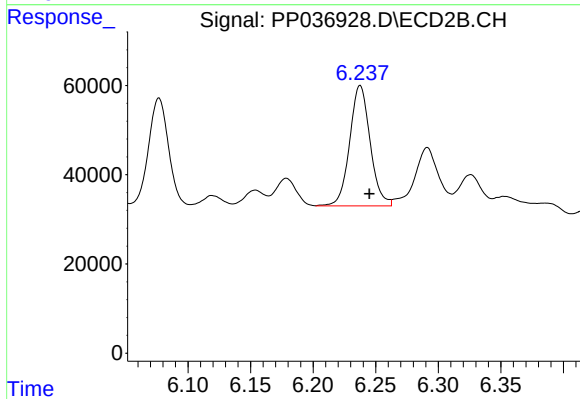

#27 AR-1254-2

R.T.: 6.237 min
Delta R.T.: -0.008 min
Response: 307736
Conc: 206.89 ng/ml m

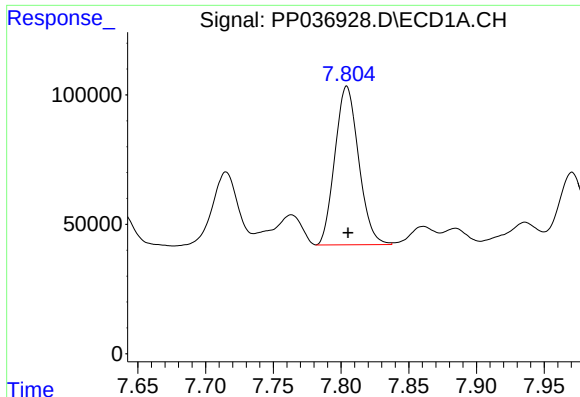


#28 AR-1254-3

R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 748559
Conc: 252.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-TP


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:12 PM

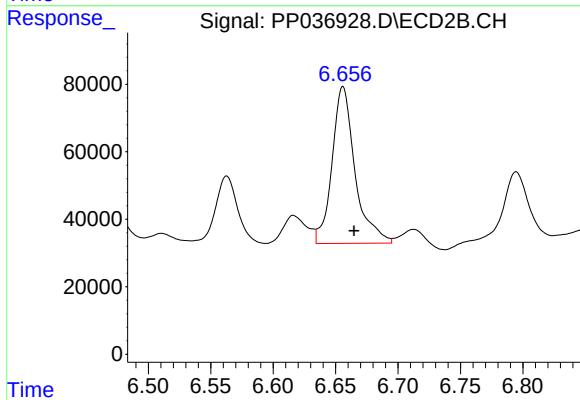


#28 AR-1254-3

R.T.: 6.656 min
Delta R.T.: -0.009 min
Response: 593996
Conc: 244.33 ng/ml m

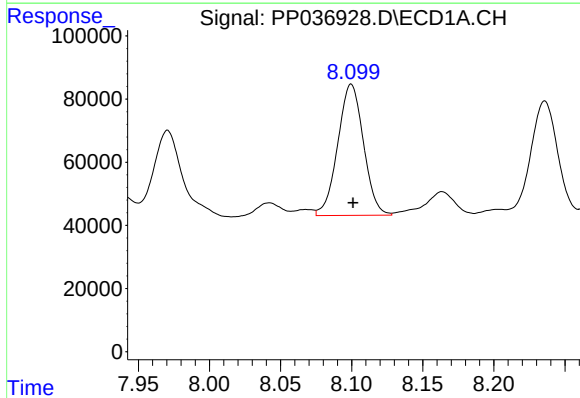


#29 AR-1254-4

R.T.: 8.100 min
Delta R.T.: -0.001 min
Response: 523824
Conc: 238.28 ng/ml

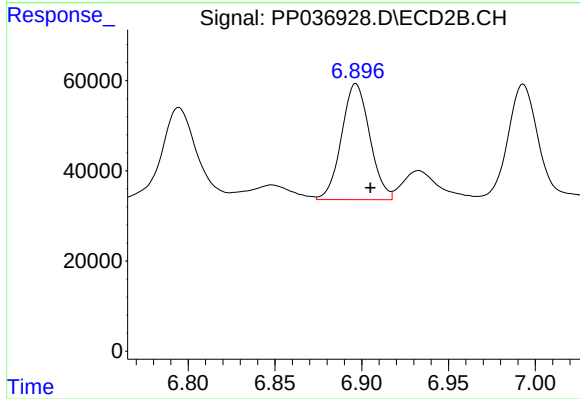

#29 AR-1254-4

R.T.: 6.897 min
Delta R.T.: -0.008 min
Response: 291640
Conc: 188.46 ng/ml

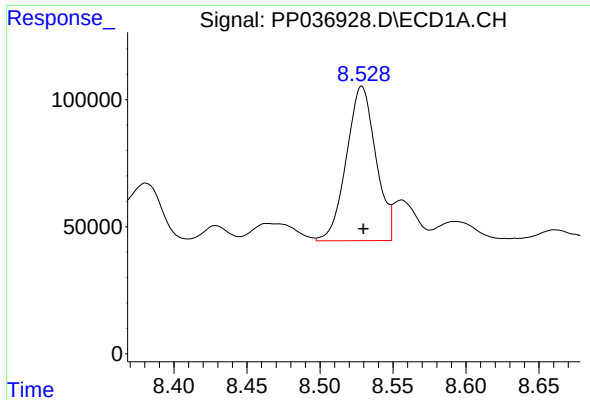


#30 AR-1254-5

R.T.: 8.529 min
Delta R.T.: 0.000 min
Response: 850112
Conc: 357.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-TP

Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:12 PM

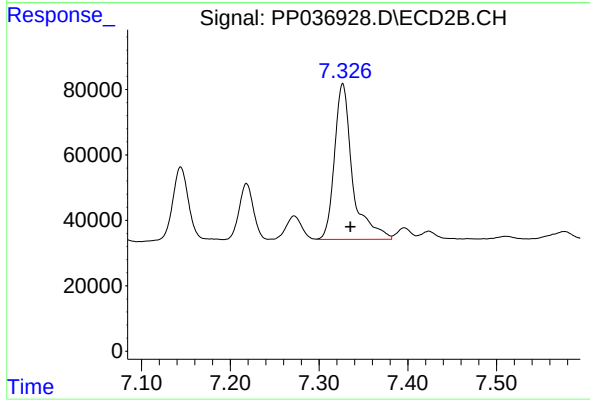

#30 AR-1254-5

R.T.: 7.327 min
Delta R.T.: -0.009 min
Response: 672277
Conc: 312.65 ng/ml