

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063021\
 Data File : PP036941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2021 23:10
 Operator : DD\AJ
 Sample : M2882-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DRIP-COMP-AUD-1121-1122

Manual Integrations
 APPROVED

mohammad
 7/1/2021 12:07:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:00:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.955	1044094	480191	23.623m	15.503 #
2) SA Decachlor...	10.994	9.250	926311	495139	21.594	15.483 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063021\
Data File : PP036941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2021 23:10
Operator : DD\AJ
Sample : M2882-03
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DRIP-COMP-AUD-1121-1122


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:00:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

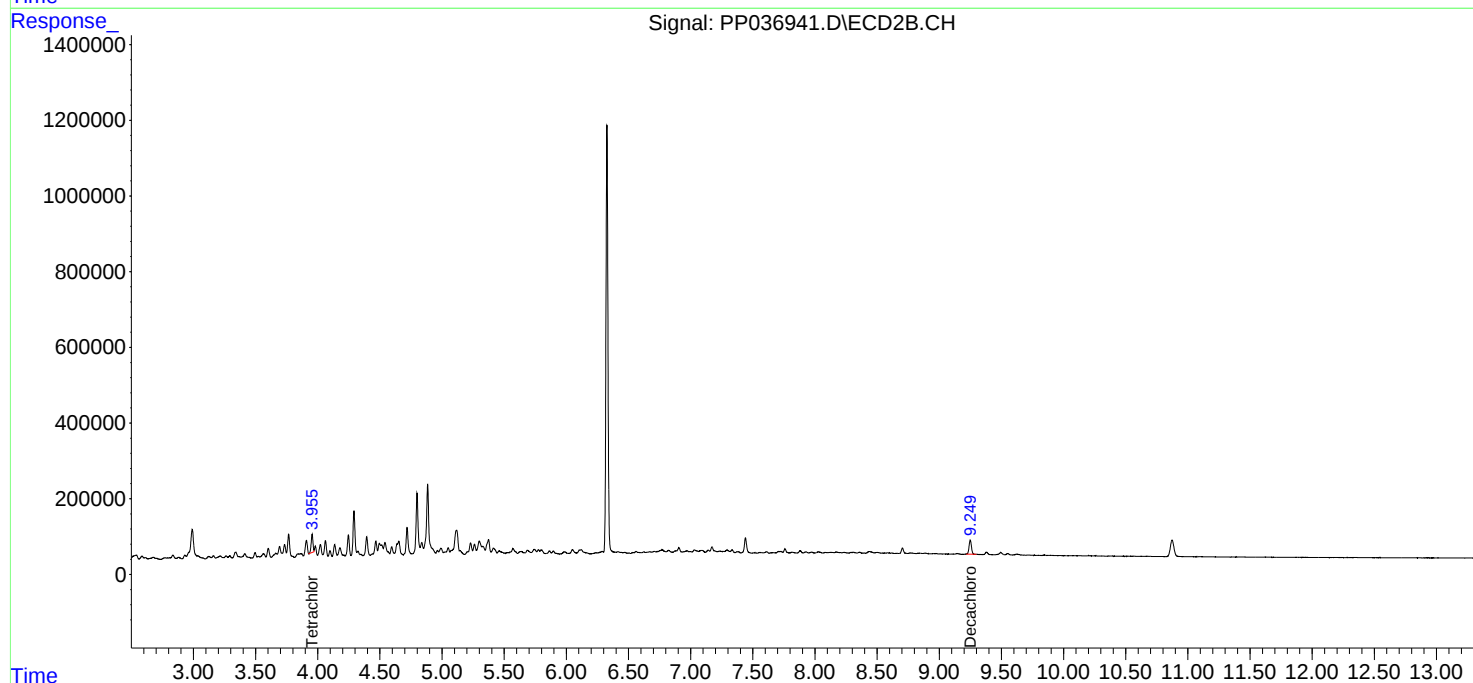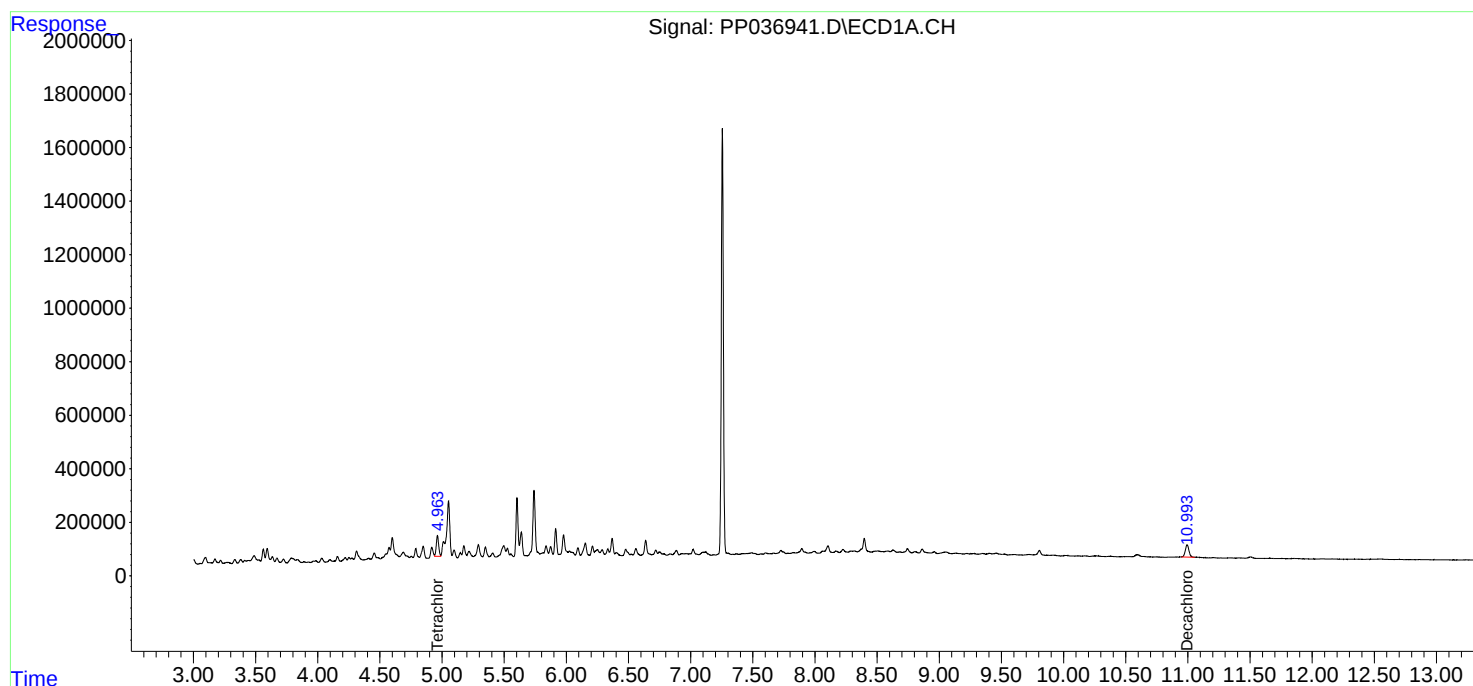

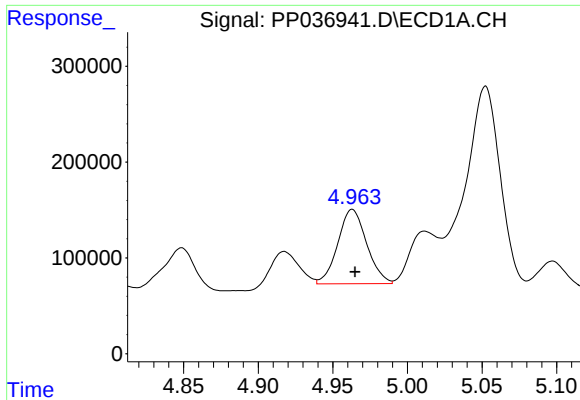

#1 Tetrachloro-m-xylene

R.T.: 4.963 min

Delta R.T.: -0.002 min


Response: 1044094

Conc: 23.62 ng/ml m

Instrument :
ECD_P
ClientSampleId :
DRIP-COMP-AUD-1121-1122

Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:15 PM

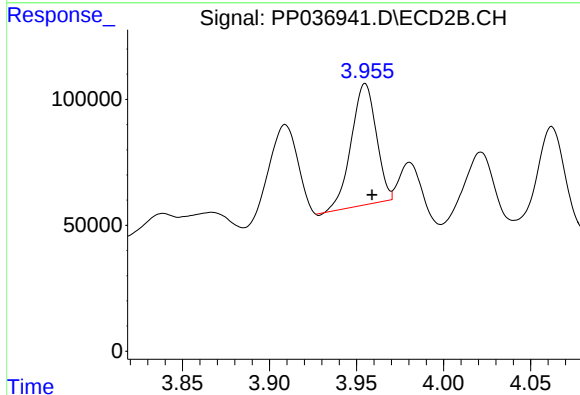


#1 Tetrachloro-m-xylene

R.T.: 3.955 min

Delta R.T.: -0.004 min

Response: 480191

Conc: 15.50 ng/ml

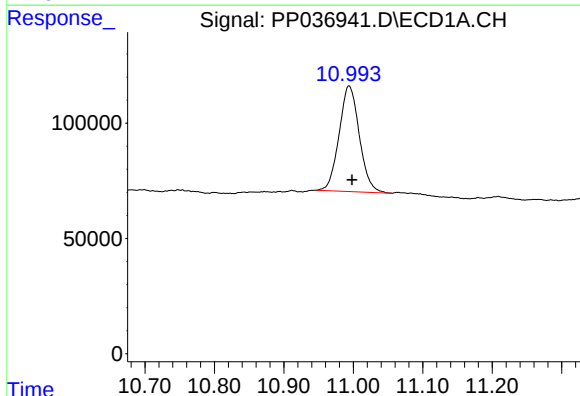


#2 Decachlorobiphenyl

R.T.: 10.994 min

Delta R.T.: -0.004 min

Response: 926311

Conc: 21.59 ng/ml

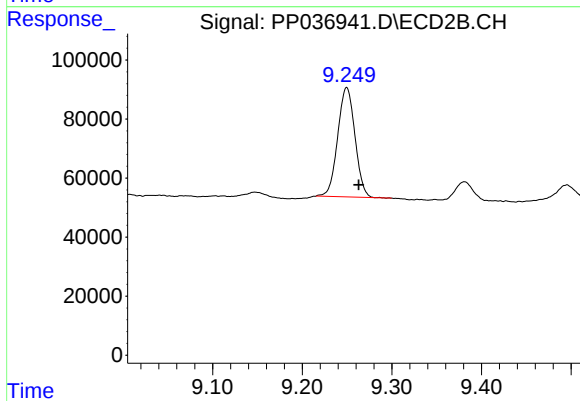

#2 Decachlorobiphenyl

R.T.: 9.250 min

Delta R.T.: -0.013 min

Response: 495139

Conc: 15.48 ng/ml