

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063021\
 Data File : PP036942.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2021 23:27
 Operator : DD\AJ
 Sample : M2882-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEALPOT-AUD-1123

Manual Integrations
 APPROVED

mohammad
 7/1/2021 12:07:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:01:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.964	3.956	341605	221163	7.729m	7.140m
2) SA Decachlor...	10.997	9.251	333320	189298	7.770	5.919

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063021\
Data File : PP036942.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2021 23:27
Operator : DD\AJ
Sample : M2882-05
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SEALPOT-AUD-1123


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:01:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

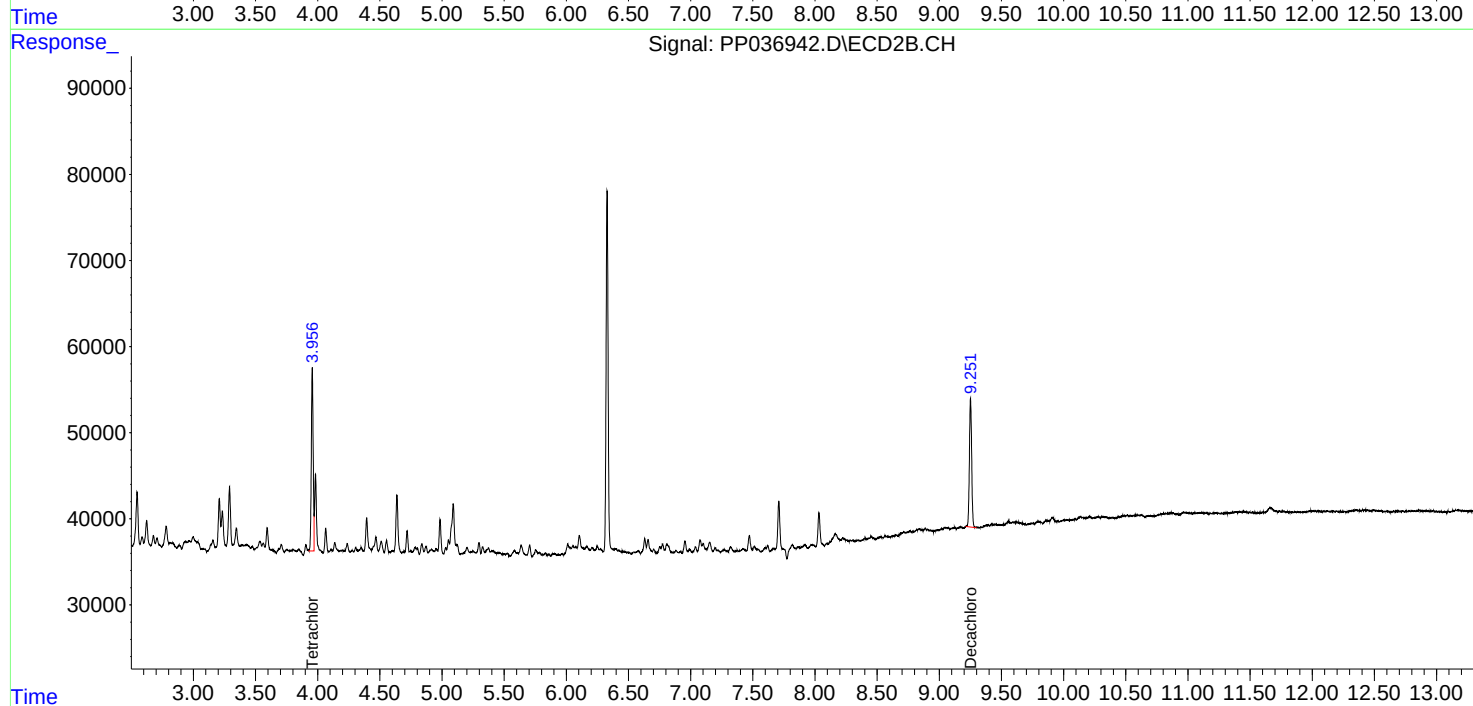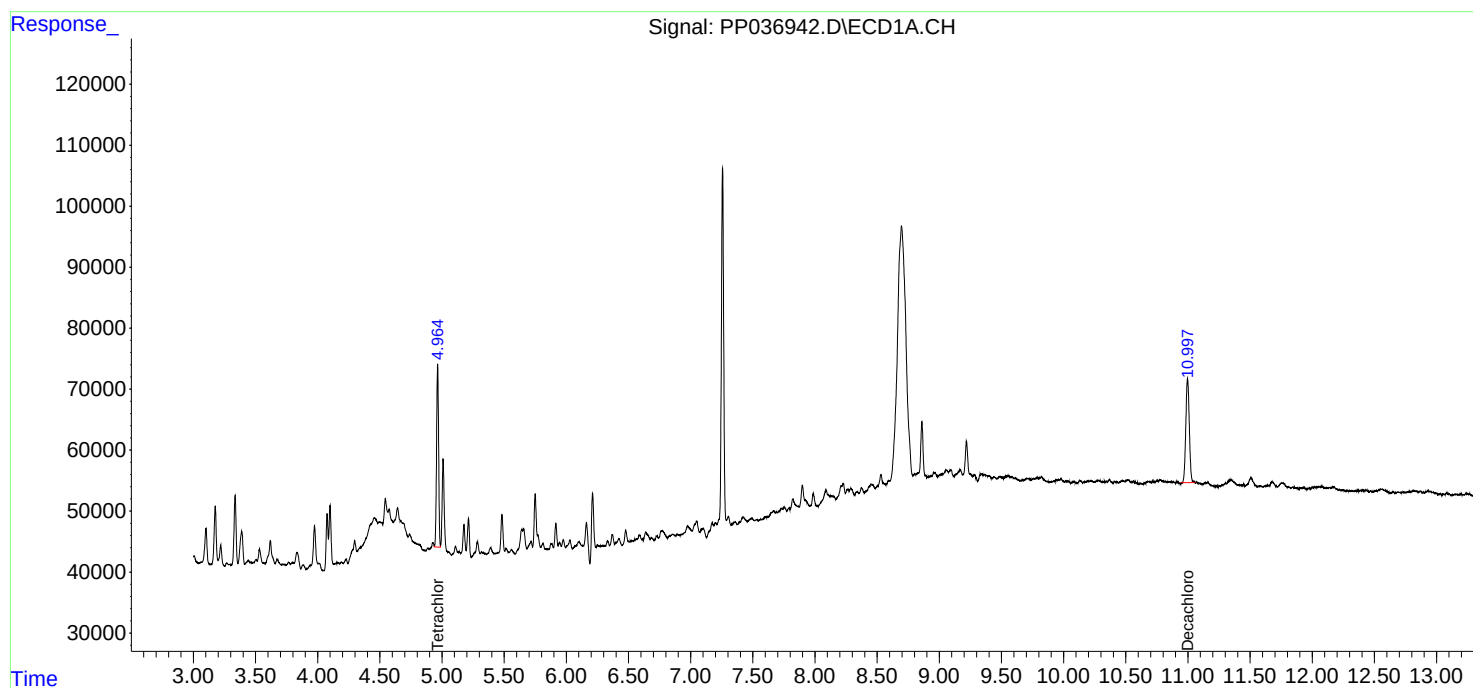

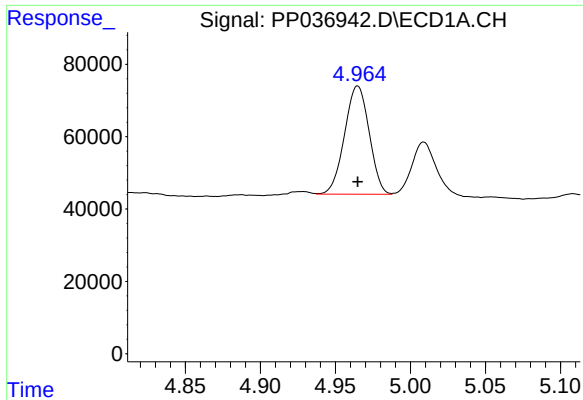


#1 Tetrachloro-m-xylene

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 341605
Conc: 7.73 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SEALPOT-AUD-1123


Manual Integrations
APPROVED

mohammad
7/1/2021 12:07:18 PM

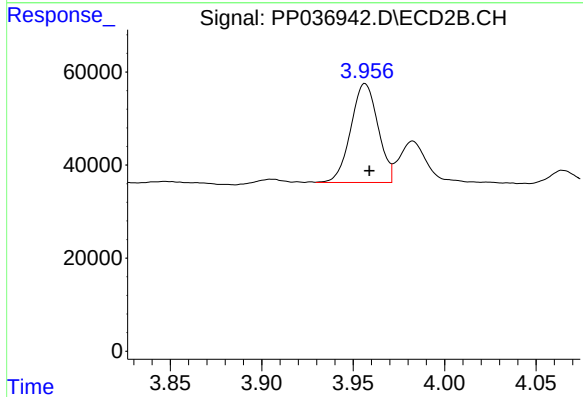


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.003 min
Response: 221163
Conc: 7.14 ng/ml m

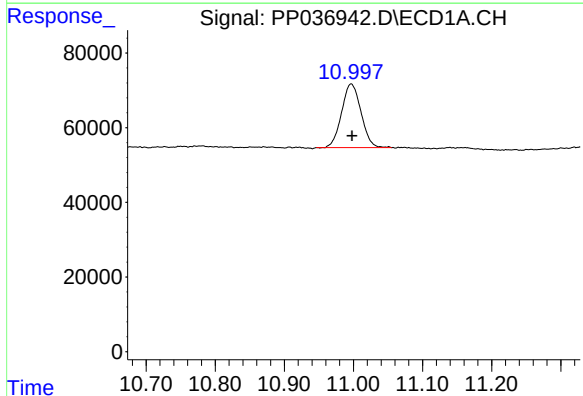

#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: -0.001 min
Response: 333320
Conc: 7.77 ng/ml

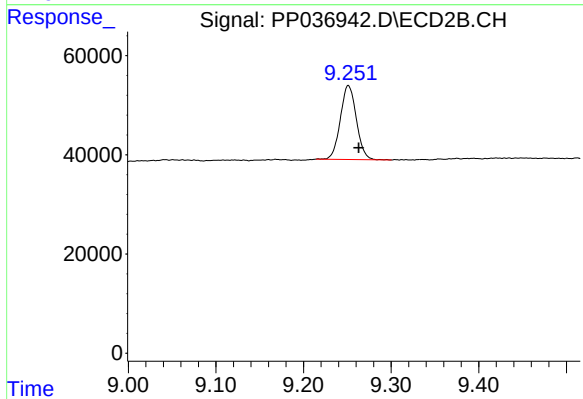

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.012 min
Response: 189298
Conc: 5.92 ng/ml