

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
 Data File : PP049092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 18:36
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:50:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.593	23126253	41864354	16.268	16.349
2) SA Decachlor...	10.091	8.566	23487245	20007668	19.148	17.750
Target Compounds						
8) L2 AR-1221-1	4.561	3.805	570793	688315	33.483	20.507 #
9) L2 AR-1221-2	4.650	3.890	608115	1097152	47.568	42.739
10) L2 AR-1221-3	4.722	3.965	851766	1492183	21.523	20.292



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
Data File : PP049092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 18:36
Operator : YP\AJ
Sample : N3214-07
Misc : AR1221 MDL 25 PPB
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:50:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

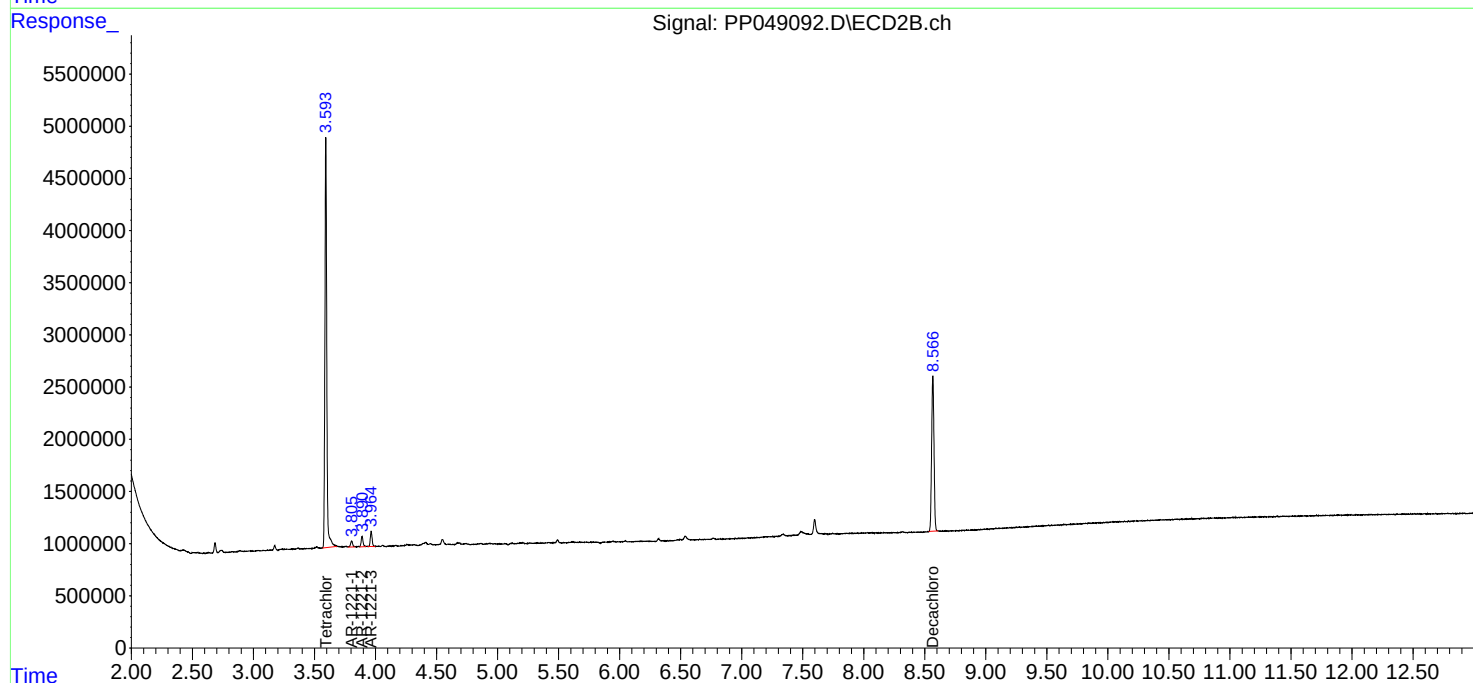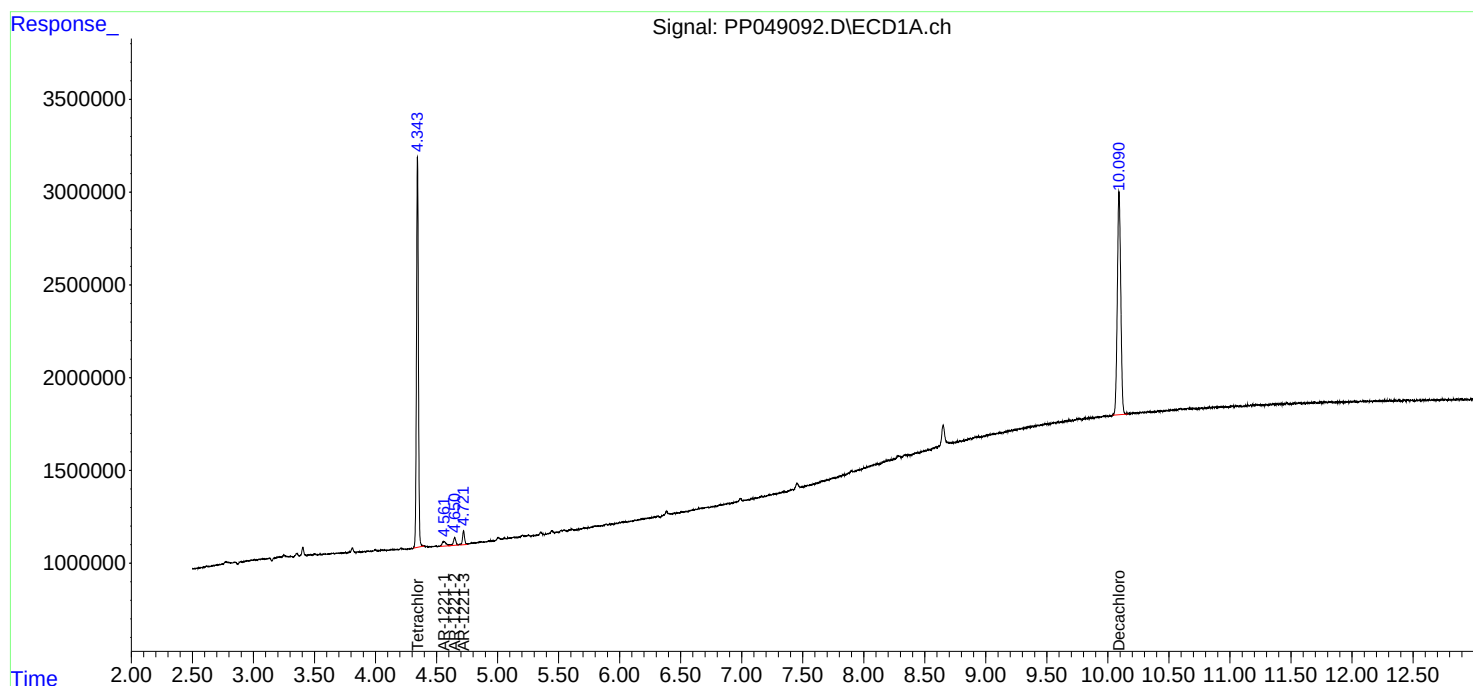


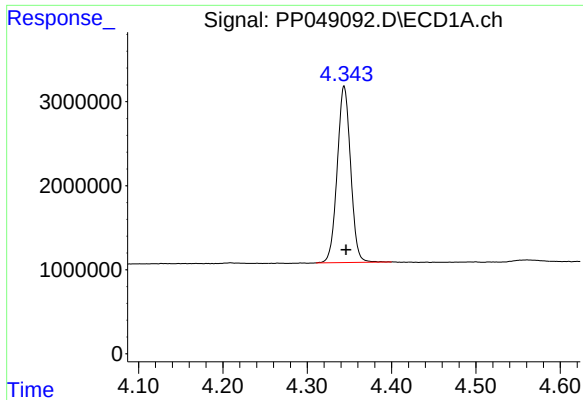

#1 Tetrachloro-m-xylene


R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 23126253
Conc: 16.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

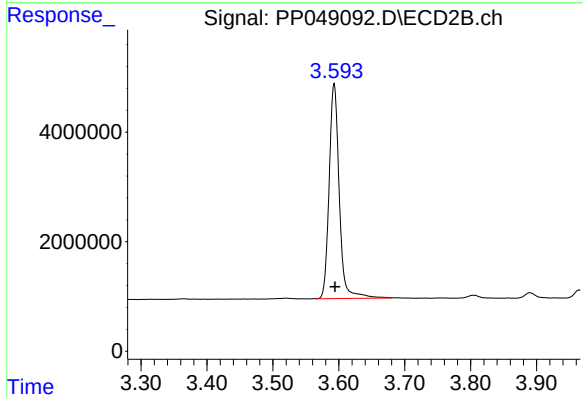


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: -0.001 min
Response: 41864354
Conc: 16.35 ng/ml

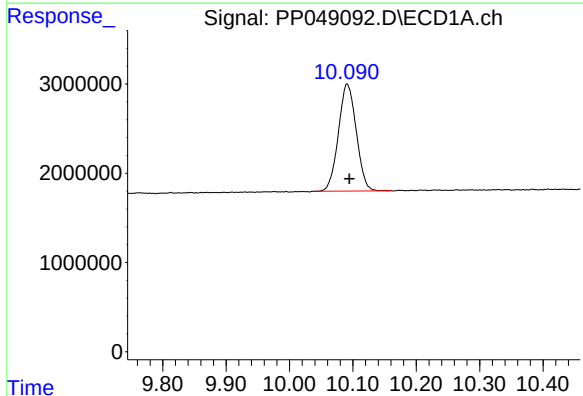


#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: -0.003 min
Response: 23487245
Conc: 19.15 ng/ml

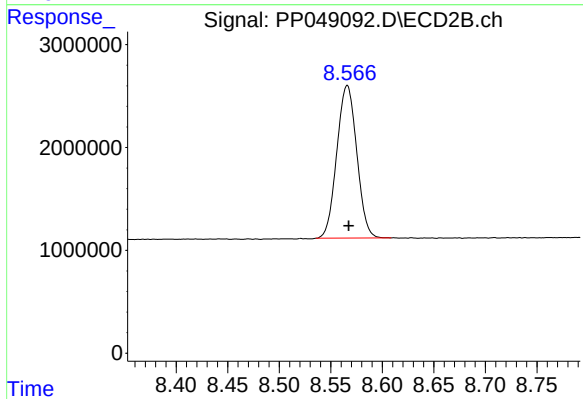

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.001 min
Response: 20007668
Conc: 17.75 ng/ml

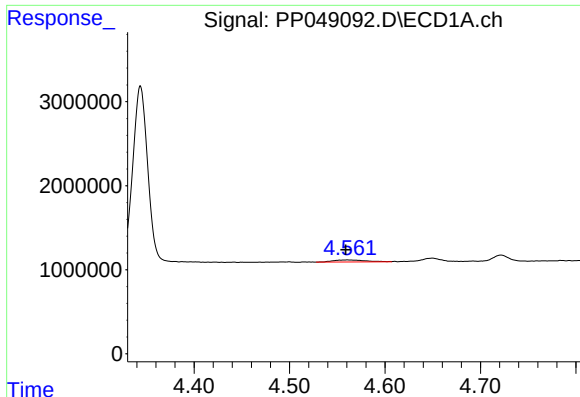

#8 AR-1221-1


R.T.: 4.561 min
Delta R.T.: 0.002 min
Response: 570793
Conc: 33.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

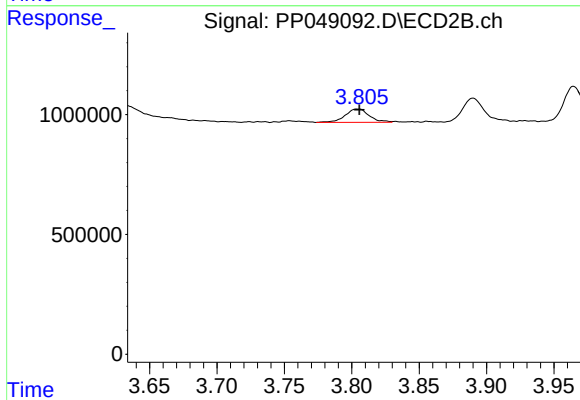


#8 AR-1221-1

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 688315
Conc: 20.51 ng/ml

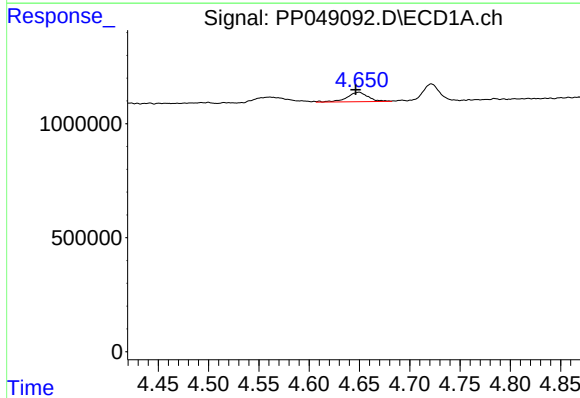


#9 AR-1221-2

R.T.: 4.650 min
Delta R.T.: 0.003 min
Response: 608115
Conc: 47.57 ng/ml

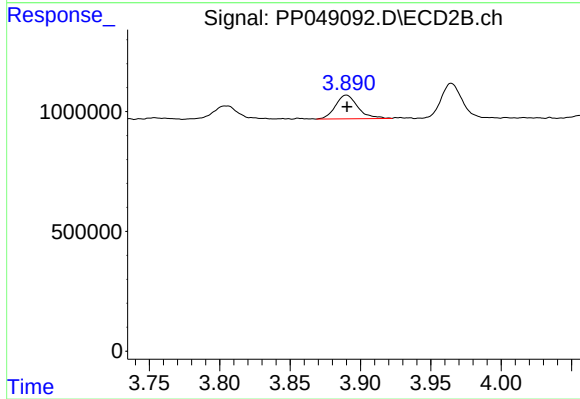

#9 AR-1221-2


R.T.: 3.890 min
Delta R.T.: 0.000 min
Response: 1097152
Conc: 42.74 ng/ml

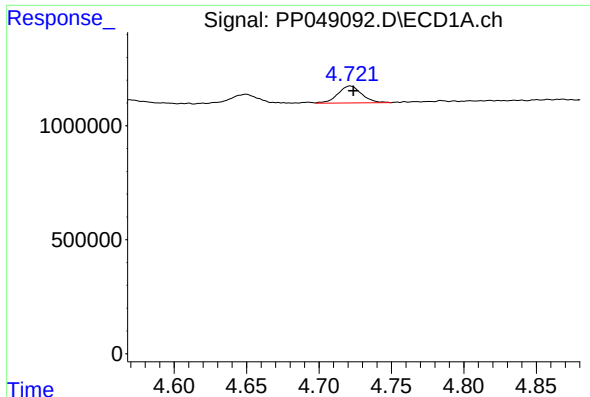

#10 AR-1221-3

R.T.: 4.722 min
Delta R.T.: -0.002 min
Response: 851766
Conc: 21.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

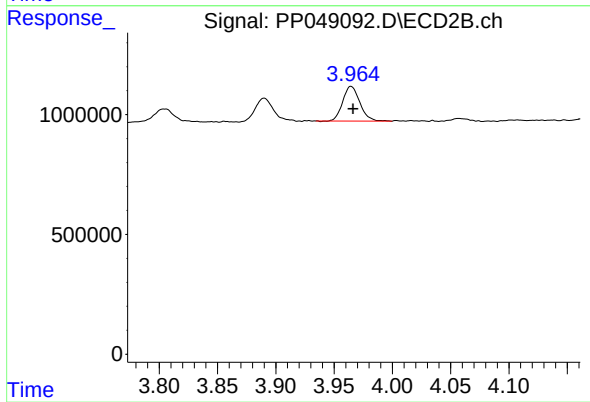

#10 AR-1221-3

R.T.: 3.965 min
Delta R.T.: -0.002 min
Response: 1492183
Conc: 20.29 ng/ml