

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
 Data File : PP049094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 19:09
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:51:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.593	26981248	49146135	18.980	19.193
2) SA Decachlor...	10.092	8.566	27619288	23202493	22.517	20.584
Target Compounds						
16) L4 AR-1242-1	5.521	4.668	996329	1686740	24.586	23.453
17) L4 AR-1242-2	5.543	4.687	1285809	2332050	22.326	23.025
18) L4 AR-1242-3	5.605	4.862	929049	1215263	25.661	21.800
19) L4 AR-1242-4	5.706	4.944	659828	1366209	22.429	24.679
20) L4 AR-1242-5	6.445	5.464	757251	1515373	22.692	21.766



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
Data File : PP049094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 19:09
Operator : YP\AJ
Sample : N3214-07
Misc : AR1242 MDL 25 PPB
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:51:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

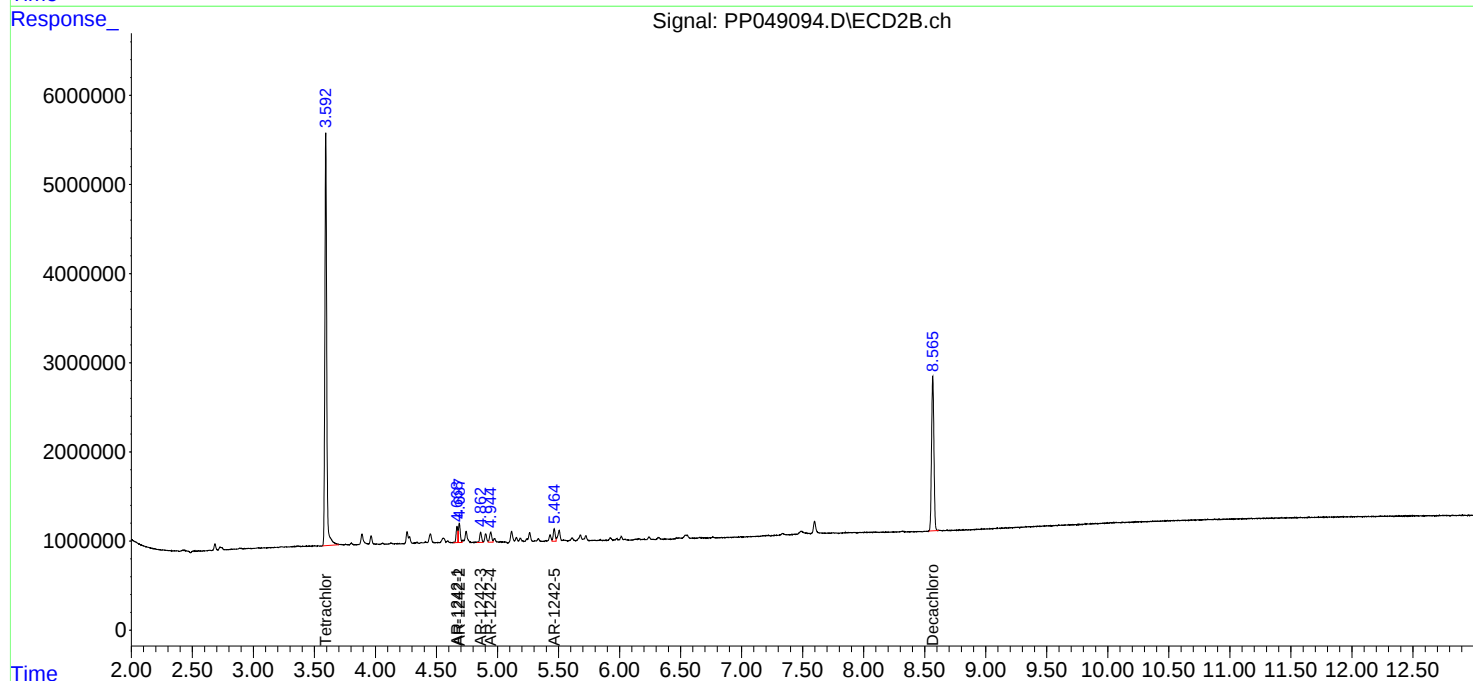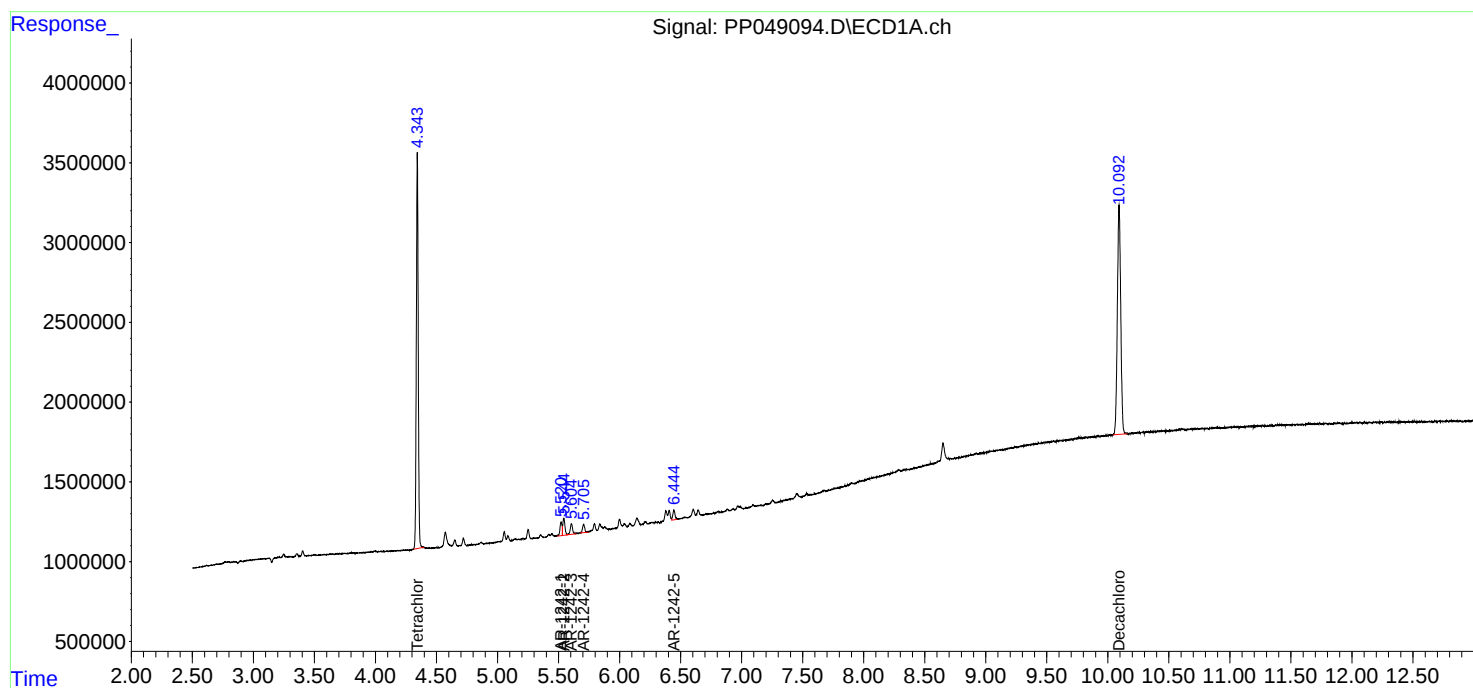


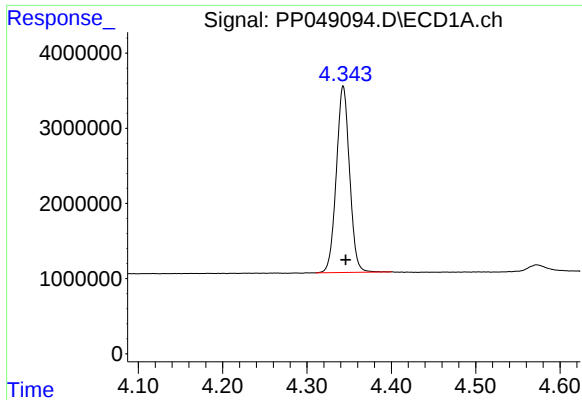

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.003 min
Response: 26981248
Conc: 18.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

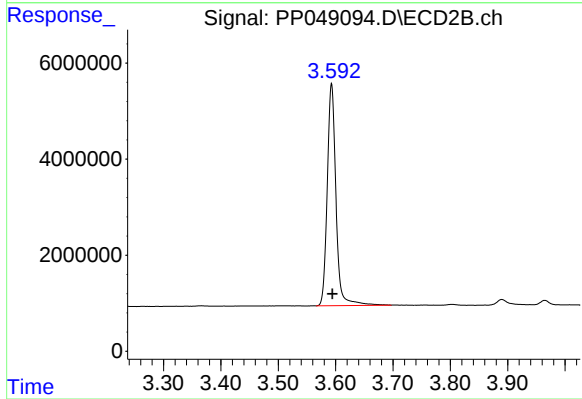


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: -0.001 min
Response: 49146135
Conc: 19.19 ng/ml

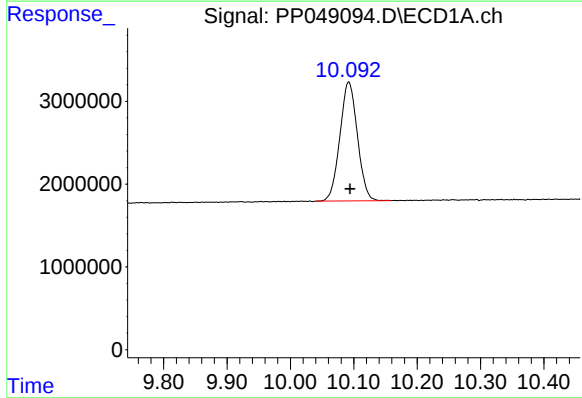


#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 27619288
Conc: 22.52 ng/ml

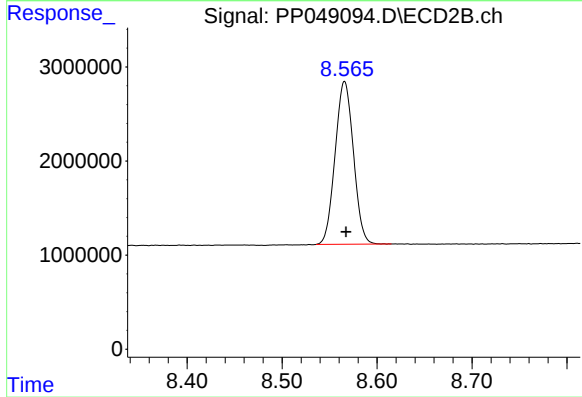

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.002 min
Response: 23202493
Conc: 20.58 ng/ml

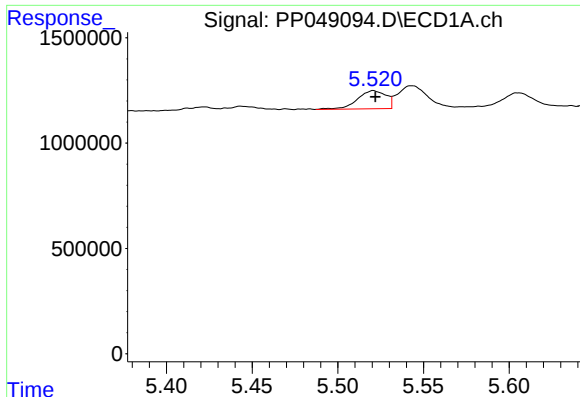

#16 AR-1242-1


R.T.: 5.521 min
Delta R.T.: -0.001 min
Response: 996329
Conc: 24.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

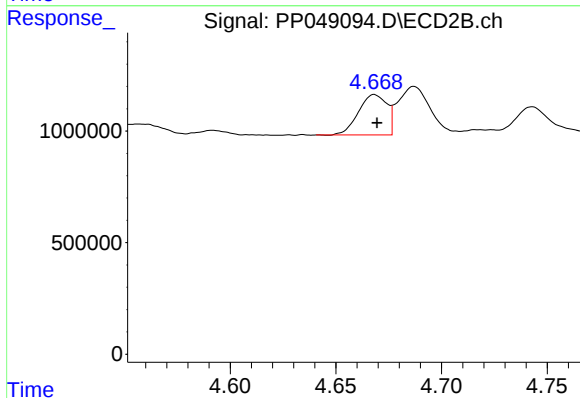


#16 AR-1242-1

R.T.: 4.668 min
Delta R.T.: -0.001 min
Response: 1686740
Conc: 23.45 ng/ml

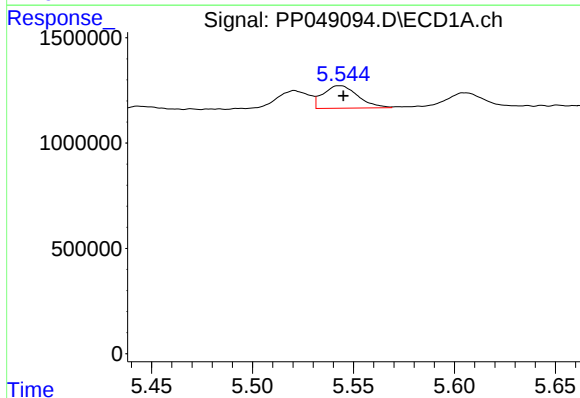


#17 AR-1242-2

R.T.: 5.543 min
Delta R.T.: -0.002 min
Response: 1285809
Conc: 22.33 ng/ml

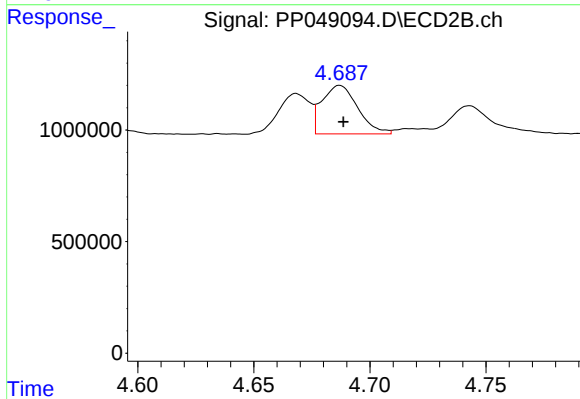

#17 AR-1242-2


R.T.: 4.687 min
Delta R.T.: -0.001 min
Response: 2332050
Conc: 23.03 ng/ml

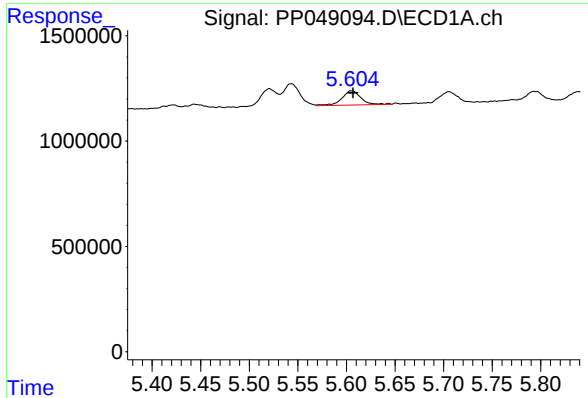

#18 AR-1242-3


R.T.: 5.605 min
Delta R.T.: -0.001 min
Response: 929049
Conc: 25.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

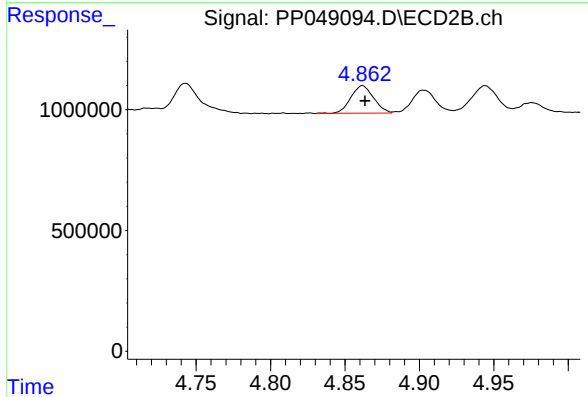


#18 AR-1242-3

R.T.: 4.862 min
Delta R.T.: -0.002 min
Response: 1215263
Conc: 21.80 ng/ml

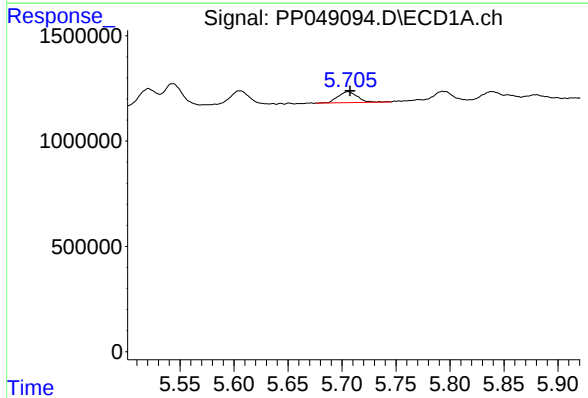


#19 AR-1242-4

R.T.: 5.706 min
Delta R.T.: -0.002 min
Response: 659828
Conc: 22.43 ng/ml

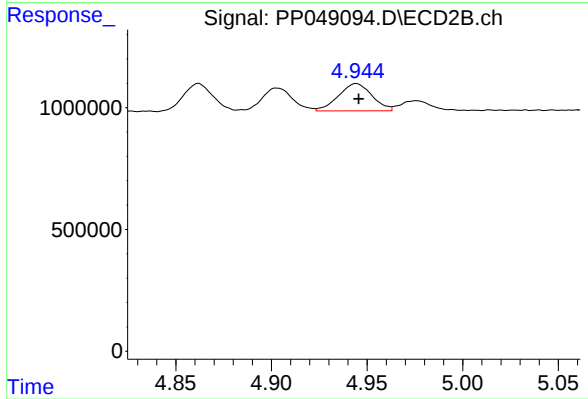

#19 AR-1242-4


R.T.: 4.944 min
Delta R.T.: -0.001 min
Response: 1366209
Conc: 24.68 ng/ml

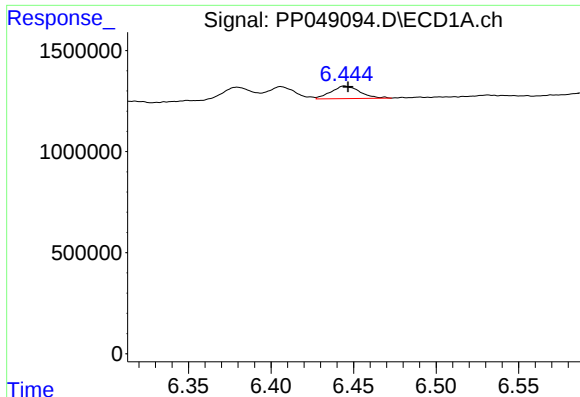

#20 AR-1242-5

R.T.: 6.445 min
Delta R.T.: -0.002 min
Response: 757251
Conc: 22.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

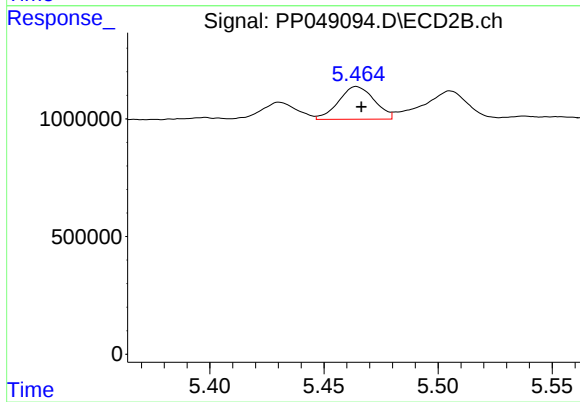

#20 AR-1242-5

R.T.: 5.464 min
Delta R.T.: -0.002 min
Response: 1515373
Conc: 21.77 ng/ml