

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
 Data File : PP049095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 19:25
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:51:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.593	27713877	50277315	19.495	19.635
2) SA Decachlor...	10.090	8.566	28085488	23699575	22.897	21.025
Target Compounds						
21) L5 AR-1248-1	5.520	4.668	772933	1307231	24.035	22.491
22) L5 AR-1248-2	5.794	4.903	1159506	1983644	24.943	29.558
23) L5 AR-1248-3	6.000	4.945	1261821	2151435	23.564	26.250
24) L5 AR-1248-4	6.407	5.114	1407366	2560078	22.773	25.951
25) L5 AR-1248-5	6.445	5.506	1312029	2817047	22.757	28.083



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
Data File : PP049095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 19:25
Operator : YP\AJ
Sample : N3214-07
Misc : AR1248 MDL 25 PPB
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:51:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

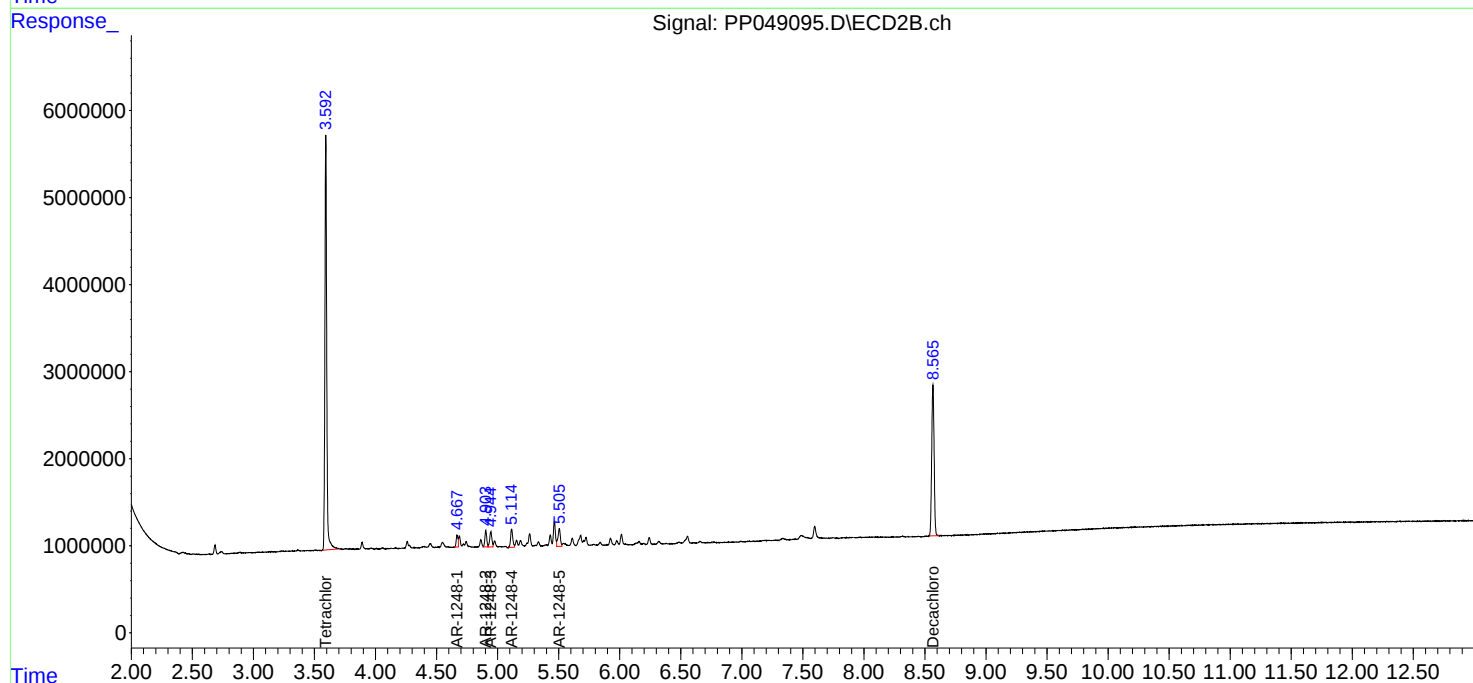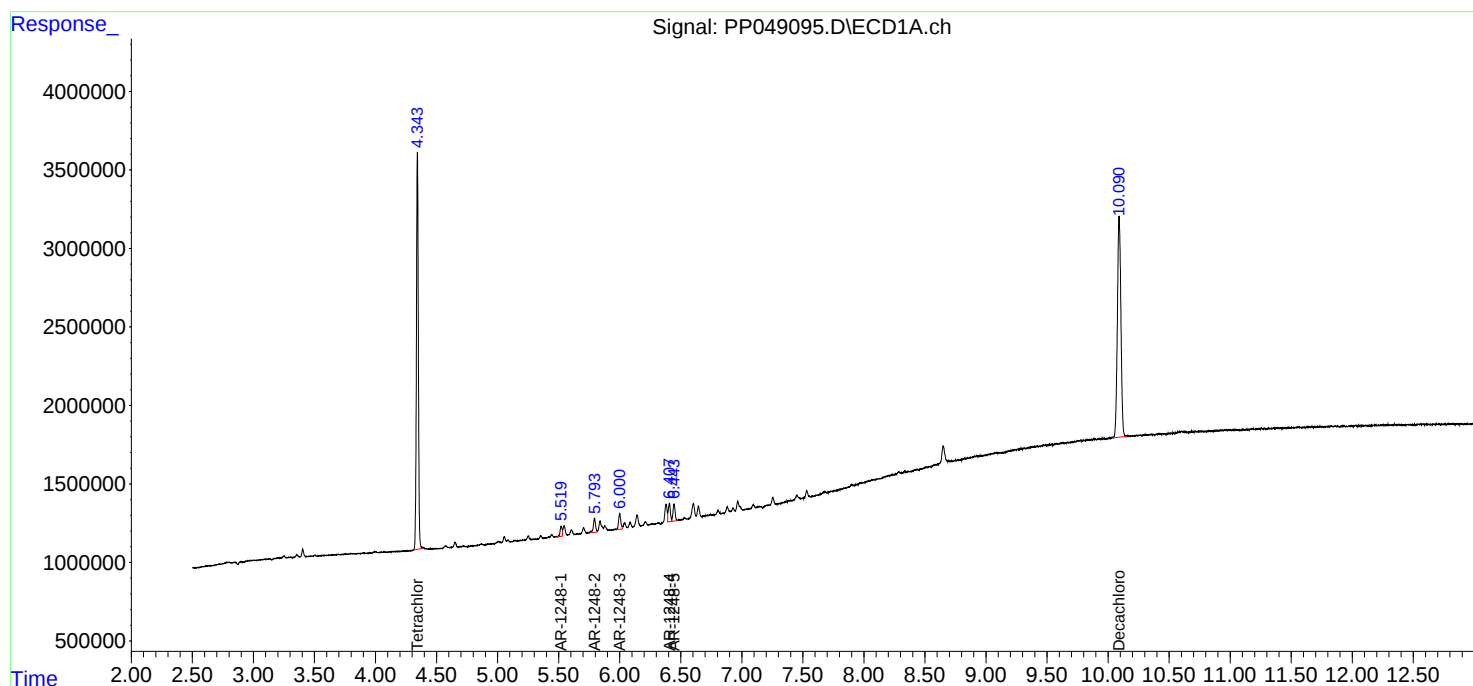


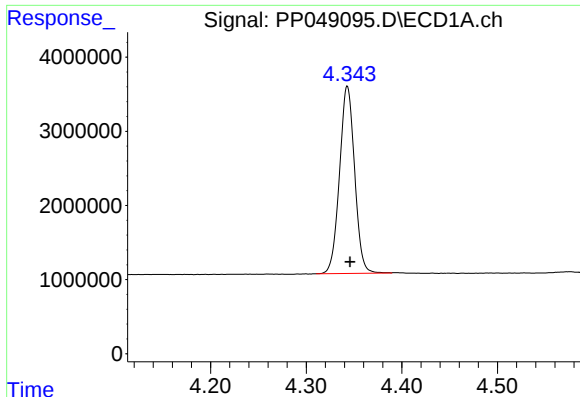

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.003 min
Response: 27713877
Conc: 19.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

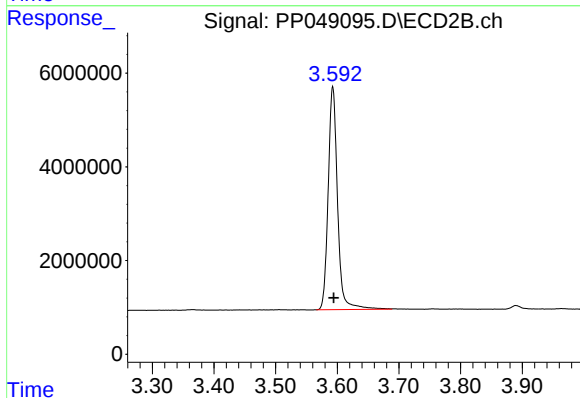


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: -0.001 min
Response: 50277315
Conc: 19.63 ng/ml

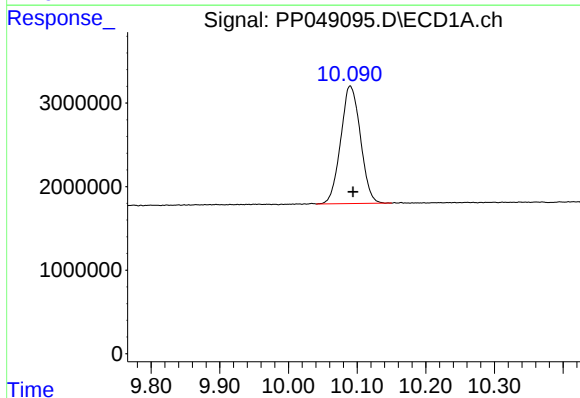


#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: -0.004 min
Response: 28085488
Conc: 22.90 ng/ml

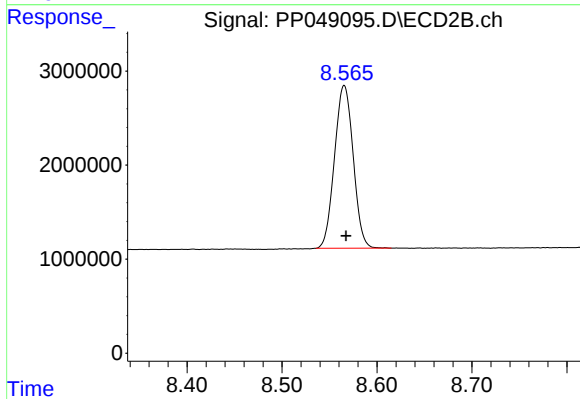

#2 Decachlorobiphenyl


R.T.: 8.566 min
Delta R.T.: -0.002 min
Response: 23699575
Conc: 21.02 ng/ml

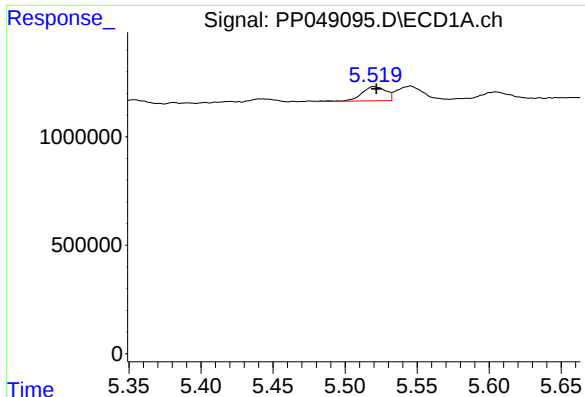

#21 AR-1248-1


R.T.: 5.520 min
Delta R.T.: -0.001 min
Response: 772933
Conc: 24.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

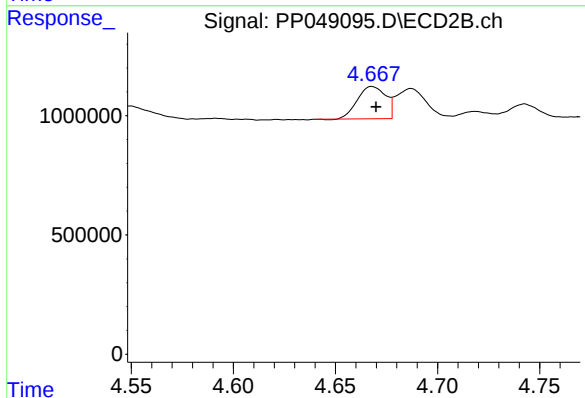


#21 AR-1248-1

R.T.: 4.668 min
Delta R.T.: -0.002 min
Response: 1307231
Conc: 22.49 ng/ml

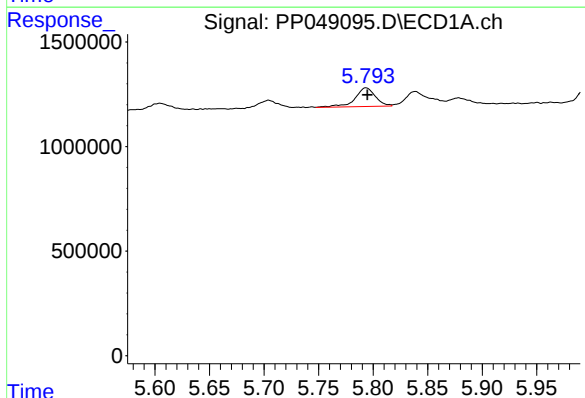


#22 AR-1248-2

R.T.: 5.794 min
Delta R.T.: -0.001 min
Response: 1159506
Conc: 24.94 ng/ml

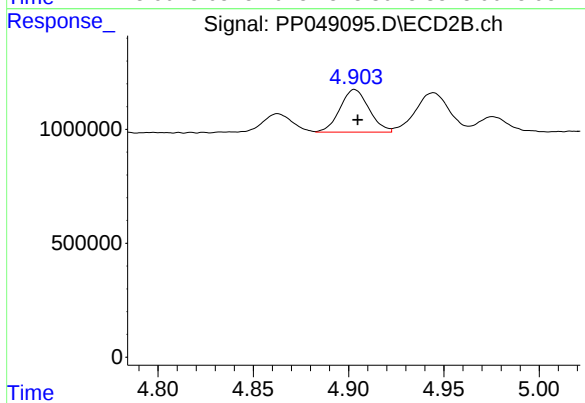

#22 AR-1248-2


R.T.: 4.903 min
Delta R.T.: -0.002 min
Response: 1983644
Conc: 29.56 ng/ml

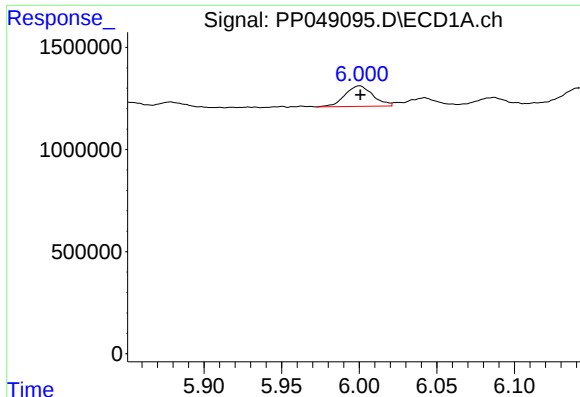

#23 AR-1248-3


R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 1261821
Conc: 23.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

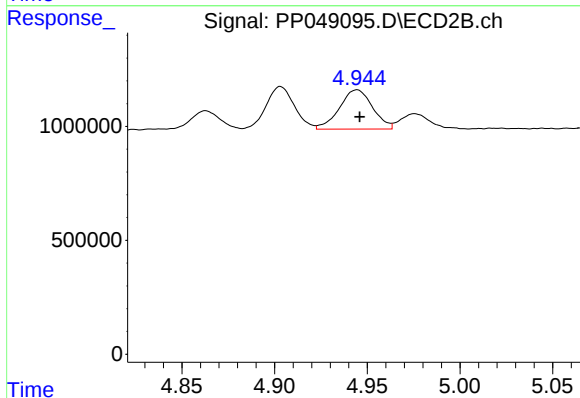


#23 AR-1248-3

R.T.: 4.945 min
Delta R.T.: -0.001 min
Response: 2151435
Conc: 26.25 ng/ml

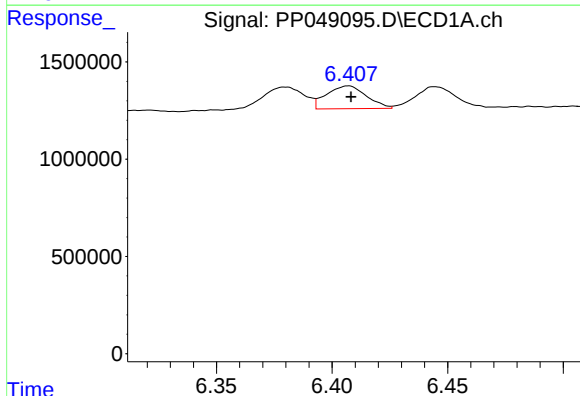


#24 AR-1248-4

R.T.: 6.407 min
Delta R.T.: -0.001 min
Response: 1407366
Conc: 22.77 ng/ml

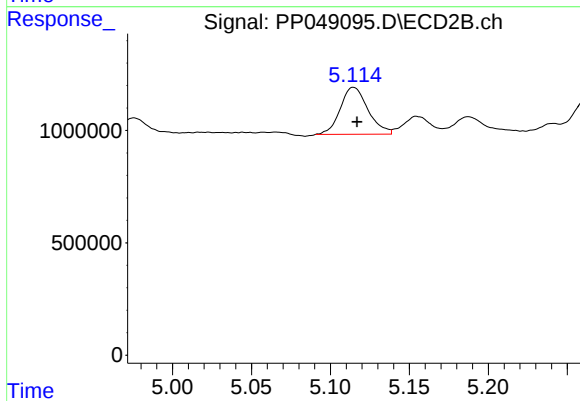

#24 AR-1248-4


R.T.: 5.114 min
Delta R.T.: -0.002 min
Response: 2560078
Conc: 25.95 ng/ml

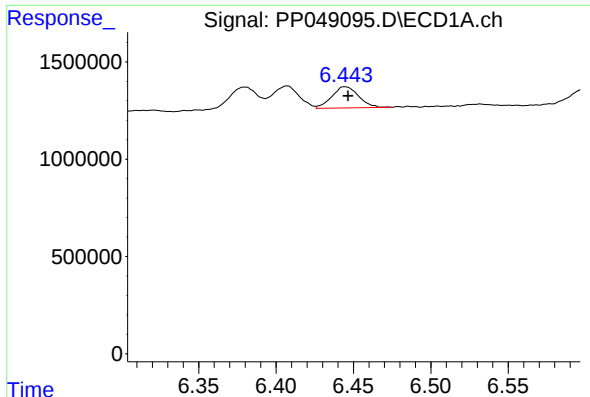

#25 AR-1248-5

R.T.: 6.445 min
Delta R.T.: -0.002 min
Response: 1312029
Conc: 22.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

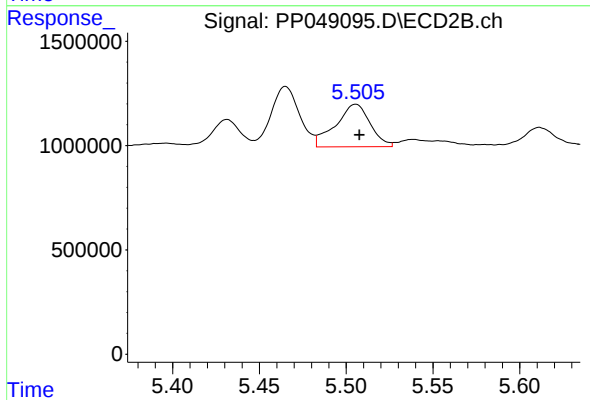

#25 AR-1248-5

R.T.: 5.506 min
Delta R.T.: -0.002 min
Response: 2817047
Conc: 28.08 ng/ml