

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
 Data File : PP049098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 20:15
 Operator : YP\AJ
 Sample : N3214-07
 Misc : AR1268 MDL 25PPB
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:52:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.593	27579543	49853251	19.401	19.469
2) SA Decachlor...	10.092	8.565	30230009	25218832	24.645	22.373
Target Compounds						
41) L9 AR-1268-1	8.598	7.478	5058718	6828781	26.937	31.743
42) L9 AR-1268-2	8.694	7.542	4526183	5664462	25.870	29.612
43) L9 AR-1268-3	8.916	7.748	3963515	4490680	27.668	29.485
44) L9 AR-1268-4	9.350	8.033	1850943	1703068	28.894	26.723
45) L9 AR-1268-5	9.760	8.317	11865750	10660946	25.727	26.719



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063022\
Data File : PP049098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 20:15
Operator : YP\AJ
Sample : N3214-07
Misc : AR1268 MDL 25PPB
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:52:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

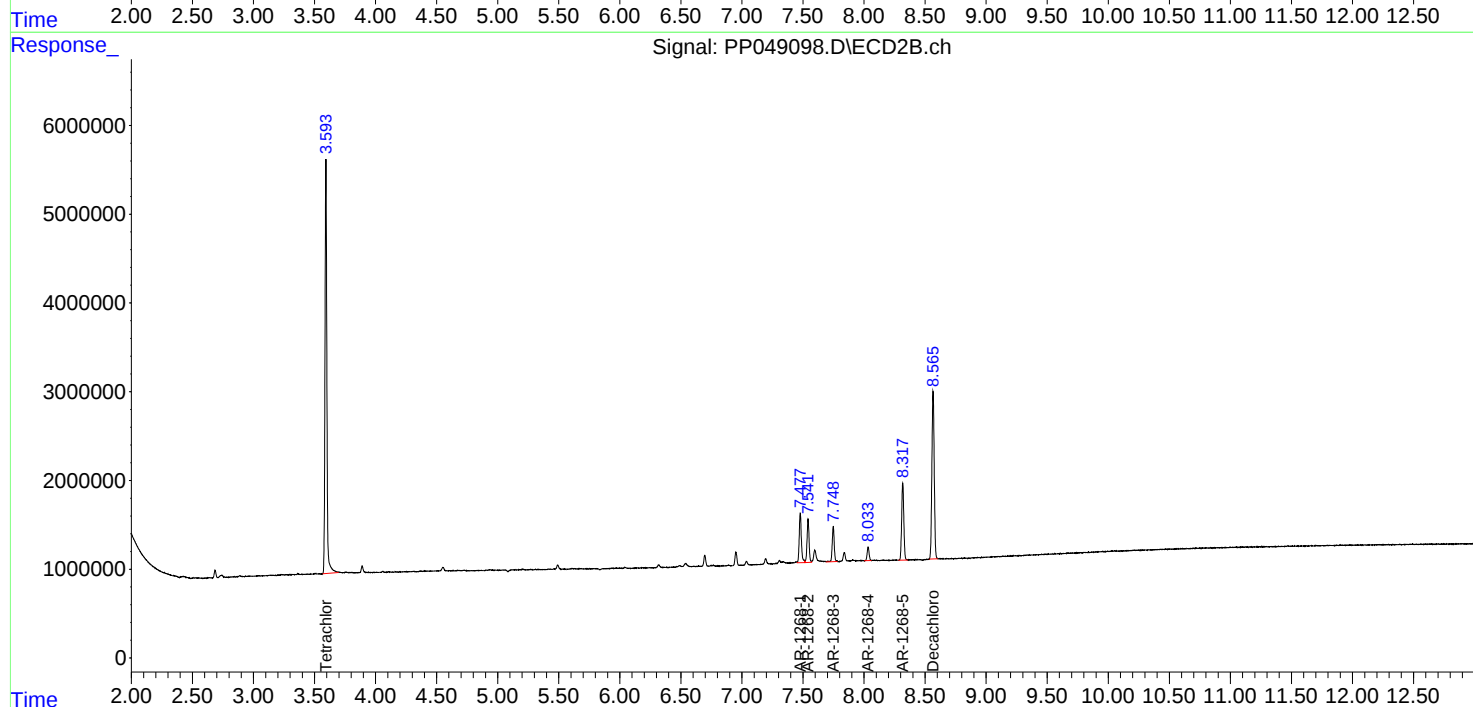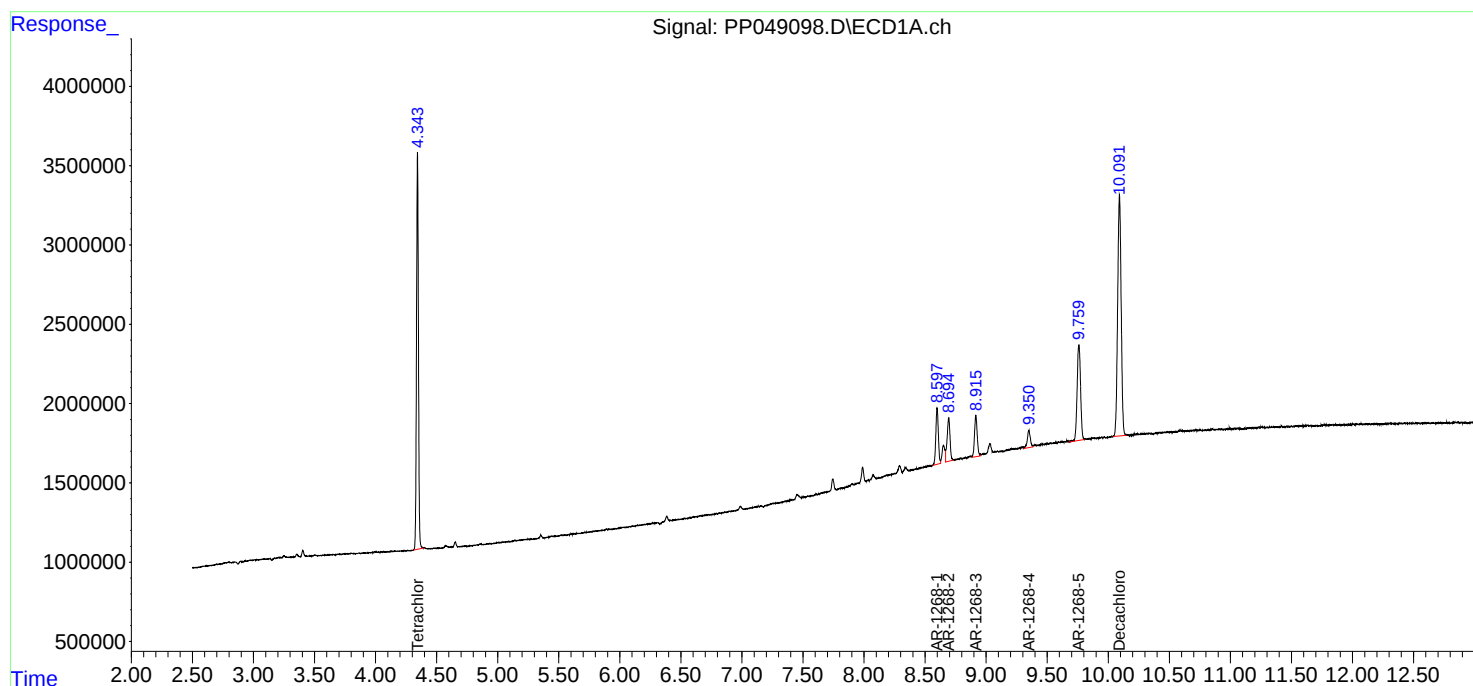


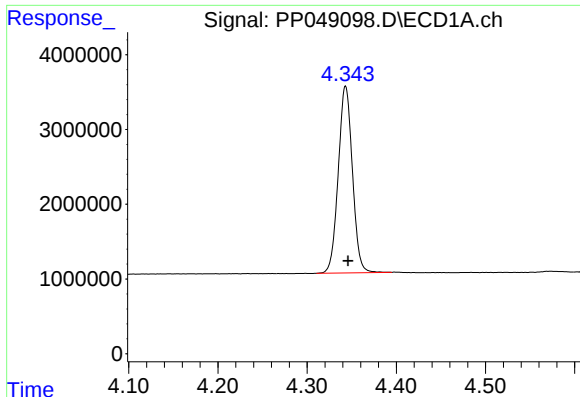

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.003 min
Response: 27579543
Conc: 19.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

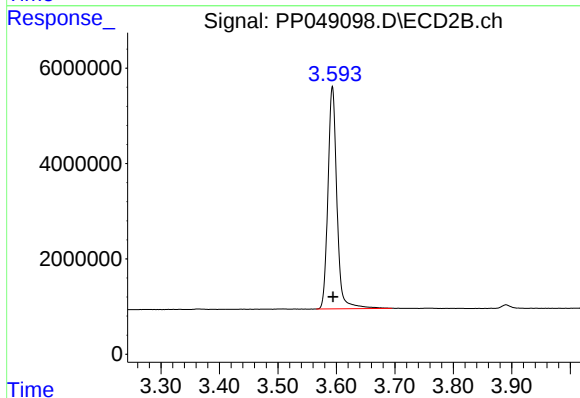


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 49853251
Conc: 19.47 ng/ml

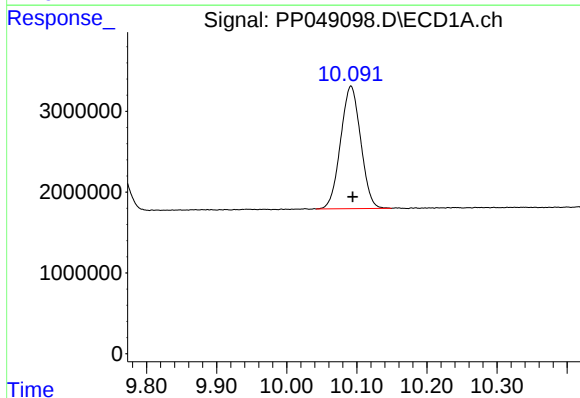


#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.003 min
Response: 30230009
Conc: 24.65 ng/ml

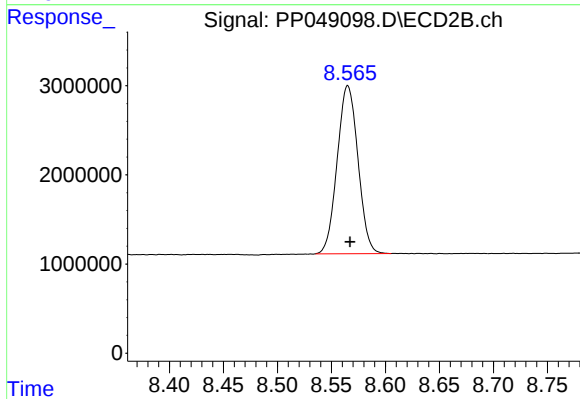

#2 Decachlorobiphenyl


R.T.: 8.565 min
Delta R.T.: -0.002 min
Response: 25218832
Conc: 22.37 ng/ml

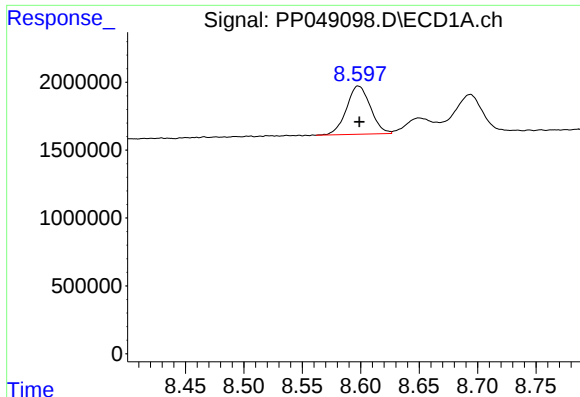

#41 AR-1268-1


R.T.: 8.598 min
Delta R.T.: 0.000 min
Response: 5058718
Conc: 26.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

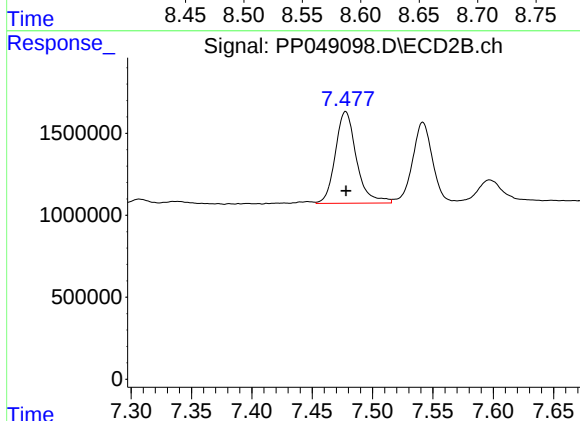


#41 AR-1268-1

R.T.: 7.478 min
Delta R.T.: 0.000 min
Response: 6828781
Conc: 31.74 ng/ml

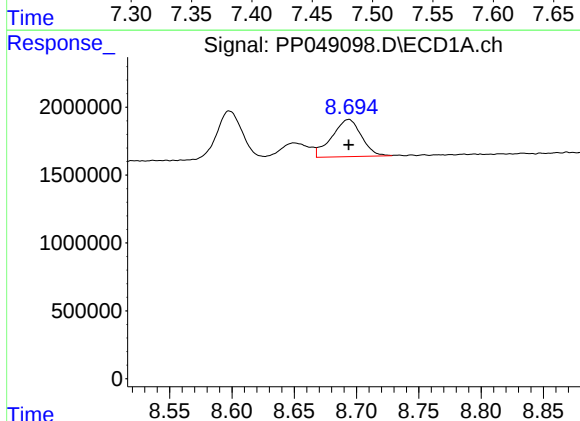


#42 AR-1268-2

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 4526183
Conc: 25.87 ng/ml

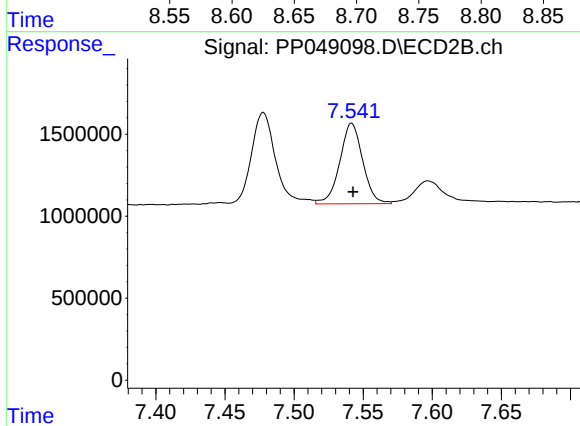

#42 AR-1268-2


R.T.: 7.542 min
Delta R.T.: 0.000 min
Response: 5664462
Conc: 29.61 ng/ml

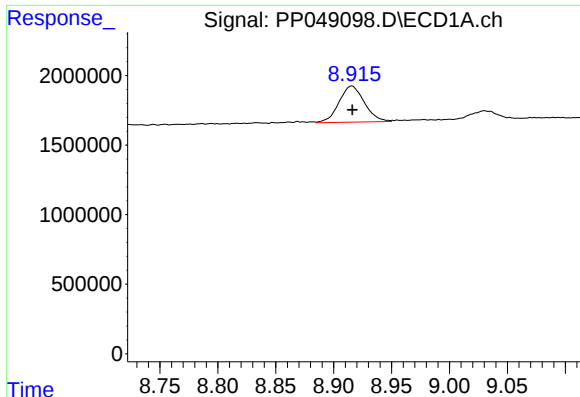

#43 AR-1268-3


R.T.: 8.916 min
Delta R.T.: 0.000 min
Response: 3963515
Conc: 27.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

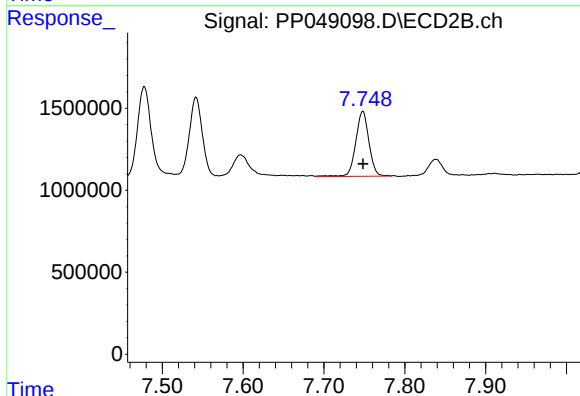


#43 AR-1268-3

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 4490680
Conc: 29.48 ng/ml

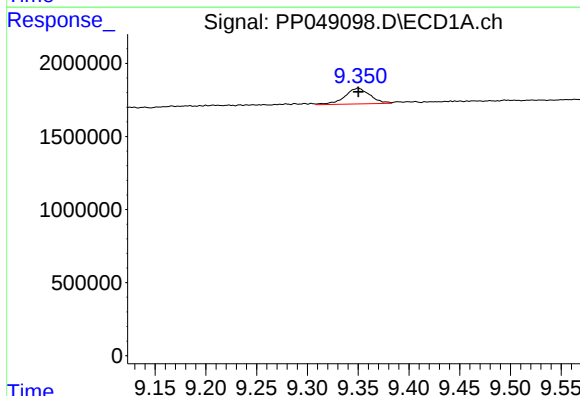


#44 AR-1268-4

R.T.: 9.350 min
Delta R.T.: 0.000 min
Response: 1850943
Conc: 28.89 ng/ml

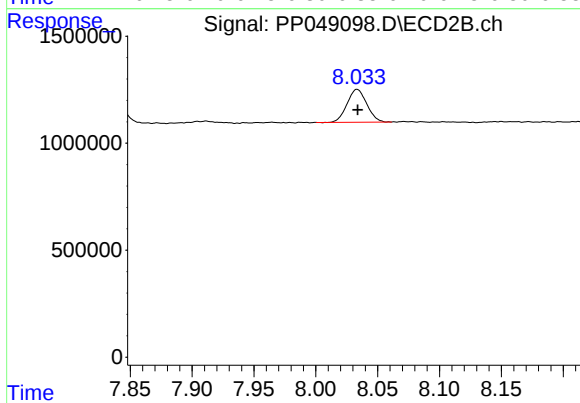

#44 AR-1268-4


R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 1703068
Conc: 26.72 ng/ml

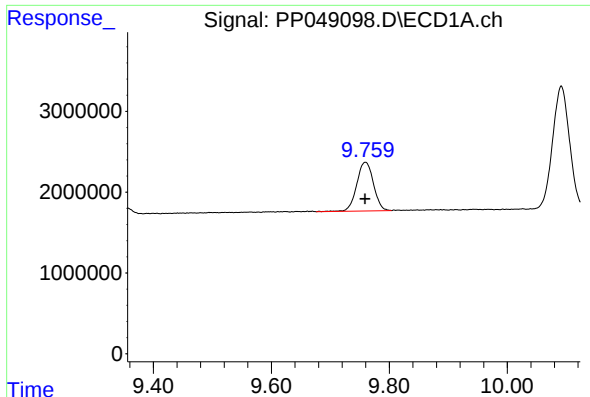

#45 AR-1268-5

R.T.: 9.760 min
Delta R.T.: 0.000 min
Response: 11865750
Conc: 25.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

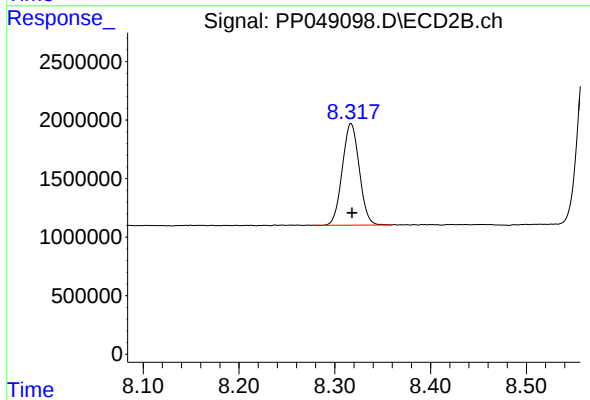

#45 AR-1268-5

R.T.: 8.317 min
Delta R.T.: -0.001 min
Response: 10660946
Conc: 26.72 ng/ml