

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
 Data File : PP073373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2025 11:01
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 14:31:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.526f	3.817f	118356	69309	0.056	0.038 #
2)	SA Decachlor...	10.196	8.808	371701	62877	0.218	0.047 #
Target Compounds							
3)	L1 AR-1016-1	5.634	4.865	439261	289310	6.044	4.210 #
4)	L1 AR-1016-2	5.666	4.865	180660	289310	1.737	2.875 #
5)	L1 AR-1016-3	5.732	5.055	203640	236322	3.116	4.319 #
6)	L1 AR-1016-4	5.841	5.100	273393	405320	5.229	9.098 #
7)	L1 AR-1016-5	6.129	5.306	1037501	247647	20.748	4.480 #
8)	L2 AR-1221-1	4.688	4.000	109308	212797	4.433	7.919 #
9)	L2 AR-1221-2	4.789	4.102	185153	170463	9.176	8.445
10)	L2 AR-1221-3	4.846	4.165	115977	57241	1.884	0.975 #
11)	L3 AR-1232-1	4.846	4.165	115977	57241	2.470	1.256 #
12)	L3 AR-1232-2	5.403	4.865	60013	289310	2.683	6.254 #
13)	L3 AR-1232-3	5.666	5.055	180660	236322	3.501	9.623 #
14)	L3 AR-1232-4	5.841	5.181	273393	668375	10.592	30.907 #
15)	L3 AR-1232-5	5.924	5.306	393146	247647	11.022	10.834
16)	L4 AR-1242-1	5.634	4.865	439261	289310	7.517	5.239 #
17)	L4 AR-1242-2	5.666	4.865	180660	289310	2.087	3.640 #
18)	L4 AR-1242-3	5.732	5.055	203640	236322	3.864	5.457 #
19)	L4 AR-1242-4	5.841	5.181f	273393	668375	6.219	16.104 #
20)	L4 AR-1242-5	6.565	5.651	607216	435302	12.252	8.278 #
21)	L5 AR-1248-1	5.634	4.865	439261	289310	9.234	6.637 #
22)	L5 AR-1248-2	5.924	5.100	393146	405320	6.715	6.917
23)	L5 AR-1248-3	6.129	5.181f	1037501	668375	15.901	11.039 #
24)	L5 AR-1248-4	6.523	5.306	1063970	247647	12.508	3.537 #
25)	L5 AR-1248-5	6.565	5.719	607216	79932	7.255	1.125 #
26)	L6 AR-1254-1	6.502	5.651	414657	435302	4.926	3.970
27)	L6 AR-1254-2	6.696	5.831	9904233	8396294	78.981	88.806
28)	L6 AR-1254-3	7.072	6.228	6983781	3186699	53.226	21.598 #
29)	L6 AR-1254-4	7.314f	6.456	968683	376697	8.087	3.879 #
30)	L6 AR-1254-5	7.780	6.854	539.7E6	515.6E6	4723.360	3966.984
31)	L7 AR-1260-1	7.211	6.369	870983	122270	9.874	1.291 #
32)	L7 AR-1260-2	7.468	6.535	1029.8E6	4798026	7578.444	41.207 #
33)	L7 AR-1260-3	7.866	6.661	649041	-100236	5.686	N.D. #
34)	L7 AR-1260-4	8.111f	7.165	359730	69687	3.491	0.794 #
35)	L7 AR-1260-5	8.386	7.398	96670	153221	0.402	0.718 #
36)	L8 AR-1262-1	8.030f	6.854f	699792	515.6E6	4.728	3568.707 #
37)	L8 AR-1262-2	8.386	7.165	96670	69687	0.305	0.570 #
38)	L8 AR-1262-3	8.726	7.668	773552	68527	3.615	0.608 #
39)	L8 AR-1262-4	8.794	7.744	238125	152347	1.511	0.831 #
40)	L8 AR-1262-5	9.435	8.253	247829	181093	2.215	2.092
41)	L9 AR-1268-1	8.726	7.668	773552	68527	2.163	0.239 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
 Data File : PP073373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2025 11:01
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 14:31:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.794	7.744	238125	152347	0.781	0.593
43) L9	AR-1268-3	9.016	7.951	533703	308382	2.010	1.428 #
44) L9	AR-1268-4	9.435	8.253	247829	181093	2.118	1.923
45) L9	AR-1268-5	9.878	8.565	112888	29014	0.153	0.050 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
Data File : PP073373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2025 11:01
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 14:31:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

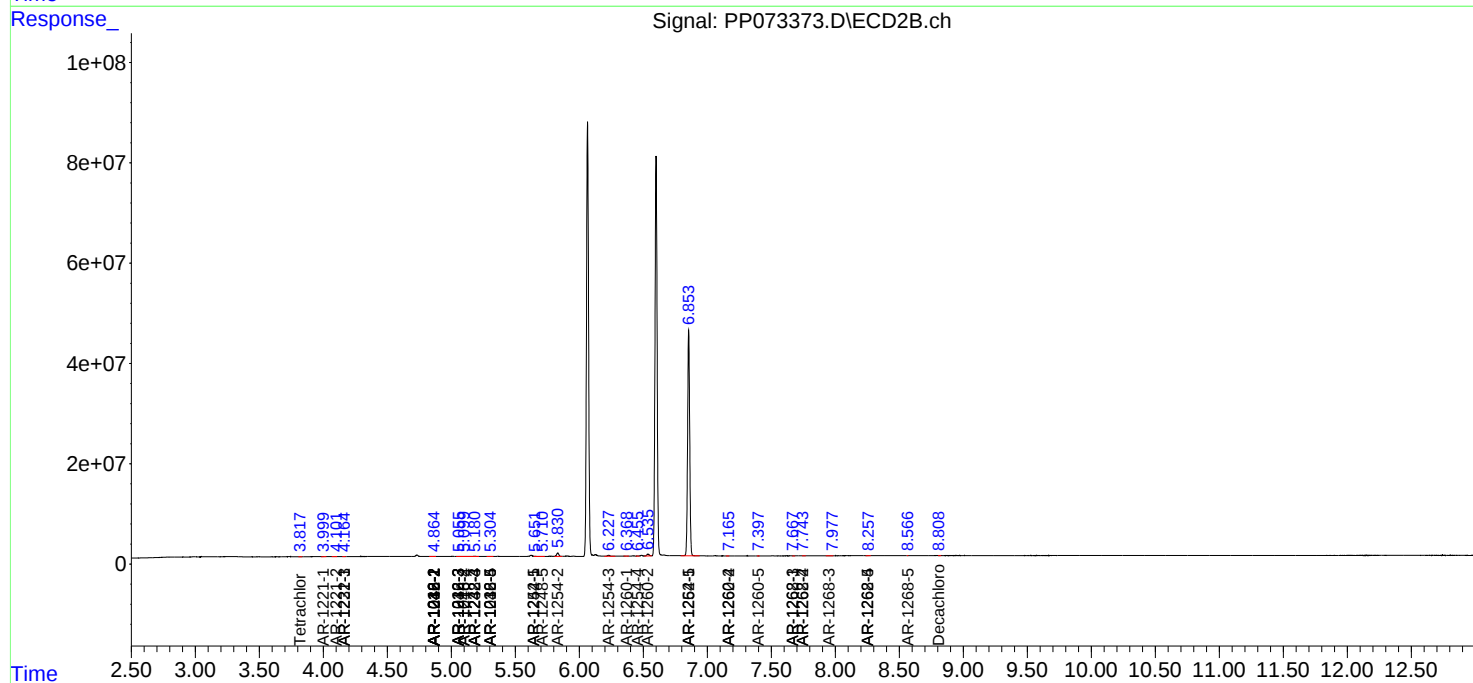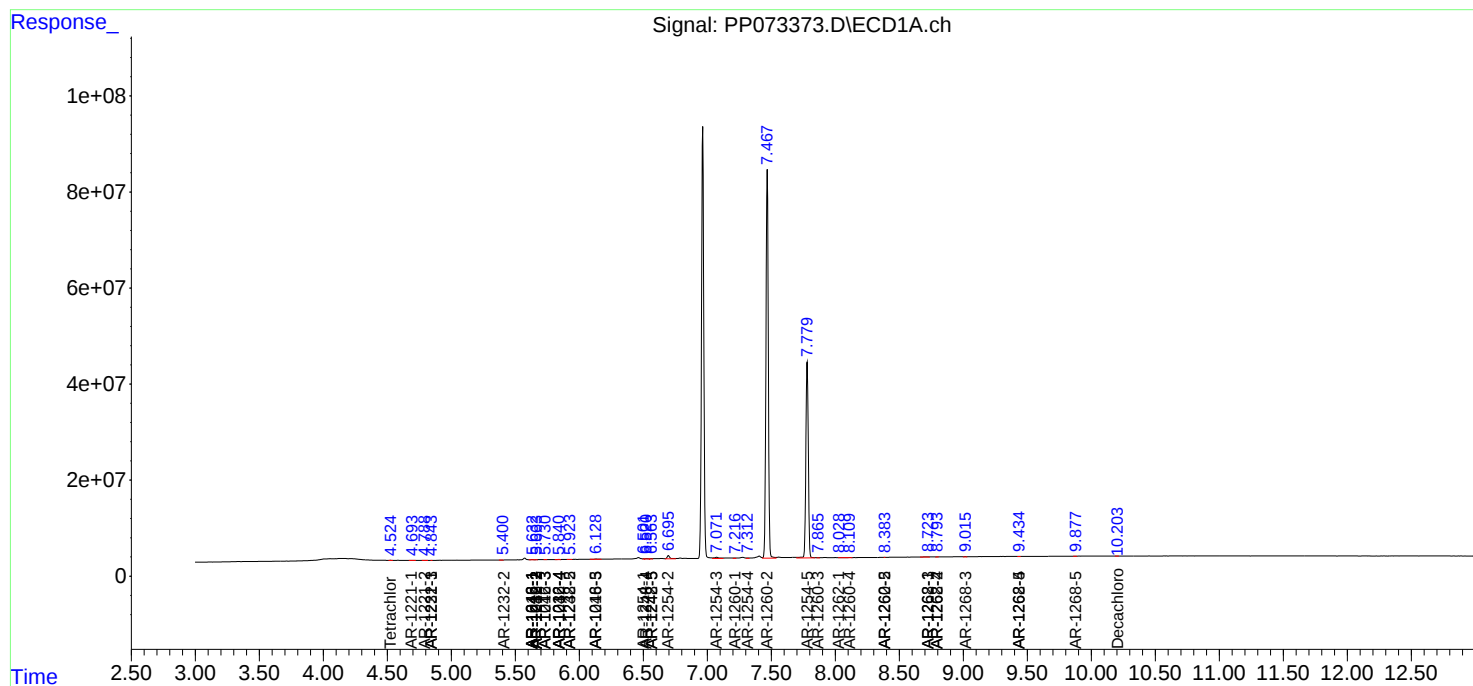


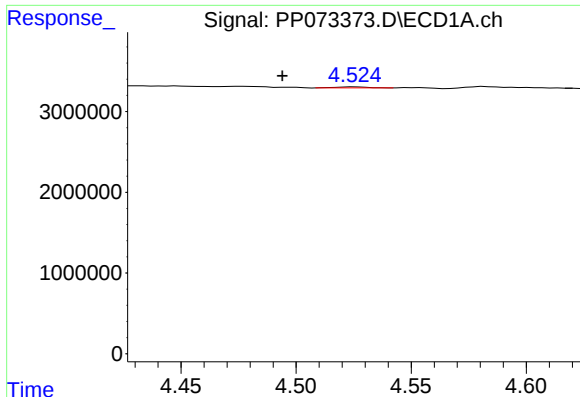

#1 Tetrachloro-m-xylene


R.T.: 4.526 min
Delta R.T.: 0.032 min
Response: 118356
Conc: 0.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

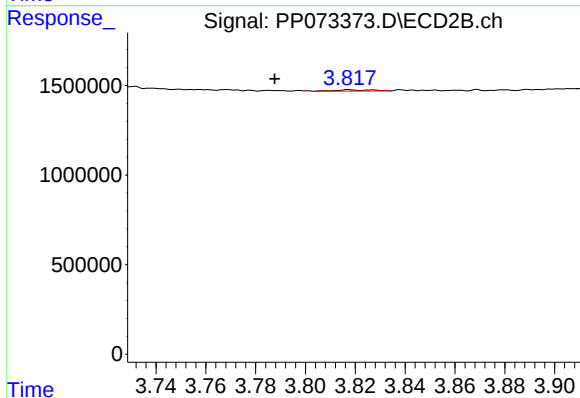


#1 Tetrachloro-m-xylene

R.T.: 3.817 min
Delta R.T.: 0.030 min
Response: 69309
Conc: 0.04 ng/ml

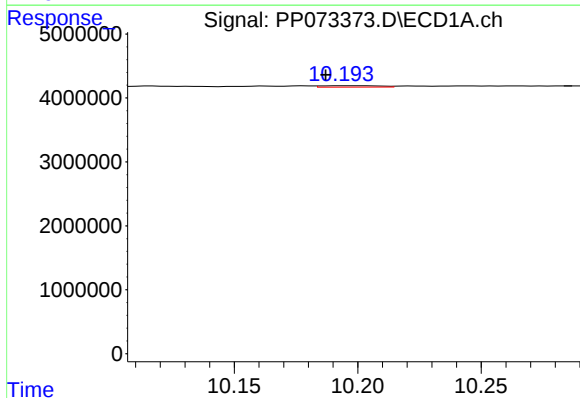


#2 Decachlorobiphenyl

R.T.: 10.196 min
Delta R.T.: 0.009 min
Response: 371701
Conc: 0.22 ng/ml

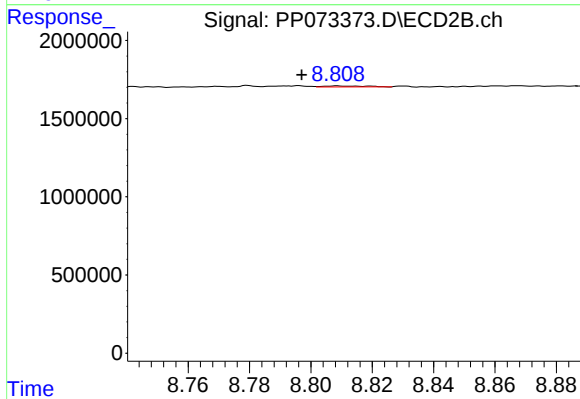

#2 Decachlorobiphenyl


R.T.: 8.808 min
Delta R.T.: 0.011 min
Response: 62877
Conc: 0.05 ng/ml

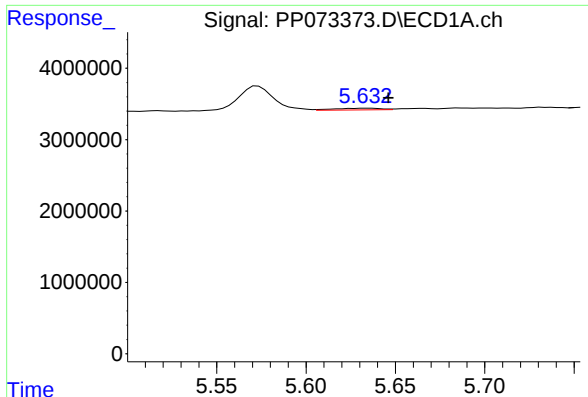

#3 AR-1016-1


R.T.: 5.634 min
Delta R.T.: -0.012 min
Response: 439261
Conc: 6.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

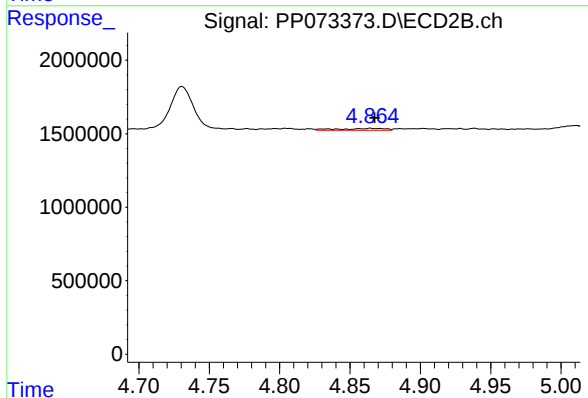


#3 AR-1016-1

R.T.: 4.865 min
Delta R.T.: -0.003 min
Response: 289310
Conc: 4.21 ng/ml

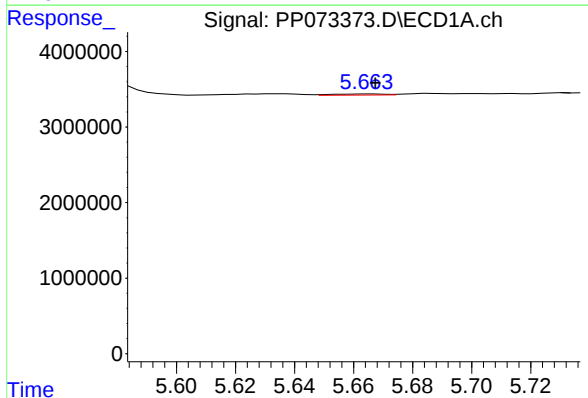


#4 AR-1016-2

R.T.: 5.666 min
Delta R.T.: -0.001 min
Response: 180660
Conc: 1.74 ng/ml

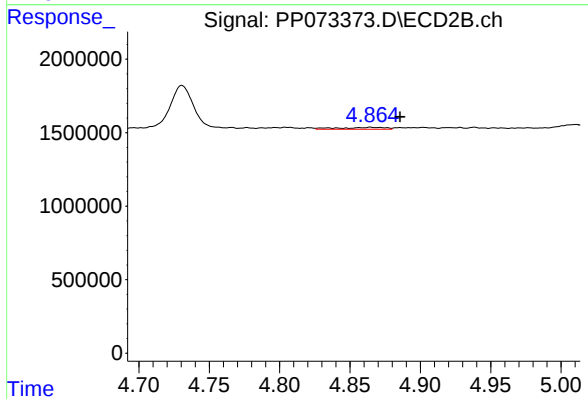

#4 AR-1016-2


R.T.: 4.865 min
Delta R.T.: -0.021 min
Response: 289310
Conc: 2.87 ng/ml

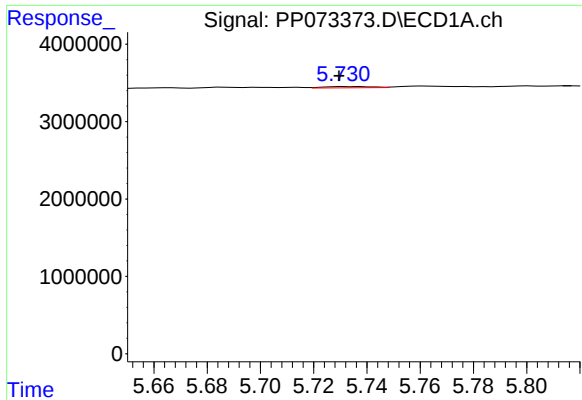

#5 AR-1016-3


R.T.: 5.732 min
Delta R.T.: 0.003 min
Response: 203640
Conc: 3.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

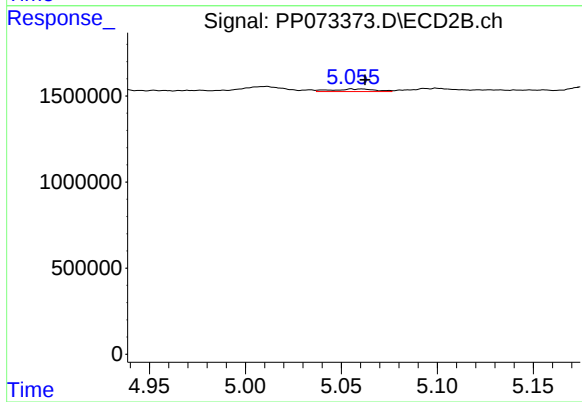


#5 AR-1016-3

R.T.: 5.055 min
Delta R.T.: -0.007 min
Response: 236322
Conc: 4.32 ng/ml

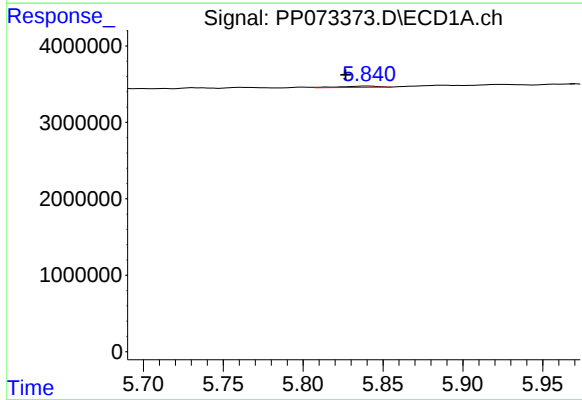


#6 AR-1016-4

R.T.: 5.841 min
Delta R.T.: 0.014 min
Response: 273393
Conc: 5.23 ng/ml

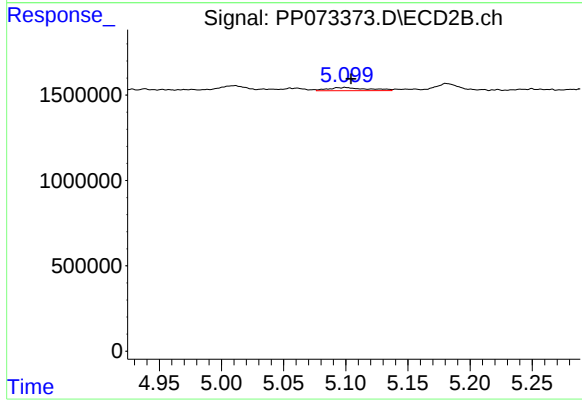

#6 AR-1016-4


R.T.: 5.100 min
Delta R.T.: -0.004 min
Response: 405320
Conc: 9.10 ng/ml

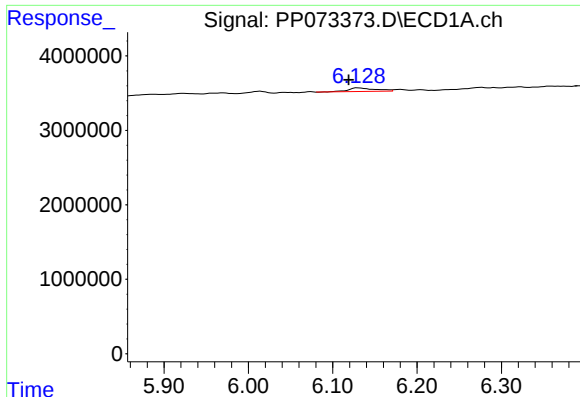

#7 AR-1016-5


R.T.: 6.129 min
Delta R.T.: 0.010 min
Response: 1037501
Conc: 20.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

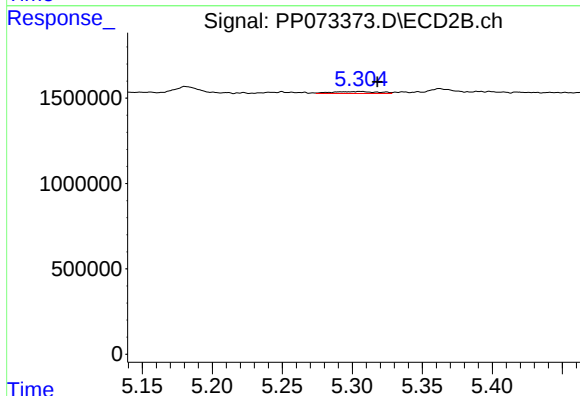


#7 AR-1016-5

R.T.: 5.306 min
Delta R.T.: -0.012 min
Response: 247647
Conc: 4.48 ng/ml

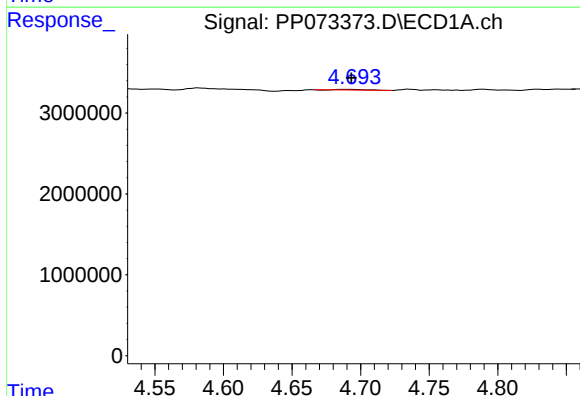


#8 AR-1221-1

R.T.: 4.688 min
Delta R.T.: -0.005 min
Response: 109308
Conc: 4.43 ng/ml

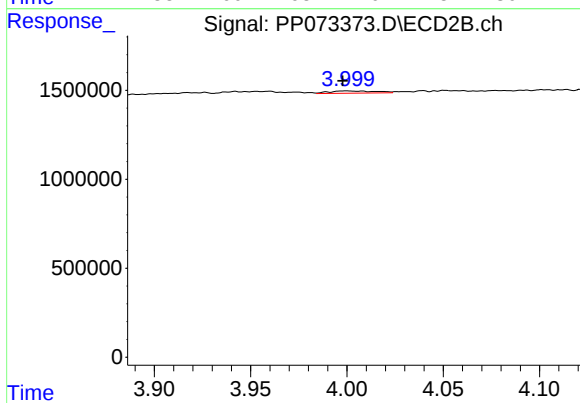

#8 AR-1221-1


R.T.: 4.000 min
Delta R.T.: 0.002 min
Response: 212797
Conc: 7.92 ng/ml

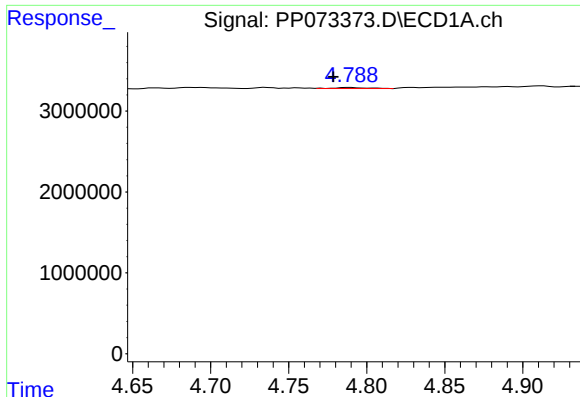

#9 AR-1221-2


R.T.: 4.789 min
Delta R.T.: 0.011 min
Response: 185153
Conc: 9.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

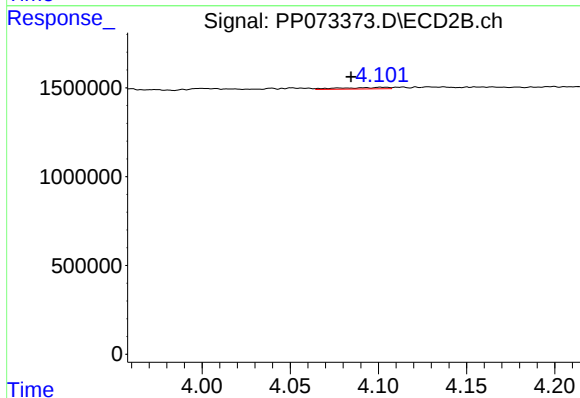


#9 AR-1221-2

R.T.: 4.102 min
Delta R.T.: 0.017 min
Response: 170463
Conc: 8.44 ng/ml

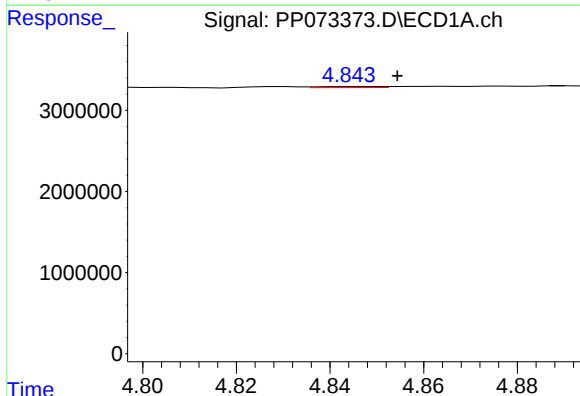


#10 AR-1221-3

R.T.: 4.846 min
Delta R.T.: -0.009 min
Response: 115977
Conc: 1.88 ng/ml

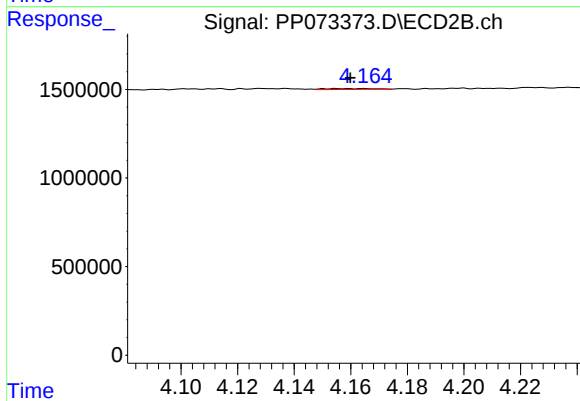

#10 AR-1221-3


R.T.: 4.165 min
Delta R.T.: 0.005 min
Response: 57241
Conc: 0.97 ng/ml

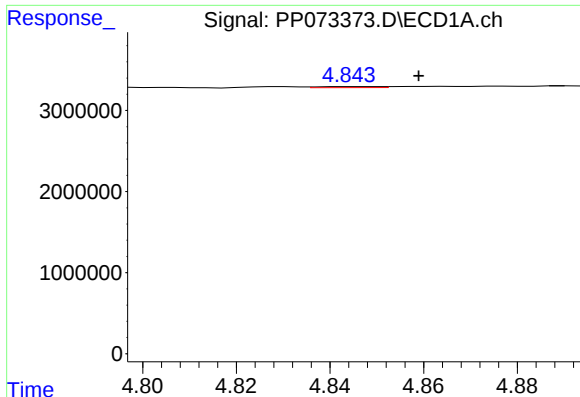

#11 AR-1232-1


R.T.: 4.846 min
Delta R.T.: -0.013 min
Response: 115977
Conc: 2.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

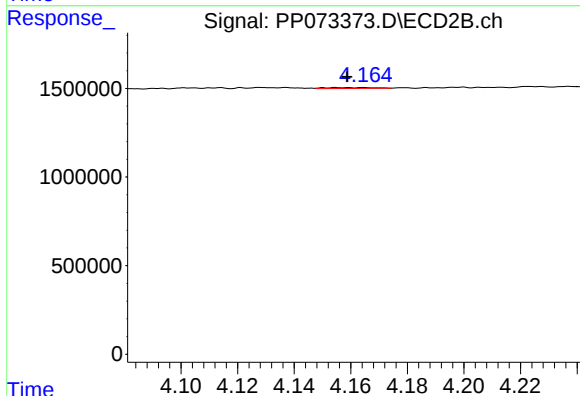


#11 AR-1232-1

R.T.: 4.165 min
Delta R.T.: 0.006 min
Response: 57241
Conc: 1.26 ng/ml

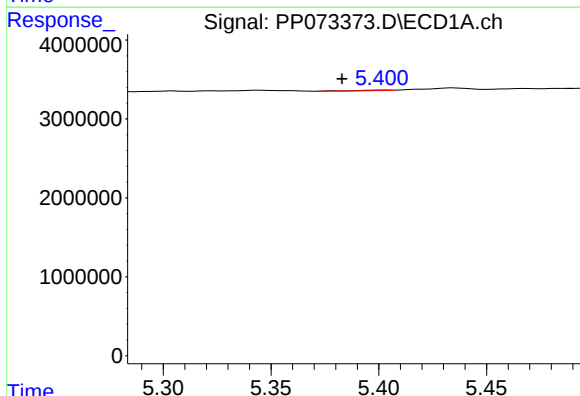


#12 AR-1232-2

R.T.: 5.403 min
Delta R.T.: 0.020 min
Response: 60013
Conc: 2.68 ng/ml

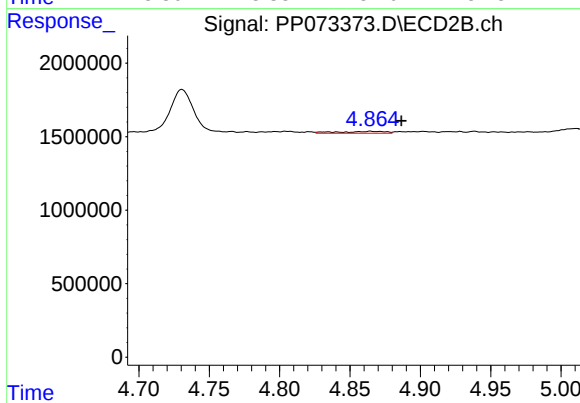

#12 AR-1232-2


R.T.: 4.865 min
Delta R.T.: -0.022 min
Response: 289310
Conc: 6.25 ng/ml

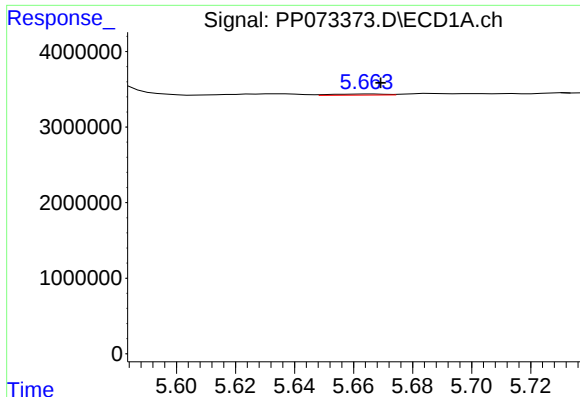

#13 AR-1232-3


R.T.: 5.666 min
Delta R.T.: -0.003 min
Response: 180660
Conc: 3.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

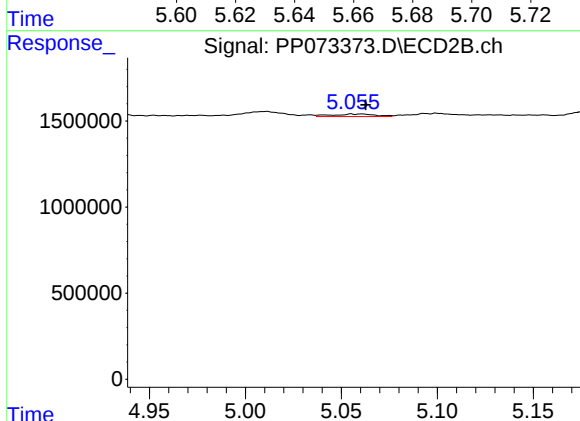


#13 AR-1232-3

R.T.: 5.055 min
Delta R.T.: -0.007 min
Response: 236322
Conc: 9.62 ng/ml

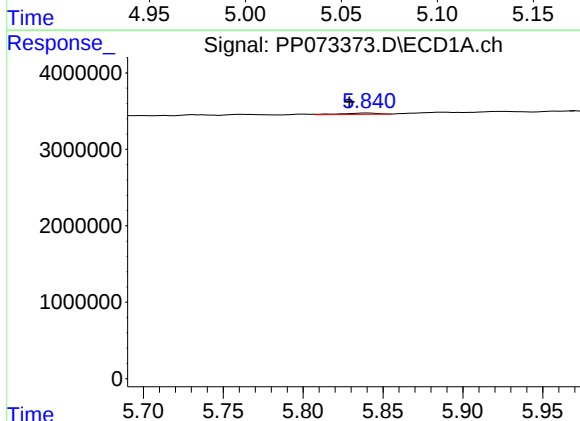


#14 AR-1232-4

R.T.: 5.841 min
Delta R.T.: 0.012 min
Response: 273393
Conc: 10.59 ng/ml

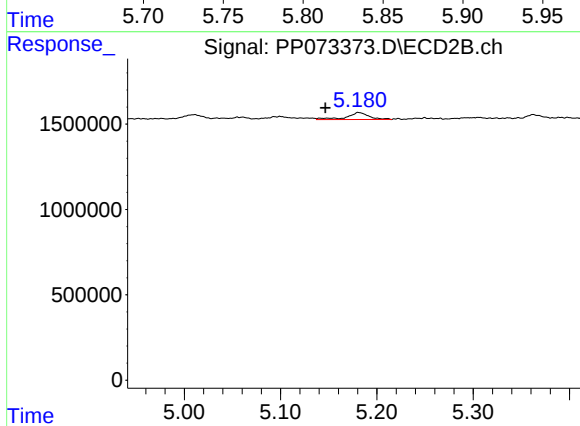

#14 AR-1232-4


R.T.: 5.181 min
Delta R.T.: 0.034 min
Response: 668375
Conc: 30.91 ng/ml

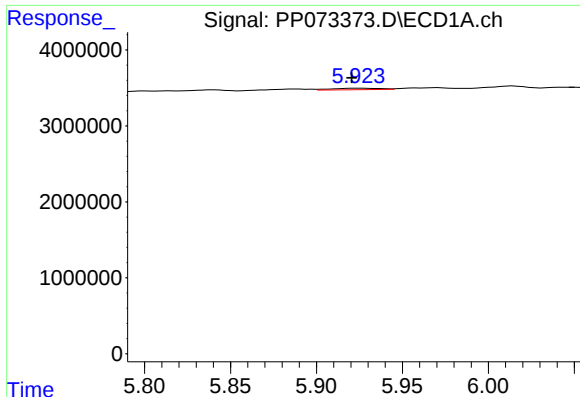

#15 AR-1232-5


R.T.: 5.924 min
Delta R.T.: 0.004 min
Response: 393146
Conc: 11.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

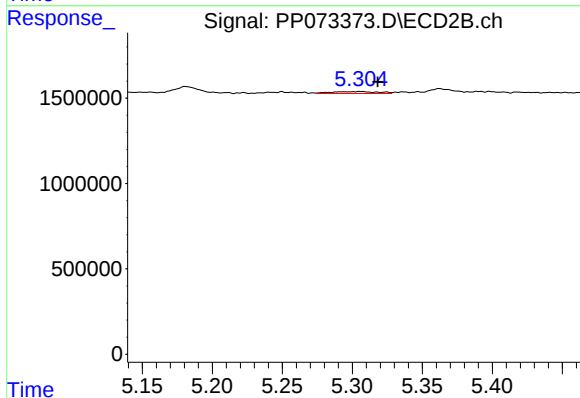


#15 AR-1232-5

R.T.: 5.306 min
Delta R.T.: -0.012 min
Response: 247647
Conc: 10.83 ng/ml

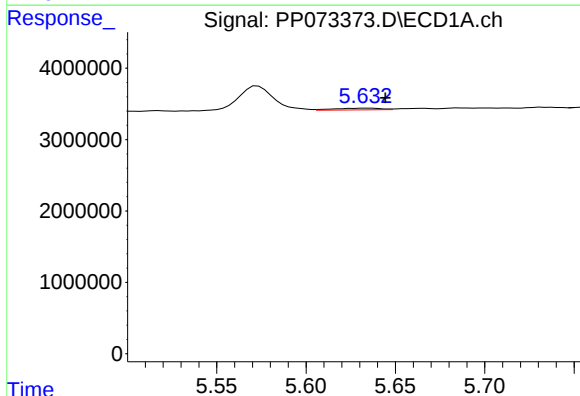


#16 AR-1242-1

R.T.: 5.634 min
Delta R.T.: -0.010 min
Response: 439261
Conc: 7.52 ng/ml

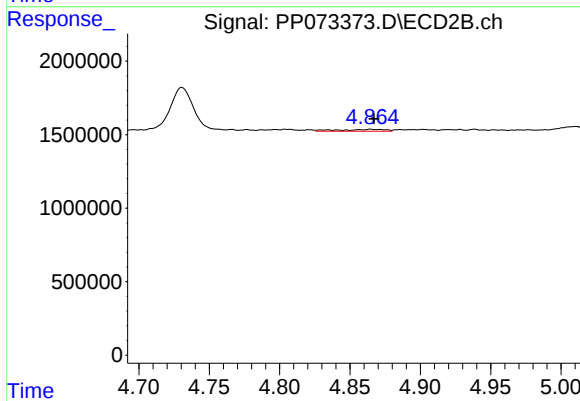

#16 AR-1242-1


R.T.: 4.865 min
Delta R.T.: -0.002 min
Response: 289310
Conc: 5.24 ng/ml

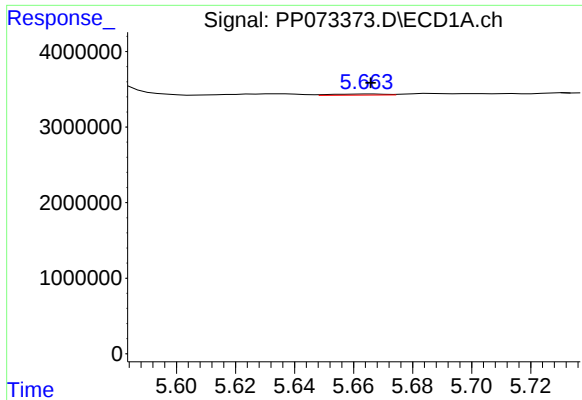

#17 AR-1242-2


R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 180660
Conc: 2.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

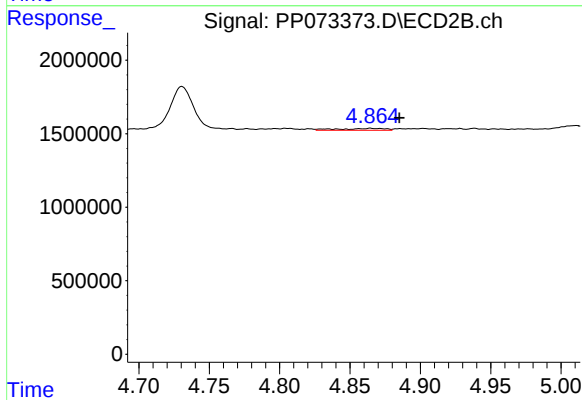


#17 AR-1242-2

R.T.: 4.865 min
Delta R.T.: -0.020 min
Response: 289310
Conc: 3.64 ng/ml

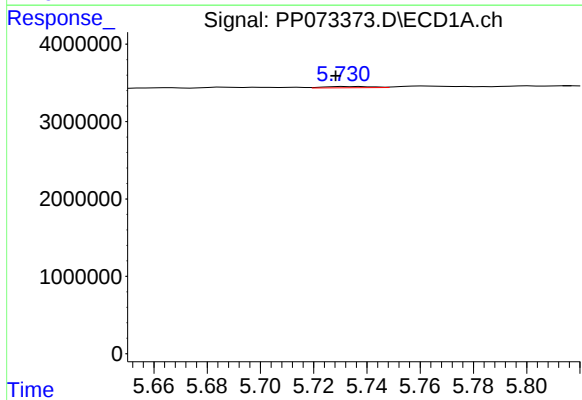


#18 AR-1242-3

R.T.: 5.732 min
Delta R.T.: 0.004 min
Response: 203640
Conc: 3.86 ng/ml

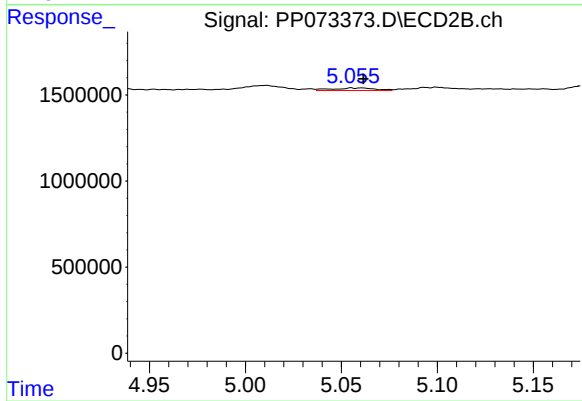

#18 AR-1242-3


R.T.: 5.055 min
Delta R.T.: -0.006 min
Response: 236322
Conc: 5.46 ng/ml

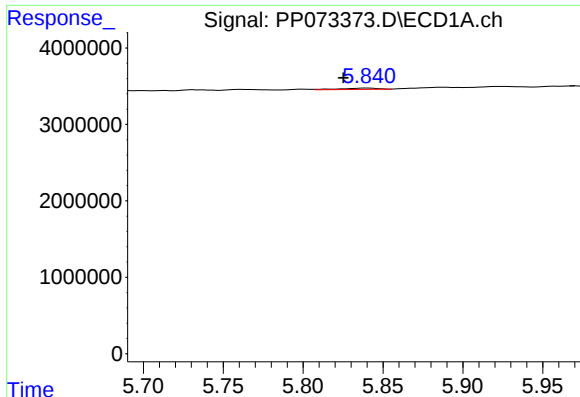

#19 AR-1242-4


R.T.: 5.841 min
Delta R.T.: 0.016 min
Response: 273393
Conc: 6.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

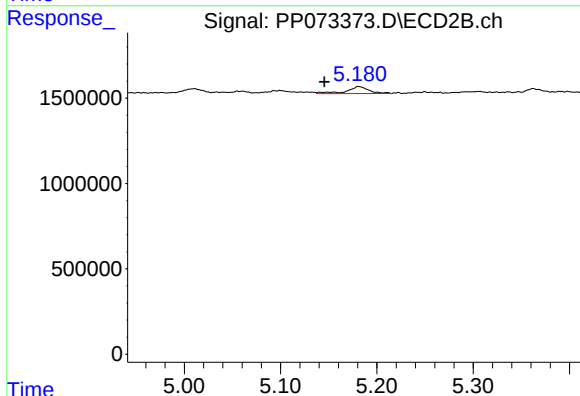


#19 AR-1242-4

R.T.: 5.181 min
Delta R.T.: 0.036 min
Response: 668375
Conc: 16.10 ng/ml

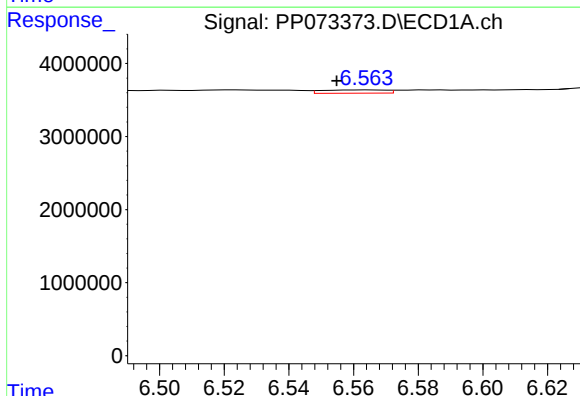


#20 AR-1242-5

R.T.: 6.565 min
Delta R.T.: 0.010 min
Response: 607216
Conc: 12.25 ng/ml

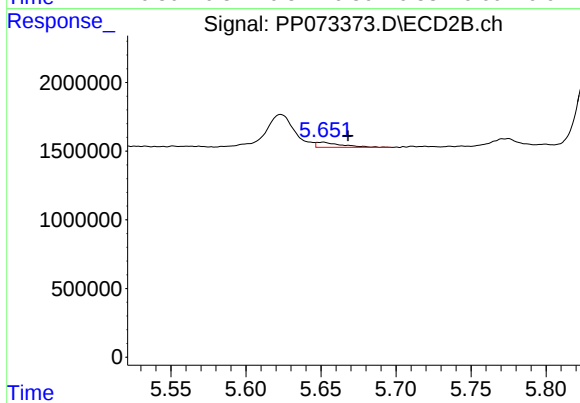

#20 AR-1242-5


R.T.: 5.651 min
Delta R.T.: -0.017 min
Response: 435302
Conc: 8.28 ng/ml

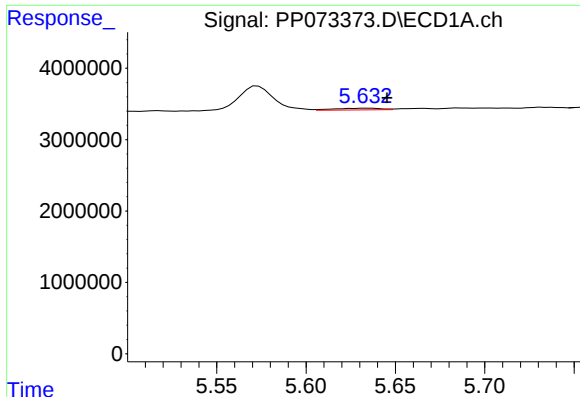

#21 AR-1248-1


R.T.: 5.634 min
Delta R.T.: -0.011 min
Response: 439261
Conc: 9.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

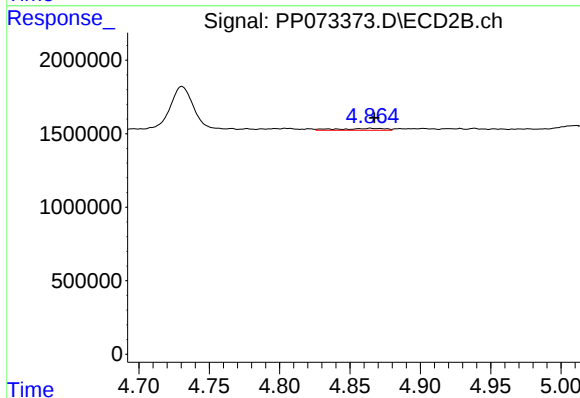


#21 AR-1248-1

R.T.: 4.865 min
Delta R.T.: -0.003 min
Response: 289310
Conc: 6.64 ng/ml

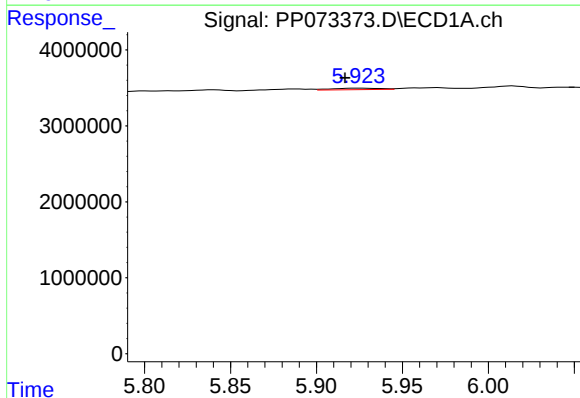


#22 AR-1248-2

R.T.: 5.924 min
Delta R.T.: 0.007 min
Response: 393146
Conc: 6.71 ng/ml

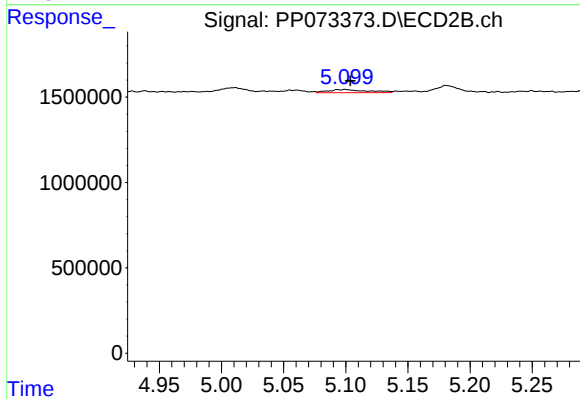

#22 AR-1248-2


R.T.: 5.100 min
Delta R.T.: -0.004 min
Response: 405320
Conc: 6.92 ng/ml

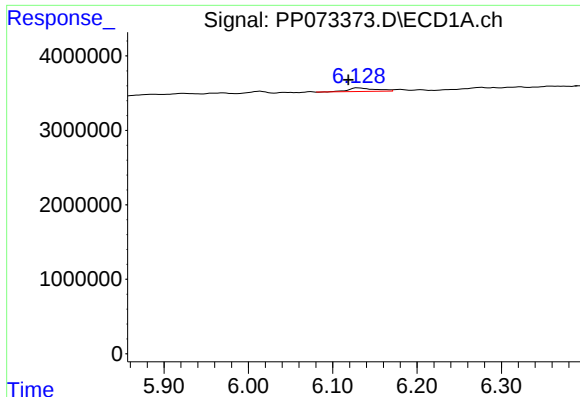

#23 AR-1248-3


R.T.: 6.129 min
Delta R.T.: 0.011 min
Response: 1037501
Conc: 15.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

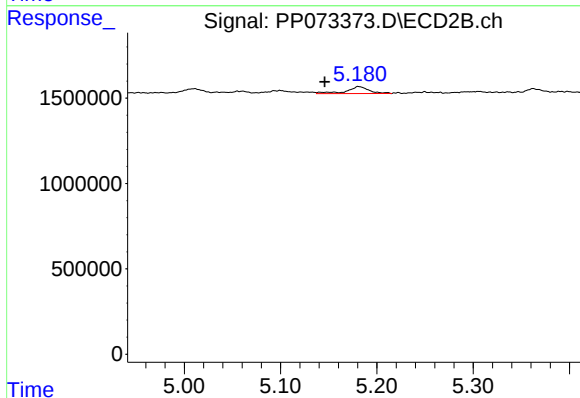


#23 AR-1248-3

R.T.: 5.181 min
Delta R.T.: 0.035 min
Response: 668375
Conc: 11.04 ng/ml

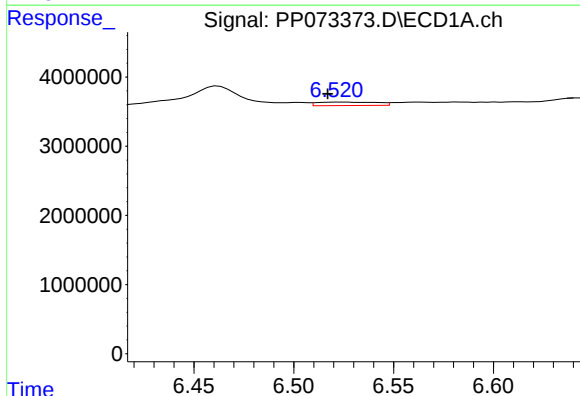


#24 AR-1248-4

R.T.: 6.523 min
Delta R.T.: 0.006 min
Response: 1063970
Conc: 12.51 ng/ml

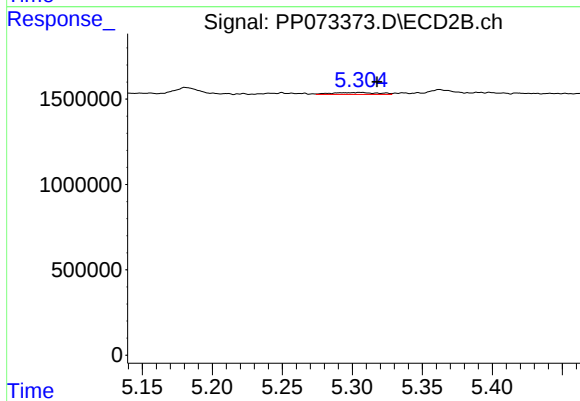

#24 AR-1248-4


R.T.: 5.306 min
Delta R.T.: -0.011 min
Response: 247647
Conc: 3.54 ng/ml

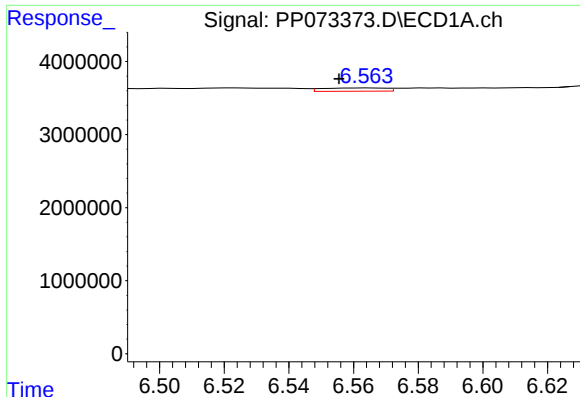

#25 AR-1248-5


R.T.: 6.565 min
Delta R.T.: 0.009 min
Response: 607216
Conc: 7.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

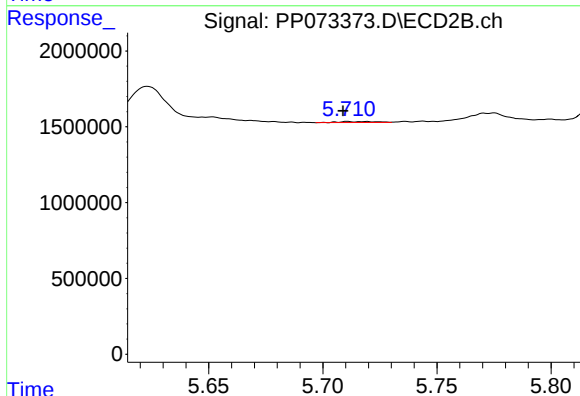


#25 AR-1248-5

R.T.: 5.719 min
Delta R.T.: 0.010 min
Response: 79932
Conc: 1.13 ng/ml

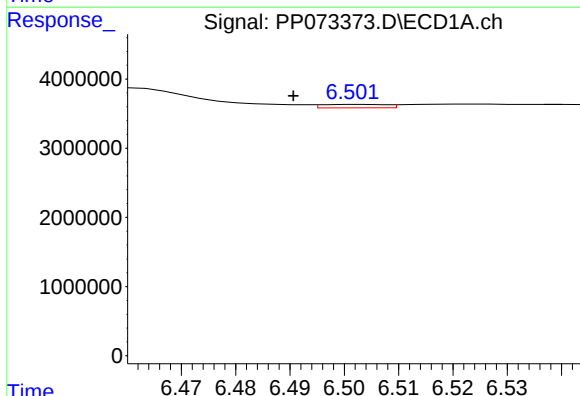


#26 AR-1254-1

R.T.: 6.502 min
Delta R.T.: 0.012 min
Response: 414657
Conc: 4.93 ng/ml

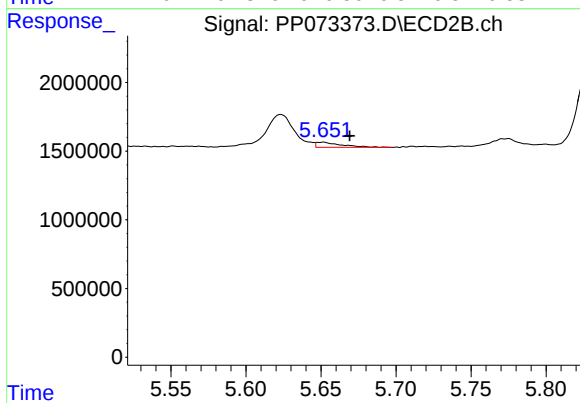

#26 AR-1254-1


R.T.: 5.651 min
Delta R.T.: -0.018 min
Response: 435302
Conc: 3.97 ng/ml

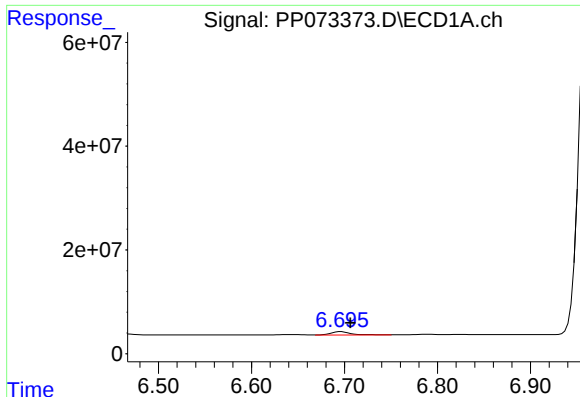

#27 AR-1254-2


R.T.: 6.696 min
Delta R.T.: -0.011 min
Response: 9904233
Conc: 78.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

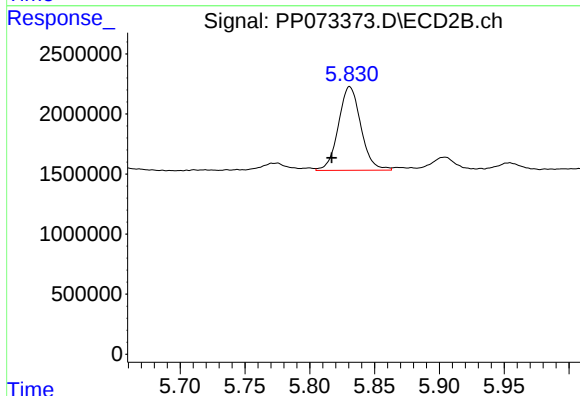


#27 AR-1254-2

R.T.: 5.831 min
Delta R.T.: 0.014 min
Response: 8396294
Conc: 88.81 ng/ml

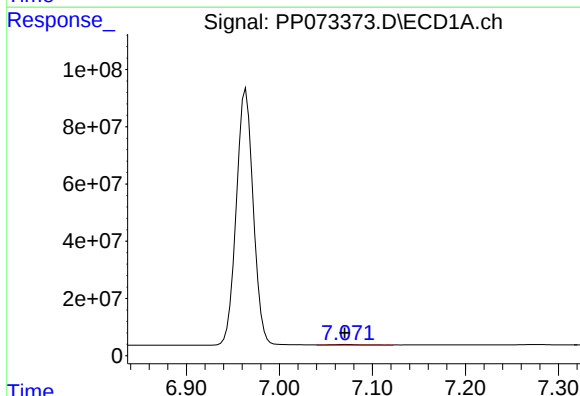


#28 AR-1254-3

R.T.: 7.072 min
Delta R.T.: 0.002 min
Response: 6983781
Conc: 53.23 ng/ml

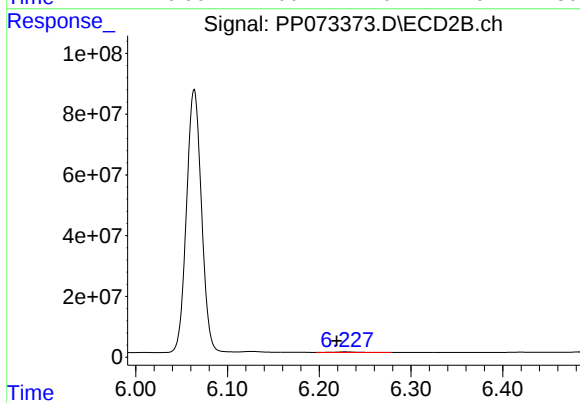

#28 AR-1254-3


R.T.: 6.228 min
Delta R.T.: 0.009 min
Response: 3186699
Conc: 21.60 ng/ml

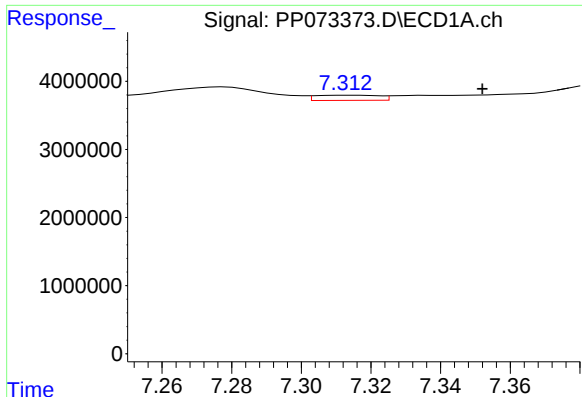

#29 AR-1254-4


R.T.: 7.314 min
Delta R.T.: -0.038 min
Response: 968683
Conc: 8.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

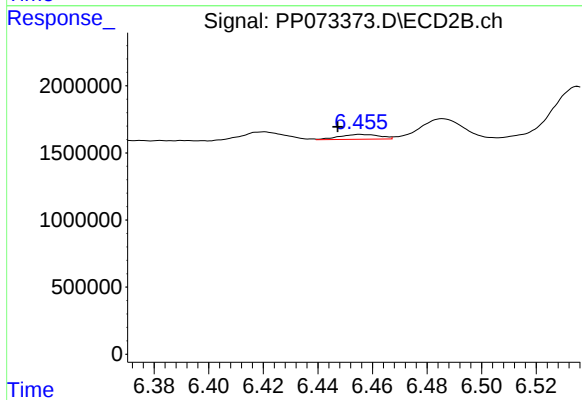


#29 AR-1254-4

R.T.: 6.456 min
Delta R.T.: 0.008 min
Response: 376697
Conc: 3.88 ng/ml

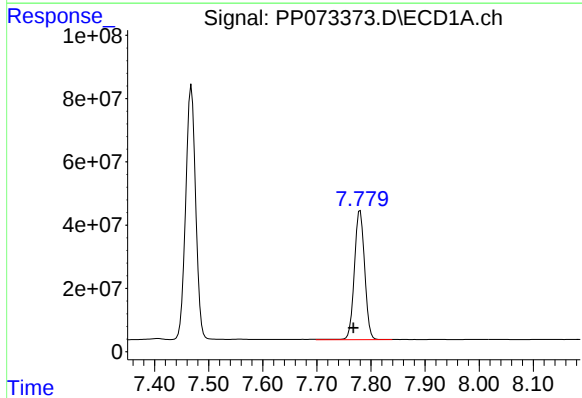


#30 AR-1254-5

R.T.: 7.780 min
Delta R.T.: 0.012 min
Response: 539674431
Conc: 4723.36 ng/ml

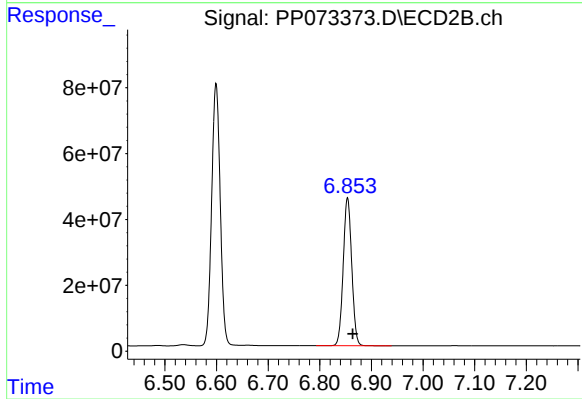

#30 AR-1254-5


R.T.: 6.854 min
Delta R.T.: -0.010 min
Response: 515559914
Conc: 3966.98 ng/ml

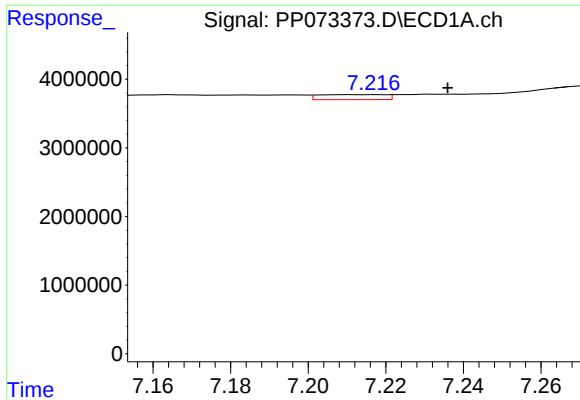

#31 AR-1260-1


R.T.: 7.211 min
Delta R.T.: -0.025 min
Response: 870983
Conc: 9.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

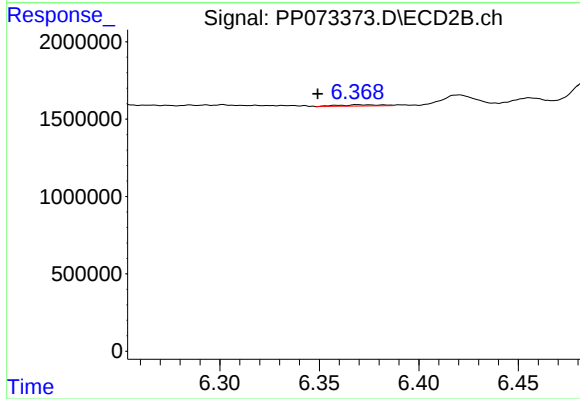


#31 AR-1260-1

R.T.: 6.369 min
Delta R.T.: 0.020 min
Response: 122270
Conc: 1.29 ng/ml

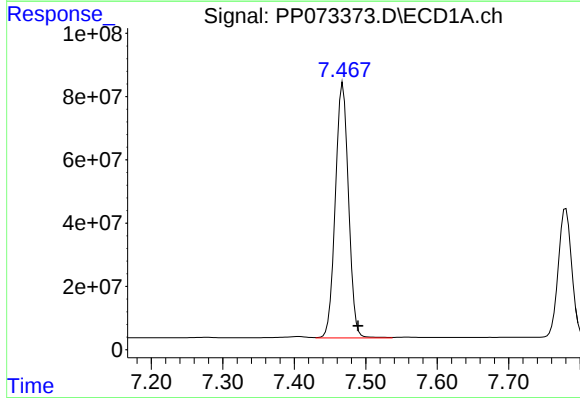


#32 AR-1260-2

R.T.: 7.468 min
Delta R.T.: -0.021 min
Response: 1029787222
Conc: 7578.44 ng/ml

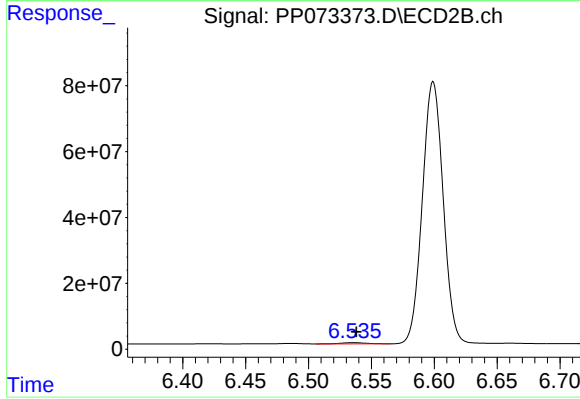

#32 AR-1260-2


R.T.: 6.535 min
Delta R.T.: -0.003 min
Response: 4798026
Conc: 41.21 ng/ml

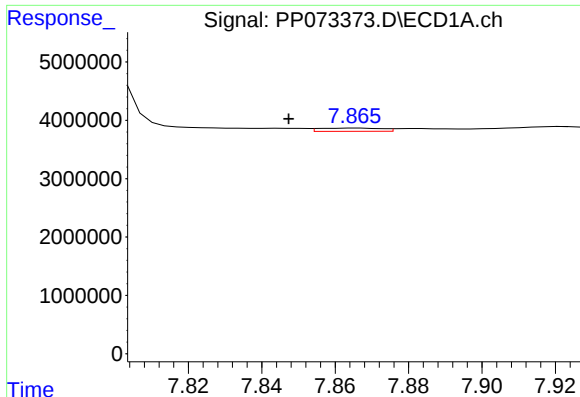

#33 AR-1260-3


R.T.: 7.866 min
Delta R.T.: 0.018 min
Response: 649041
Conc: 5.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

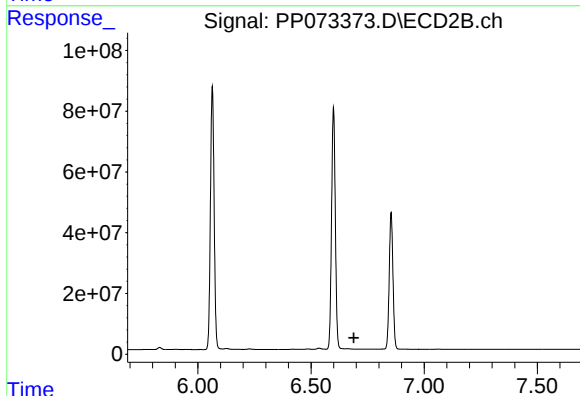


#33 AR-1260-3

R.T.: 6.661 min
Delta R.T.: -0.029 min
Response: -100236
Conc: N.D.

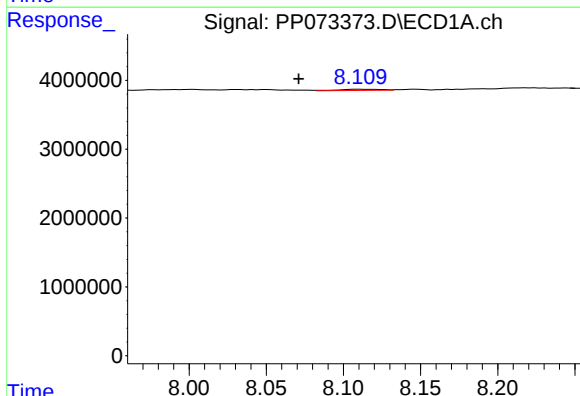


#34 AR-1260-4

R.T.: 8.111 min
Delta R.T.: 0.040 min
Response: 359730
Conc: 3.49 ng/ml

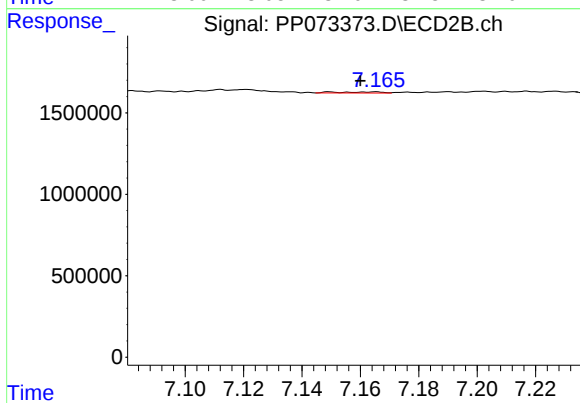

#34 AR-1260-4


R.T.: 7.165 min
Delta R.T.: 0.005 min
Response: 69687
Conc: 0.79 ng/ml

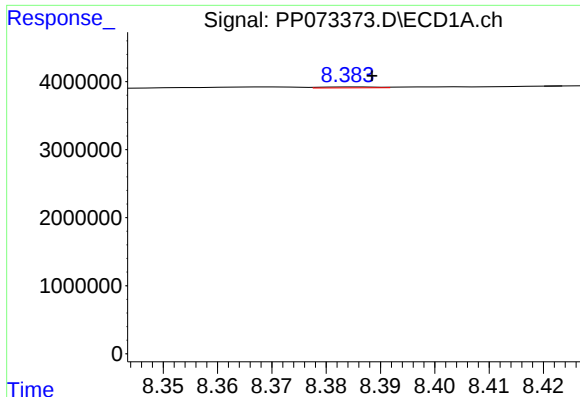

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 96670
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

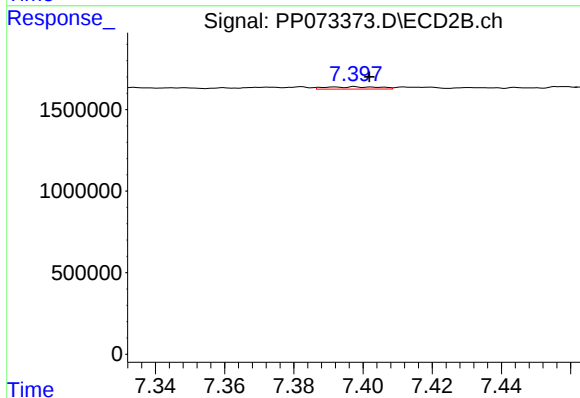


#35 AR-1260-5

R.T.: 7.398 min
Delta R.T.: -0.004 min
Response: 153221
Conc: 0.72 ng/ml

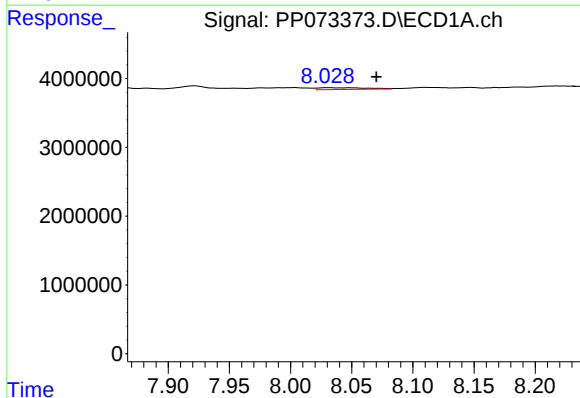


#36 AR-1262-1

R.T.: 8.030 min
Delta R.T.: -0.040 min
Response: 699792
Conc: 4.73 ng/ml

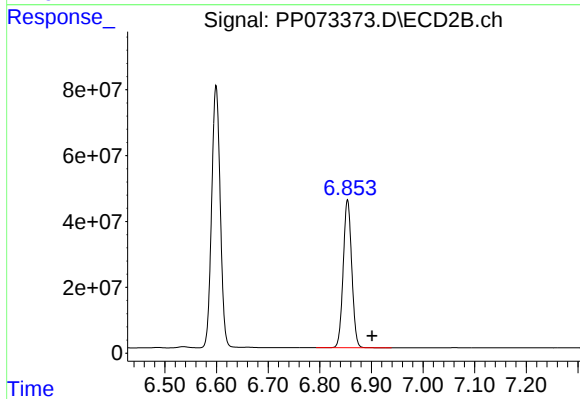

#36 AR-1262-1


R.T.: 6.854 min
Delta R.T.: -0.047 min
Response: 515559914
Conc: 3568.71 ng/ml

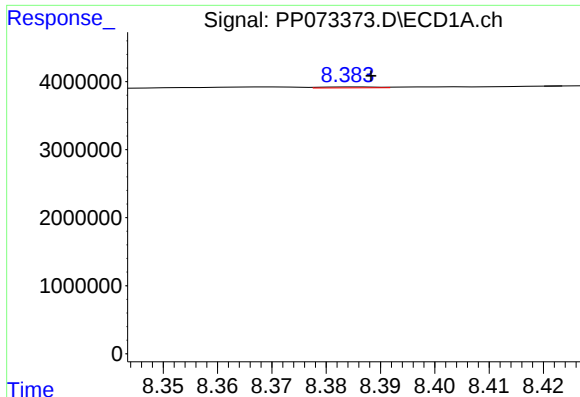

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 96670
Conc: 0.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

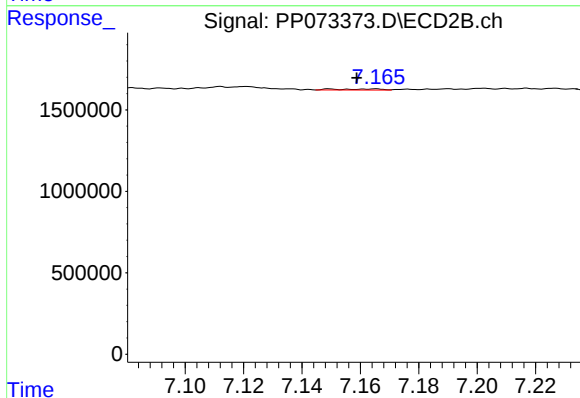


#37 AR-1262-2

R.T.: 7.165 min
Delta R.T.: 0.007 min
Response: 69687
Conc: 0.57 ng/ml

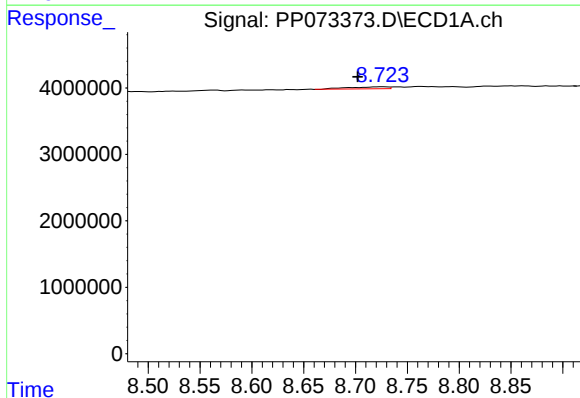


#38 AR-1262-3

R.T.: 8.726 min
Delta R.T.: 0.024 min
Response: 773552
Conc: 3.62 ng/ml

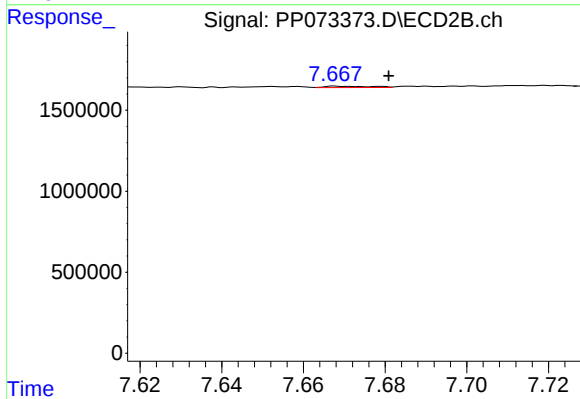

#38 AR-1262-3


R.T.: 7.668 min
Delta R.T.: -0.012 min
Response: 68527
Conc: 0.61 ng/ml

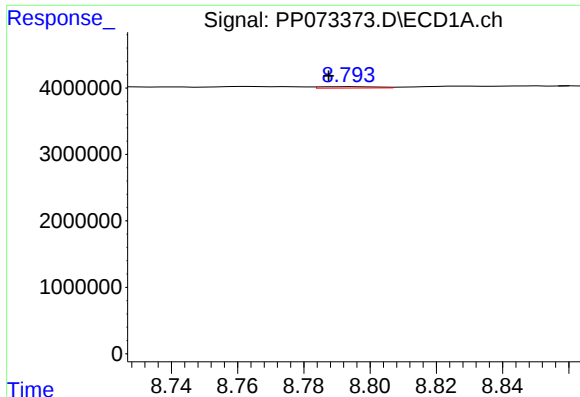

#39 AR-1262-4


R.T.: 8.794 min
Delta R.T.: 0.006 min
Response: 238125
Conc: 1.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

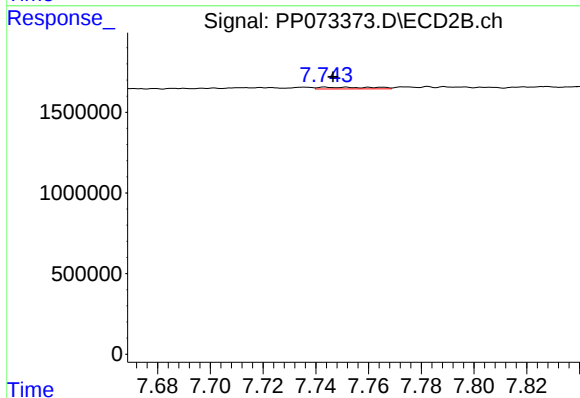


#39 AR-1262-4

R.T.: 7.744 min
Delta R.T.: -0.003 min
Response: 152347
Conc: 0.83 ng/ml

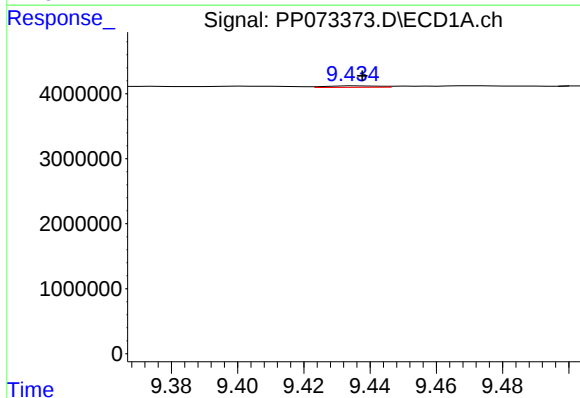


#40 AR-1262-5

R.T.: 9.435 min
Delta R.T.: -0.002 min
Response: 247829
Conc: 2.22 ng/ml

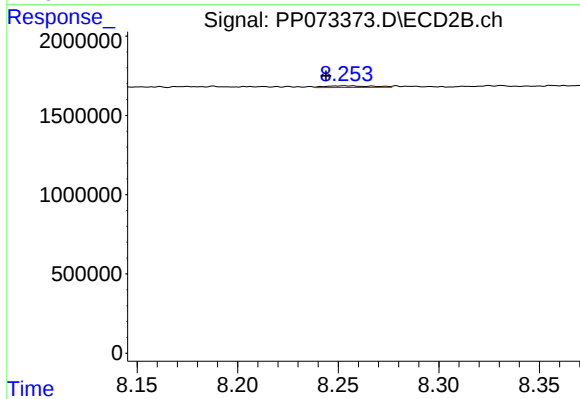

#40 AR-1262-5


R.T.: 8.253 min
Delta R.T.: 0.009 min
Response: 181093
Conc: 2.09 ng/ml

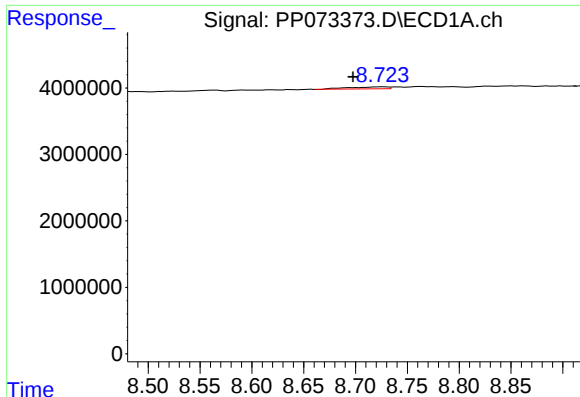

#41 AR-1268-1


R.T.: 8.726 min
Delta R.T.: 0.028 min
Response: 773552
Conc: 2.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

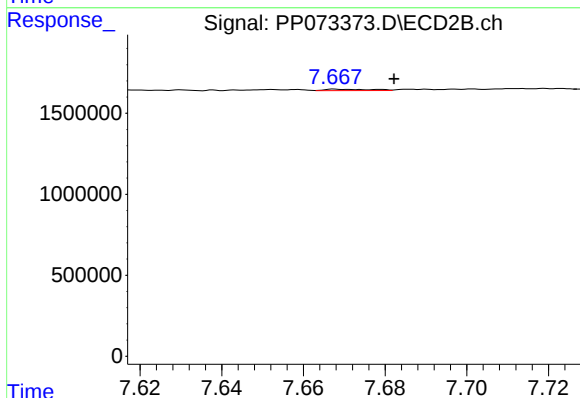


#41 AR-1268-1

R.T.: 7.668 min
Delta R.T.: -0.014 min
Response: 68527
Conc: 0.24 ng/ml

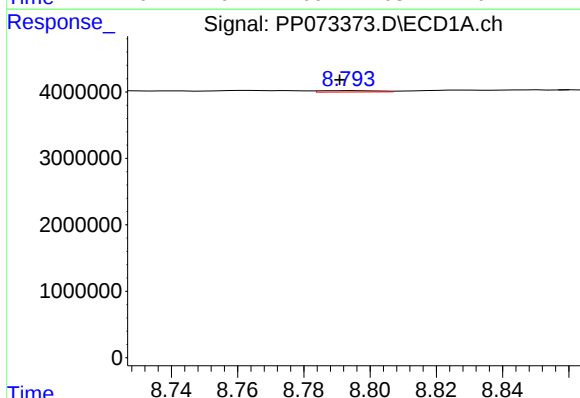


#42 AR-1268-2

R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 238125
Conc: 0.78 ng/ml

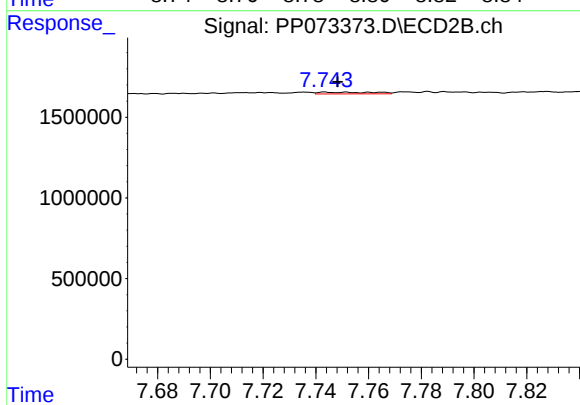

#42 AR-1268-2


R.T.: 7.744 min
Delta R.T.: -0.005 min
Response: 152347
Conc: 0.59 ng/ml

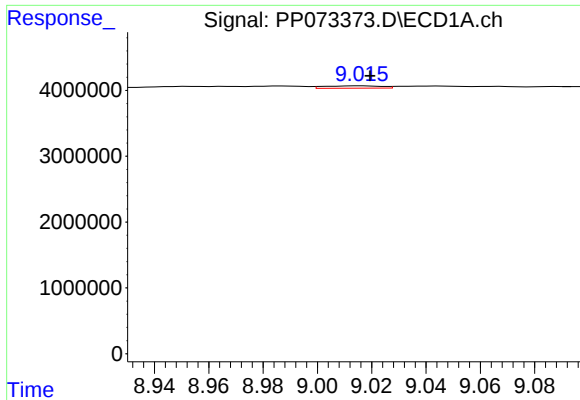

#43 AR-1268-3


R.T.: 9.016 min
Delta R.T.: -0.003 min
Response: 533703
Conc: 2.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

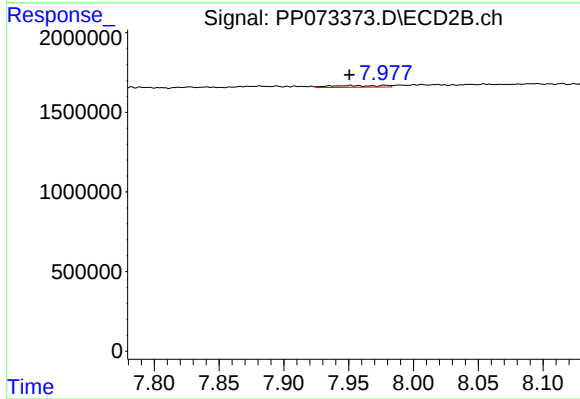


#43 AR-1268-3

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 308382
Conc: 1.43 ng/ml

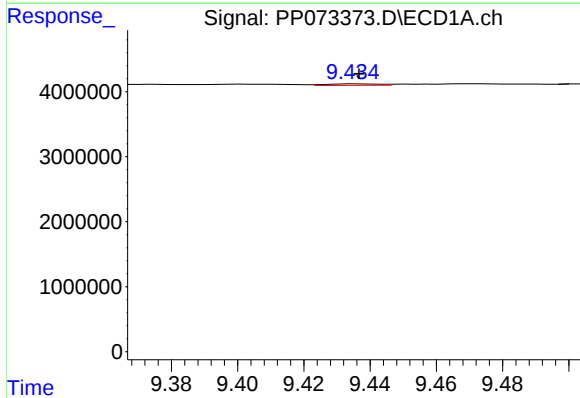


#44 AR-1268-4

R.T.: 9.435 min
Delta R.T.: -0.001 min
Response: 247829
Conc: 2.12 ng/ml

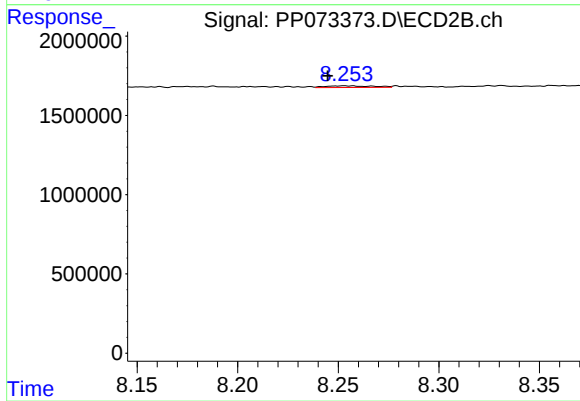

#44 AR-1268-4


R.T.: 8.253 min
Delta R.T.: 0.009 min
Response: 181093
Conc: 1.92 ng/ml

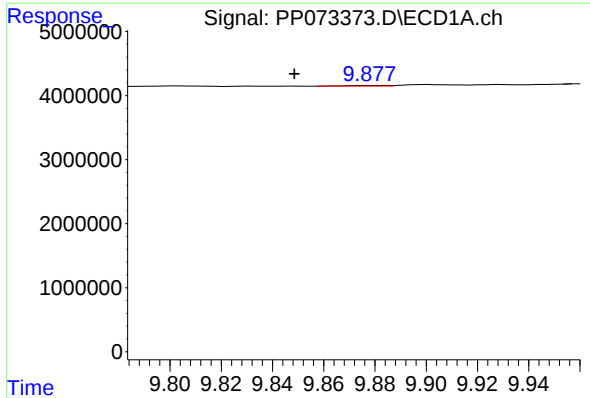

#45 AR-1268-5

R.T.: 9.878 min
Delta R.T.: 0.030 min
Response: 112888
Conc: 0.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

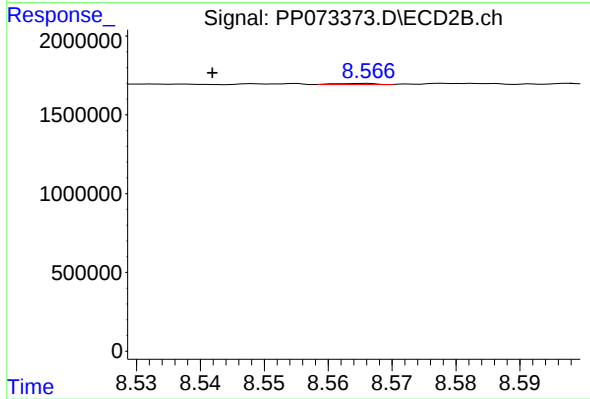

#45 AR-1268-5

R.T.: 8.565 min
Delta R.T.: 0.023 min
Response: 29014
Conc: 0.05 ng/ml