

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
Data File : PP073394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2025 20:23
Operator : YP\AJ
Sample : Q2457-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OK-2-062725

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:39:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.785	35427089	35708821	16.784m	19.818
2) SA Decachlor...	10.179	8.789	28149792	24323949	16.473	18.224m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
Data File : PP073394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2025 20:23
Operator : YP\AJ
Sample : Q2457-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OK-2-062725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:39:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

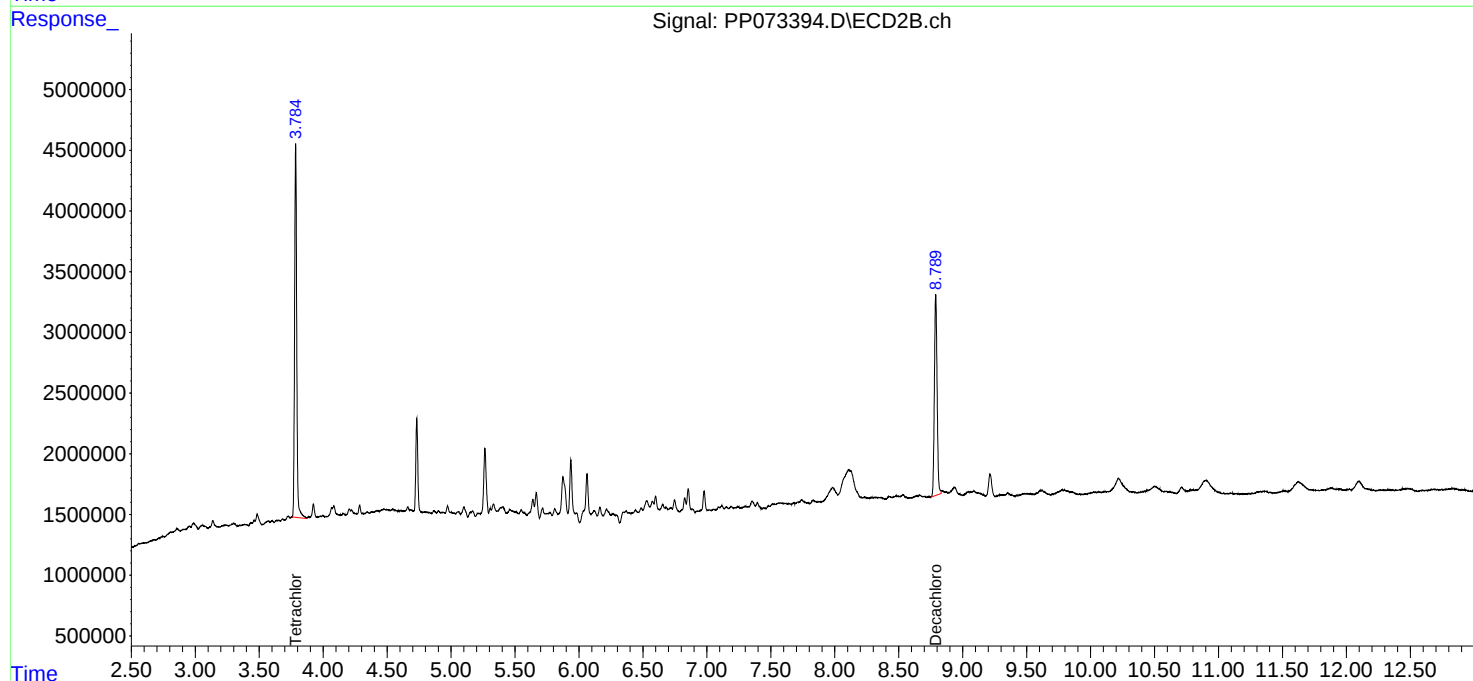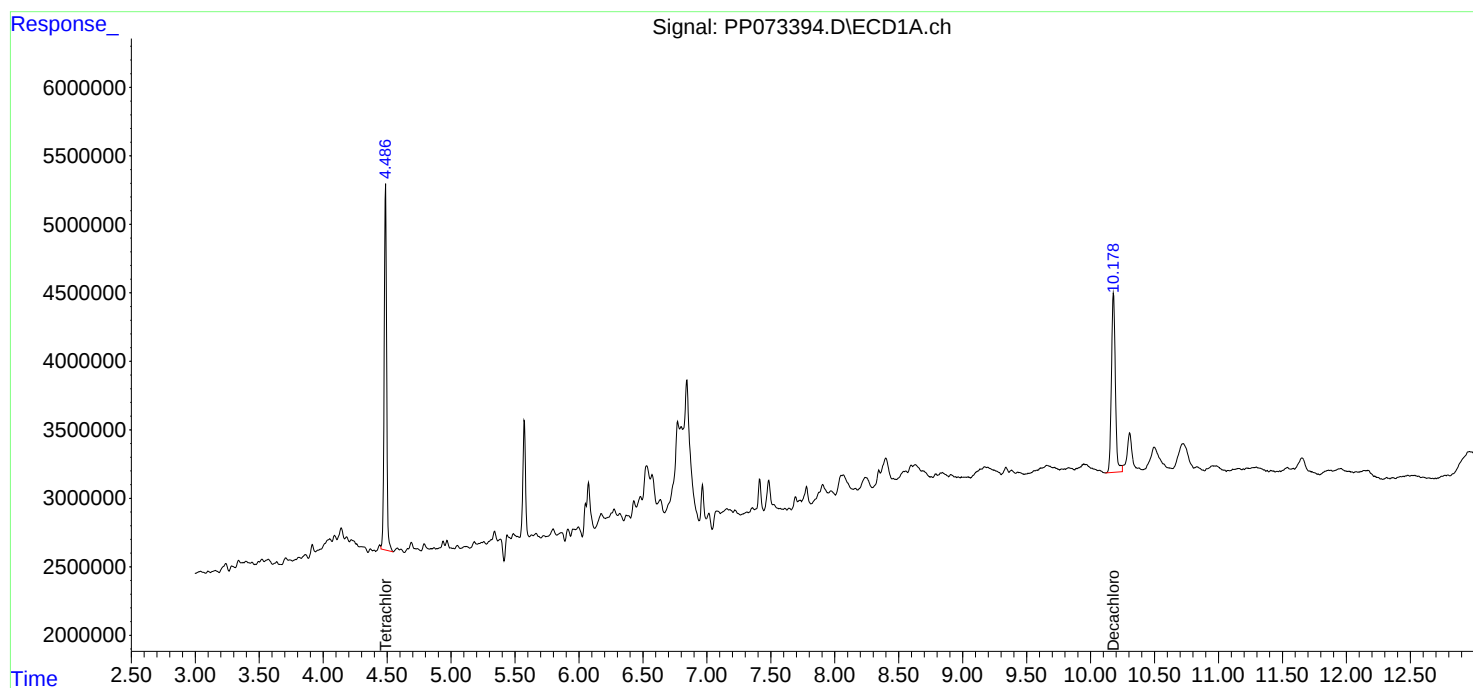

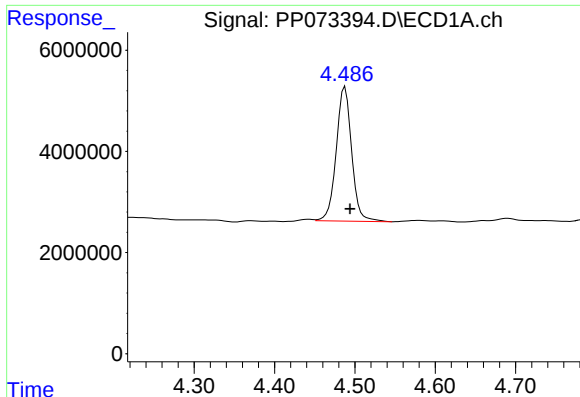


#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: -0.008 min
Response: 35427089
Conc: 16.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-2-062725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/02/2025

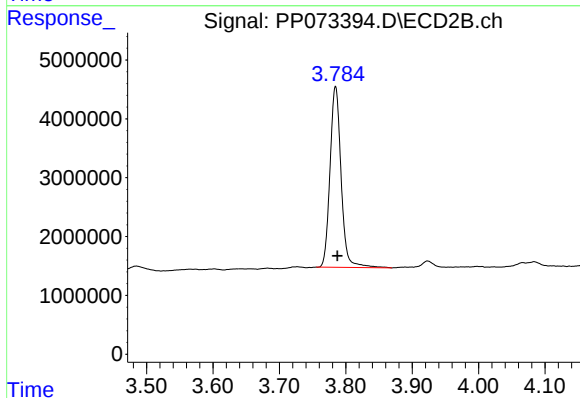


#1 Tetrachloro-m-xylene

R.T.: 3.785 min
Delta R.T.: -0.003 min
Response: 35708821
Conc: 19.82 ng/ml

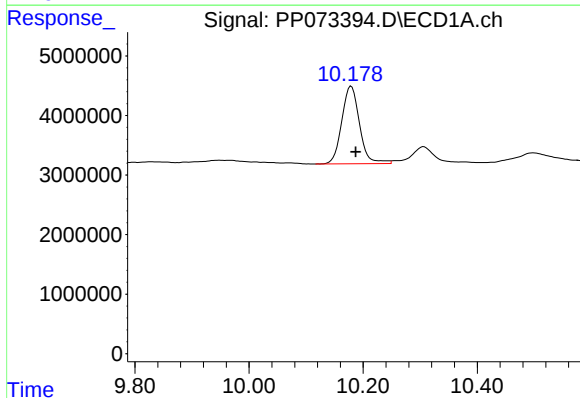

#2 Decachlorobiphenyl

R.T.: 10.179 min
Delta R.T.: -0.008 min
Response: 28149792
Conc: 16.47 ng/ml

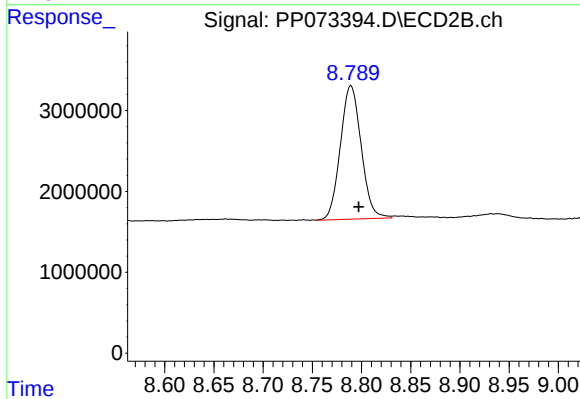

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.008 min
Response: 24323949
Conc: 18.22 ng/ml m