

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
 Data File : PP073406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2025 01:02
 Operator : YP\AJ
 Sample : Q2451-06 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KQA08OZ-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/01/2025
 Supervised By :mohammad ahmed 07/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 07:30:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.783	2091480	2675618	0.991m	1.485 #
2) SA Decachlor...	10.179	8.789	1373200	1713083	0.804m	1.283 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP063025\
Data File : PP073406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2025 01:02
Operator : YP\AJ
Sample : Q2451-06 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KQA08OZ-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 07:30:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

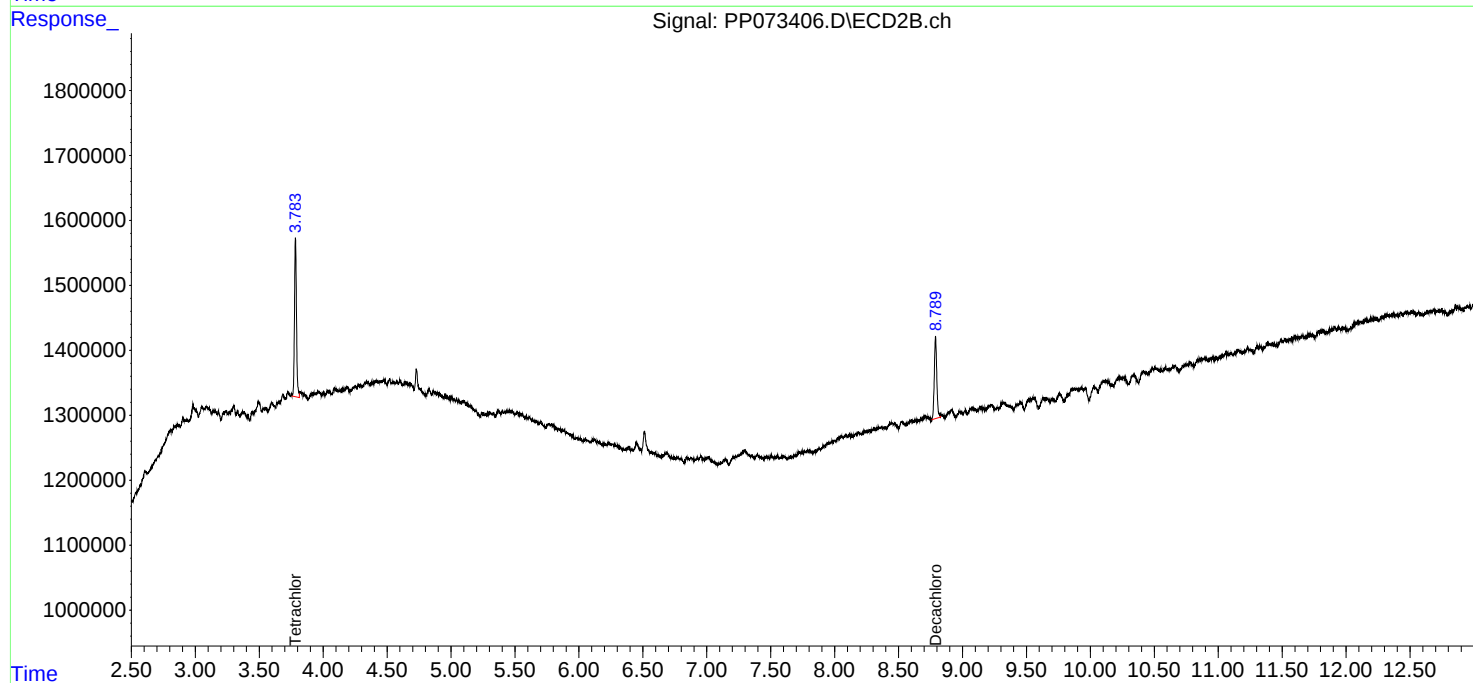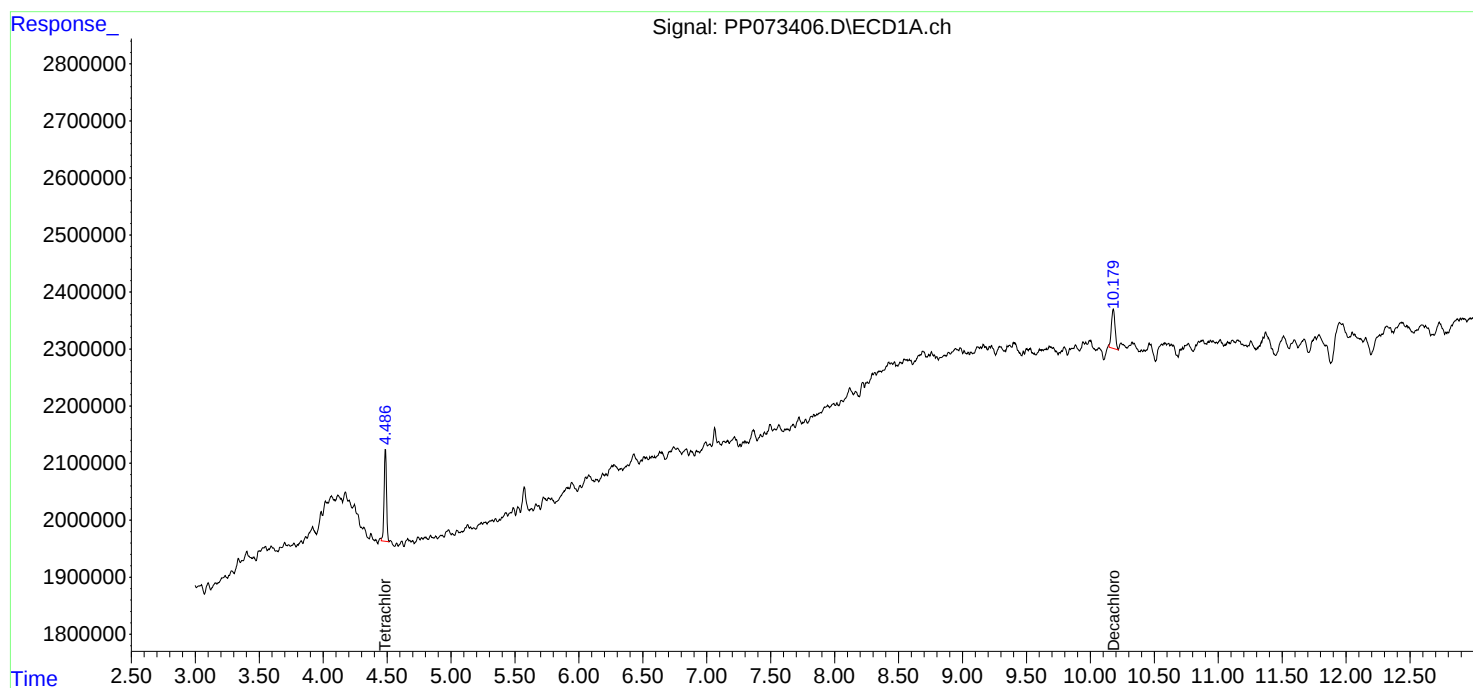

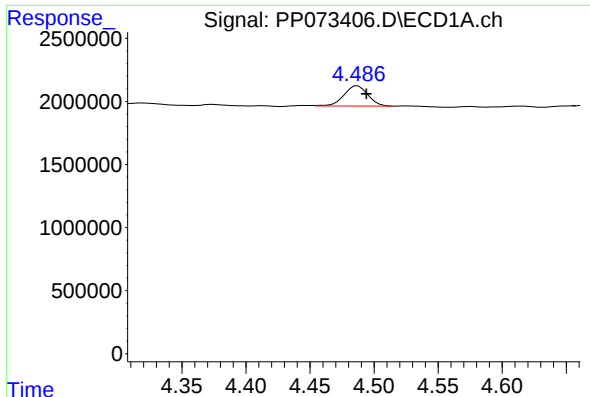


#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: -0.008 min
Response: 2091480
Conc: 0.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
KQA08OZ-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/02/2025

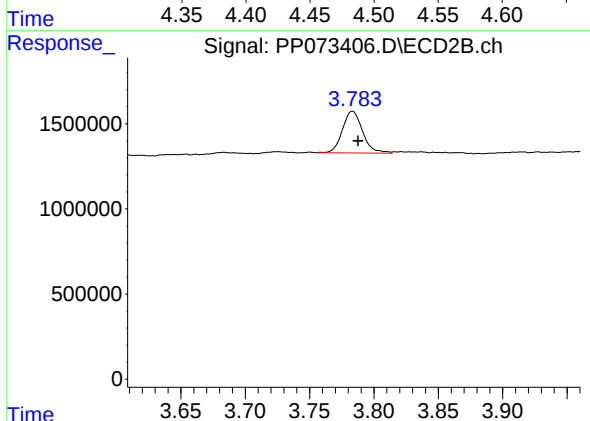


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.004 min
Response: 2675618
Conc: 1.48 ng/ml

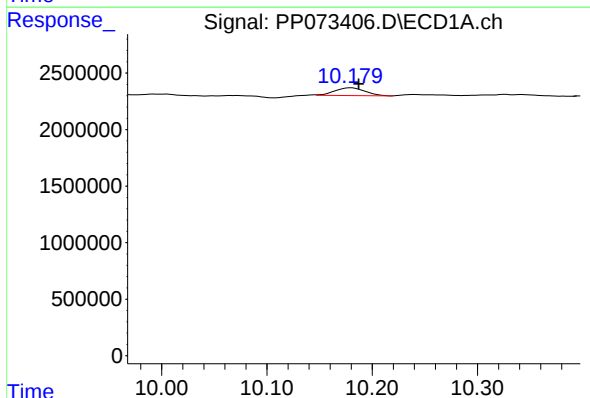

#2 Decachlorobiphenyl

R.T.: 10.179 min
Delta R.T.: -0.008 min
Response: 1373200
Conc: 0.80 ng/ml m

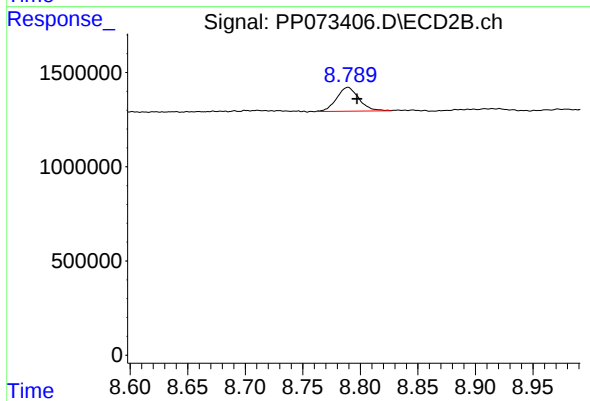

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.008 min
Response: 1713083
Conc: 1.28 ng/ml