

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070121\
 Data File : PP036959.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2021 13:13
 Operator : DD\AJ
 Sample : M2900-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:29:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.962	3.953	804115	517879	18.193	16.720
2)	SA Decachlor...	10.993	9.248	777621	471710	18.127	14.750
Target Compounds							
9)	L2 AR-1221-2	5.314	0.000	10533	0	24.443	N.D. #
27)	L6 AR-1254-2	7.424	0.000	9141	0	3.378	N.D. #
28)	L6 AR-1254-3	7.820	0.000	34546	0	11.663	N.D. #
30)	L6 AR-1254-5	8.527	0.000	25663	0	10.791	N.D. #
32)	L7 AR-1260-2	8.208f	0.000	7441	0	2.903	N.D. #
34)	L7 AR-1260-4	8.835	0.000	858	0	0.362	N.D. #
38)	L8 AR-1262-3	0.000	8.158f	0	16276	N.D.	10.227 #
41)	L9 AR-1268-1	0.000	8.158f	0	16276	N.D.	3.495 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070121\
Data File : PP036959.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2021 13:13
Operator : DD\AJ
Sample : M2900-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:29:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

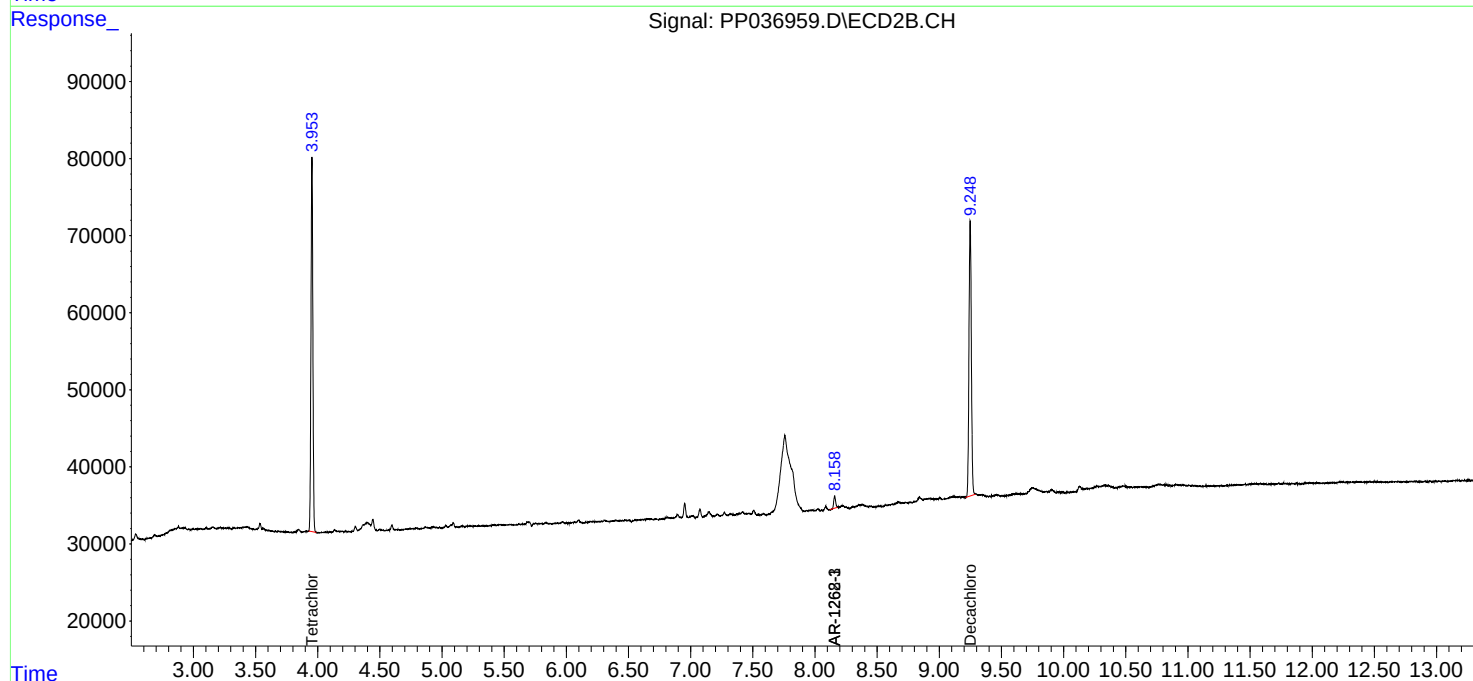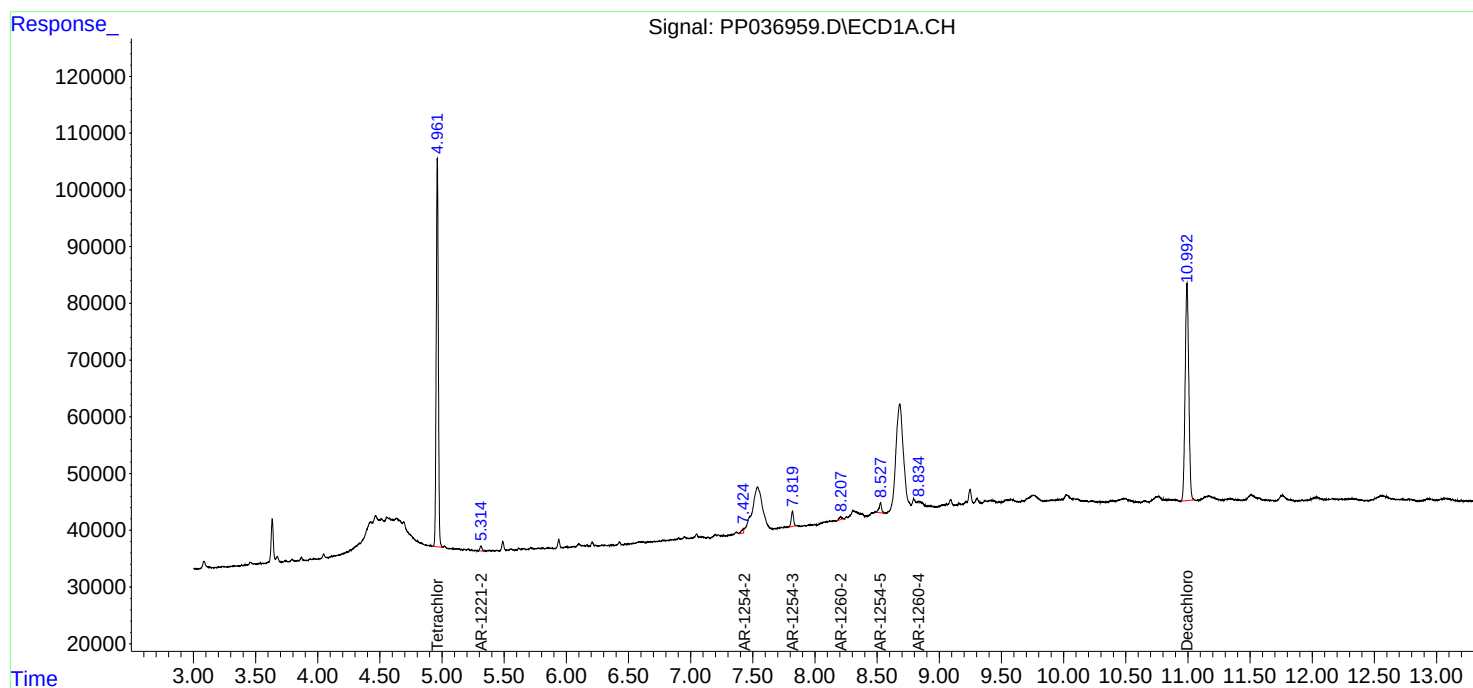


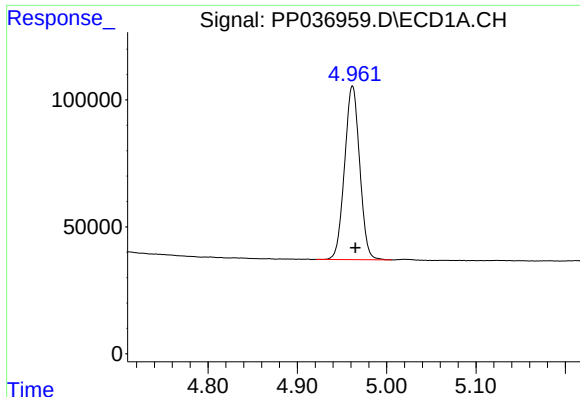

#1 Tetrachloro-m-xylene


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 804115
Conc: 18.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

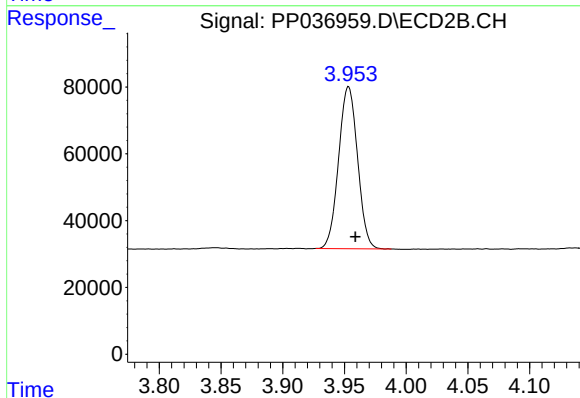


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.006 min
Response: 517879
Conc: 16.72 ng/ml

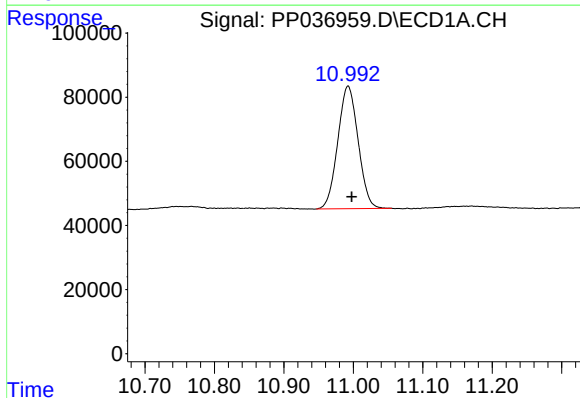


#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: -0.005 min
Response: 777621
Conc: 18.13 ng/ml

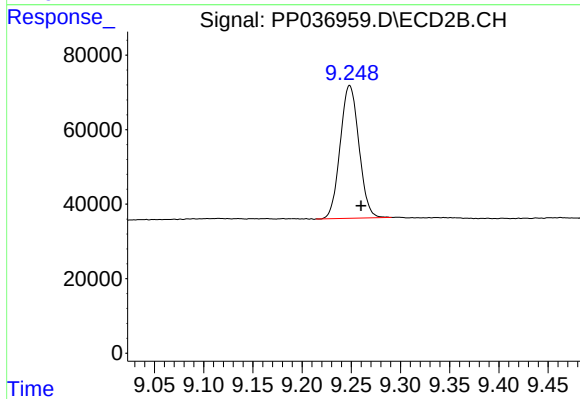

#2 Decachlorobiphenyl


R.T.: 9.248 min
Delta R.T.: -0.012 min
Response: 471710
Conc: 14.75 ng/ml

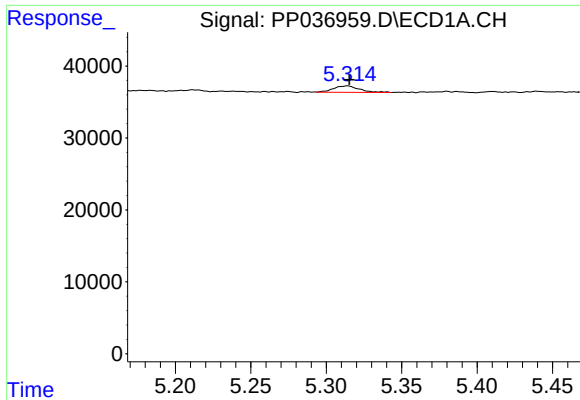

#9 AR-1221-2


R.T.: 5.314 min
Delta R.T.: -0.001 min
Response: 10533
Conc: 24.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

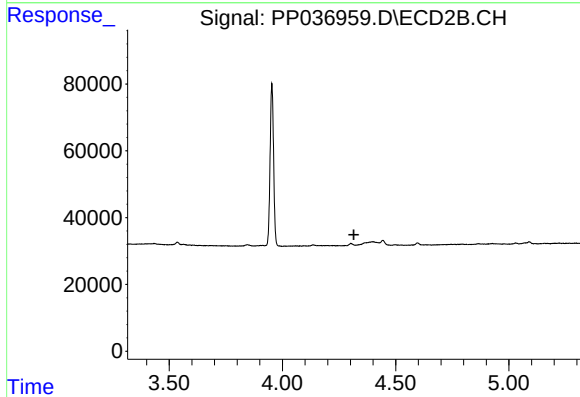


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

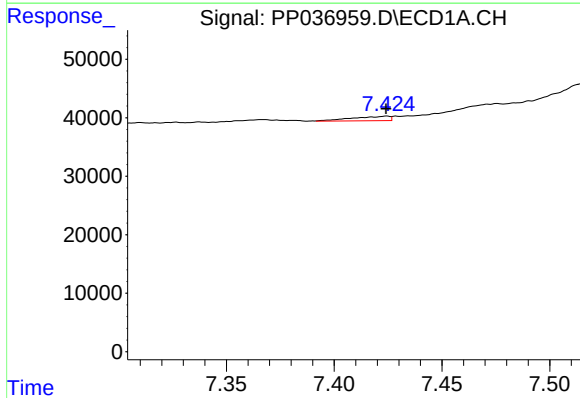


#27 AR-1254-2

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 9141
Conc: 3.38 ng/ml

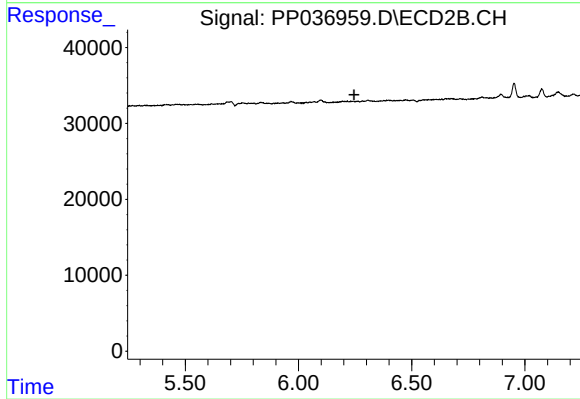

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

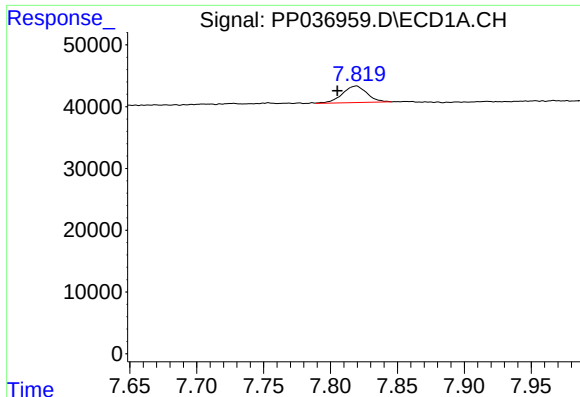

#28 AR-1254-3


R.T.: 7.820 min
Delta R.T.: 0.014 min
Response: 34546
Conc: 11.66 ng/ml

Instrument :
ECD_P
ClientSampleId :

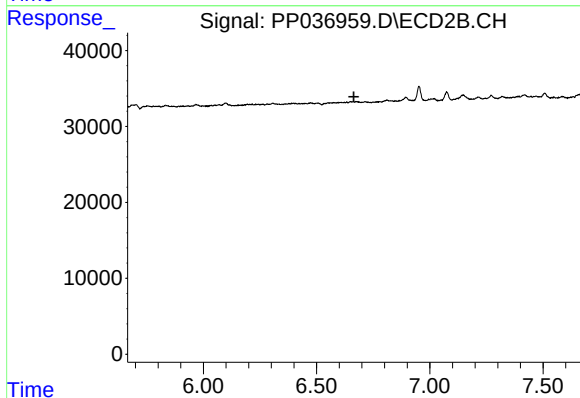


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

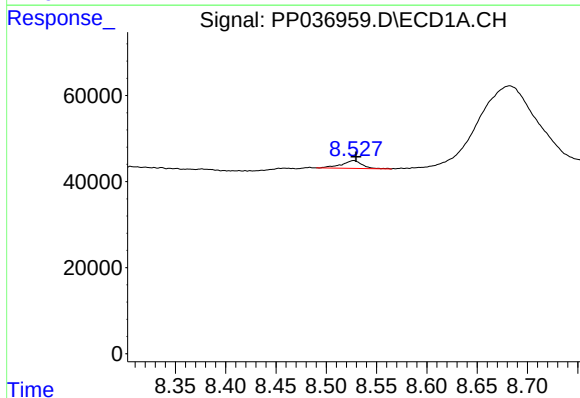


#30 AR-1254-5

R.T.: 8.527 min
Delta R.T.: -0.002 min
Response: 25663
Conc: 10.79 ng/ml

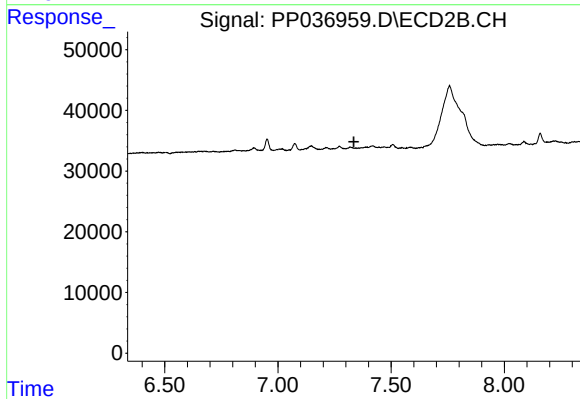

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.335 min
Response: 0
Conc: N.D.

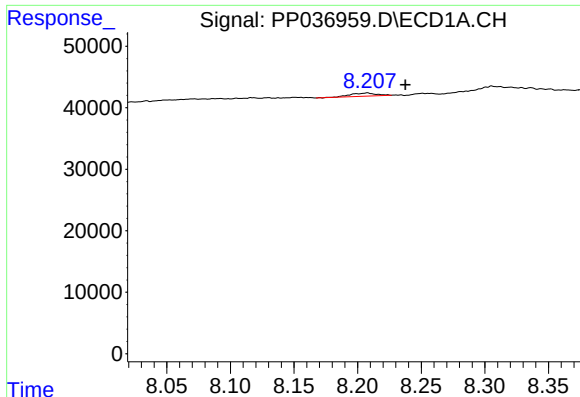

#32 AR-1260-2


R.T.: 8.208 min
Delta R.T.: -0.030 min
Response: 7441
Conc: 2.90 ng/ml

Instrument :
ECD_P
ClientSampleId :

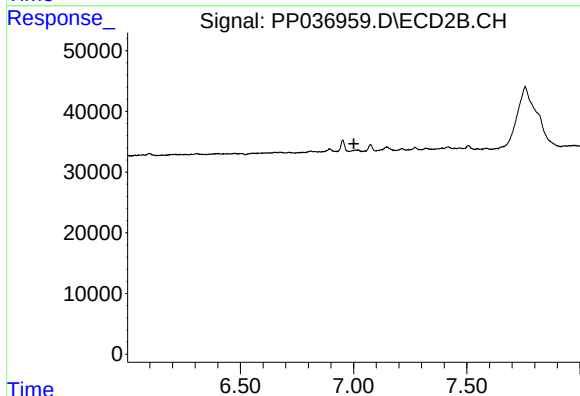


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.001 min
Response: 0
Conc: N.D.

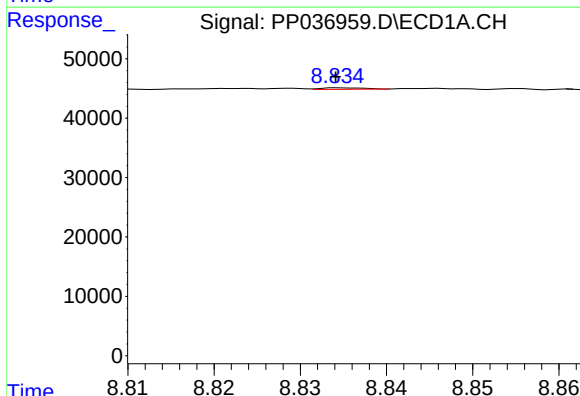


#34 AR-1260-4

R.T.: 8.835 min
Delta R.T.: 0.000 min
Response: 858
Conc: 0.36 ng/ml

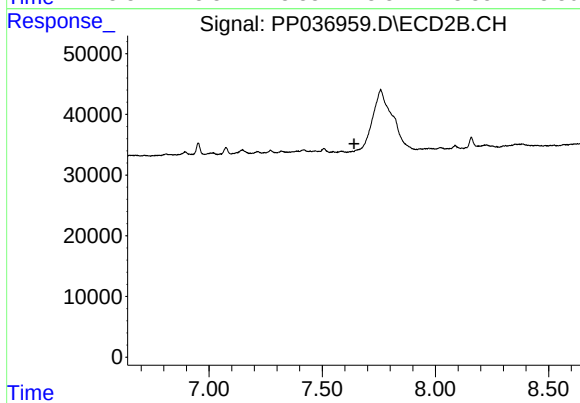

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.640 min
Response: 0
Conc: N.D.

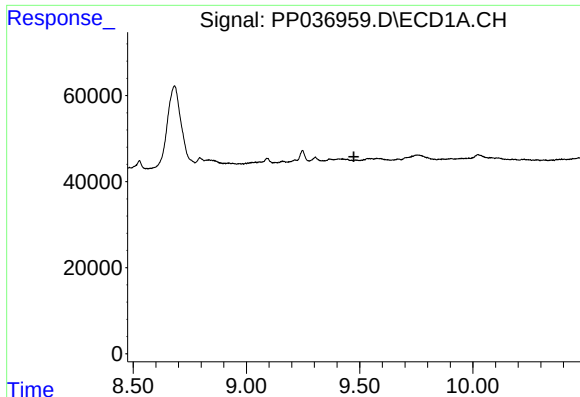

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

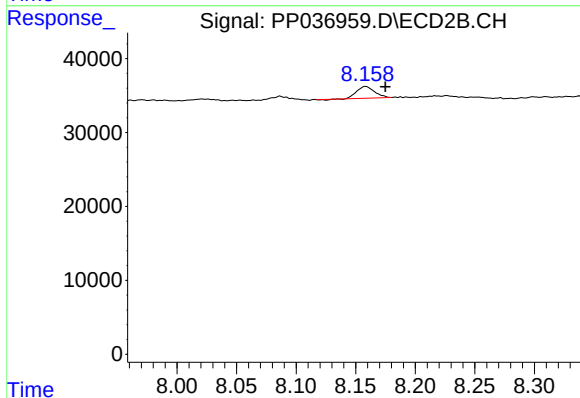


#38 AR-1262-3

R.T.: 8.158 min
Delta R.T.: -0.017 min
Response: 16276
Conc: 10.23 ng/ml

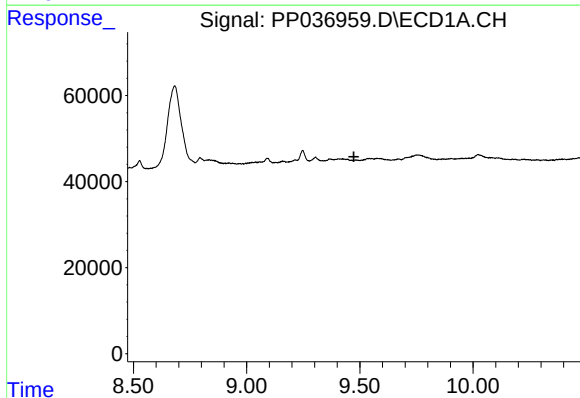

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.473 min
Response: 0
Conc: N.D.

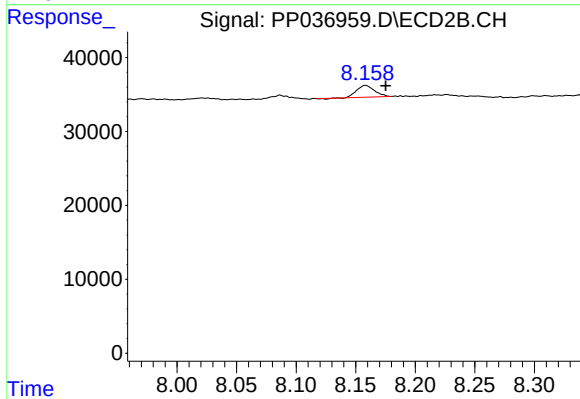

#41 AR-1268-1

R.T.: 8.158 min
Delta R.T.: -0.017 min
Response: 16276
Conc: 3.50 ng/ml