

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070122\
 Data File : PP049147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 15:23
 Operator : YP\AJ
 Sample : N3455-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SP-EXC-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2022
 Supervised By :Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 16:55:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.593	26099062	43398260	18.359	16.948m
2) SA Decachlor...	10.096	8.568	20975239	17319655	17.100	15.365

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070122\
Data File : PP049147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 15:23
Operator : YP\AJ
Sample : N3455-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SP-EXC-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 16:55:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

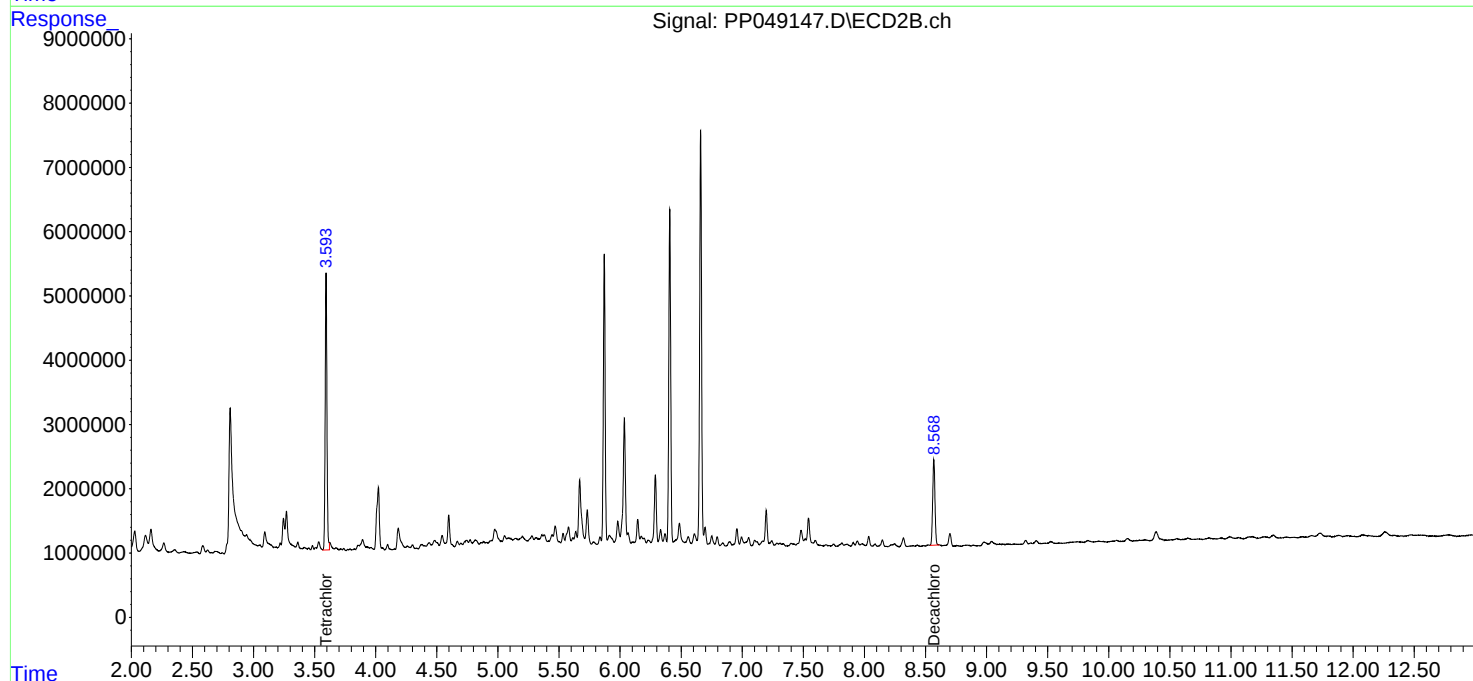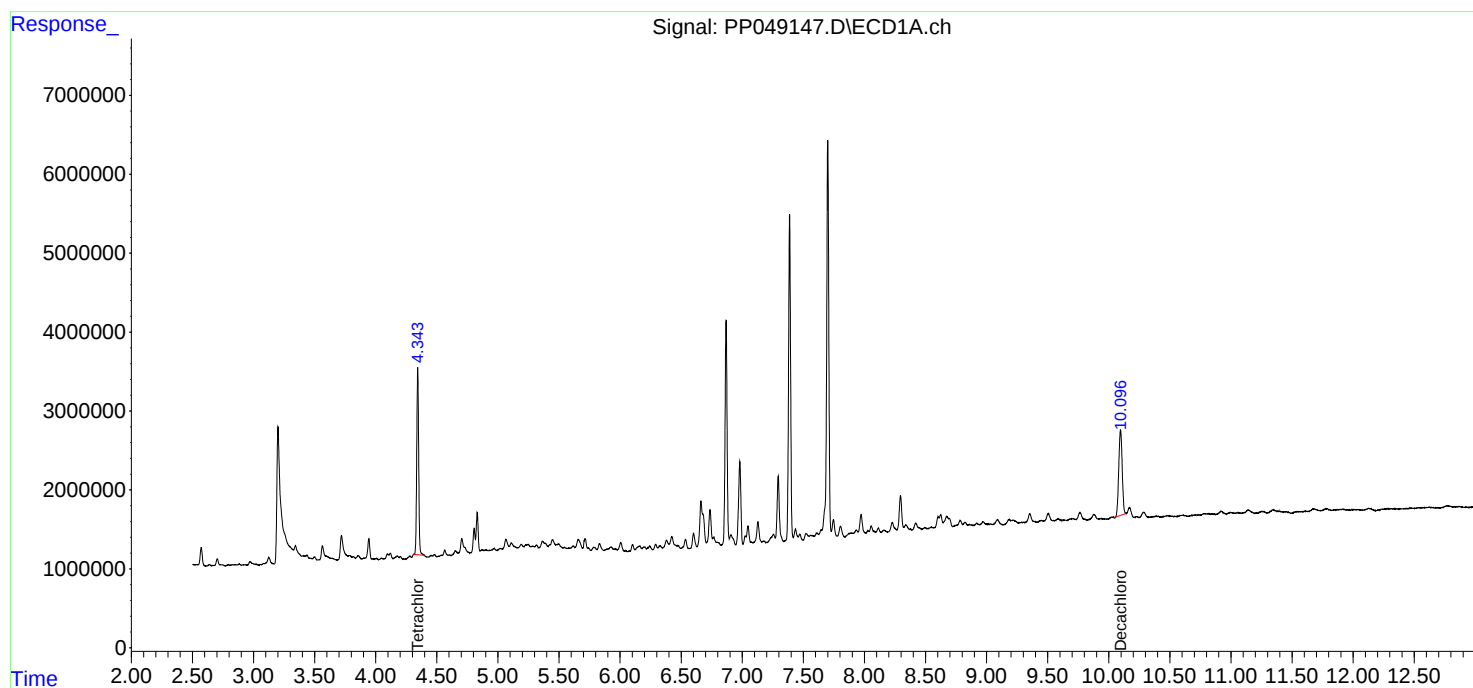

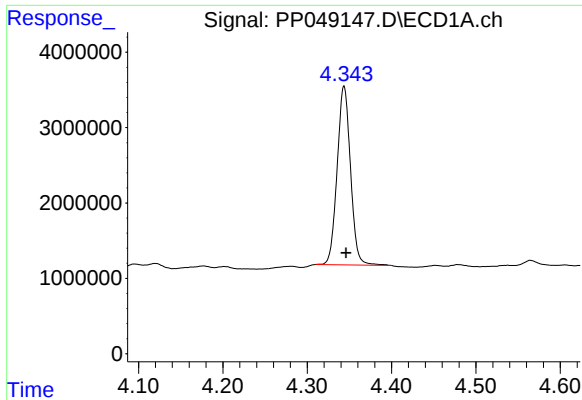


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 26099062
Conc: 18.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-EXC-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

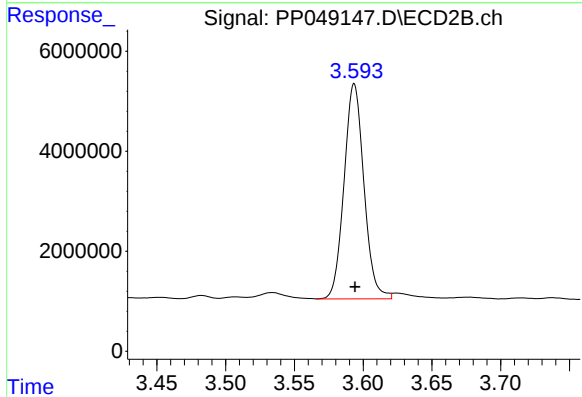


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: -0.001 min
Response: 43398260
Conc: 16.95 ng/ml m

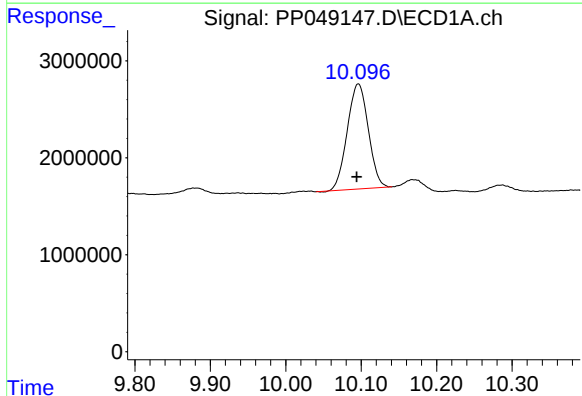

#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.002 min
Response: 20975239
Conc: 17.10 ng/ml

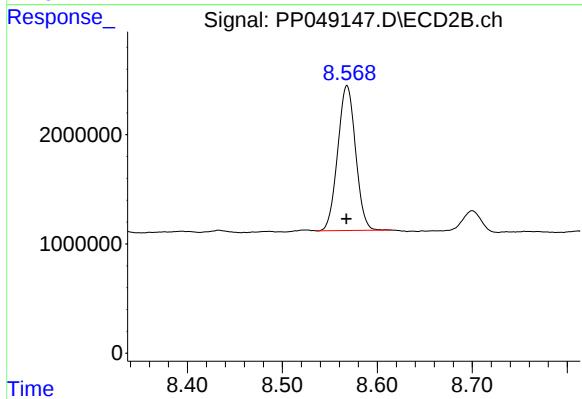

#2 Decachlorobiphenyl

R.T.: 8.568 min
Delta R.T.: 0.000 min
Response: 17319655
Conc: 15.37 ng/ml