

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
 Data File : PP036992.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2021 16:46
 Operator : DD\AJ
 Sample : M2904-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:02:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.962	3.953	865052	546376	19.572	17.640
2)	SA Decachlor...	10.997	9.250	703468	422460	16.399	13.210
Target Compounds							
8)	L2 AR-1221-1	5.210	0.000	19678	0	35.050	N.D. #
9)	L2 AR-1221-2	5.316	0.000	10480	0	24.320	N.D. #
27)	L6 AR-1254-2	7.425	0.000	13749	0	5.081	N.D. #
28)	L6 AR-1254-3	7.819	6.680	43416	3177	14.657	1.307 #
30)	L6 AR-1254-5	8.553f	7.325	17266	11550	7.260	5.372 #
32)	L7 AR-1260-2	8.234	0.000	25063	0	9.779	N.D. #
36)	L8 AR-1262-1	0.000	7.325	0	11550	N.D.	9.691 #
45)	L9 AR-1268-5	10.670	0.000	22646	0	1.473	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
Data File : PP036992.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2021 16:46
Operator : DD\AJ
Sample : M2904-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:02:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

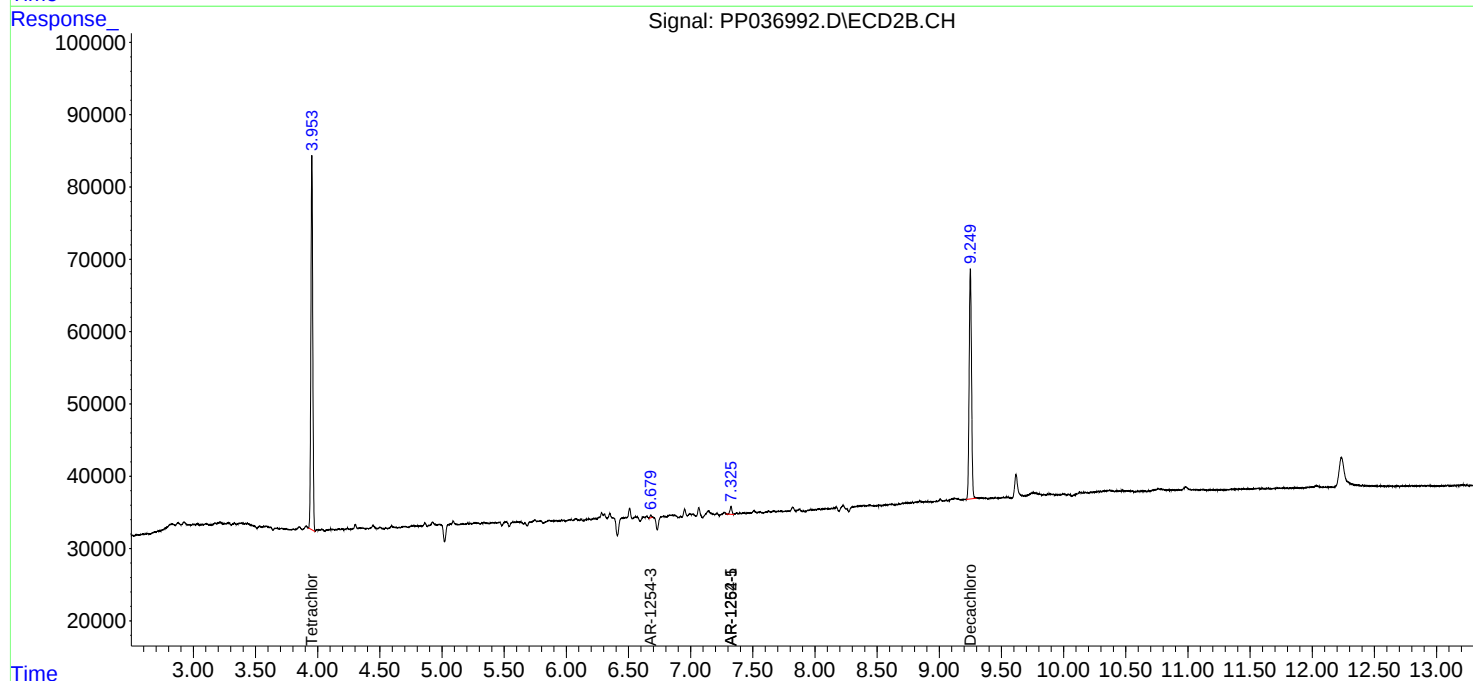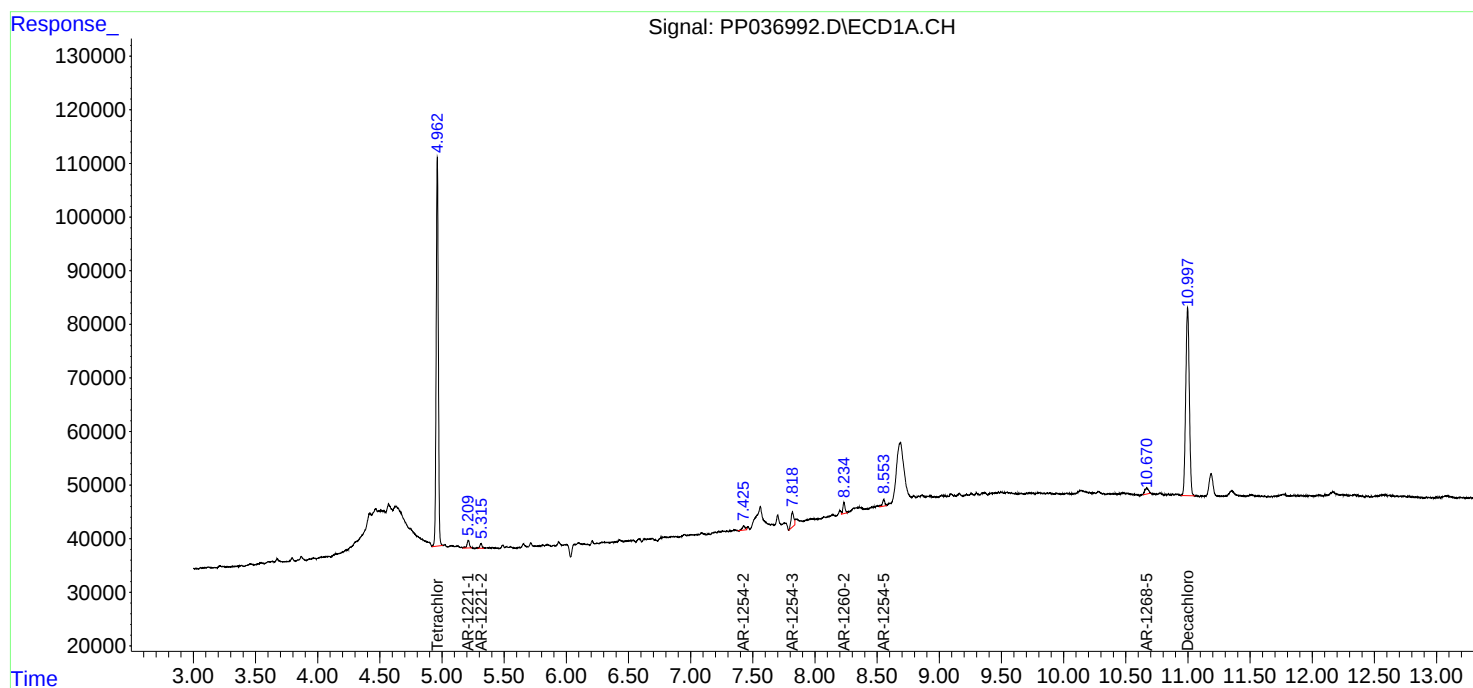


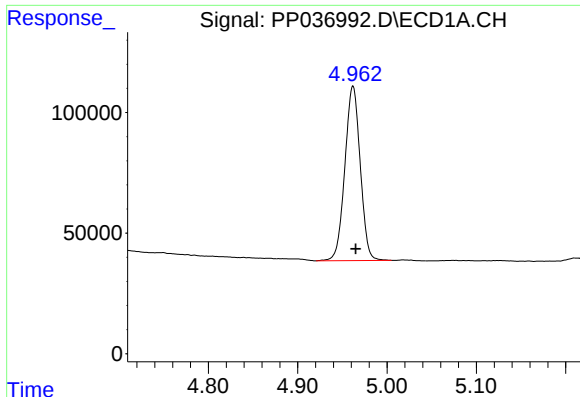

#1 Tetrachloro-m-xylene


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 865052
Conc: 19.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

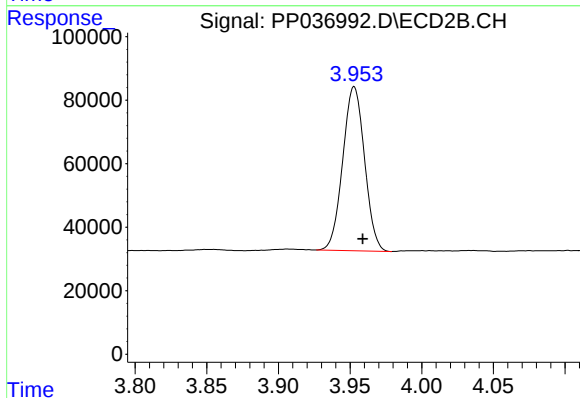


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.006 min
Response: 546376
Conc: 17.64 ng/ml

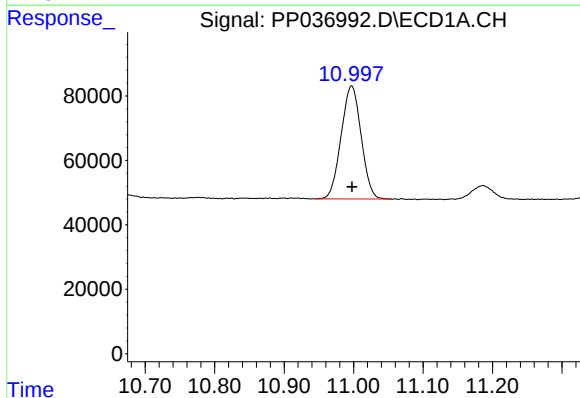


#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 703468
Conc: 16.40 ng/ml

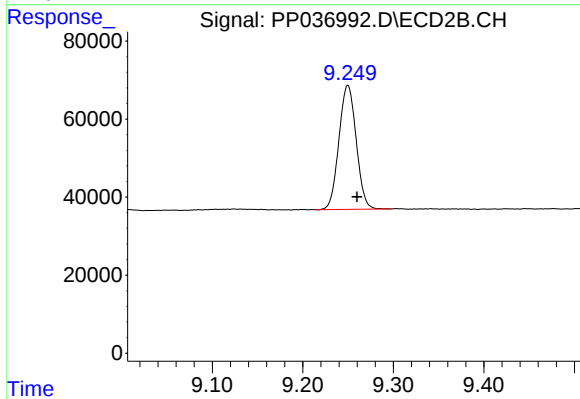

#2 Decachlorobiphenyl


R.T.: 9.250 min
Delta R.T.: -0.010 min
Response: 422460
Conc: 13.21 ng/ml

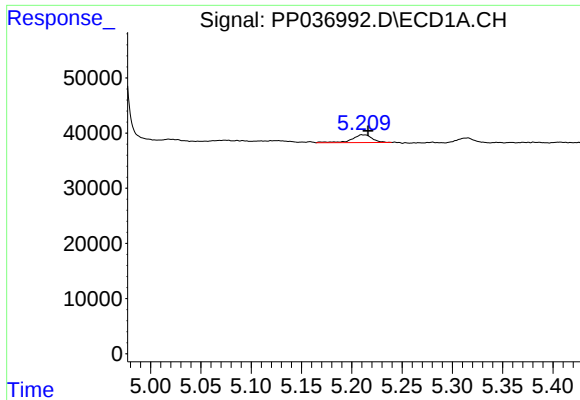

#8 AR-1221-1


R.T.: 5.210 min
Delta R.T.: -0.006 min
Response: 19678
Conc: 35.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

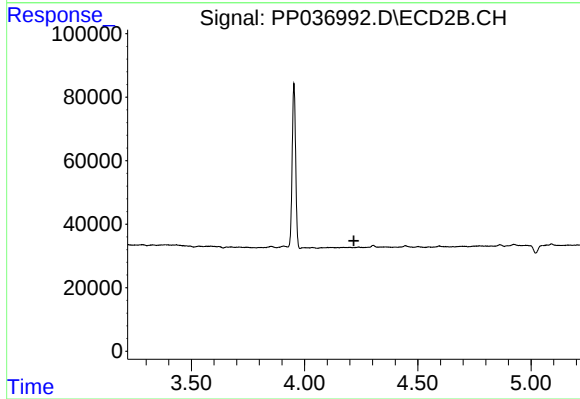


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

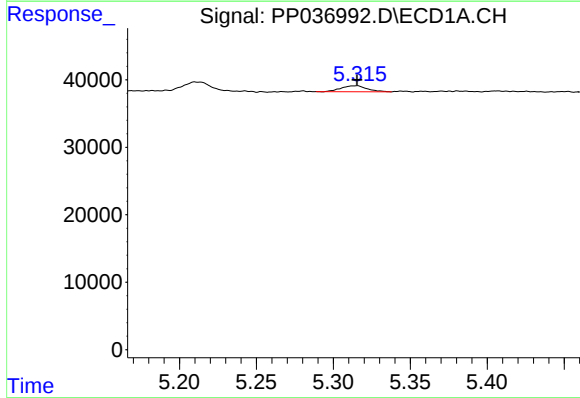


#9 AR-1221-2

R.T.: 5.316 min
Delta R.T.: 0.000 min
Response: 10480
Conc: 24.32 ng/ml

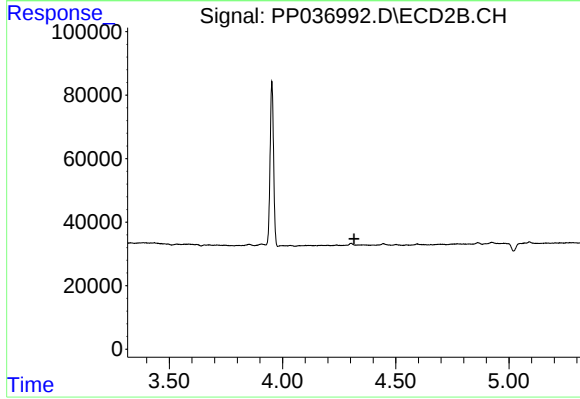

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

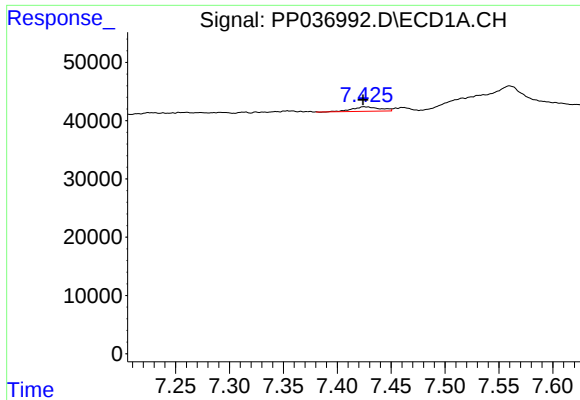

#27 AR-1254-2


R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 13749
Conc: 5.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

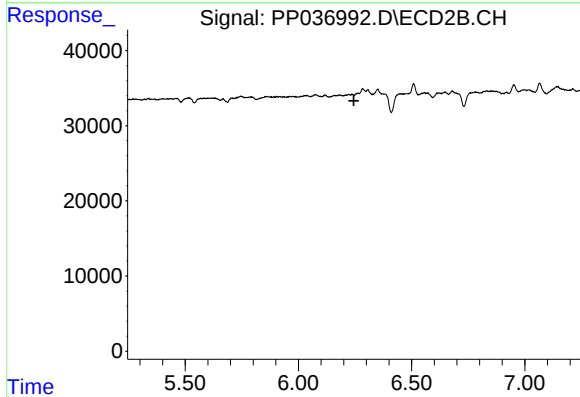


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

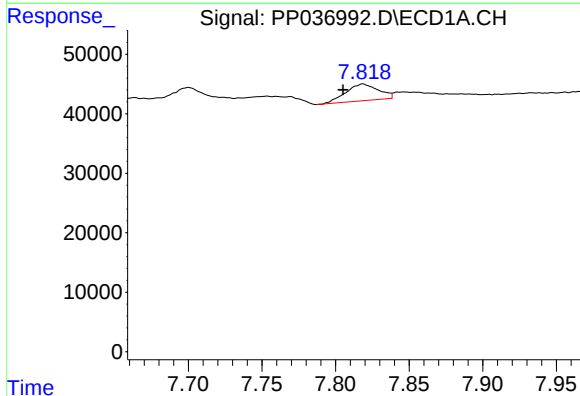


#28 AR-1254-3

R.T.: 7.819 min
Delta R.T.: 0.014 min
Response: 43416
Conc: 14.66 ng/ml

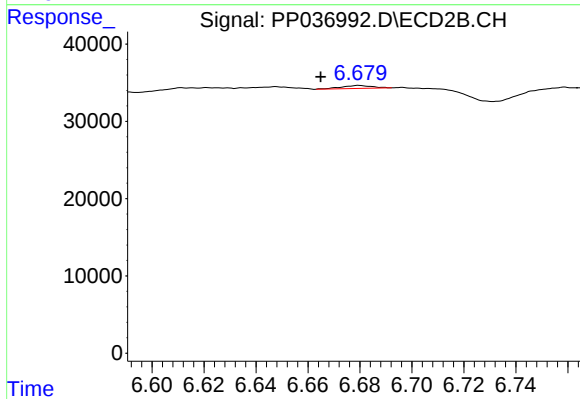

#28 AR-1254-3


R.T.: 6.680 min
Delta R.T.: 0.015 min
Response: 3177
Conc: 1.31 ng/ml

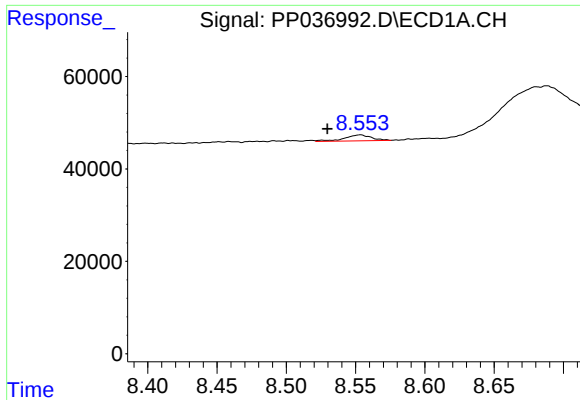

#30 AR-1254-5


R.T.: 8.553 min
Delta R.T.: 0.024 min
Response: 17266
Conc: 7.26 ng/ml

Instrument :
ECD_P
ClientSampleId :

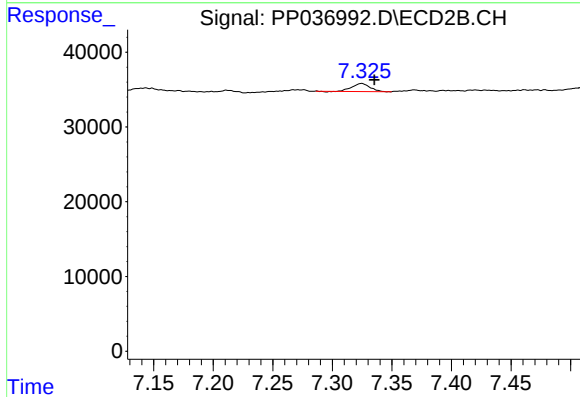


#30 AR-1254-5

R.T.: 7.325 min
Delta R.T.: -0.010 min
Response: 11550
Conc: 5.37 ng/ml

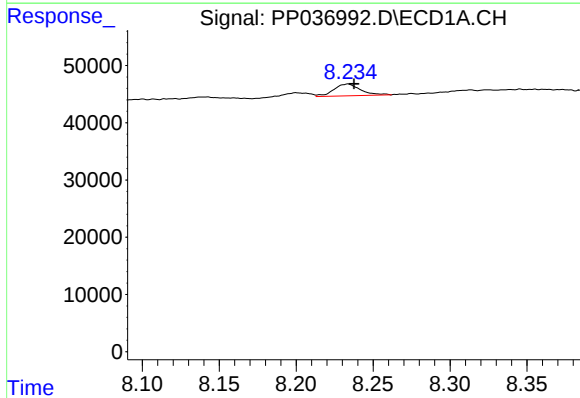


#32 AR-1260-2

R.T.: 8.234 min
Delta R.T.: -0.004 min
Response: 25063
Conc: 9.78 ng/ml

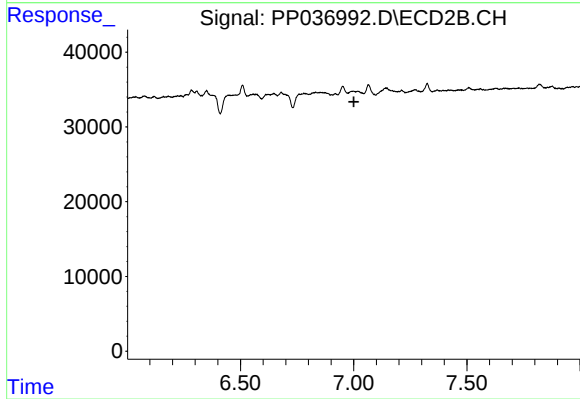

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.001 min
Response: 0
Conc: N.D.

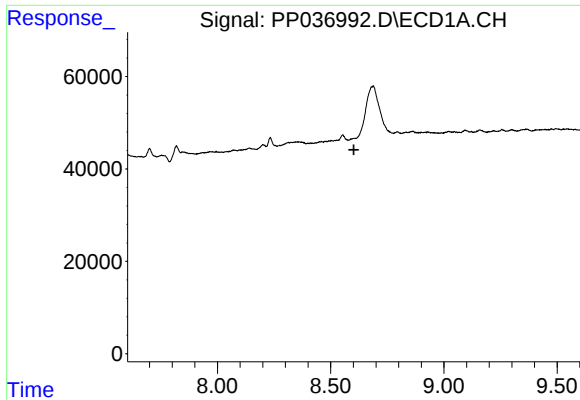

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

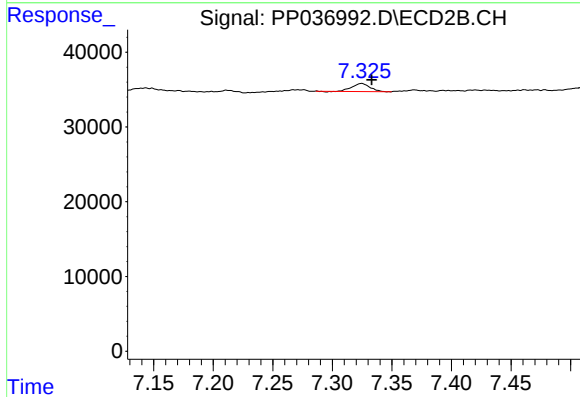


#36 AR-1262-1

R.T.: 7.325 min
Delta R.T.: -0.008 min
Response: 11550
Conc: 9.69 ng/ml

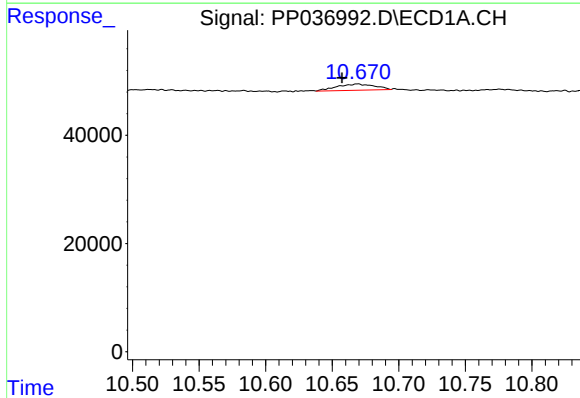

#45 AR-1268-5

R.T.: 10.670 min
Delta R.T.: 0.012 min
Response: 22646
Conc: 1.47 ng/ml

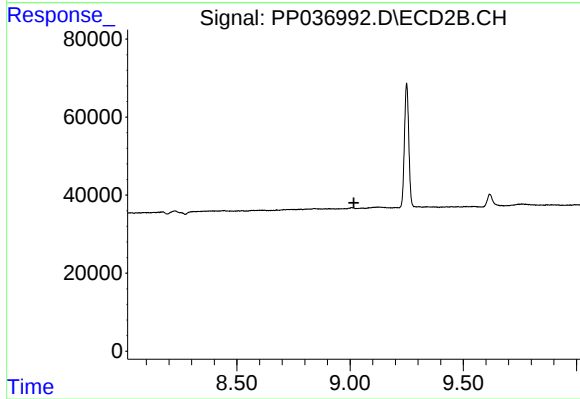

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.017 min
Response: 0
Conc: N.D.