

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
 Data File : PP036978.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2021 12:29
 Operator : DD\AJ
 Sample : M2915-02 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

mohammad
 7/6/2021 10:09:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:55:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.960	3.953	147579	116116	3.339m	3.749m
2) SA Decachlor...	10.997	9.252	223009	148157	5.199	4.633m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
Data File : PP036978.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2021 12:29
Operator : DD\AJ
Sample : M2915-02 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
02-A-02-B-02-C


Manual Integrations
APPROVED

mohammad
7/6/2021 10:09:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:55:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

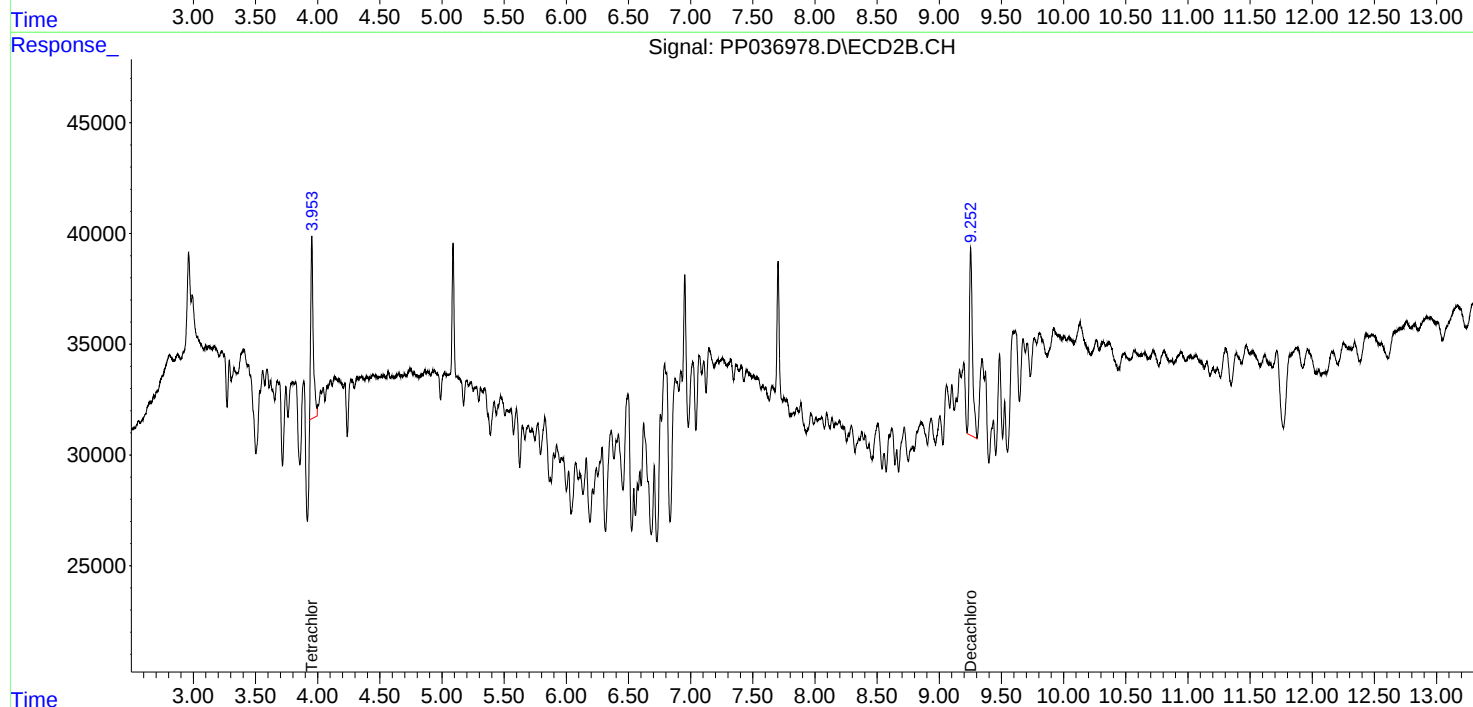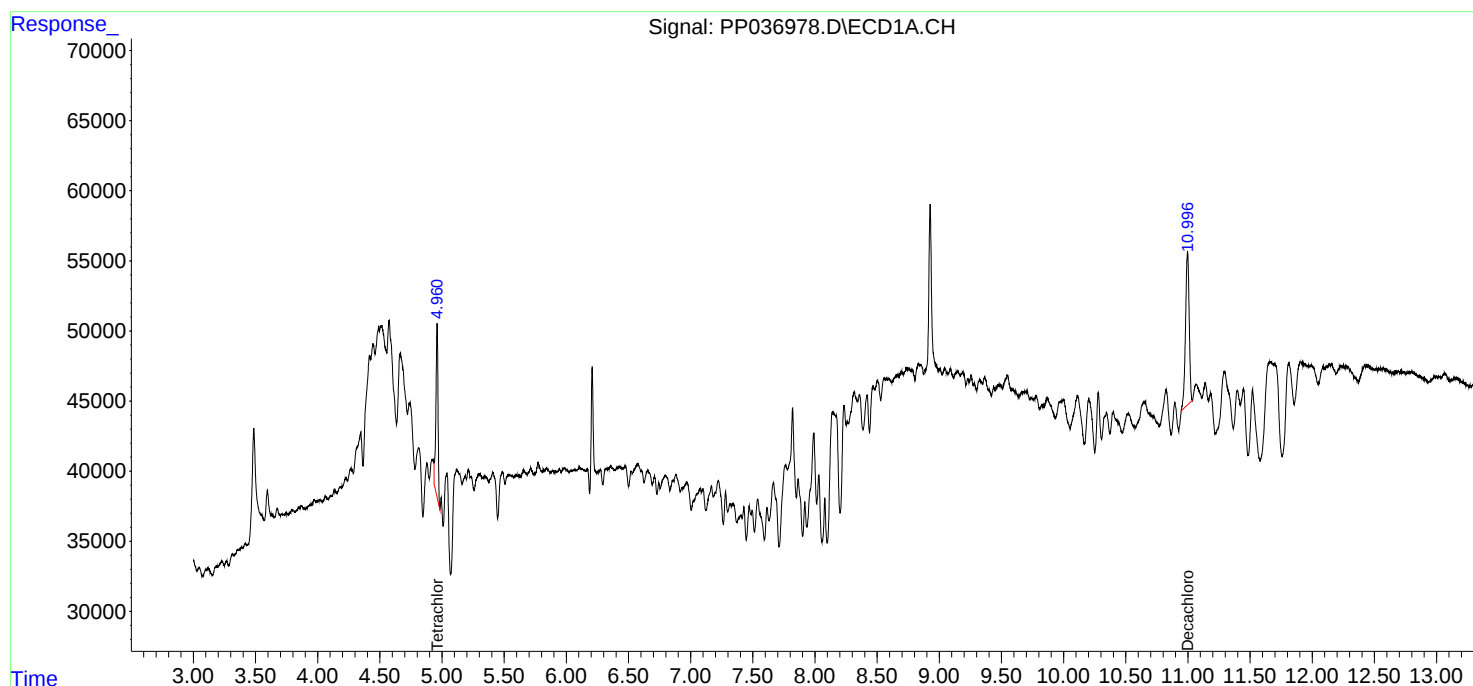

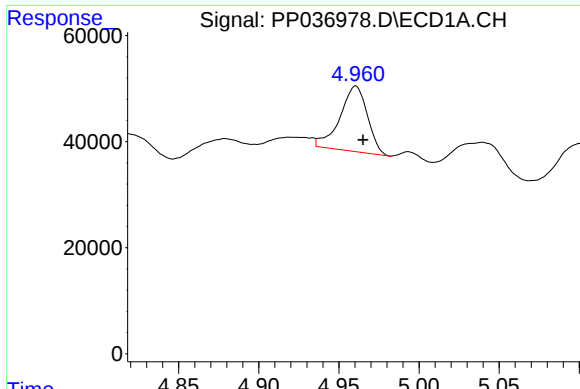


#1 Tetrachloro-m-xylene

R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 147579
Conc: 3.34 ng/ml m

Instrument :
ECD_P
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

mohammad
7/6/2021 10:09:40 AM

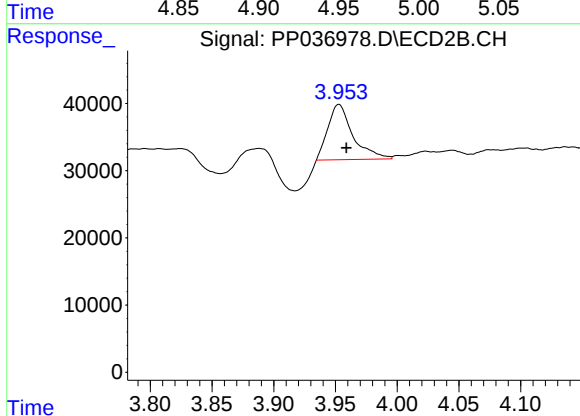


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.006 min
Response: 116116
Conc: 3.75 ng/ml m

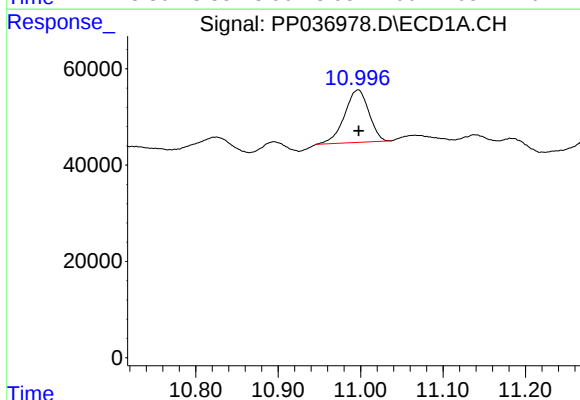

#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: -0.001 min
Response: 223009
Conc: 5.20 ng/ml

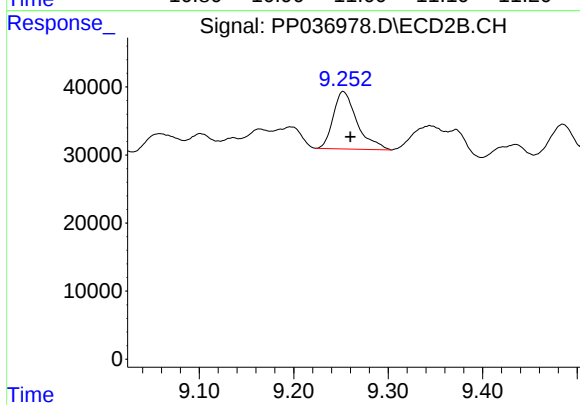

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.008 min
Response: 148157
Conc: 4.63 ng/ml m