

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
 Data File : PP037005.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2021 20:27
 Operator : DD\AJ
 Sample : M2919-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-01-B9-B9A-B10-B10A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:10:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.953	898567	575772	20.330	18.589
2) SA Decachlor...	10.996	9.250	751571	451699	17.520	14.124

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
Data File : PP037005.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2021 20:27
Operator : DD\AJ
Sample : M2919-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B9-B9A-B10-B10A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:10:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

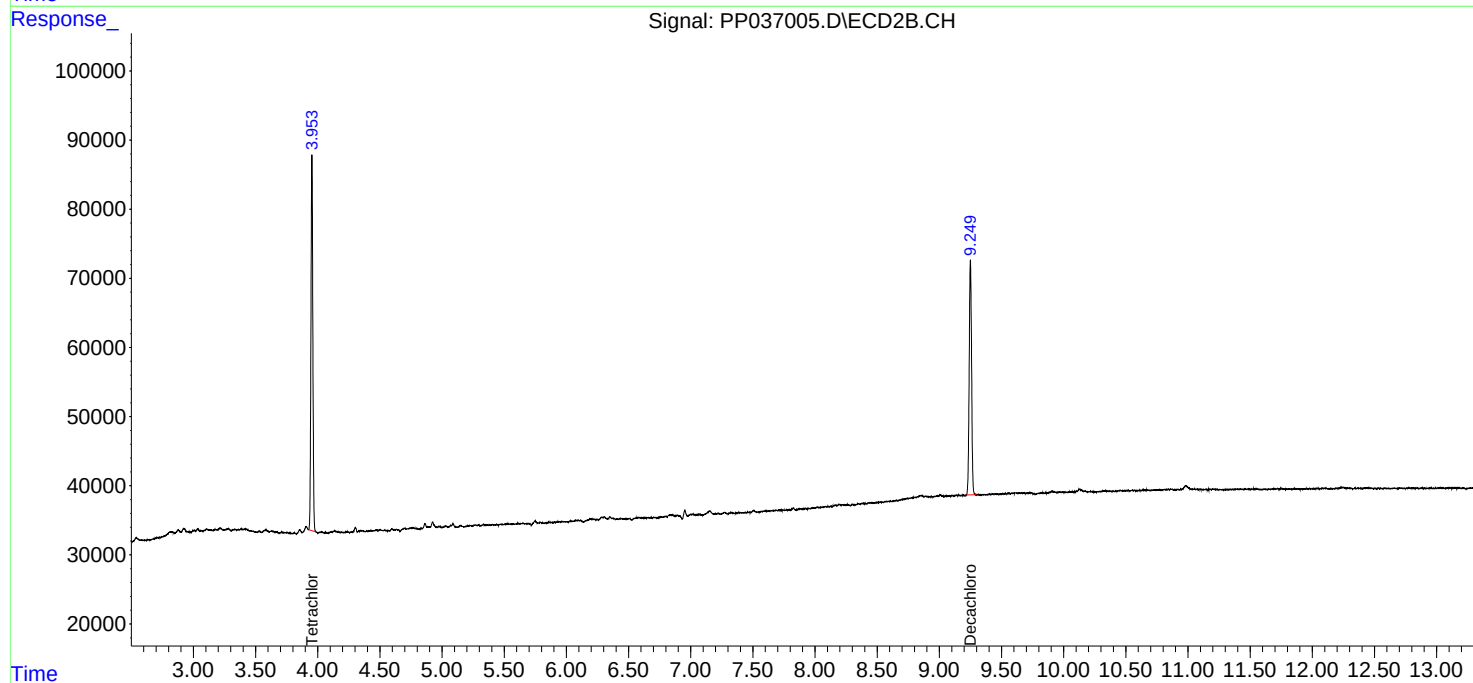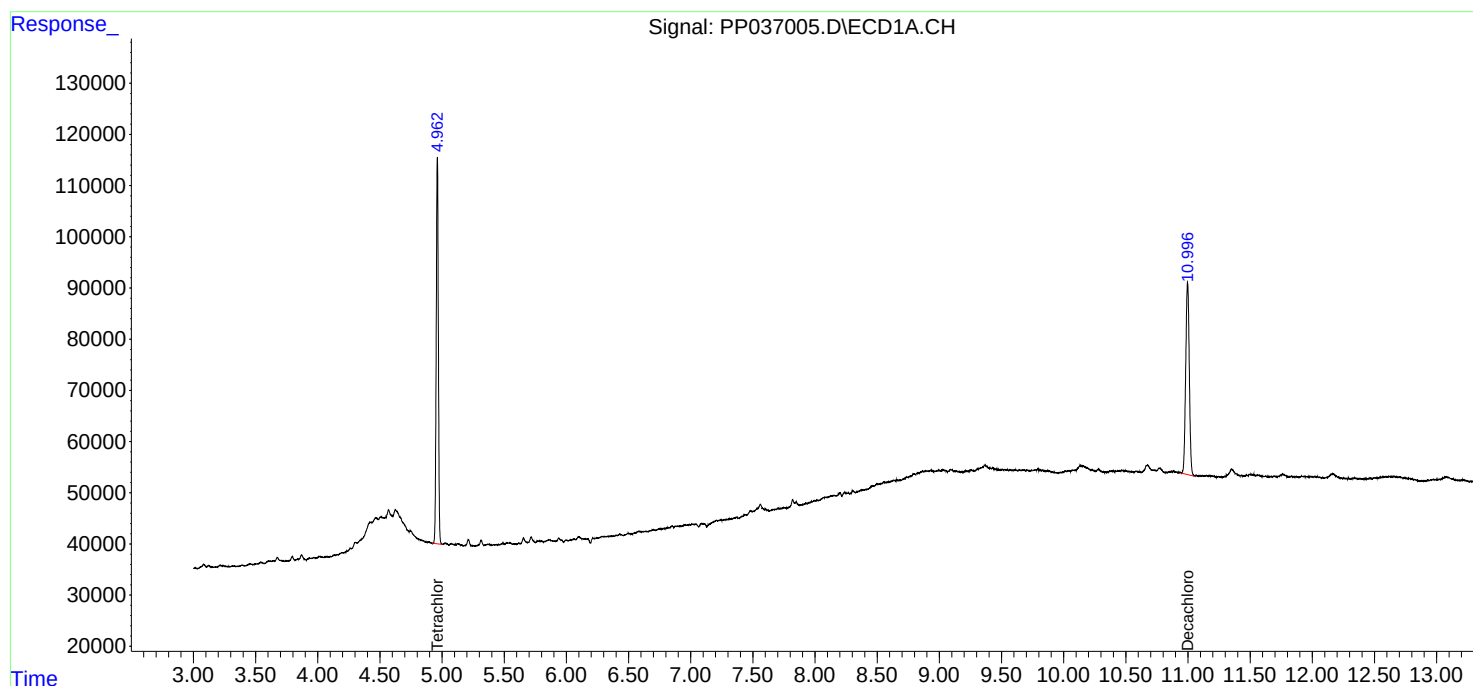


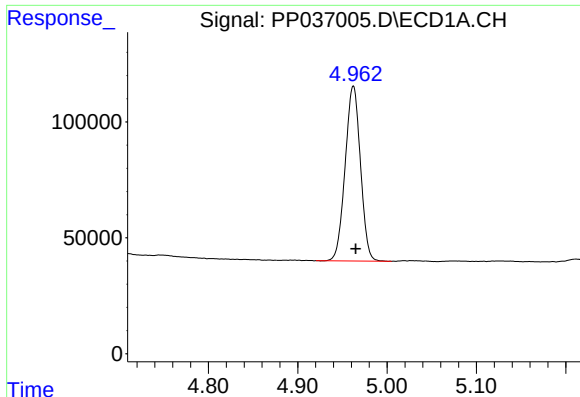

#1 Tetrachloro-m-xylene


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 898567
Conc: 20.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-B9-B9A-B10-B10A

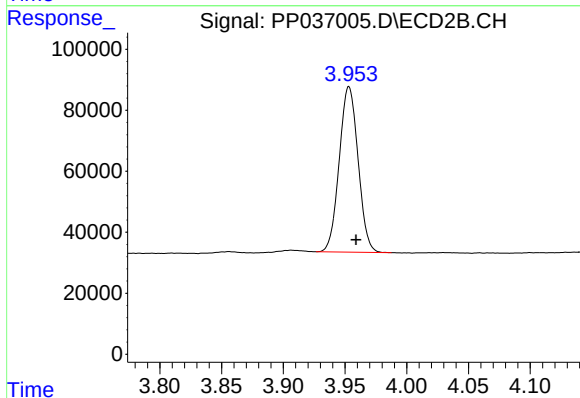


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.006 min
Response: 575772
Conc: 18.59 ng/ml

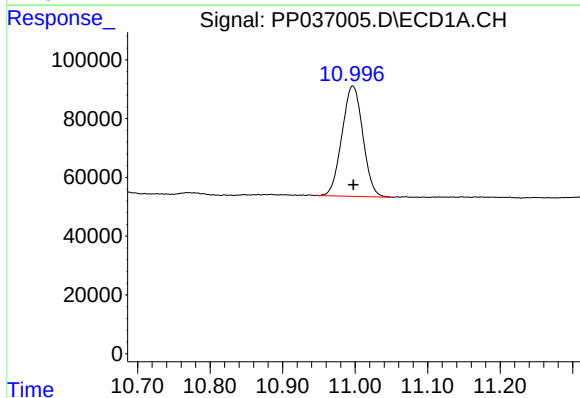

#2 Decachlorobiphenyl

R.T.: 10.996 min
Delta R.T.: -0.001 min
Response: 751571
Conc: 17.52 ng/ml

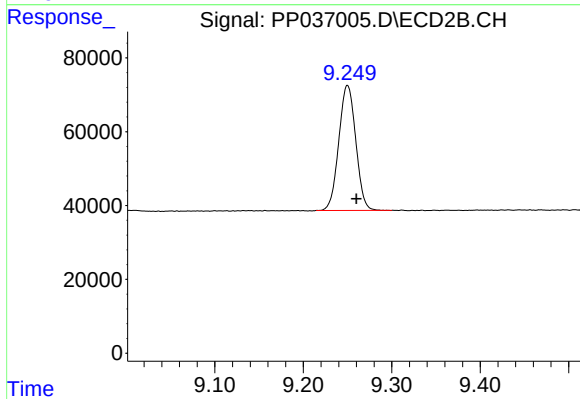

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.010 min
Response: 451699
Conc: 14.12 ng/ml