

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
 Data File : PP037012.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2021 22:42
 Operator : DD\AJ
 Sample : M2915-06RE
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 06-A-06-B-06-CRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:14:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.960	3.952	701682	486921	15.876m	15.721

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070221\
Data File : PP037012.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2021 22:42
Operator : DD\AJ
Sample : M2915-06RE
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
06-A-06-B-06-CRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:14:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

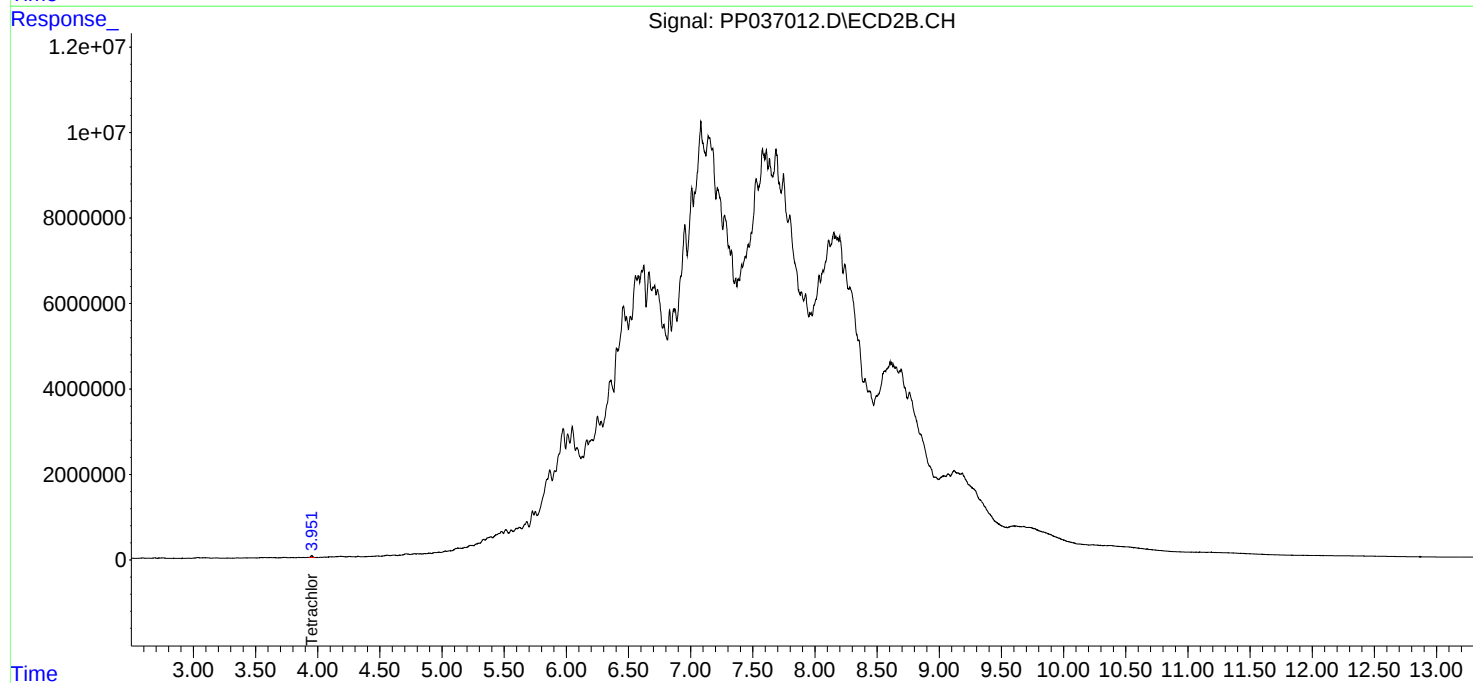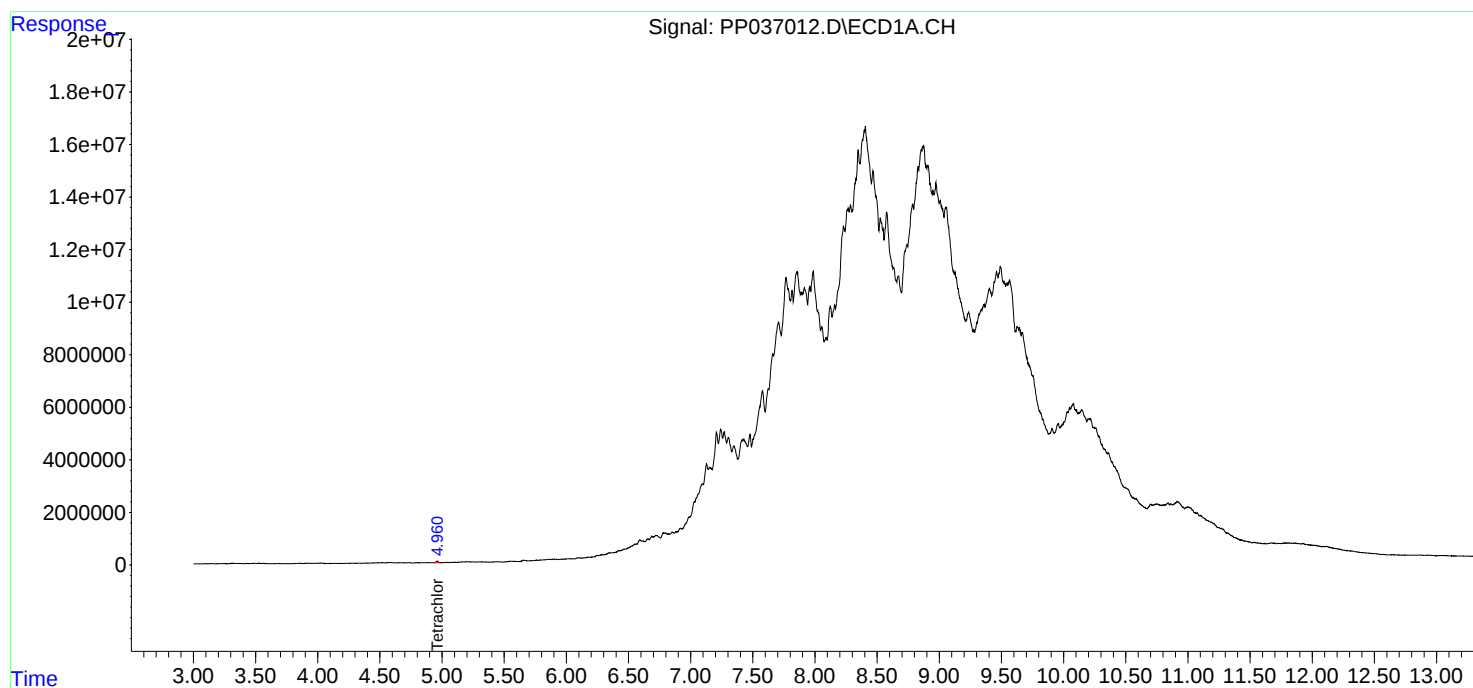

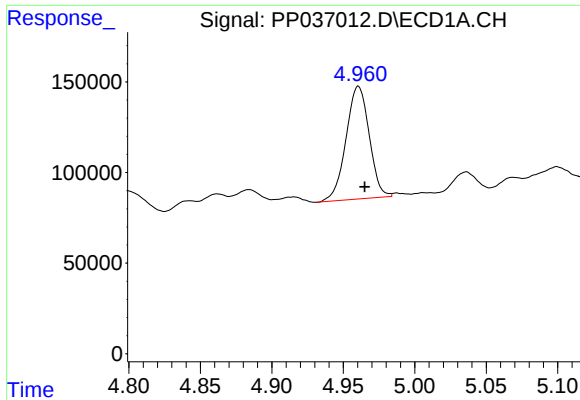

#1 Tetrachloro-m-xylene


R.T.: 4.960 min

Delta R.T.: -0.005 min

Response: 701682

Conc: 15.88 ng/ml m

Instrument :
ECD_P
ClientSampleId :
06-A-06-B-06-CRE

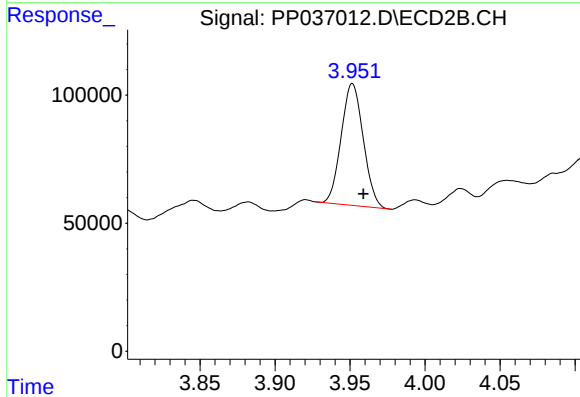


#1 Tetrachloro-m-xylene

R.T.: 3.952 min

Delta R.T.: -0.007 min

Response: 486921

Conc: 15.72 ng/ml

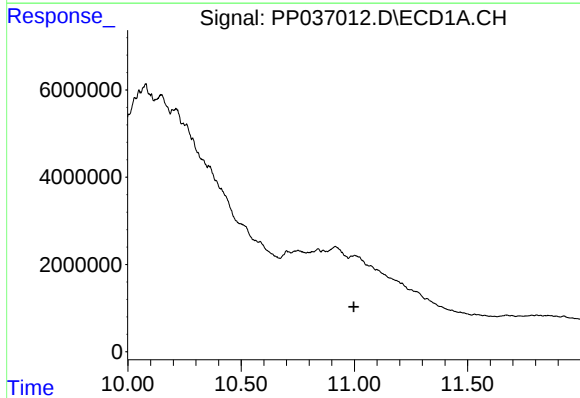


#2 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 10.998 min

Response: 0

Conc: N.D.

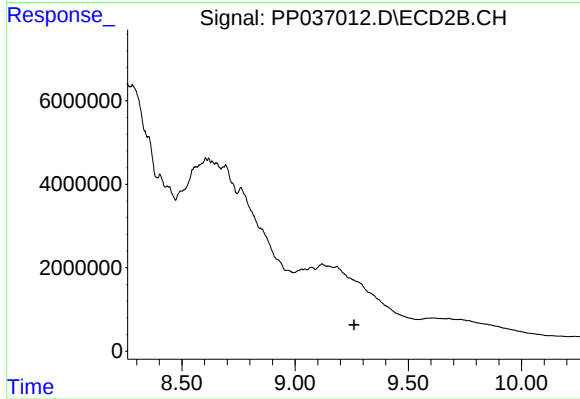

#2 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 9.260 min

Response: 0

Conc: N.D.