

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
 Data File : PP073453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 11:34
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:35:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.493	3.819f	-28589	63199	N.D.	0.036
2)	SA Decachlor...	10.205	8.790	184357	131624	0.130	0.095 #
Target Compounds							
3)	L1 AR-1016-1	5.660	4.866	118794	306503	2.169	4.764 #
4)	L1 AR-1016-2	5.660	4.866	118794	306503	1.436	3.216 #
5)	L1 AR-1016-3	5.750	5.042	303138	196314	5.746	3.894 #
6)	L1 AR-1016-4	5.864f	5.099	305631	493848	6.942	12.147 #
7)	L1 AR-1016-5	6.134	5.327	859453	55319	21.376	1.079 #
8)	L2 AR-1221-1	4.728f	4.007	171236	295579	9.073	10.982
9)	L2 AR-1221-2	4.783	4.055	107534	353991	6.673	17.217 #
10)	L2 AR-1221-3	4.848	4.150	109872	98741	2.124	1.627
11)	L3 AR-1232-1	4.848	4.150	109872	98741	2.749	2.098
12)	L3 AR-1232-2	5.383	4.866	72443	306503	3.523	6.521 #
13)	L3 AR-1232-3	5.660	5.042	118794	196314	2.806	7.927 #
14)	L3 AR-1232-4	5.864f	5.139	305631	129740	14.179	6.056 #
15)	L3 AR-1232-5	5.944	5.299	661552	70434	47.036	3.014 #
16)	L4 AR-1242-1	5.660	4.866	118794	306503	2.338	5.248 #
17)	L4 AR-1242-2	5.660	4.866	118794	306503	1.567	3.553 #
18)	L4 AR-1242-3	5.750	5.042	303138	196314	6.311	4.278 #
19)	L4 AR-1242-4	5.864f	5.139	305631	129740	7.937	2.955 #
20)	L4 AR-1242-5	6.548	5.646	482633	366056	11.355	6.690 #
21)	L5 AR-1248-1	5.660	4.866	118794	306503	3.037	6.967 #
22)	L5 AR-1248-2	5.944	5.099	661552	493848	12.819	8.384 #
23)	L5 AR-1248-3	6.134	5.139	859453	129740	15.167	2.150 #
24)	L5 AR-1248-4	6.548f	5.327	482633	55319	6.857	0.776 #
25)	L5 AR-1248-5	6.548	5.684	482633	332682	6.896	4.523 #
26)	L6 AR-1254-1	6.466	5.646	4300744	366056	60.632	3.341 #
27)	L6 AR-1254-2	6.701	5.829	4964740	4802786	48.136	49.523
28)	L6 AR-1254-3	7.073	6.226	5765216	2975980	50.716	20.198 #
29)	L6 AR-1254-4	7.323	6.454	291749	290037	2.933	3.215
30)	L6 AR-1254-5	7.784	6.852	530.4E6	618.8E6	5596.025	4649.997
31)	L7 AR-1260-1	7.220	6.354	364242	64355	5.108	0.697 #
32)	L7 AR-1260-2	7.472	6.533	884.3E6	5725893	8412.914	46.328 #
33)	L7 AR-1260-3	7.853	6.659	1696924	-13076	18.414	N.D. #
34)	L7 AR-1260-4	8.080	7.115f	845874	295153	9.573	3.400 #
35)	L7 AR-1260-5	8.360	7.392	38646	84317	0.196	0.386 #
36)	L8 AR-1262-1	8.080	6.852f	845874	618.8E6	7.341	4123.887 #
37)	L8 AR-1262-2	8.360	7.115f	38646	295153	0.155	2.364 #
38)	L8 AR-1262-3	8.705	7.659	396448	92496	2.428	0.832 #
39)	L8 AR-1262-4	8.767	7.720	742671	541605	6.087	2.971 #
40)	L8 AR-1262-5	9.437	8.179f	477625	40642	5.493	0.466 #
41)	L9 AR-1268-1	8.705	7.659	396448	92496	1.377	0.313 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
Data File : PP073453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 11:34
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:35:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.767	7.720	742671	541605	2.976	2.068 #
43)	L9 AR-1268-3	9.007	7.945	432239	57925	1.965	0.264 #
44)	L9 AR-1268-4	9.437	8.179f	477625	40642	4.982	0.430 #
45)	L9 AR-1268-5	9.850	8.543	92040	98602	0.148	0.159



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
Data File : PP073453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 11:34
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:35:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

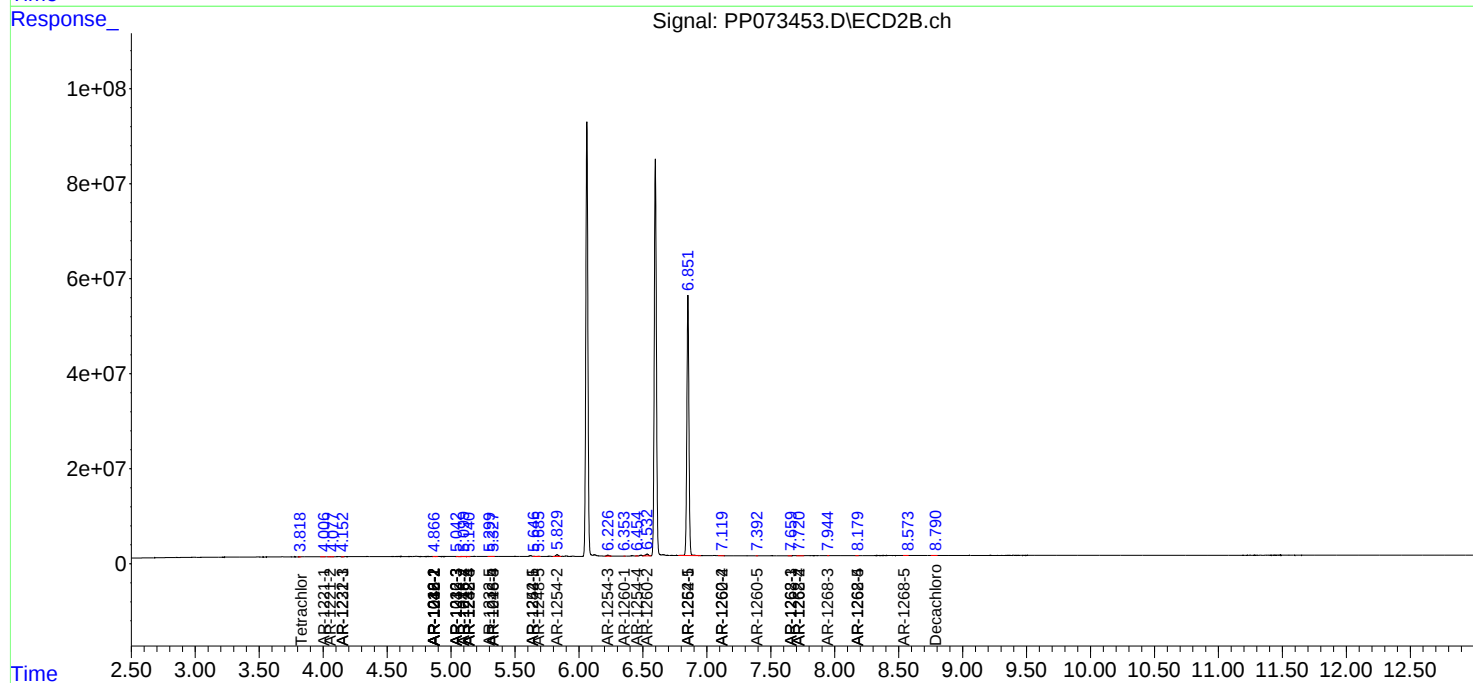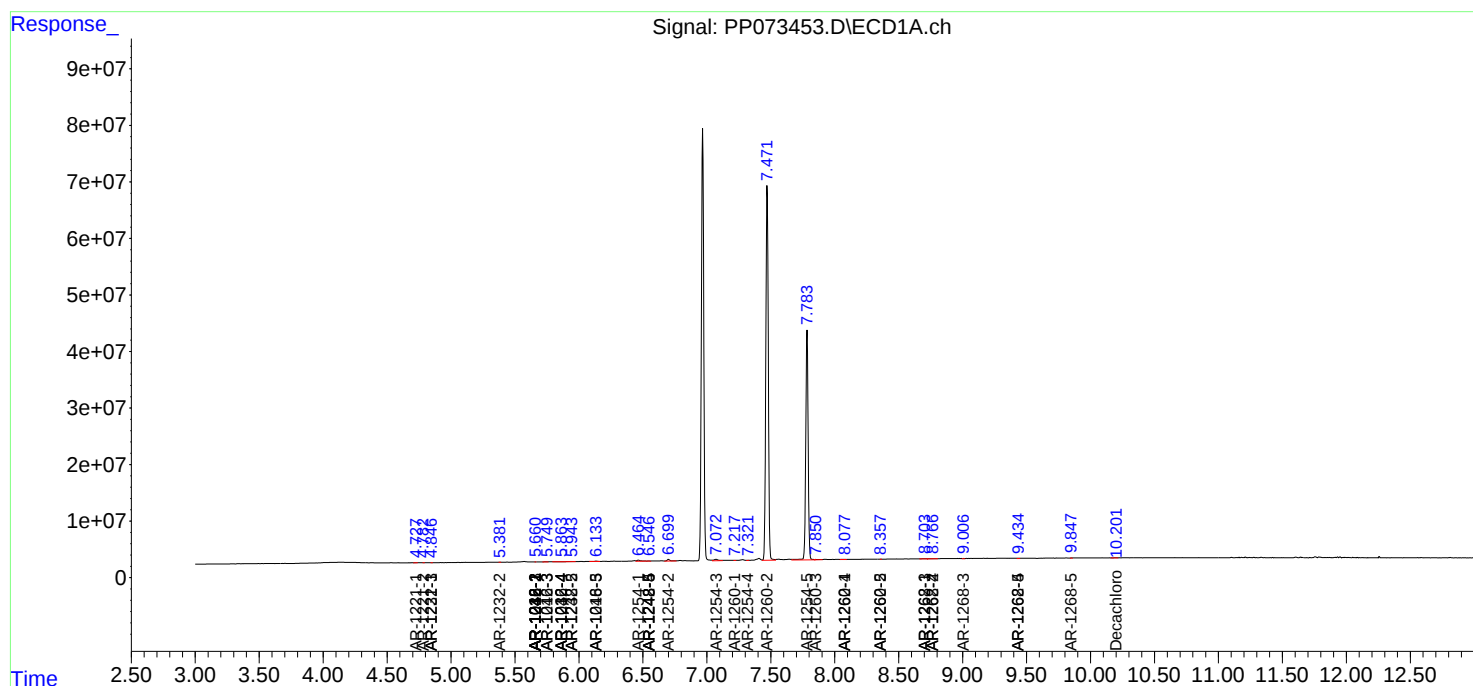


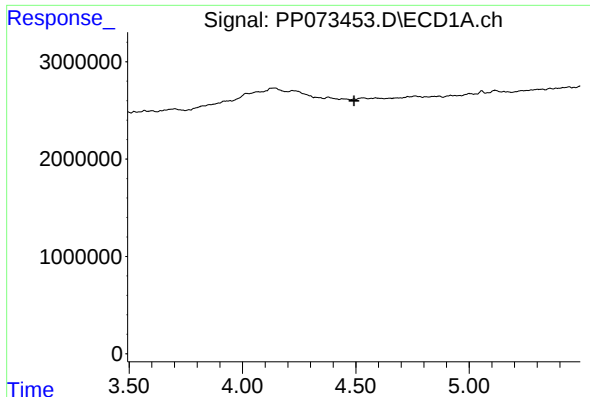

#1 Tetrachloro-m-xylene


R.T.: 4.493 min
Delta R.T.: 0.000 min
Response: -28589
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

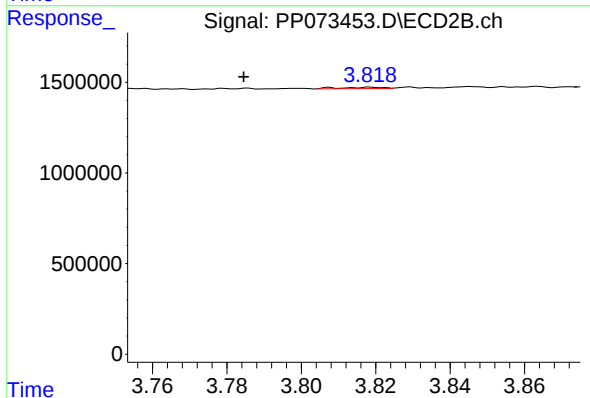


#1 Tetrachloro-m-xylene

R.T.: 3.819 min
Delta R.T.: 0.034 min
Response: 63199
Conc: 0.04 ng/ml

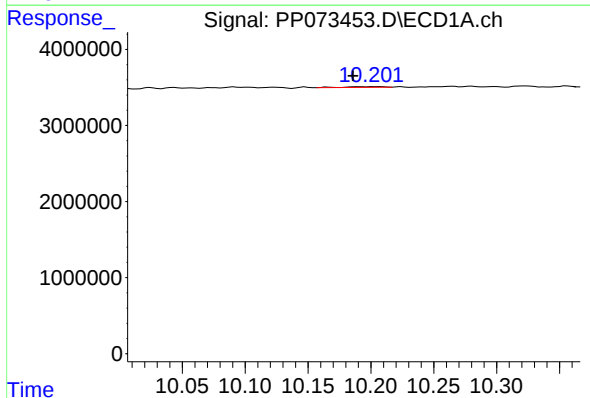


#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.019 min
Response: 184357
Conc: 0.13 ng/ml

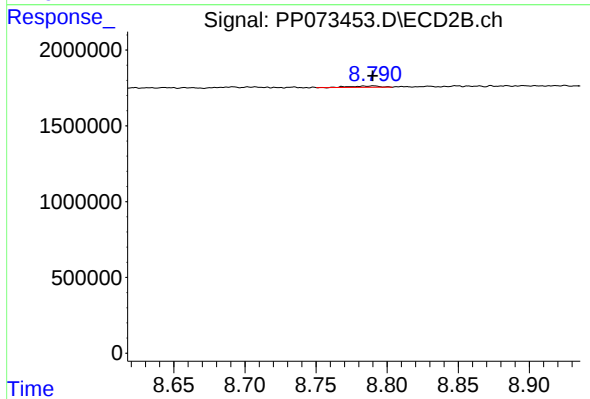

#2 Decachlorobiphenyl


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 131624
Conc: 0.10 ng/ml

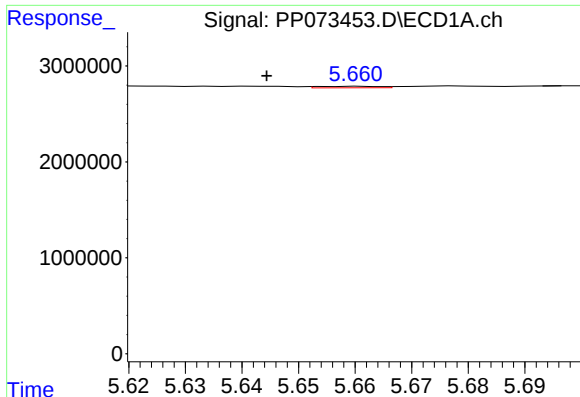

#3 AR-1016-1


R.T.: 5.660 min
Delta R.T.: 0.016 min
Response: 118794
Conc: 2.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

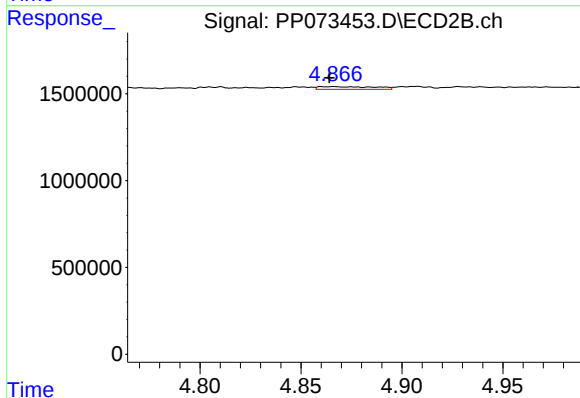


#3 AR-1016-1

R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 306503
Conc: 4.76 ng/ml

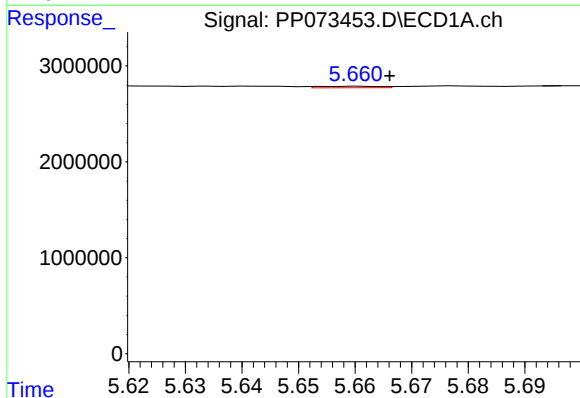


#4 AR-1016-2

R.T.: 5.660 min
Delta R.T.: -0.006 min
Response: 118794
Conc: 1.44 ng/ml

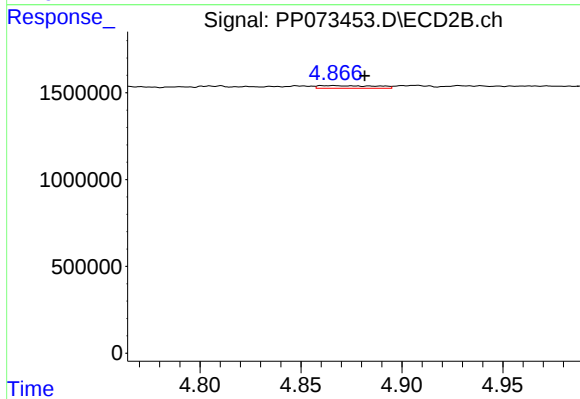

#4 AR-1016-2


R.T.: 4.866 min
Delta R.T.: -0.015 min
Response: 306503
Conc: 3.22 ng/ml

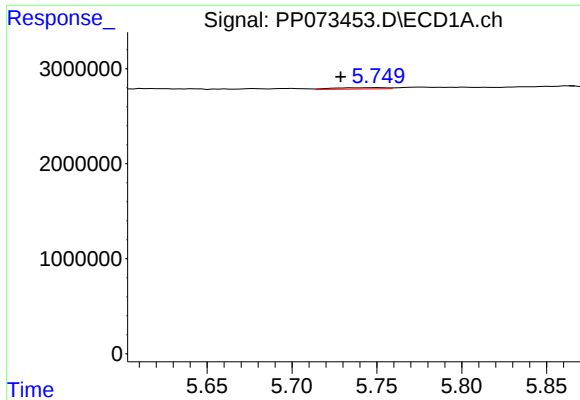

#5 AR-1016-3


R.T.: 5.750 min
Delta R.T.: 0.022 min
Response: 303138
Conc: 5.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

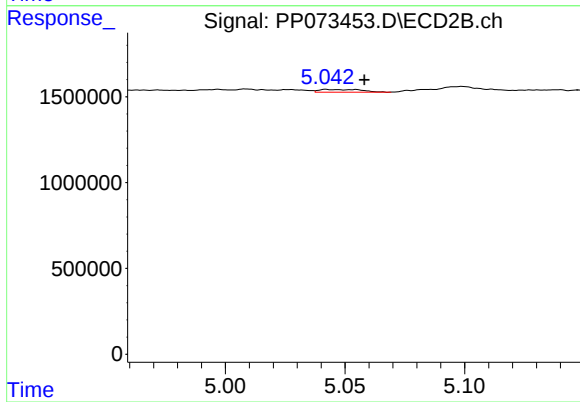


#5 AR-1016-3

R.T.: 5.042 min
Delta R.T.: -0.016 min
Response: 196314
Conc: 3.89 ng/ml

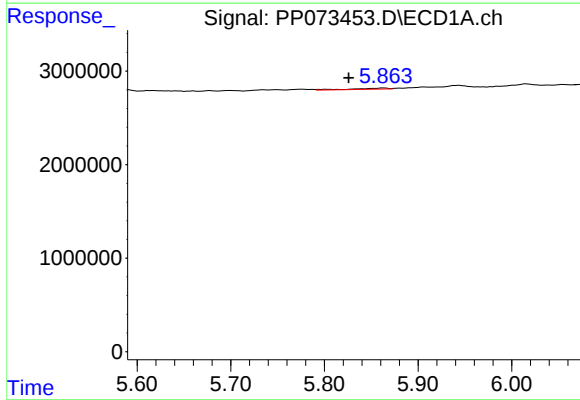


#6 AR-1016-4

R.T.: 5.864 min
Delta R.T.: 0.038 min
Response: 305631
Conc: 6.94 ng/ml

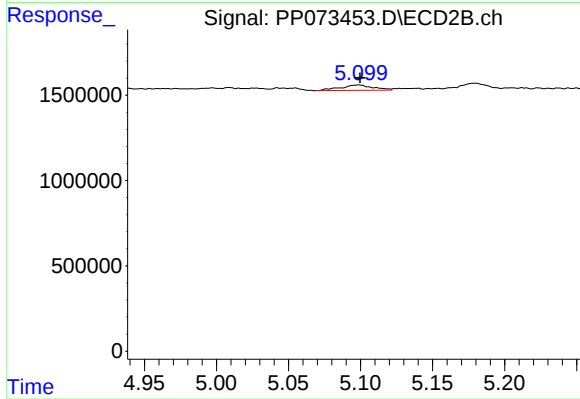

#6 AR-1016-4


R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 493848
Conc: 12.15 ng/ml

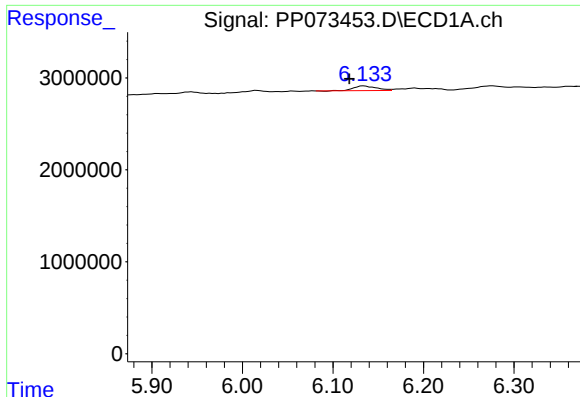

#7 AR-1016-5


R.T.: 6.134 min
Delta R.T.: 0.016 min
Response: 859453
Conc: 21.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

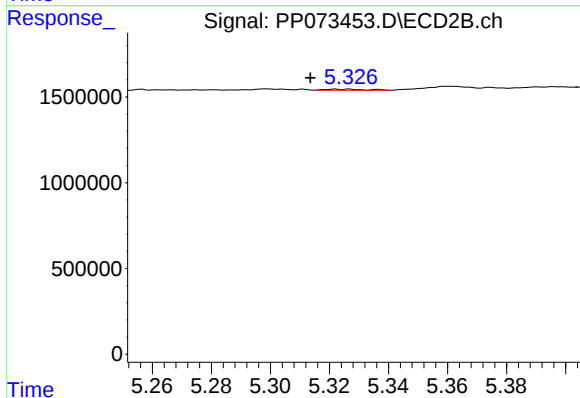


#7 AR-1016-5

R.T.: 5.327 min
Delta R.T.: 0.013 min
Response: 55319
Conc: 1.08 ng/ml

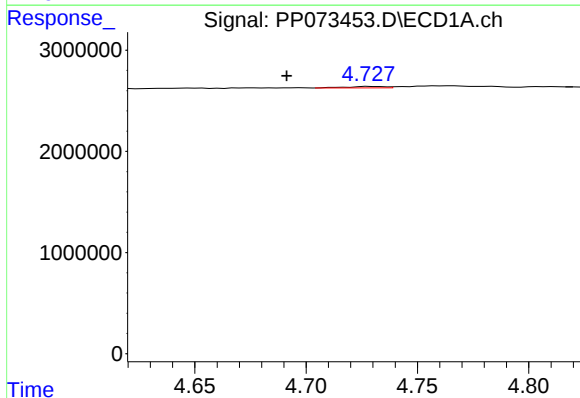


#8 AR-1221-1

R.T.: 4.728 min
Delta R.T.: 0.037 min
Response: 171236
Conc: 9.07 ng/ml

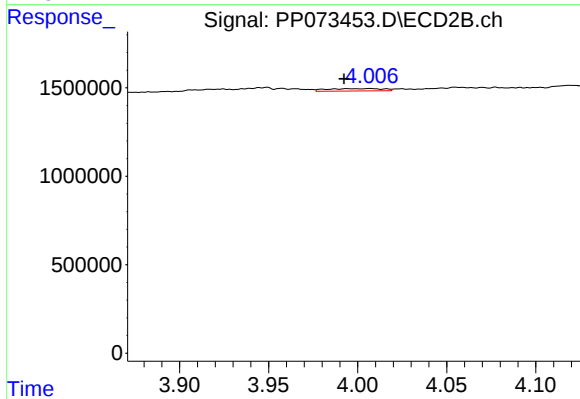

#8 AR-1221-1


R.T.: 4.007 min
Delta R.T.: 0.015 min
Response: 295579
Conc: 10.98 ng/ml

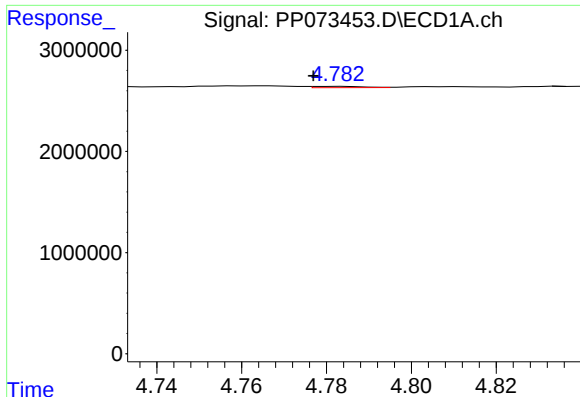

#9 AR-1221-2


R.T.: 4.783 min
Delta R.T.: 0.006 min
Response: 107534
Conc: 6.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

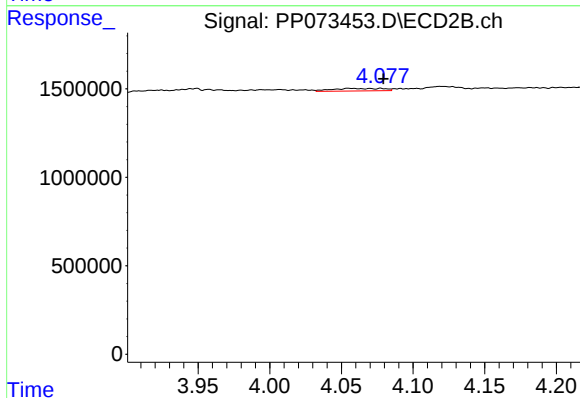


#9 AR-1221-2

R.T.: 4.055 min
Delta R.T.: -0.024 min
Response: 353991
Conc: 17.22 ng/ml

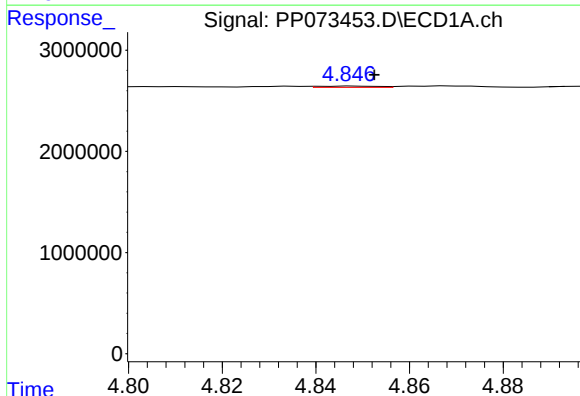


#10 AR-1221-3

R.T.: 4.848 min
Delta R.T.: -0.005 min
Response: 109872
Conc: 2.12 ng/ml

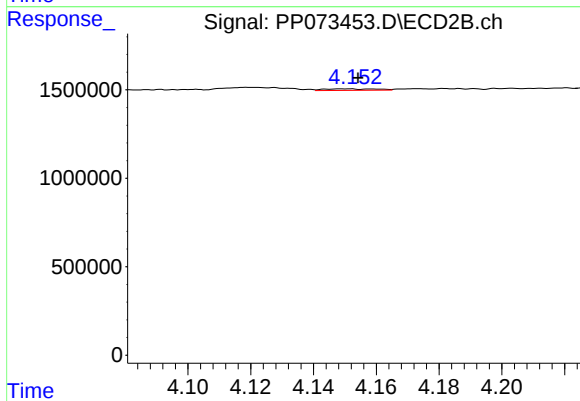

#10 AR-1221-3


R.T.: 4.150 min
Delta R.T.: -0.004 min
Response: 98741
Conc: 1.63 ng/ml

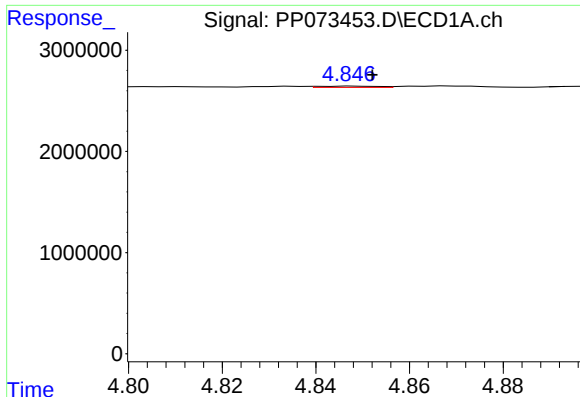

#11 AR-1232-1


R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 109872
Conc: 2.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

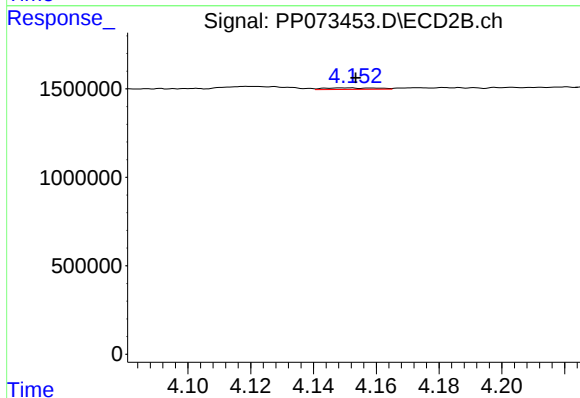


#11 AR-1232-1

R.T.: 4.150 min
Delta R.T.: -0.003 min
Response: 98741
Conc: 2.10 ng/ml

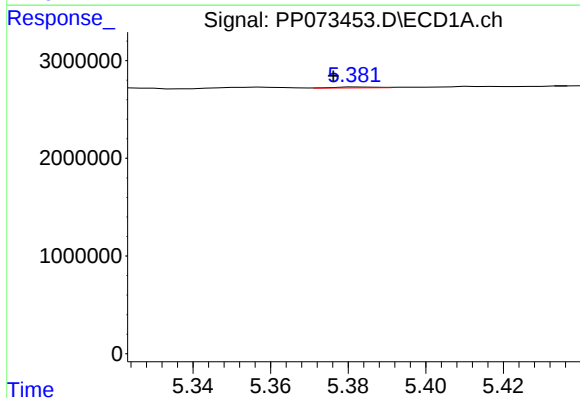


#12 AR-1232-2

R.T.: 5.383 min
Delta R.T.: 0.007 min
Response: 72443
Conc: 3.52 ng/ml

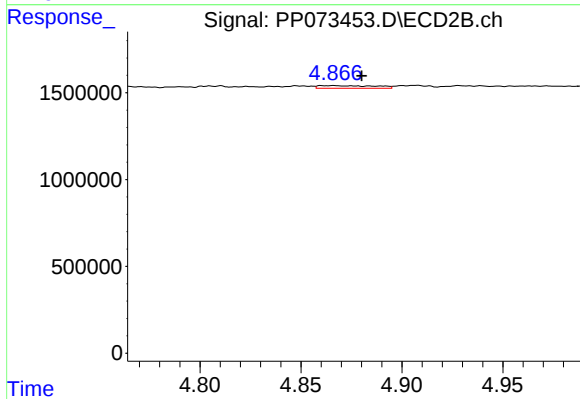

#12 AR-1232-2


R.T.: 4.866 min
Delta R.T.: -0.014 min
Response: 306503
Conc: 6.52 ng/ml

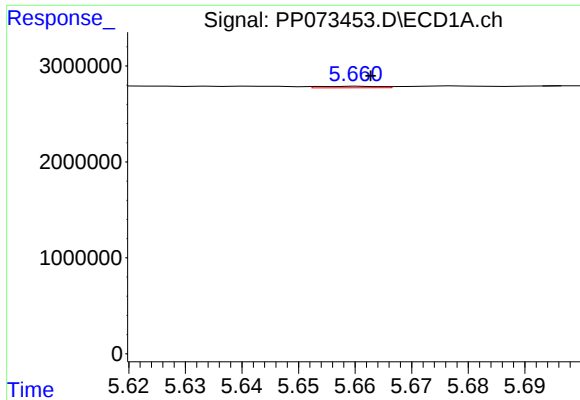

#13 AR-1232-3


R.T.: 5.660 min
Delta R.T.: -0.002 min
Response: 118794
Conc: 2.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

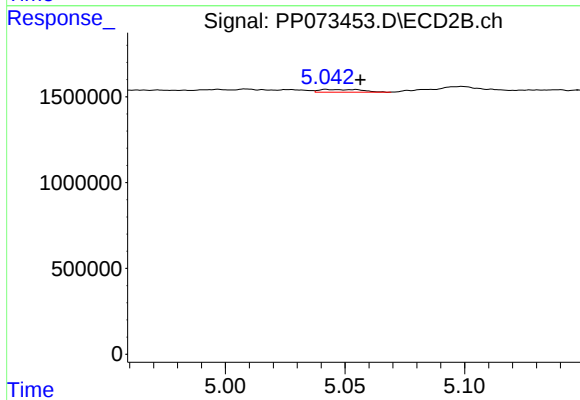


#13 AR-1232-3

R.T.: 5.042 min
Delta R.T.: -0.014 min
Response: 196314
Conc: 7.93 ng/ml

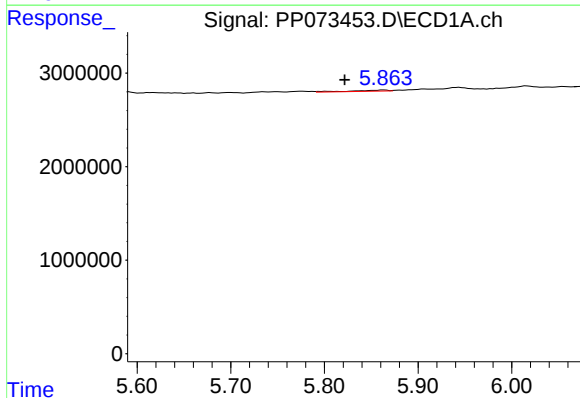


#14 AR-1232-4

R.T.: 5.864 min
Delta R.T.: 0.042 min
Response: 305631
Conc: 14.18 ng/ml

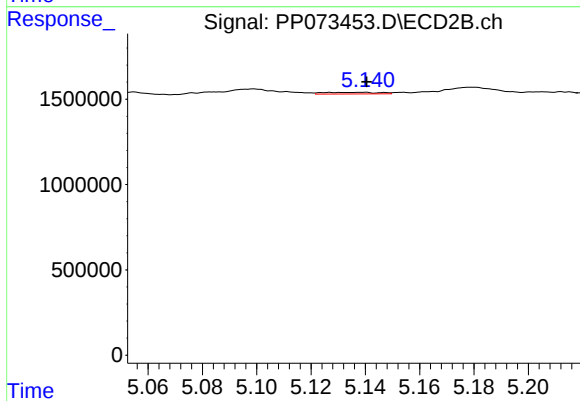

#14 AR-1232-4


R.T.: 5.139 min
Delta R.T.: -0.001 min
Response: 129740
Conc: 6.06 ng/ml

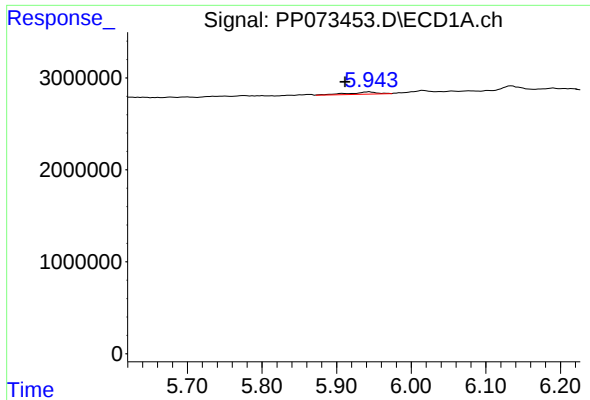

#15 AR-1232-5


R.T.: 5.944 min
Delta R.T.: 0.032 min
Response: 661552
Conc: 47.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

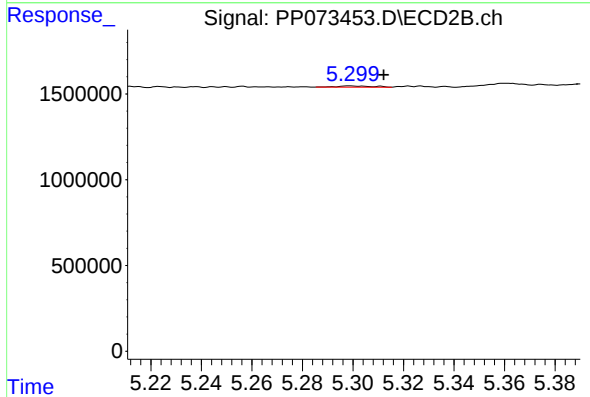


#15 AR-1232-5

R.T.: 5.299 min
Delta R.T.: -0.014 min
Response: 70434
Conc: 3.01 ng/ml

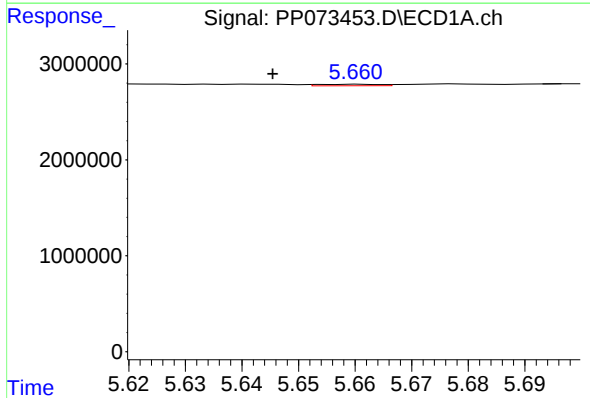


#16 AR-1242-1

R.T.: 5.660 min
Delta R.T.: 0.015 min
Response: 118794
Conc: 2.34 ng/ml

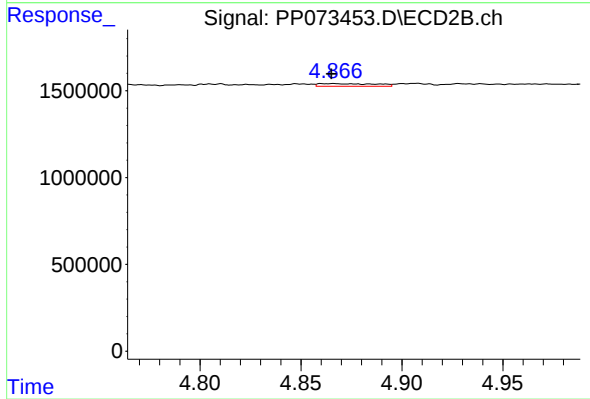

#16 AR-1242-1


R.T.: 4.866 min
Delta R.T.: 0.001 min
Response: 306503
Conc: 5.25 ng/ml

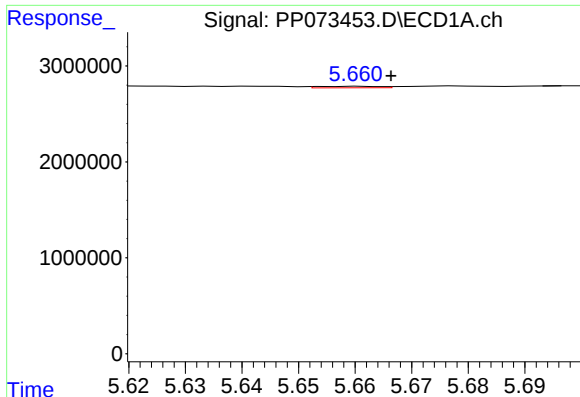

#17 AR-1242-2


R.T.: 5.660 min
Delta R.T.: -0.006 min
Response: 118794
Conc: 1.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

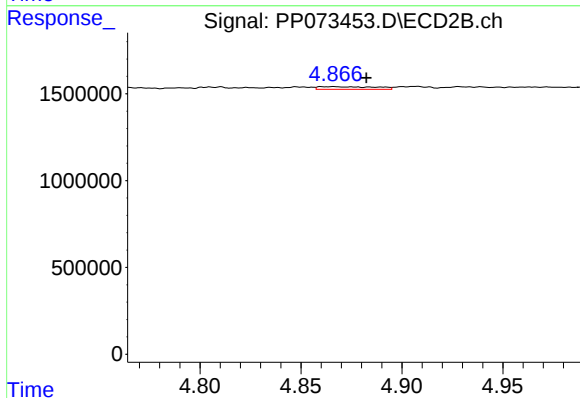


#17 AR-1242-2

R.T.: 4.866 min
Delta R.T.: -0.016 min
Response: 306503
Conc: 3.55 ng/ml

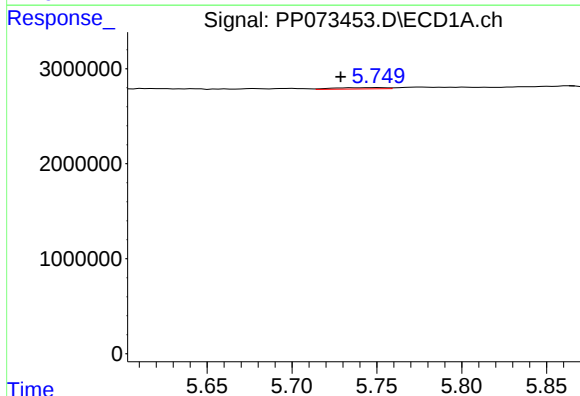


#18 AR-1242-3

R.T.: 5.750 min
Delta R.T.: 0.021 min
Response: 303138
Conc: 6.31 ng/ml

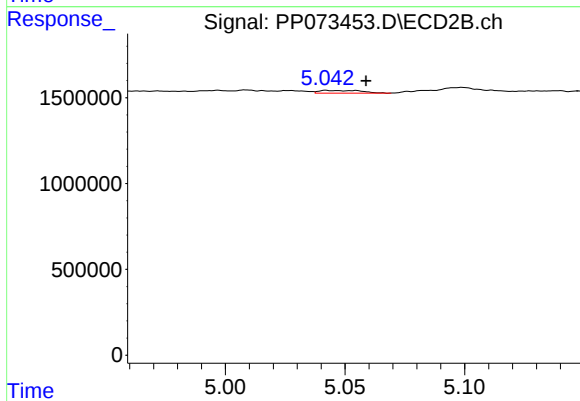

#18 AR-1242-3


R.T.: 5.042 min
Delta R.T.: -0.016 min
Response: 196314
Conc: 4.28 ng/ml

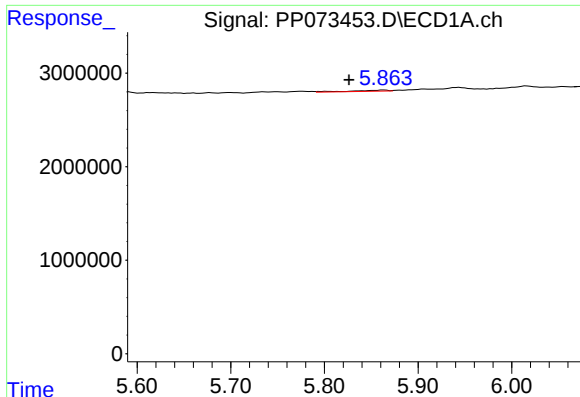

#19 AR-1242-4


R.T.: 5.864 min
Delta R.T.: 0.037 min
Response: 305631
Conc: 7.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

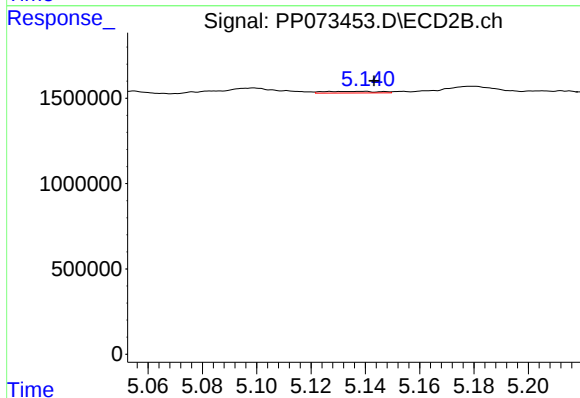


#19 AR-1242-4

R.T.: 5.139 min
Delta R.T.: -0.004 min
Response: 129740
Conc: 2.95 ng/ml

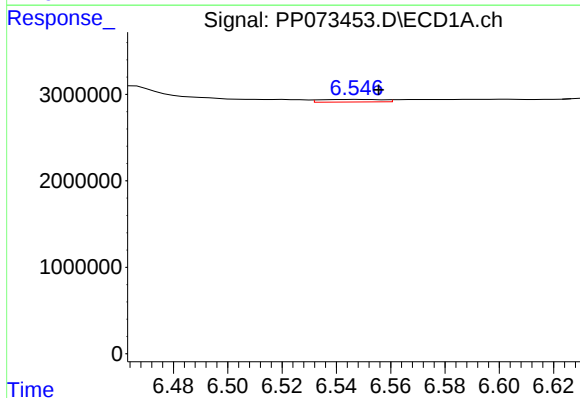


#20 AR-1242-5

R.T.: 6.548 min
Delta R.T.: -0.008 min
Response: 482633
Conc: 11.36 ng/ml

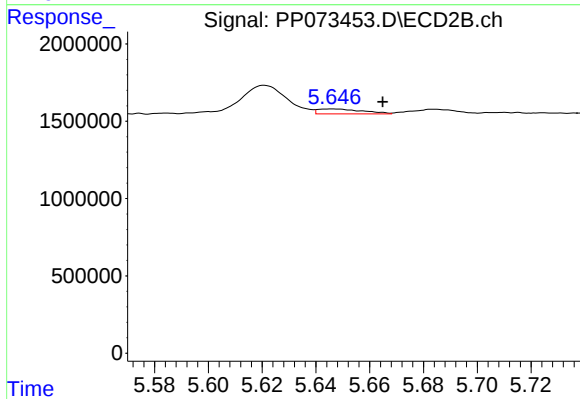

#20 AR-1242-5


R.T.: 5.646 min
Delta R.T.: -0.019 min
Response: 366056
Conc: 6.69 ng/ml

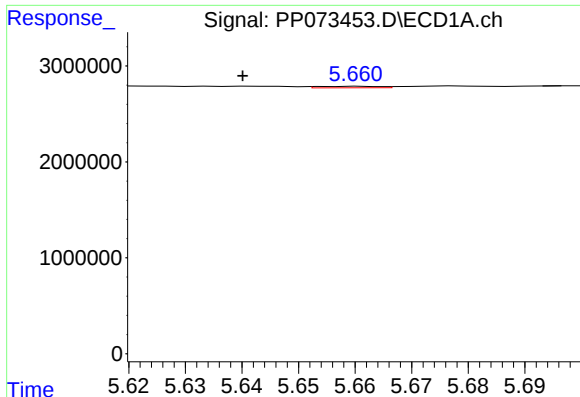

#21 AR-1248-1


R.T.: 5.660 min
Delta R.T.: 0.020 min
Response: 118794
Conc: 3.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

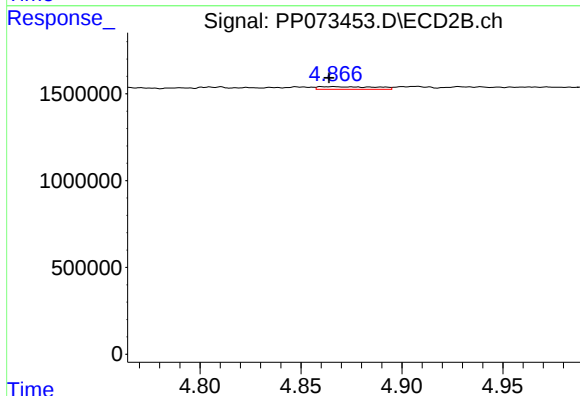


#21 AR-1248-1

R.T.: 4.866 min
Delta R.T.: 0.003 min
Response: 306503
Conc: 6.97 ng/ml

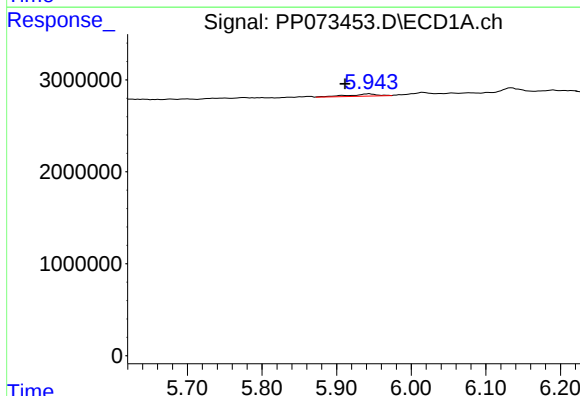


#22 AR-1248-2

R.T.: 5.944 min
Delta R.T.: 0.032 min
Response: 661552
Conc: 12.82 ng/ml

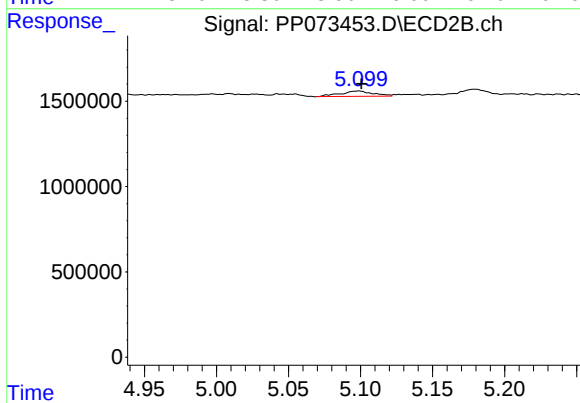

#22 AR-1248-2


R.T.: 5.099 min
Delta R.T.: -0.002 min
Response: 493848
Conc: 8.38 ng/ml

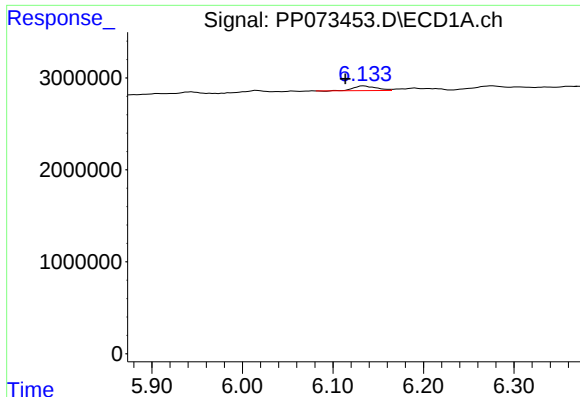

#23 AR-1248-3


R.T.: 6.134 min
Delta R.T.: 0.020 min
Response: 859453
Conc: 15.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

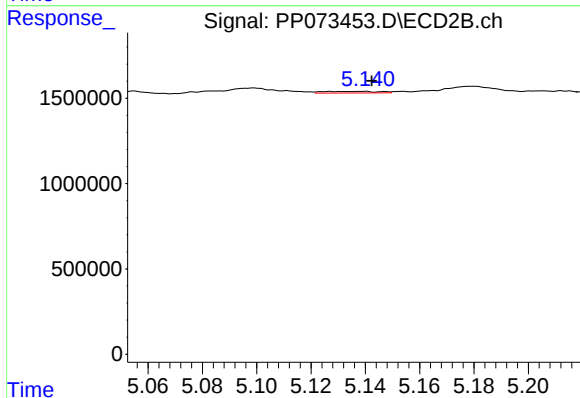


#23 AR-1248-3

R.T.: 5.139 min
Delta R.T.: -0.003 min
Response: 129740
Conc: 2.15 ng/ml

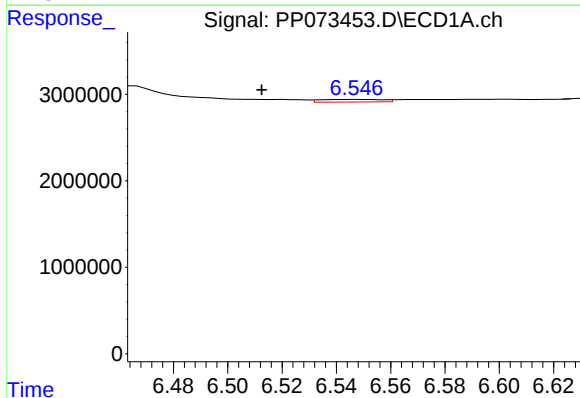


#24 AR-1248-4

R.T.: 6.548 min
Delta R.T.: 0.035 min
Response: 482633
Conc: 6.86 ng/ml

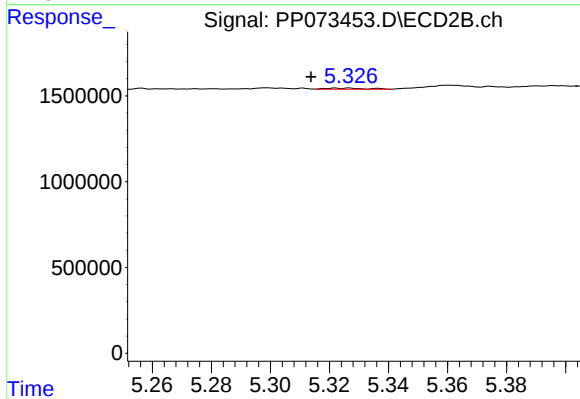

#24 AR-1248-4


R.T.: 5.327 min
Delta R.T.: 0.013 min
Response: 55319
Conc: 0.78 ng/ml

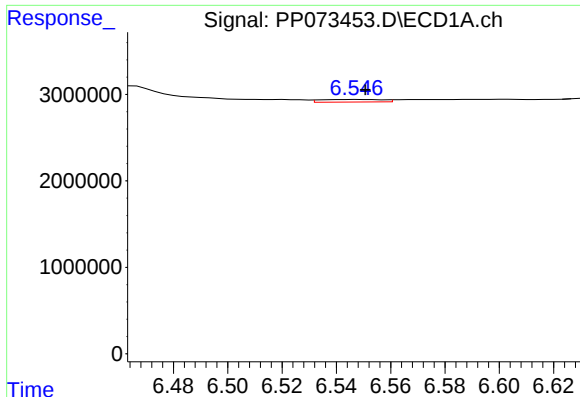

#25 AR-1248-5


R.T.: 6.548 min
Delta R.T.: -0.003 min
Response: 482633
Conc: 6.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

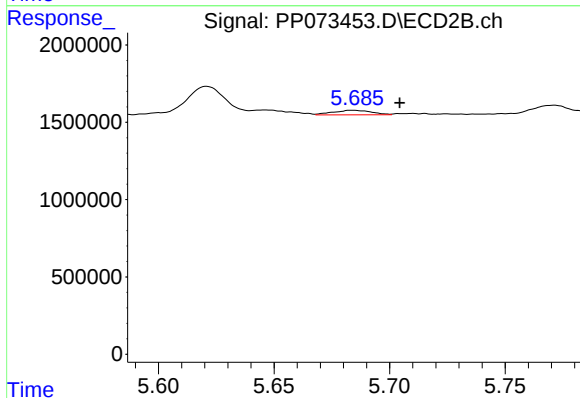


#25 AR-1248-5

R.T.: 5.684 min
Delta R.T.: -0.020 min
Response: 332682
Conc: 4.52 ng/ml

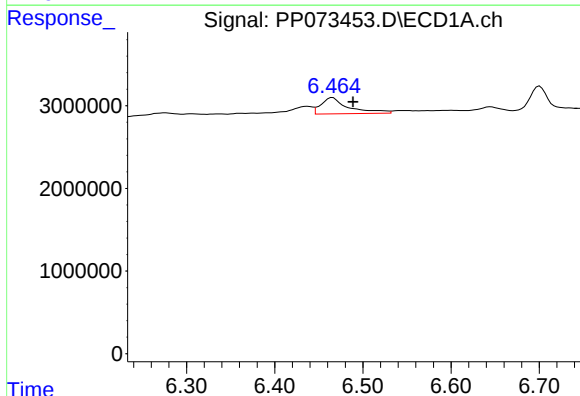


#26 AR-1254-1

R.T.: 6.466 min
Delta R.T.: -0.023 min
Response: 4300744
Conc: 60.63 ng/ml

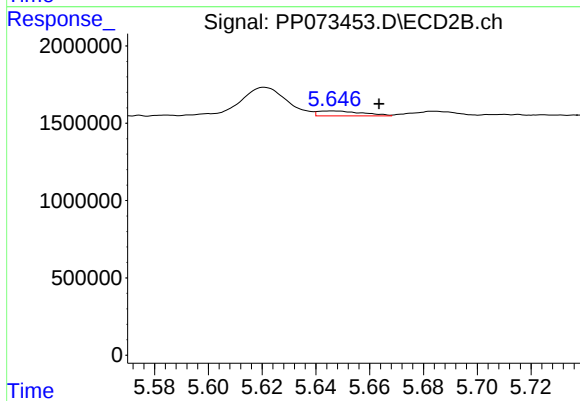

#26 AR-1254-1


R.T.: 5.646 min
Delta R.T.: -0.017 min
Response: 366056
Conc: 3.34 ng/ml

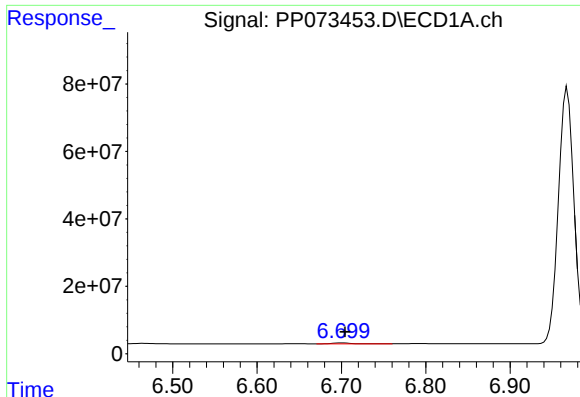

#27 AR-1254-2


R.T.: 6.701 min
Delta R.T.: -0.004 min
Response: 4964740
Conc: 48.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

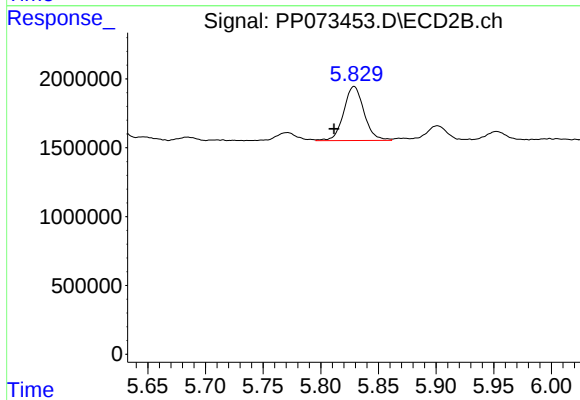


#27 AR-1254-2

R.T.: 5.829 min
Delta R.T.: 0.017 min
Response: 4802786
Conc: 49.52 ng/ml

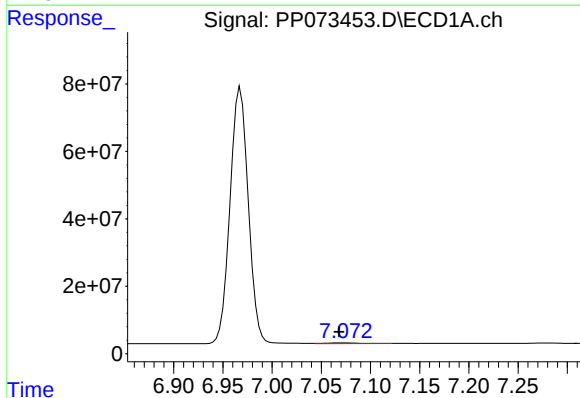


#28 AR-1254-3

R.T.: 7.073 min
Delta R.T.: 0.005 min
Response: 5765216
Conc: 50.72 ng/ml

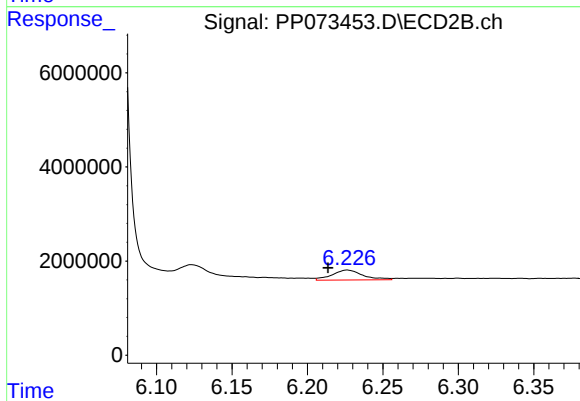

#28 AR-1254-3


R.T.: 6.226 min
Delta R.T.: 0.013 min
Response: 2975980
Conc: 20.20 ng/ml

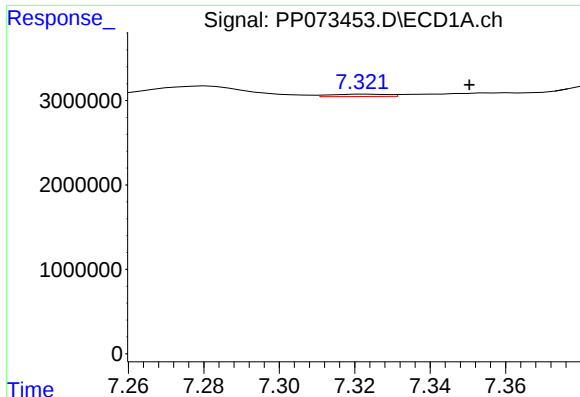

#29 AR-1254-4


R.T.: 7.323 min
Delta R.T.: -0.027 min
Response: 291749
Conc: 2.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

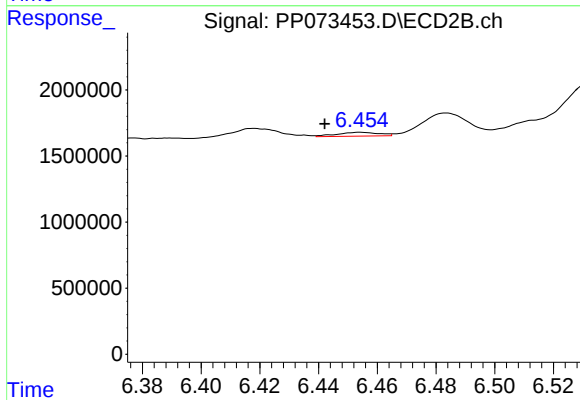


#29 AR-1254-4

R.T.: 6.454 min
Delta R.T.: 0.012 min
Response: 290037
Conc: 3.21 ng/ml

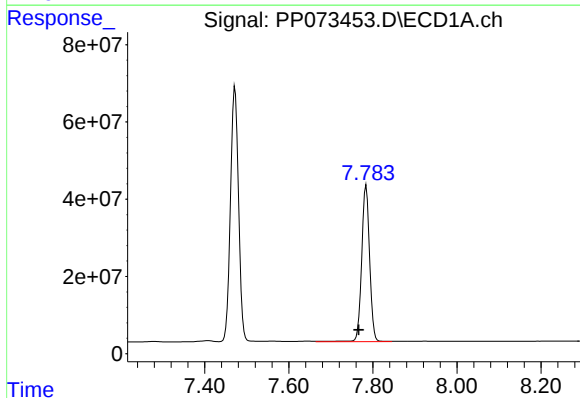


#30 AR-1254-5

R.T.: 7.784 min
Delta R.T.: 0.018 min
Response: 530354425
Conc: 5596.02 ng/ml

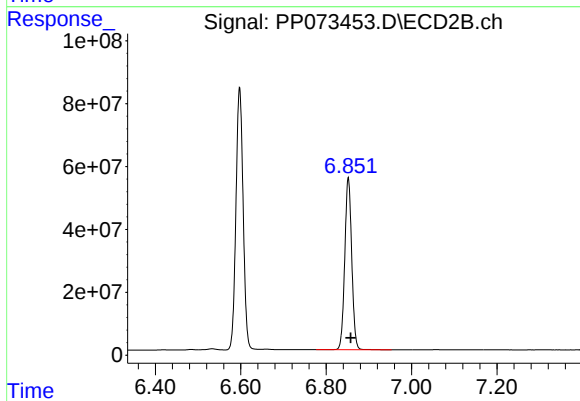

#30 AR-1254-5


R.T.: 6.852 min
Delta R.T.: -0.006 min
Response: 618800820
Conc: 4650.00 ng/ml

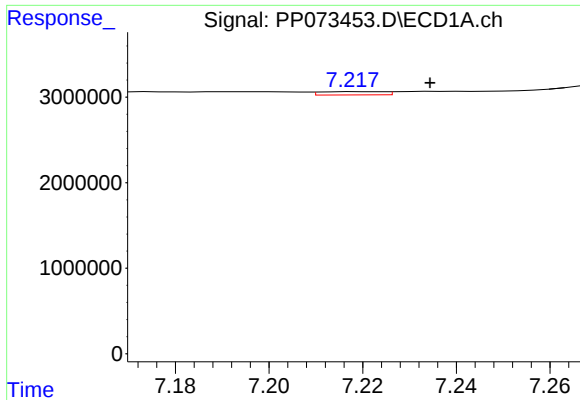

#31 AR-1260-1


R.T.: 7.220 min
Delta R.T.: -0.015 min
Response: 364242
Conc: 5.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

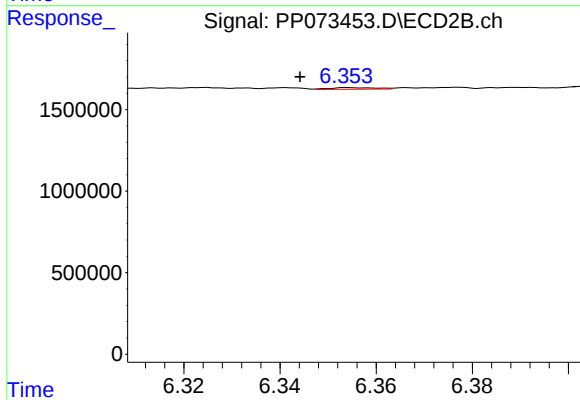


#31 AR-1260-1

R.T.: 6.354 min
Delta R.T.: 0.010 min
Response: 64355
Conc: 0.70 ng/ml

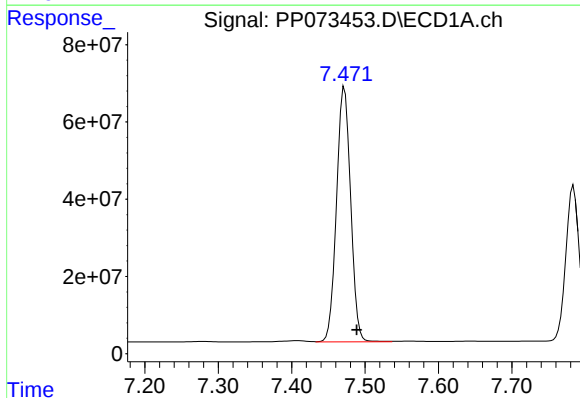


#32 AR-1260-2

R.T.: 7.472 min
Delta R.T.: -0.017 min
Response: 884292649
Conc: 8412.91 ng/ml

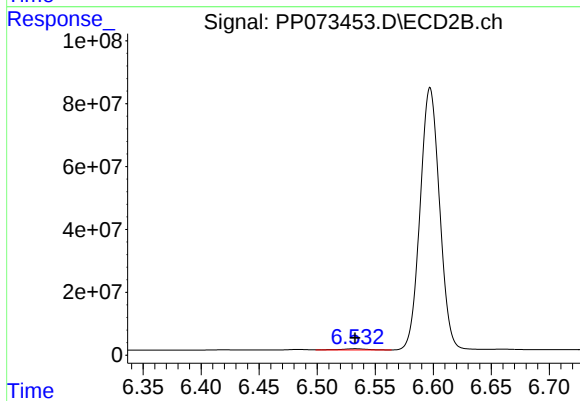

#32 AR-1260-2


R.T.: 6.533 min
Delta R.T.: 0.000 min
Response: 5725893
Conc: 46.33 ng/ml

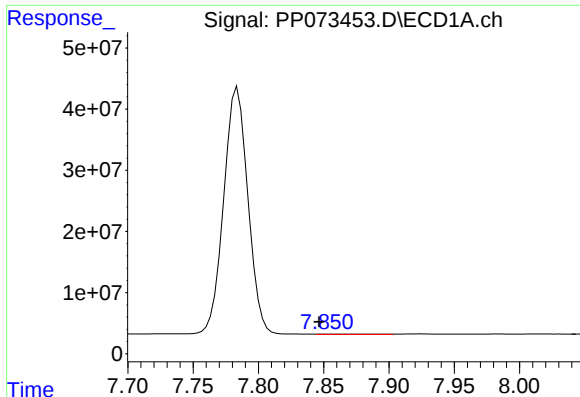

#33 AR-1260-3


R.T.: 7.853 min
Delta R.T.: 0.006 min
Response: 1696924
Conc: 18.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

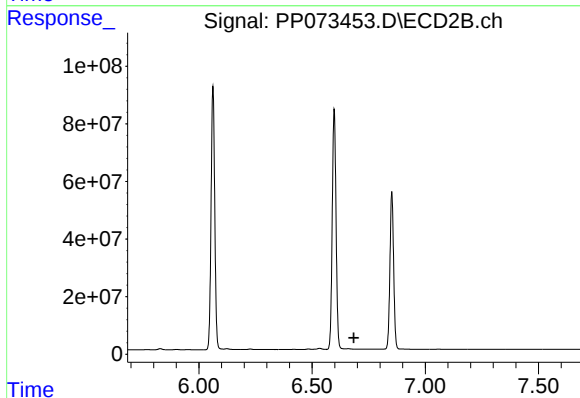


#33 AR-1260-3

R.T.: 6.659 min
Delta R.T.: -0.025 min
Response: -13076
Conc: N.D.

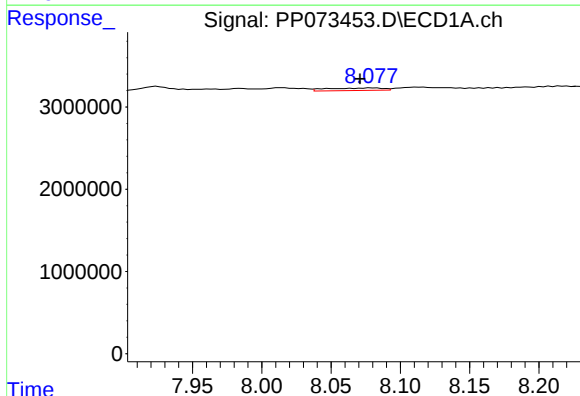


#34 AR-1260-4

R.T.: 8.080 min
Delta R.T.: 0.009 min
Response: 845874
Conc: 9.57 ng/ml

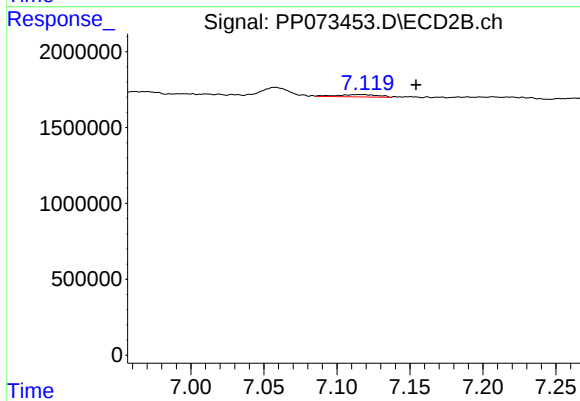

#34 AR-1260-4


R.T.: 7.115 min
Delta R.T.: -0.039 min
Response: 295153
Conc: 3.40 ng/ml

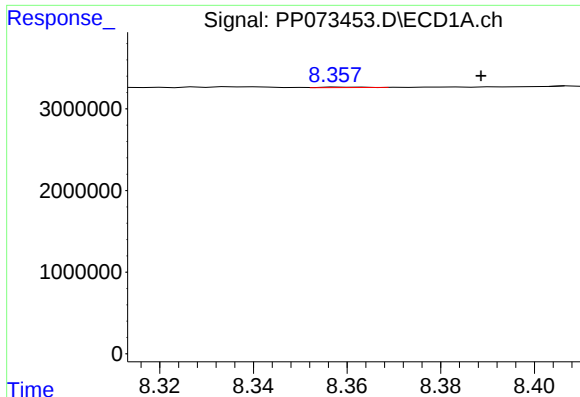

#35 AR-1260-5


R.T.: 8.360 min
Delta R.T.: -0.029 min
Response: 38646
Conc: 0.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

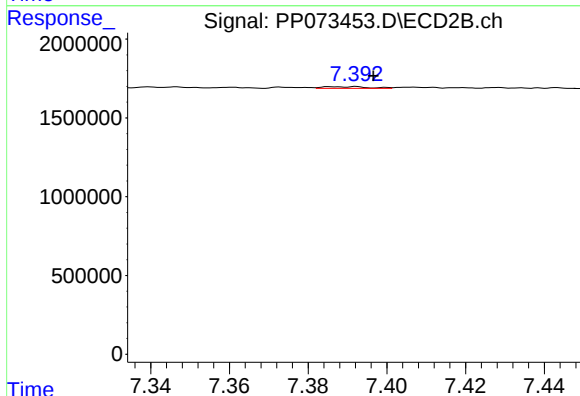


#35 AR-1260-5

R.T.: 7.392 min
Delta R.T.: -0.005 min
Response: 84317
Conc: 0.39 ng/ml

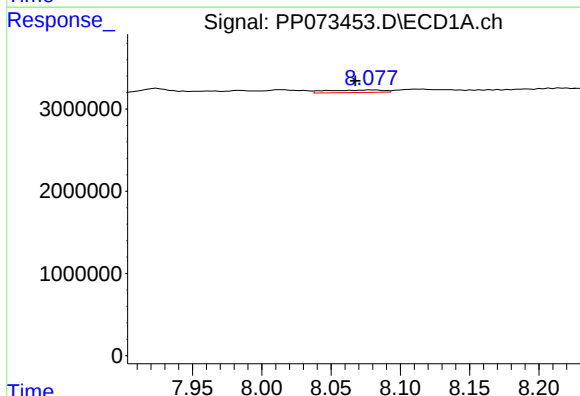


#36 AR-1262-1

R.T.: 8.080 min
Delta R.T.: 0.012 min
Response: 845874
Conc: 7.34 ng/ml

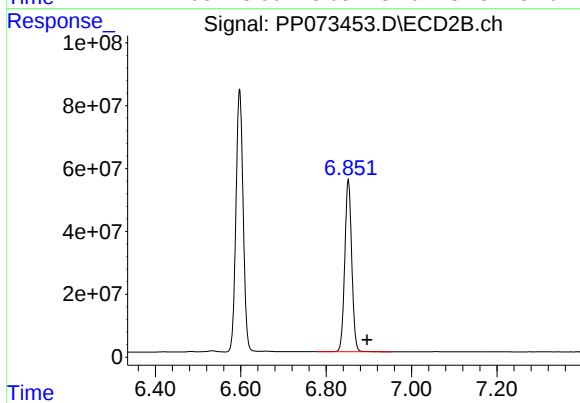

#36 AR-1262-1


R.T.: 6.852 min
Delta R.T.: -0.044 min
Response: 618800820
Conc: 4123.89 ng/ml

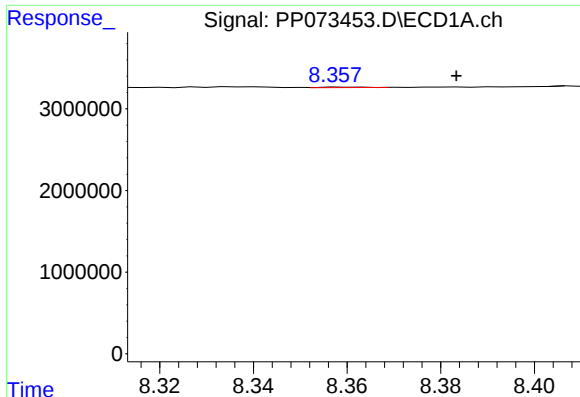

#37 AR-1262-2


R.T.: 8.360 min
Delta R.T.: -0.024 min
Response: 38646
Conc: 0.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

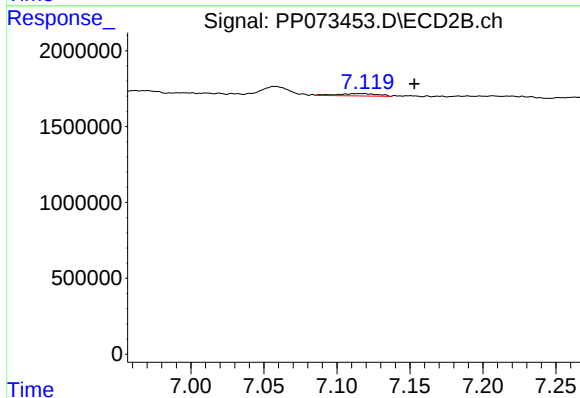


#37 AR-1262-2

R.T.: 7.115 min
Delta R.T.: -0.038 min
Response: 295153
Conc: 2.36 ng/ml

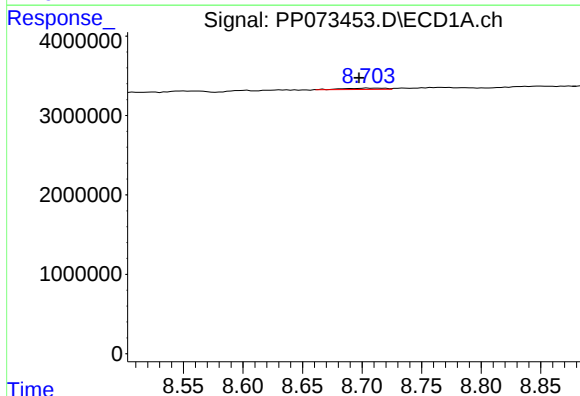


#38 AR-1262-3

R.T.: 8.705 min
Delta R.T.: 0.007 min
Response: 396448
Conc: 2.43 ng/ml

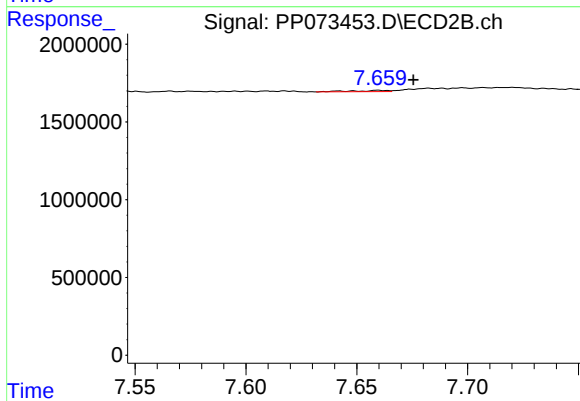

#38 AR-1262-3


R.T.: 7.659 min
Delta R.T.: -0.016 min
Response: 92496
Conc: 0.83 ng/ml

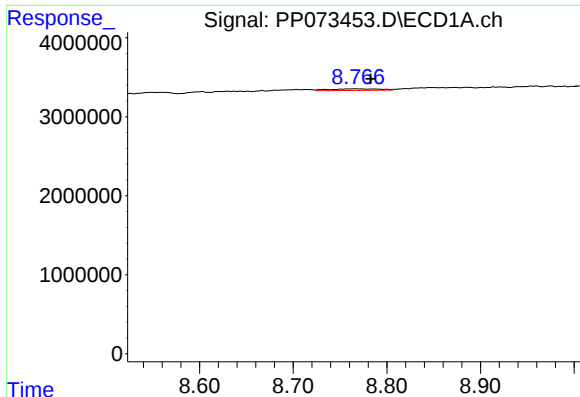

#39 AR-1262-4


R.T.: 8.767 min
Delta R.T.: -0.016 min
Response: 742671
Conc: 6.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

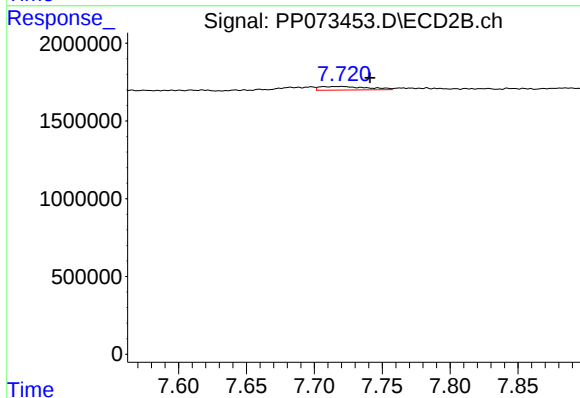


#39 AR-1262-4

R.T.: 7.720 min
Delta R.T.: -0.021 min
Response: 541605
Conc: 2.97 ng/ml

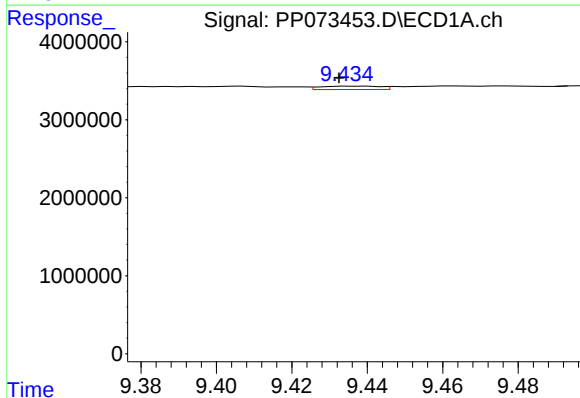


#40 AR-1262-5

R.T.: 9.437 min
Delta R.T.: 0.005 min
Response: 477625
Conc: 5.49 ng/ml

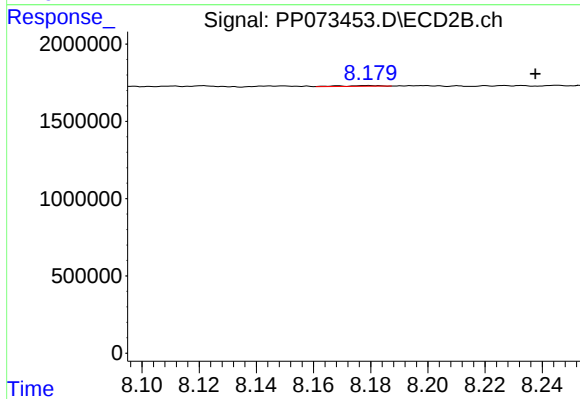

#40 AR-1262-5


R.T.: 8.179 min
Delta R.T.: -0.058 min
Response: 40642
Conc: 0.47 ng/ml

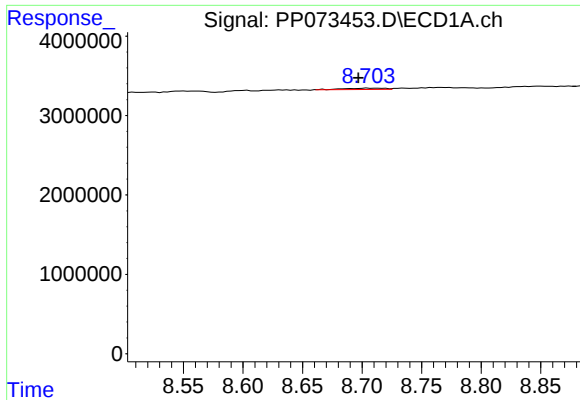

#41 AR-1268-1


R.T.: 8.705 min
Delta R.T.: 0.008 min
Response: 396448
Conc: 1.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

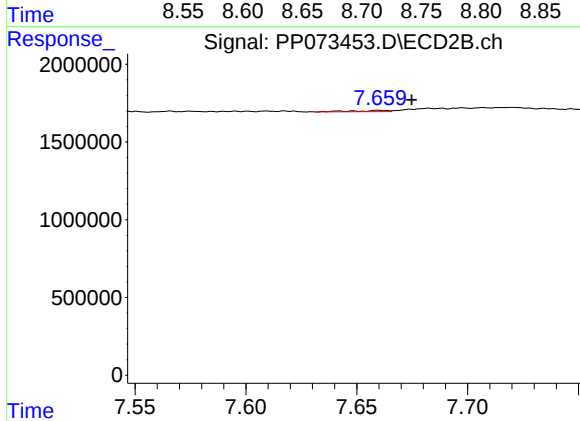


#41 AR-1268-1

R.T.: 7.659 min
Delta R.T.: -0.015 min
Response: 92496
Conc: 0.31 ng/ml

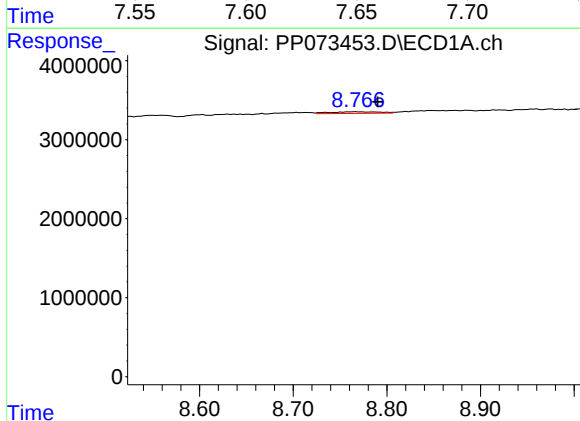


#42 AR-1268-2

R.T.: 8.767 min
Delta R.T.: -0.023 min
Response: 742671
Conc: 2.98 ng/ml

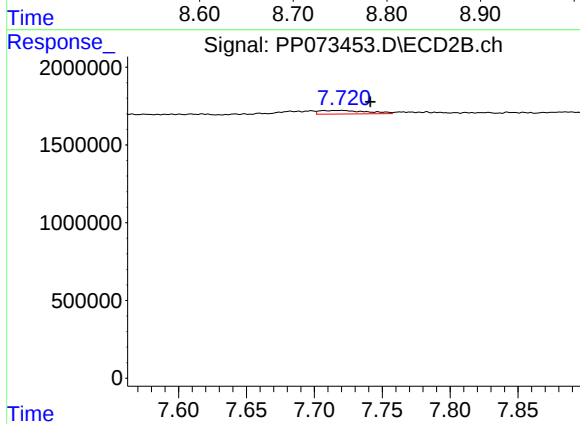

#42 AR-1268-2


R.T.: 7.720 min
Delta R.T.: -0.021 min
Response: 541605
Conc: 2.07 ng/ml

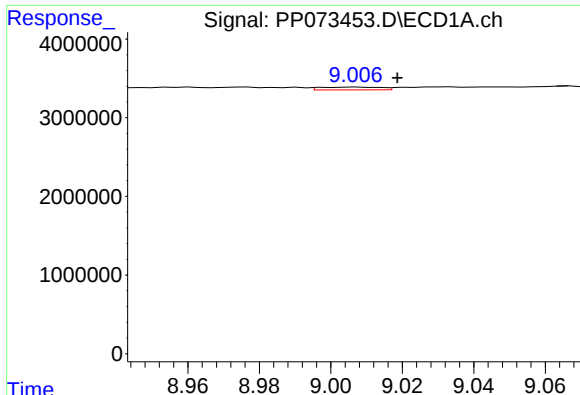

#43 AR-1268-3


R.T.: 9.007 min
Delta R.T.: -0.011 min
Response: 432239
Conc: 1.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

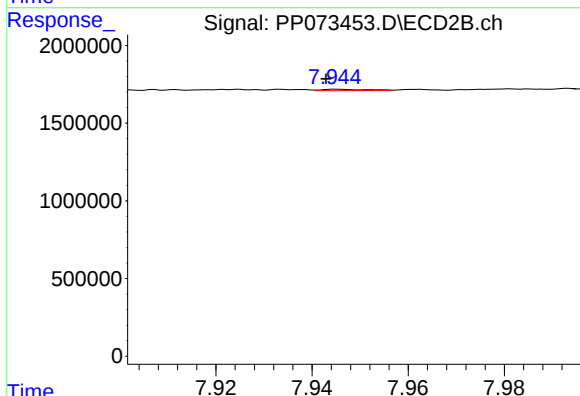


#43 AR-1268-3

R.T.: 7.945 min
Delta R.T.: 0.002 min
Response: 57925
Conc: 0.26 ng/ml

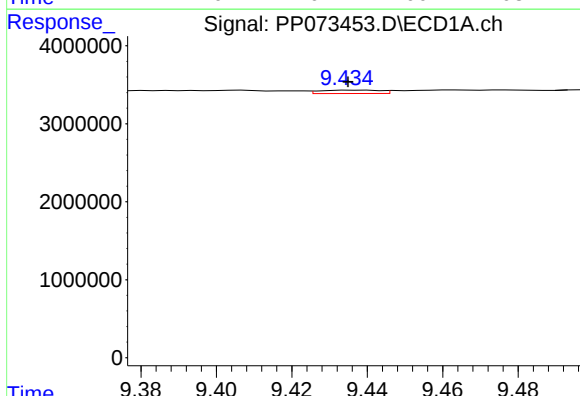


#44 AR-1268-4

R.T.: 9.437 min
Delta R.T.: 0.003 min
Response: 477625
Conc: 4.98 ng/ml

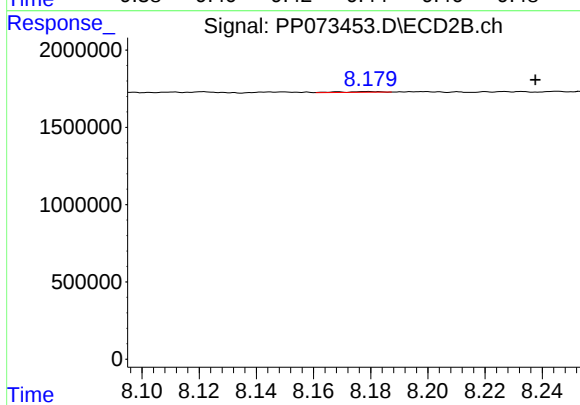

#44 AR-1268-4


R.T.: 8.179 min
Delta R.T.: -0.058 min
Response: 40642
Conc: 0.43 ng/ml

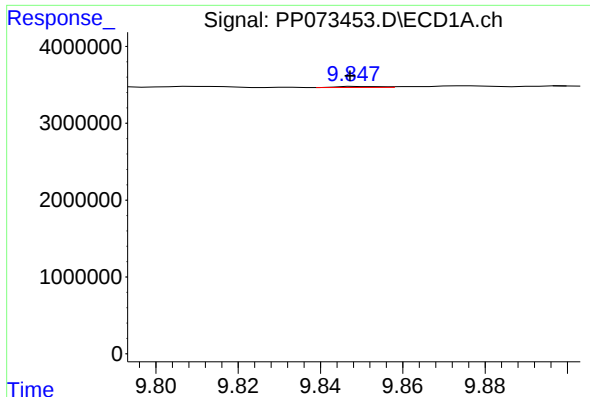

#45 AR-1268-5

R.T.: 9.850 min
Delta R.T.: 0.003 min
Response: 92040
Conc: 0.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

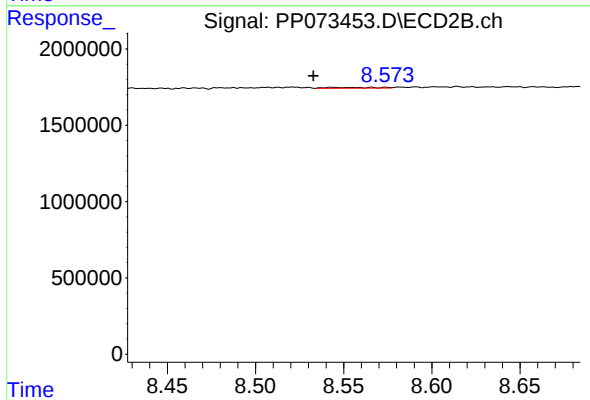

#45 AR-1268-5

R.T.: 8.543 min
Delta R.T.: 0.011 min
Response: 98602
Conc: 0.16 ng/ml