

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
 Data File : PP073469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 20:26
 Operator : YP\AJ
 Sample : Q2484-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-57

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2025
 Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:40:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.783	27577497	33472727	17.276m	18.873
2) SA Decachlor...	10.177	8.788	12422261	15821625	8.742	11.435 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
Data File : PP073469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 20:26
Operator : YP\AJ
Sample : Q2484-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-57


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:40:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

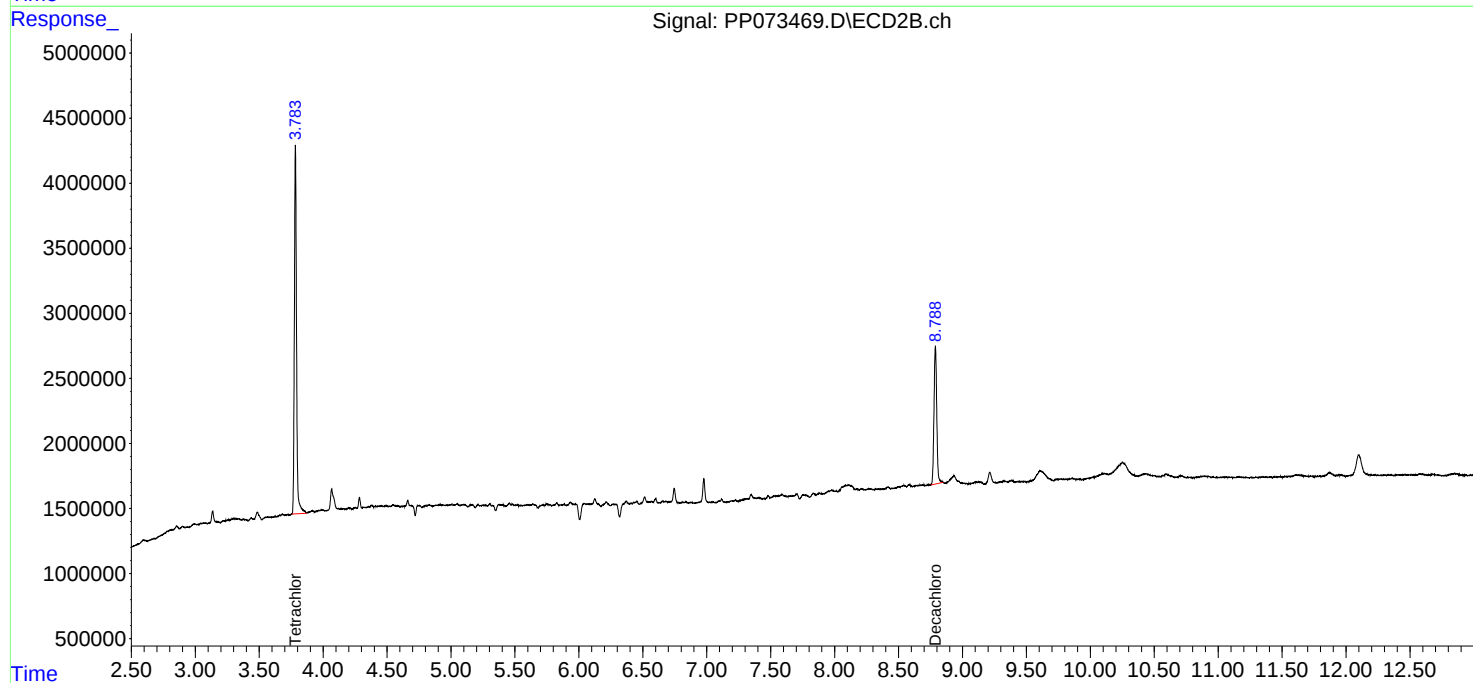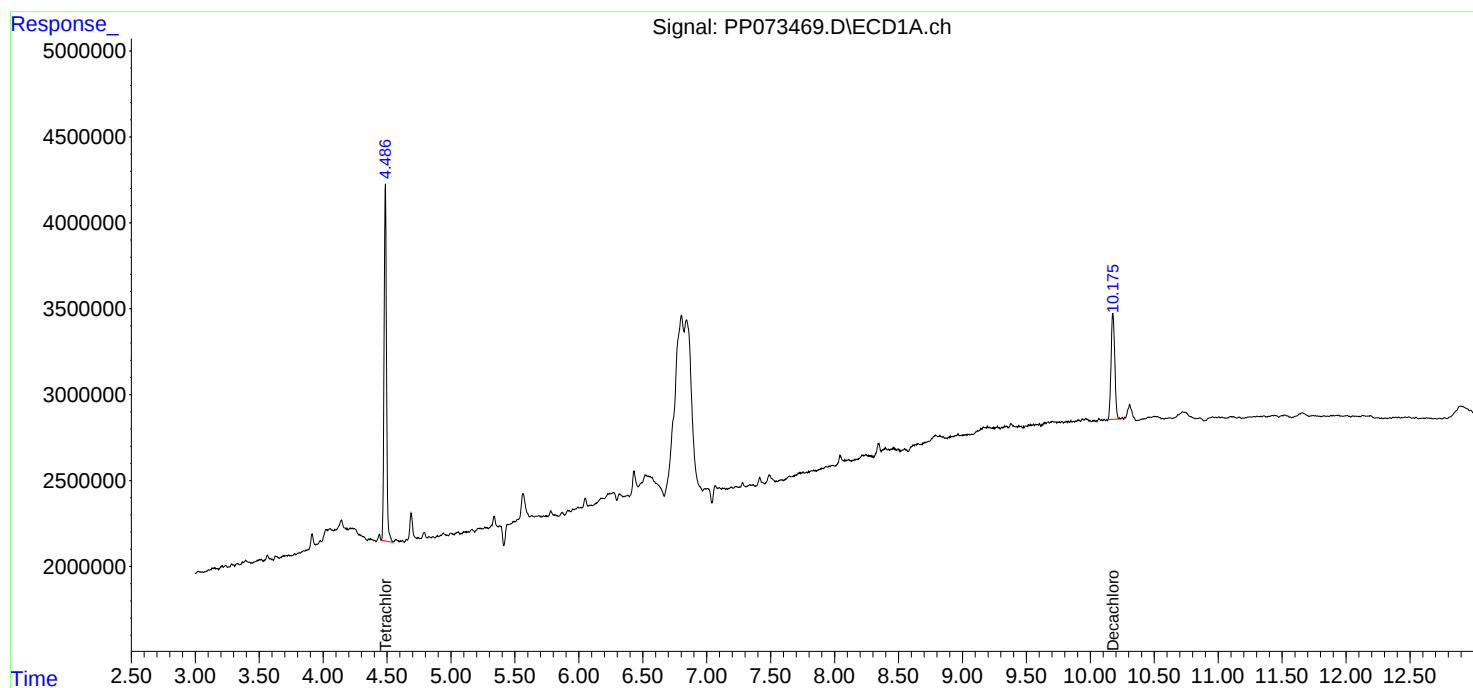

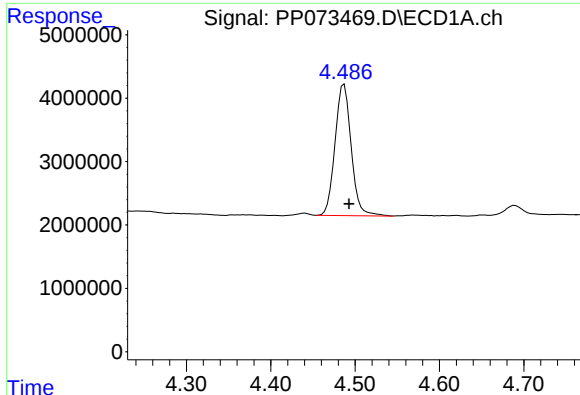

#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: -0.007 min
Response: 27577497
Conc: 17.28 ng/ml

Instrument :

ECD_P

ClientSampleId :


TP-57

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 07/03/2025

Supervised By :mohammad ahmed 07/04/2025

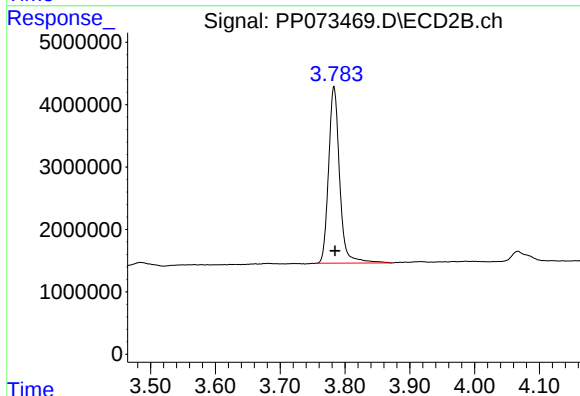


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.001 min
Response: 33472727
Conc: 18.87 ng/ml

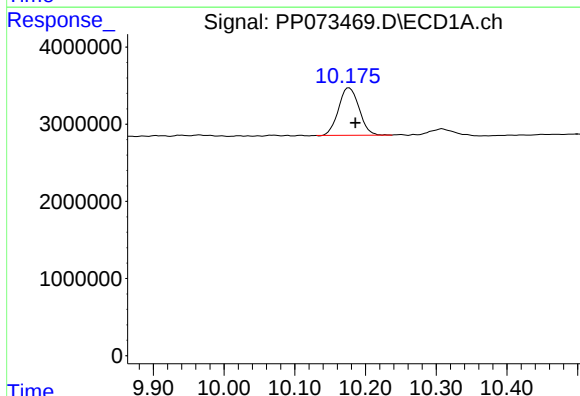

#2 Decachlorobiphenyl

R.T.: 10.177 min
Delta R.T.: -0.009 min
Response: 12422261
Conc: 8.74 ng/ml

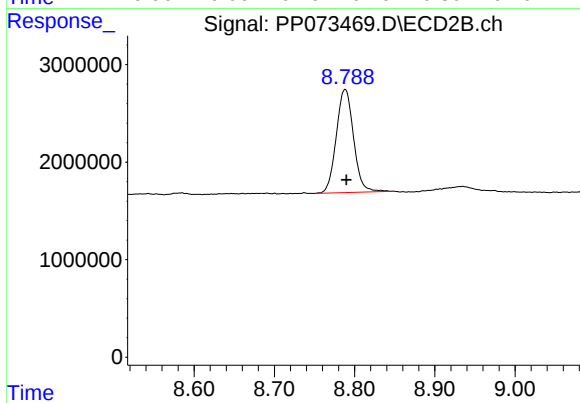

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 15821625
Conc: 11.43 ng/ml