

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
 Data File : PP073475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 22:04
 Operator : YP\AJ
 Sample : Q2477-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 50728

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2025
 Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:42:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.784	24701741	34914664	15.474m	19.686 #
2) SA Decachlor...	10.179	8.787	14749193	17662795	10.380	12.765

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
Data File : PP073475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 22:04
Operator : YP\AJ
Sample : Q2477-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
50728


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:42:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

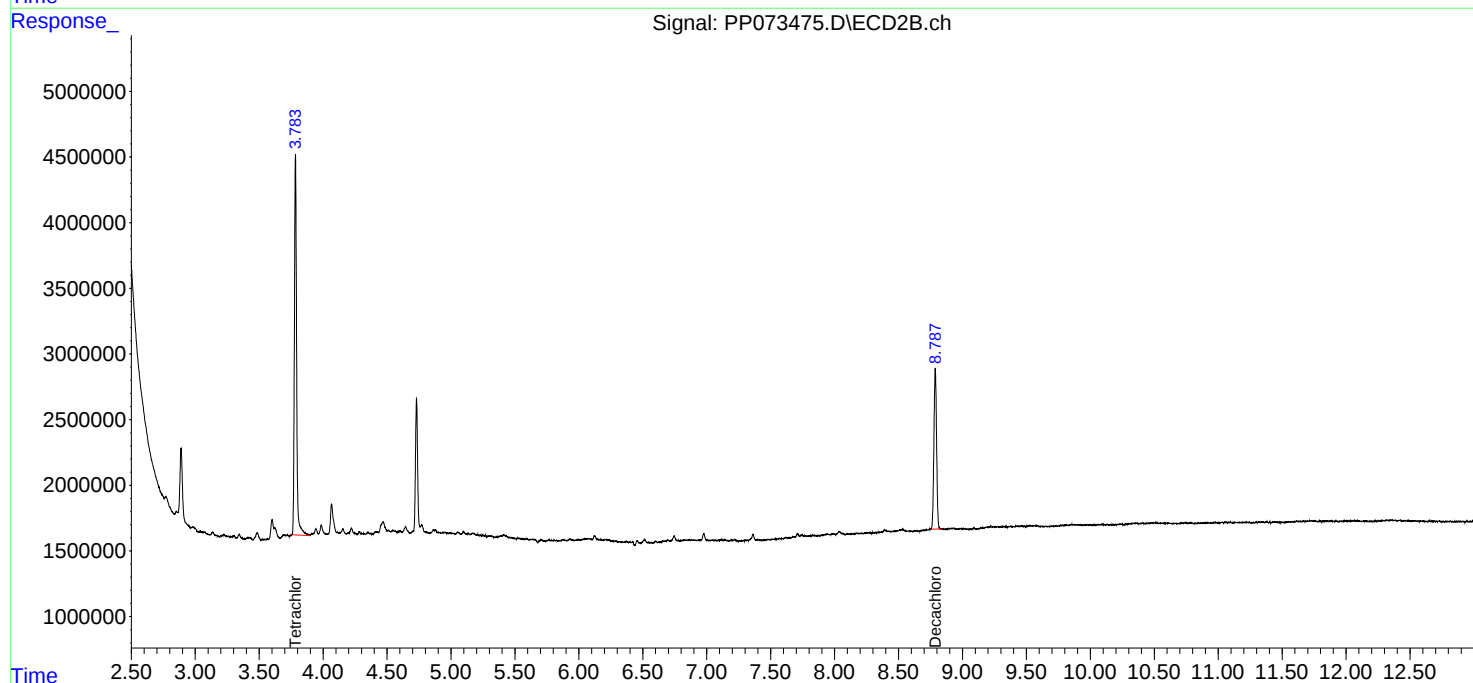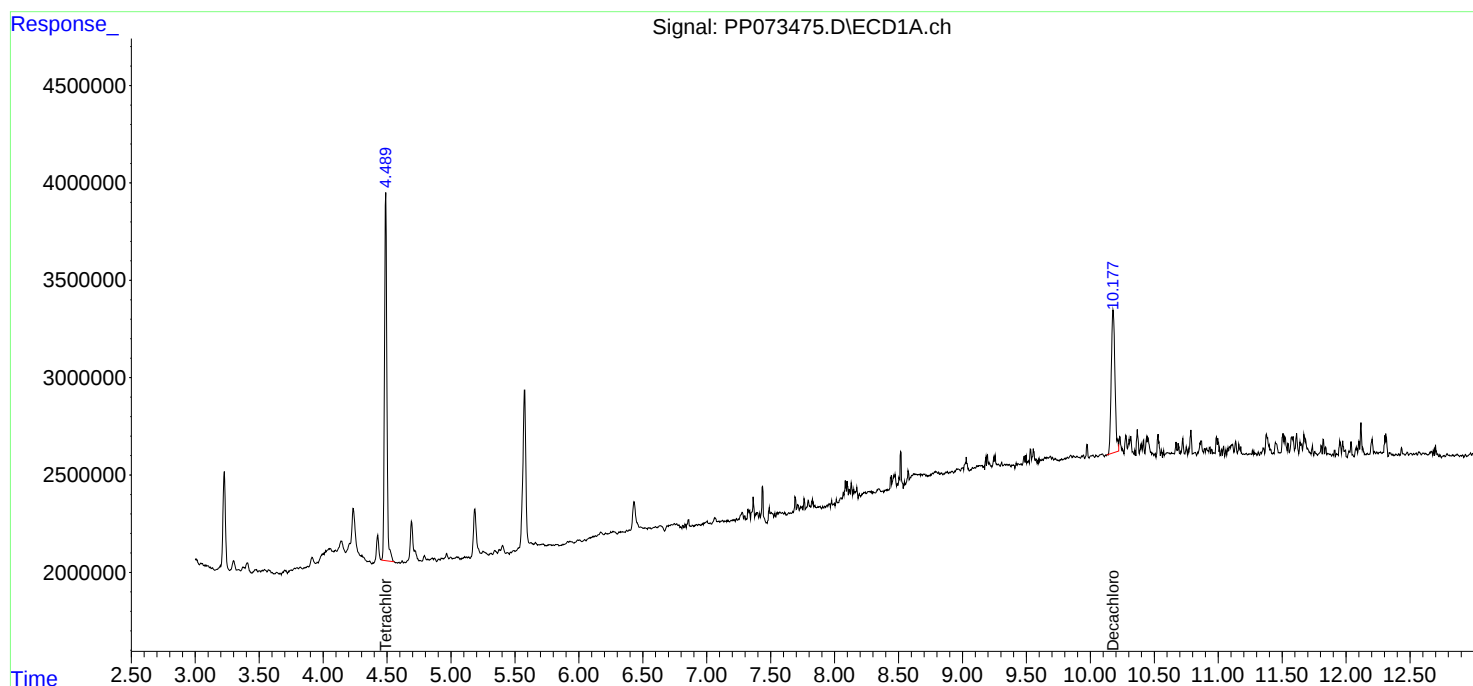

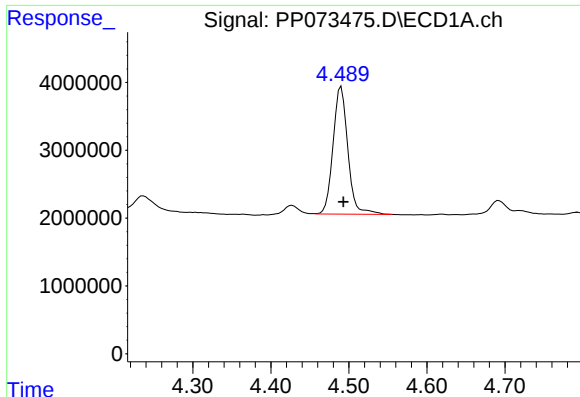


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.004 min
Response: 24701741
Conc: 15.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
50728


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

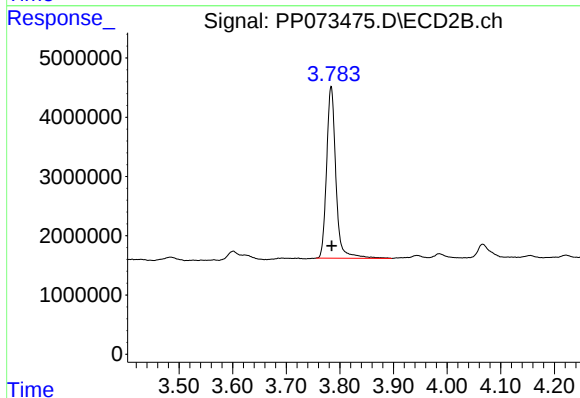


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: 0.000 min
Response: 34914664
Conc: 19.69 ng/ml

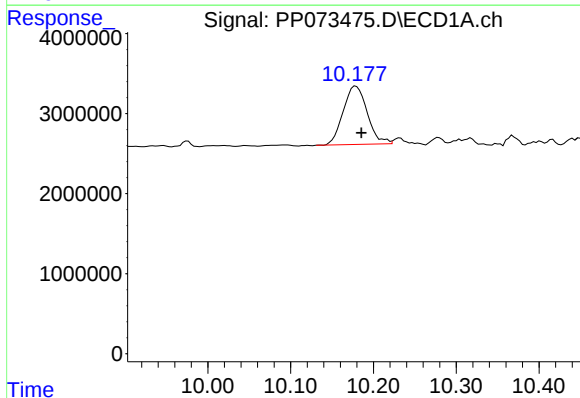

#2 Decachlorobiphenyl

R.T.: 10.179 min
Delta R.T.: -0.007 min
Response: 14749193
Conc: 10.38 ng/ml

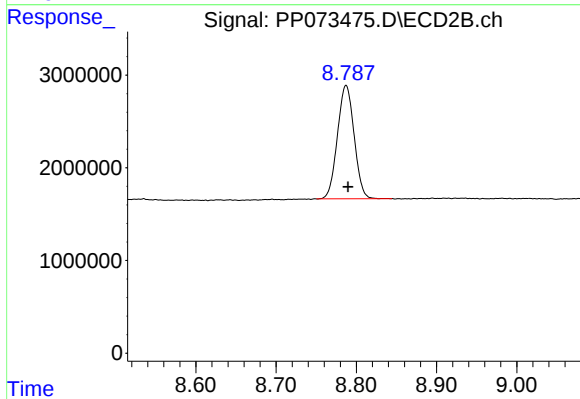

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.003 min
Response: 17662795
Conc: 12.77 ng/ml