

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070425\
 Data File : PP073525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jul 2025 12:15
 Operator : YP\AJ
 Sample : Q2487-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 G1(6-12)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/07/2025
 Supervised By :mohammad ahmed 07/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 23:28:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.779	38253624	32516631	23.964m	18.334m
2) SA Decachlor...	10.174	8.780	16231582	20126860	11.423m	14.546 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070425\
Data File : PP073525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jul 2025 12:15
Operator : YP\AJ
Sample : Q2487-16
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
G1(6-12)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2025
Supervised By :mohammad ahmed 07/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 23:28:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

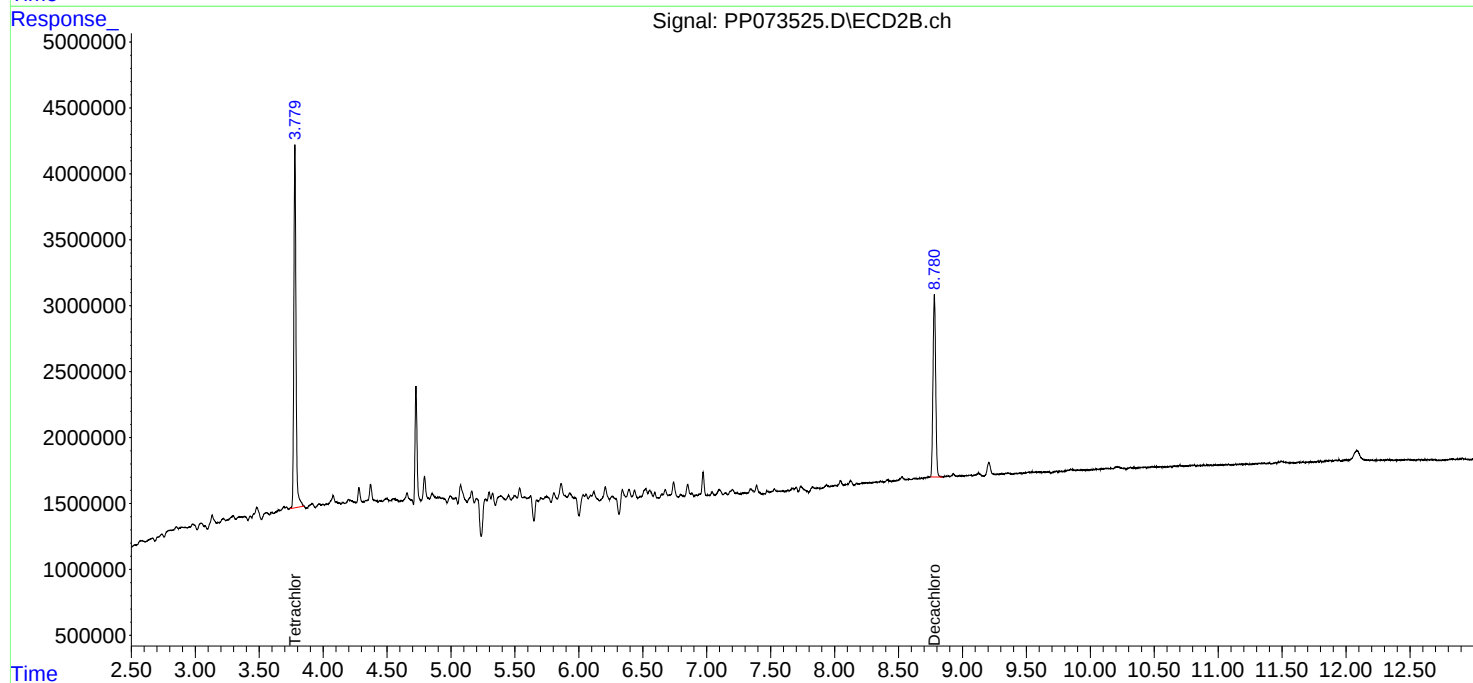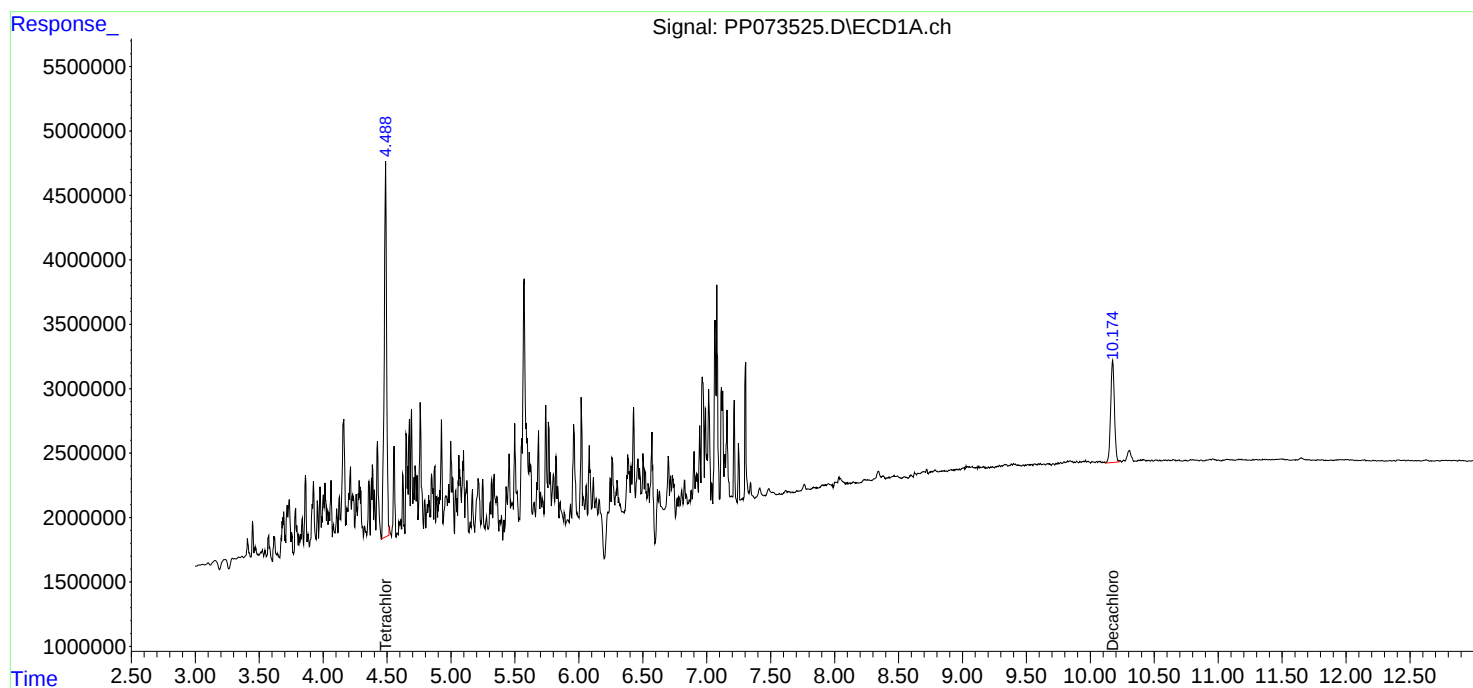

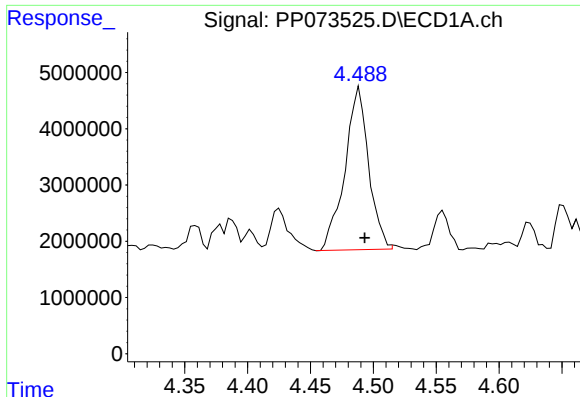


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: -0.005 min
Response: 38253624
Conc: 23.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
G1(6-12)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2025
Supervised By :mohammad ahmed 07/08/2025

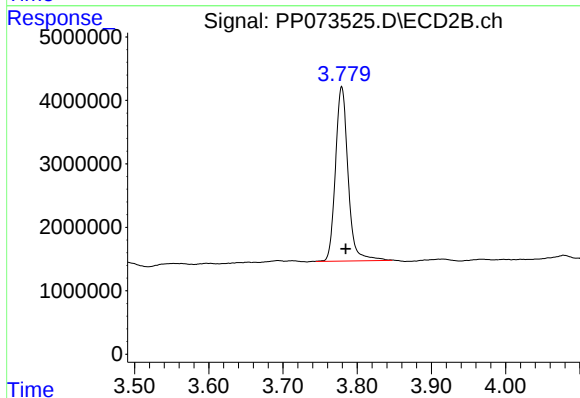


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.006 min
Response: 32516631
Conc: 18.33 ng/ml m

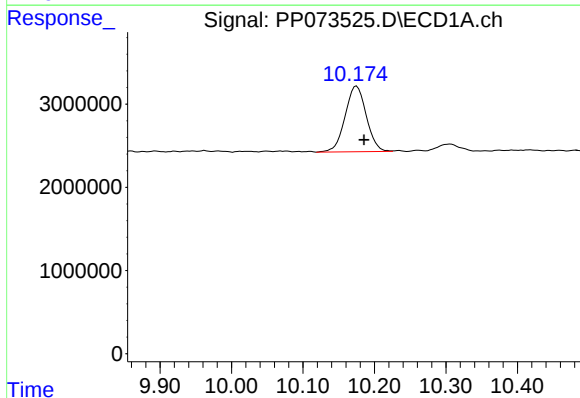

#2 Decachlorobiphenyl

R.T.: 10.174 min
Delta R.T.: -0.012 min
Response: 16231582
Conc: 11.42 ng/ml m

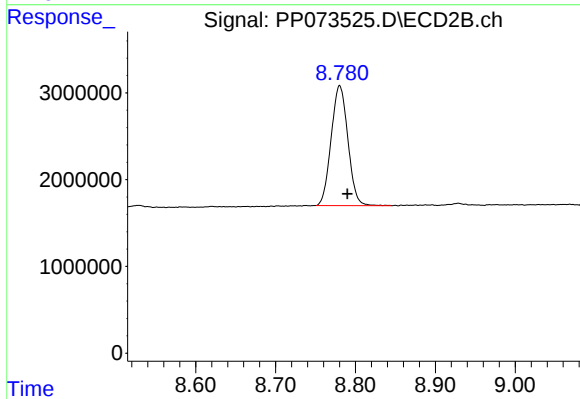

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.010 min
Response: 20126860
Conc: 14.55 ng/ml