

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070522\
 Data File : PP049199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 19:53
 Operator : YP\AJ
 Sample : N3576-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-072416-05

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/06/2022
 Supervised By :Ankita Jodhani 07/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 00:00:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.346	3.596	35404128	60975564	24.905	23.813
2) SA Decachlor...	10.100	8.569	46660311	24537744	38.040m	21.768 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070522\
Data File : PP049199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 19:53
Operator : YP\AJ
Sample : N3576-05
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-072416-05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/06/2022
Supervised By :Ankita Jodhani 07/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 00:00:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

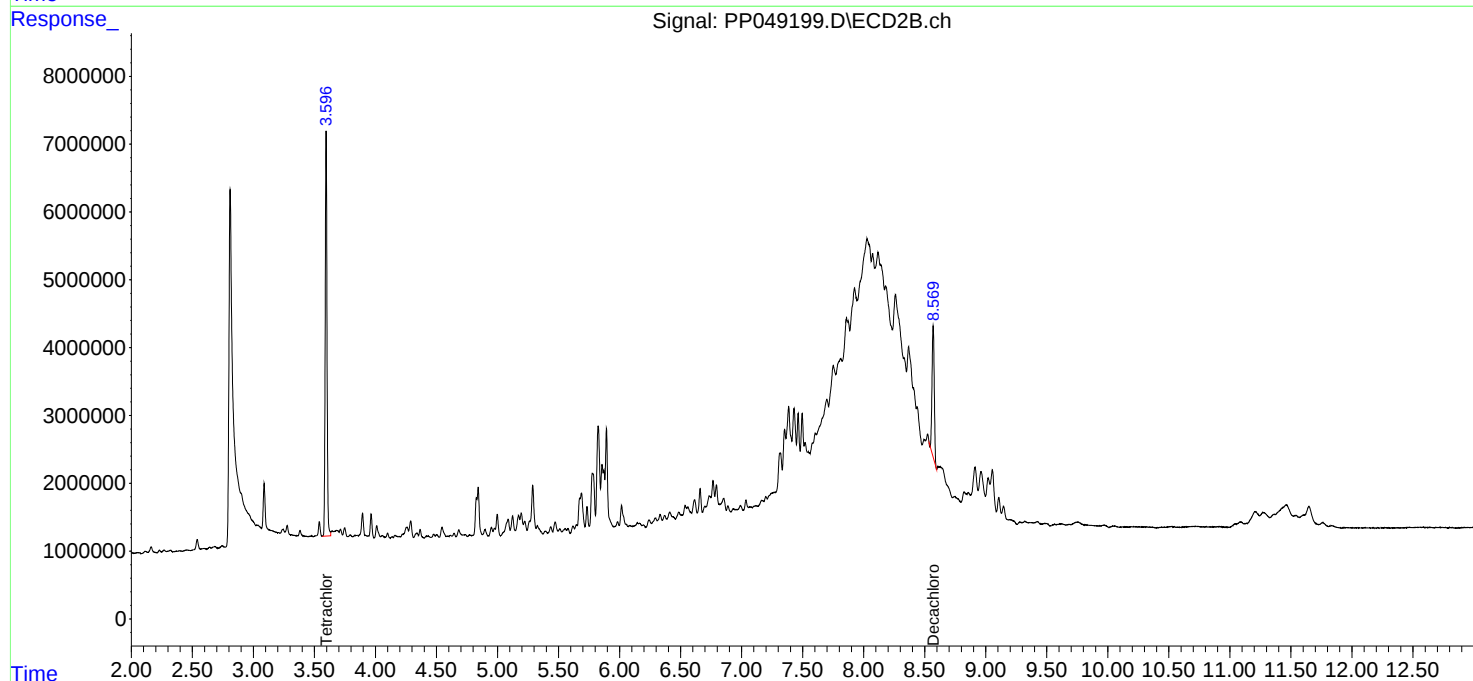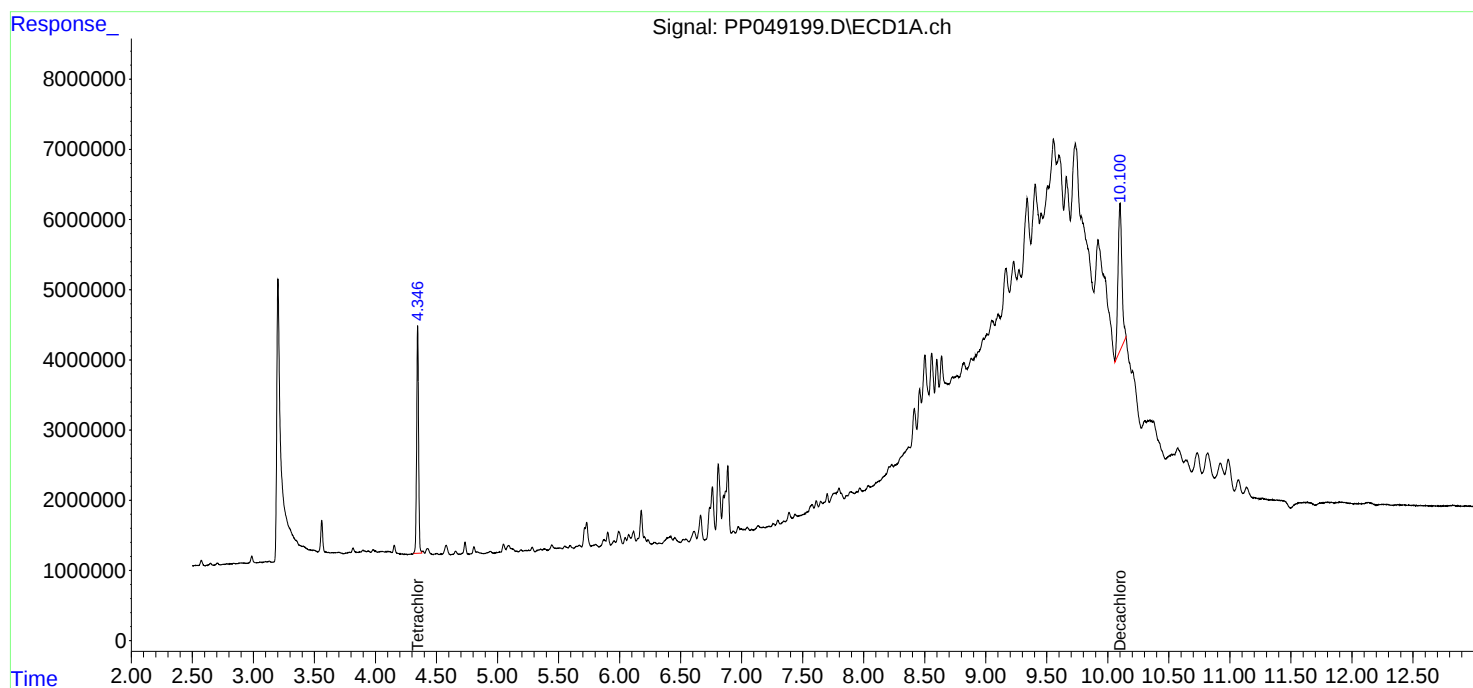

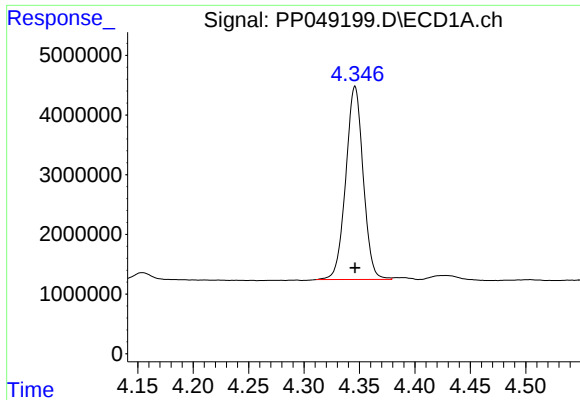


#1 Tetrachloro-m-xylene

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 35404128
Conc: 24.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-072416-05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/06/2022
Supervised By :Ankita Jodhani 07/06/2022

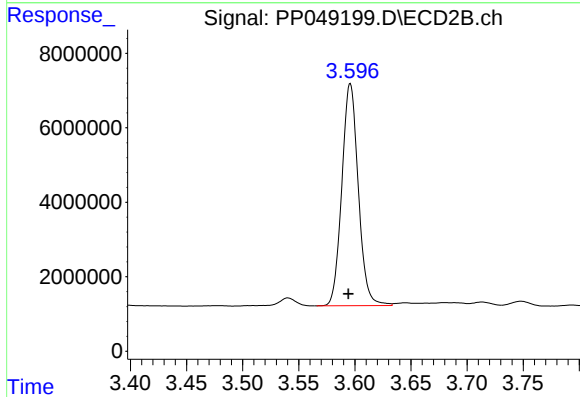


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.002 min
Response: 60975564
Conc: 23.81 ng/ml

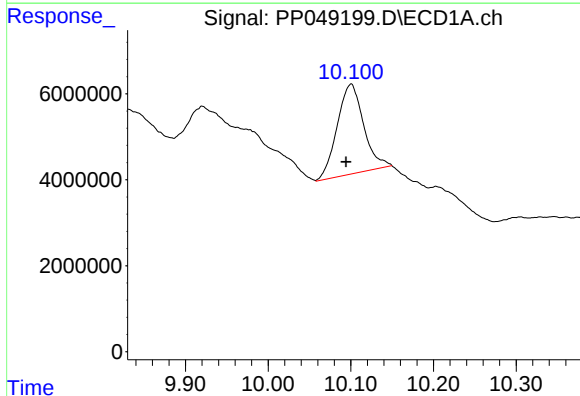

#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.006 min
Response: 46660311
Conc: 38.04 ng/ml m

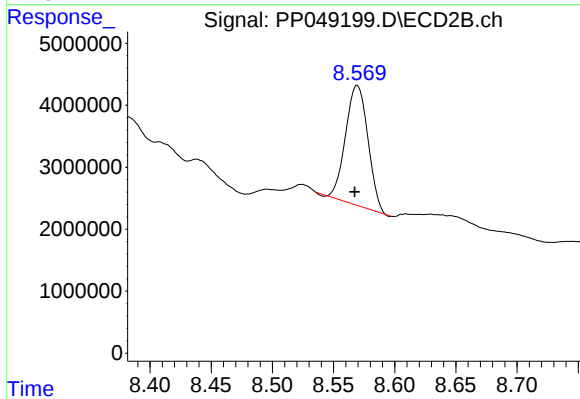

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: 0.002 min
Response: 24537744
Conc: 21.77 ng/ml