

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070621\
 Data File : PP037017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2021 15:58
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 08:35:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.952	0.000	5300	0	0.117	N.D. #
2)	SA Decachlor...	10.997	0.000	54423	0	1.182	N.D. #
Target Compounds							
9)	L2 AR-1221-2	5.308	0.000	8060	0	19.896	N.D. #
28)	L6 AR-1254-3	7.820f	0.000	27196	0	8.821	N.D. #
31)	L7 AR-1260-1	7.964	0.000	11827	0	5.373	N.D. #
32)	L7 AR-1260-2	8.208f	0.000	29530	0	10.616	N.D. #
33)	L7 AR-1260-3	8.601	7.146	4787	29370	2.368	17.141 #
34)	L7 AR-1260-4	8.806f	0.000	2790	0	1.134	N.D. #
36)	L8 AR-1262-1	8.601	0.000	4787	0	1.644	N.D. #
45)	L9 AR-1268-5	10.666	0.000	37704	0	2.381	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070621\
Data File : PP037017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 15:58
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 08:35:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

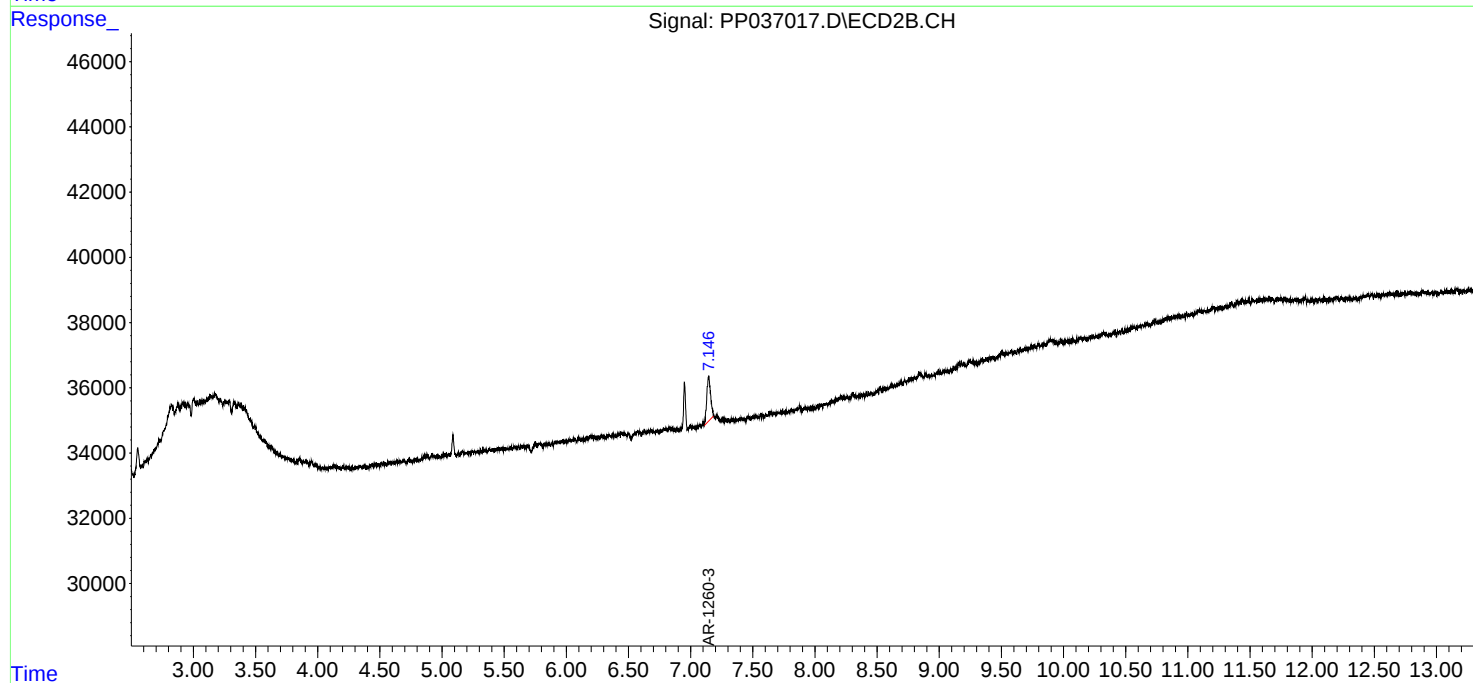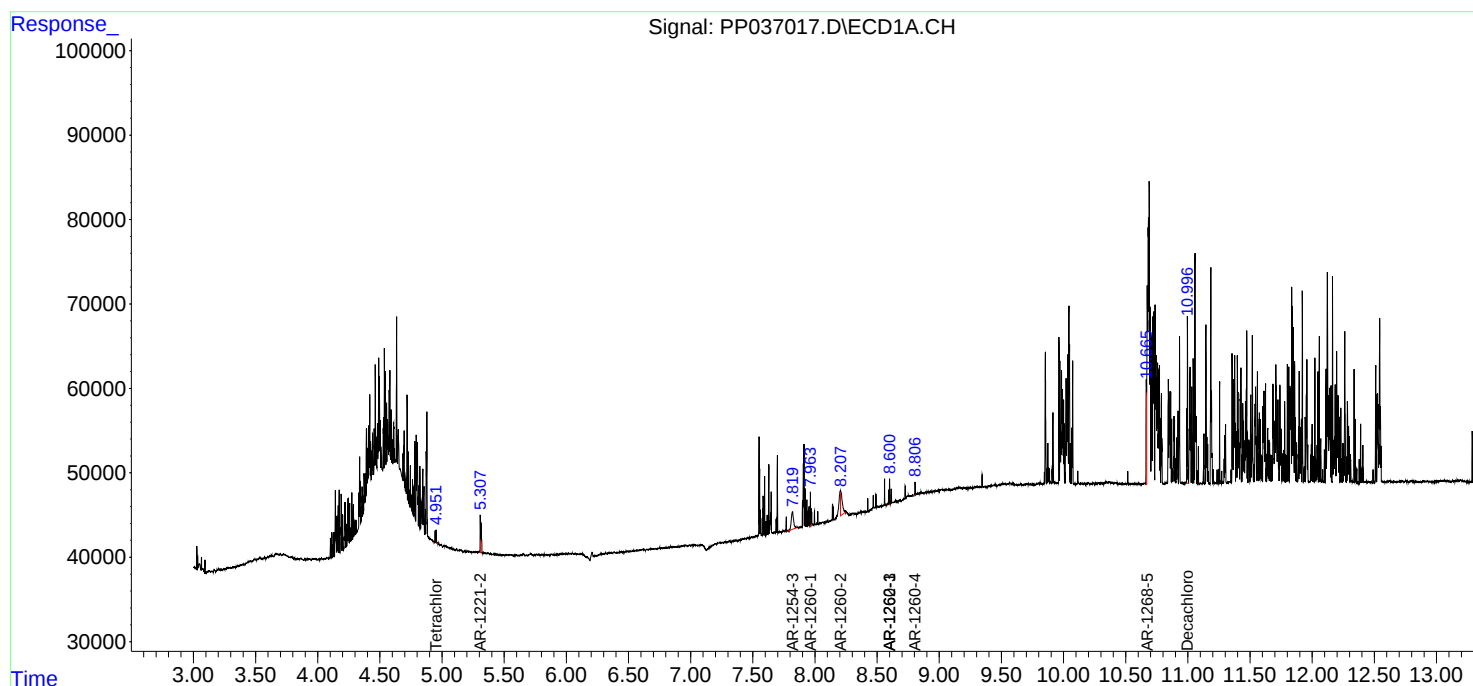


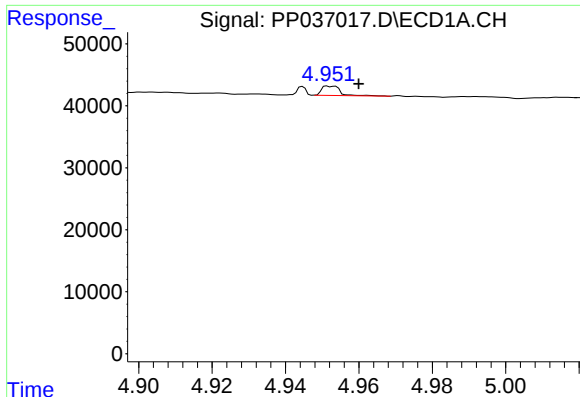

#1 Tetrachloro-m-xylene


R.T.: 4.952 min
Delta R.T.: -0.008 min
Response: 5300
Conc: 0.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

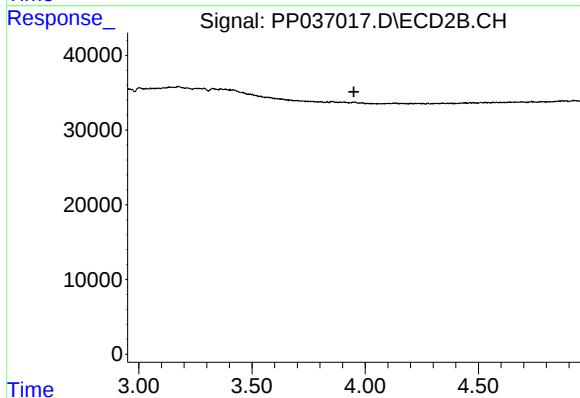


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.950 min
Response: 0
Conc: N.D.

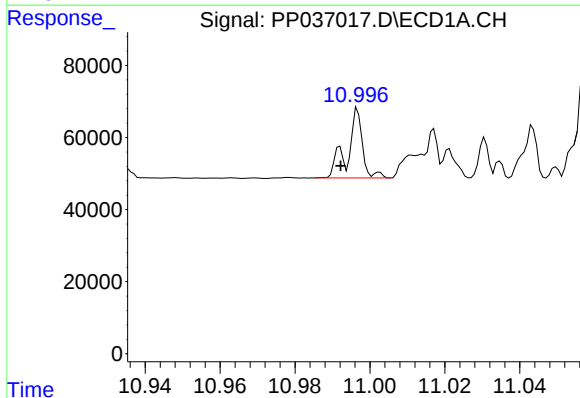


#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: 0.005 min
Response: 54423
Conc: 1.18 ng/ml

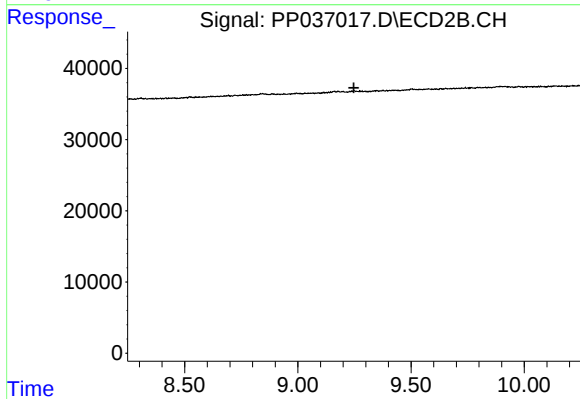

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.247 min
Response: 0
Conc: N.D.

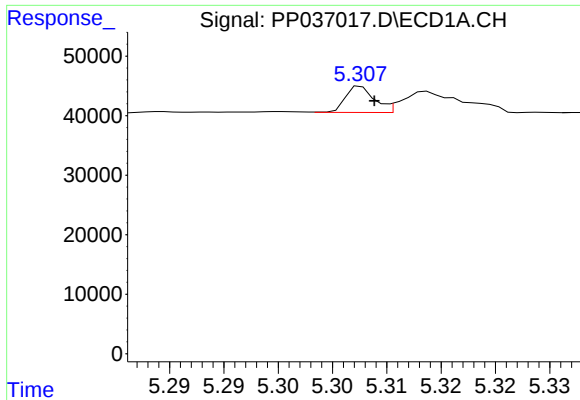

#9 AR-1221-2


R.T.: 5.308 min
Delta R.T.: -0.001 min
Response: 8060
Conc: 19.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

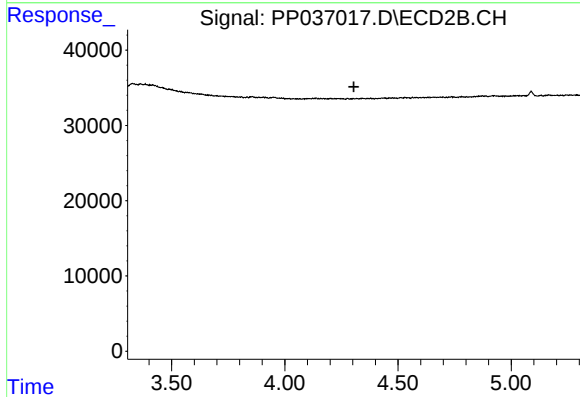


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

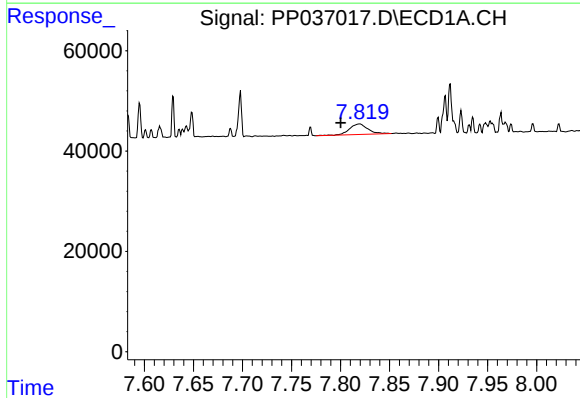


#28 AR-1254-3

R.T.: 7.820 min
Delta R.T.: 0.020 min
Response: 27196
Conc: 8.82 ng/ml

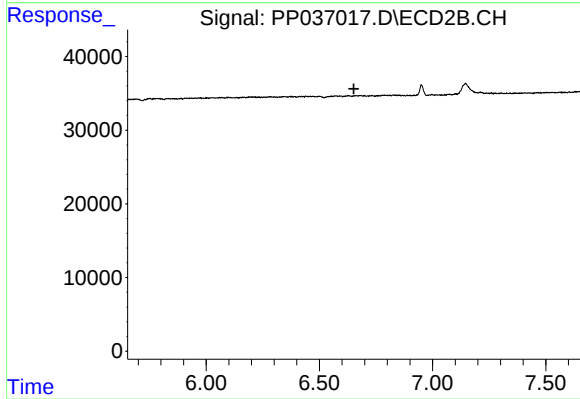

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

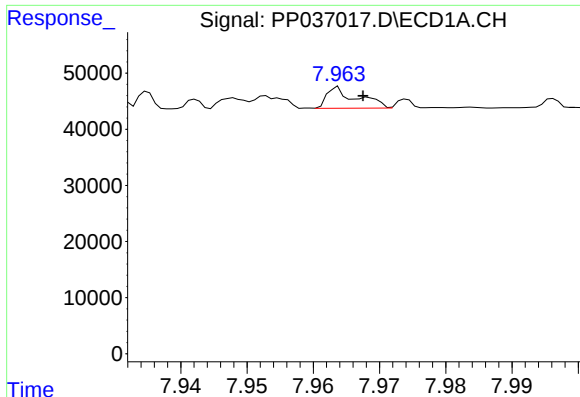

#31 AR-1260-1


R.T.: 7.964 min
Delta R.T.: -0.004 min
Response: 11827
Conc: 5.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

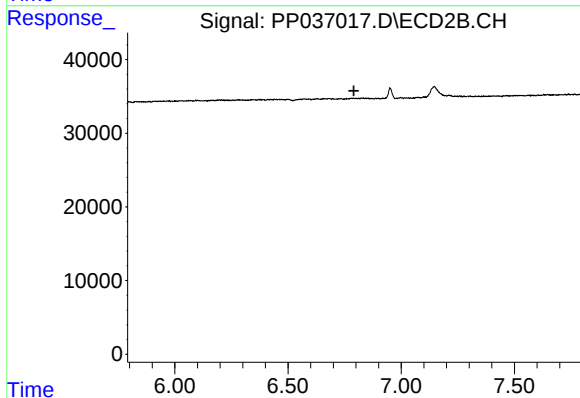


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.791 min
Response: 0
Conc: N.D.

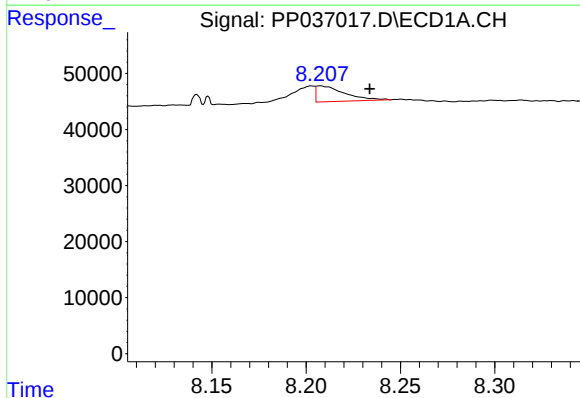


#32 AR-1260-2

R.T.: 8.208 min
Delta R.T.: -0.026 min
Response: 29530
Conc: 10.62 ng/ml

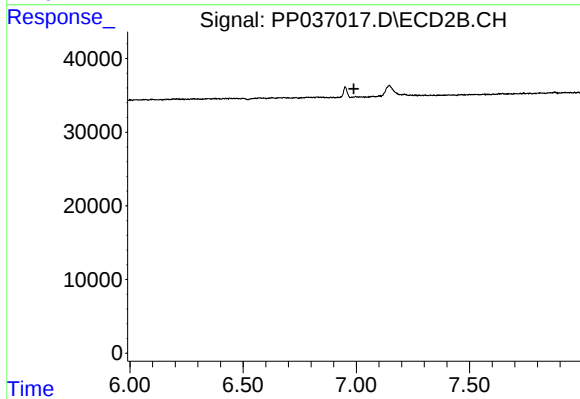

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

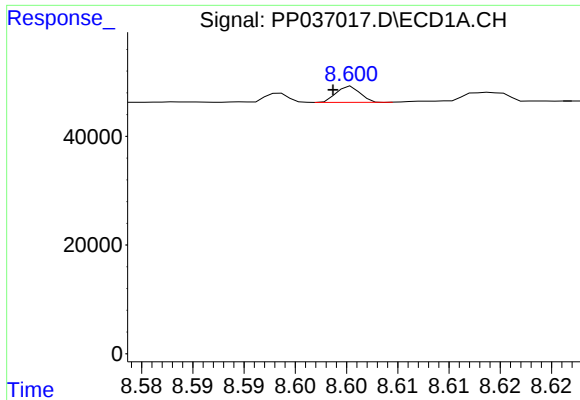

#33 AR-1260-3


R.T.: 8.601 min
Delta R.T.: 0.002 min
Response: 4787
Conc: 2.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

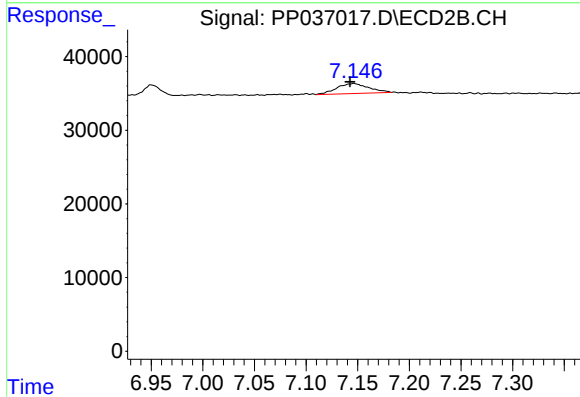


#33 AR-1260-3

R.T.: 7.146 min
Delta R.T.: 0.003 min
Response: 29370
Conc: 17.14 ng/ml

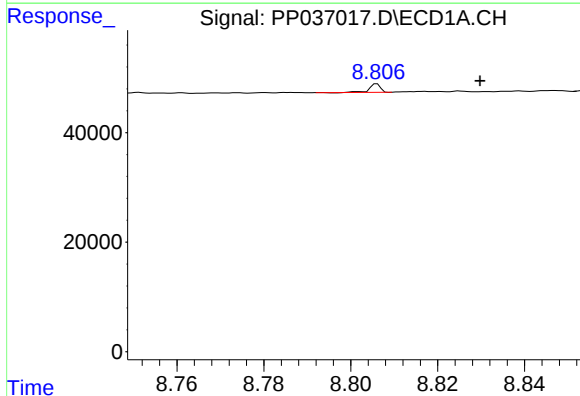


#34 AR-1260-4

R.T.: 8.806 min
Delta R.T.: -0.024 min
Response: 2790
Conc: 1.13 ng/ml

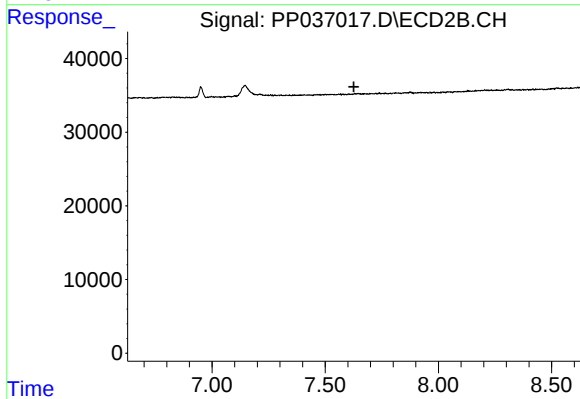

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.627 min
Response: 0
Conc: N.D.

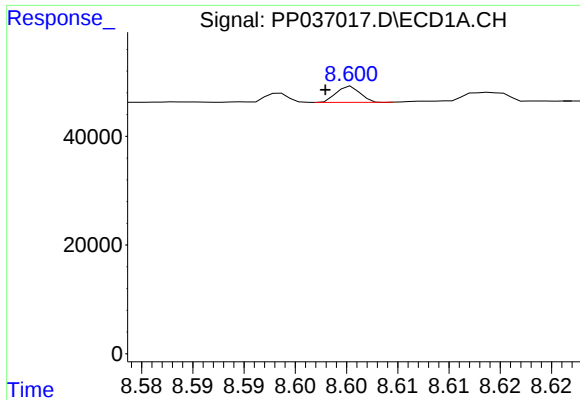

#36 AR-1262-1


R.T.: 8.601 min
Delta R.T.: 0.003 min
Response: 4787
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

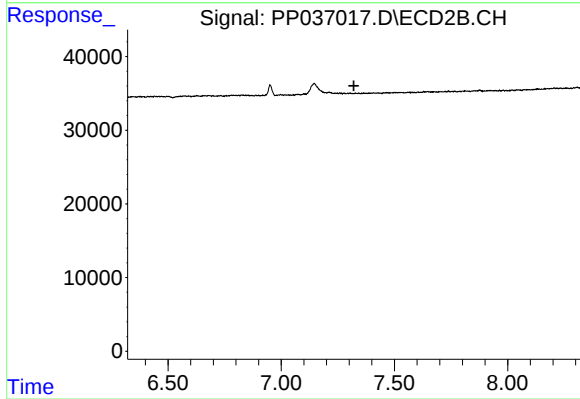


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.321 min
Response: 0
Conc: N.D.

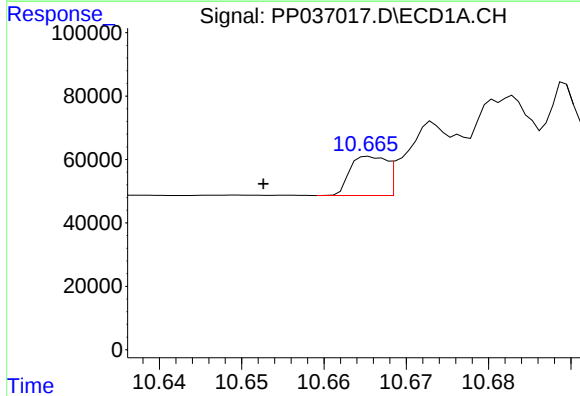

#45 AR-1268-5

R.T.: 10.666 min
Delta R.T.: 0.013 min
Response: 37704
Conc: 2.38 ng/ml

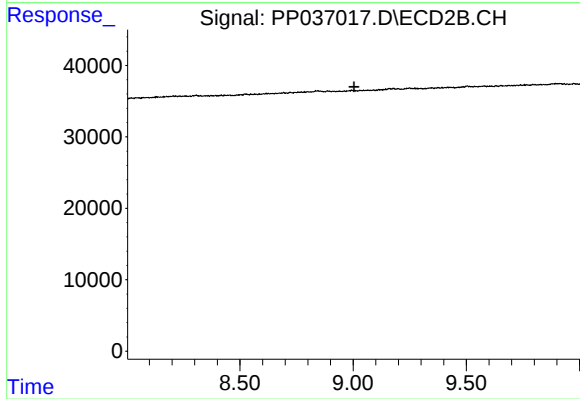

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.004 min
Response: 0
Conc: N.D.