

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070725\
 Data File : PP073541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 10:22
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 11:07:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.473	3.817f	6432	101856	0.004	0.057 #
2)	SA Decachlor...	10.192	0.000	118320	0	0.083	N.D. #
Target Compounds							
3)	L1 AR-1016-1	5.632	4.870	419131	79126	7.651	1.230 #
4)	L1 AR-1016-2	5.669	4.883	361812	89854	4.372	0.943 #
5)	L1 AR-1016-3	5.735	5.040	171045	184750	3.242	3.664
6)	L1 AR-1016-4	5.834	5.096	83917	517479	1.906	12.728 #
7)	L1 AR-1016-5	6.129	5.296	968700	300809	24.093	5.870 #
8)	L2 AR-1221-1	4.730f	4.001	86584	186009	4.588	6.911 #
9)	L2 AR-1221-2	4.765	4.082	215882	406156	13.396	19.754 #
10)	L2 AR-1221-3	4.858	4.162	143200	95639	2.768	1.576 #
11)	L3 AR-1232-1	4.858	4.162	143200	95639	3.583	2.032 #
12)	L3 AR-1232-2	5.369	4.883	87049	89854	4.233	1.912 #
13)	L3 AR-1232-3	5.669	5.040	361812	184750	8.547	7.460
14)	L3 AR-1232-4	5.834	5.144	83917	34168	3.893	1.595 #
15)	L3 AR-1232-5	5.930	5.296	185352	300809	13.178	12.871
16)	L4 AR-1242-1	5.632	4.870	419131	79126	8.249	1.355 #
17)	L4 AR-1242-2	5.669	4.883	361812	89854	4.772	1.041 #
18)	L4 AR-1242-3	5.735	5.040	171045	184750	3.561	4.026
19)	L4 AR-1242-4	5.834	5.144	83917	34168	2.179	0.778 #
20)	L4 AR-1242-5	6.557	5.647	206682	332435	4.863	6.076
21)	L5 AR-1248-1	5.632	4.870	419131	79126	10.714	1.799 #
22)	L5 AR-1248-2	5.930	5.096	185352	517479	3.591	8.785 #
23)	L5 AR-1248-3	6.129	5.144	968700	34168	17.095	0.566 #
24)	L5 AR-1248-4	6.519	5.296	682727	300809	9.700	4.218 #
25)	L5 AR-1248-5	6.557	5.686	206682	181118	2.953	2.463
26)	L6 AR-1254-1	6.462	5.647	2690641	332435	37.933	3.035 #
27)	L6 AR-1254-2	6.697	5.827	3335151	4694099	32.336	48.402 #
28)	L6 AR-1254-3	7.071	6.225	3775558	2780313	33.213	18.870 #
29)	L6 AR-1254-4	7.404f	6.452	6534487	347464	65.682	3.851 #
30)	L6 AR-1254-5	7.781	6.850	462.2E6	694.9E6	4876.755	5221.546
31)	L7 AR-1260-1	7.208	6.349	261448	49562	3.666	0.537 #
32)	L7 AR-1260-2	7.469	6.529	702.0E6	5465349	6678.387	44.220 #
33)	L7 AR-1260-3	7.850	6.657	240155	117779	2.606	1.177 #
34)	L7 AR-1260-4	8.073	7.190f	289290	112493	3.274	1.296 #
35)	L7 AR-1260-5	8.406	7.411	72558	47490	0.368	0.218 #
36)	L8 AR-1262-1	8.073	6.850f	289290	694.9E6	2.511	4630.770 #
37)	L8 AR-1262-2	8.363	7.190f	251585	112493	1.010	0.901
38)	L8 AR-1262-3	8.692	7.680	70332	73496	0.431	0.661 #
39)	L8 AR-1262-4	8.773	7.750	235456	63335	1.930	0.347 #
40)	L8 AR-1262-5	9.458	8.250	259789	36319	2.988	0.416 #
41)	L9 AR-1268-1	8.692	7.680	70332	73496	0.244	0.249

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070725\
 Data File : PP073541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 10:22
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 11:07:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.773	7.750	235456	63335	0.943	0.242 #
43) L9	AR-1268-3	9.010	7.949	201964	82588	0.918	0.377 #
44) L9	AR-1268-4	9.458	8.250	259789	36319	2.710	0.384 #
45) L9	AR-1268-5	9.850	8.579f	68673	42773	0.110	0.069 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070725\
Data File : PP073541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 10:22
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 11:07:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

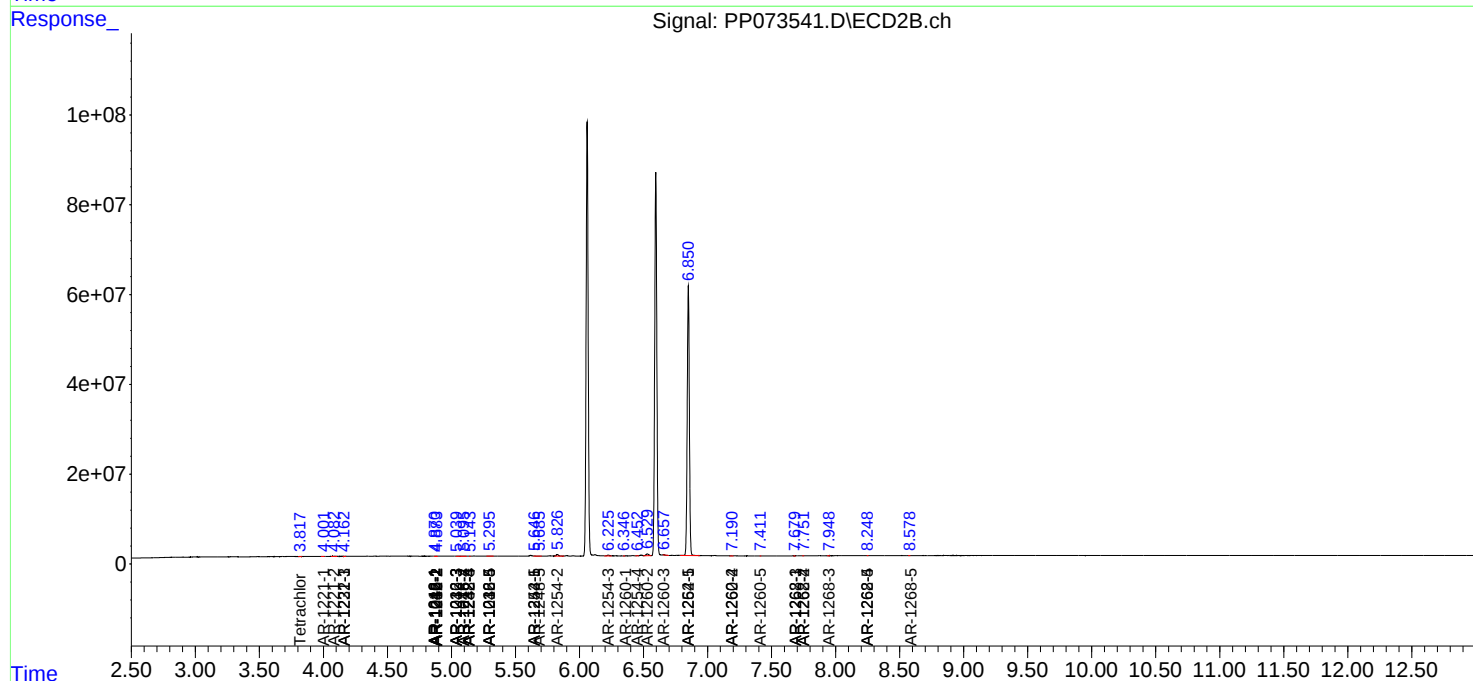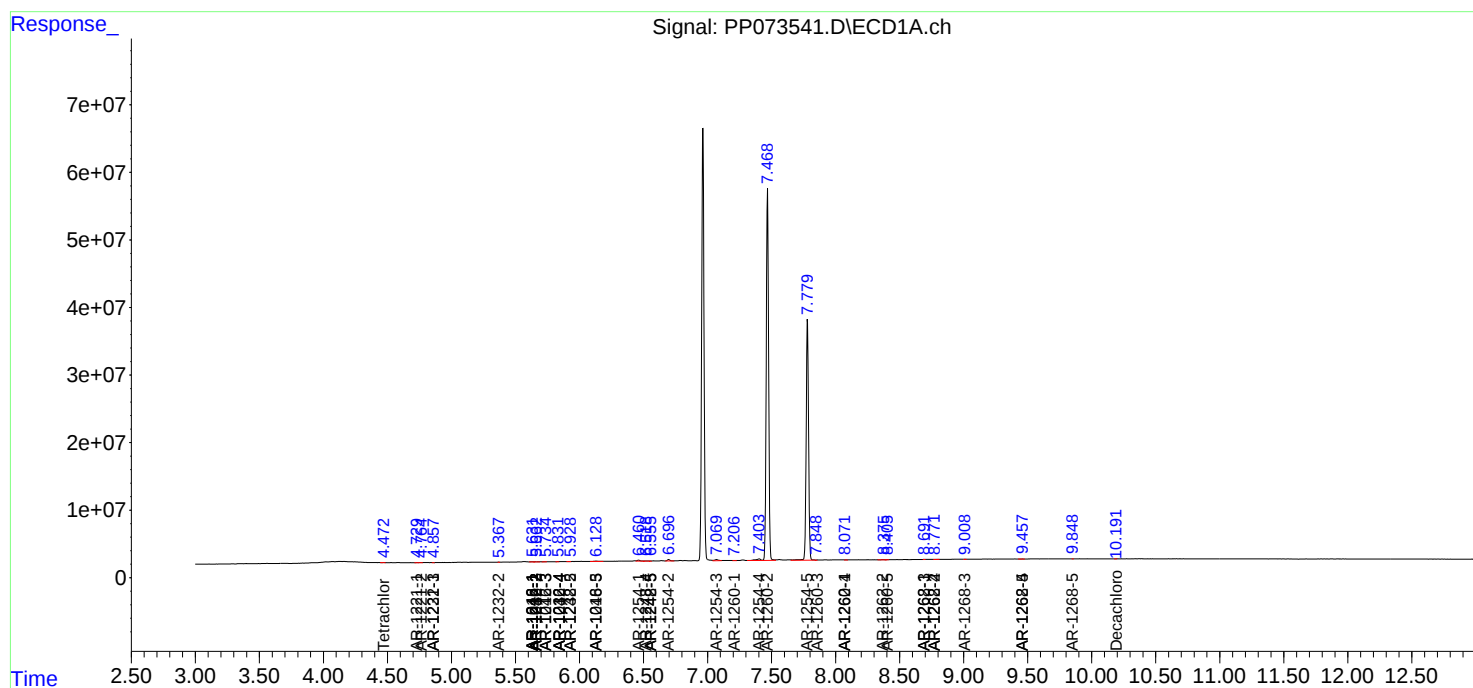


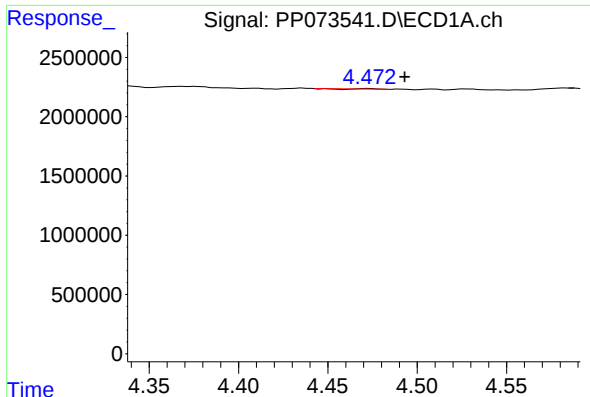

#1 Tetrachloro-m-xylene


R.T.: 4.473 min
Delta R.T.: -0.020 min
Response: 6432
Conc: 0.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

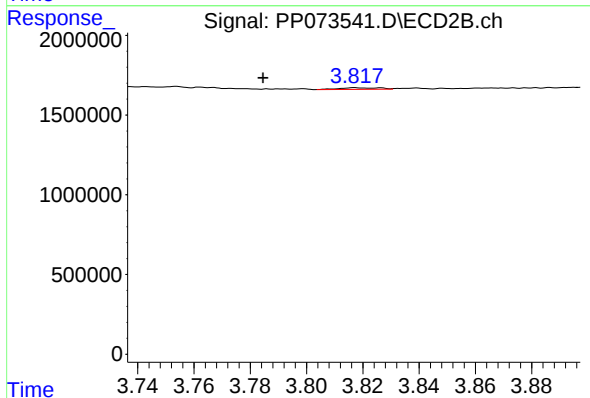


#1 Tetrachloro-m-xylene

R.T.: 3.817 min
Delta R.T.: 0.033 min
Response: 101856
Conc: 0.06 ng/ml

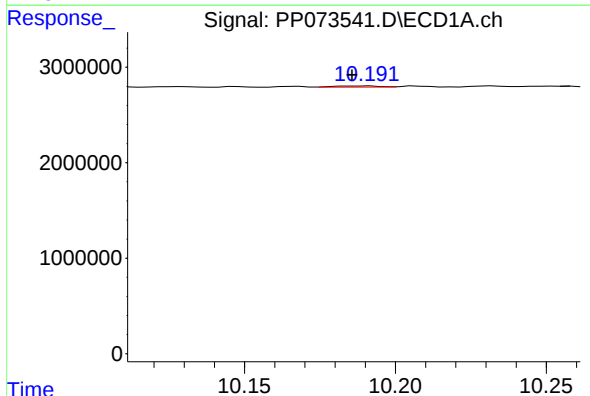


#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: 0.006 min
Response: 118320
Conc: 0.08 ng/ml

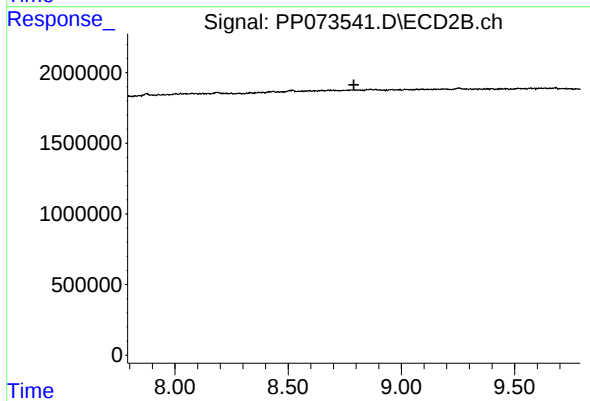

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 8.790 min
Response: 0
Conc: N.D.

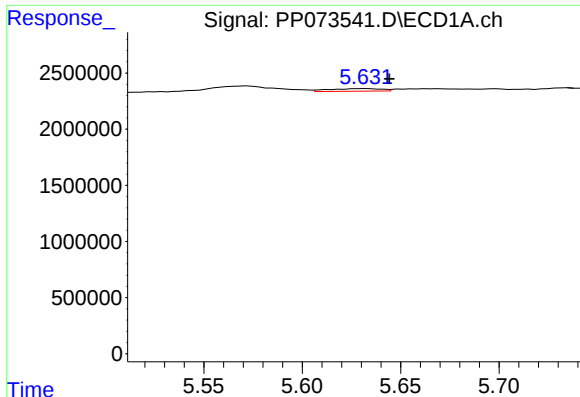

#3 AR-1016-1


R.T.: 5.632 min
Delta R.T.: -0.012 min
Response: 419131
Conc: 7.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

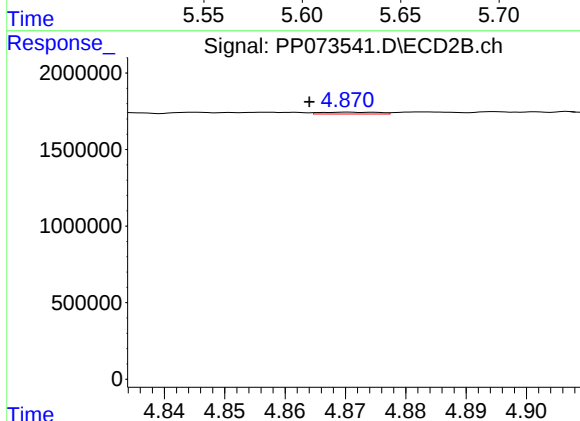


#3 AR-1016-1

R.T.: 4.870 min
Delta R.T.: 0.006 min
Response: 79126
Conc: 1.23 ng/ml

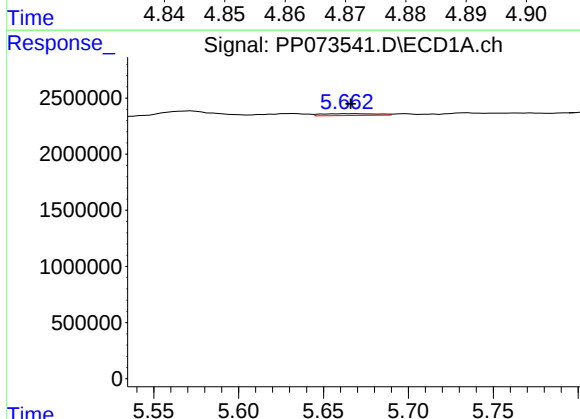


#4 AR-1016-2

R.T.: 5.669 min
Delta R.T.: 0.003 min
Response: 361812
Conc: 4.37 ng/ml

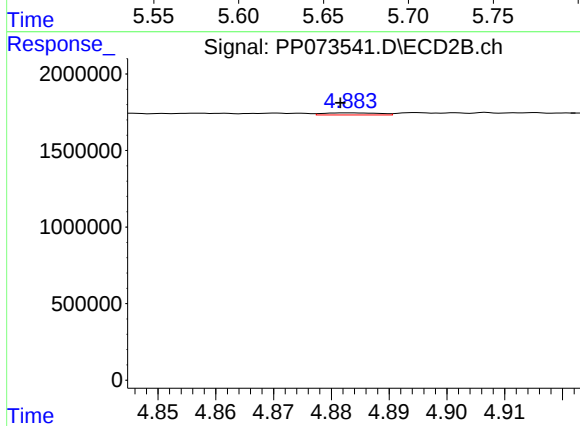

#4 AR-1016-2


R.T.: 4.883 min
Delta R.T.: 0.001 min
Response: 89854
Conc: 0.94 ng/ml

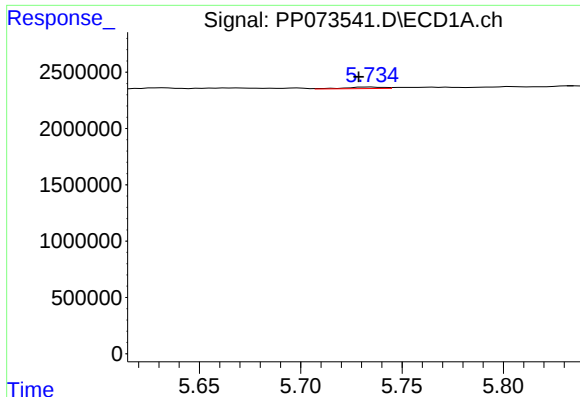

#5 AR-1016-3


R.T.: 5.735 min
Delta R.T.: 0.007 min
Response: 171045
Conc: 3.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

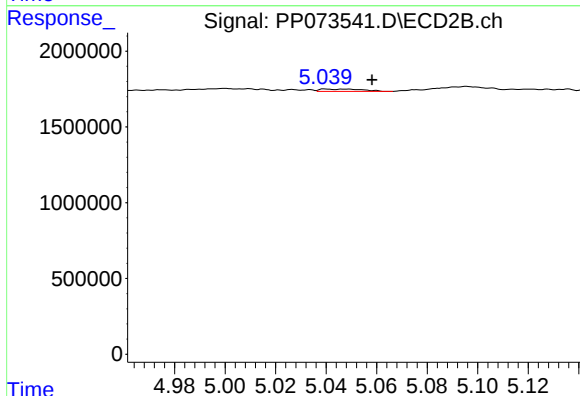


#5 AR-1016-3

R.T.: 5.040 min
Delta R.T.: -0.018 min
Response: 184750
Conc: 3.66 ng/ml

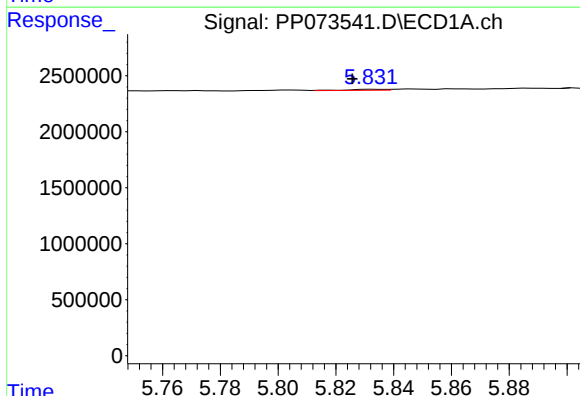


#6 AR-1016-4

R.T.: 5.834 min
Delta R.T.: 0.008 min
Response: 83917
Conc: 1.91 ng/ml

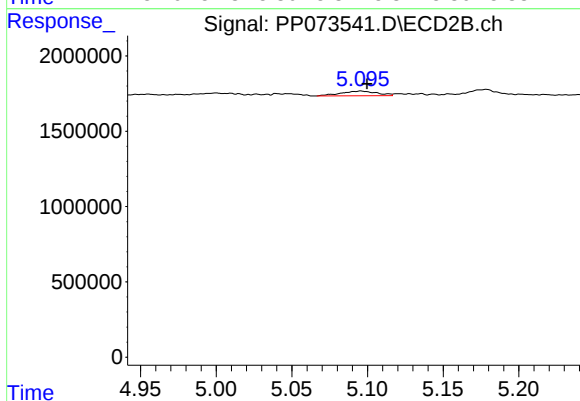

#6 AR-1016-4


R.T.: 5.096 min
Delta R.T.: -0.004 min
Response: 517479
Conc: 12.73 ng/ml

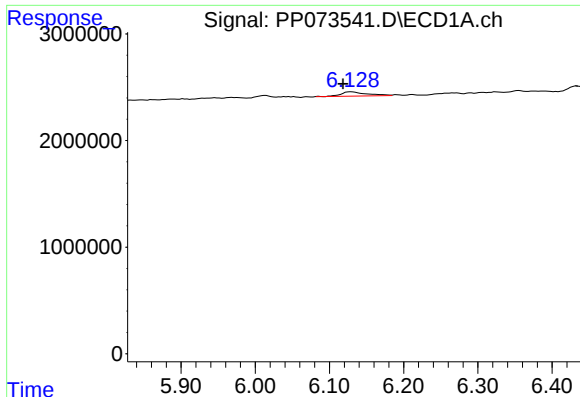

#7 AR-1016-5


R.T.: 6.129 min
Delta R.T.: 0.011 min
Response: 968700
Conc: 24.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

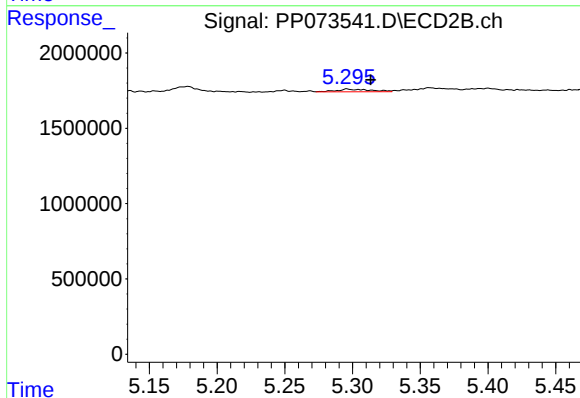


#7 AR-1016-5

R.T.: 5.296 min
Delta R.T.: -0.018 min
Response: 300809
Conc: 5.87 ng/ml

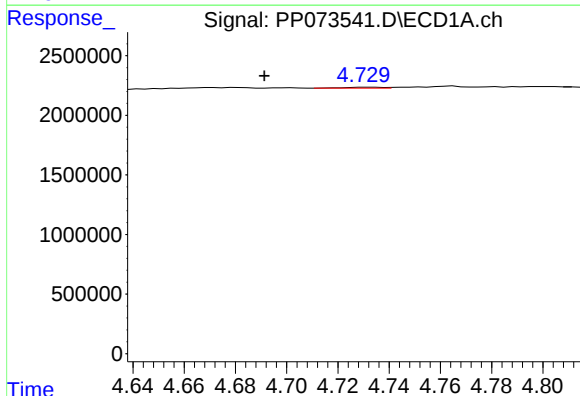


#8 AR-1221-1

R.T.: 4.730 min
Delta R.T.: 0.039 min
Response: 86584
Conc: 4.59 ng/ml

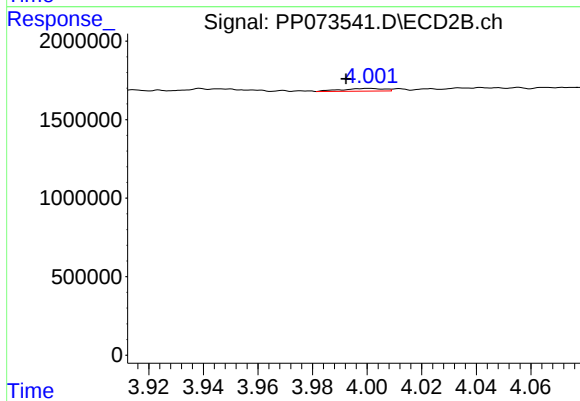

#8 AR-1221-1


R.T.: 4.001 min
Delta R.T.: 0.009 min
Response: 186009
Conc: 6.91 ng/ml

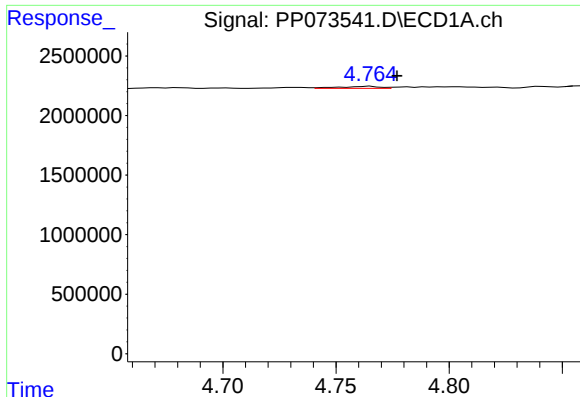

#9 AR-1221-2


R.T.: 4.765 min
Delta R.T.: -0.012 min
Response: 215882
Conc: 13.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

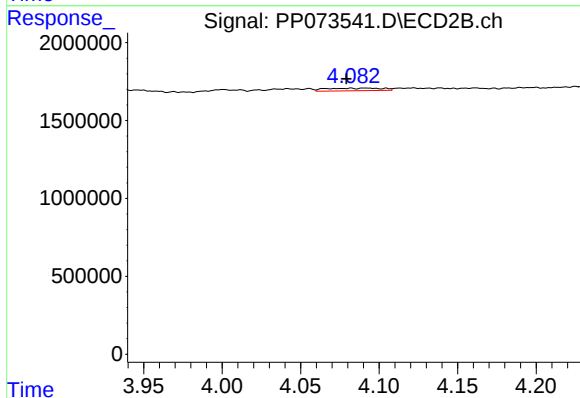


#9 AR-1221-2

R.T.: 4.082 min
Delta R.T.: 0.003 min
Response: 406156
Conc: 19.75 ng/ml

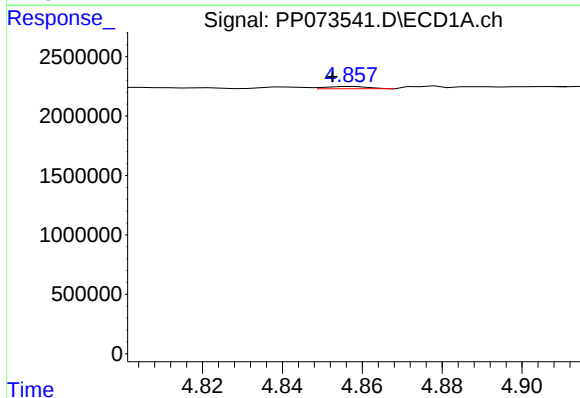


#10 AR-1221-3

R.T.: 4.858 min
Delta R.T.: 0.005 min
Response: 143200
Conc: 2.77 ng/ml

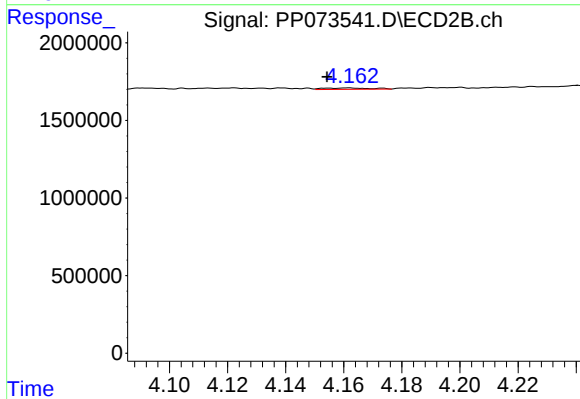

#10 AR-1221-3


R.T.: 4.162 min
Delta R.T.: 0.007 min
Response: 95639
Conc: 1.58 ng/ml

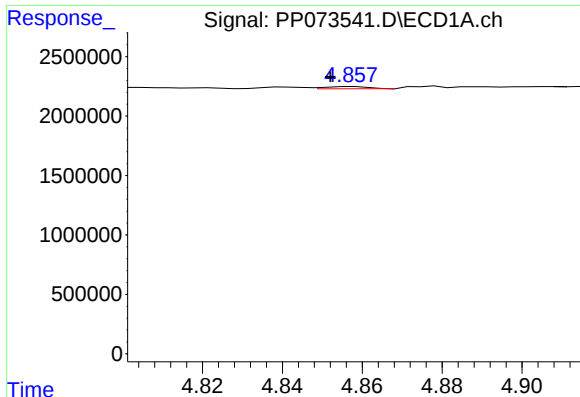

#11 AR-1232-1


R.T.: 4.858 min
Delta R.T.: 0.006 min
Response: 143200
Conc: 3.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

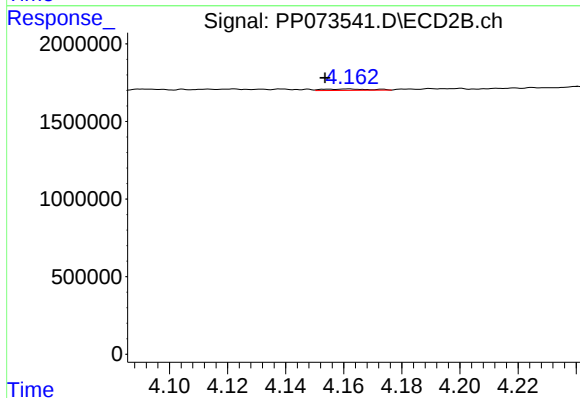


#11 AR-1232-1

R.T.: 4.162 min
Delta R.T.: 0.008 min
Response: 95639
Conc: 2.03 ng/ml

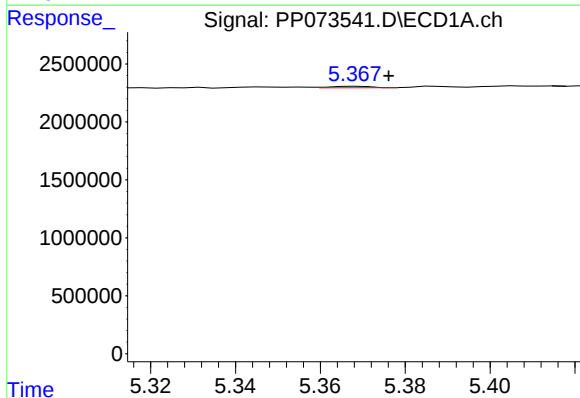


#12 AR-1232-2

R.T.: 5.369 min
Delta R.T.: -0.007 min
Response: 87049
Conc: 4.23 ng/ml

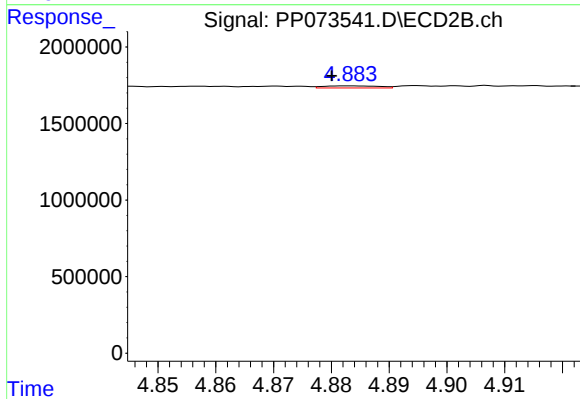

#12 AR-1232-2


R.T.: 4.883 min
Delta R.T.: 0.003 min
Response: 89854
Conc: 1.91 ng/ml

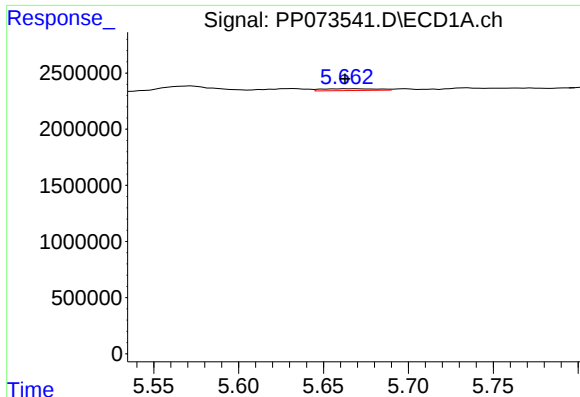

#13 AR-1232-3


R.T.: 5.669 min
Delta R.T.: 0.006 min
Response: 361812
Conc: 8.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

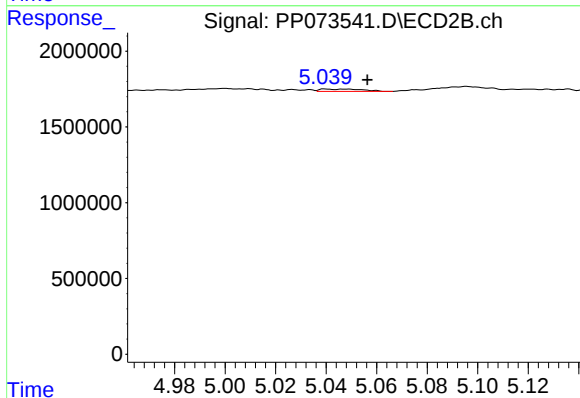


#13 AR-1232-3

R.T.: 5.040 min
Delta R.T.: -0.016 min
Response: 184750
Conc: 7.46 ng/ml

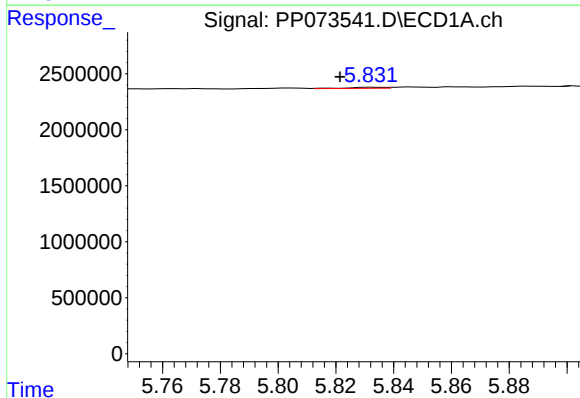


#14 AR-1232-4

R.T.: 5.834 min
Delta R.T.: 0.012 min
Response: 83917
Conc: 3.89 ng/ml

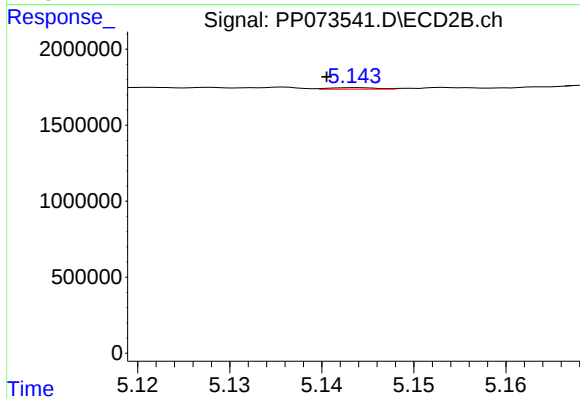

#14 AR-1232-4


R.T.: 5.144 min
Delta R.T.: 0.003 min
Response: 34168
Conc: 1.59 ng/ml

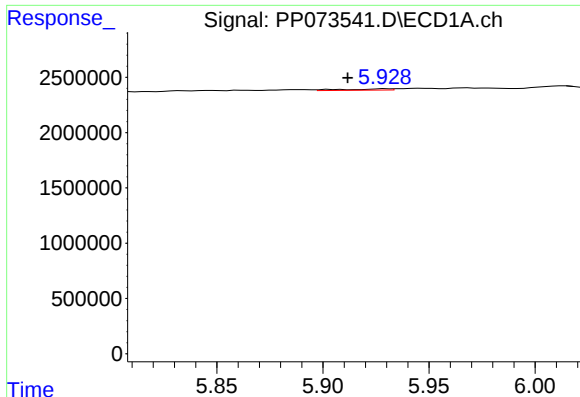

#15 AR-1232-5


R.T.: 5.930 min
Delta R.T.: 0.018 min
Response: 185352
Conc: 13.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

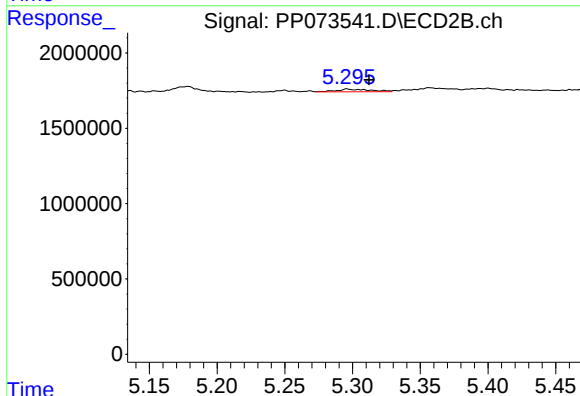


#15 AR-1232-5

R.T.: 5.296 min
Delta R.T.: -0.016 min
Response: 300809
Conc: 12.87 ng/ml

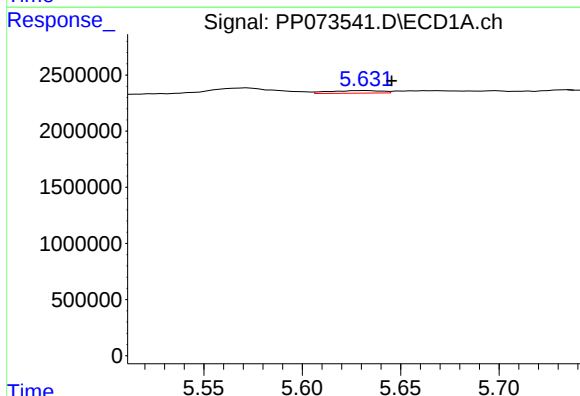


#16 AR-1242-1

R.T.: 5.632 min
Delta R.T.: -0.013 min
Response: 419131
Conc: 8.25 ng/ml

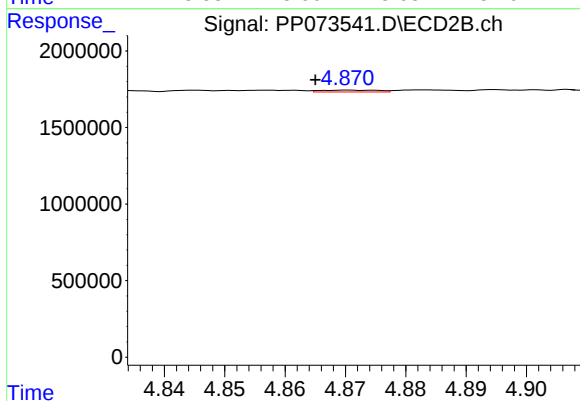

#16 AR-1242-1


R.T.: 4.870 min
Delta R.T.: 0.005 min
Response: 79126
Conc: 1.35 ng/ml

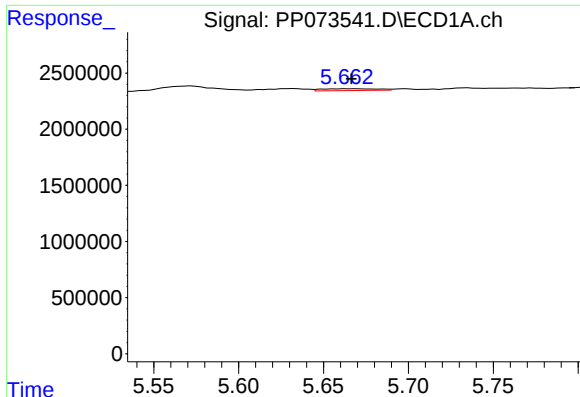

#17 AR-1242-2


R.T.: 5.669 min
Delta R.T.: 0.002 min
Response: 361812
Conc: 4.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

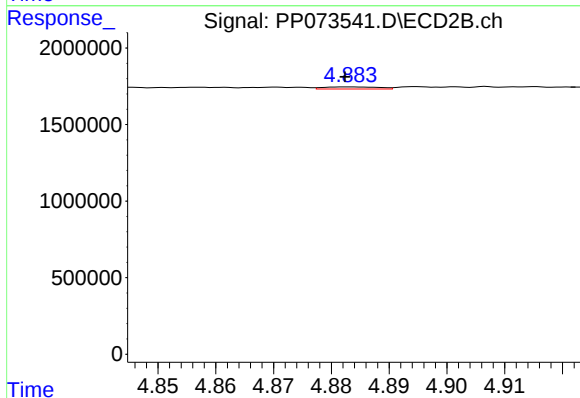


#17 AR-1242-2

R.T.: 4.883 min
Delta R.T.: 0.000 min
Response: 89854
Conc: 1.04 ng/ml

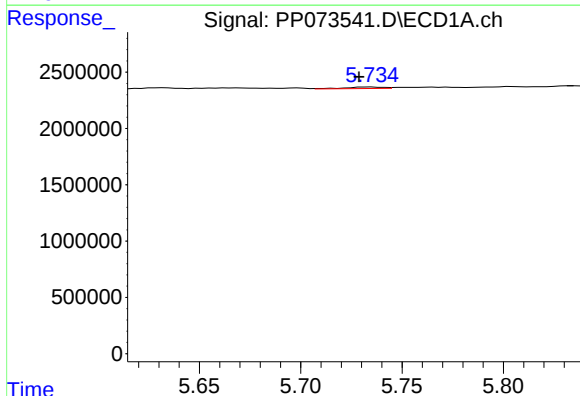


#18 AR-1242-3

R.T.: 5.735 min
Delta R.T.: 0.007 min
Response: 171045
Conc: 3.56 ng/ml

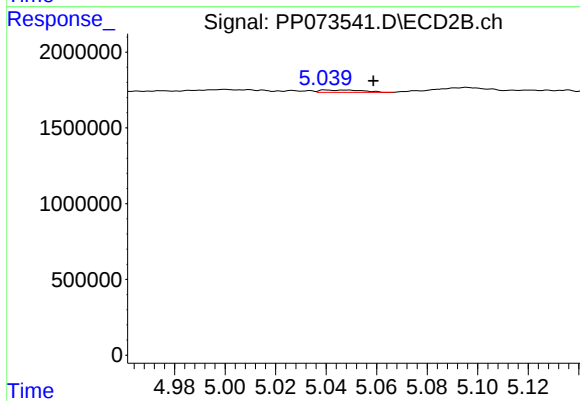

#18 AR-1242-3


R.T.: 5.040 min
Delta R.T.: -0.019 min
Response: 184750
Conc: 4.03 ng/ml

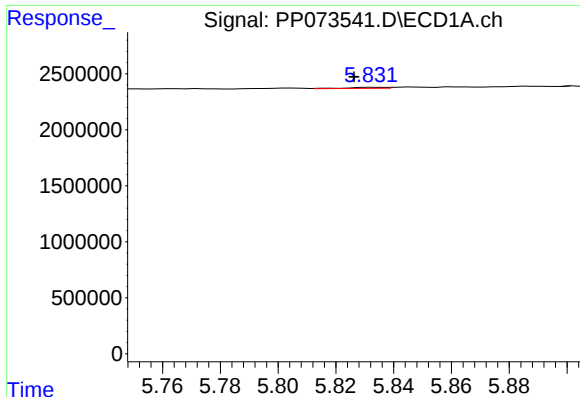

#19 AR-1242-4


R.T.: 5.834 min
Delta R.T.: 0.008 min
Response: 83917
Conc: 2.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

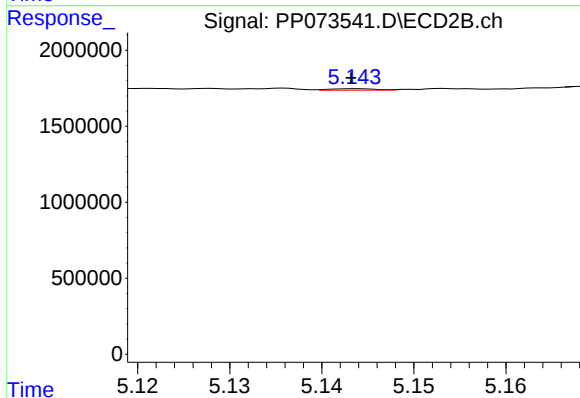


#19 AR-1242-4

R.T.: 5.144 min
Delta R.T.: 0.000 min
Response: 34168
Conc: 0.78 ng/ml

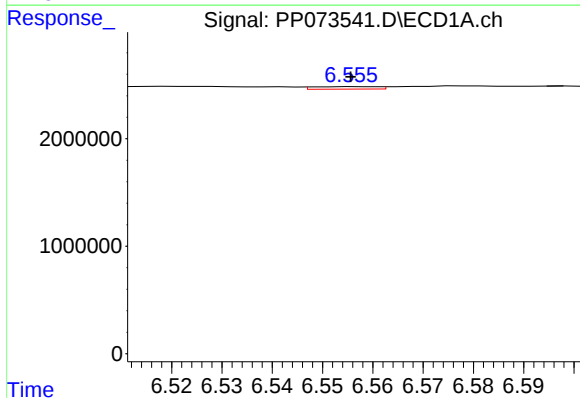


#20 AR-1242-5

R.T.: 6.557 min
Delta R.T.: 0.001 min
Response: 206682
Conc: 4.86 ng/ml

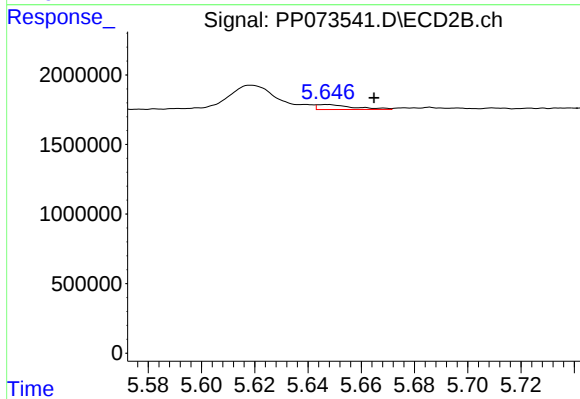

#20 AR-1242-5


R.T.: 5.647 min
Delta R.T.: -0.018 min
Response: 332435
Conc: 6.08 ng/ml

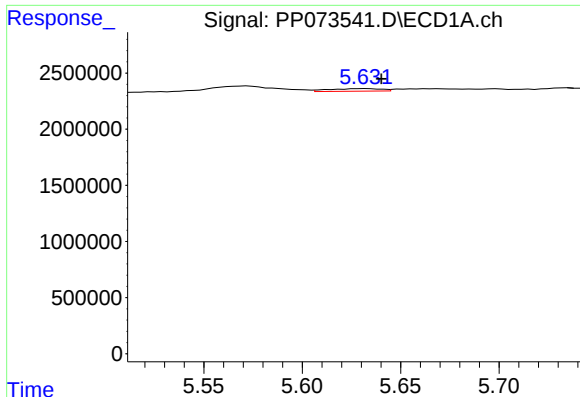

#21 AR-1248-1


R.T.: 5.632 min
Delta R.T.: -0.008 min
Response: 419131
Conc: 10.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

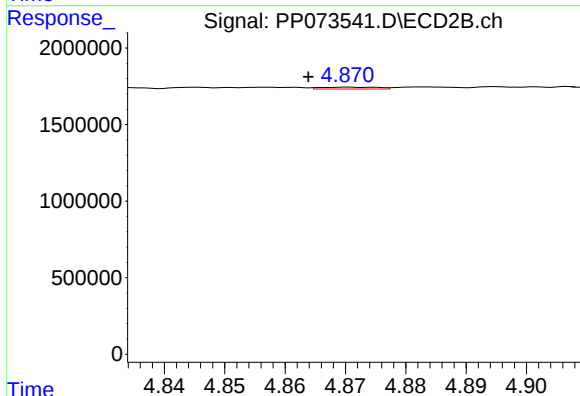


#21 AR-1248-1

R.T.: 4.870 min
Delta R.T.: 0.007 min
Response: 79126
Conc: 1.80 ng/ml

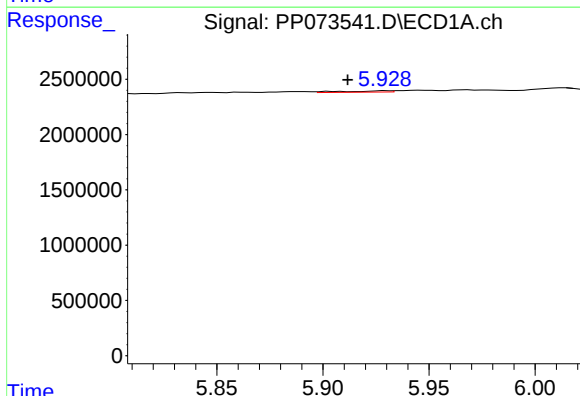


#22 AR-1248-2

R.T.: 5.930 min
Delta R.T.: 0.018 min
Response: 185352
Conc: 3.59 ng/ml

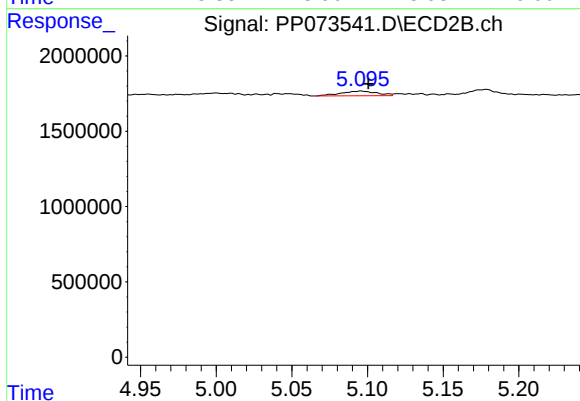

#22 AR-1248-2


R.T.: 5.096 min
Delta R.T.: -0.005 min
Response: 517479
Conc: 8.78 ng/ml

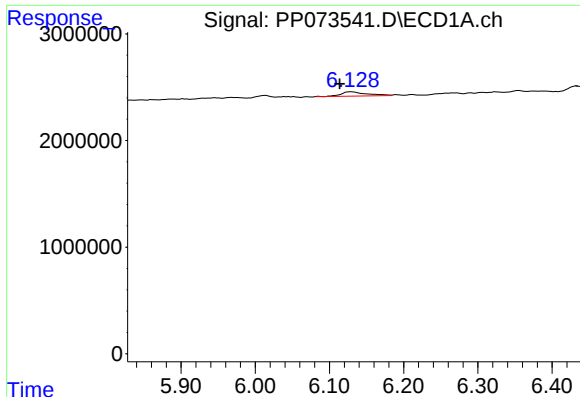

#23 AR-1248-3


R.T.: 6.129 min
Delta R.T.: 0.015 min
Response: 968700
Conc: 17.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

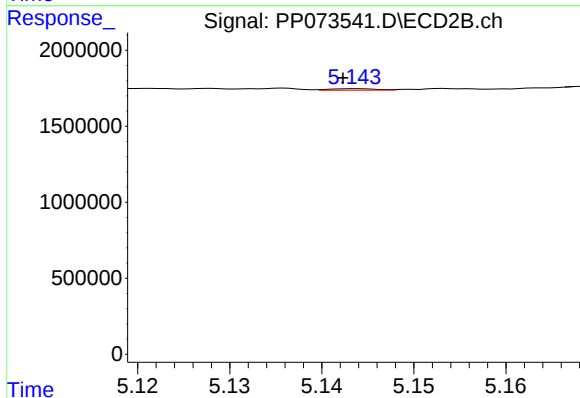


#23 AR-1248-3

R.T.: 5.144 min
Delta R.T.: 0.001 min
Response: 34168
Conc: 0.57 ng/ml

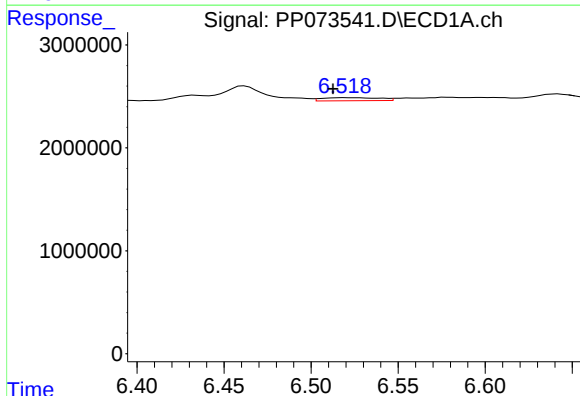


#24 AR-1248-4

R.T.: 6.519 min
Delta R.T.: 0.007 min
Response: 682727
Conc: 9.70 ng/ml

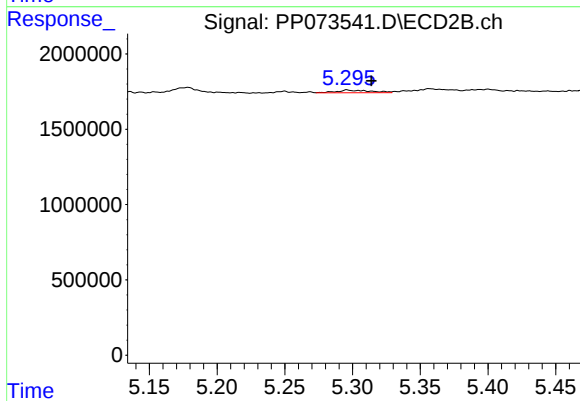

#24 AR-1248-4


R.T.: 5.296 min
Delta R.T.: -0.018 min
Response: 300809
Conc: 4.22 ng/ml

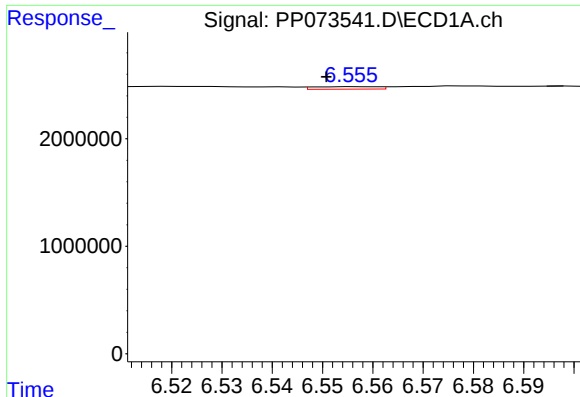

#25 AR-1248-5


R.T.: 6.557 min
Delta R.T.: 0.006 min
Response: 206682
Conc: 2.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

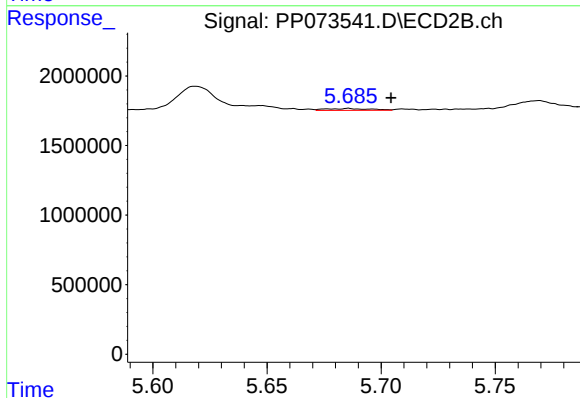


#25 AR-1248-5

R.T.: 5.686 min
Delta R.T.: -0.019 min
Response: 181118
Conc: 2.46 ng/ml

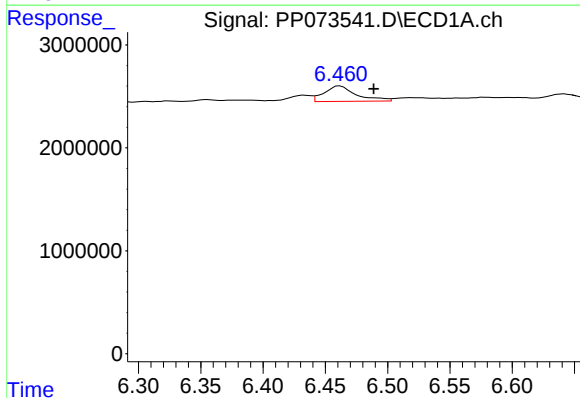


#26 AR-1254-1

R.T.: 6.462 min
Delta R.T.: -0.027 min
Response: 2690641
Conc: 37.93 ng/ml

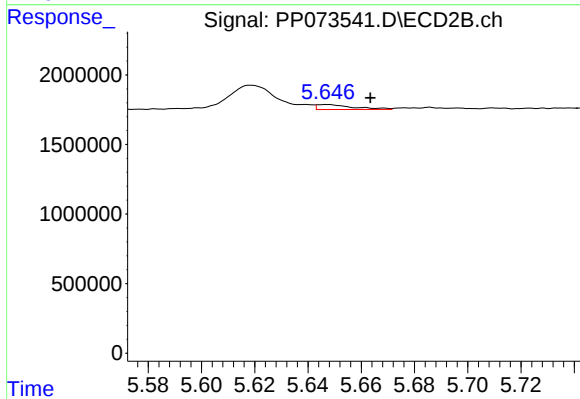

#26 AR-1254-1


R.T.: 5.647 min
Delta R.T.: -0.016 min
Response: 332435
Conc: 3.03 ng/ml

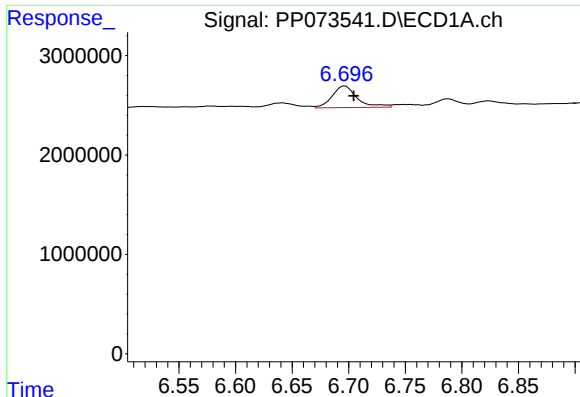

#27 AR-1254-2


R.T.: 6.697 min
Delta R.T.: -0.008 min
Response: 3335151
Conc: 32.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

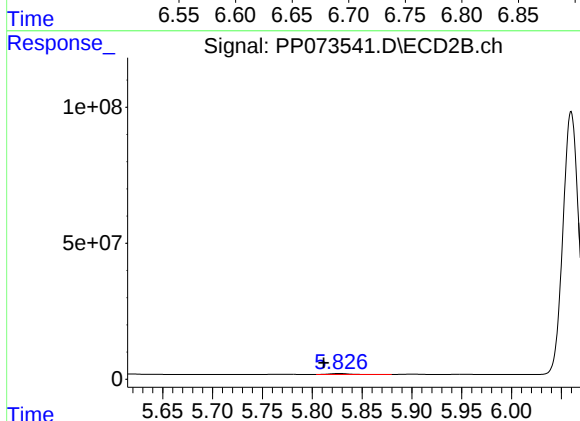


#27 AR-1254-2

R.T.: 5.827 min
Delta R.T.: 0.015 min
Response: 4694099
Conc: 48.40 ng/ml

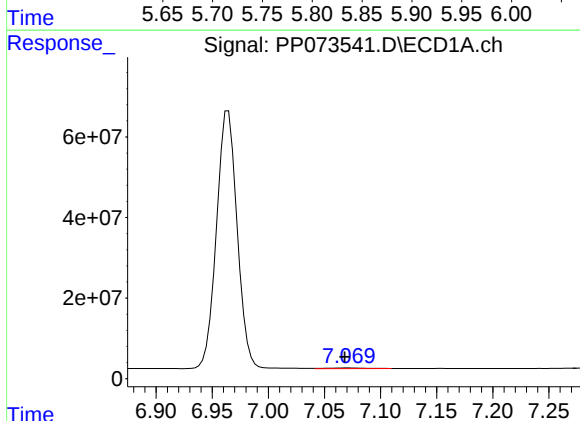


#28 AR-1254-3

R.T.: 7.071 min
Delta R.T.: 0.003 min
Response: 3775558
Conc: 33.21 ng/ml

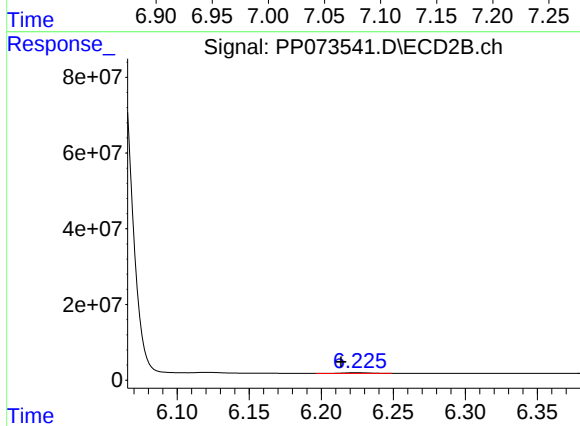

#28 AR-1254-3


R.T.: 6.225 min
Delta R.T.: 0.011 min
Response: 2780313
Conc: 18.87 ng/ml

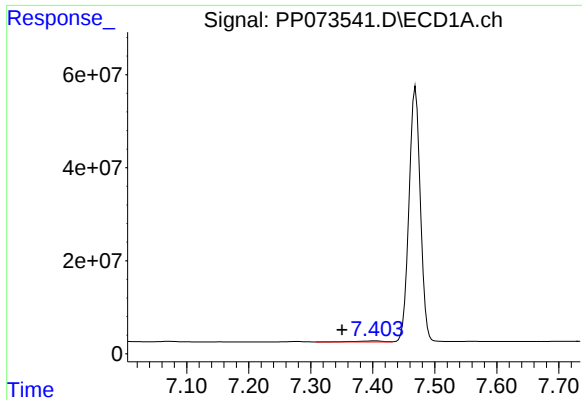

#29 AR-1254-4


R.T.: 7.404 min
Delta R.T.: 0.054 min
Response: 6534487
Conc: 65.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

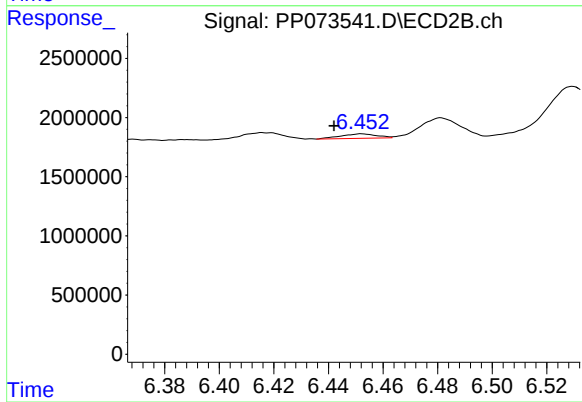


#29 AR-1254-4

R.T.: 6.452 min
Delta R.T.: 0.010 min
Response: 347464
Conc: 3.85 ng/ml

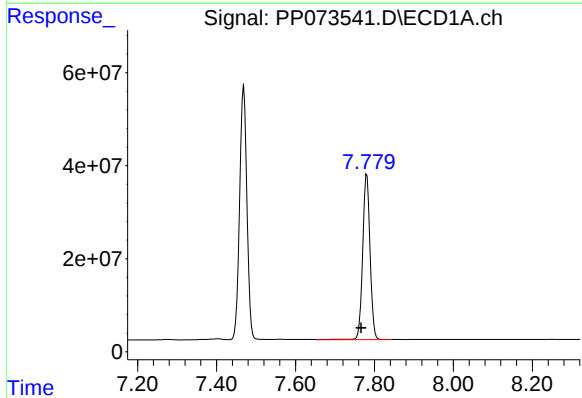


#30 AR-1254-5

R.T.: 7.781 min
Delta R.T.: 0.014 min
Response: 462186749
Conc: 4876.75 ng/ml

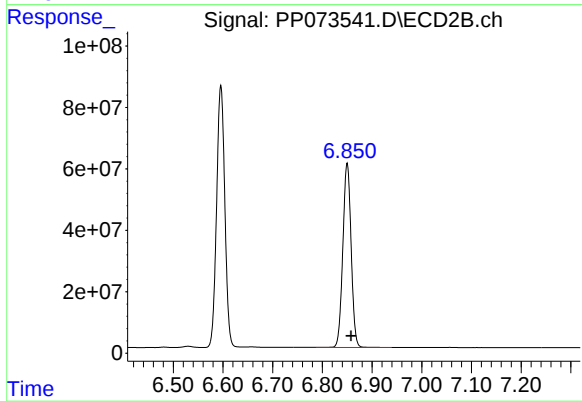

#30 AR-1254-5


R.T.: 6.850 min
Delta R.T.: -0.008 min
Response: 694860070
Conc: 5221.55 ng/ml

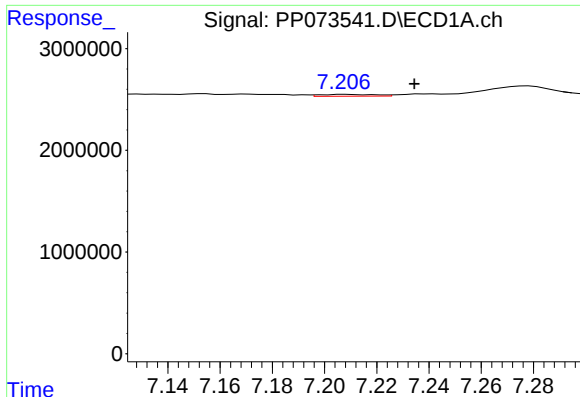

#31 AR-1260-1


R.T.: 7.208 min
Delta R.T.: -0.027 min
Response: 261448
Conc: 3.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

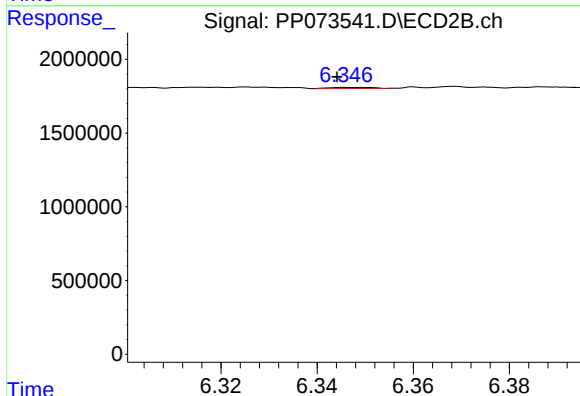


#31 AR-1260-1

R.T.: 6.349 min
Delta R.T.: 0.005 min
Response: 49562
Conc: 0.54 ng/ml

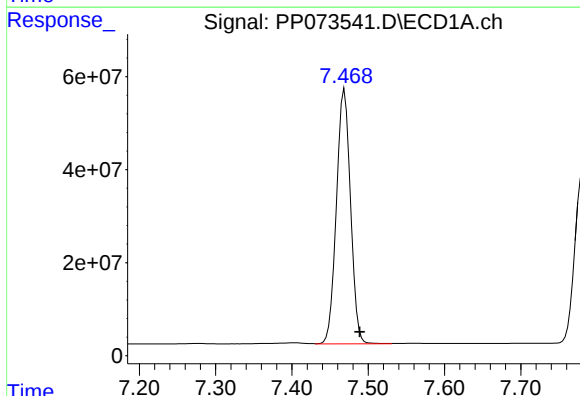


#32 AR-1260-2

R.T.: 7.469 min
Delta R.T.: -0.020 min
Response: 701974249
Conc: 6678.39 ng/ml

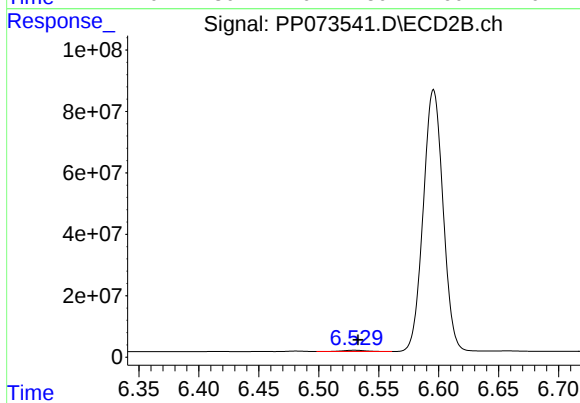

#32 AR-1260-2


R.T.: 6.529 min
Delta R.T.: -0.003 min
Response: 5465349
Conc: 44.22 ng/ml

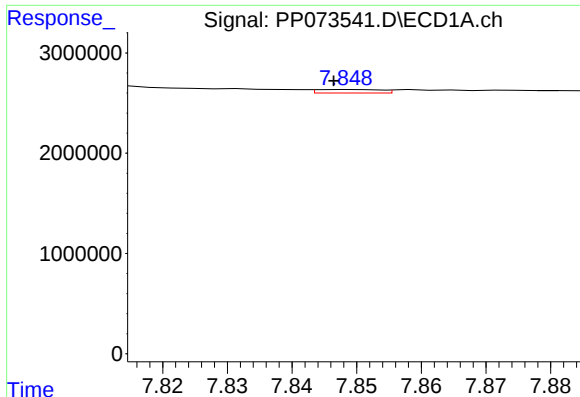

#33 AR-1260-3


R.T.: 7.850 min
Delta R.T.: 0.003 min
Response: 240155
Conc: 2.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

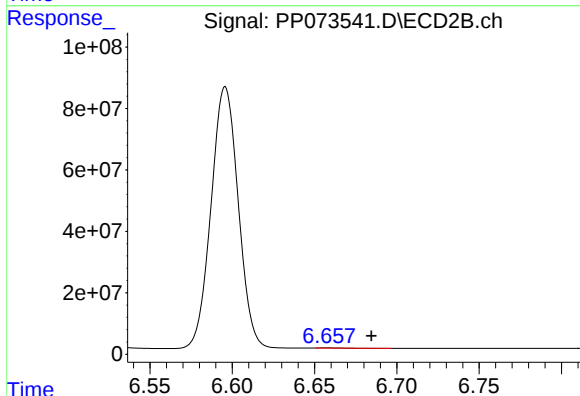


#33 AR-1260-3

R.T.: 6.657 min
Delta R.T.: -0.027 min
Response: 117779
Conc: 1.18 ng/ml

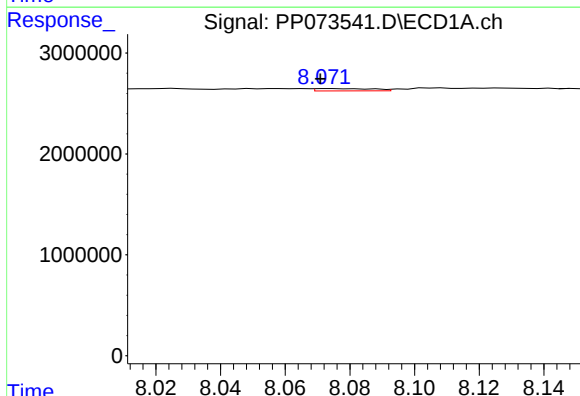


#34 AR-1260-4

R.T.: 8.073 min
Delta R.T.: 0.003 min
Response: 289290
Conc: 3.27 ng/ml

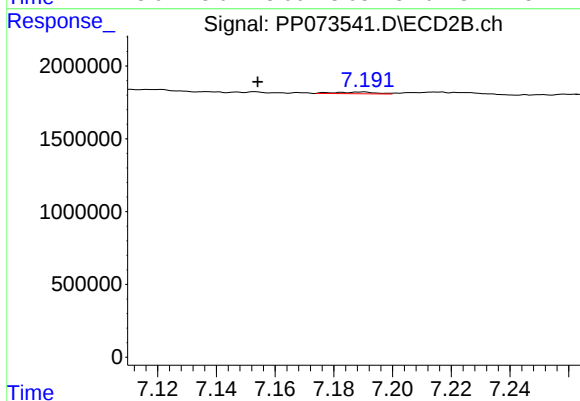

#34 AR-1260-4


R.T.: 7.190 min
Delta R.T.: 0.036 min
Response: 112493
Conc: 1.30 ng/ml

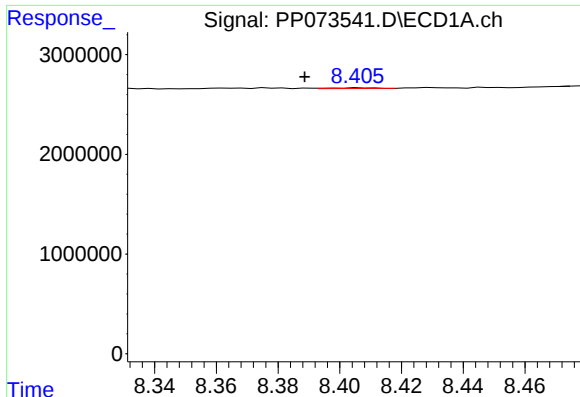

#35 AR-1260-5


R.T.: 8.406 min
Delta R.T.: 0.018 min
Response: 72558
Conc: 0.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

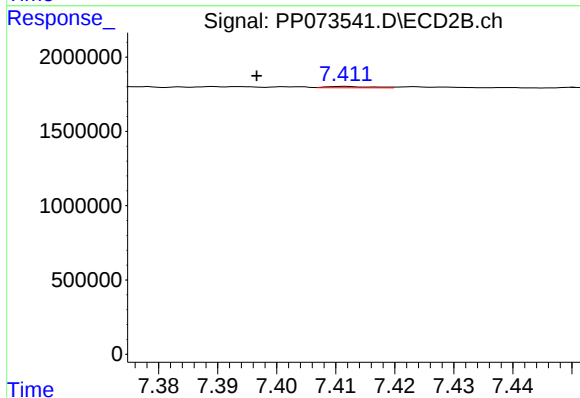


#35 AR-1260-5

R.T.: 7.411 min
Delta R.T.: 0.015 min
Response: 47490
Conc: 0.22 ng/ml

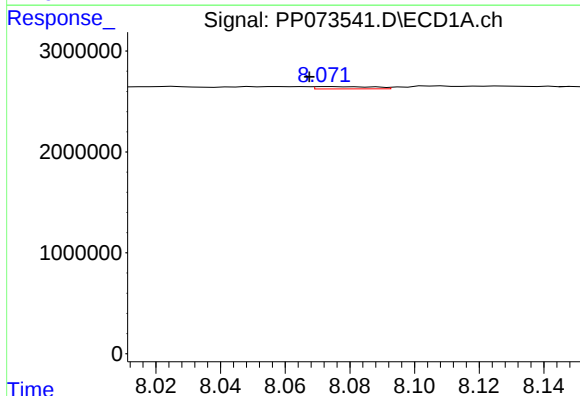


#36 AR-1262-1

R.T.: 8.073 min
Delta R.T.: 0.006 min
Response: 289290
Conc: 2.51 ng/ml

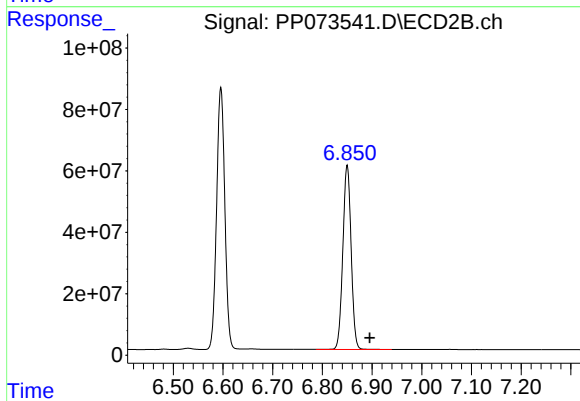

#36 AR-1262-1


R.T.: 6.850 min
Delta R.T.: -0.046 min
Response: 694860070
Conc: 4630.77 ng/ml

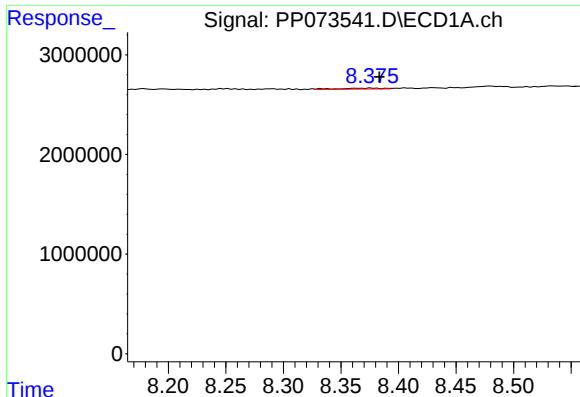

#37 AR-1262-2


R.T.: 8.363 min
Delta R.T.: -0.021 min
Response: 251585
Conc: 1.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

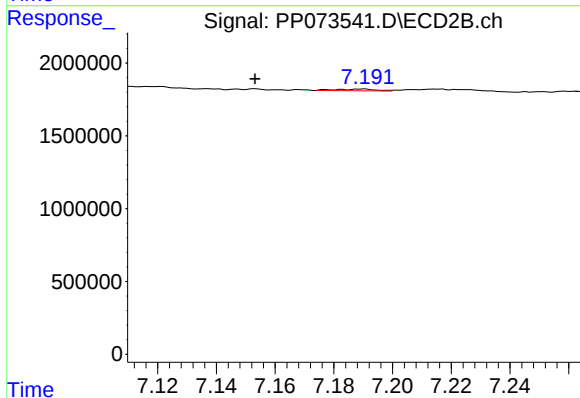


#37 AR-1262-2

R.T.: 7.190 min
Delta R.T.: 0.037 min
Response: 112493
Conc: 0.90 ng/ml

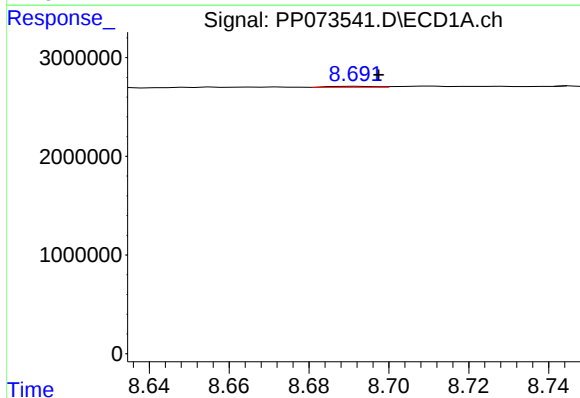


#38 AR-1262-3

R.T.: 8.692 min
Delta R.T.: -0.005 min
Response: 70332
Conc: 0.43 ng/ml

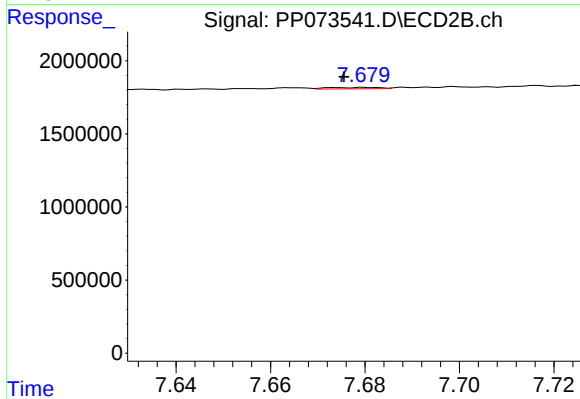

#38 AR-1262-3


R.T.: 7.680 min
Delta R.T.: 0.005 min
Response: 73496
Conc: 0.66 ng/ml

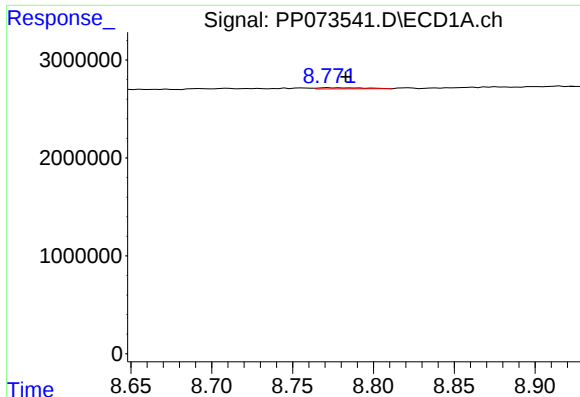

#39 AR-1262-4


R.T.: 8.773 min
Delta R.T.: -0.010 min
Response: 235456
Conc: 1.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

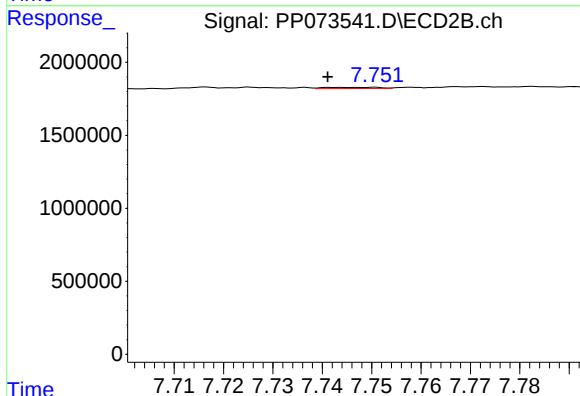


#39 AR-1262-4

R.T.: 7.750 min
Delta R.T.: 0.009 min
Response: 63335
Conc: 0.35 ng/ml

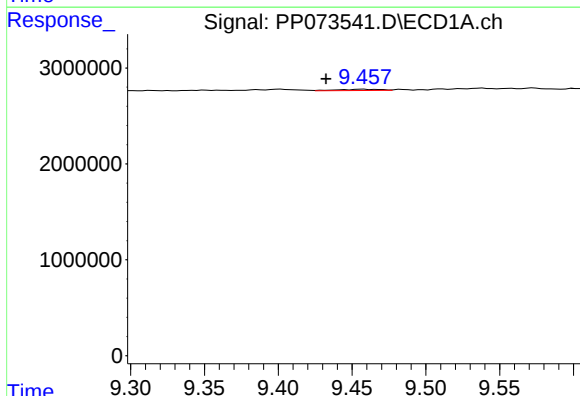


#40 AR-1262-5

R.T.: 9.458 min
Delta R.T.: 0.025 min
Response: 259789
Conc: 2.99 ng/ml

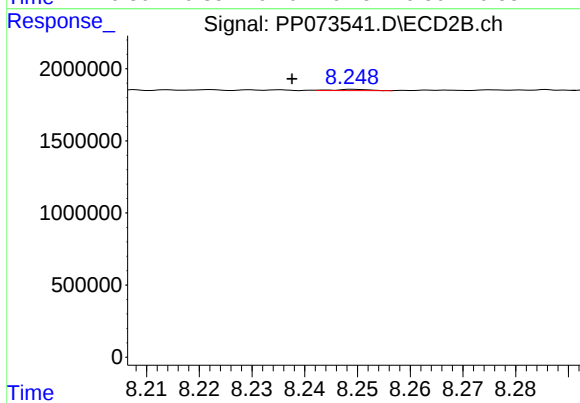

#40 AR-1262-5


R.T.: 8.250 min
Delta R.T.: 0.012 min
Response: 36319
Conc: 0.42 ng/ml

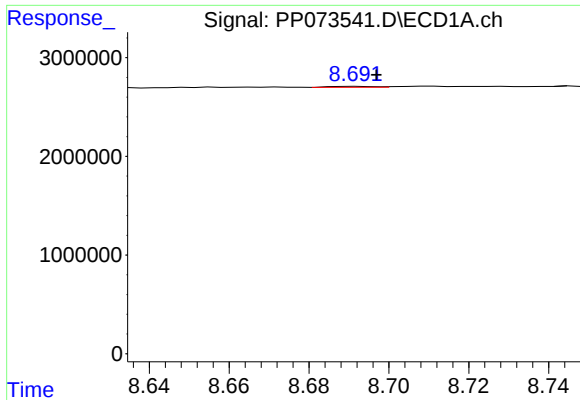

#41 AR-1268-1


R.T.: 8.692 min
Delta R.T.: -0.004 min
Response: 70332
Conc: 0.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

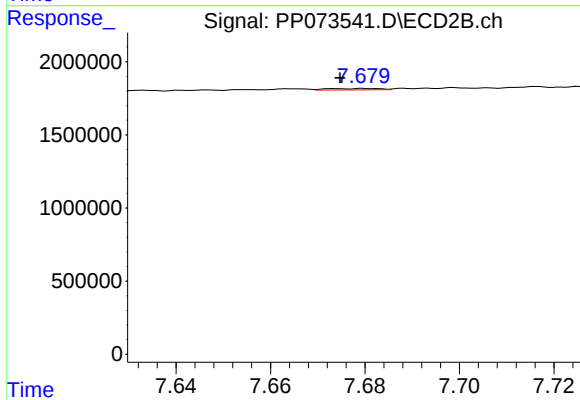


#41 AR-1268-1

R.T.: 7.680 min
Delta R.T.: 0.005 min
Response: 73496
Conc: 0.25 ng/ml

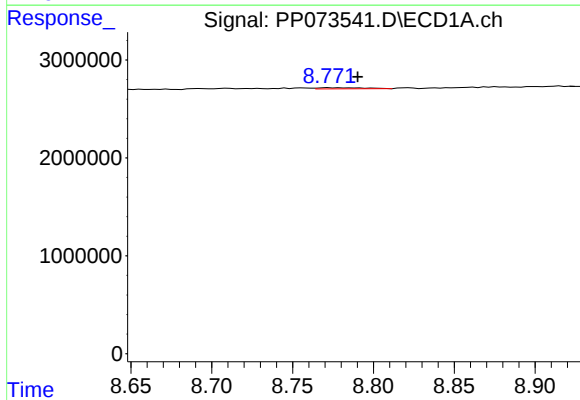


#42 AR-1268-2

R.T.: 8.773 min
Delta R.T.: -0.017 min
Response: 235456
Conc: 0.94 ng/ml

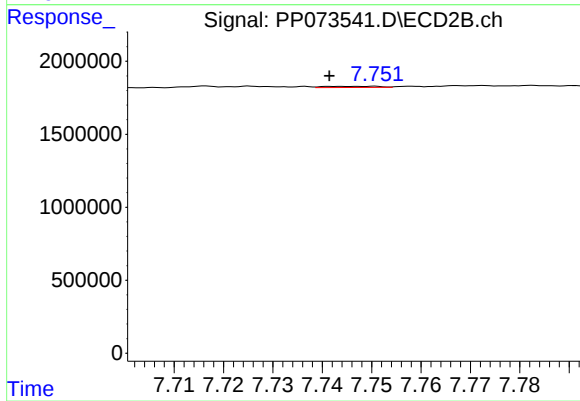

#42 AR-1268-2


R.T.: 7.750 min
Delta R.T.: 0.008 min
Response: 63335
Conc: 0.24 ng/ml

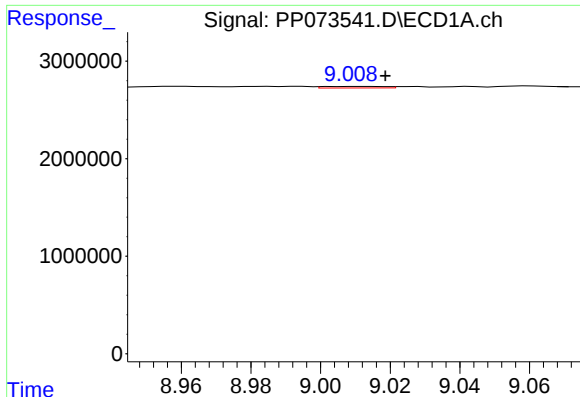

#43 AR-1268-3


R.T.: 9.010 min
Delta R.T.: -0.009 min
Response: 201964
Conc: 0.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

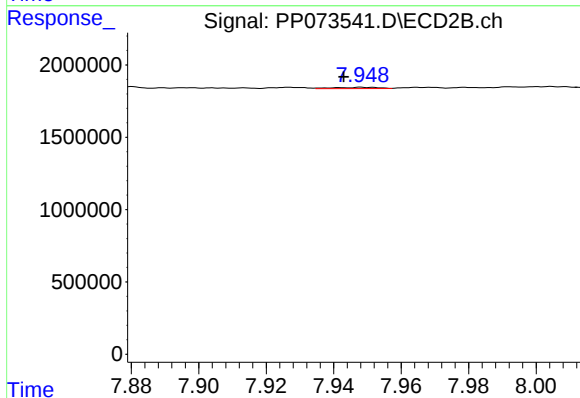


#43 AR-1268-3

R.T.: 7.949 min
Delta R.T.: 0.006 min
Response: 82588
Conc: 0.38 ng/ml

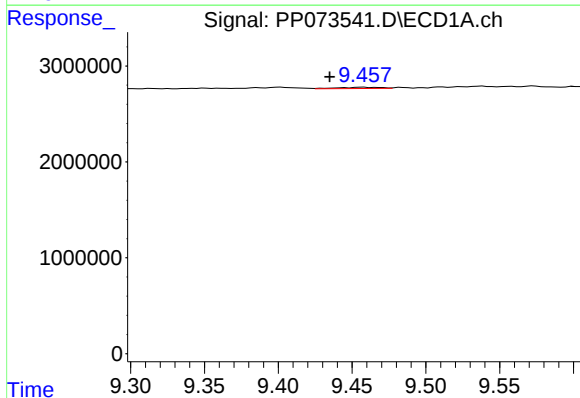


#44 AR-1268-4

R.T.: 9.458 min
Delta R.T.: 0.023 min
Response: 259789
Conc: 2.71 ng/ml

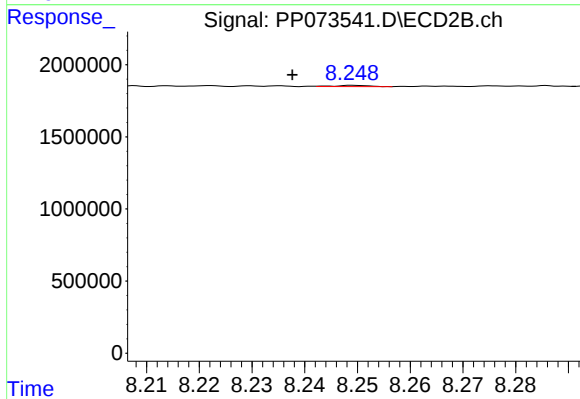

#44 AR-1268-4


R.T.: 8.250 min
Delta R.T.: 0.012 min
Response: 36319
Conc: 0.38 ng/ml

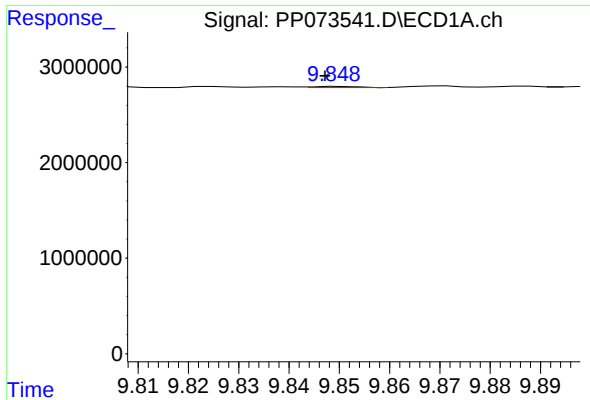

#45 AR-1268-5

R.T.: 9.850 min
Delta R.T.: 0.003 min
Response: 68673
Conc: 0.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

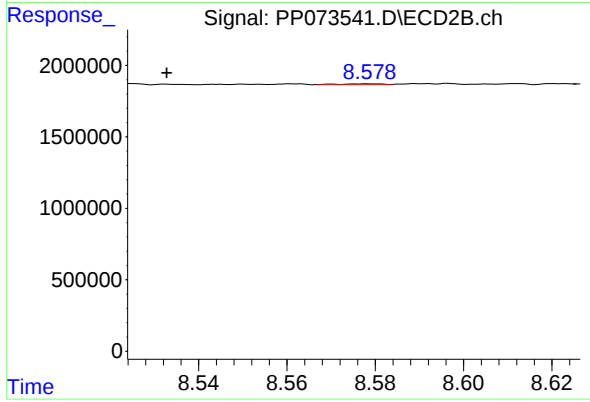

#45 AR-1268-5

R.T.: 8.579 min
Delta R.T.: 0.046 min
Response: 42773
Conc: 0.07 ng/ml