

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070821\
 Data File : PP037124.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jul 2021 18:29
 Operator : DD\AJ
 Sample : M2965-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RO-ETGI-345

Manual Integrations
 APPROVED

mohammad
 7/9/2021 11:42:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 04:06:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.959	3.949	900297	516113	19.809	18.861
2) SA Decachlor...	10.989	9.243	1058200	570411	22.987	20.493
Target Compounds						
31) L7 AR-1260-1	7.966	6.787	53760	34777	24.421m	25.168m
32) L7 AR-1260-2	8.230	6.988	81823	59306	29.414m	35.303m
33) L7 AR-1260-3	8.596	7.140	52263	47222	25.858m	27.560
34) L7 AR-1260-4	8.827	7.624	108859	37210	44.255m	27.370 #
35) L7 AR-1260-5	9.156	7.872	163833	94511	35.505	29.302m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070821\
Data File : PP037124.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jul 2021 18:29
Operator : DD\AJ
Sample : M2965-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
RO-ETGI-345


Manual Integrations
APPROVED

mohammad
7/9/2021 11:42:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 04:06:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

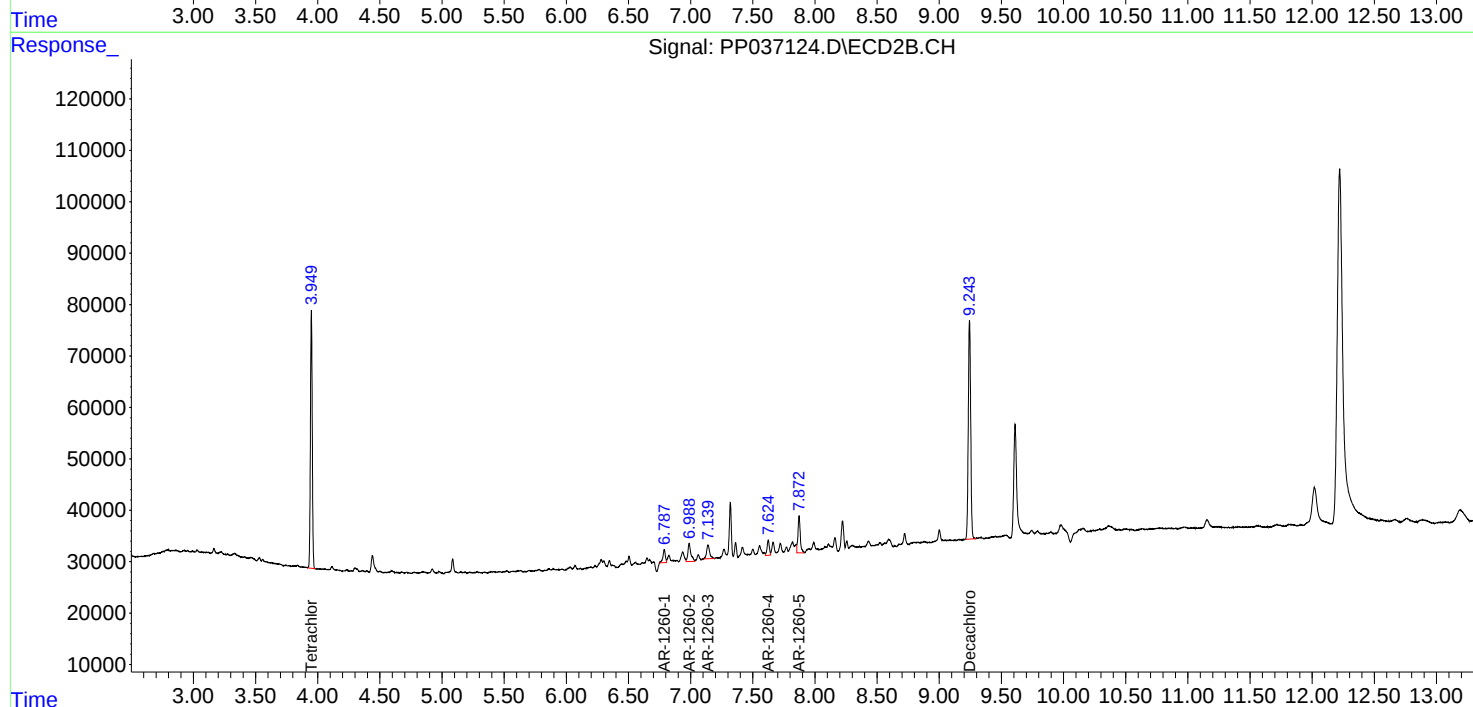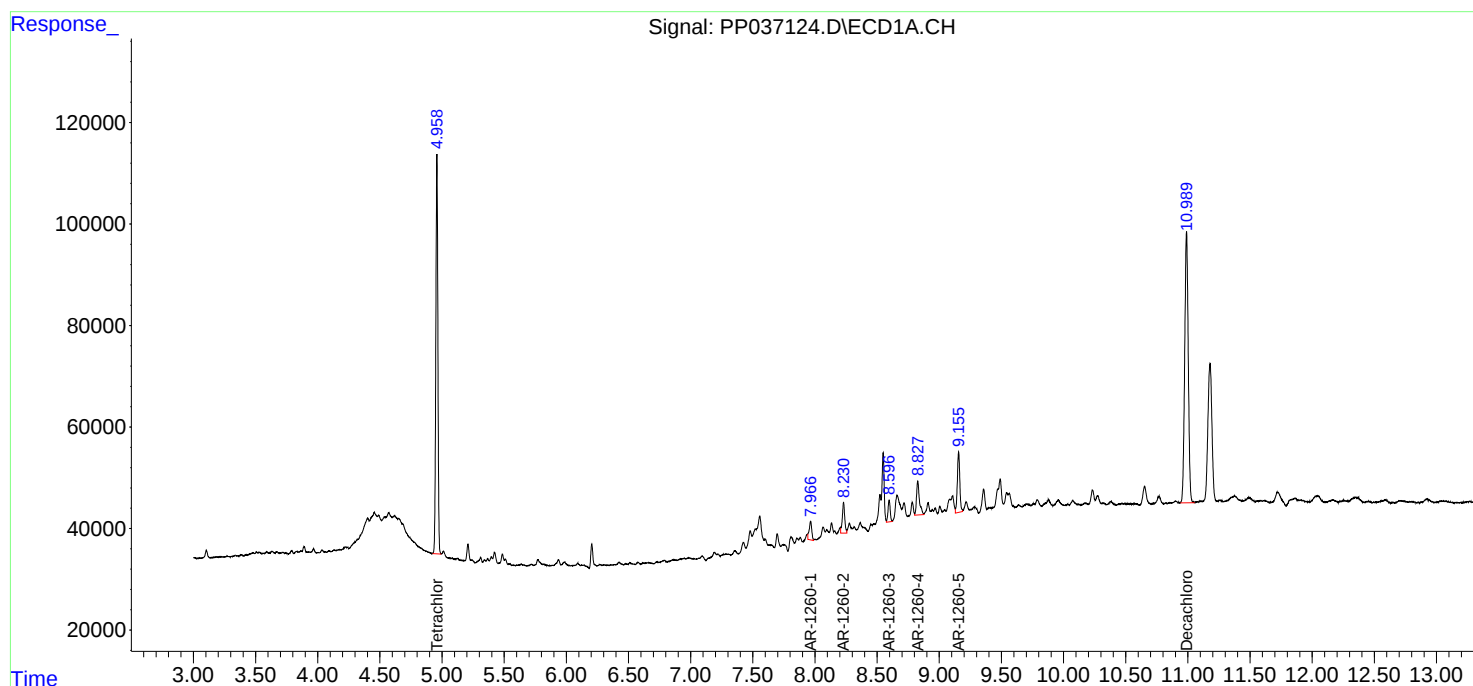

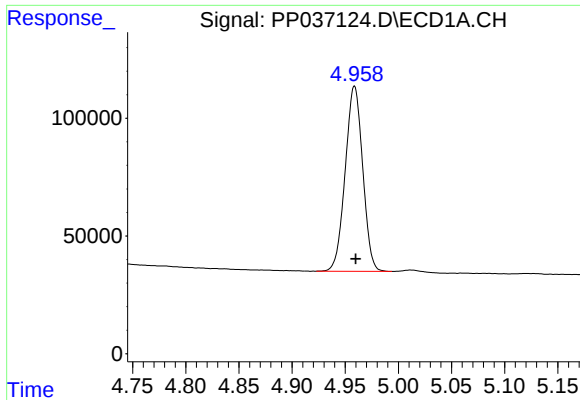


#1 Tetrachloro-m-xylene

R.T.: 4.959 min
Delta R.T.: -0.001 min
Response: 900297
Conc: 19.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-ETGI-345


Manual Integrations
APPROVED

mohammad
7/9/2021 11:42:11 AM

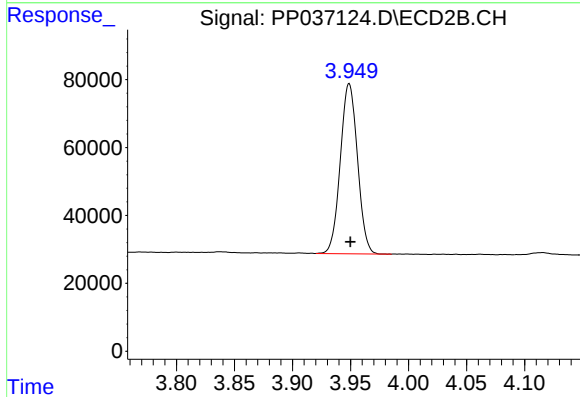


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 516113
Conc: 18.86 ng/ml

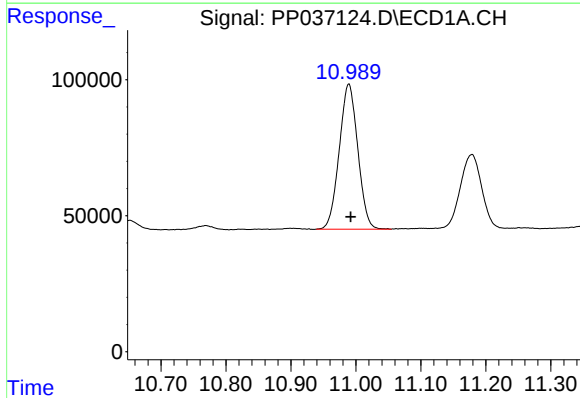


#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.003 min
Response: 1058200
Conc: 22.99 ng/ml

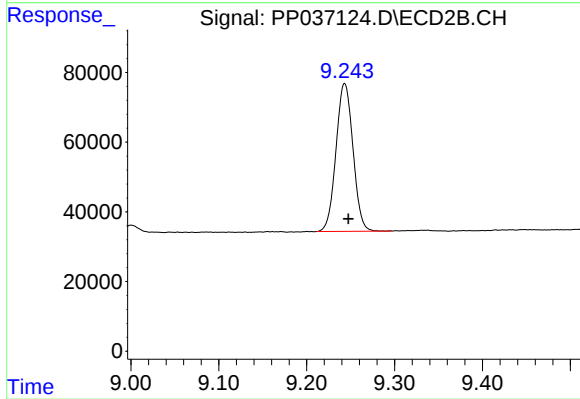

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.004 min
Response: 570411
Conc: 20.49 ng/ml

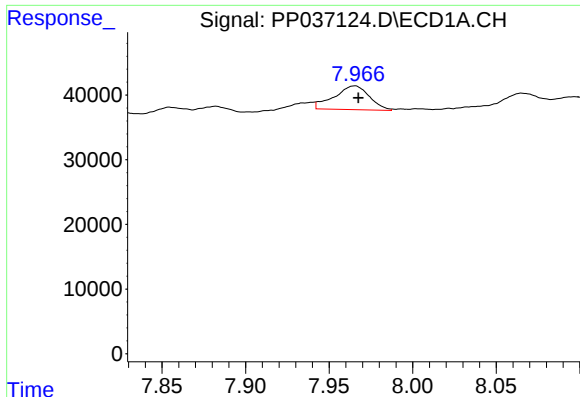


#31 AR-1260-1

R.T.: 7.966 min
Delta R.T.: -0.002 min
Response: 53760
Conc: 24.42 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RO-ETGI-345


Manual Integrations
APPROVED

mohammad
7/9/2021 11:42:11 AM

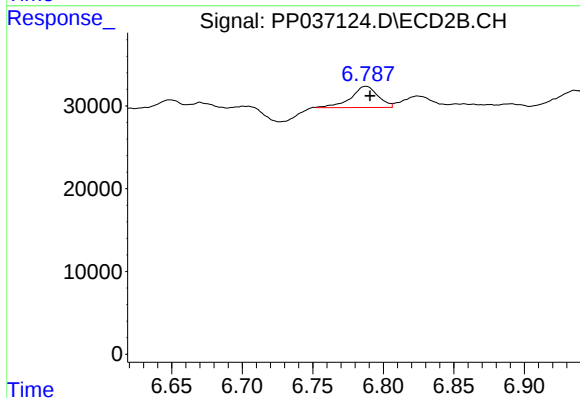


#31 AR-1260-1

R.T.: 6.787 min
Delta R.T.: -0.003 min
Response: 34777
Conc: 25.17 ng/ml m

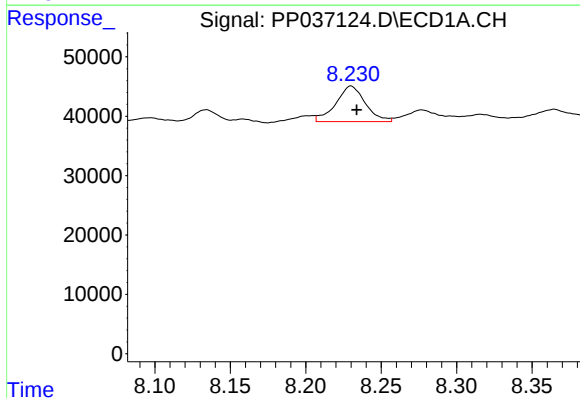


#32 AR-1260-2

R.T.: 8.230 min
Delta R.T.: -0.004 min
Response: 81823
Conc: 29.41 ng/ml m

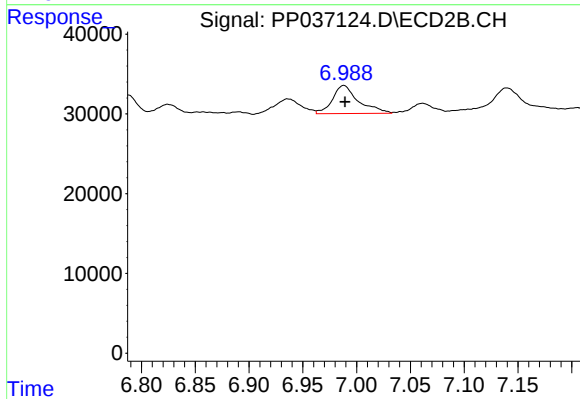

#32 AR-1260-2

R.T.: 6.988 min
Delta R.T.: -0.001 min
Response: 59306
Conc: 35.30 ng/ml m

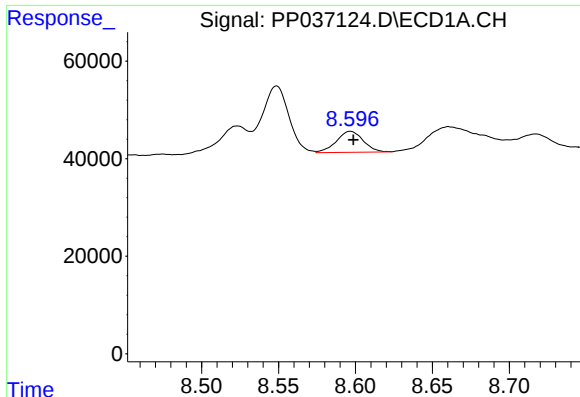


#33 AR-1260-3

R.T.: 8.596 min
Delta R.T.: -0.002 min
Response: 52263
Conc: 25.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RO-ETGI-345


Manual Integrations
APPROVED

mohammad
7/9/2021 11:42:11 AM

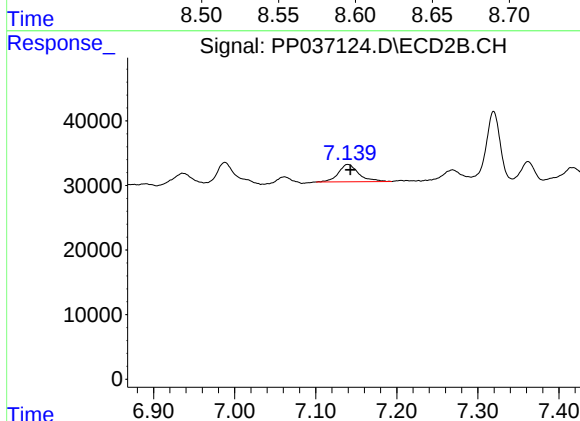


#33 AR-1260-3

R.T.: 7.140 min
Delta R.T.: -0.003 min
Response: 47222
Conc: 27.56 ng/ml

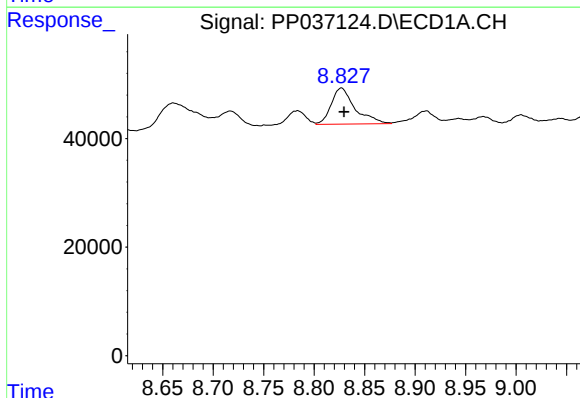


#34 AR-1260-4

R.T.: 8.827 min
Delta R.T.: -0.003 min
Response: 108859
Conc: 44.26 ng/ml m

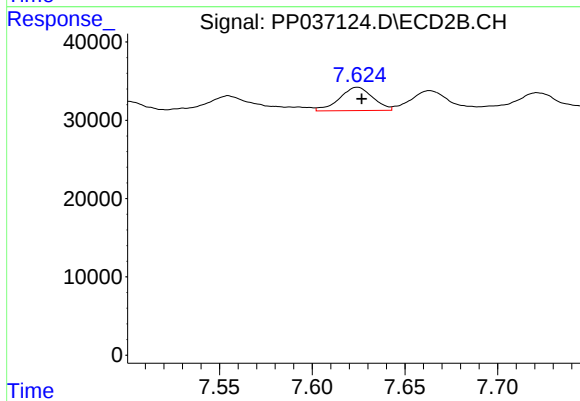

#34 AR-1260-4

R.T.: 7.624 min
Delta R.T.: -0.002 min
Response: 37210
Conc: 27.37 ng/ml

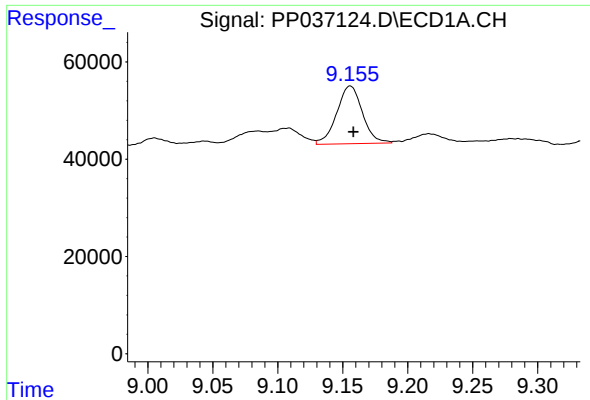


#35 AR-1260-5

R.T.: 9.156 min
Delta R.T.: -0.002 min
Response: 163833
Conc: 35.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-ETGI-345

Manual Integrations
APPROVED

mohammad
7/9/2021 11:42:11 AM

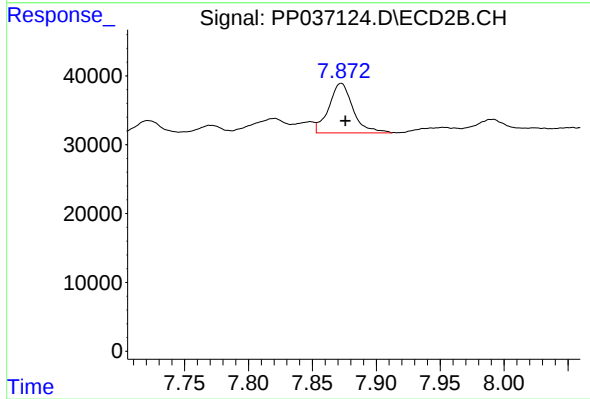

#35 AR-1260-5

R.T.: 7.872 min
Delta R.T.: -0.003 min
Response: 94511
Conc: 29.30 ng/ml m