

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070921\
 Data File : PP037153.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2021 9:22
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 15:20:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	0.000	6.094f	0	13239	N.D. 19.450 #
24)	L5	AR-1248-4	7.199f	0.000	23196	0	12.272 N.D. #
25)	L5	AR-1248-5	0.000	6.094f	0	13239	N.D. 12.481 #
26)	L6	AR-1254-1	7.199	6.094f	23196	13239	12.912 8.918 #
28)	L6	AR-1254-3	7.820f	0.000	14699	0	4.768 N.D. #
32)	L7	AR-1260-2	8.207f	0.000	16699	0	6.003 N.D. #
40)	L8	AR-1262-5	10.227	0.000	5468	0	2.572 N.D. #
43)	L9	AR-1268-3	9.785	0.000	14871	0	3.033 N.D. #
44)	L9	AR-1268-4	10.227	0.000	5468	0	2.390 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070921\
Data File : PP037153.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2021 9:22
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 15:20:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

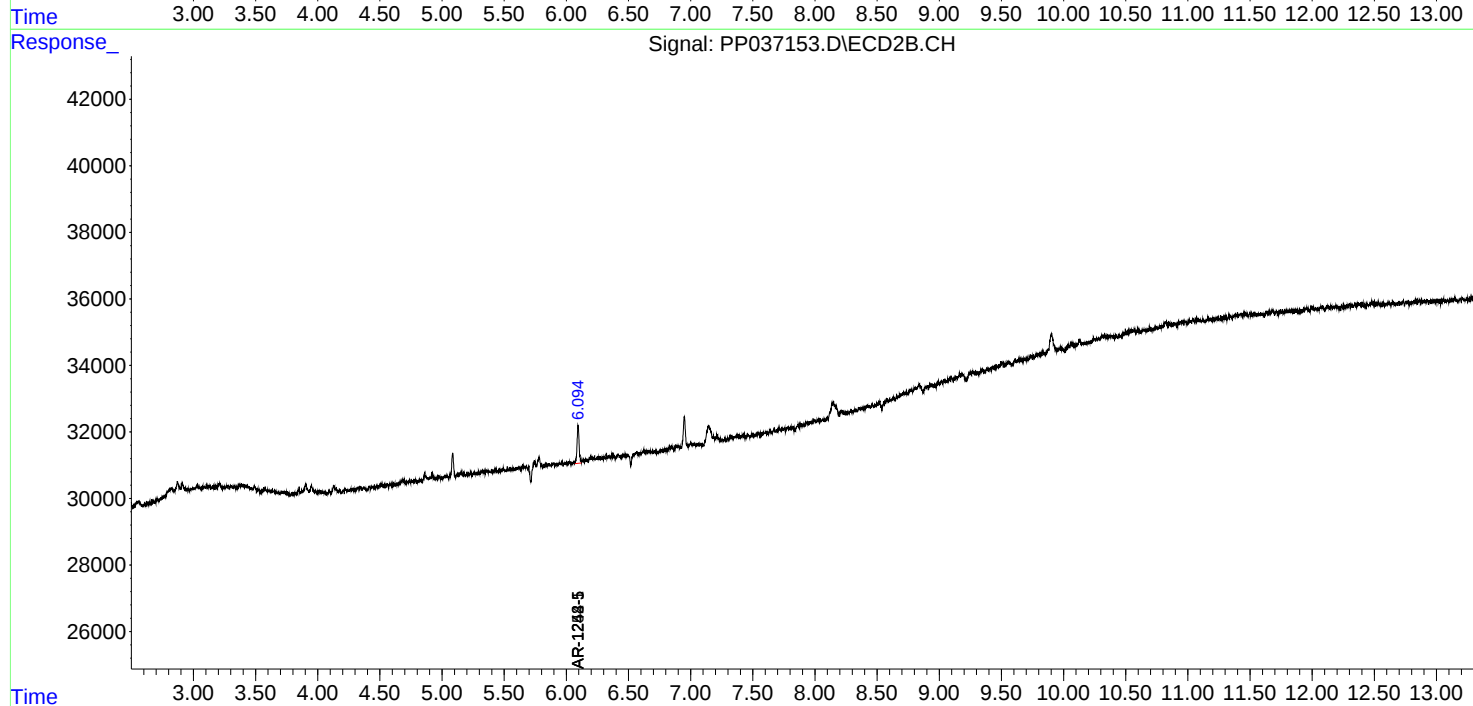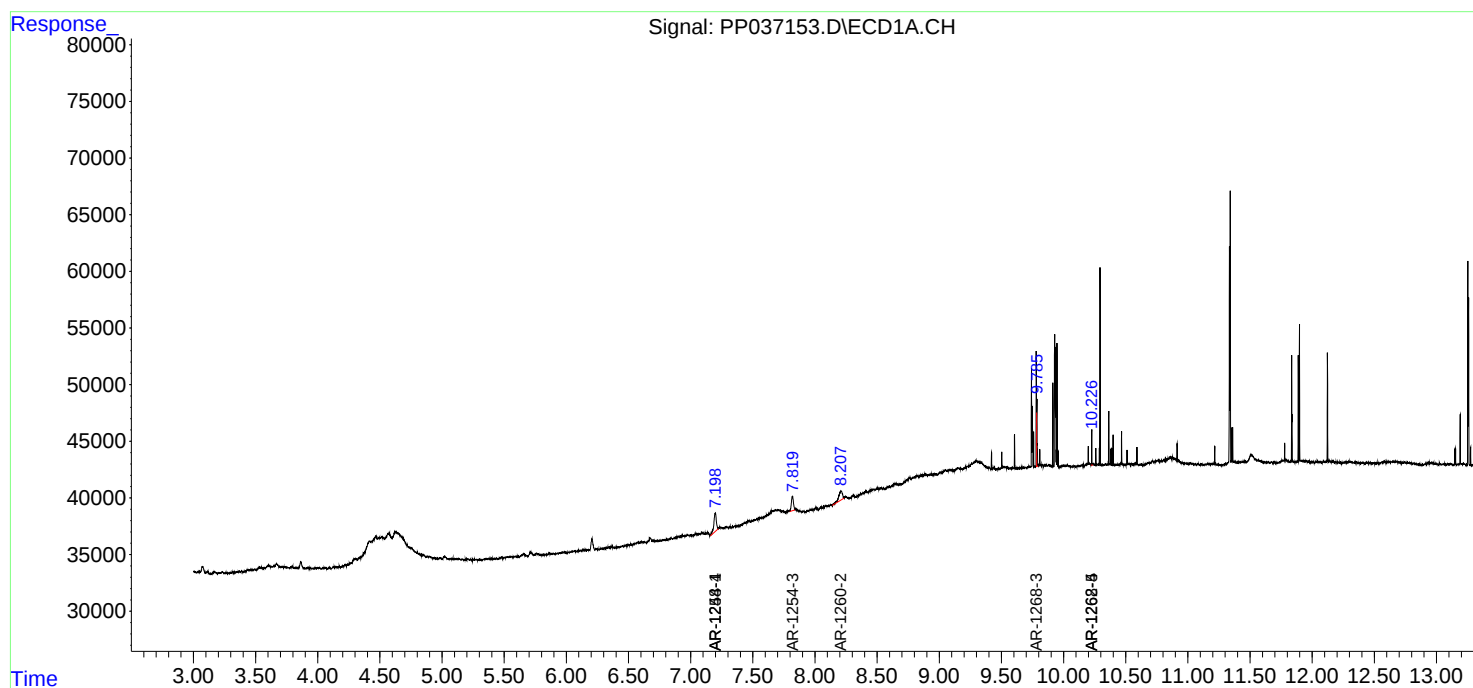


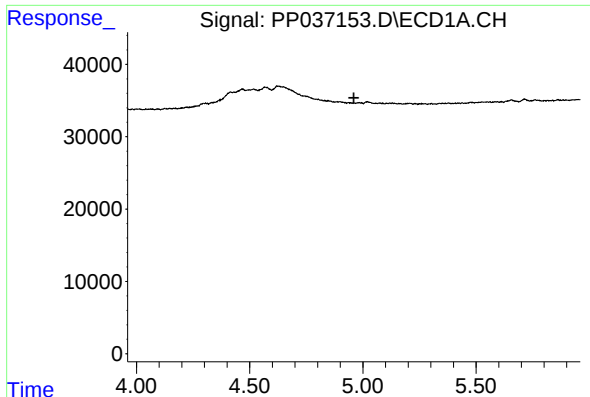

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

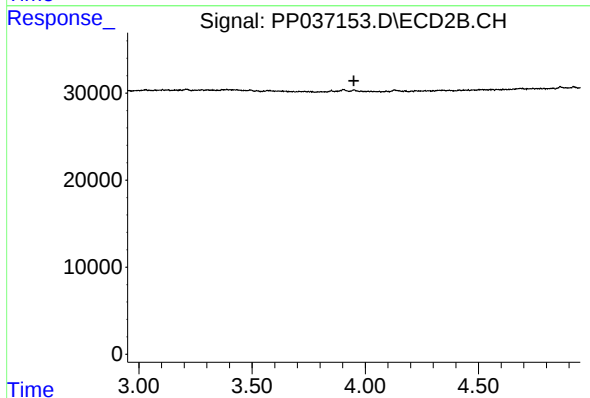


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.950 min
Response: 0
Conc: N.D.

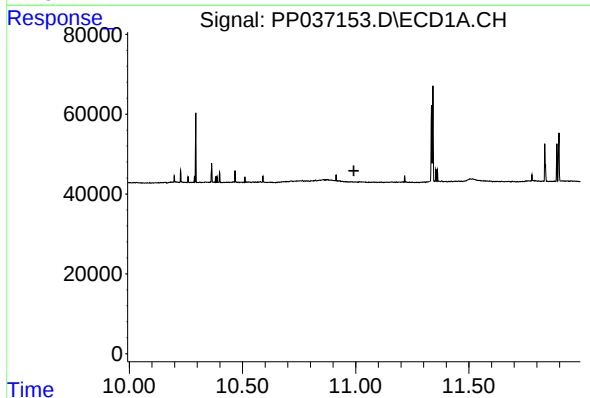


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.

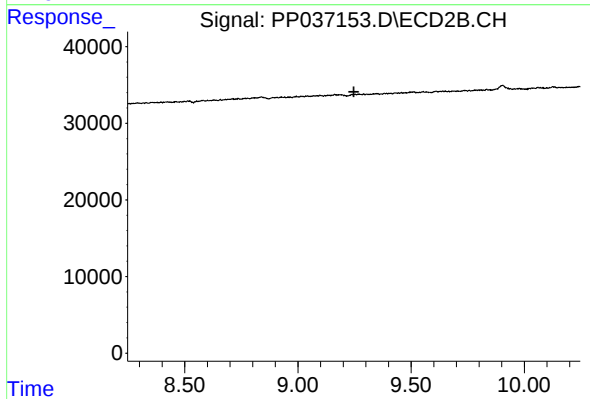

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.247 min
Response: 0
Conc: N.D.

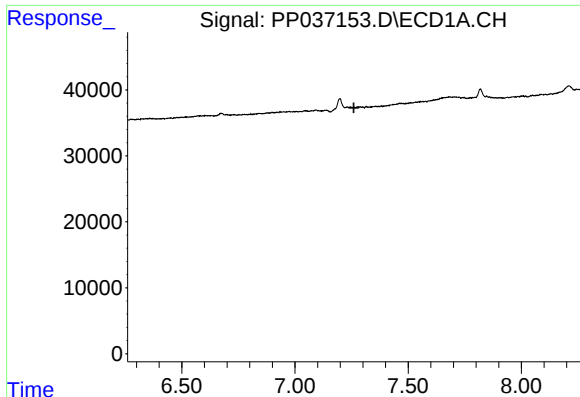

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

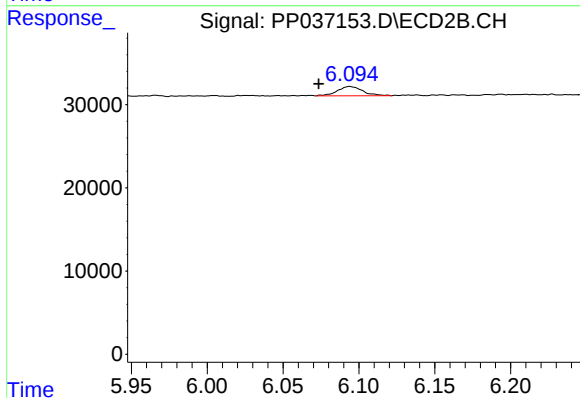


#20 AR-1242-5

R.T.: 6.094 min
Delta R.T.: 0.020 min
Response: 13239
Conc: 19.45 ng/ml

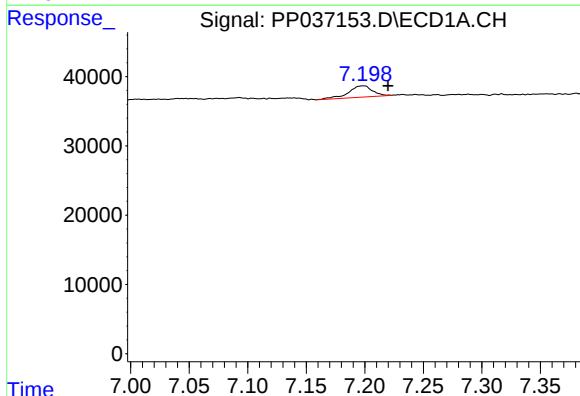


#24 AR-1248-4

R.T.: 7.199 min
Delta R.T.: -0.021 min
Response: 23196
Conc: 12.27 ng/ml

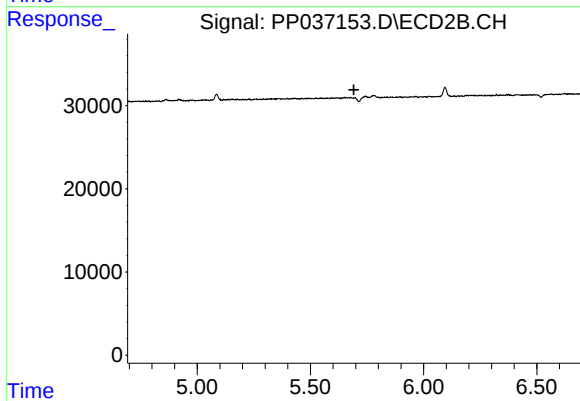

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.692 min
Response: 0
Conc: N.D.

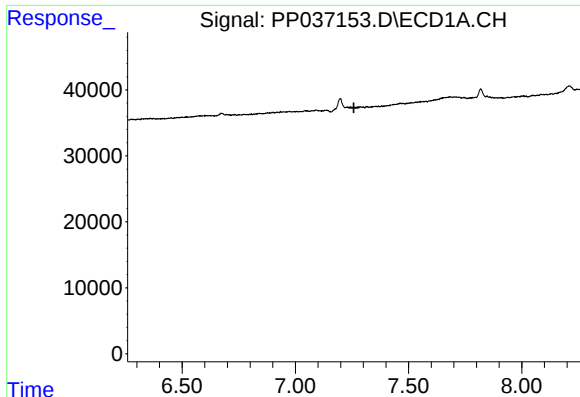

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.259 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

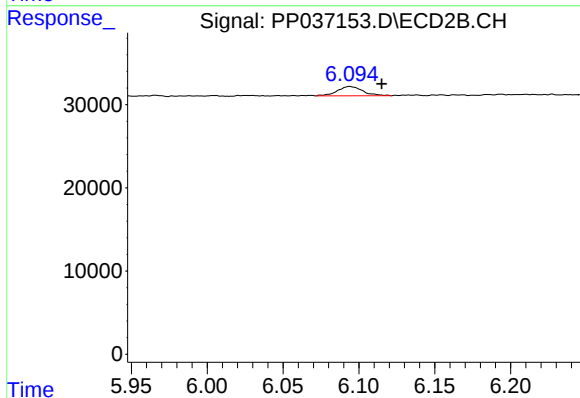


#25 AR-1248-5

R.T.: 6.094 min
Delta R.T.: -0.021 min
Response: 13239
Conc: 12.48 ng/ml

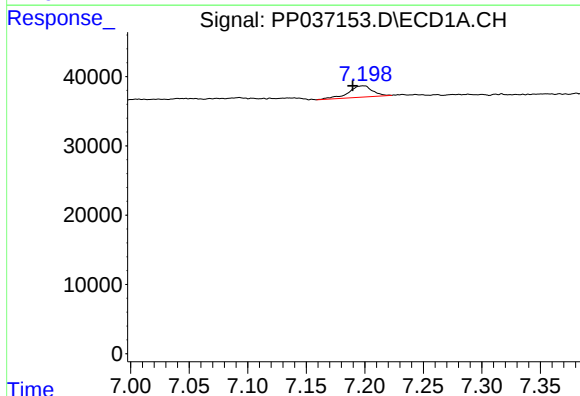


#26 AR-1254-1

R.T.: 7.199 min
Delta R.T.: 0.009 min
Response: 23196
Conc: 12.91 ng/ml

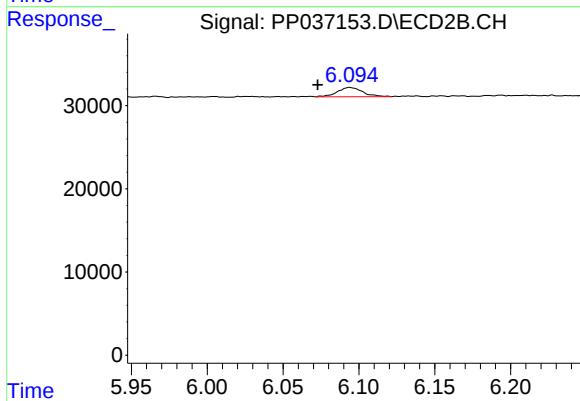

#26 AR-1254-1


R.T.: 6.094 min
Delta R.T.: 0.021 min
Response: 13239
Conc: 8.92 ng/ml

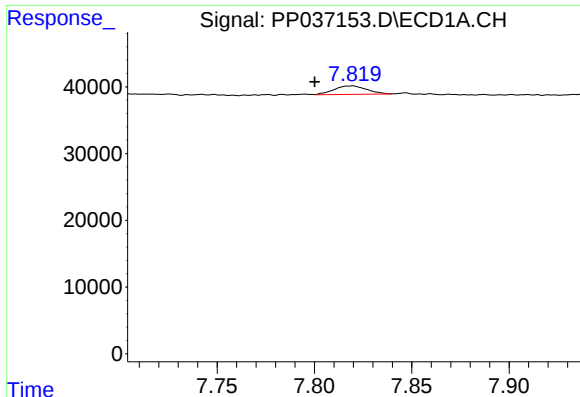

#28 AR-1254-3


R.T.: 7.820 min
Delta R.T.: 0.020 min
Response: 14699
Conc: 4.77 ng/ml

Instrument :
ECD_P
ClientSampleId :

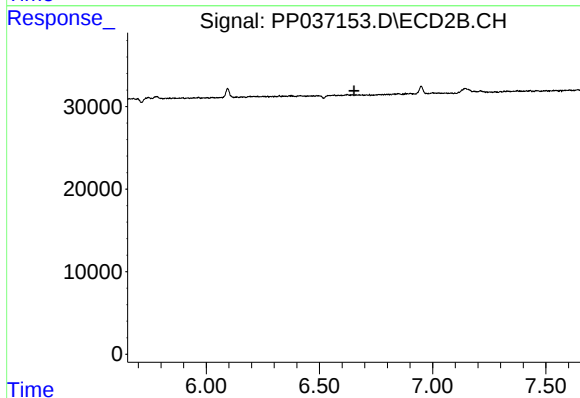


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

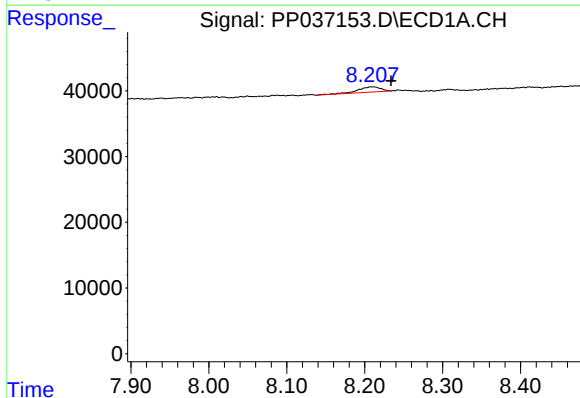


#32 AR-1260-2

R.T.: 8.207 min
Delta R.T.: -0.026 min
Response: 16699
Conc: 6.00 ng/ml

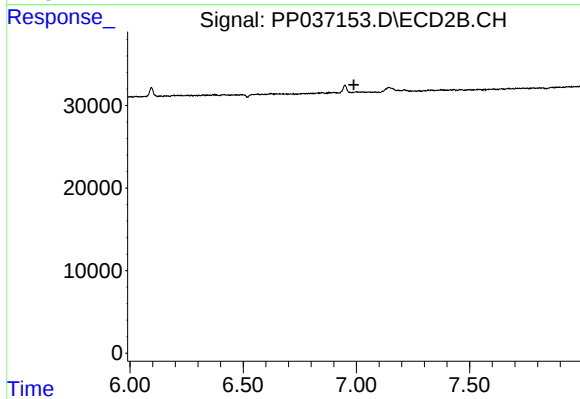

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

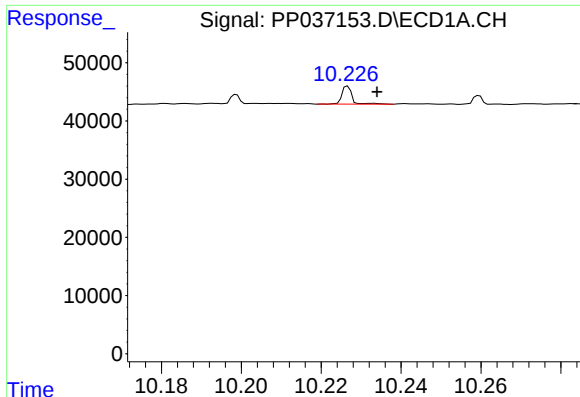

#40 AR-1262-5


R.T.: 10.227 min
Delta R.T.: -0.007 min
Response: 5468
Conc: 2.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

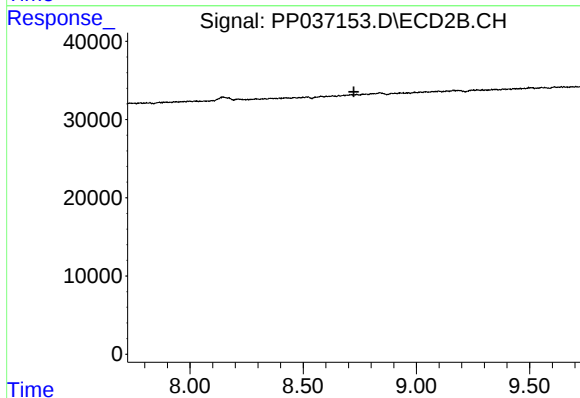


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.724 min
Response: 0
Conc: N.D.

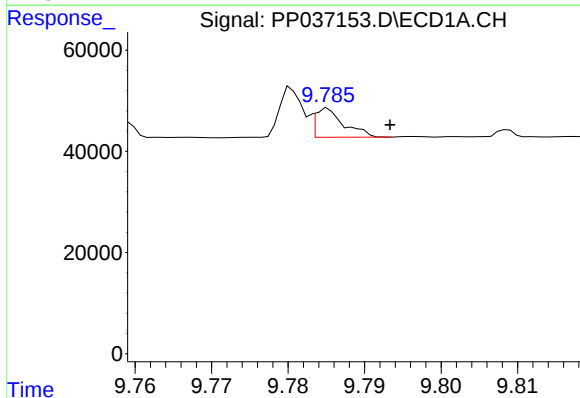


#43 AR-1268-3

R.T.: 9.785 min
Delta R.T.: -0.008 min
Response: 14871
Conc: 3.03 ng/ml

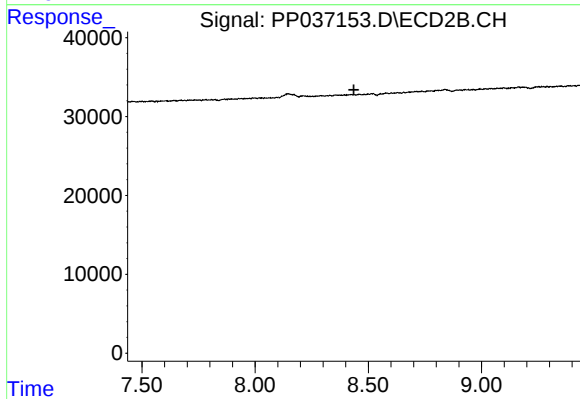

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.436 min
Response: 0
Conc: N.D.

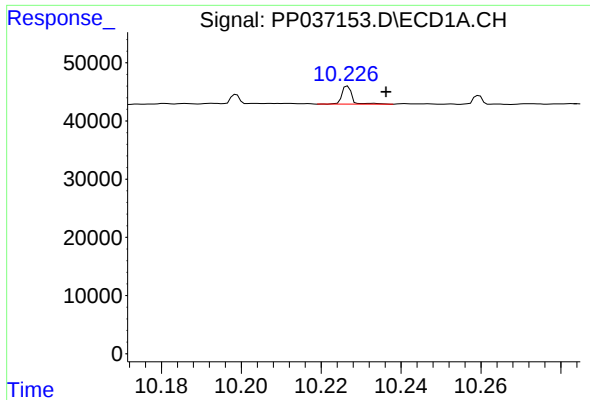

#44 AR-1268-4

R.T.: 10.227 min
Delta R.T.: -0.009 min
Response: 5468
Conc: 2.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

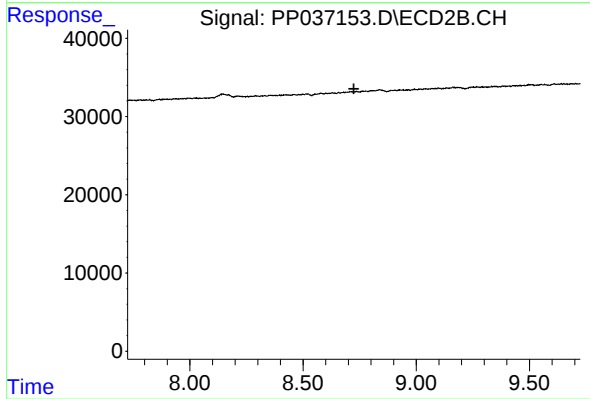

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.725 min
Response: 0
Conc: N.D.