

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070921\
 Data File : PP037164.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2021 13:00
 Operator : DD\AJ
 Sample : M2992-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33263

Manual Integrations
 APPROVED

mohammad
 7/12/2021 12:29:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 17:28:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.957	3.948	782365	452198	17.214m	16.525
2) SA Decachlor...	10.990	9.243	713940	395626	15.508	14.213

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070921\
Data File : PP037164.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2021 13:00
Operator : DD\AJ
Sample : M2992-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
33263


Manual Integrations
APPROVED

mohammad
7/12/2021 12:29:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 17:28:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

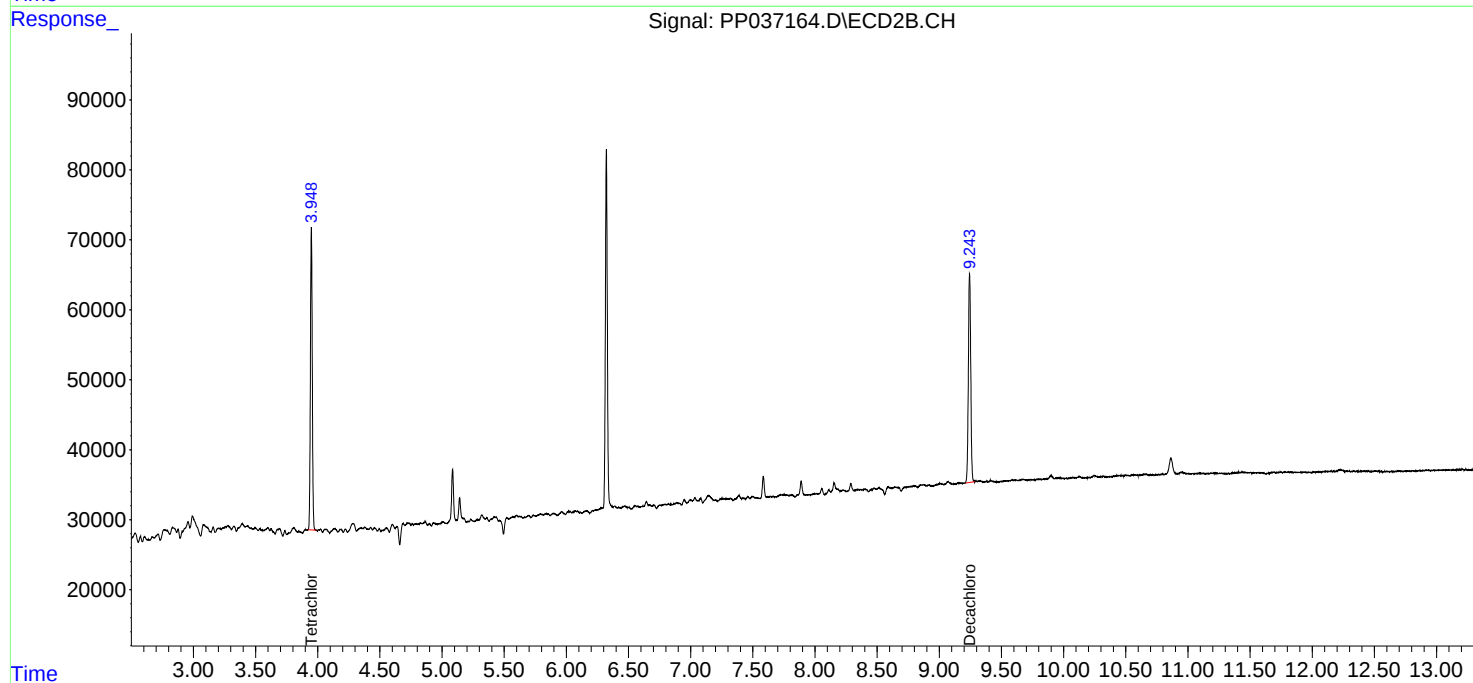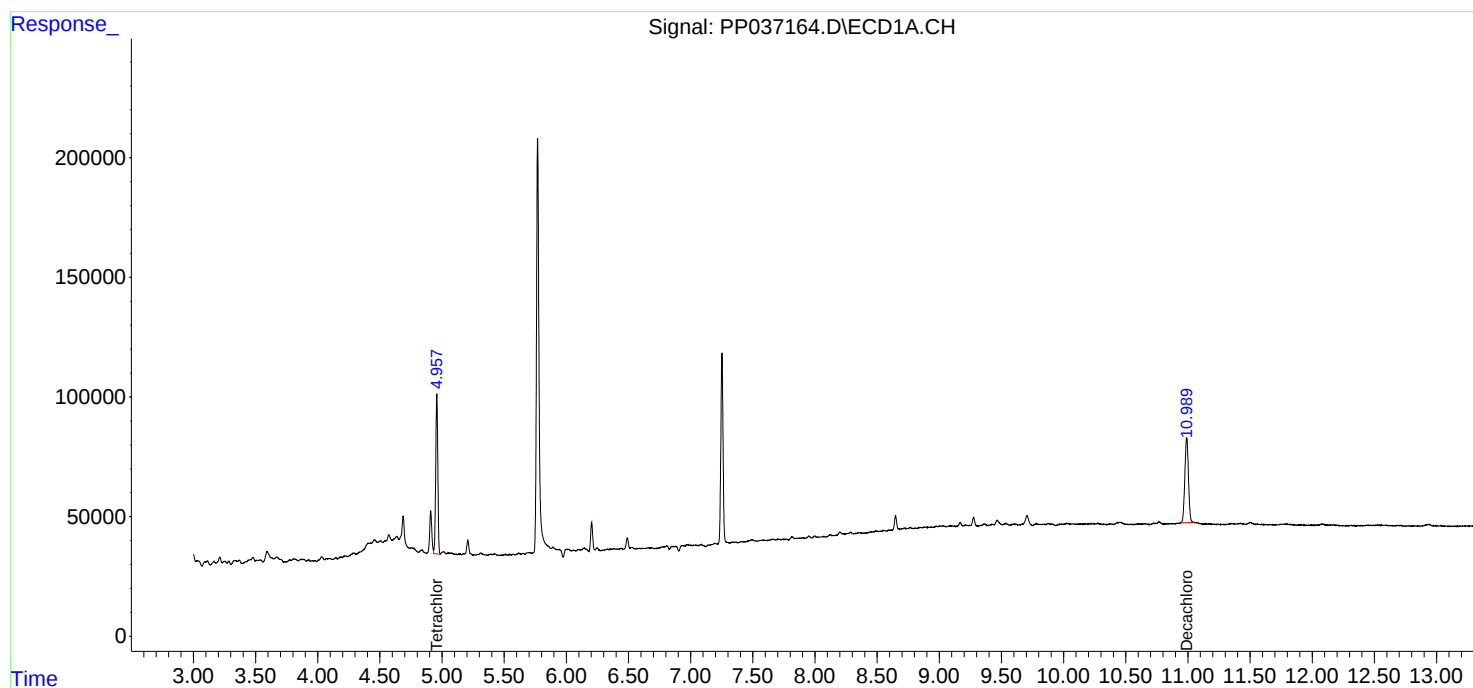

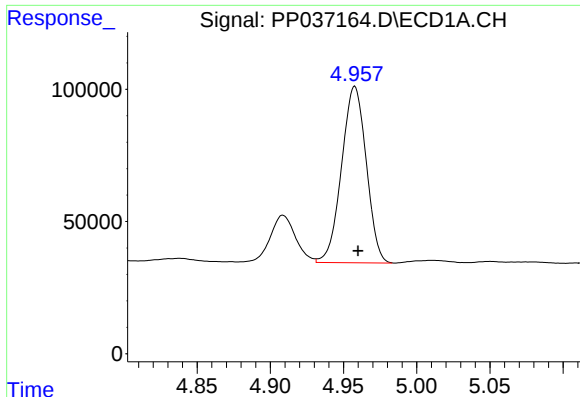


#1 Tetrachloro-m-xylene

R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 782365
Conc: 17.21 ng/ml m

Instrument :
ECD_P
ClientSampleId :
33263


Manual Integrations
APPROVED

mohammad
7/12/2021 12:29:08 PM

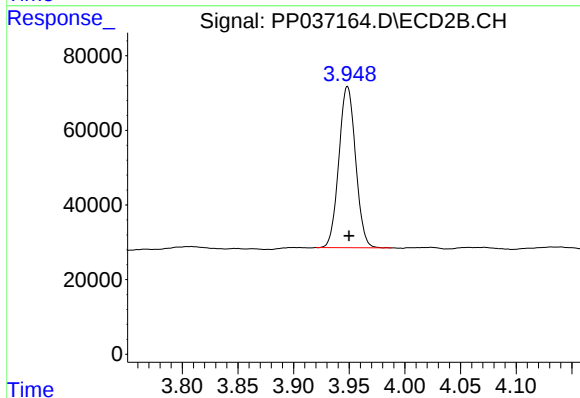


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.001 min
Response: 452198
Conc: 16.53 ng/ml

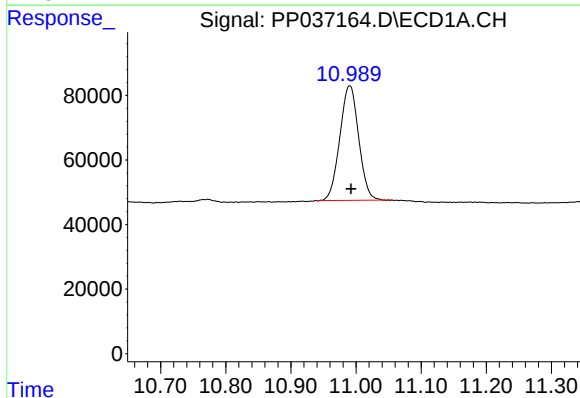

#2 Decachlorobiphenyl

R.T.: 10.990 min
Delta R.T.: -0.002 min
Response: 713940
Conc: 15.51 ng/ml

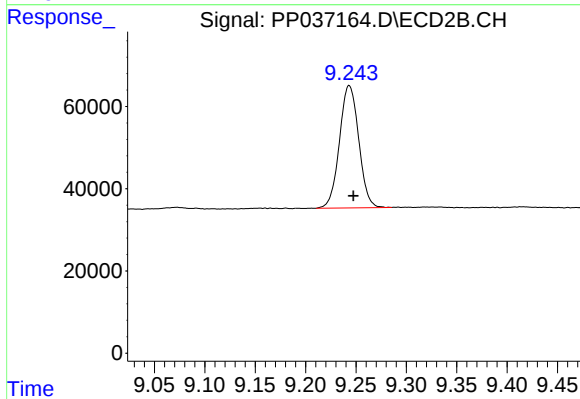

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.004 min
Response: 395626
Conc: 14.21 ng/ml