

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070924\
 Data File : PP066205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2024 13:42
 Operator : YP\AJ
 Sample : PB161963BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB161963BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/10/2024
 Supervised By :Ankita Jodhani 07/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 15:06:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 06:34:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.778	4.016	39814238	45777679	22.618	19.786m
2) SA Decachlor...	10.777	9.189	45256592	28664548	25.034	25.198

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070924\
Data File : PP066205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2024 13:42
Operator : YP\AJ
Sample : PB161963BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB161963BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/10/2024
Supervised By :Ankita Jodhani 07/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 15:06:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 06:34:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

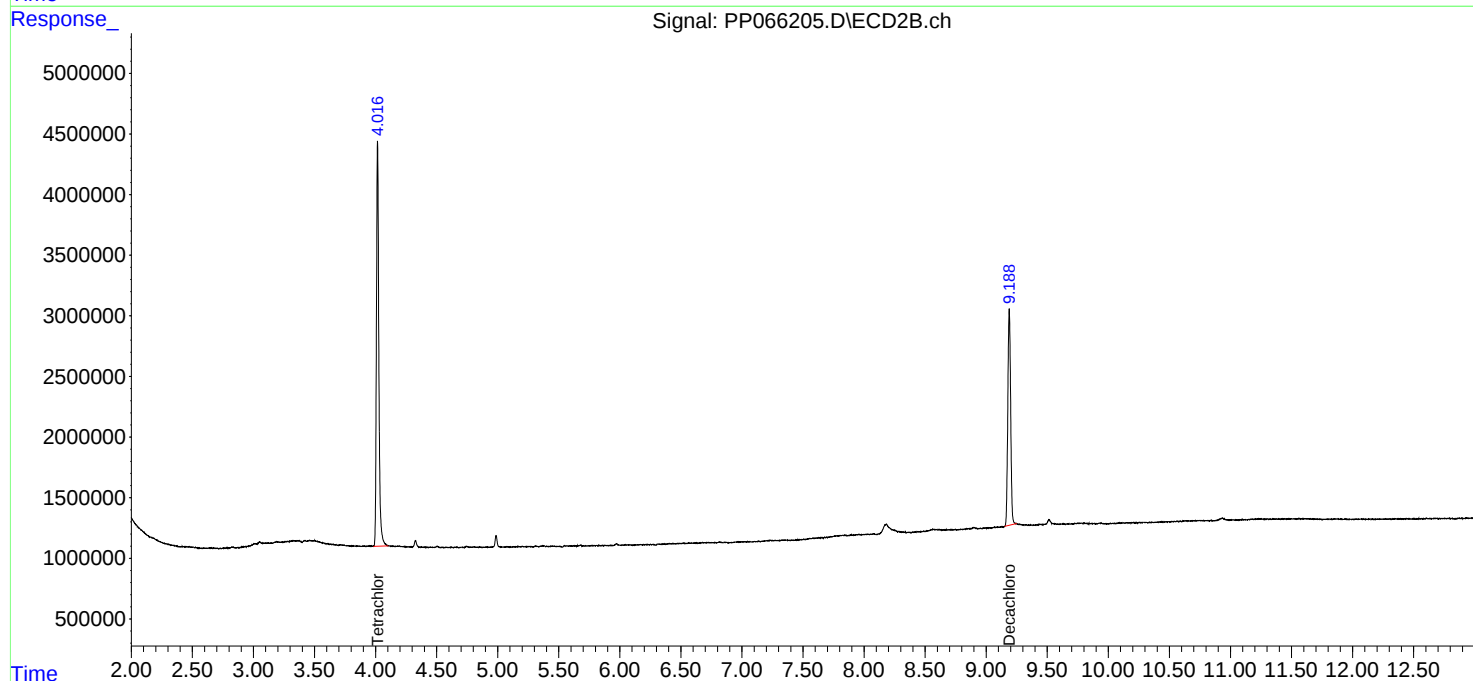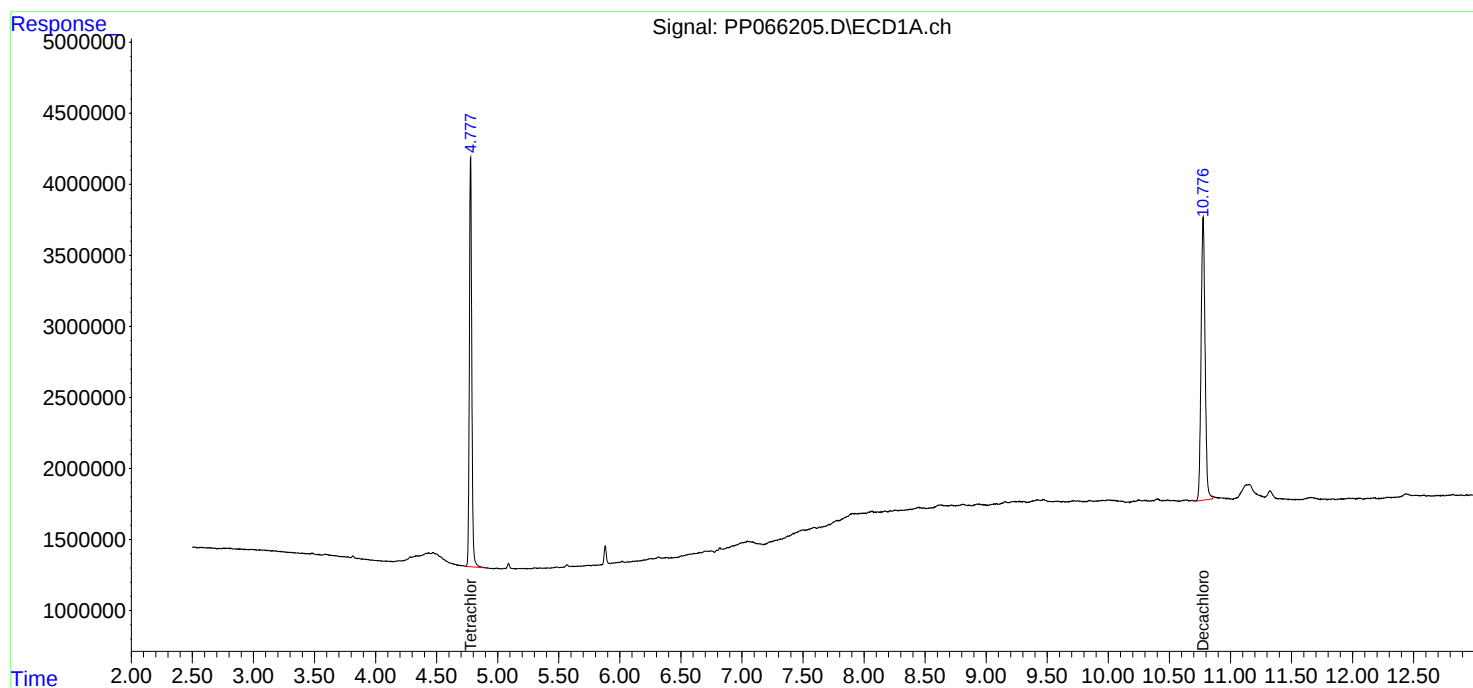

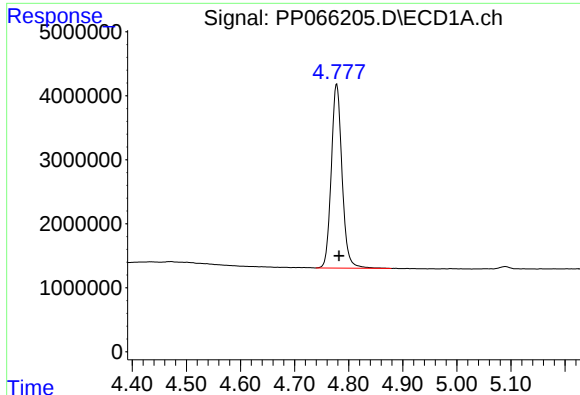

#1 Tetrachloro-m-xylene

R.T.: 4.778 min
Delta R.T.: -0.004 min
Response: 39814238
Conc: 22.62 ng/ml

Instrument :

ECD_P


ClientSampleId :

PB161963BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/10/2024
Supervised By :Ankita Jodhani 07/10/2024

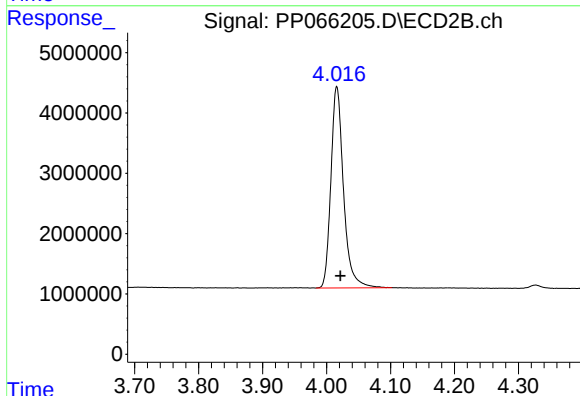


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: -0.006 min
Response: 45777679
Conc: 19.79 ng/ml m

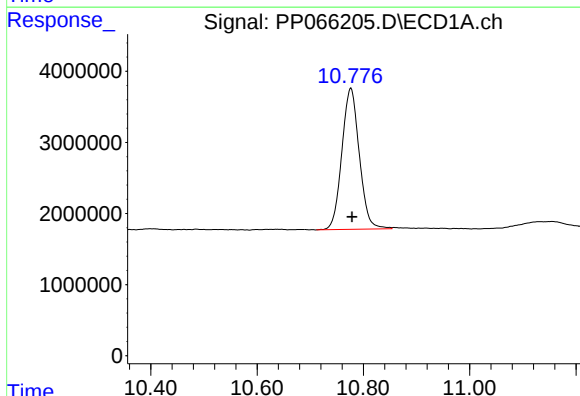

#2 Decachlorobiphenyl

R.T.: 10.777 min
Delta R.T.: -0.002 min
Response: 45256592
Conc: 25.03 ng/ml

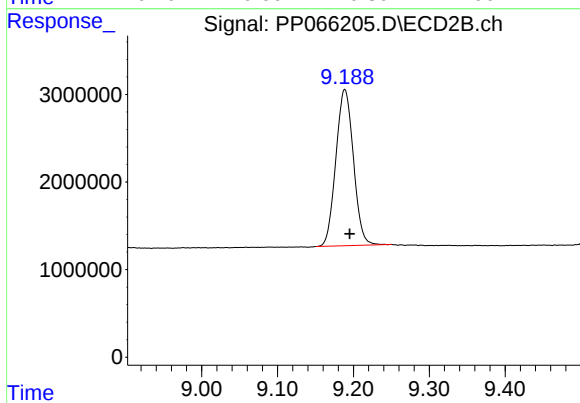

#2 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: -0.006 min
Response: 28664548
Conc: 25.20 ng/ml