

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070925\
Data File : PP073595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2025 10:45
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 11:43:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30)	L6	AR-1254-5	7.781	6.849	473.8E6	752.1E6 6429.977 5635.849



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070925\
Data File : PP073595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2025 10:45
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 11:43:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

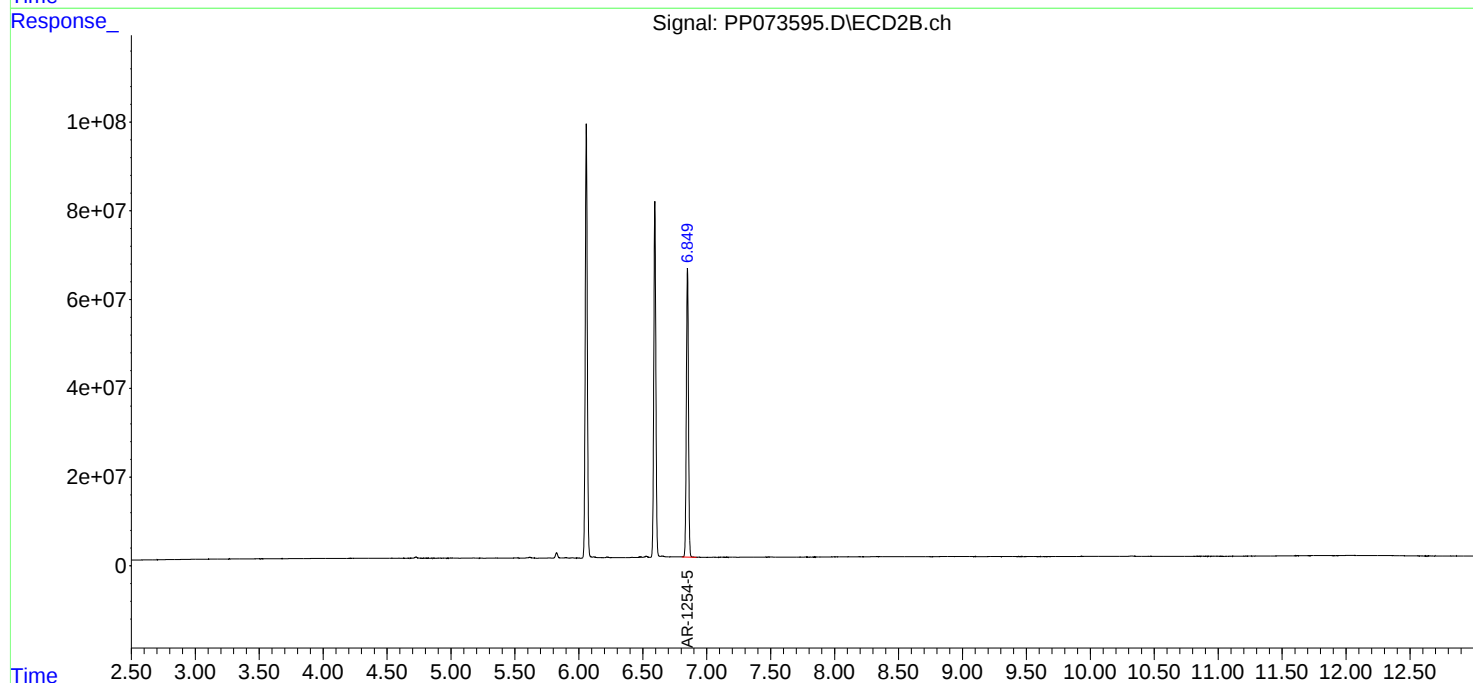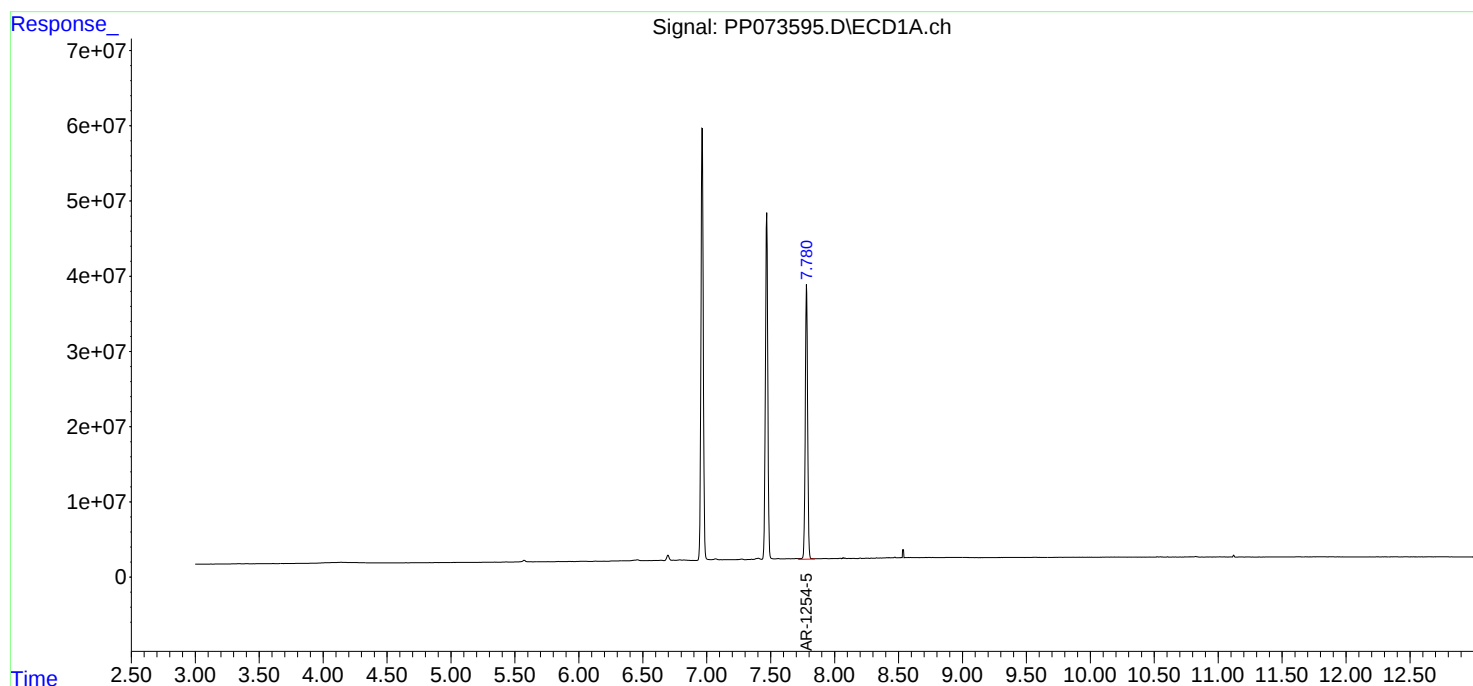


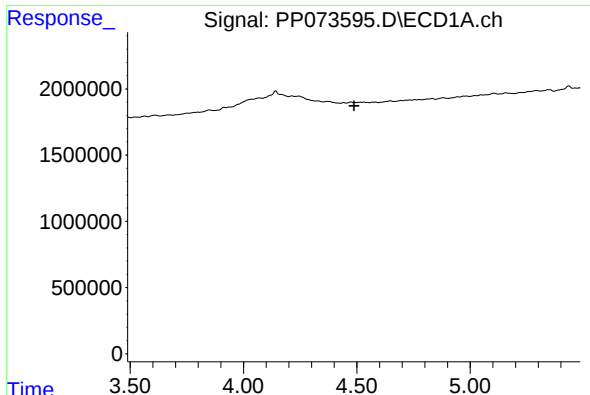

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.488 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

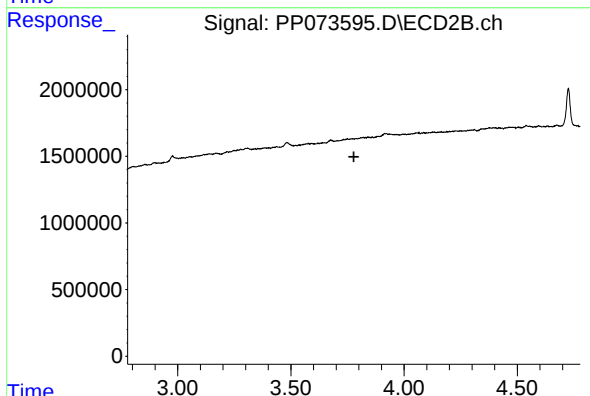


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.778 min
Response: 0
Conc: N.D.

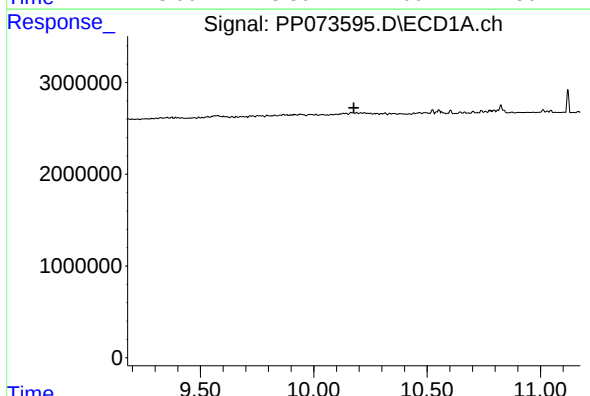


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.176 min
Response: 0
Conc: N.D.

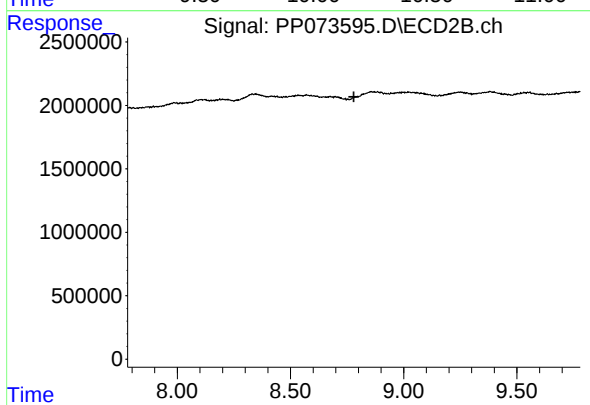

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.780 min
Response: 0
Conc: N.D.

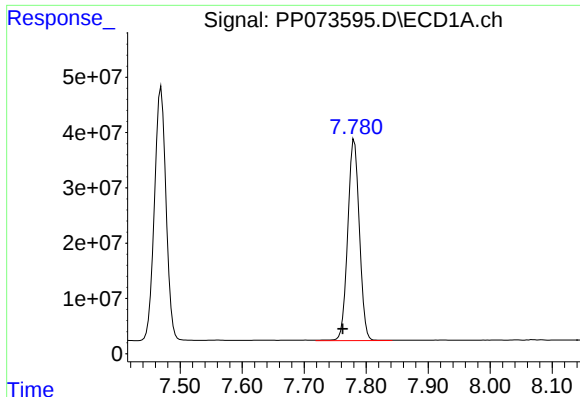

#30 AR-1254-5

R.T.: 7.781 min
Delta R.T.: 0.019 min
Response: 473759474
Conc: 6429.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

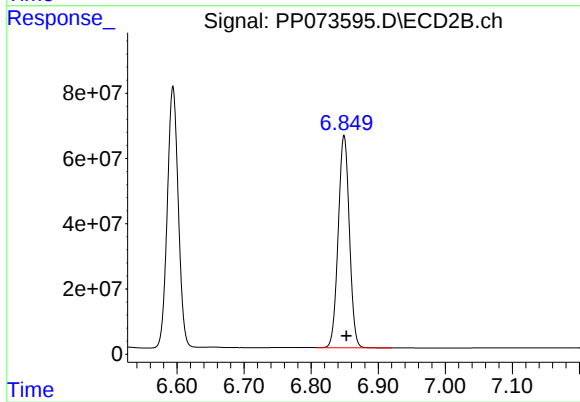

#30 AR-1254-5

R.T.: 6.849 min
Delta R.T.: -0.004 min
Response: 752075076
Conc: 5635.85 ng/ml