

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070925\
 Data File : PP073604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 13:17
 Operator : YP\AJ
 Sample : Q2509-02 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-25-0112

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/09/2025
 Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 01:39:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.776	3304558	4255871	2.413	2.310
2) SA Decachlor...	10.174	8.783	1188905	1082476	1.090m	0.818

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070925\
Data File : PP073604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2025 13:17
Operator : YP\AJ
Sample : Q2509-02 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-25-0112


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 01:39:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

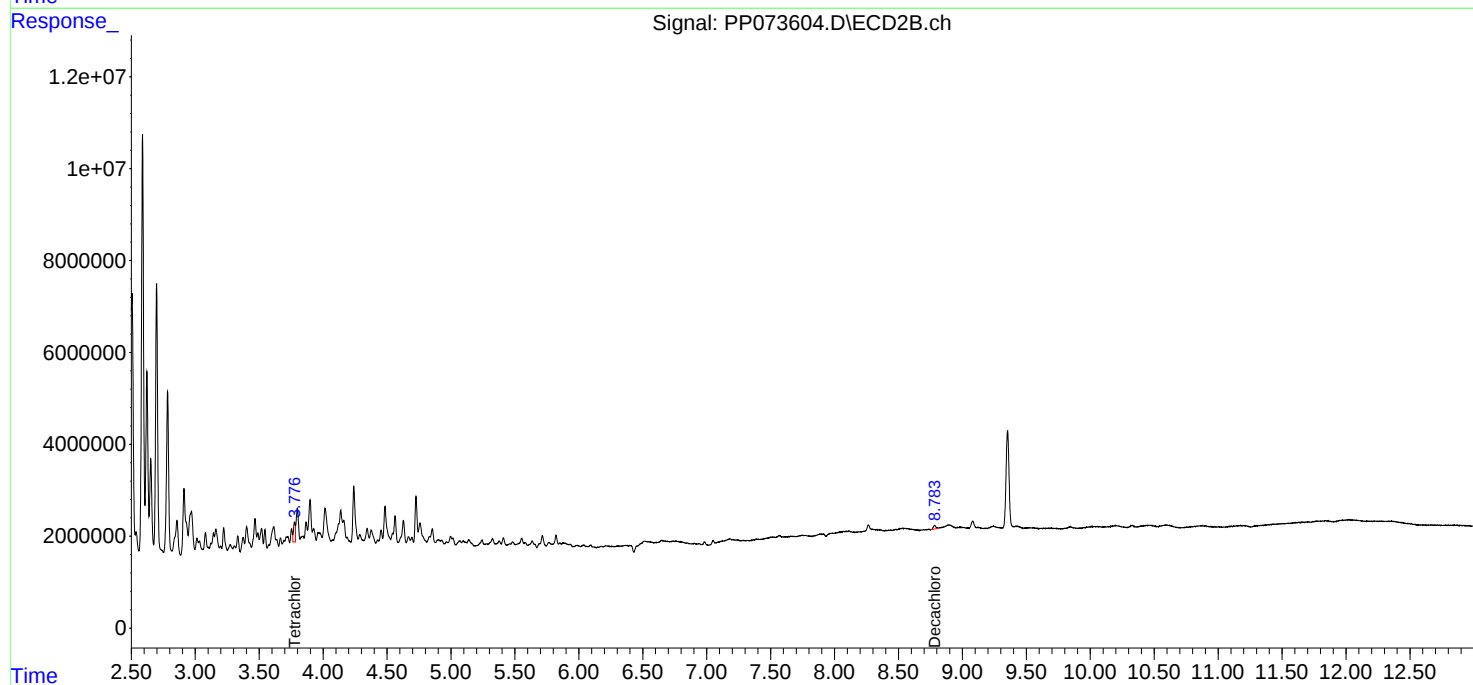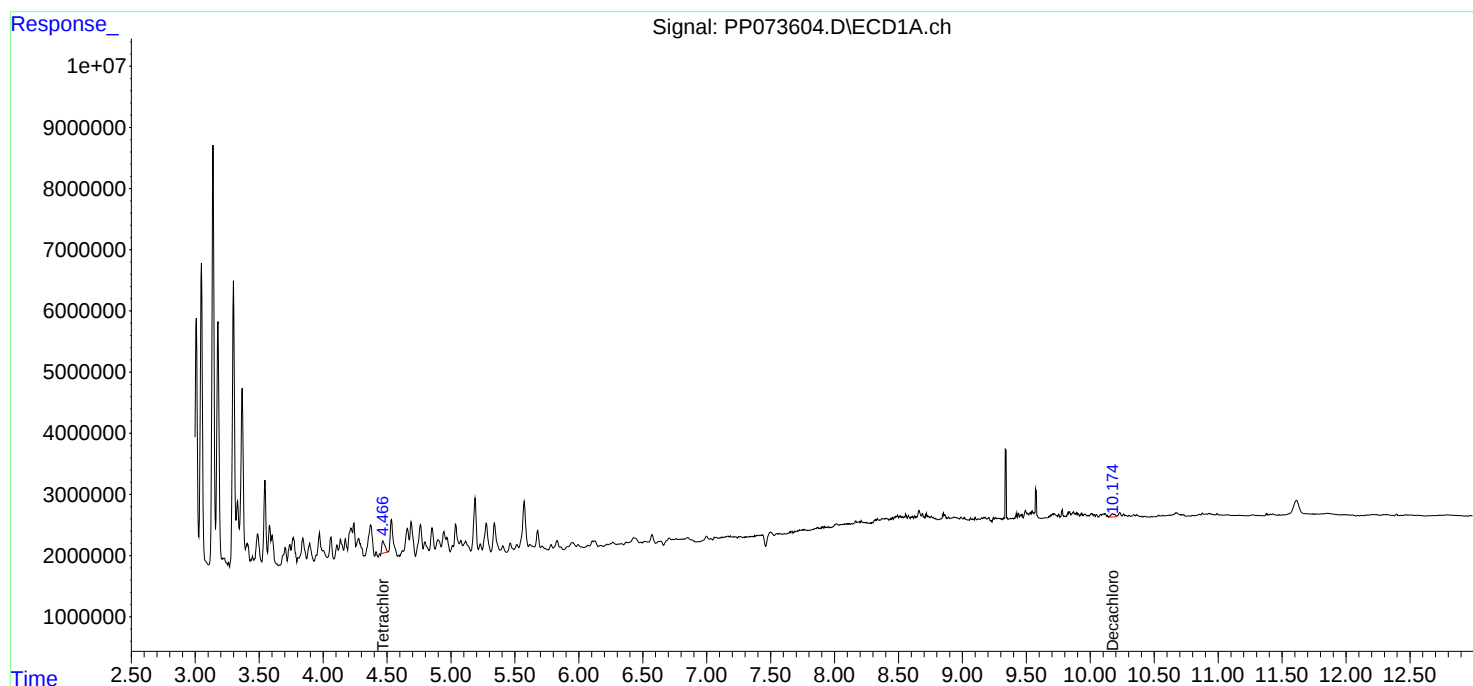

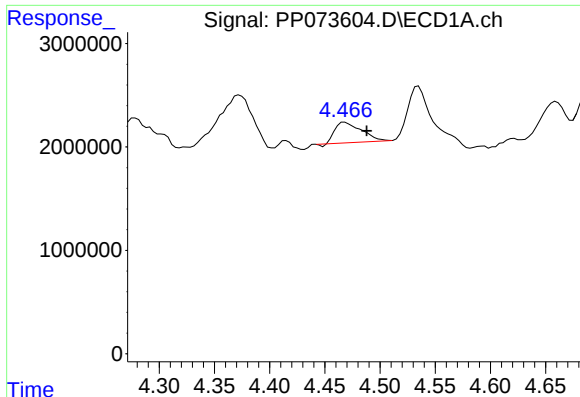


#1 Tetrachloro-m-xylene

R.T.: 4.468 min
Delta R.T.: -0.020 min
Response: 3304558
Conc: 2.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-25-0112


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/09/2025
Supervised By :mohammad ahmed 07/10/2025

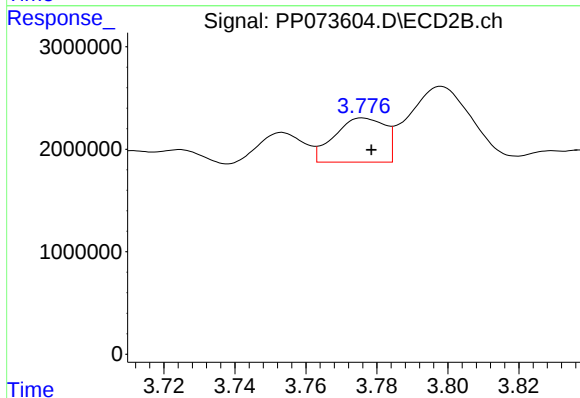


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: -0.002 min
Response: 4255871
Conc: 2.31 ng/ml

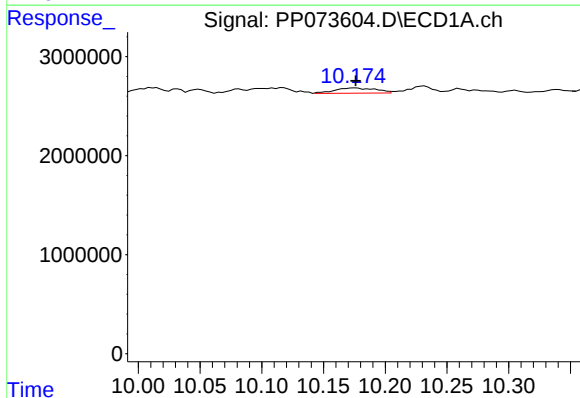

#2 Decachlorobiphenyl

R.T.: 10.174 min
Delta R.T.: -0.002 min
Response: 1188905
Conc: 1.09 ng/ml m

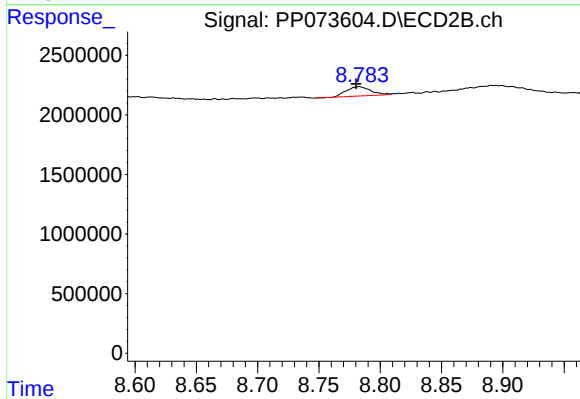

#2 Decachlorobiphenyl

R.T.: 8.783 min
Delta R.T.: 0.003 min
Response: 1082476
Conc: 0.82 ng/ml