

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071024\
 Data File : PP066218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2024 10:45
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/11/2024
 Supervised By :Ankita Jodhani 07/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 13:41:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 06:34:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.020	44650554	48673432	25.365	21.038
2) SA Decachlor...	10.776	9.193	45704357	31870956	25.282m	28.016

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071024\
Data File : PP066218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2024 10:45
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2024
Supervised By :Ankita Jodhani 07/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 13:41:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 06:34:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

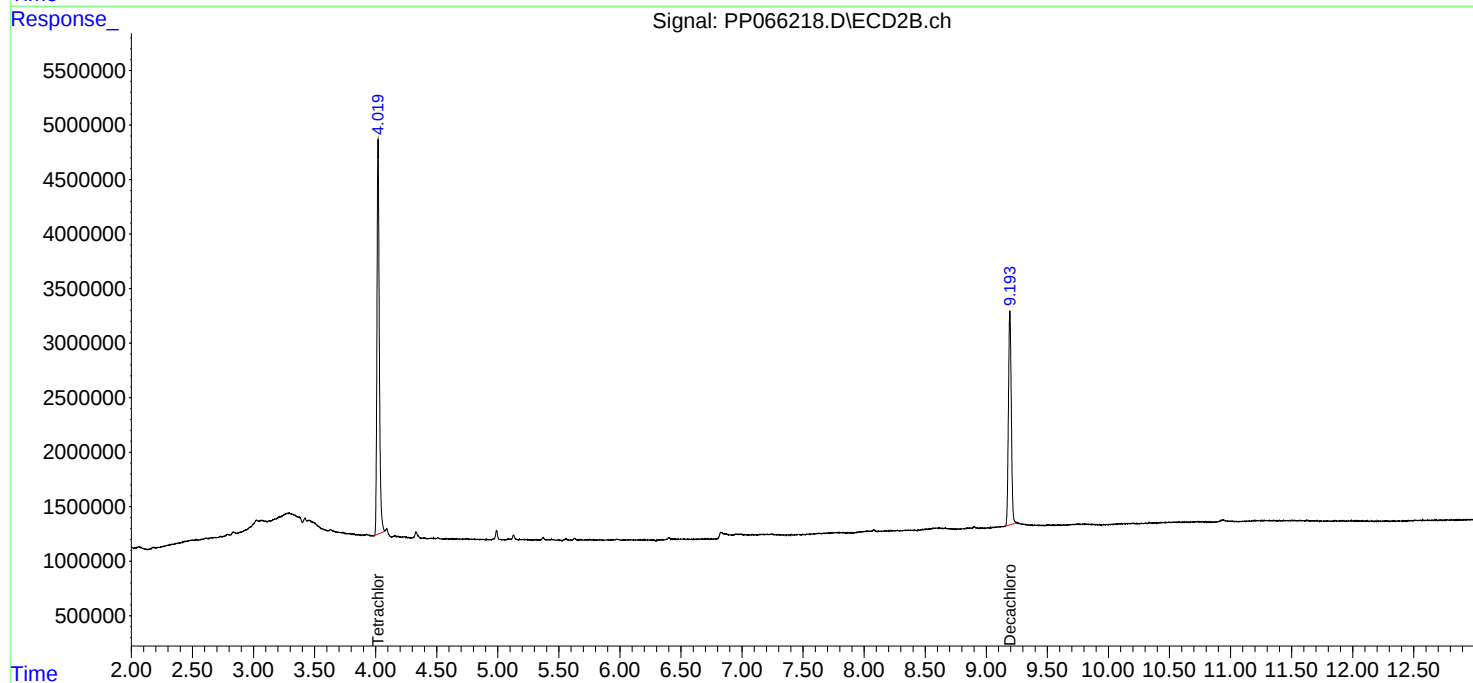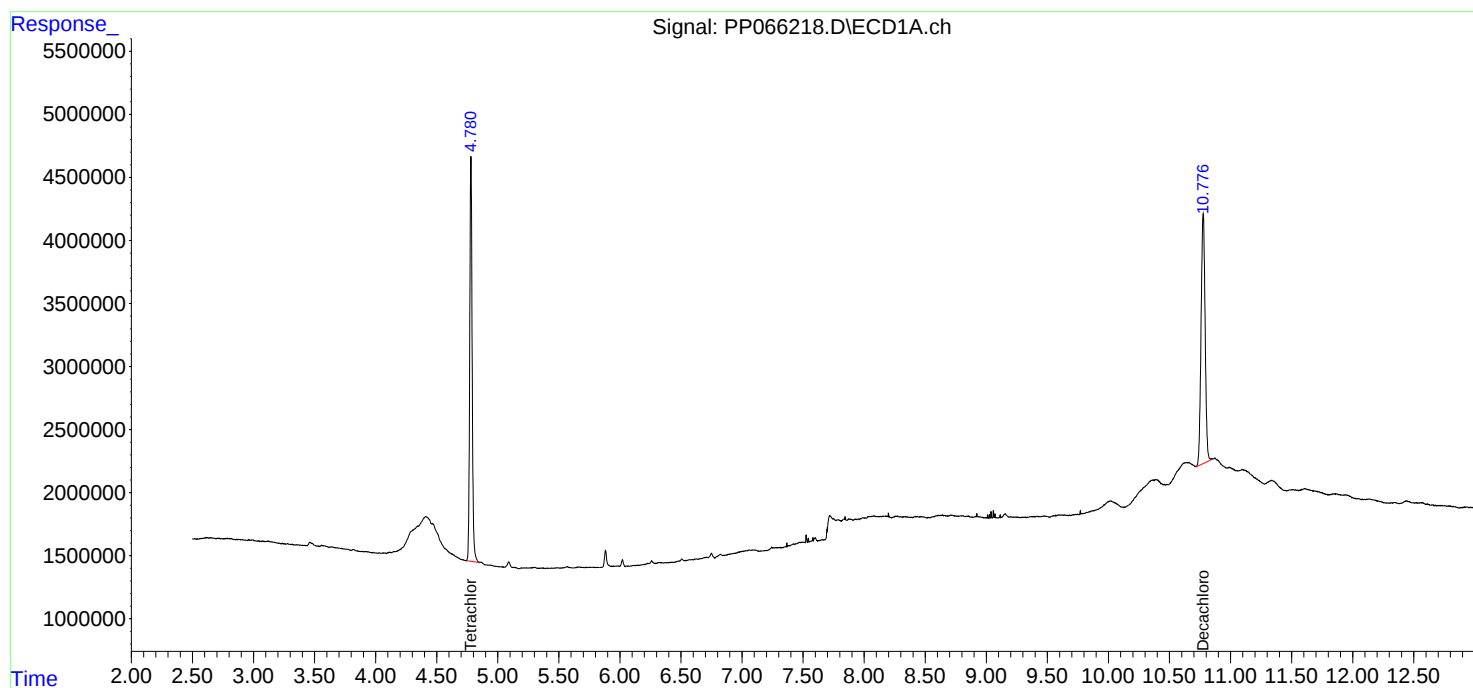

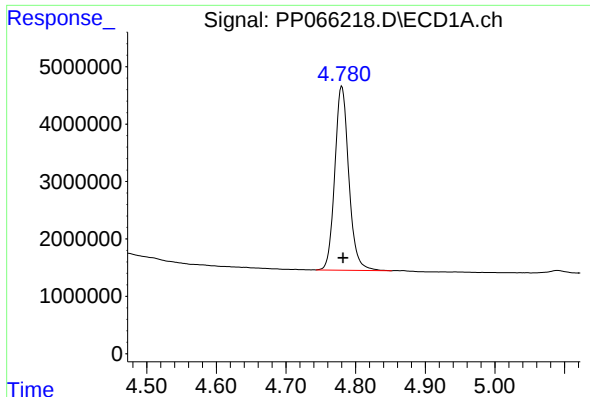


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 44650554
Conc: 25.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2024
Supervised By :Ankita Jodhani 07/11/2024

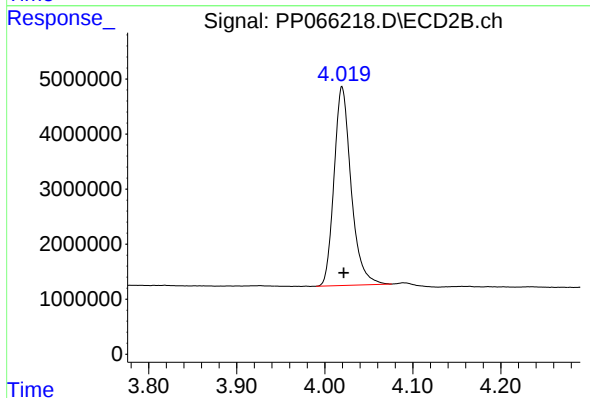


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: -0.002 min
Response: 48673432
Conc: 21.04 ng/ml

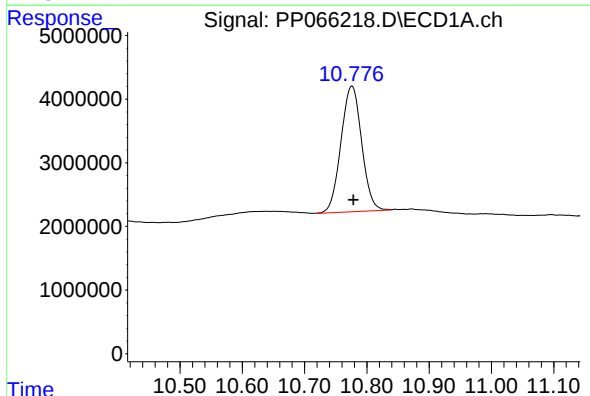

#2 Decachlorobiphenyl

R.T.: 10.776 min
Delta R.T.: -0.003 min
Response: 45704357
Conc: 25.28 ng/ml m

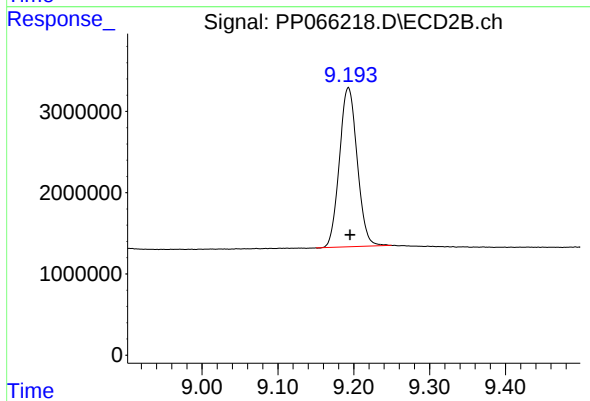

#2 Decachlorobiphenyl

R.T.: 9.193 min
Delta R.T.: -0.002 min
Response: 31870956
Conc: 28.02 ng/ml