

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071025\
 Data File : PP073684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2025 06:06
 Operator : YP\AJ
 Sample : Q2549-02 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC271242-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/10/2025
 Supervised By :mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 08:50:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.777	2425531	3357100	1.771	1.822
2) SA Decachlor...	10.174	8.781	1844781	2226958	1.691m	1.683

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071025\
Data File : PP073684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2025 06:06
Operator : YP\AJ
Sample : Q2549-02 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC271242-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/10/2025
Supervised By :mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 08:50:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

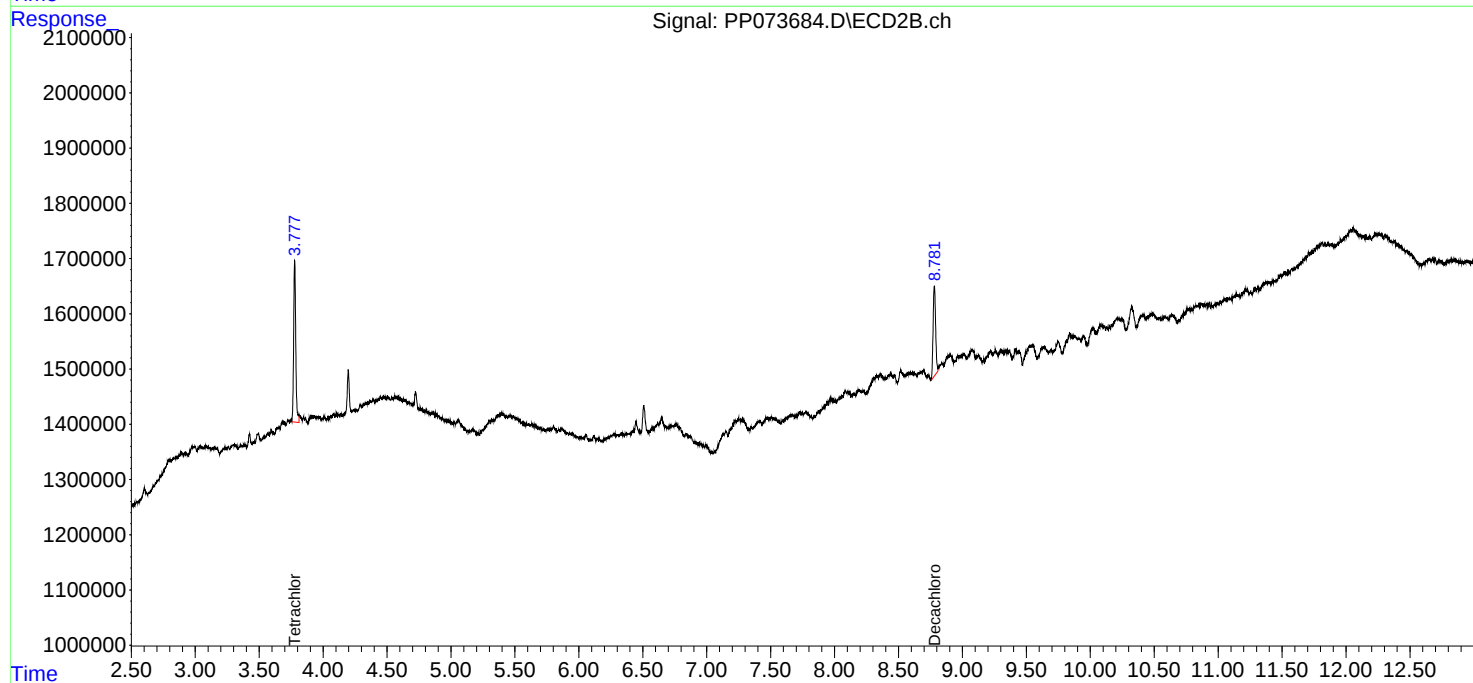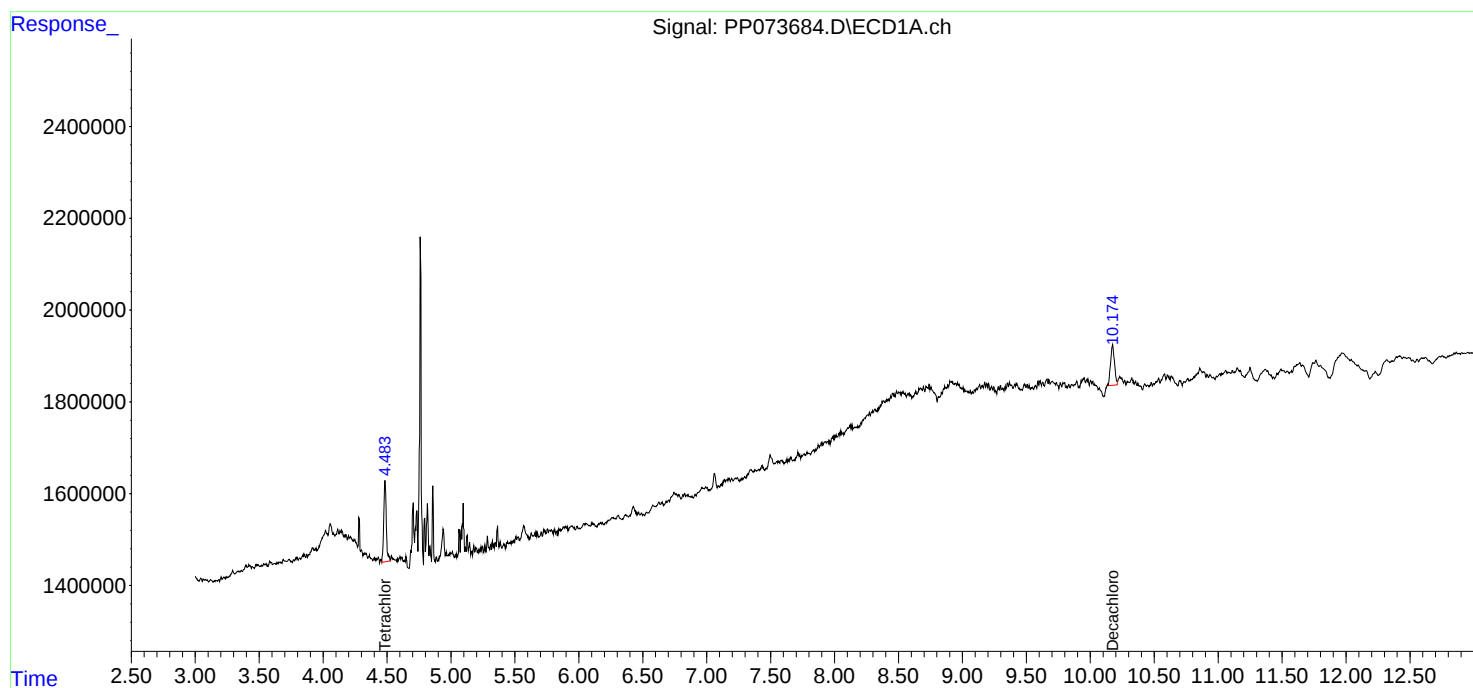

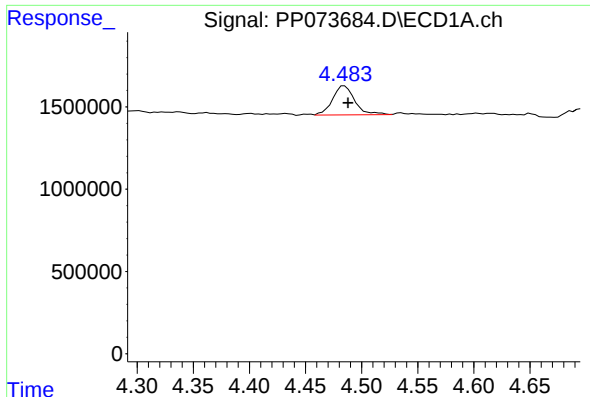


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: -0.003 min
Response: 2425531
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271242-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/10/2025
Supervised By :mohammad ahmed 07/11/2025

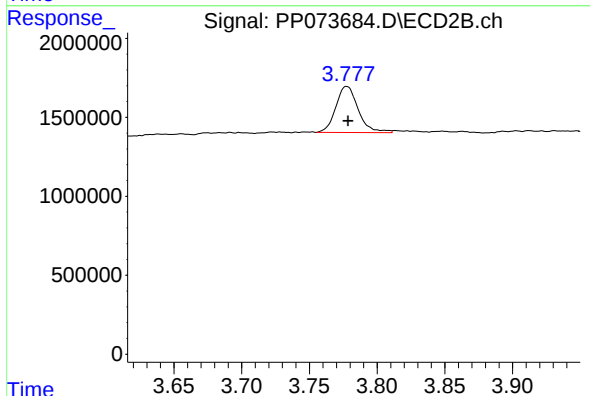


#1 Tetrachloro-m-xylene

R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 3357100
Conc: 1.82 ng/ml

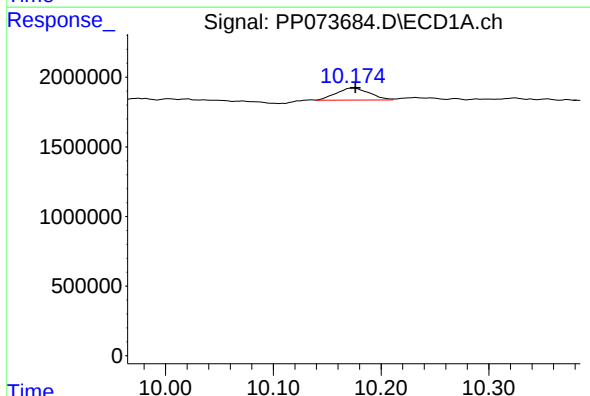

#2 Decachlorobiphenyl

R.T.: 10.174 min
Delta R.T.: -0.002 min
Response: 1844781
Conc: 1.69 ng/ml m

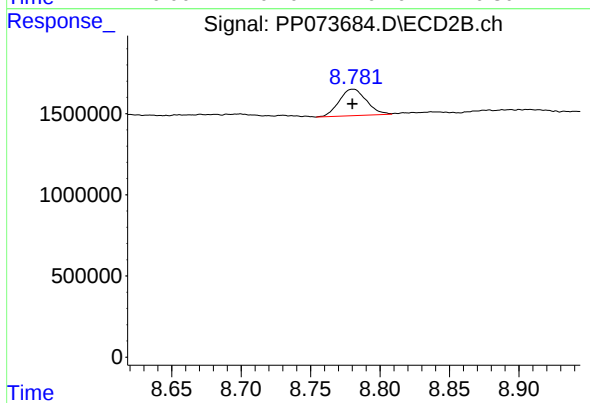

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 2226958
Conc: 1.68 ng/ml