

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071122\
 Data File : PP049336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 11:50
 Operator : YP\AJ
 Sample : N3634-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-56RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2022
 Supervised By :Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 23:56:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.596	35441323	60174471	24.931	23.500
2) SA Decachlor...	10.095	8.567	55373828	42057545	45.144	37.311
Target Compounds						
26) L6 AR-1254-1	6.379	5.467	1935002	4022958	28.706	27.403
27) L6 AR-1254-2	6.598	5.614	5188879	4673458	55.325m	37.460 #
28) L6 AR-1254-3	6.971	6.016	1648513	8309790	16.246m	46.151m#
29) L6 AR-1254-4	7.255	6.243	2366030	5003374	31.537m	46.247 #
30) L6 AR-1254-5	7.675	6.660	10236543	31035722	121.332	213.833 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071122\
Data File : PP049336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 11:50
Operator : YP\AJ
Sample : N3634-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
X127-56RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 23:56:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

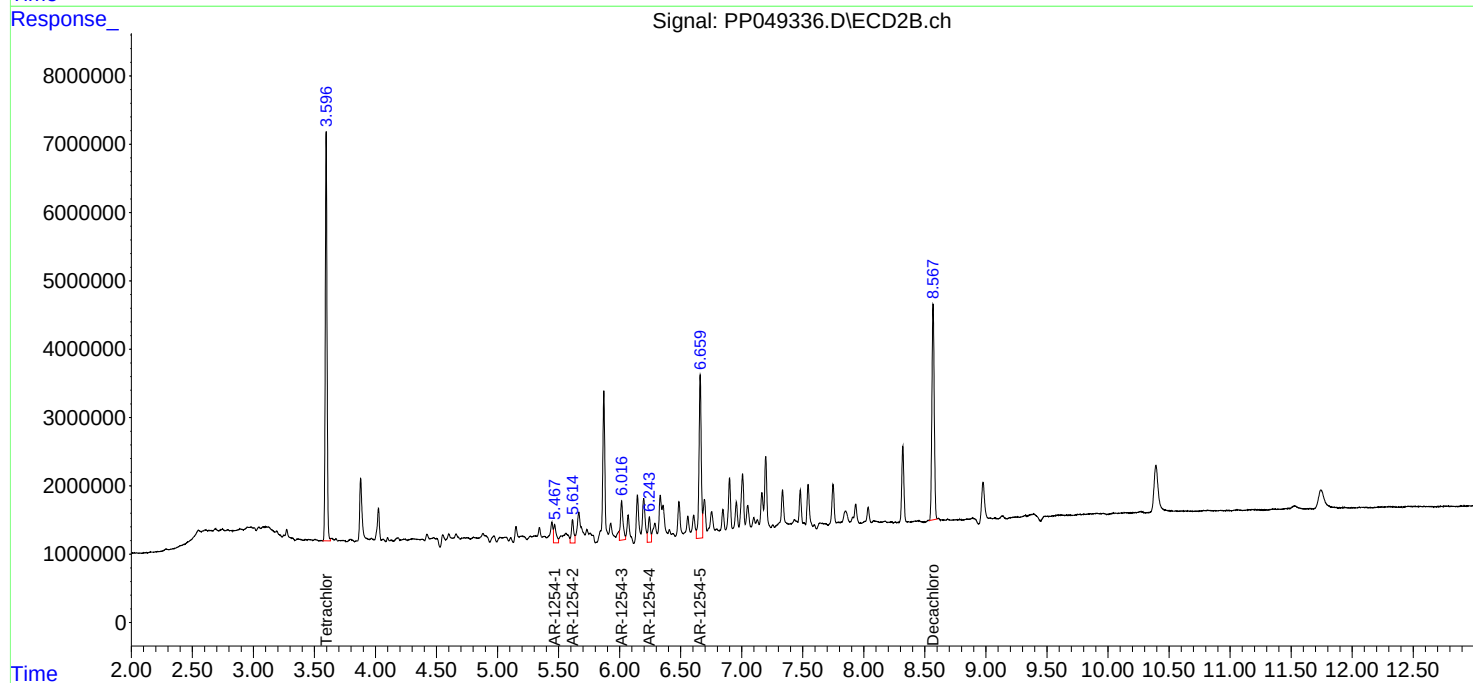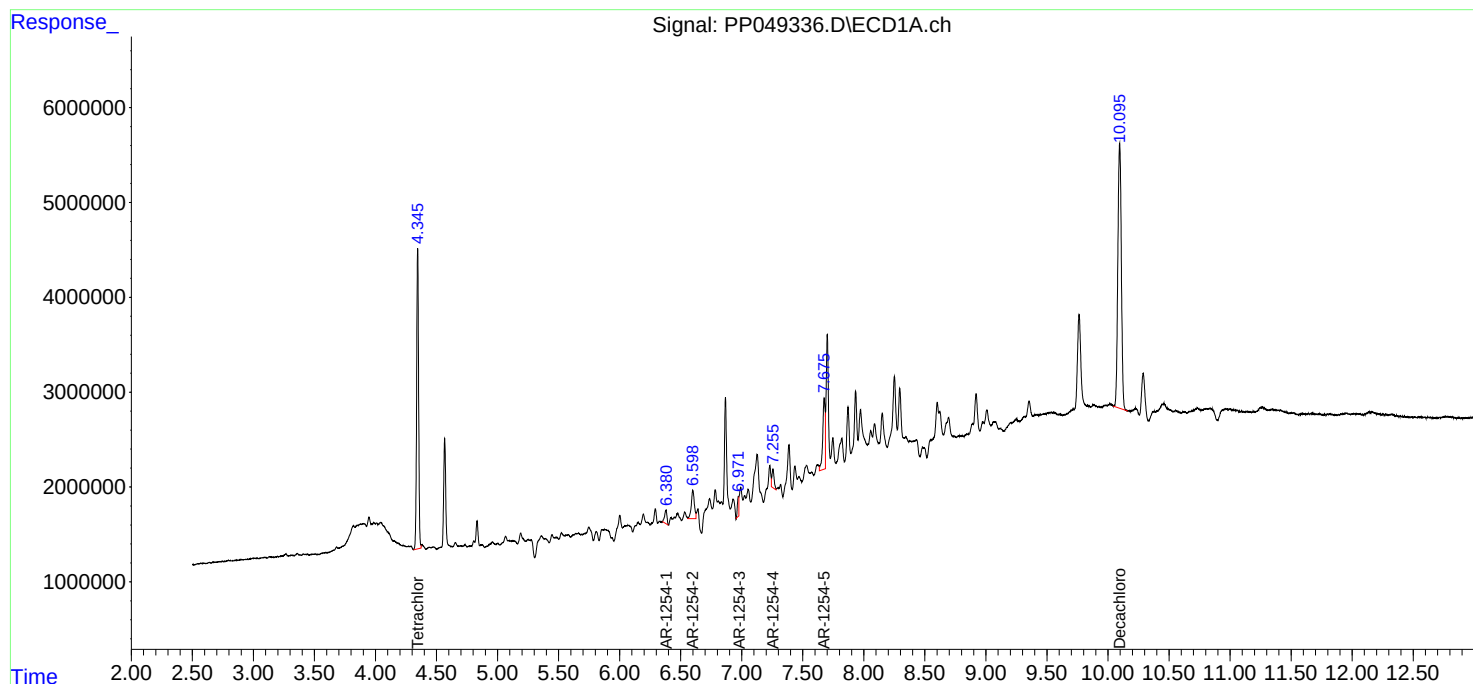

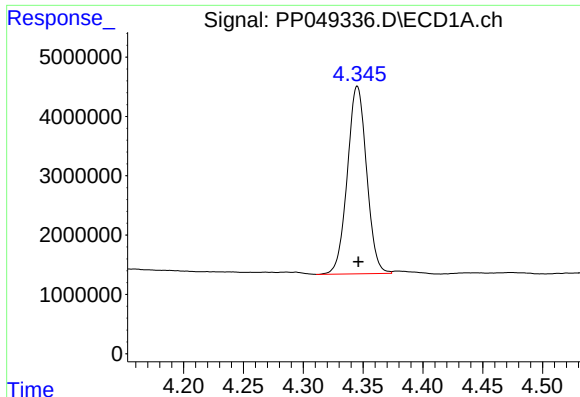


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 35441323
Conc: 24.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-56RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

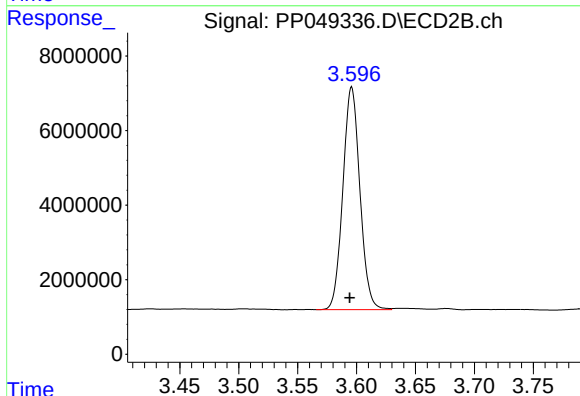


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.002 min
Response: 60174471
Conc: 23.50 ng/ml

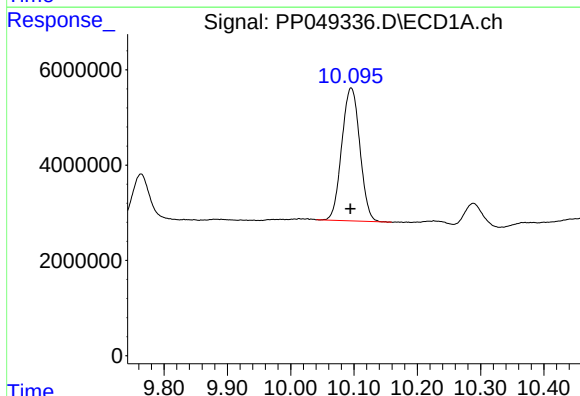


#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: 0.001 min
Response: 55373828
Conc: 45.14 ng/ml

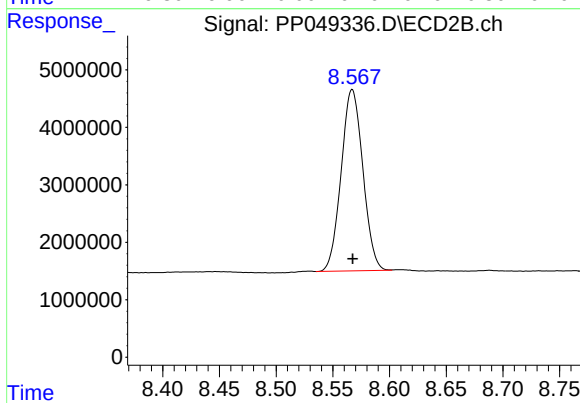

#2 Decachlorobiphenyl

R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 42057545
Conc: 37.31 ng/ml

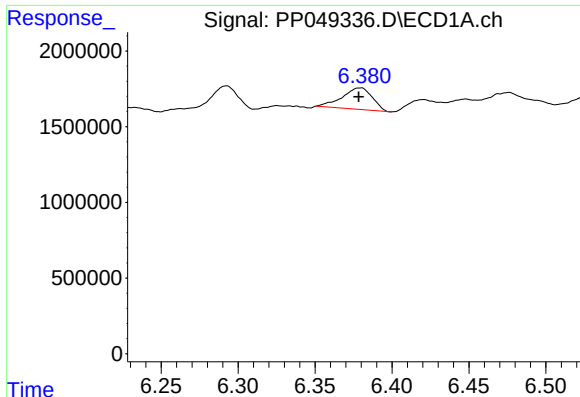


#26 AR-1254-1

R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 1935002
Conc: 28.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-56RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

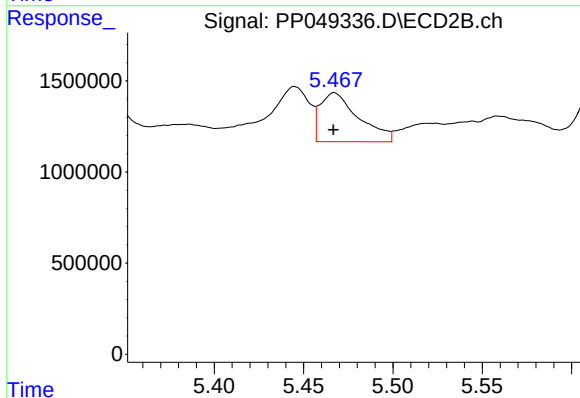


#26 AR-1254-1

R.T.: 5.467 min
Delta R.T.: 0.000 min
Response: 4022958
Conc: 27.40 ng/ml

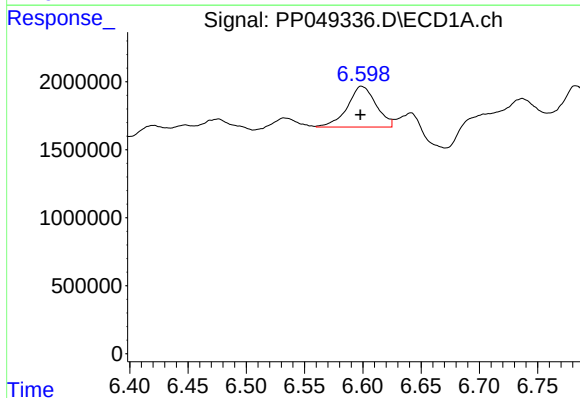


#27 AR-1254-2

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 5188879
Conc: 55.33 ng/ml m

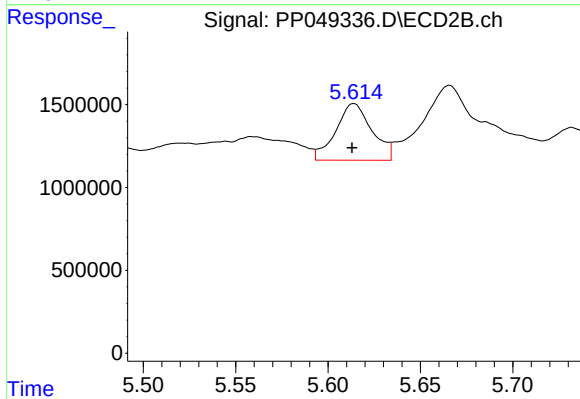

#27 AR-1254-2

R.T.: 5.614 min
Delta R.T.: 0.000 min
Response: 4673458
Conc: 37.46 ng/ml

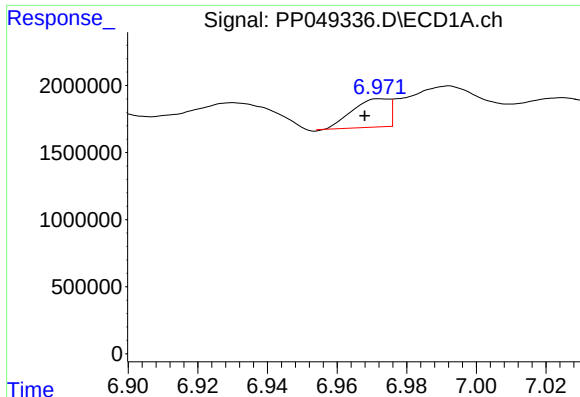


#28 AR-1254-3

R.T.: 6.971 min
Delta R.T.: 0.004 min
Response: 1648513
Conc: 16.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-56RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

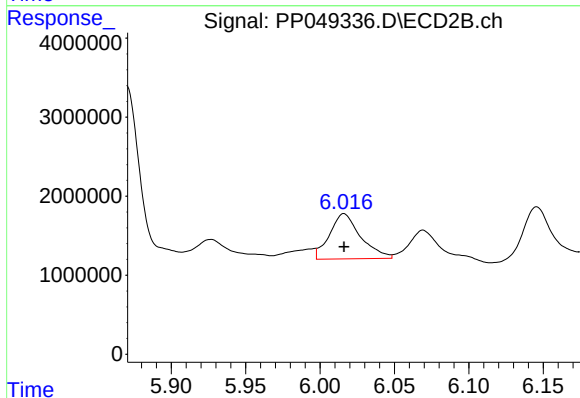


#28 AR-1254-3

R.T.: 6.016 min
Delta R.T.: 0.000 min
Response: 8309790
Conc: 46.15 ng/ml m

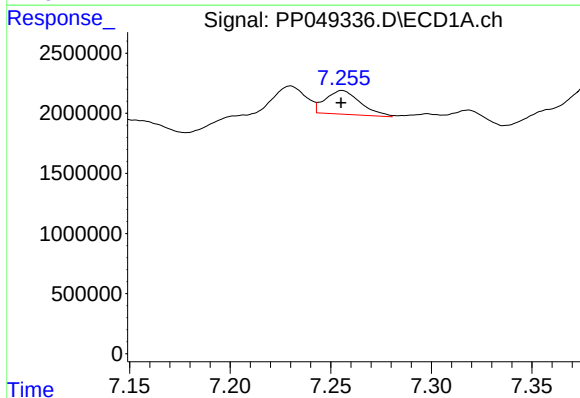


#29 AR-1254-4

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 2366030
Conc: 31.54 ng/ml m

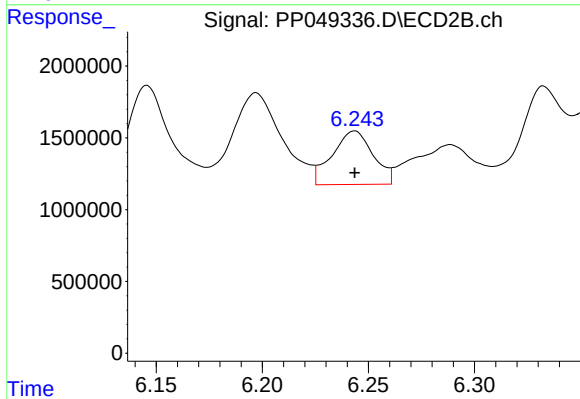

#29 AR-1254-4

R.T.: 6.243 min
Delta R.T.: 0.000 min
Response: 5003374
Conc: 46.25 ng/ml

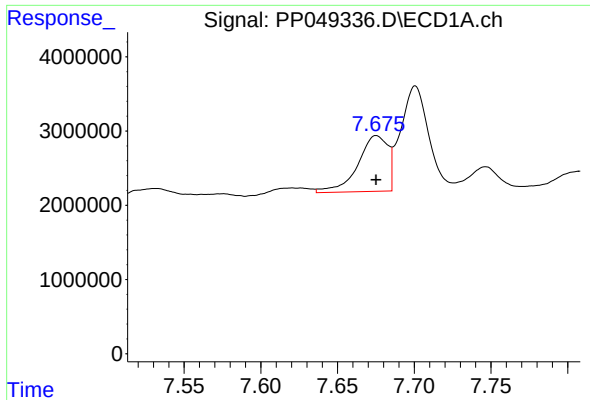


#30 AR-1254-5

R.T.: 7.675 min
Delta R.T.: 0.000 min
Response: 10236543
Conc: 121.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-56RE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

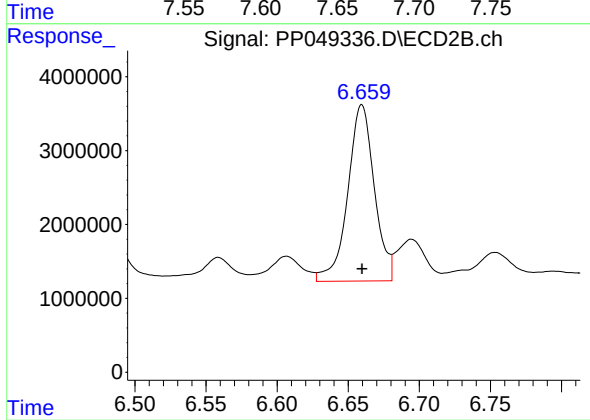

#30 AR-1254-5

R.T.: 6.660 min
Delta R.T.: 0.000 min
Response: 31035722
Conc: 213.83 ng/ml