

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071122\
 Data File : PP049370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 21:12
 Operator : YP\AJ
 Sample : N3656-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S5-03-S

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2022
 Supervised By :Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:17:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.594	33108542	57504595	23.290	22.457
2) SA Decachlor...	10.091	8.564	26752499	22048492	21.810	19.560
Target Compounds						
41) L9 AR-1268-1	8.598	7.477	5778898	7151678	30.772	33.244
42) L9 AR-1268-2	8.693	7.541	4721678	6704457	26.987	35.049 #
43) L9 AR-1268-3	8.915	7.746	2799793	3522467	19.544m	23.128
44) L9 AR-1268-4	9.350	8.034	2351615	1454216	36.709	22.818 #
45) L9 AR-1268-5	9.759	8.316	8050599	6627840	17.455	16.611

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071122\
Data File : PP049370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 21:12
Operator : YP\AJ
Sample : N3656-05
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S5-03-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:17:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

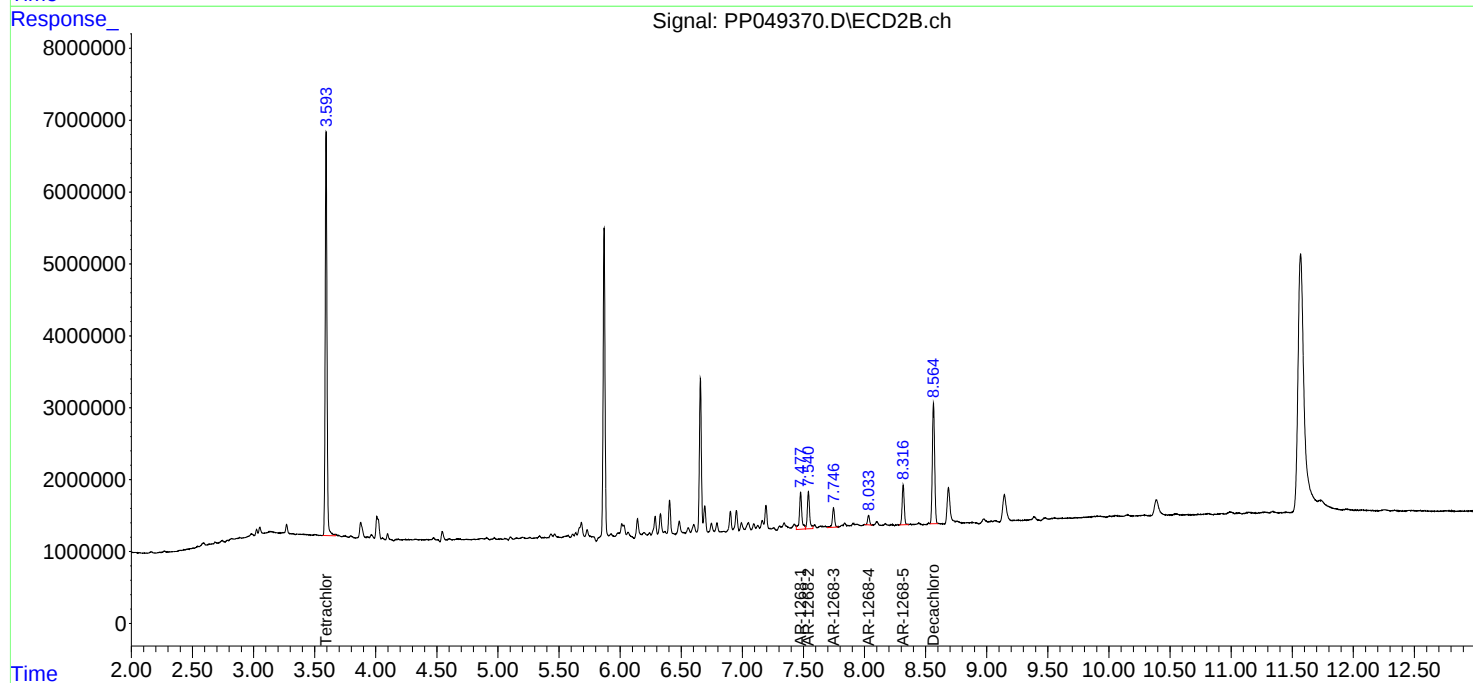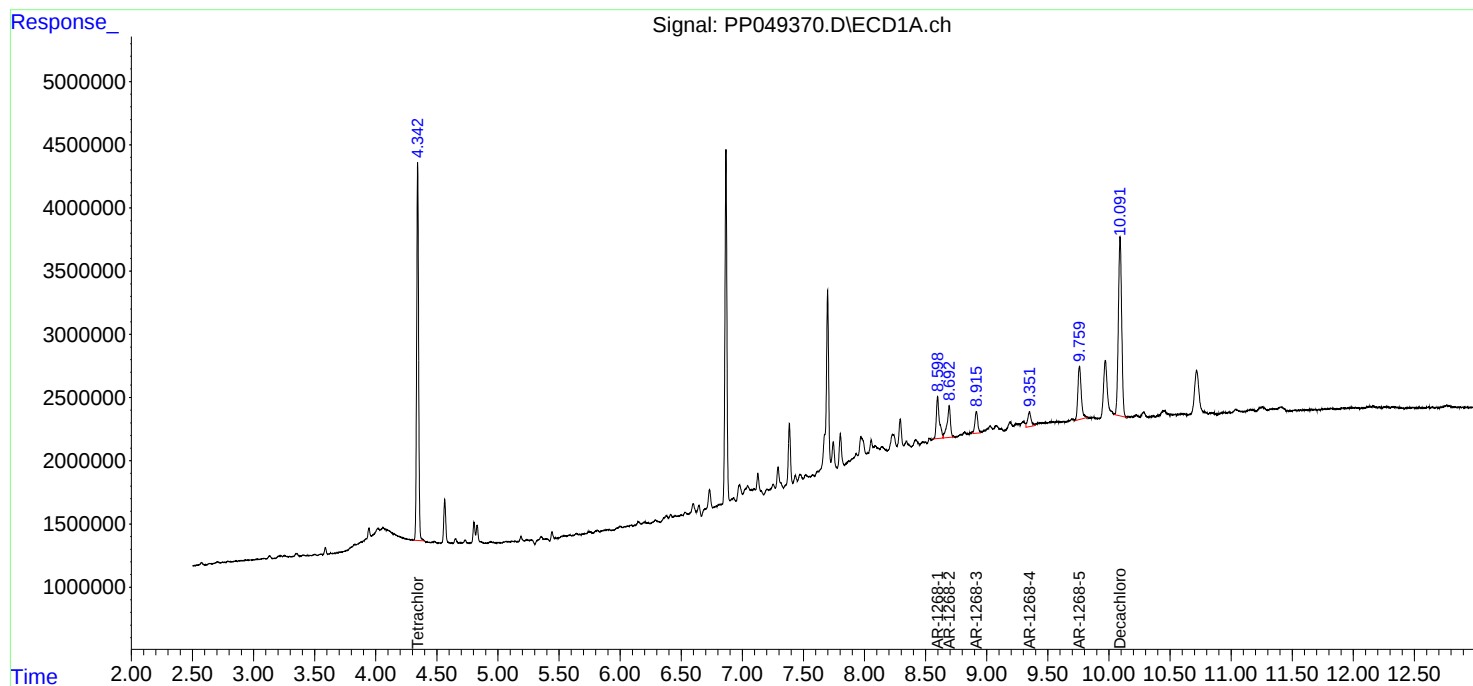

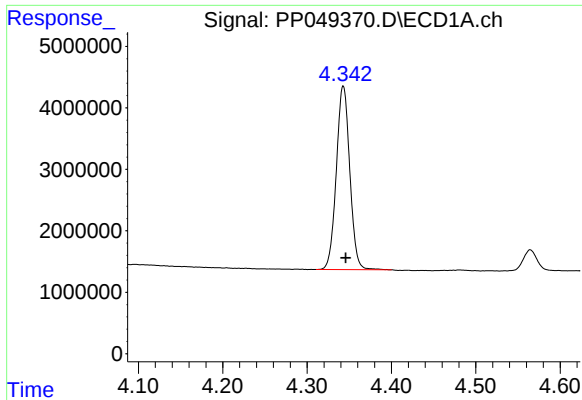


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.003 min
Response: 33108542
Conc: 23.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

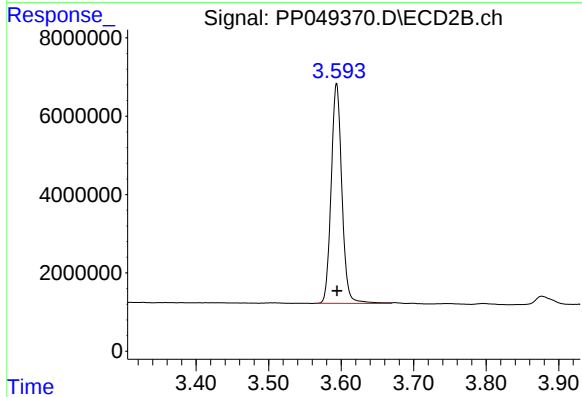


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 57504595
Conc: 22.46 ng/ml

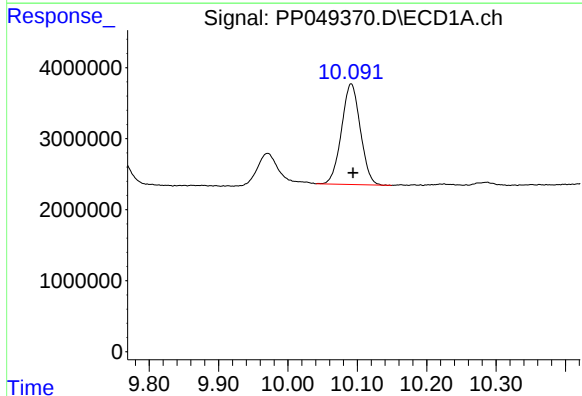


#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: -0.003 min
Response: 26752499
Conc: 21.81 ng/ml

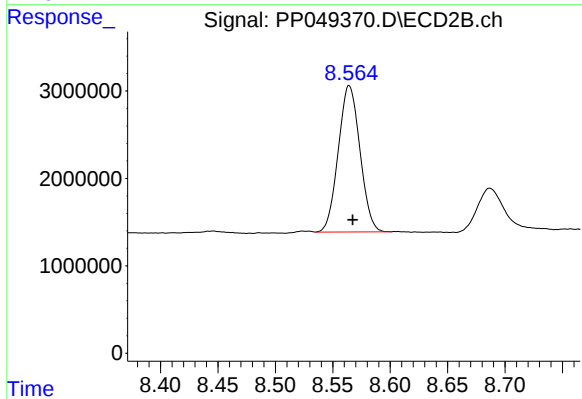

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.003 min
Response: 22048492
Conc: 19.56 ng/ml

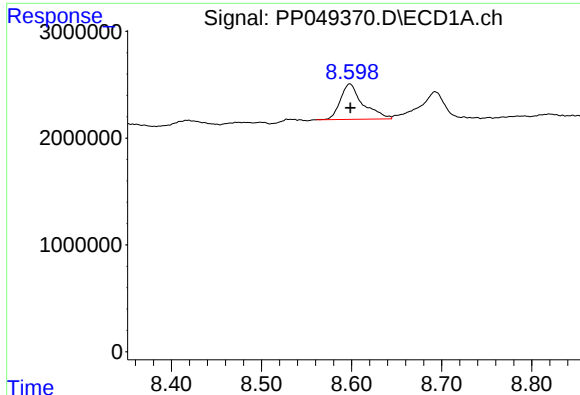


#41 AR-1268-1

R.T.: 8.598 min
Delta R.T.: 0.000 min
Response: 5778898
Conc: 30.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

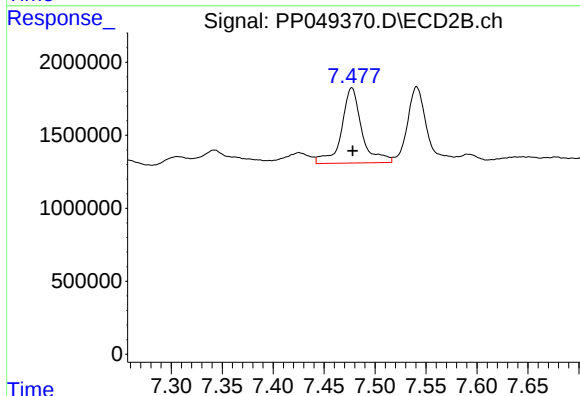


#41 AR-1268-1

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 7151678
Conc: 33.24 ng/ml

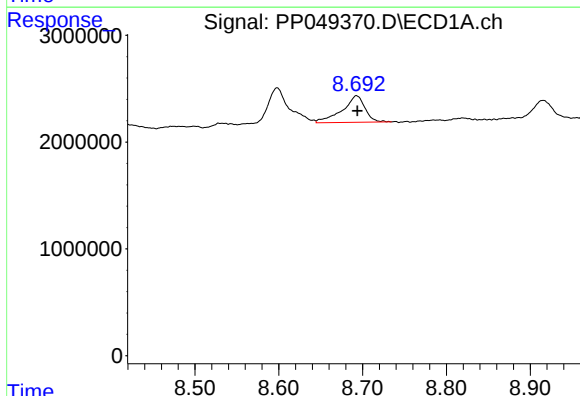


#42 AR-1268-2

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 4721678
Conc: 26.99 ng/ml

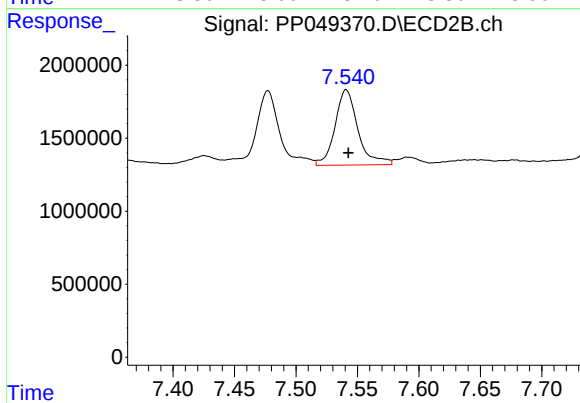

#42 AR-1268-2

R.T.: 7.541 min
Delta R.T.: -0.002 min
Response: 6704457
Conc: 35.05 ng/ml

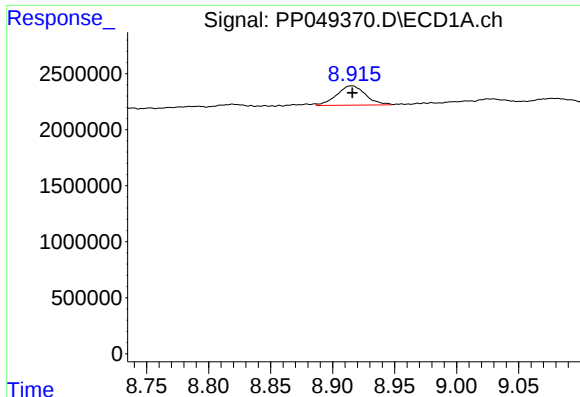


#43 AR-1268-3

R.T.: 8.915 min
Delta R.T.: 0.000 min
Response: 2799793
Conc: 19.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

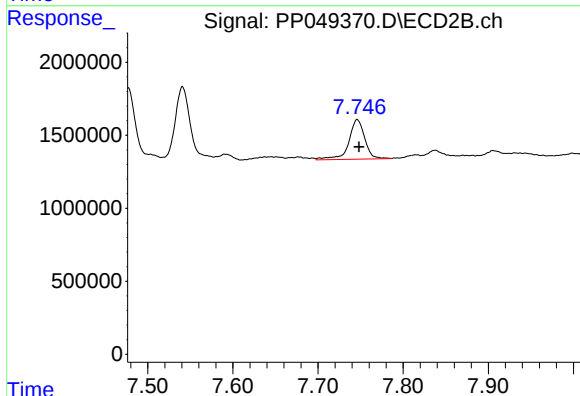


#43 AR-1268-3

R.T.: 7.746 min
Delta R.T.: -0.002 min
Response: 3522467
Conc: 23.13 ng/ml

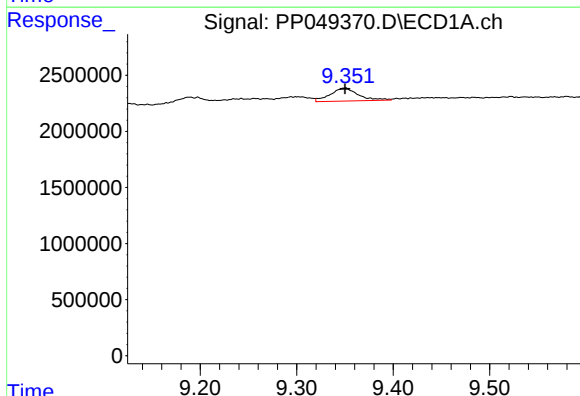


#44 AR-1268-4

R.T.: 9.350 min
Delta R.T.: 0.000 min
Response: 2351615
Conc: 36.71 ng/ml

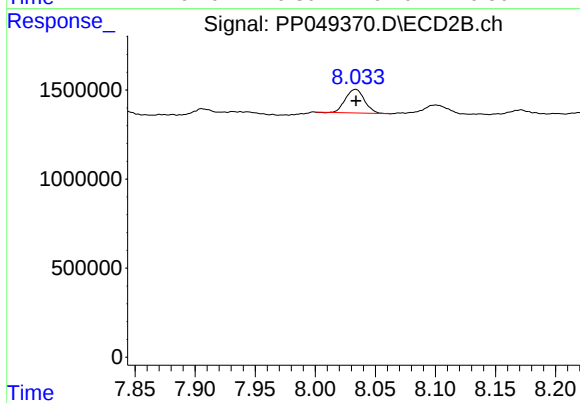

#44 AR-1268-4

R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 1454216
Conc: 22.82 ng/ml

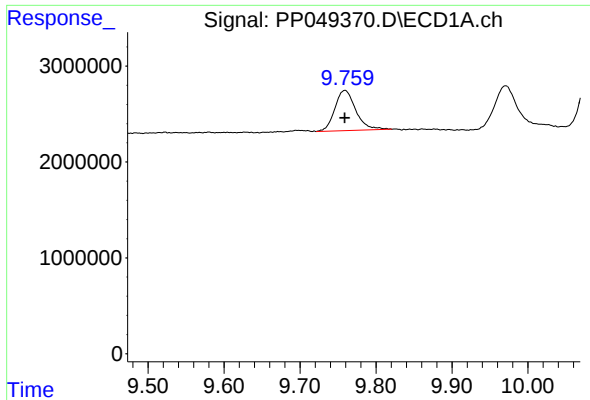


#45 AR-1268-5

R.T.: 9.759 min
Delta R.T.: 0.000 min
Response: 8050599
Conc: 17.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
S5-03-S

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

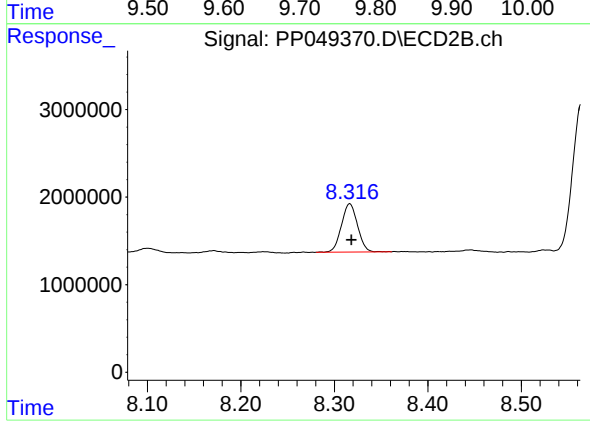

#45 AR-1268-5

R.T.: 8.316 min
Delta R.T.: -0.002 min
Response: 6627840
Conc: 16.61 ng/ml