

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071122\
 Data File : PP049375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 23:04
 Operator : YP\AJ
 Sample : N3665-01 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1-MASTIC

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2022
 Supervised By :Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:20:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 29 09:37:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.581	2171676	7331864	1.528m	2.863 #
2) SA Decachlor...	10.092	8.563	1879749	4594568	1.532m	4.076 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071122\
Data File : PP049375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 23:04
Operator : YP\AJ
Sample : N3665-01 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1-MASTIC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:20:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 29 09:37:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

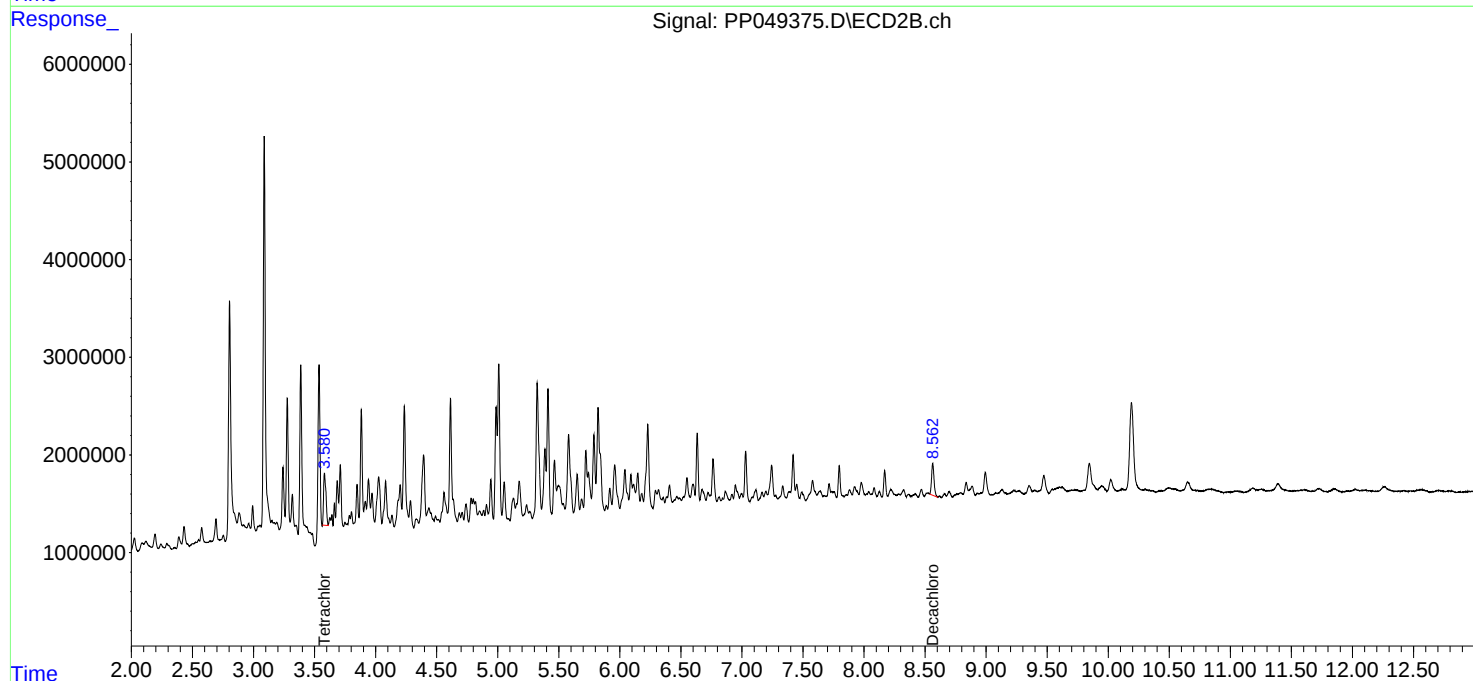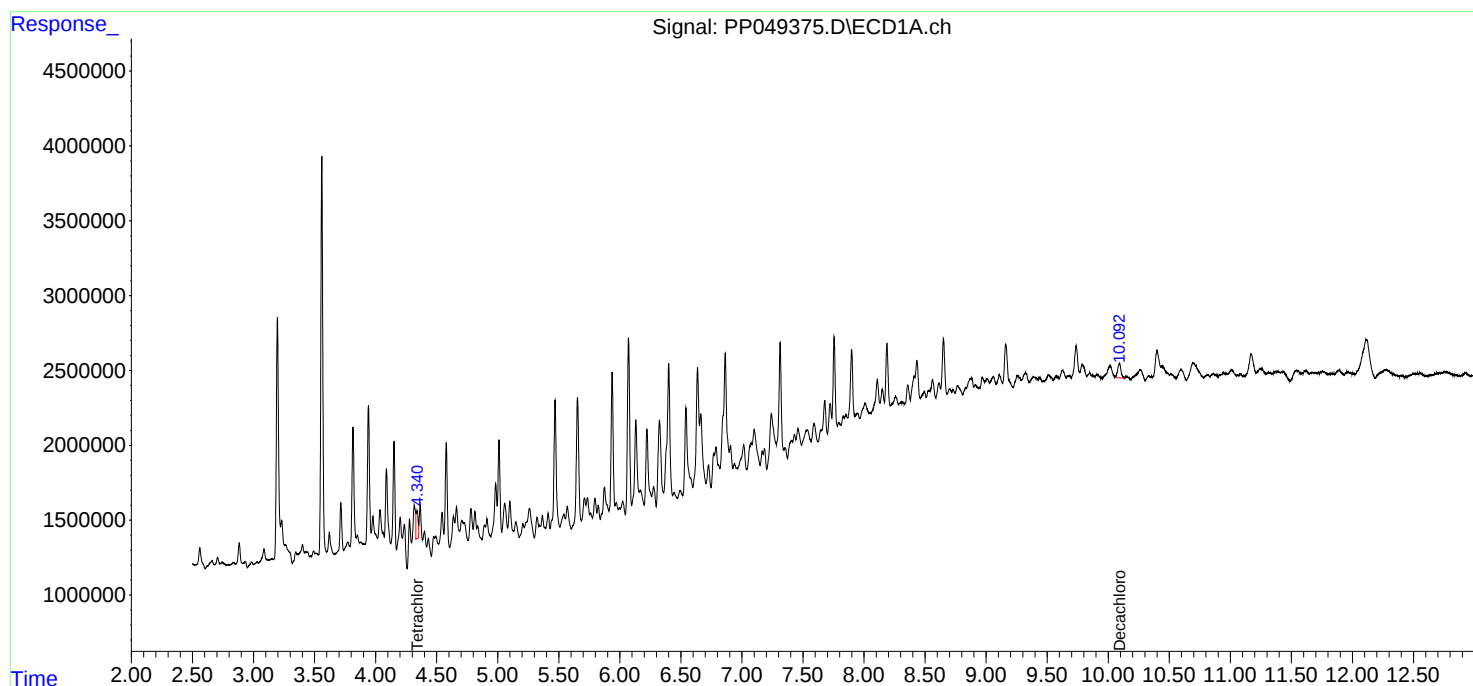

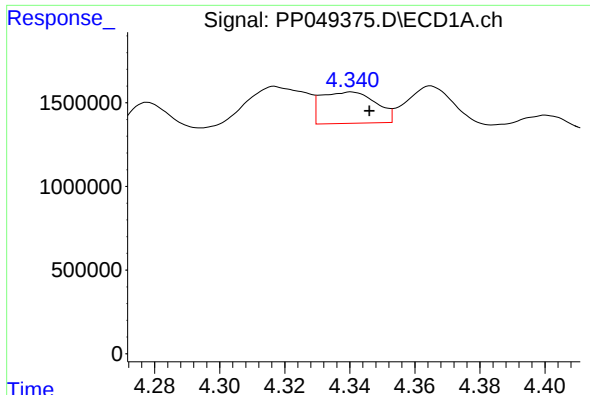


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: -0.006 min
Response: 2171676
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
1-MASTIC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

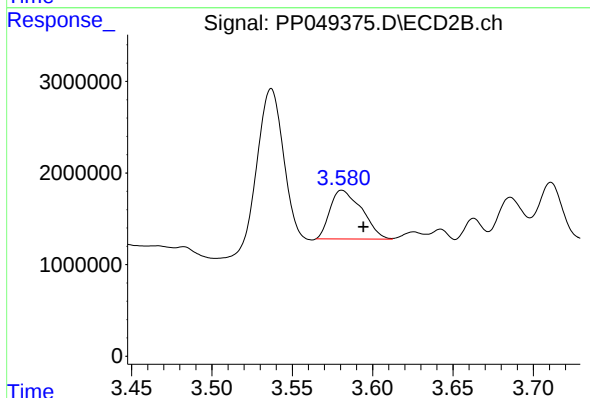


#1 Tetrachloro-m-xylene

R.T.: 3.581 min
Delta R.T.: -0.013 min
Response: 7331864
Conc: 2.86 ng/ml

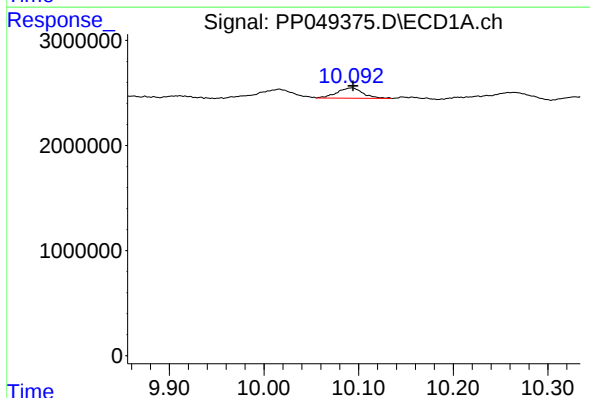

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 1879749
Conc: 1.53 ng/ml m

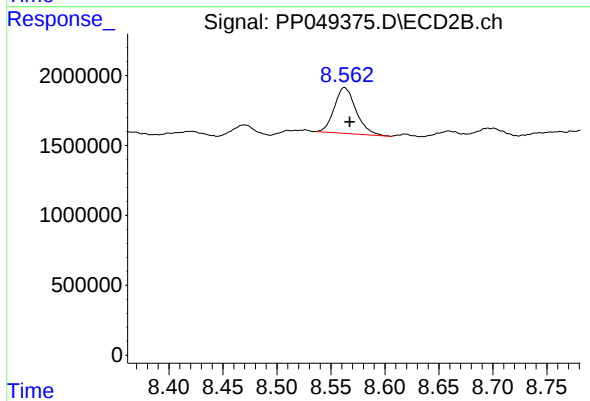

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: -0.005 min
Response: 4594568
Conc: 4.08 ng/ml