

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071125\
 Data File : PP073696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2025 10:45
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 11:39:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.471	3.781	84624	54526	0.062	0.030 #
2)	SA Decachlor...	10.167	8.777	60826	51956	0.056	0.039 #
Target Compounds							
3)	L1 AR-1016-1	5.622	4.858	109707	121229	2.309	1.778
4)	L1 AR-1016-2	5.656	4.858	106862	121229	1.501	1.190
5)	L1 AR-1016-3	5.729	5.040	133366	151694	3.054	2.804
6)	L1 AR-1016-4	5.808	5.096	37701	796328	1.049	18.148 #
7)	L1 AR-1016-5	6.124	5.313	375972	1408642	12.000	25.808 #
8)	L2 AR-1221-1	4.640f	3.984	63982	76652	3.581	2.834
9)	L2 AR-1221-2	4.767	4.081	32764	46542	2.426	2.286
10)	L2 AR-1221-3	4.848	4.147	117502	18191	2.824	0.296 #
11)	L3 AR-1232-1	4.848	4.147	117502	18191	3.599	0.390 #
12)	L3 AR-1232-2	5.370	4.858	113596	121229	6.988	2.544 #
13)	L3 AR-1232-3	5.656	5.040	106862	151694	3.239	6.061 #
14)	L3 AR-1232-4	5.808	5.134	37701	93496	2.293	4.317 #
15)	L3 AR-1232-5	5.891	5.313	212499	1408642	20.103	62.430 #
16)	L4 AR-1242-1	5.622	4.858	109707	121229	2.873	2.099 #
17)	L4 AR-1242-2	5.656	4.858	106862	121229	1.785	1.402
18)	L4 AR-1242-3	5.715	5.040	67738	151694	1.850	3.302 #
19)	L4 AR-1242-4	5.808	5.134	37701	93496	1.173	2.112 #
20)	L4 AR-1242-5	6.553	5.640	259357	1991938	7.922	36.058 #
21)	L5 AR-1248-1	5.622	4.858	109707	121229	3.554	2.700
22)	L5 AR-1248-2	5.891	5.096	212499	796328	5.323	12.941 #
23)	L5 AR-1248-3	6.124	5.134	375972	93496	8.466	1.459 #
24)	L5 AR-1248-4	6.508	5.313	304089	1408642	5.521	18.688 #
25)	L5 AR-1248-5	6.553	5.713	259357	382478	4.822	5.128
26)	L6 AR-1254-1	6.481	5.640	527162	1991938	9.837	17.167 #
27)	L6 AR-1254-2	6.692	5.793	6433483	457231	77.243	4.544 #
28)	L6 AR-1254-3	7.064	6.221	4682201	4105661	53.007	26.583 #
29)	L6 AR-1254-4	7.325	6.448	722349	383639	9.182	4.057 #
30)	L6 AR-1254-5	7.777	6.847	435.3E6	765.2E6	5908.474	5734.328
31)	L7 AR-1260-1	7.239	6.321	921558	447870	15.630	4.591 #
32)	L7 AR-1260-2	7.465	6.528	600.0E6	5516595	6260.422	44.910 #
34)	L7 AR-1260-4	8.065	7.174	135681	208685	2.078	2.334
35)	L7 AR-1260-5	8.329f	7.386	169265	322024	1.122	1.433 #
36)	L8 AR-1262-1	8.065	6.847f	135681	765.2E6	1.559	5181.176 #
37)	L8 AR-1262-2	8.329f	7.174	169265	208685	0.855	1.633 #
38)	L8 AR-1262-3	8.690	7.674	83961	153392	0.668	1.345 #
39)	L8 AR-1262-4	8.775	7.730	116756	42973	1.252	0.233 #
40)	L8 AR-1262-5	9.408	8.184f	107288	185565	1.693	2.198 #
41)	L9 AR-1268-1	8.690	7.674	83961	153392	0.376	0.499 #
42)	L9 AR-1268-2	8.775	7.730	116756	42973	0.613	0.162 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071125\
 Data File : PP073696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2025 10:45
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 11:39:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.013	7.961	491080	164934	2.966	0.731 #
44) L9	AR-1268-4	9.408	8.184f	107288	185565	1.543	1.996 #
45) L9	AR-1268-5	9.855	8.522	122915	44059	0.267	0.071 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071125\
Data File : PP073696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2025 10:45
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 11:39:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

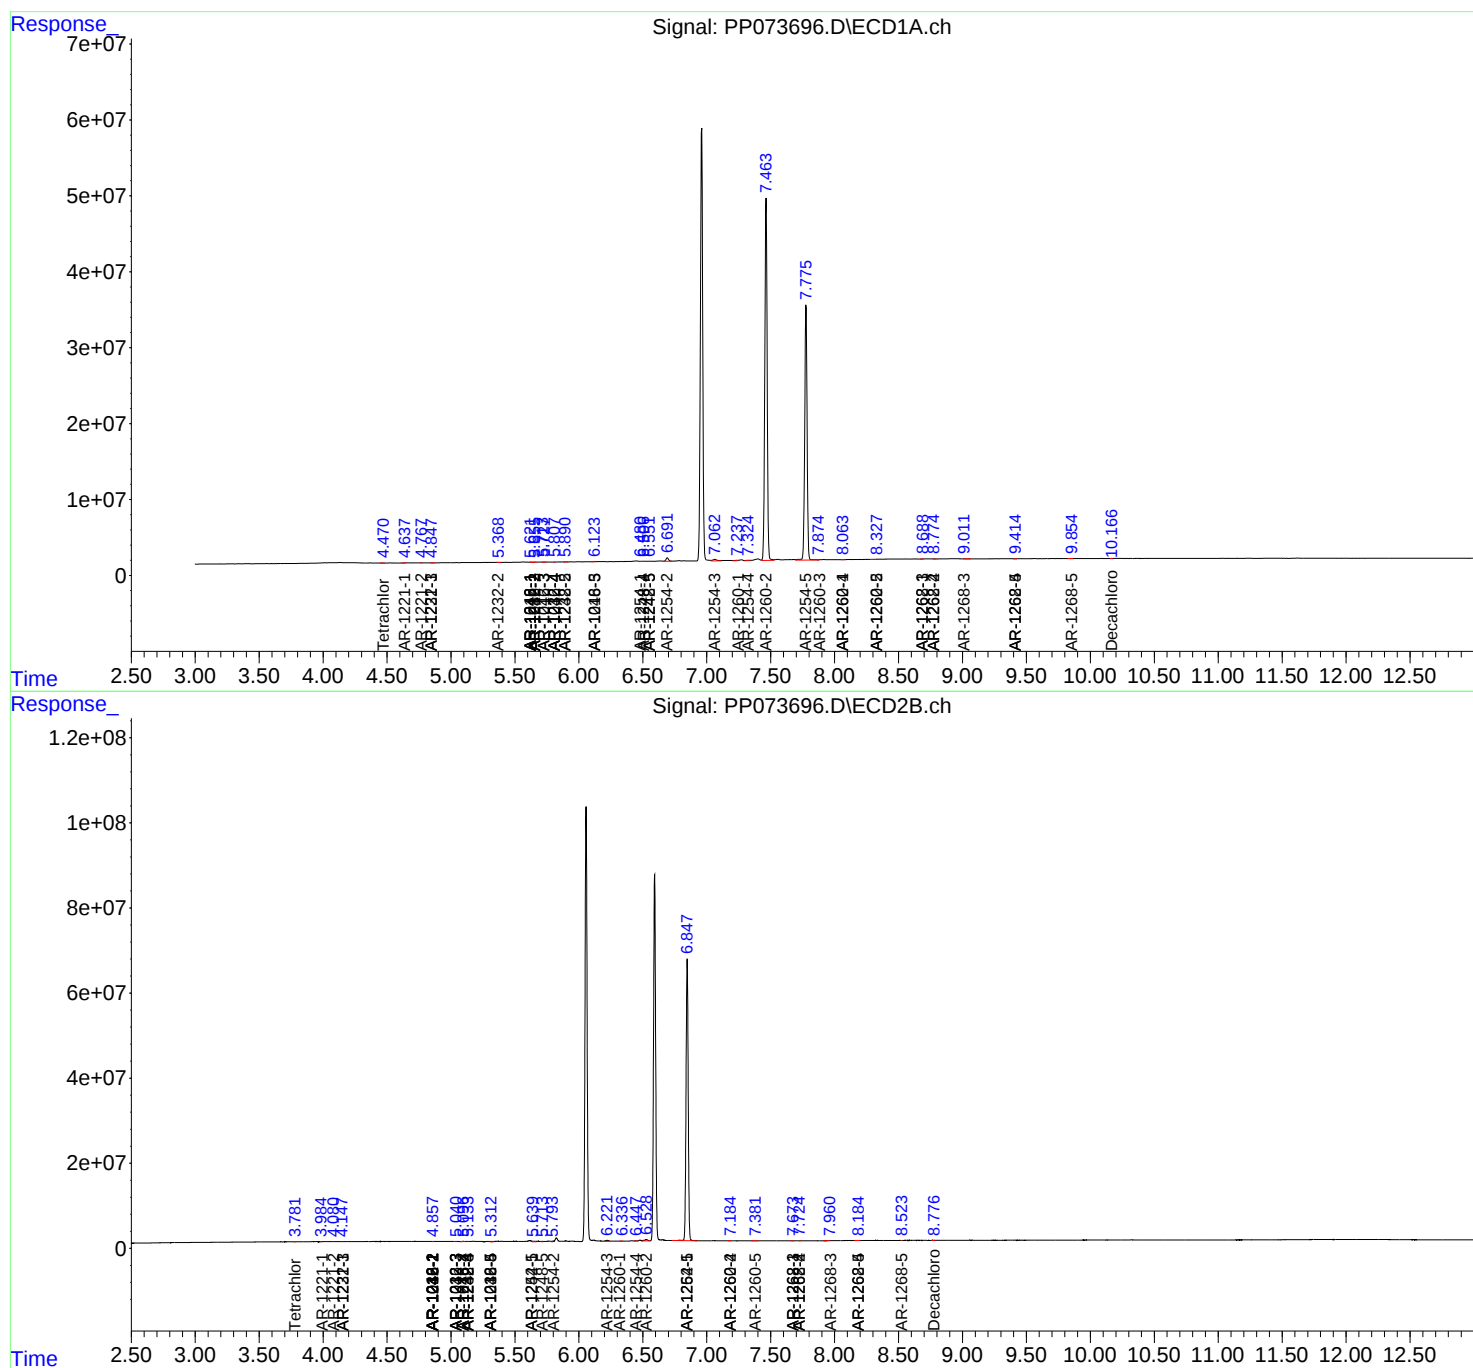


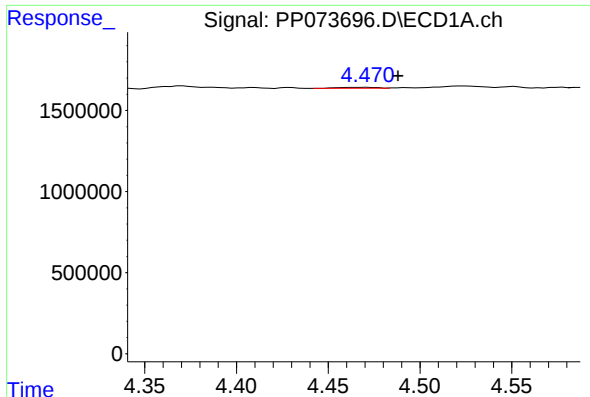

#1 Tetrachloro-m-xylene


R.T.: 4.471 min
Delta R.T.: -0.017 min
Response: 84624
Conc: 0.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

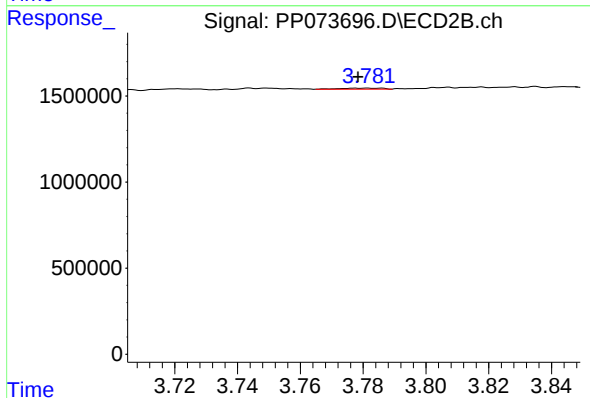


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: 0.003 min
Response: 54526
Conc: 0.03 ng/ml

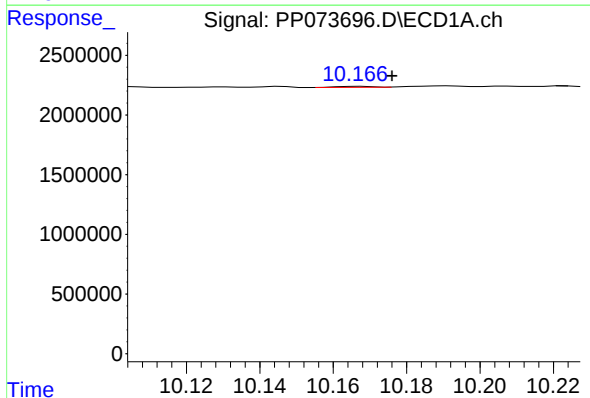


#2 Decachlorobiphenyl

R.T.: 10.167 min
Delta R.T.: -0.009 min
Response: 60826
Conc: 0.06 ng/ml

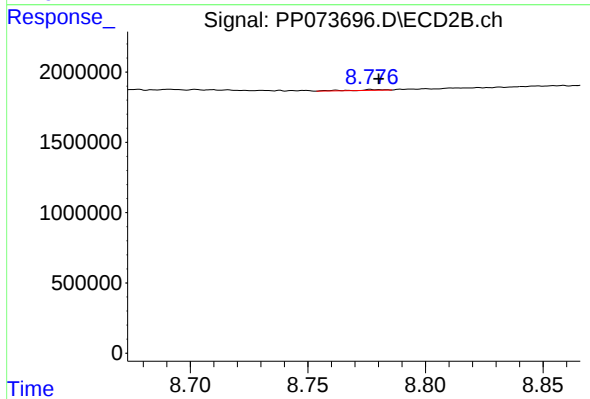

#2 Decachlorobiphenyl


R.T.: 8.777 min
Delta R.T.: -0.003 min
Response: 51956
Conc: 0.04 ng/ml

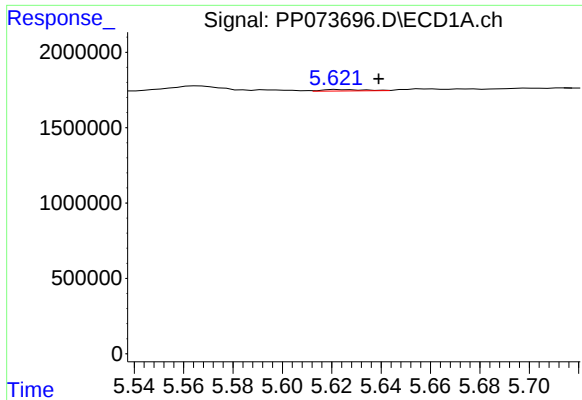

#3 AR-1016-1


R.T.: 5.622 min
Delta R.T.: -0.017 min
Response: 109707
Conc: 2.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

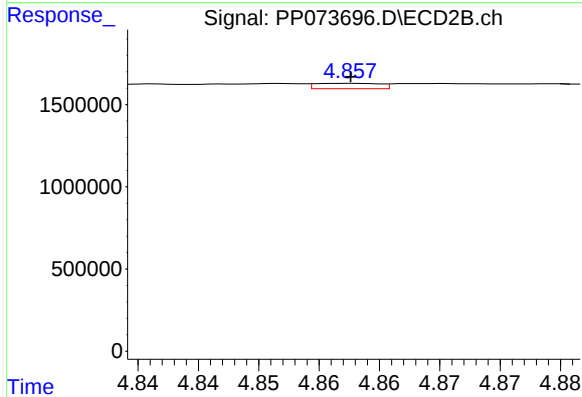


#3 AR-1016-1

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 121229
Conc: 1.78 ng/ml

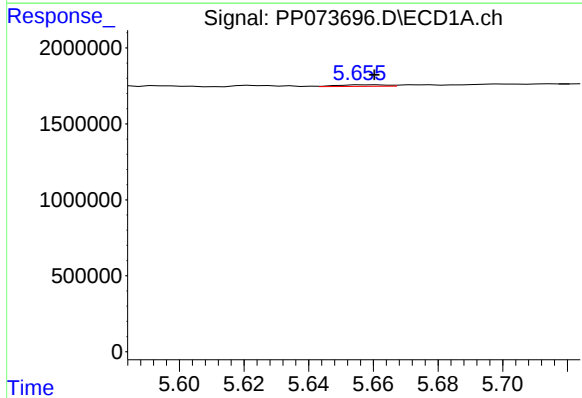


#4 AR-1016-2

R.T.: 5.656 min
Delta R.T.: -0.004 min
Response: 106862
Conc: 1.50 ng/ml

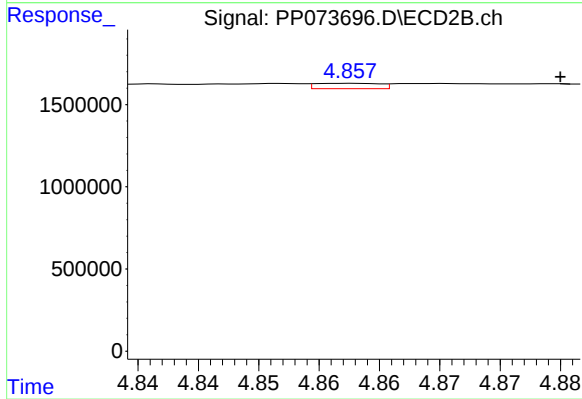

#4 AR-1016-2


R.T.: 4.858 min
Delta R.T.: -0.017 min
Response: 121229
Conc: 1.19 ng/ml

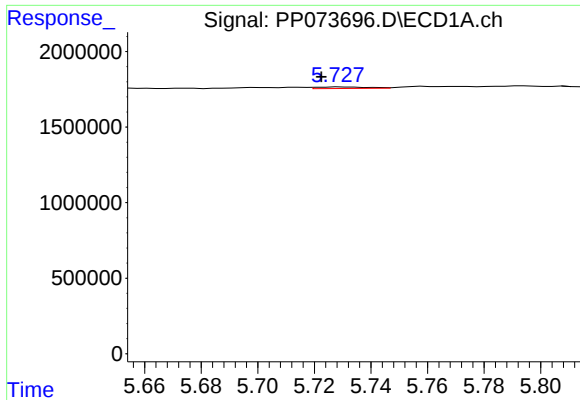

#5 AR-1016-3


R.T.: 5.729 min
Delta R.T.: 0.006 min
Response: 133366
Conc: 3.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

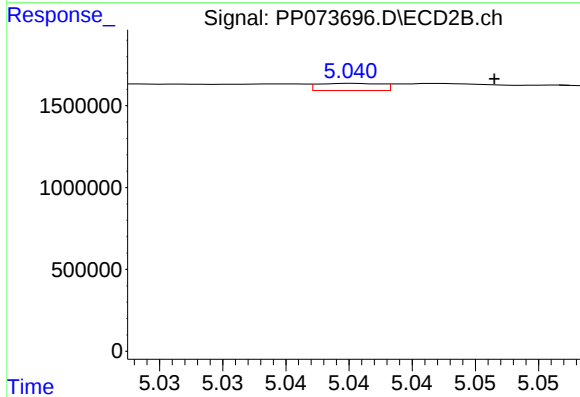


#5 AR-1016-3

R.T.: 5.040 min
Delta R.T.: -0.011 min
Response: 151694
Conc: 2.80 ng/ml

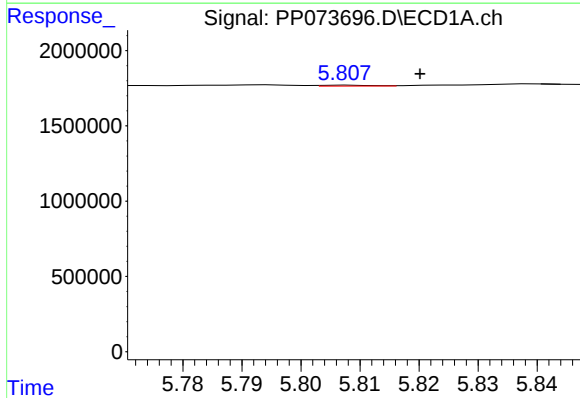


#6 AR-1016-4

R.T.: 5.808 min
Delta R.T.: -0.012 min
Response: 37701
Conc: 1.05 ng/ml

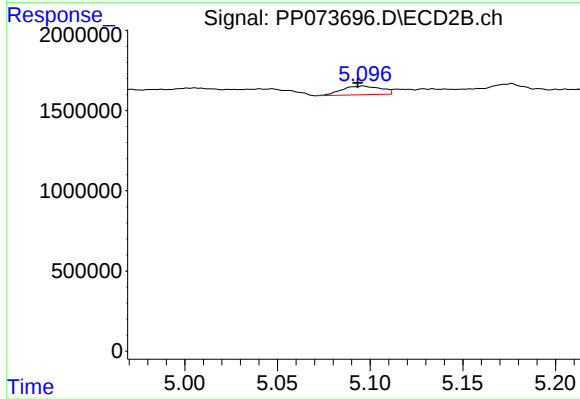

#6 AR-1016-4


R.T.: 5.096 min
Delta R.T.: 0.003 min
Response: 796328
Conc: 18.15 ng/ml

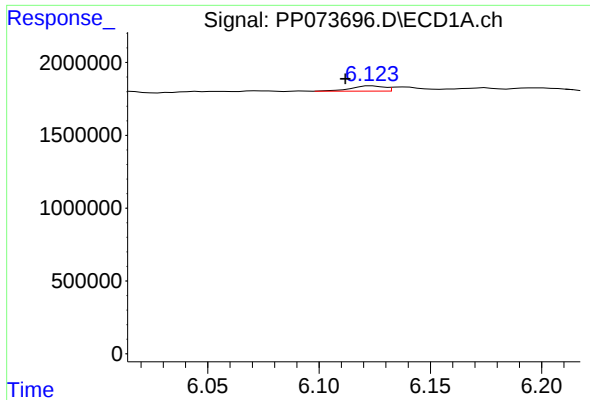

#7 AR-1016-5


R.T.: 6.124 min
Delta R.T.: 0.012 min
Response: 375972
Conc: 12.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

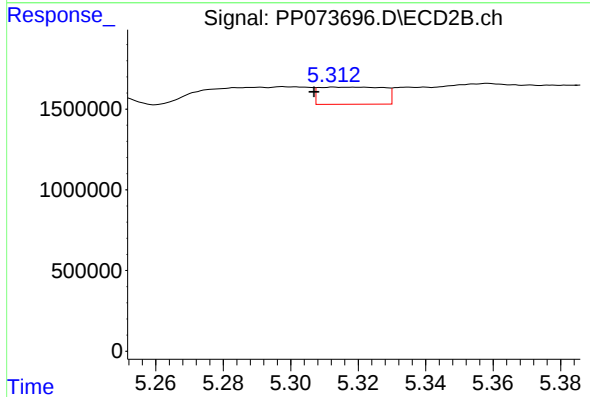


#7 AR-1016-5

R.T.: 5.313 min
Delta R.T.: 0.006 min
Response: 1408642
Conc: 25.81 ng/ml

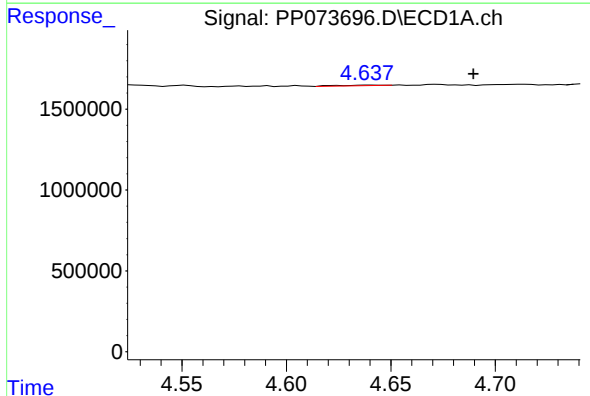


#8 AR-1221-1

R.T.: 4.640 min
Delta R.T.: -0.049 min
Response: 63982
Conc: 3.58 ng/ml

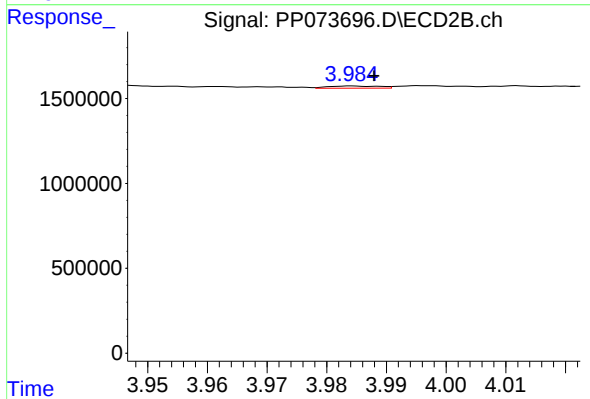

#8 AR-1221-1


R.T.: 3.984 min
Delta R.T.: -0.004 min
Response: 76652
Conc: 2.83 ng/ml

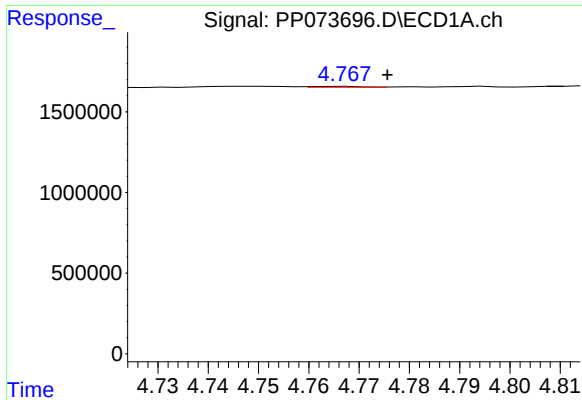

#9 AR-1221-2


R.T.: 4.767 min
Delta R.T.: -0.008 min
Response: 32764
Conc: 2.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

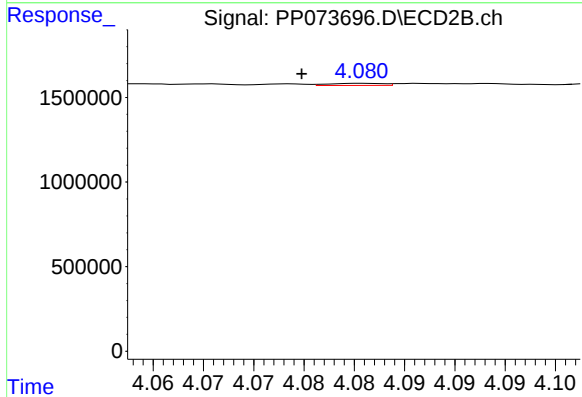


#9 AR-1221-2

R.T.: 4.081 min
Delta R.T.: 0.006 min
Response: 46542
Conc: 2.29 ng/ml

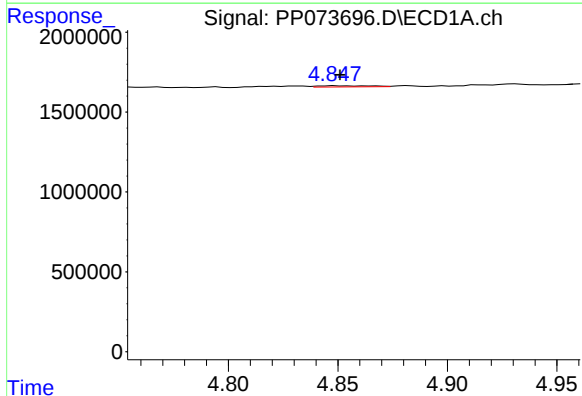


#10 AR-1221-3

R.T.: 4.848 min
Delta R.T.: -0.002 min
Response: 117502
Conc: 2.82 ng/ml

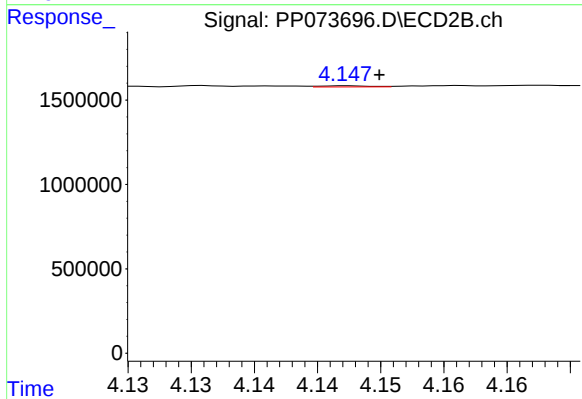

#10 AR-1221-3


R.T.: 4.147 min
Delta R.T.: -0.002 min
Response: 18191
Conc: 0.30 ng/ml

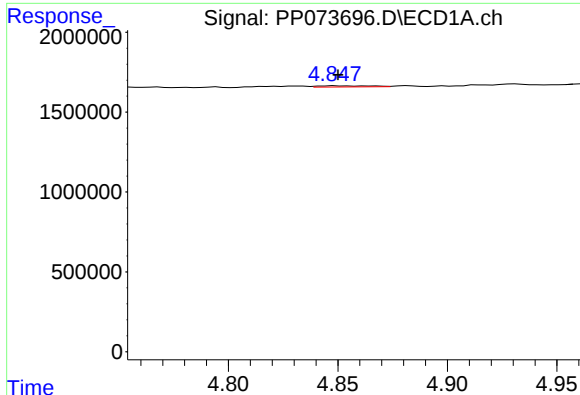

#11 AR-1232-1


R.T.: 4.848 min
Delta R.T.: -0.002 min
Response: 117502
Conc: 3.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

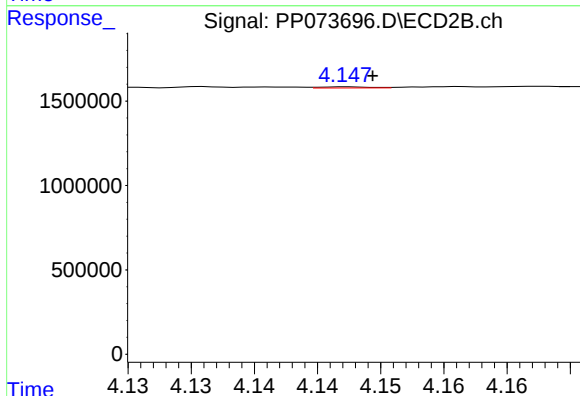


#11 AR-1232-1

R.T.: 4.147 min
Delta R.T.: -0.002 min
Response: 18191
Conc: 0.39 ng/ml

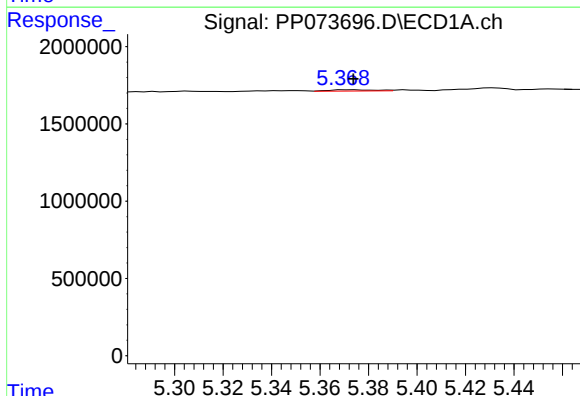


#12 AR-1232-2

R.T.: 5.370 min
Delta R.T.: -0.004 min
Response: 113596
Conc: 6.99 ng/ml

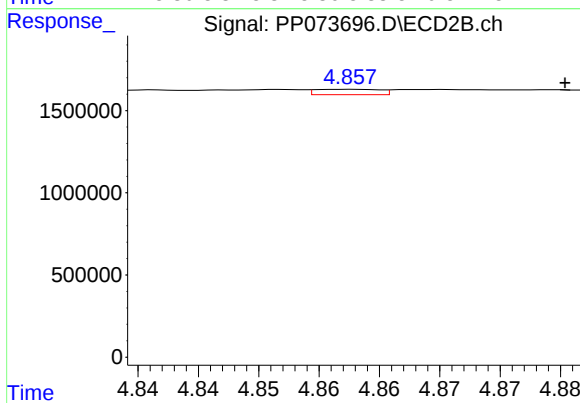

#12 AR-1232-2


R.T.: 4.858 min
Delta R.T.: -0.018 min
Response: 121229
Conc: 2.54 ng/ml

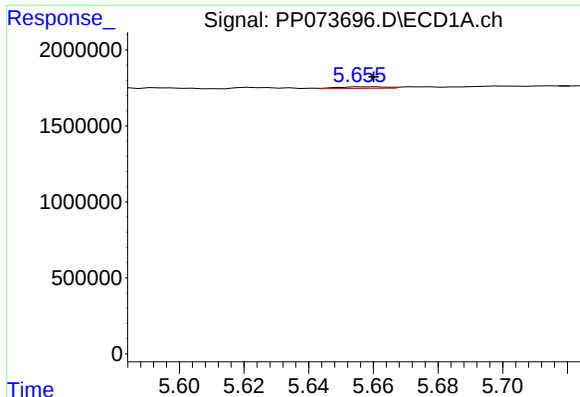

#13 AR-1232-3


R.T.: 5.656 min
Delta R.T.: -0.004 min
Response: 106862
Conc: 3.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

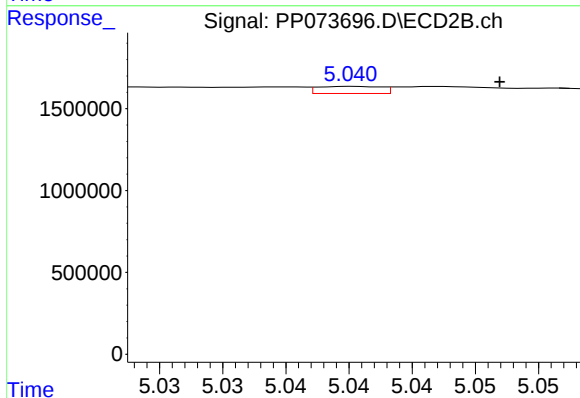


#13 AR-1232-3

R.T.: 5.040 min
Delta R.T.: -0.012 min
Response: 151694
Conc: 6.06 ng/ml

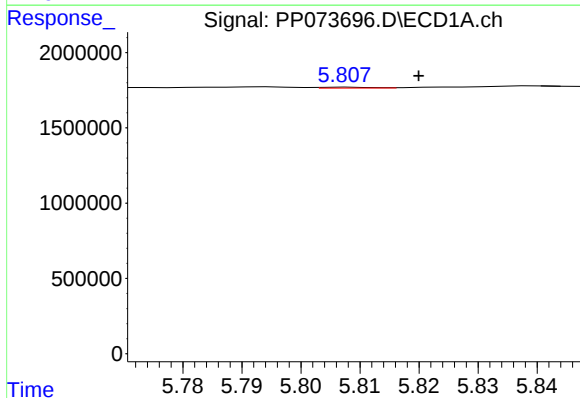


#14 AR-1232-4

R.T.: 5.808 min
Delta R.T.: -0.012 min
Response: 37701
Conc: 2.29 ng/ml

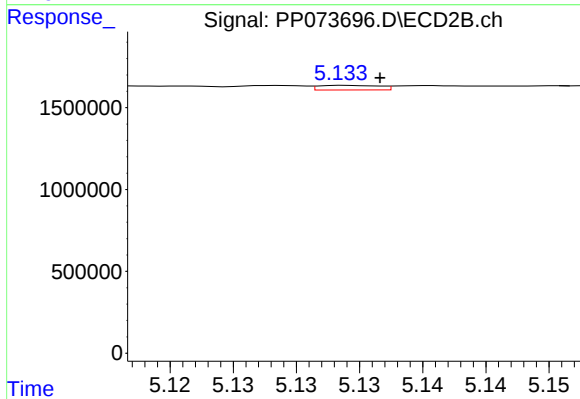

#14 AR-1232-4


R.T.: 5.134 min
Delta R.T.: -0.003 min
Response: 93496
Conc: 4.32 ng/ml

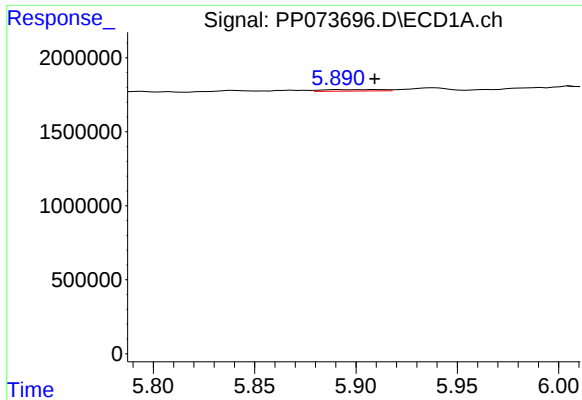

#15 AR-1232-5


R.T.: 5.891 min
Delta R.T.: -0.018 min
Response: 212499
Conc: 20.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

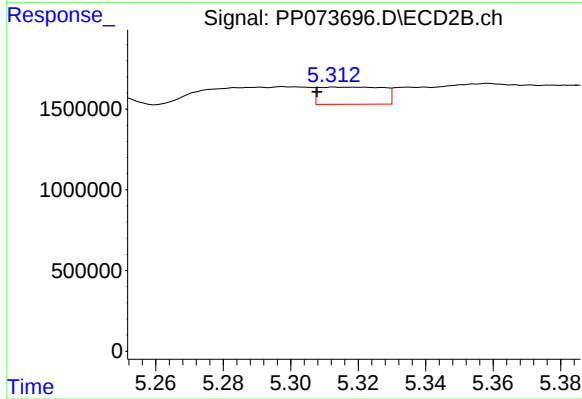


#15 AR-1232-5

R.T.: 5.313 min
Delta R.T.: 0.005 min
Response: 1408642
Conc: 62.43 ng/ml

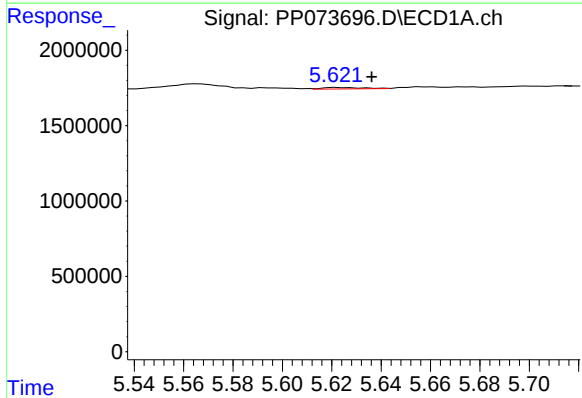


#16 AR-1242-1

R.T.: 5.622 min
Delta R.T.: -0.014 min
Response: 109707
Conc: 2.87 ng/ml

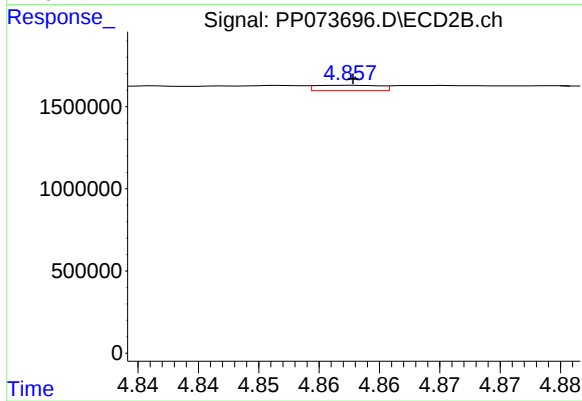

#16 AR-1242-1


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 121229
Conc: 2.10 ng/ml

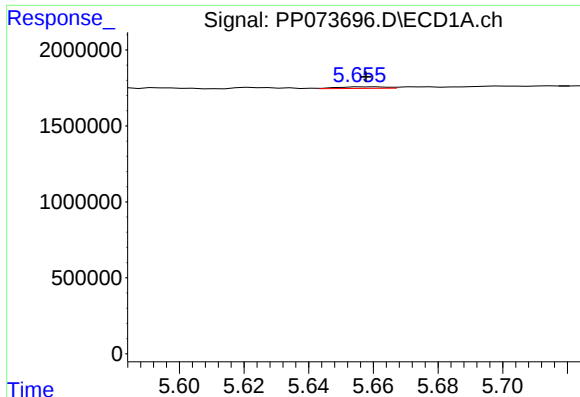

#17 AR-1242-2


R.T.: 5.656 min
Delta R.T.: -0.001 min
Response: 106862
Conc: 1.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

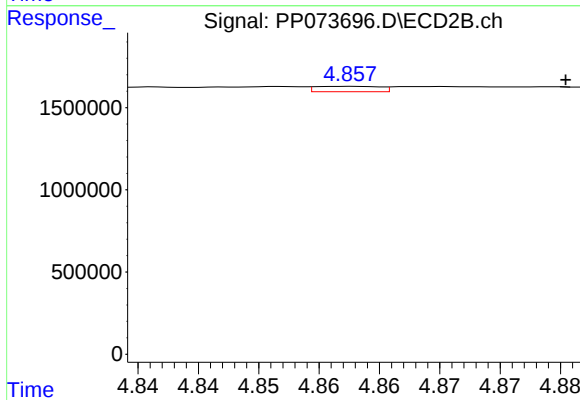


#17 AR-1242-2

R.T.: 4.858 min
Delta R.T.: -0.018 min
Response: 121229
Conc: 1.40 ng/ml

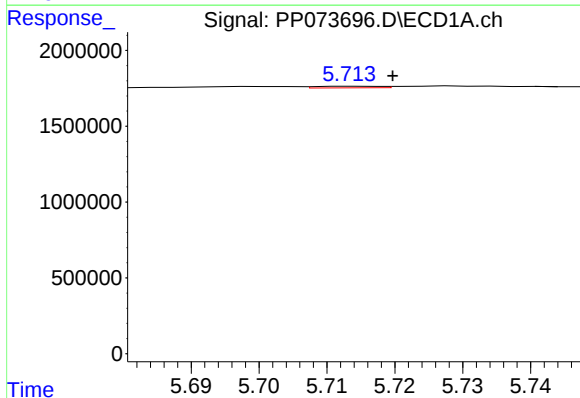


#18 AR-1242-3

R.T.: 5.715 min
Delta R.T.: -0.005 min
Response: 67738
Conc: 1.85 ng/ml

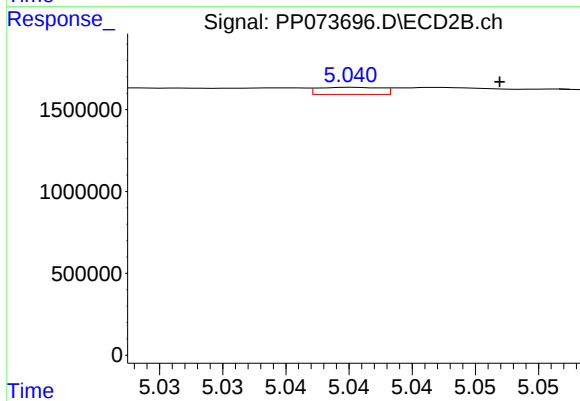

#18 AR-1242-3


R.T.: 5.040 min
Delta R.T.: -0.012 min
Response: 151694
Conc: 3.30 ng/ml

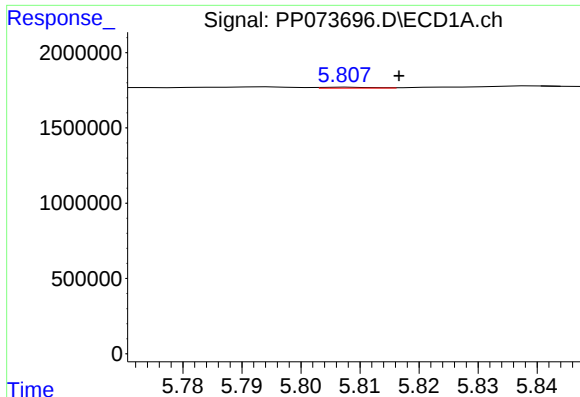

#19 AR-1242-4


R.T.: 5.808 min
Delta R.T.: -0.008 min
Response: 37701
Conc: 1.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

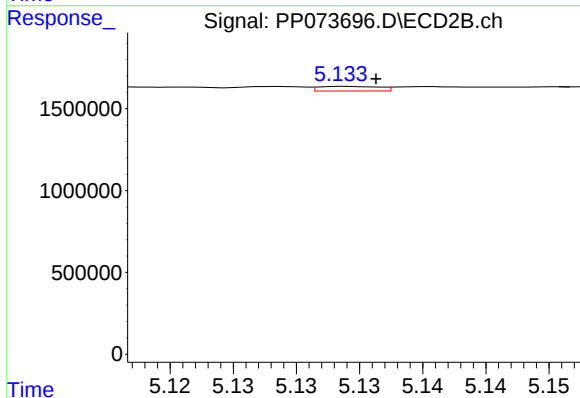


#19 AR-1242-4

R.T.: 5.134 min
Delta R.T.: -0.002 min
Response: 93496
Conc: 2.11 ng/ml

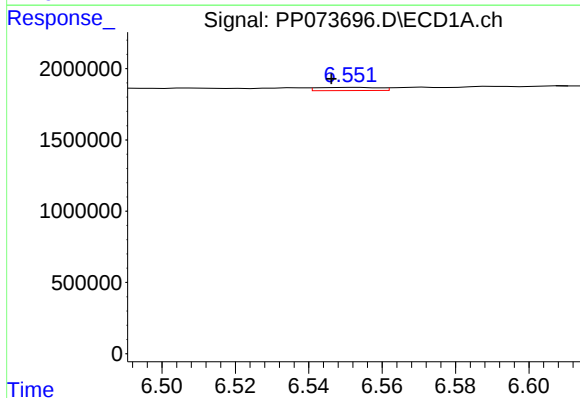


#20 AR-1242-5

R.T.: 6.553 min
Delta R.T.: 0.006 min
Response: 259357
Conc: 7.92 ng/ml

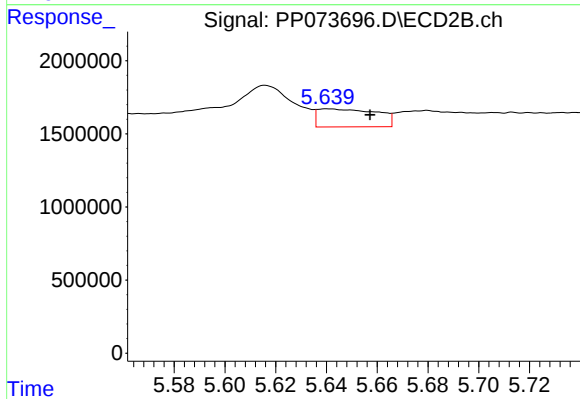

#20 AR-1242-5


R.T.: 5.640 min
Delta R.T.: -0.017 min
Response: 1991938
Conc: 36.06 ng/ml

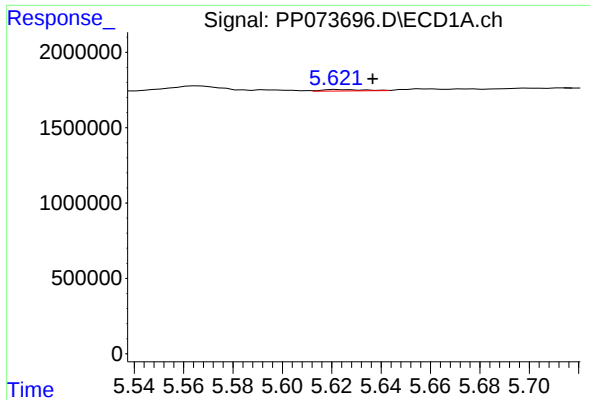

#21 AR-1248-1


R.T.: 5.622 min
Delta R.T.: -0.014 min
Response: 109707
Conc: 3.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

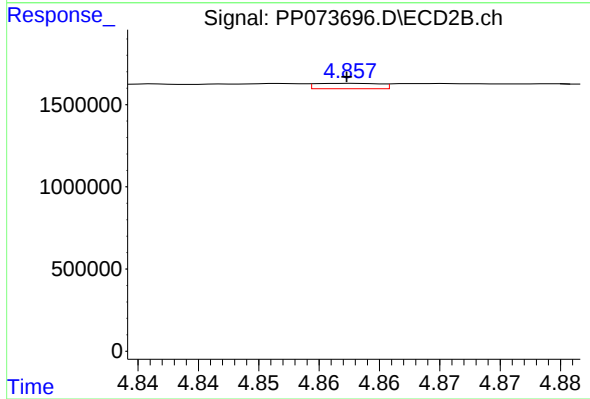


#21 AR-1248-1

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 121229
Conc: 2.70 ng/ml

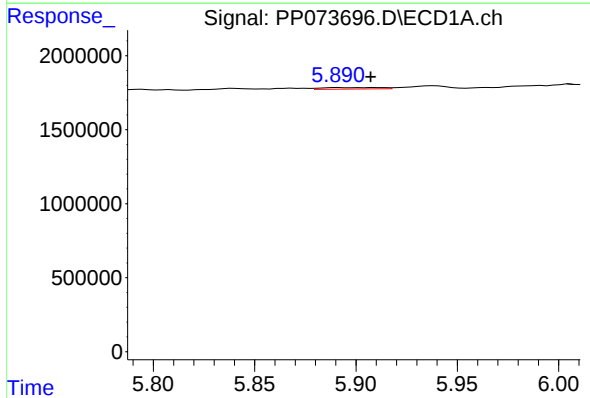


#22 AR-1248-2

R.T.: 5.891 min
Delta R.T.: -0.016 min
Response: 212499
Conc: 5.32 ng/ml

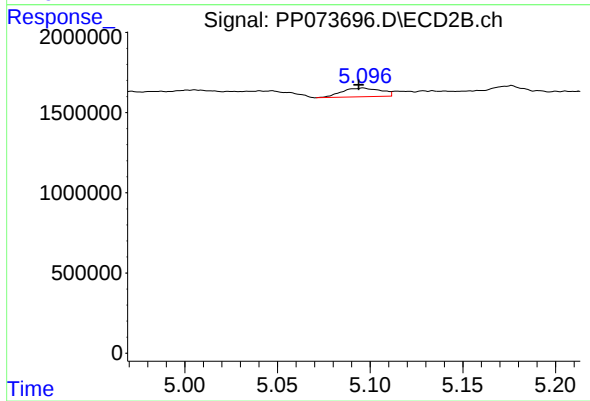

#22 AR-1248-2


R.T.: 5.096 min
Delta R.T.: 0.002 min
Response: 796328
Conc: 12.94 ng/ml

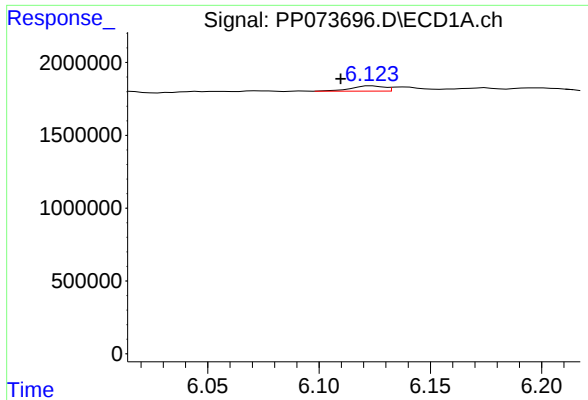

#23 AR-1248-3


R.T.: 6.124 min
Delta R.T.: 0.014 min
Response: 375972
Conc: 8.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

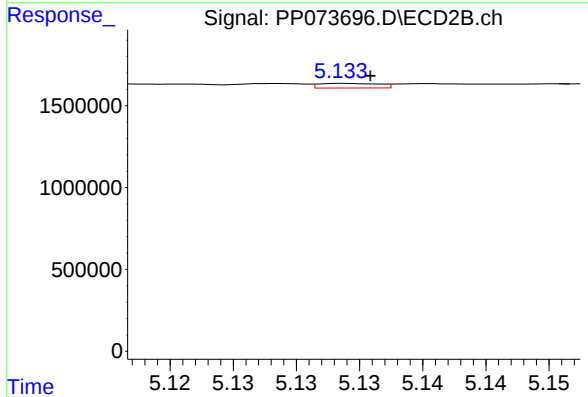


#23 AR-1248-3

R.T.: 5.134 min
Delta R.T.: -0.002 min
Response: 93496
Conc: 1.46 ng/ml

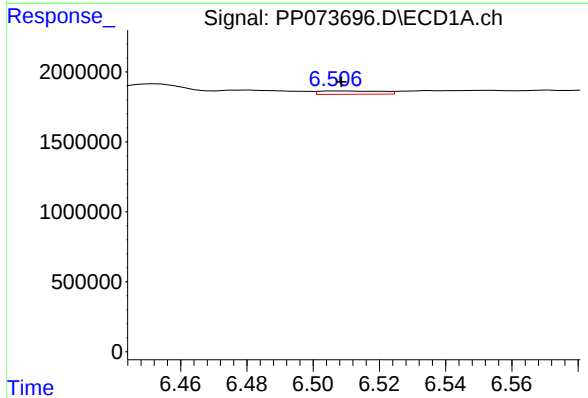


#24 AR-1248-4

R.T.: 6.508 min
Delta R.T.: 0.000 min
Response: 304089
Conc: 5.52 ng/ml

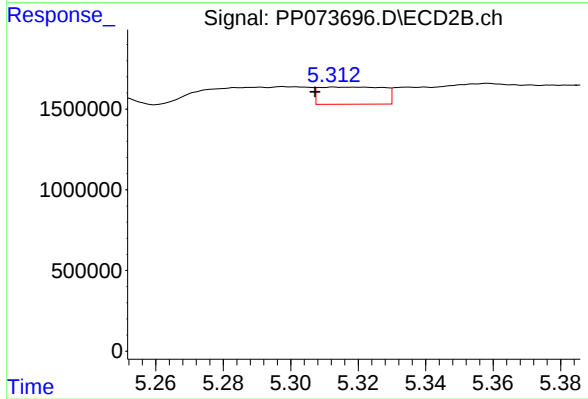

#24 AR-1248-4


R.T.: 5.313 min
Delta R.T.: 0.005 min
Response: 1408642
Conc: 18.69 ng/ml

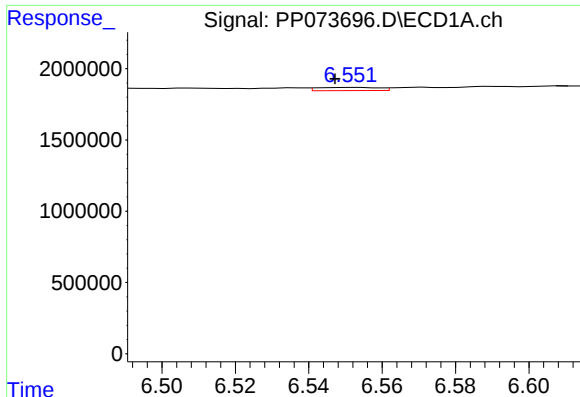

#25 AR-1248-5


R.T.: 6.553 min
Delta R.T.: 0.005 min
Response: 259357
Conc: 4.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

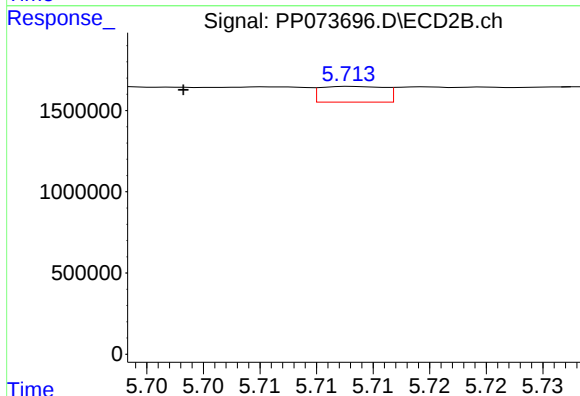


#25 AR-1248-5

R.T.: 5.713 min
Delta R.T.: 0.015 min
Response: 382478
Conc: 5.13 ng/ml

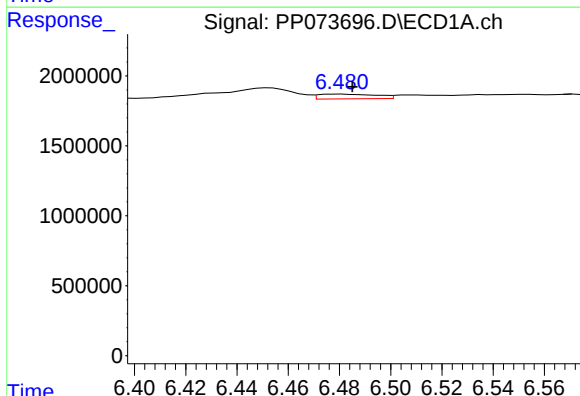


#26 AR-1254-1

R.T.: 6.481 min
Delta R.T.: -0.004 min
Response: 527162
Conc: 9.84 ng/ml

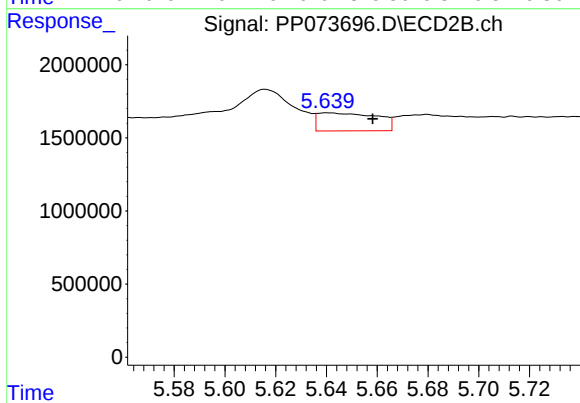

#26 AR-1254-1


R.T.: 5.640 min
Delta R.T.: -0.018 min
Response: 1991938
Conc: 17.17 ng/ml

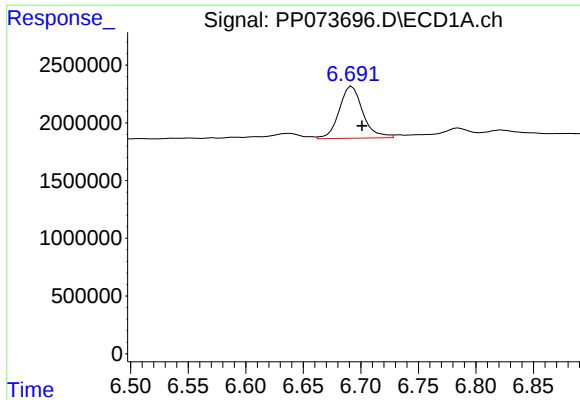

#27 AR-1254-2


R.T.: 6.692 min
Delta R.T.: -0.009 min
Response: 6433483
Conc: 77.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

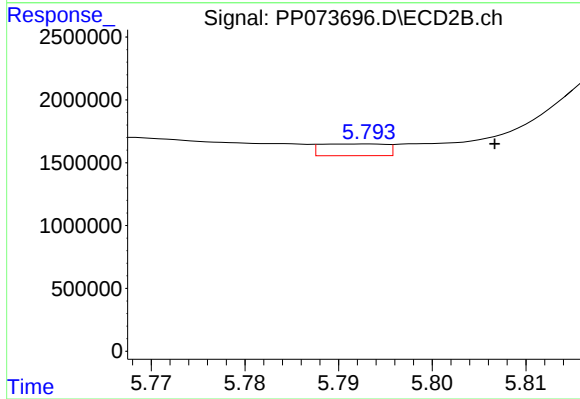


#27 AR-1254-2

R.T.: 5.793 min
Delta R.T.: -0.014 min
Response: 457231
Conc: 4.54 ng/ml

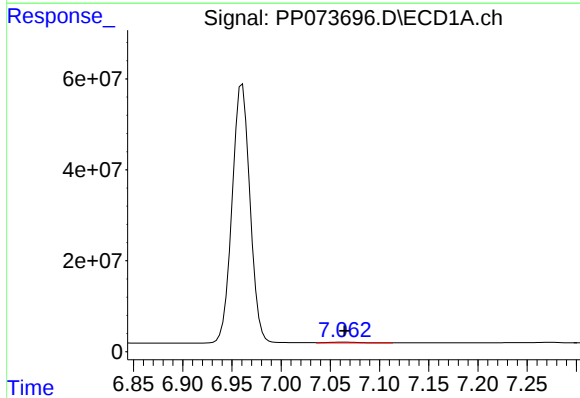


#28 AR-1254-3

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 4682201
Conc: 53.01 ng/ml

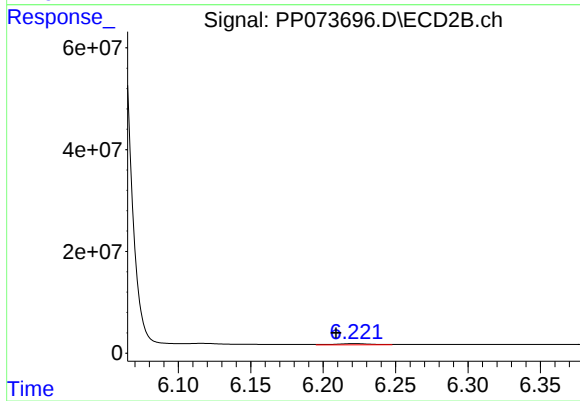

#28 AR-1254-3


R.T.: 6.221 min
Delta R.T.: 0.012 min
Response: 4105661
Conc: 26.58 ng/ml

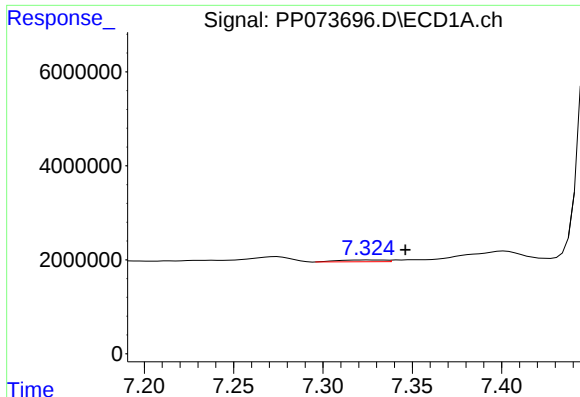

#29 AR-1254-4


R.T.: 7.325 min
Delta R.T.: -0.021 min
Response: 722349
Conc: 9.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

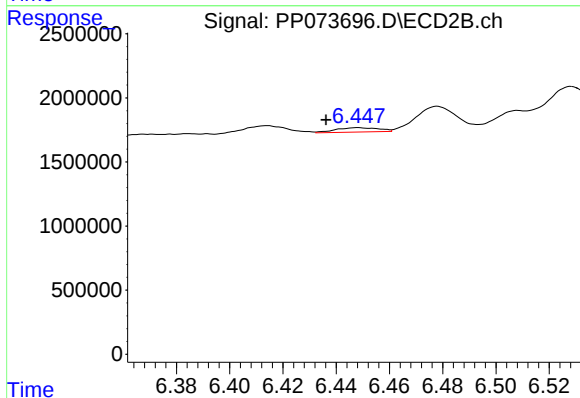


#29 AR-1254-4

R.T.: 6.448 min
Delta R.T.: 0.012 min
Response: 383639
Conc: 4.06 ng/ml

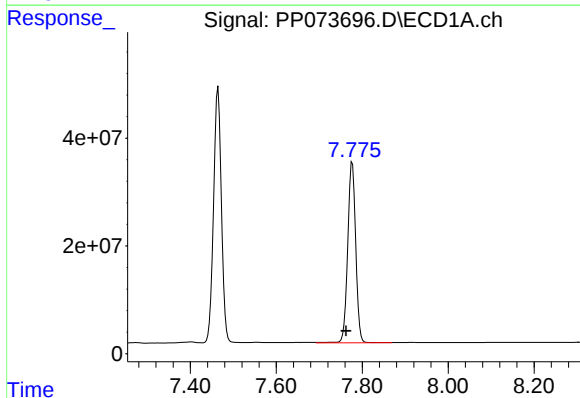


#30 AR-1254-5

R.T.: 7.777 min
Delta R.T.: 0.015 min
Response: 435335212
Conc: 5908.47 ng/ml

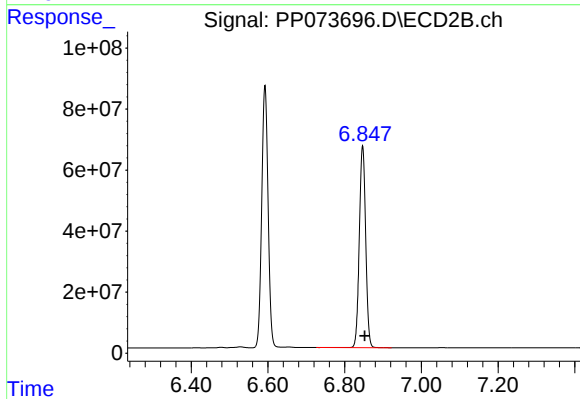

#30 AR-1254-5


R.T.: 6.847 min
Delta R.T.: -0.006 min
Response: 765216639
Conc: 5734.33 ng/ml

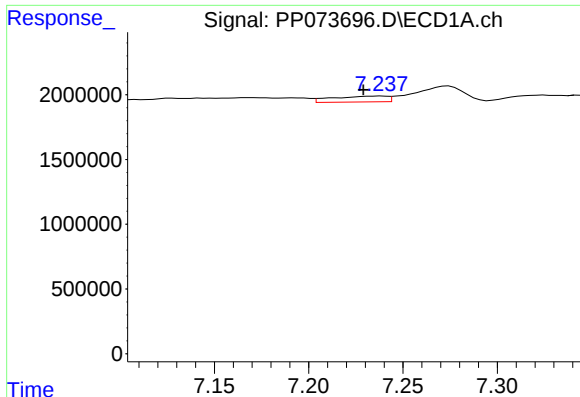

#31 AR-1260-1


R.T.: 7.239 min
Delta R.T.: 0.010 min
Response: 921558
Conc: 15.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

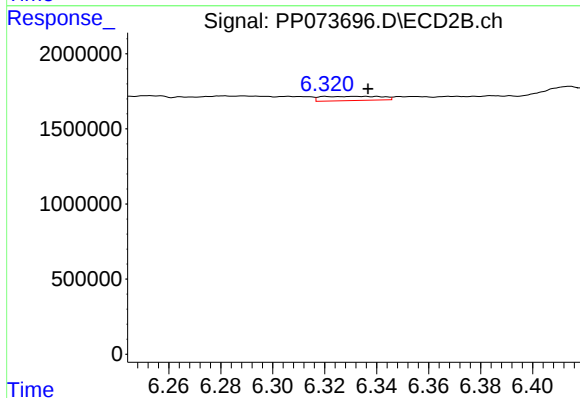


#31 AR-1260-1

R.T.: 6.321 min
Delta R.T.: -0.016 min
Response: 447870
Conc: 4.59 ng/ml

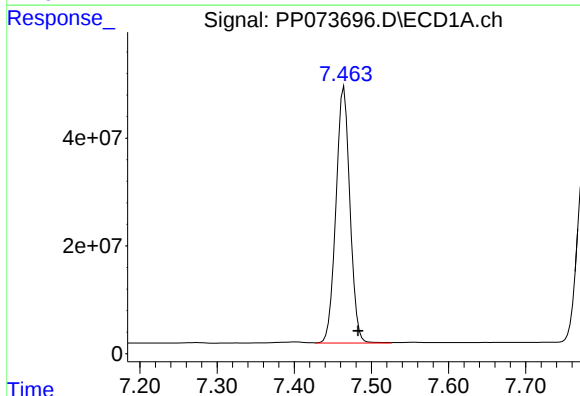


#32 AR-1260-2

R.T.: 7.465 min
Delta R.T.: -0.018 min
Response: 599997972
Conc: 6260.42 ng/ml

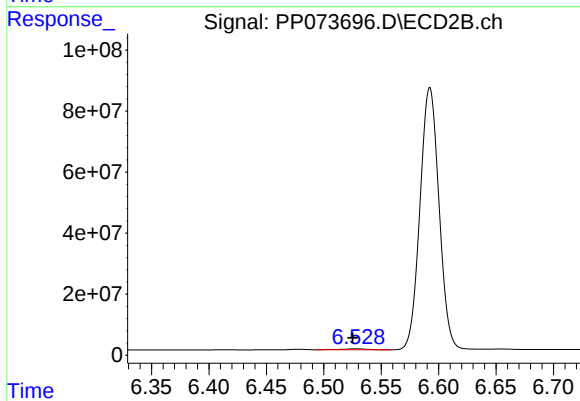

#32 AR-1260-2


R.T.: 6.528 min
Delta R.T.: 0.003 min
Response: 5516595
Conc: 44.91 ng/ml

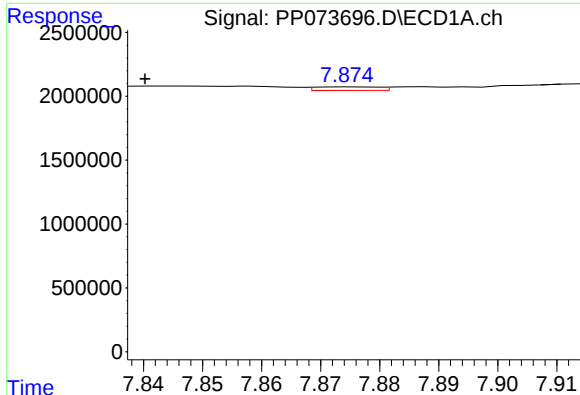

#33 AR-1260-3


R.T.: 7.876 min
Delta R.T.: 0.036 min
Response: 209720
Conc: 2.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

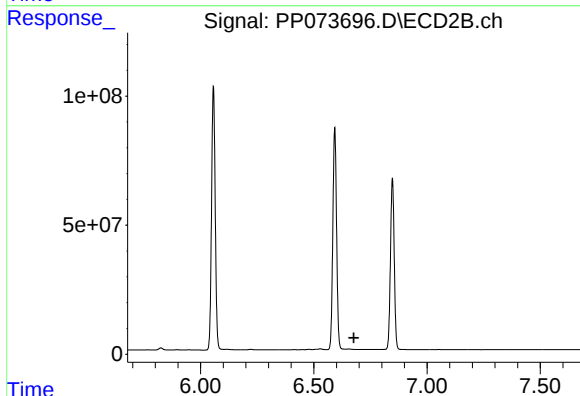


#33 AR-1260-3

R.T.: 6.655 min
Delta R.T.: -0.022 min
Response: -1018886
Conc: N.D.

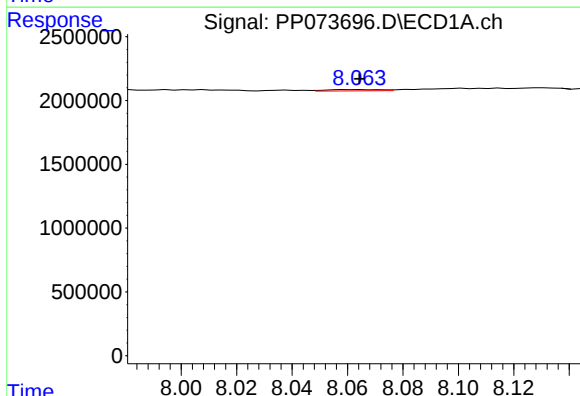


#34 AR-1260-4

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 135681
Conc: 2.08 ng/ml

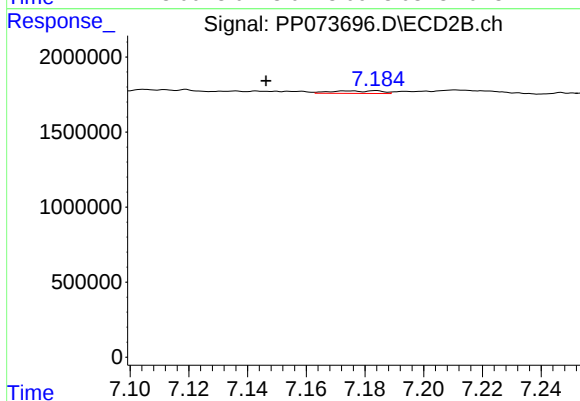

#34 AR-1260-4


R.T.: 7.174 min
Delta R.T.: 0.028 min
Response: 208685
Conc: 2.33 ng/ml

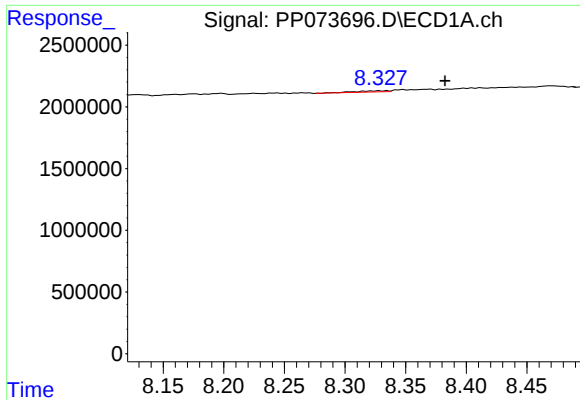

#35 AR-1260-5


R.T.: 8.329 min
Delta R.T.: -0.054 min
Response: 169265
Conc: 1.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

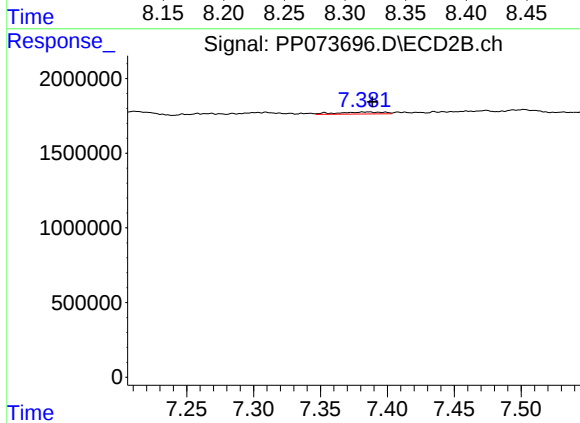


#35 AR-1260-5

R.T.: 7.386 min
Delta R.T.: -0.002 min
Response: 322024
Conc: 1.43 ng/ml

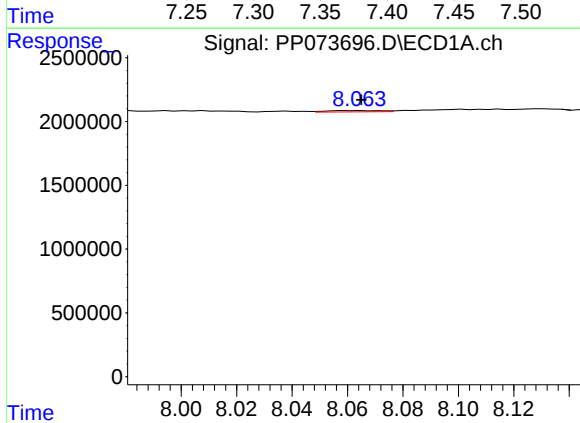


#36 AR-1262-1

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 135681
Conc: 1.56 ng/ml

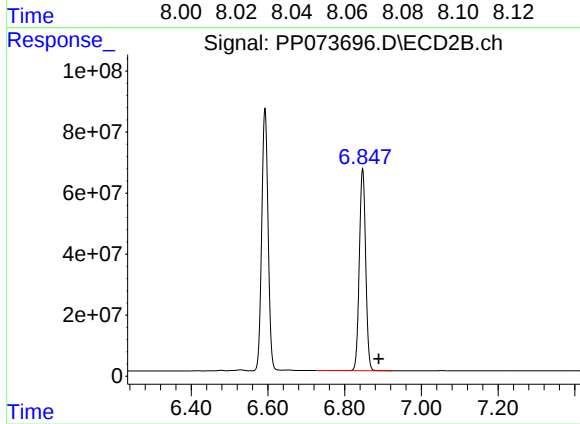

#36 AR-1262-1


R.T.: 6.847 min
Delta R.T.: -0.042 min
Response: 765216639
Conc: 5181.18 ng/ml

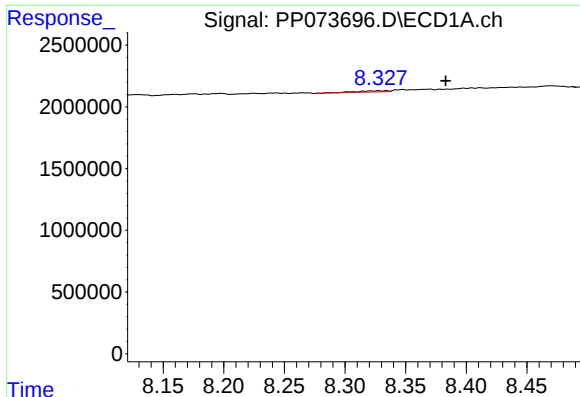

#37 AR-1262-2


R.T.: 8.329 min
Delta R.T.: -0.055 min
Response: 169265
Conc: 0.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

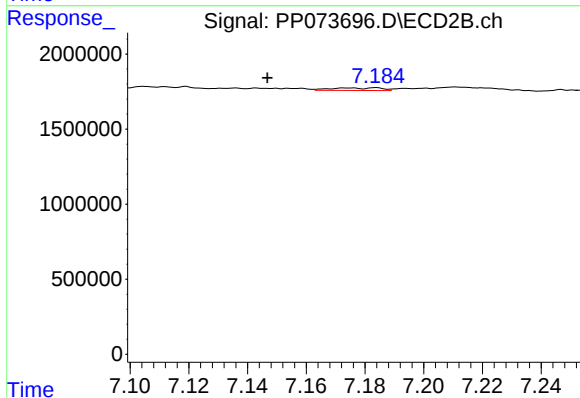


#37 AR-1262-2

R.T.: 7.174 min
Delta R.T.: 0.028 min
Response: 208685
Conc: 1.63 ng/ml

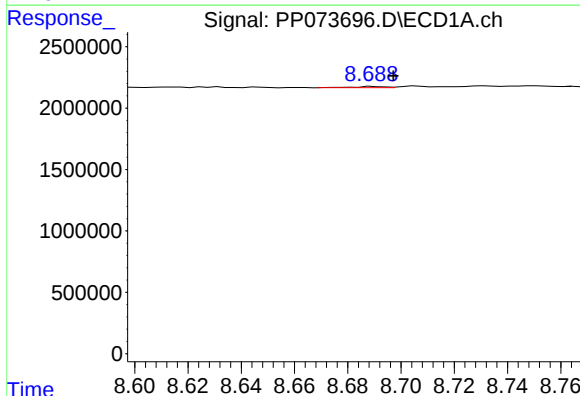


#38 AR-1262-3

R.T.: 8.690 min
Delta R.T.: -0.008 min
Response: 83961
Conc: 0.67 ng/ml

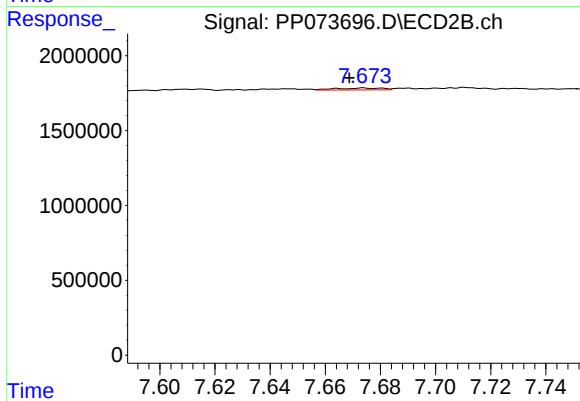

#38 AR-1262-3


R.T.: 7.674 min
Delta R.T.: 0.005 min
Response: 153392
Conc: 1.35 ng/ml

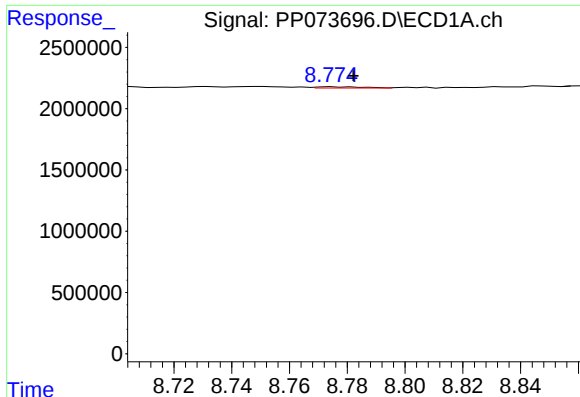

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.007 min
Response: 116756
Conc: 1.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

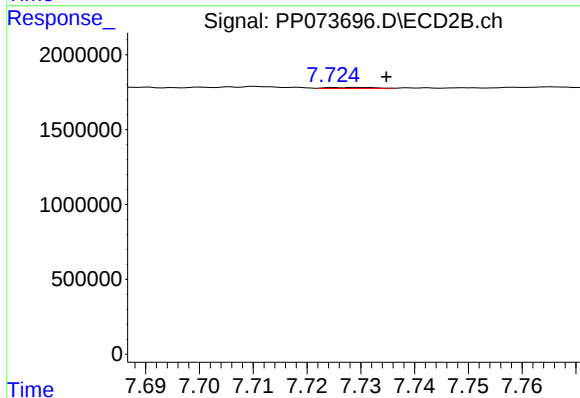


#39 AR-1262-4

R.T.: 7.730 min
Delta R.T.: -0.005 min
Response: 42973
Conc: 0.23 ng/ml

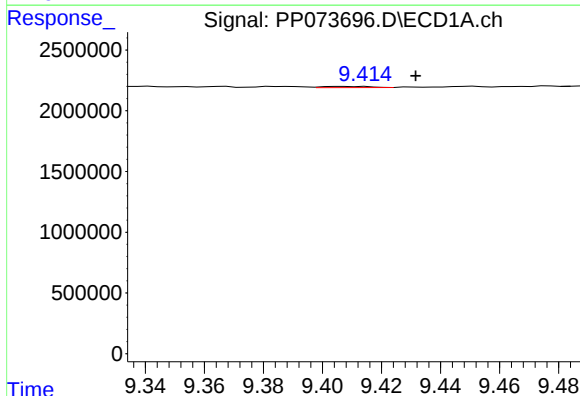


#40 AR-1262-5

R.T.: 9.408 min
Delta R.T.: -0.024 min
Response: 107288
Conc: 1.69 ng/ml

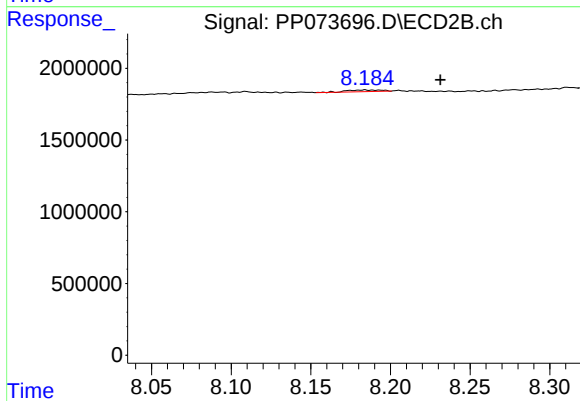

#40 AR-1262-5


R.T.: 8.184 min
Delta R.T.: -0.047 min
Response: 185565
Conc: 2.20 ng/ml

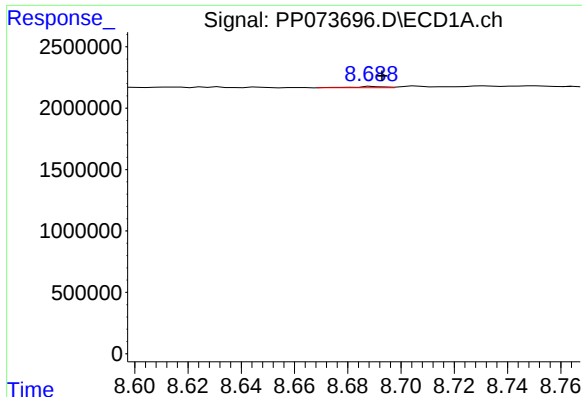

#41 AR-1268-1


R.T.: 8.690 min
Delta R.T.: -0.003 min
Response: 83961
Conc: 0.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

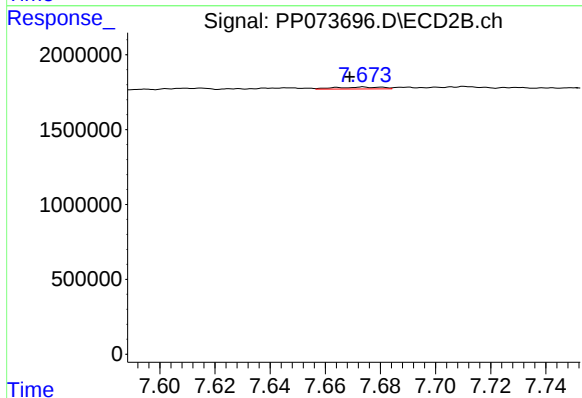


#41 AR-1268-1

R.T.: 7.674 min
Delta R.T.: 0.005 min
Response: 153392
Conc: 0.50 ng/ml

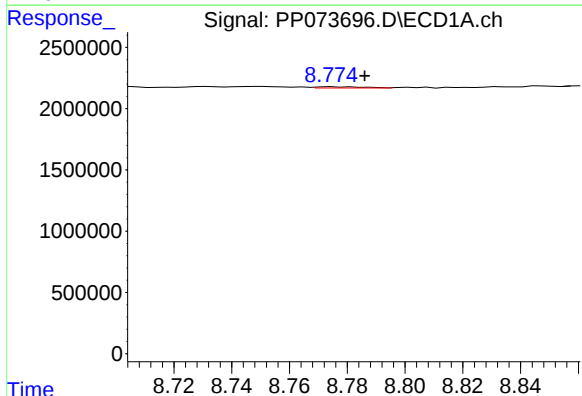


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.011 min
Response: 116756
Conc: 0.61 ng/ml

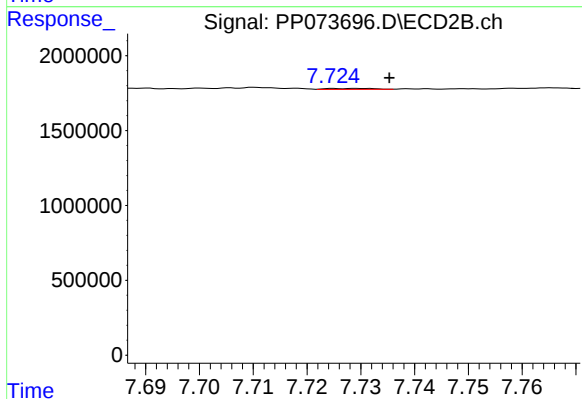

#42 AR-1268-2


R.T.: 7.730 min
Delta R.T.: -0.006 min
Response: 42973
Conc: 0.16 ng/ml

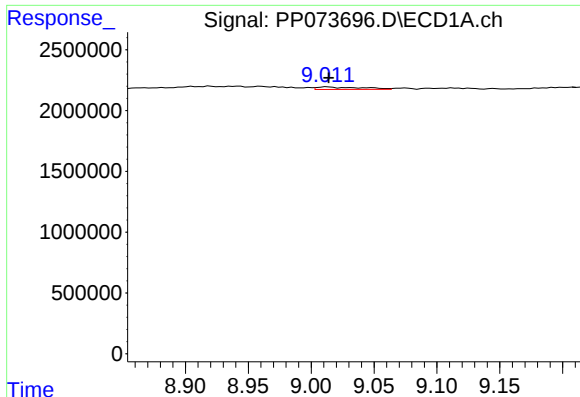

#43 AR-1268-3


R.T.: 9.013 min
Delta R.T.: -0.001 min
Response: 491080
Conc: 2.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

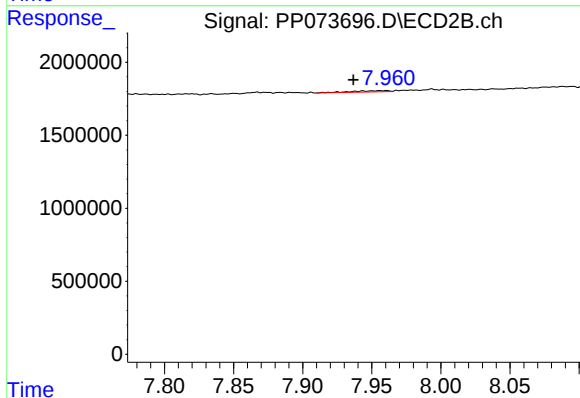


#43 AR-1268-3

R.T.: 7.961 min
Delta R.T.: 0.024 min
Response: 164934
Conc: 0.73 ng/ml

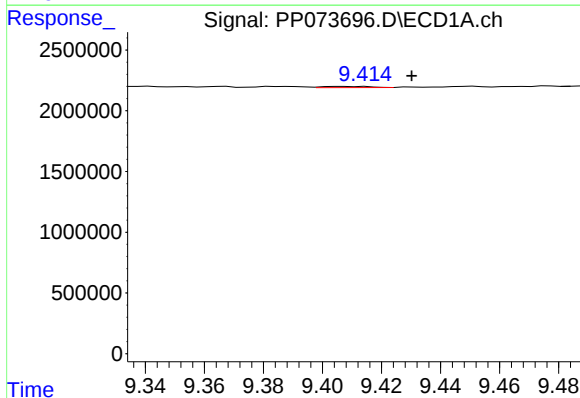


#44 AR-1268-4

R.T.: 9.408 min
Delta R.T.: -0.023 min
Response: 107288
Conc: 1.54 ng/ml

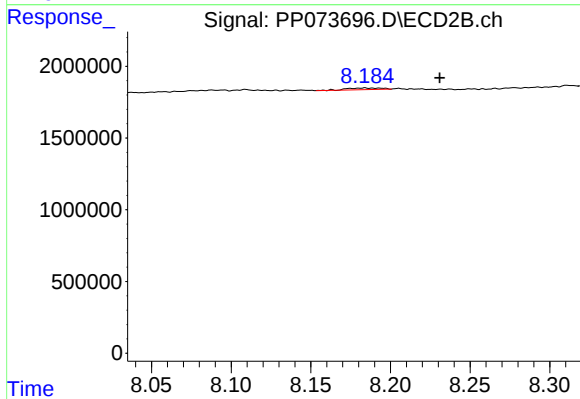

#44 AR-1268-4


R.T.: 8.184 min
Delta R.T.: -0.047 min
Response: 185565
Conc: 2.00 ng/ml

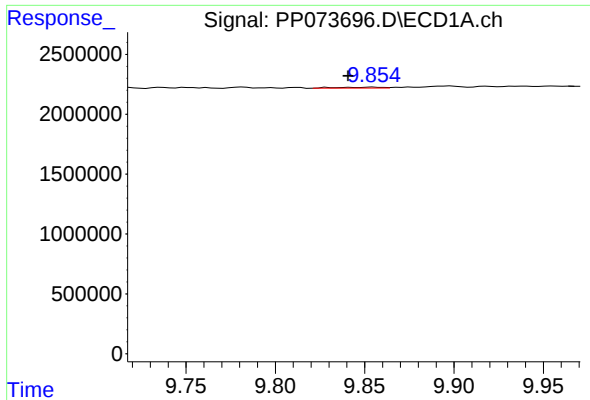

#45 AR-1268-5

R.T.: 9.855 min
Delta R.T.: 0.014 min
Response: 122915
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

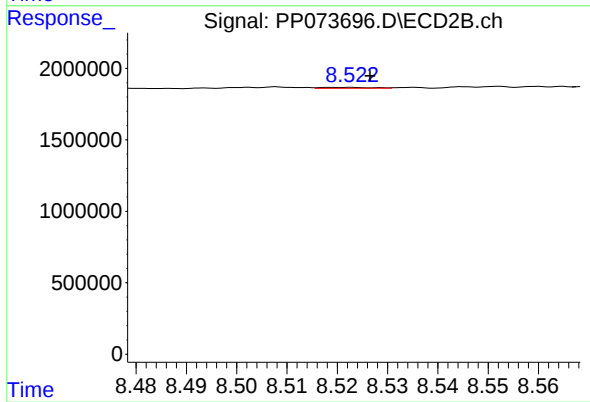

#45 AR-1268-5

R.T.: 8.522 min
Delta R.T.: -0.004 min
Response: 44059
Conc: 0.07 ng/ml