

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071221\
 Data File : PP037227.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jul 2021 13:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 15:33:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.957	3.948	965389	568440	21.241	20.773
2)	SA Decachlor...	10.986	9.241	1039224	599261	22.574	21.529
Target Compounds							
8)	L2 AR-1221-1	5.207	0.000	26903	0	50.725	N.D. #
9)	L2 AR-1221-2	5.308	0.000	12726	0	31.413	N.D. #
15)	L3 AR-1232-5	6.566	0.000	17354	0	45.123	N.D. #
22)	L5 AR-1248-2	6.566	0.000	17354	0	11.689	N.D. #
24)	L5 AR-1248-4	7.193f	0.000	10340	0	5.471	N.D. #
26)	L6 AR-1254-1	7.193	0.000	10340	0	5.756	N.D. #
28)	L6 AR-1254-3	7.814	0.000	14872	0	4.824	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071221\
Data File : PP037227.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2021 13:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 15:33:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

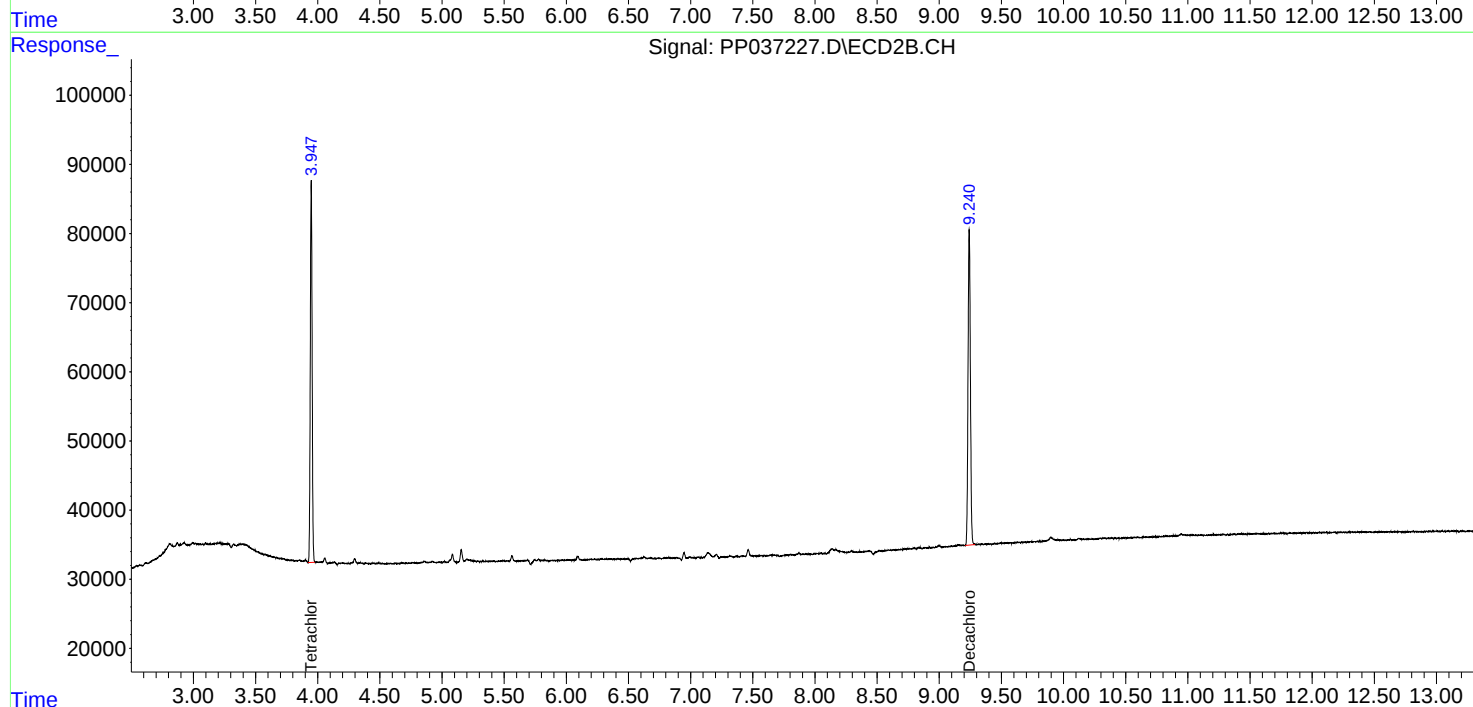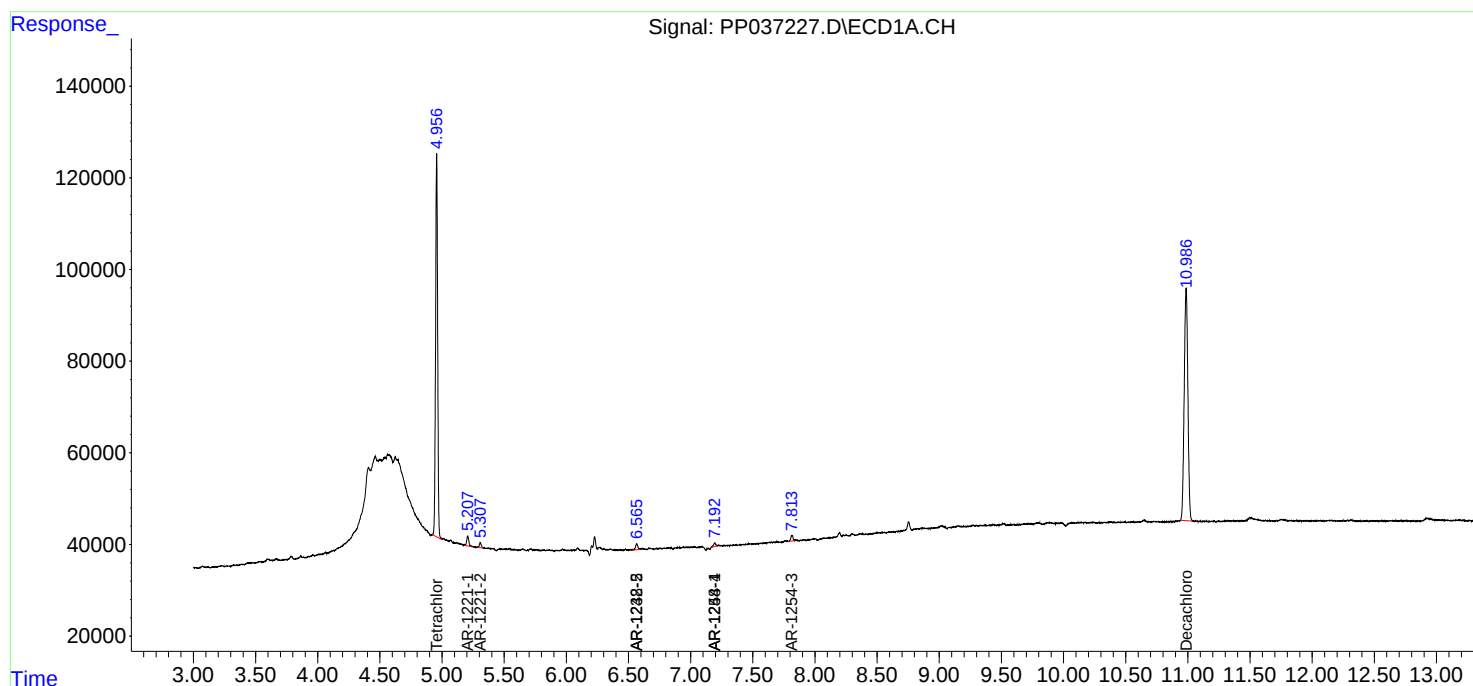


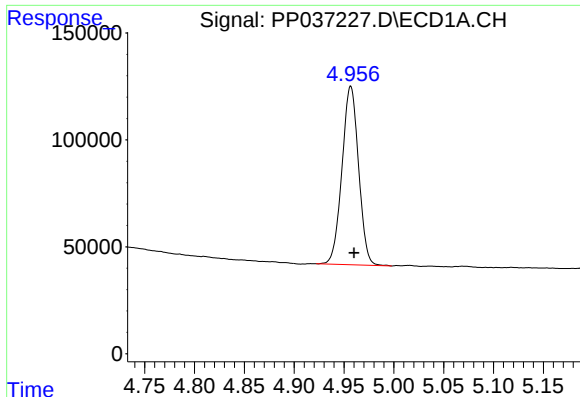

#1 Tetrachloro-m-xylene


R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 965389
Conc: 21.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

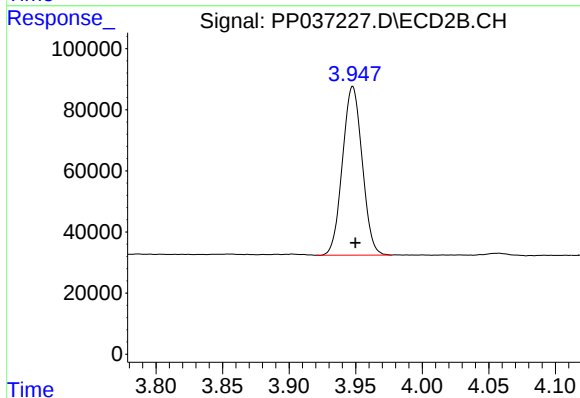


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 568440
Conc: 20.77 ng/ml

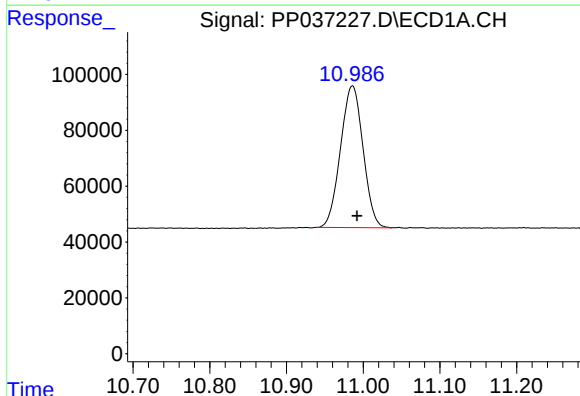


#2 Decachlorobiphenyl

R.T.: 10.986 min
Delta R.T.: -0.006 min
Response: 1039224
Conc: 22.57 ng/ml

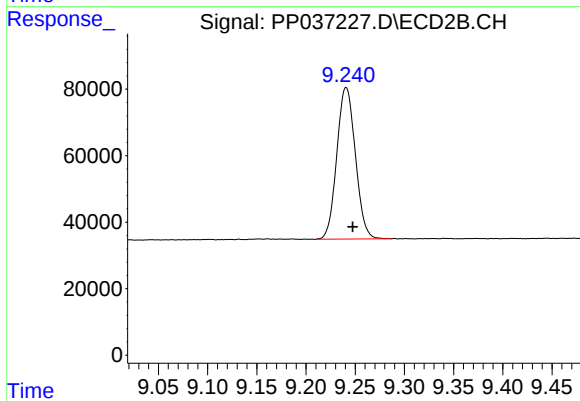

#2 Decachlorobiphenyl


R.T.: 9.241 min
Delta R.T.: -0.007 min
Response: 599261
Conc: 21.53 ng/ml

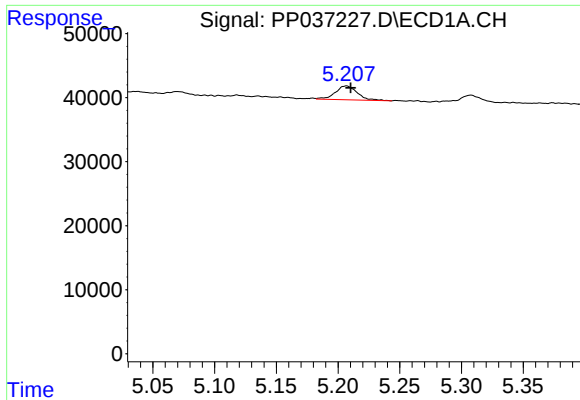

#8 AR-1221-1


R.T.: 5.207 min
Delta R.T.: -0.003 min
Response: 26903
Conc: 50.72 ng/ml

Instrument :
ECD_P
ClientSampleId :

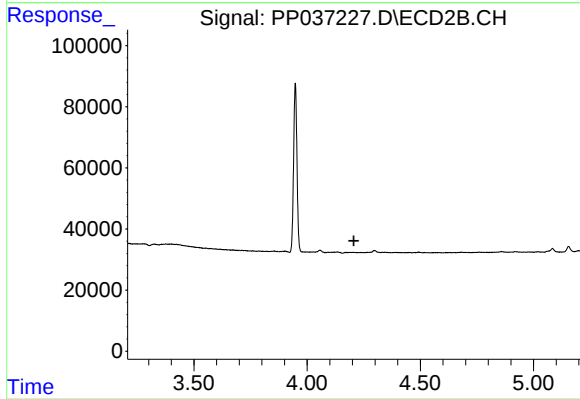


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

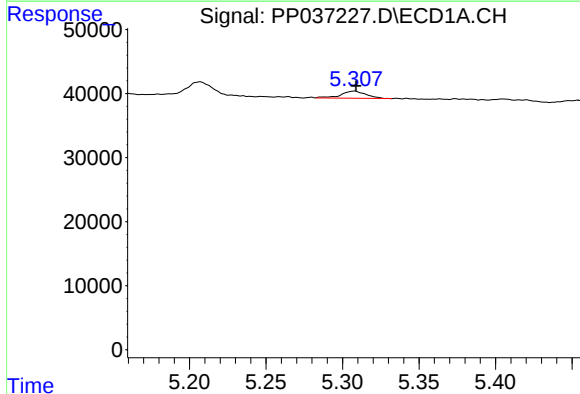


#9 AR-1221-2

R.T.: 5.308 min
Delta R.T.: -0.001 min
Response: 12726
Conc: 31.41 ng/ml

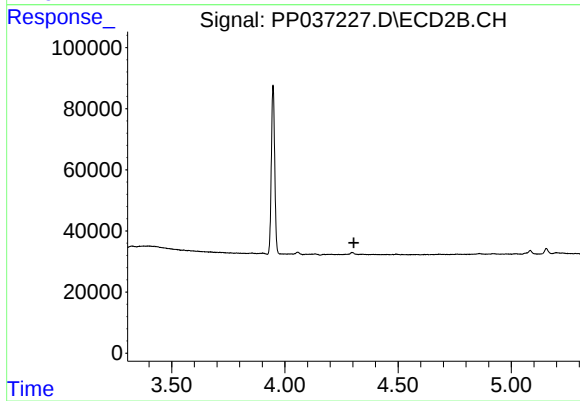

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

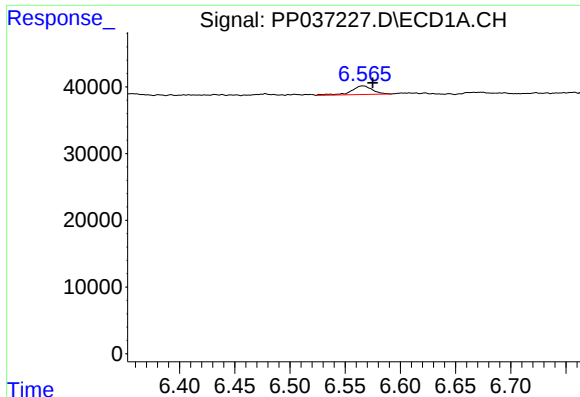

#15 AR-1232-5


R.T.: 6.566 min
Delta R.T.: -0.009 min
Response: 17354
Conc: 45.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

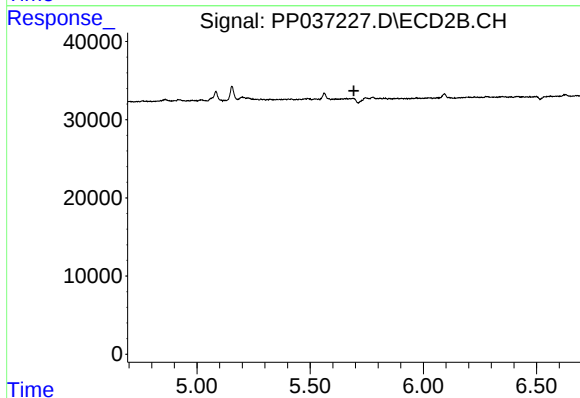


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.694 min
Response: 0
Conc: N.D.

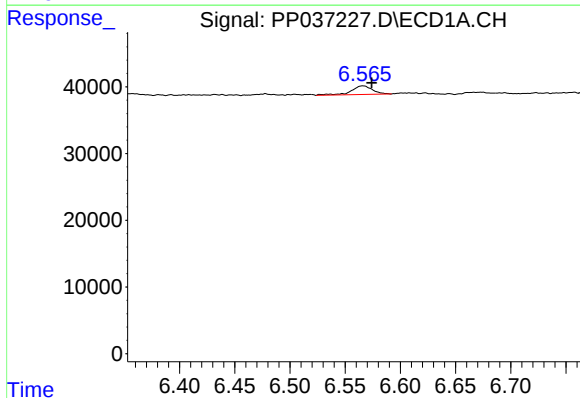


#22 AR-1248-2

R.T.: 6.566 min
Delta R.T.: -0.008 min
Response: 17354
Conc: 11.69 ng/ml

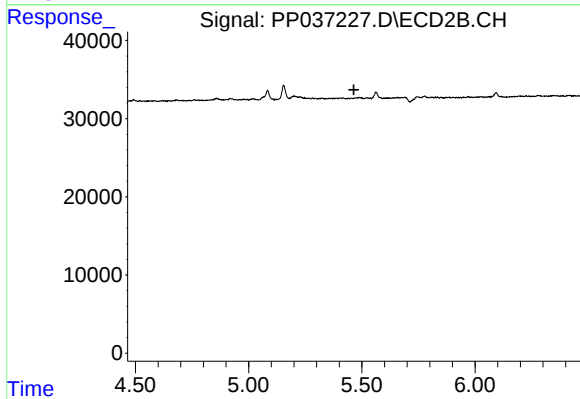

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.465 min
Response: 0
Conc: N.D.

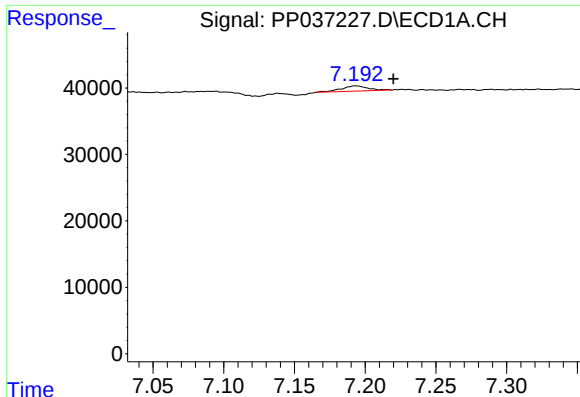

#24 AR-1248-4


R.T.: 7.193 min
Delta R.T.: -0.027 min
Response: 10340
Conc: 5.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

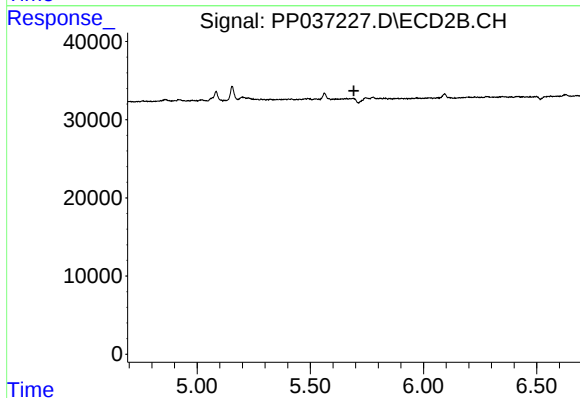


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

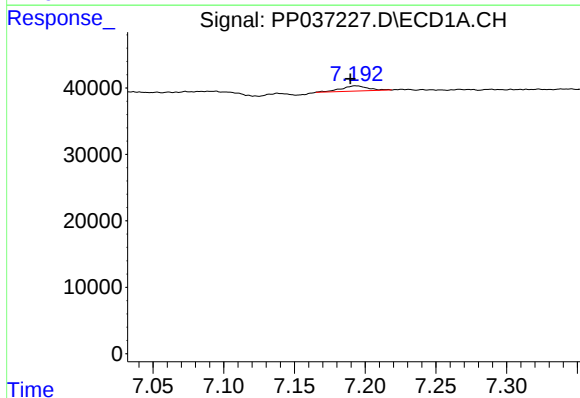


#26 AR-1254-1

R.T.: 7.193 min
Delta R.T.: 0.003 min
Response: 10340
Conc: 5.76 ng/ml

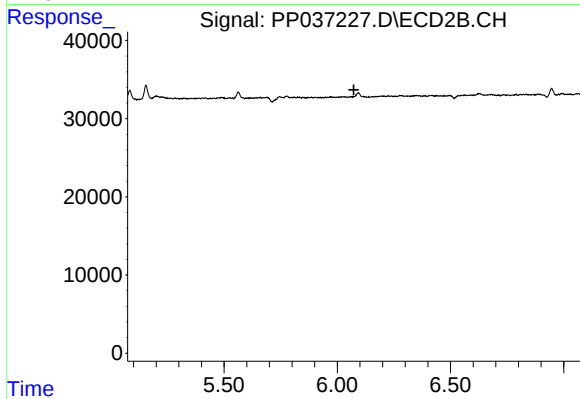

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

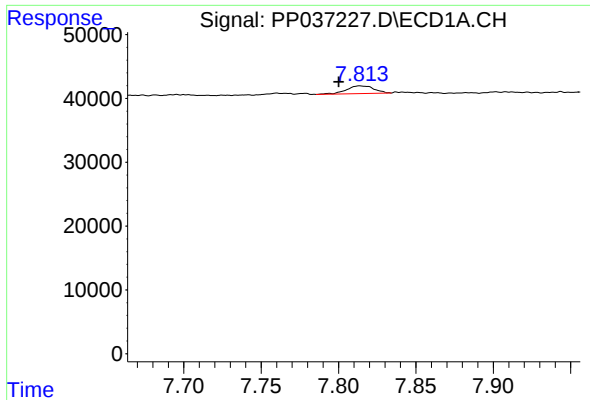

#28 AR-1254-3

R.T.: 7.814 min
Delta R.T.: 0.014 min
Response: 14872
Conc: 4.82 ng/ml

Instrument :
ECD_P
ClientSampleId :

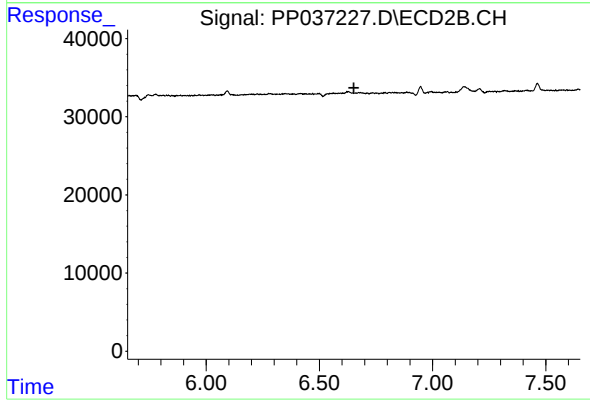

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.