

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071221\
 Data File : PP037243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jul 2021 18:01
 Operator : DD\AJ
 Sample : PB137615BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB137615BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 05:38:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.956	3.947	958678	555538	21.093	20.302
2)	SA Decachlor...	10.982	9.239	1057026	598327	22.961	21.496
Target Compounds							
8)	L2 AR-1221-1	5.205	0.000	41814	0	78.839	N.D. #
9)	L2 AR-1221-2	5.308	0.000	11966	0	29.536	N.D. #
20)	L4 AR-1242-5	0.000	6.091f	0	9544	N.D.	14.021 #
24)	L5 AR-1248-4	7.193f	0.000	16291	0	8.619	N.D. #
25)	L5 AR-1248-5	0.000	6.091f	0	9544	N.D.	8.997 #
26)	L6 AR-1254-1	7.193	6.091f	16291	9544	9.068	6.429 #
28)	L6 AR-1254-3	7.815	0.000	15892	0	5.155	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071221\
Data File : PP037243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2021 18:01
Operator : DD\AJ
Sample : PB137615BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB137615BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 05:38:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

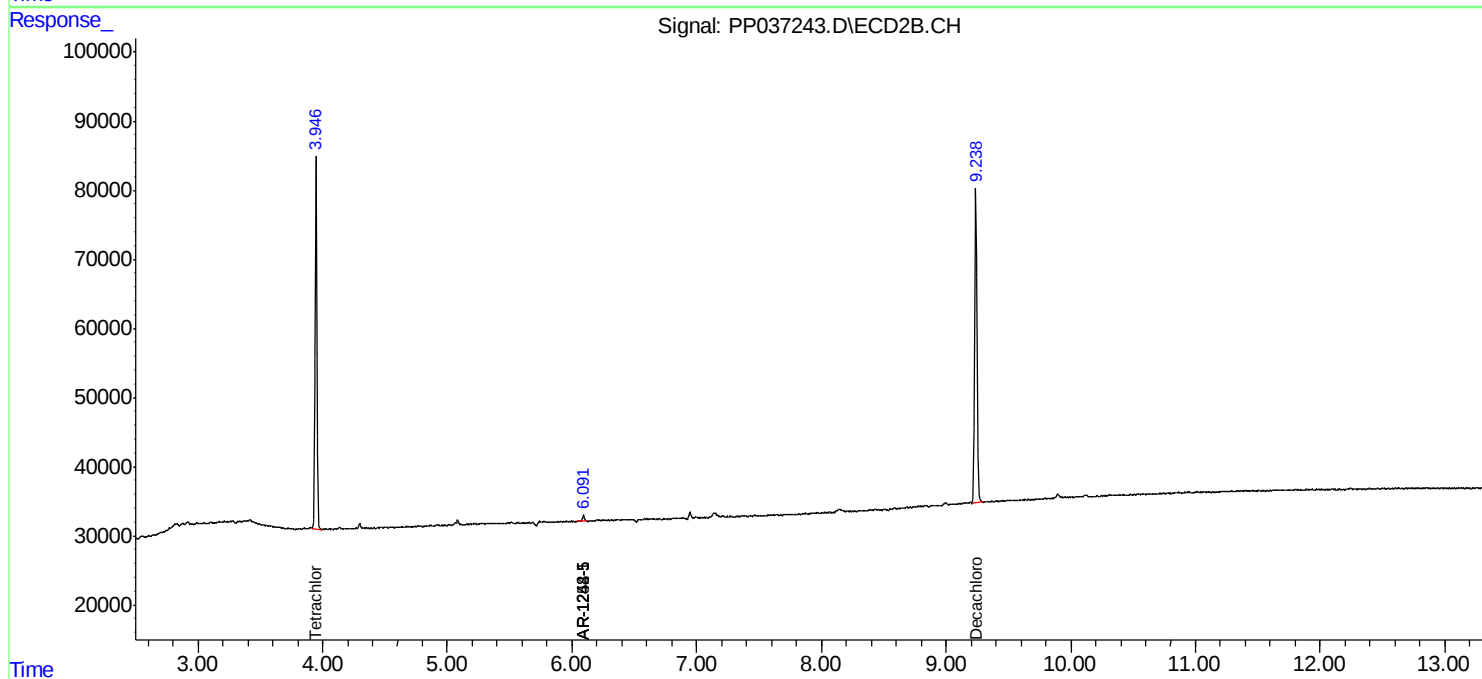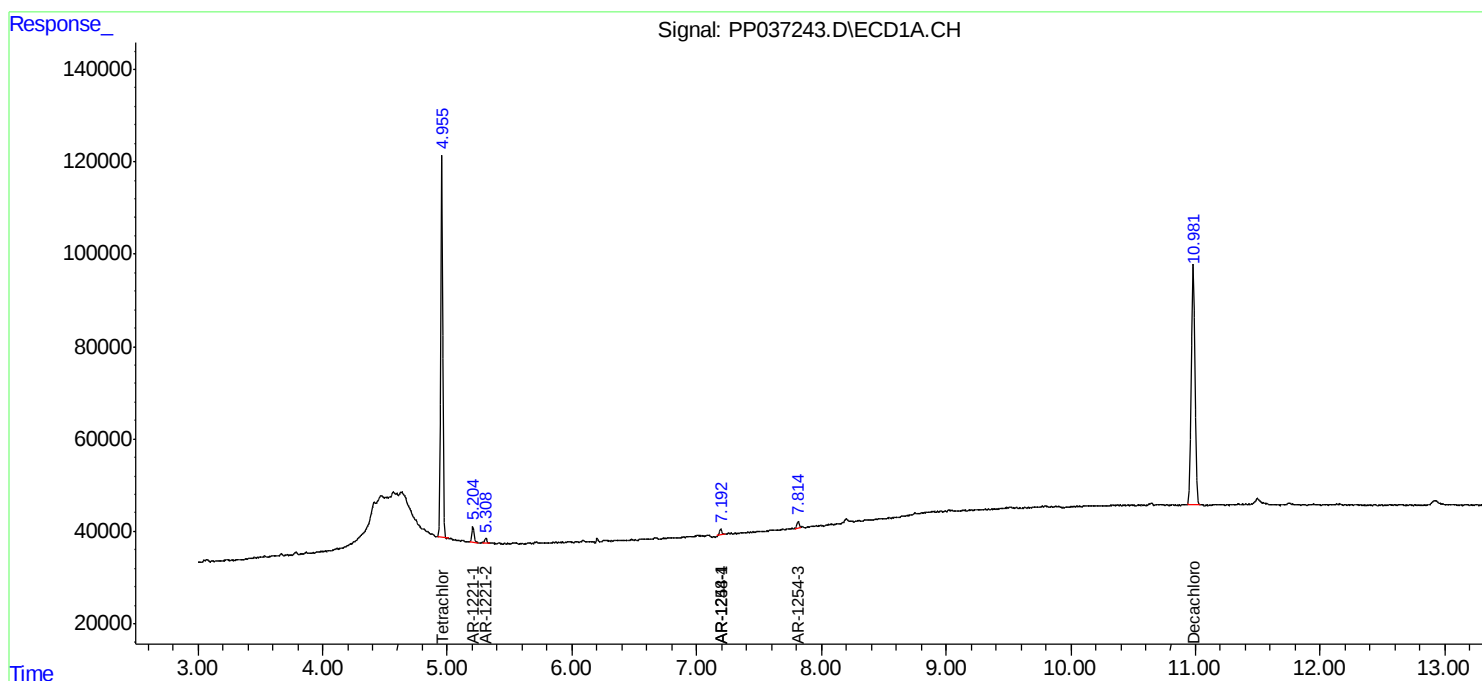


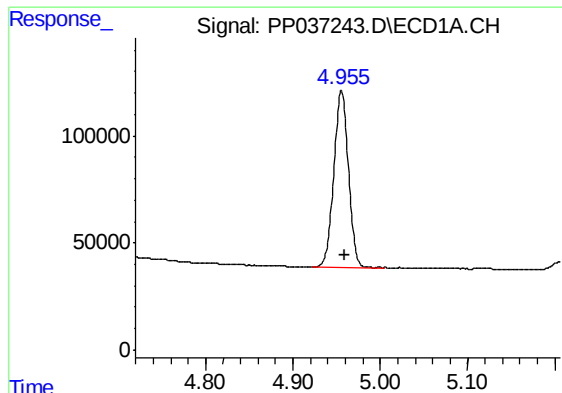

#1 Tetrachloro-m-xylene


R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 958678
Conc: 21.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137615BL

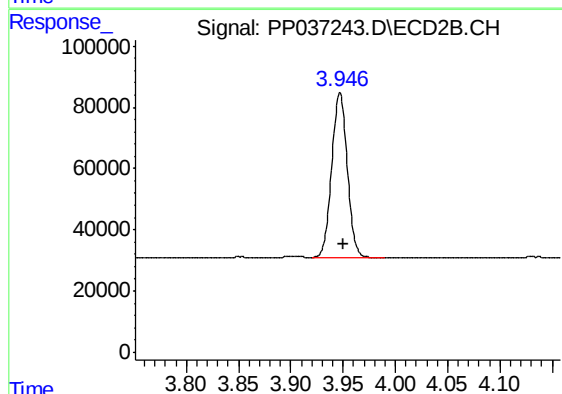


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 555538
Conc: 20.30 ng/ml

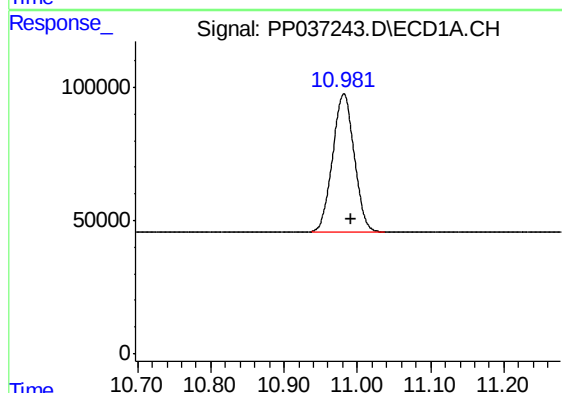


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 1057026
Conc: 22.96 ng/ml

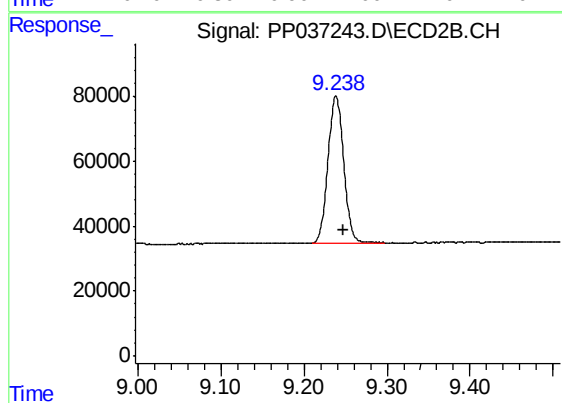

#2 Decachlorobiphenyl


R.T.: 9.239 min
Delta R.T.: -0.009 min
Response: 598327
Conc: 21.50 ng/ml

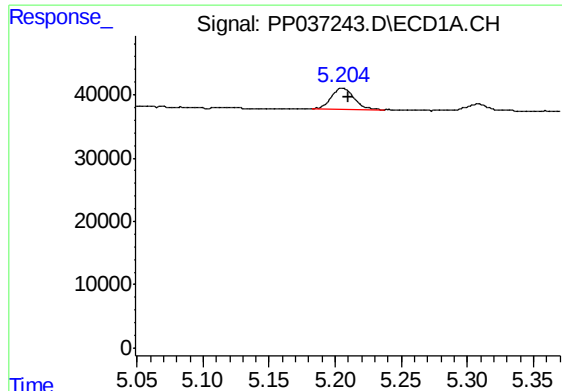

#8 AR-1221-1


R.T.: 5.205 min
Delta R.T.: -0.005 min
Response: 41814
Conc: 78.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137615BL

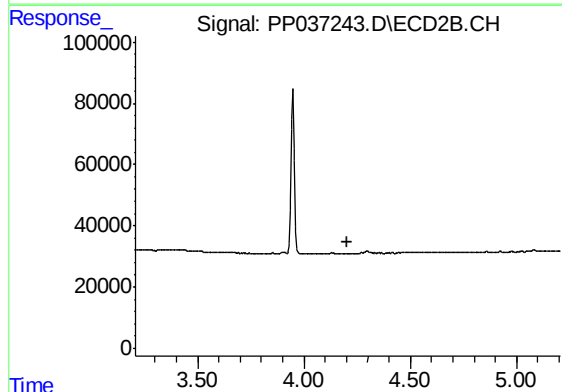


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

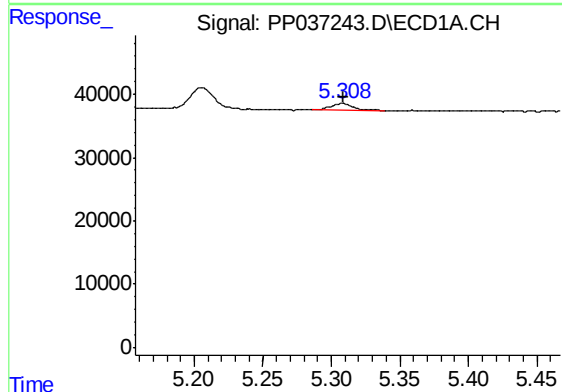


#9 AR-1221-2

R.T.: 5.308 min
Delta R.T.: 0.000 min
Response: 11966
Conc: 29.54 ng/ml

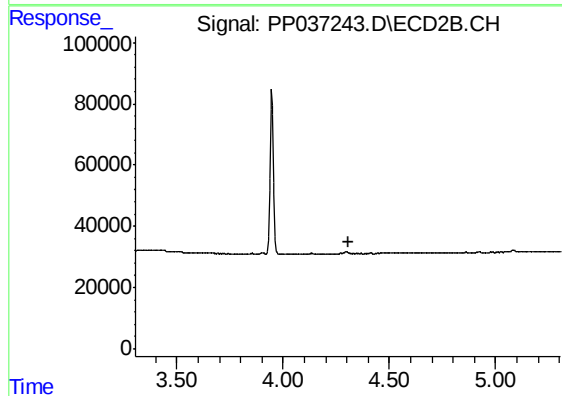

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

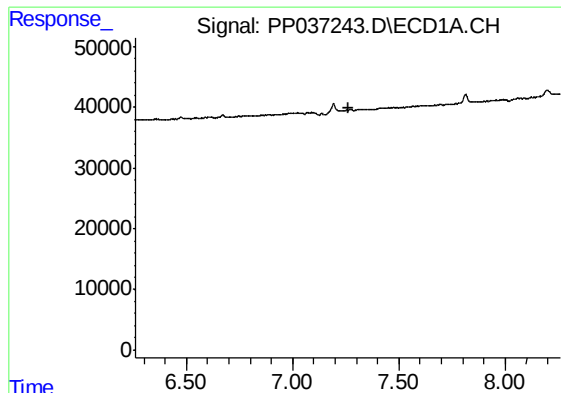

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB137615BL

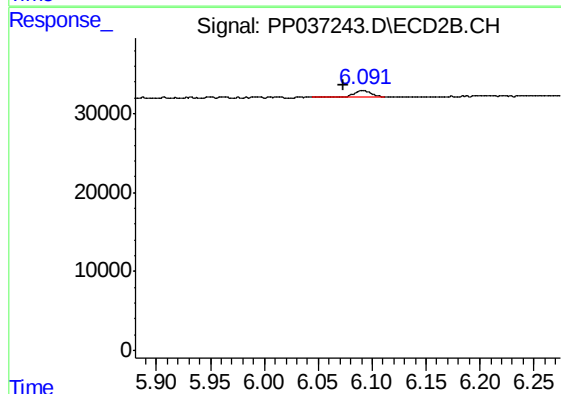


#20 AR-1242-5

R.T.: 6.091 min
Delta R.T.: 0.018 min
Response: 9544
Conc: 14.02 ng/ml

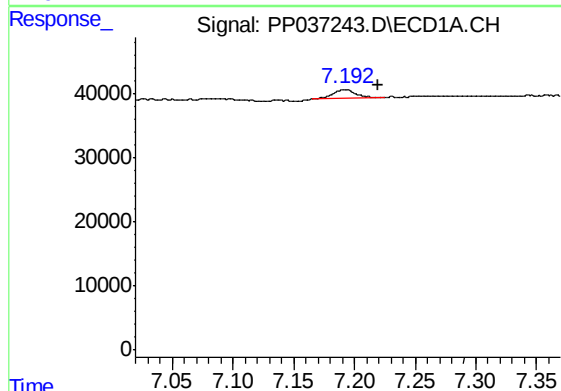


#24 AR-1248-4

R.T.: 7.193 min
Delta R.T.: -0.027 min
Response: 16291
Conc: 8.62 ng/ml

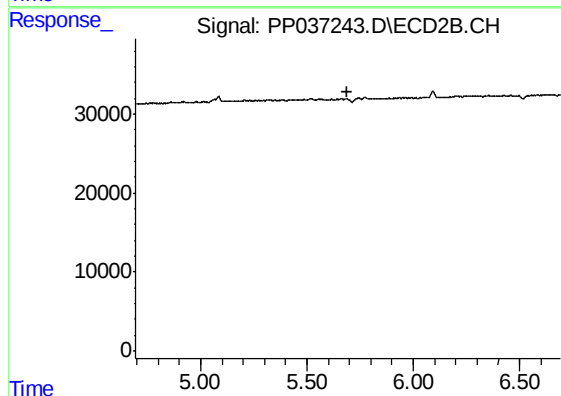

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

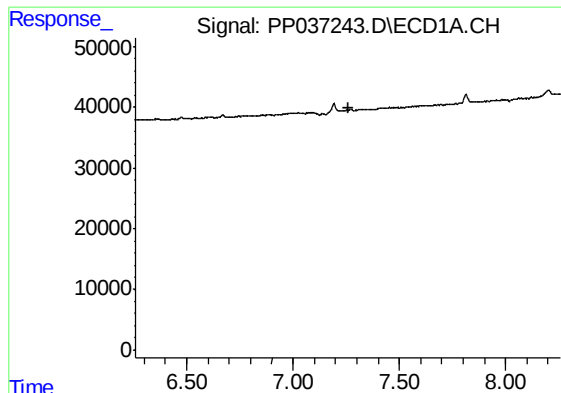

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.259 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB137615BL

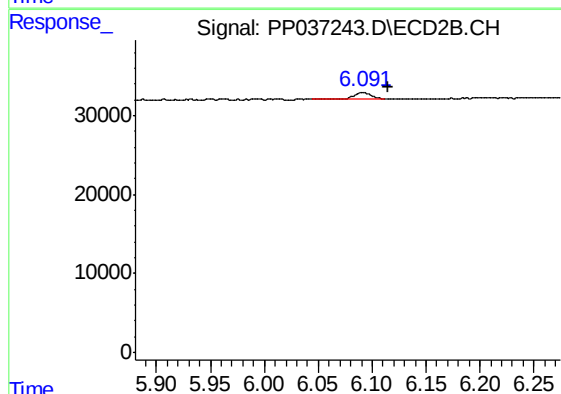


#25 AR-1248-5

R.T.: 6.091 min
Delta R.T.: -0.024 min
Response: 9544
Conc: 9.00 ng/ml

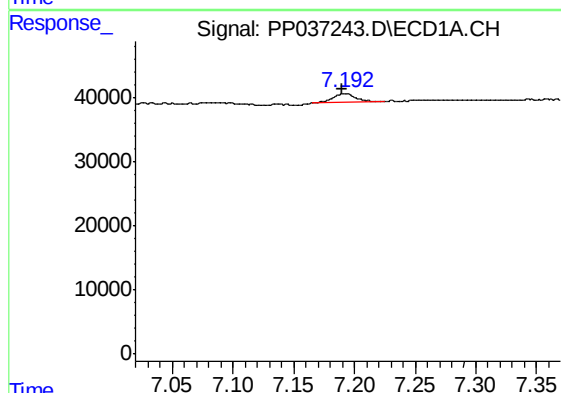


#26 AR-1254-1

R.T.: 7.193 min
Delta R.T.: 0.003 min
Response: 16291
Conc: 9.07 ng/ml

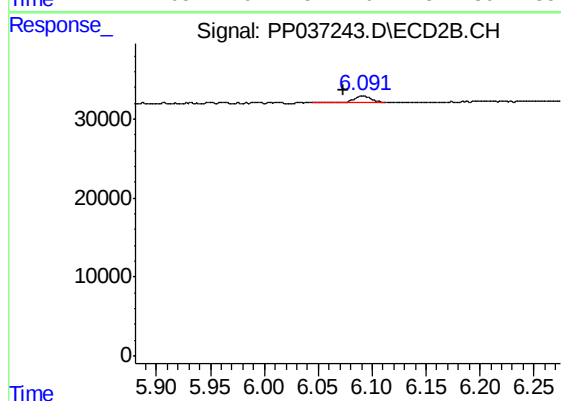

#26 AR-1254-1


R.T.: 6.091 min
Delta R.T.: 0.018 min
Response: 9544
Conc: 6.43 ng/ml

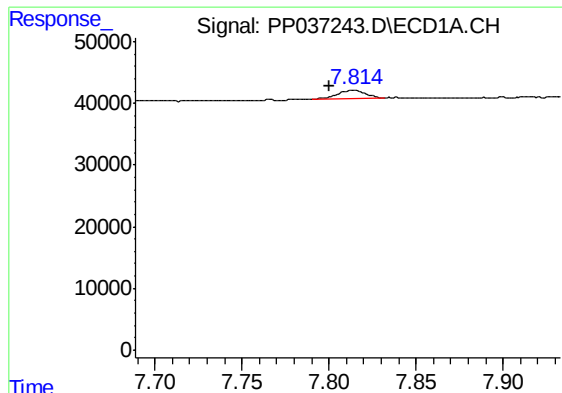

#28 AR-1254-3

R.T.: 7.815 min
Delta R.T.: 0.015 min
Response: 15892
Conc: 5.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB137615BL

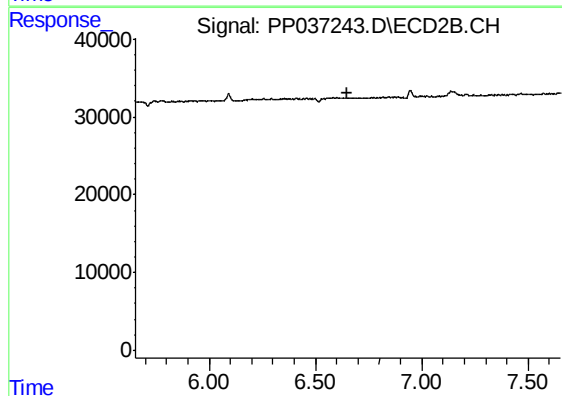

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.