

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071225\
 Data File : PP073716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2025 11:30
 Operator : YP\AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 13:32:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.525f	3.766	214758	12730	0.157	0.007 #
2)	SA Decachlor...	10.188	8.773	116668	74586	0.107	0.056 #
Target Compounds							
3)	L1 AR-1016-1	5.644	4.855	121082	62673	2.548	0.919 #
4)	L1 AR-1016-2	5.666	4.874	99986	19033	1.404	0.187 #
5)	L1 AR-1016-3	5.728	5.039	49822	389099	1.141	7.191 #
6)	L1 AR-1016-4	5.826	5.094	30356	773614	0.845	17.630 #
7)	L1 AR-1016-5	6.131	5.307	563373	515548	17.982	9.445 #
8)	L2 AR-1221-1	4.710	3.986	68123	24582	3.813	0.909 #
9)	L2 AR-1221-2	4.784	4.082	31498	65574	2.332	3.221 #
10)	L2 AR-1221-3	4.847	4.151	112350	18366	2.700	0.299 #
11)	L3 AR-1232-1	4.847	4.151	112350	18366	3.441	0.394 #
12)	L3 AR-1232-2	5.386	4.874	28185	19033	1.734	0.399 #
13)	L3 AR-1232-3	5.666	5.039	99986	389099	3.030	15.546 #
14)	L3 AR-1232-4	5.826	5.133	30356	182504	1.846	8.427 #
15)	L3 AR-1232-5	5.885	5.307	140209	515548	13.264	22.849 #
16)	L4 AR-1242-1	5.632	4.855	133819	62673	3.504	1.085 #
17)	L4 AR-1242-2	5.666	4.874	99986	19033	1.670	0.220 #
18)	L4 AR-1242-3	5.728	5.039	49822	389099	1.360	8.468 #
19)	L4 AR-1242-4	5.826	5.133	30356	182504	0.945	4.123 #
20)	L4 AR-1242-5	6.549	5.641	322114	494248	9.839	8.947
21)	L5 AR-1248-1	5.632	4.855	133819	62673	4.335	1.396 #
22)	L5 AR-1248-2	5.885	5.094	140209	773614	3.512	12.572 #
23)	L5 AR-1248-3	6.131	5.133	563373	182504	12.686	2.849 #
24)	L5 AR-1248-4	6.523	5.307	488311	515548	8.865	6.840
25)	L5 AR-1248-5	6.549	5.678	322114	718081	5.988	9.627 #
26)	L6 AR-1254-1	6.482	5.641	907943	494248	16.943	4.260 #
27)	L6 AR-1254-2	6.696	5.824	5280390	8445802	63.398	83.935 #
28)	L6 AR-1254-3	7.067	6.221	5792841	4411399	65.581	28.563 #
29)	L6 AR-1254-4	7.322	6.451	351637	423225	4.470	4.476
30)	L6 AR-1254-5	7.781	6.847	544.1E6	895.2E6	7384.380	6708.067
31)	L7 AR-1260-1	7.206	6.330	498081	216337	8.448	2.217 #
32)	L7 AR-1260-2	7.468	6.526	711.7E6	6773320	7426.400	55.140 #
33)	L7 AR-1260-3	7.882f	6.656	500111	-111519	6.844	N.D. #
34)	L7 AR-1260-4	8.065	7.165	280273	42150	4.292	0.471 #
35)	L7 AR-1260-5	8.391	7.387	310856	50371	2.061	0.224 #
36)	L8 AR-1262-1	8.065	6.847f	280273	895.2E6	3.221	6060.985 #
37)	L8 AR-1262-2	8.391	7.165	310856	42150	1.570	0.330 #
38)	L8 AR-1262-3	8.698	7.668	119382	108384	0.950	0.951
39)	L8 AR-1262-4	8.782	7.733	313718	82894	3.364	0.450 #
40)	L8 AR-1262-5	9.441	8.226	53829	53127	0.849	0.629 #
41)	L9 AR-1268-1	8.698	7.668	119382	108384	0.535	0.353 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071225\
Data File : PP073716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2025 11:30
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 13:32:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.782	7.733	313718	82894	1.647	0.312 #
43)	L9 AR-1268-3	9.014	7.935	520908	25667	3.146	0.114 #
44)	L9 AR-1268-4	9.441	8.226	53829	53127	0.774	0.571 #
45)	L9 AR-1268-5	9.838	8.538	79045	11574	0.171	0.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071225\
Data File : PP073716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2025 11:30
Operator : YP\AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 13:32:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

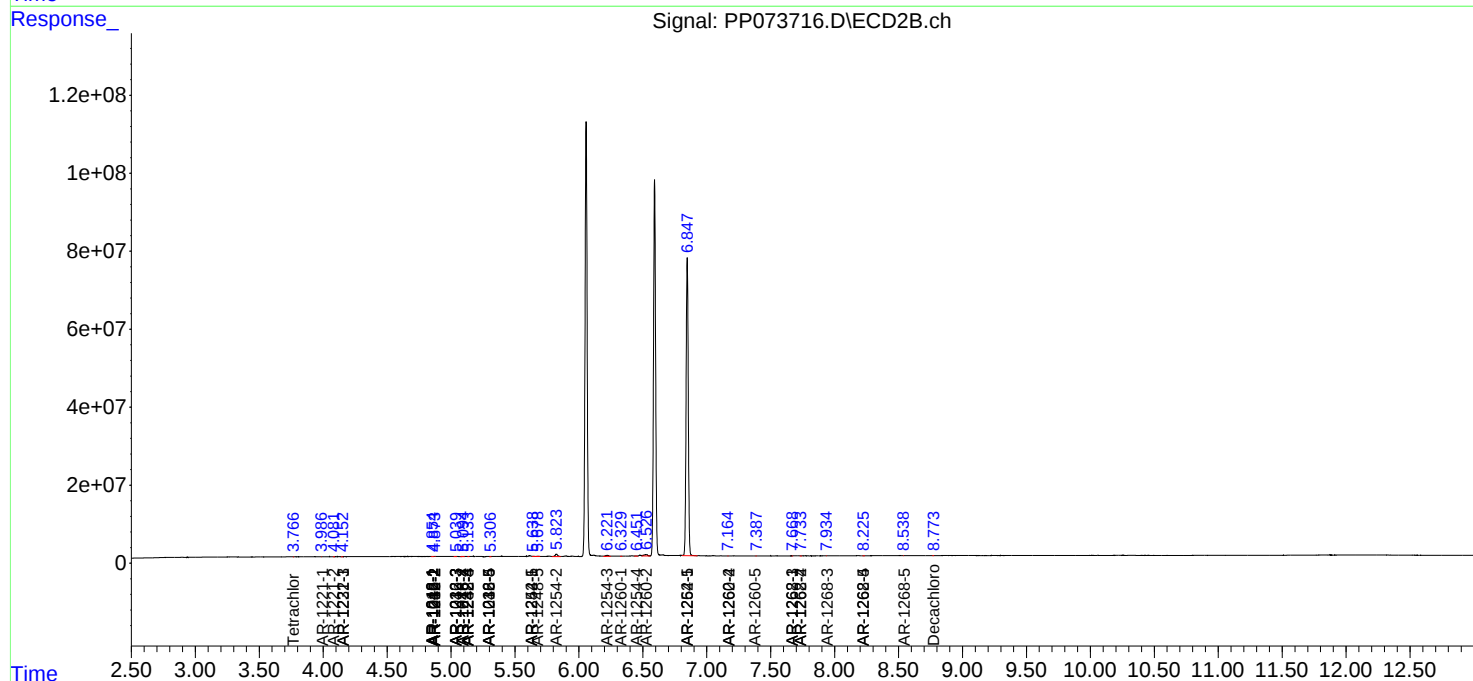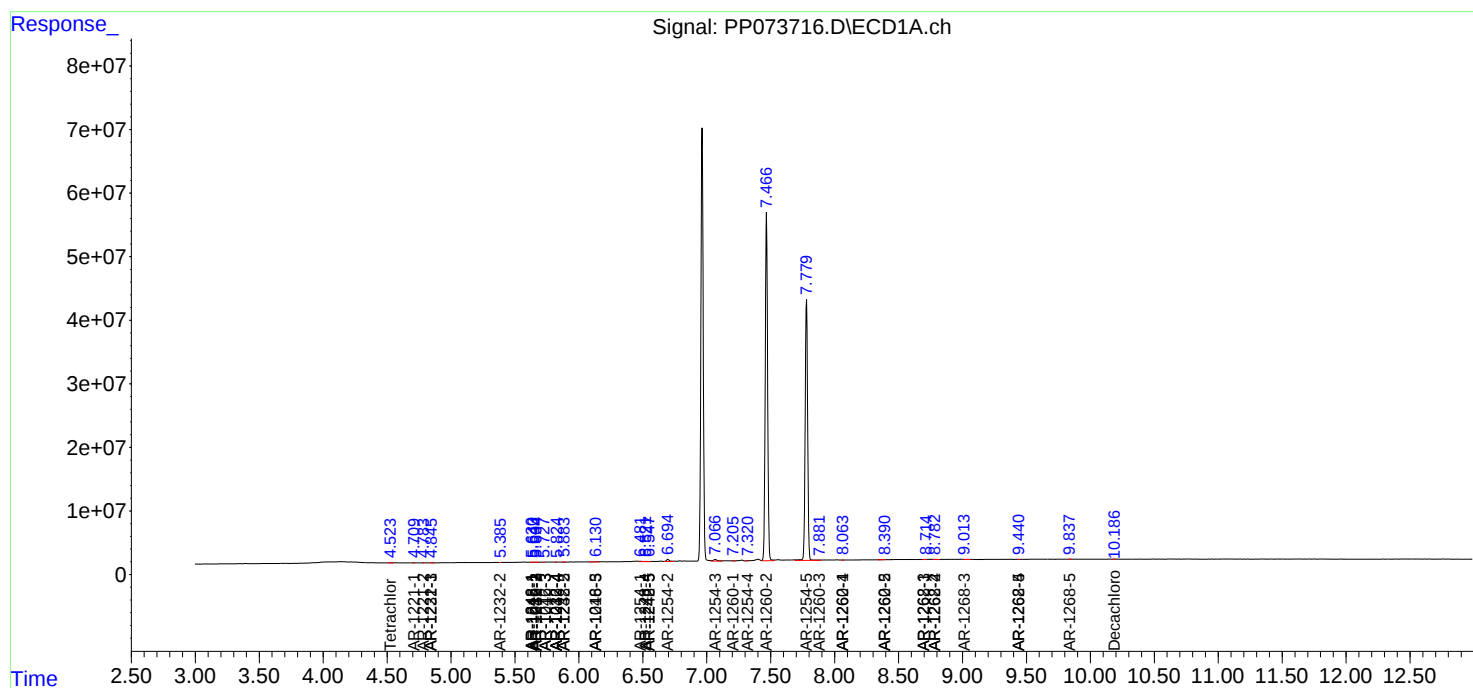


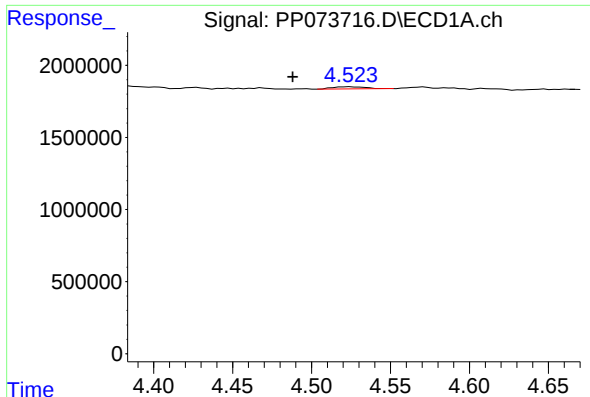

#1 Tetrachloro-m-xylene


R.T.: 4.525 min
Delta R.T.: 0.037 min
Response: 214758
Conc: 0.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

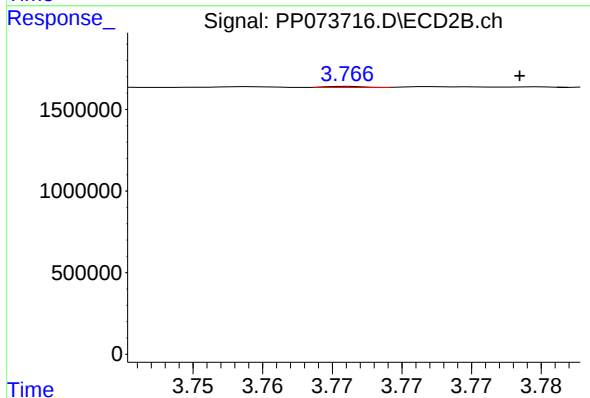


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.012 min
Response: 12730
Conc: 0.01 ng/ml

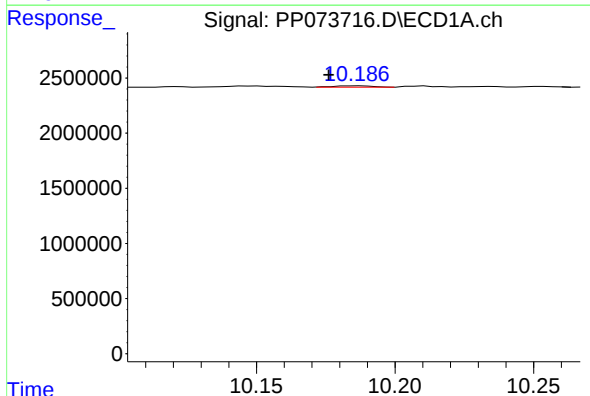


#2 Decachlorobiphenyl

R.T.: 10.188 min
Delta R.T.: 0.012 min
Response: 116668
Conc: 0.11 ng/ml

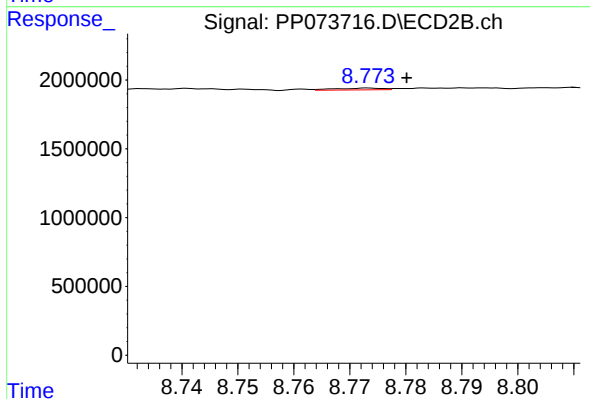

#2 Decachlorobiphenyl


R.T.: 8.773 min
Delta R.T.: -0.007 min
Response: 74586
Conc: 0.06 ng/ml

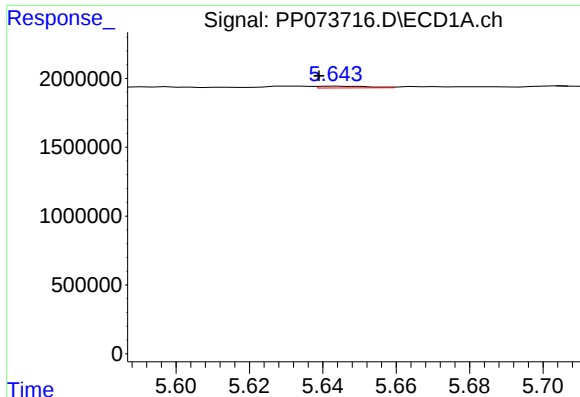

#3 AR-1016-1


R.T.: 5.644 min
Delta R.T.: 0.005 min
Response: 121082
Conc: 2.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

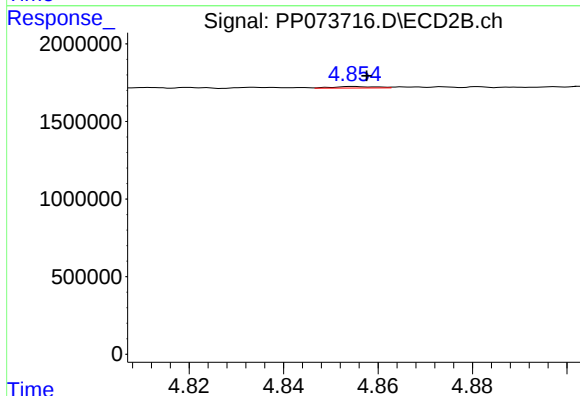


#3 AR-1016-1

R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 62673
Conc: 0.92 ng/ml

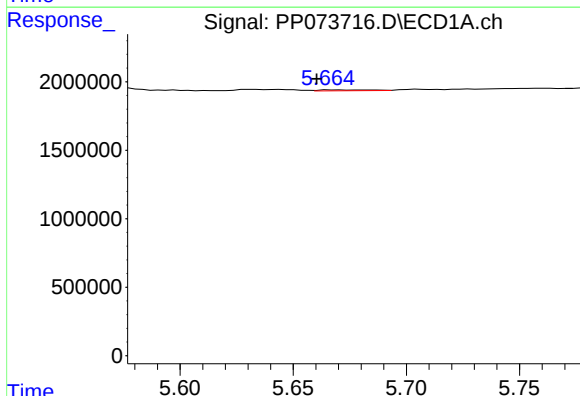


#4 AR-1016-2

R.T.: 5.666 min
Delta R.T.: 0.006 min
Response: 99986
Conc: 1.40 ng/ml

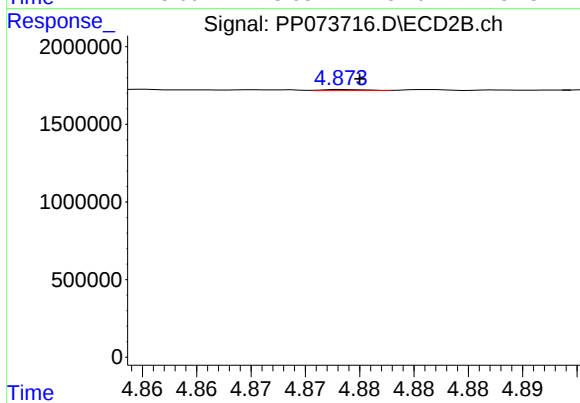

#4 AR-1016-2


R.T.: 4.874 min
Delta R.T.: -0.001 min
Response: 19033
Conc: 0.19 ng/ml

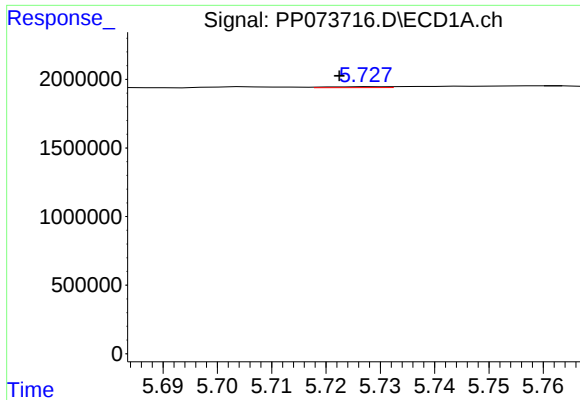

#5 AR-1016-3


R.T.: 5.728 min
Delta R.T.: 0.006 min
Response: 49822
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

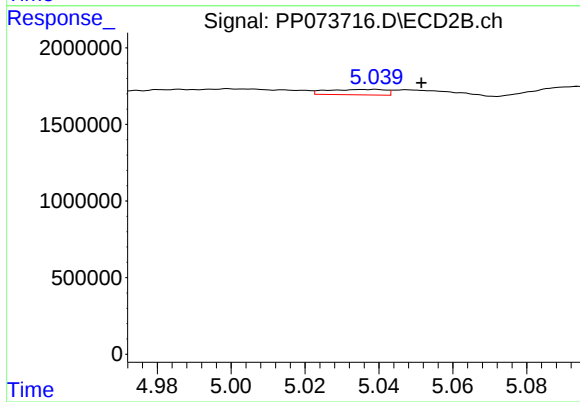


#5 AR-1016-3

R.T.: 5.039 min
Delta R.T.: -0.012 min
Response: 389099
Conc: 7.19 ng/ml

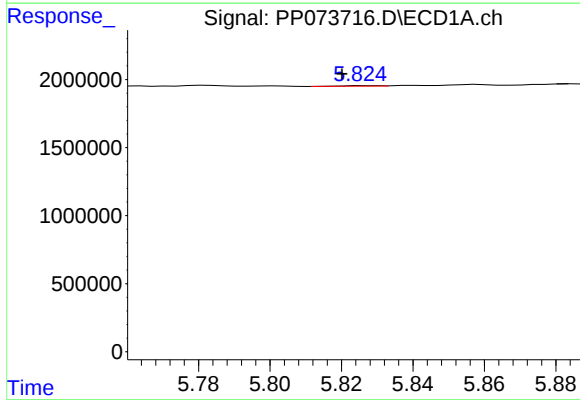


#6 AR-1016-4

R.T.: 5.826 min
Delta R.T.: 0.006 min
Response: 30356
Conc: 0.84 ng/ml

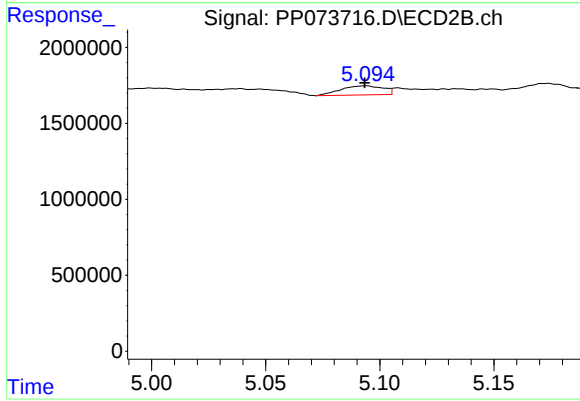

#6 AR-1016-4


R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 773614
Conc: 17.63 ng/ml

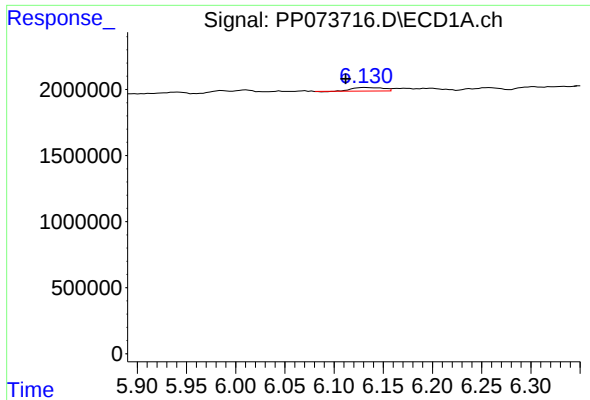

#7 AR-1016-5


R.T.: 6.131 min
Delta R.T.: 0.019 min
Response: 563373
Conc: 17.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

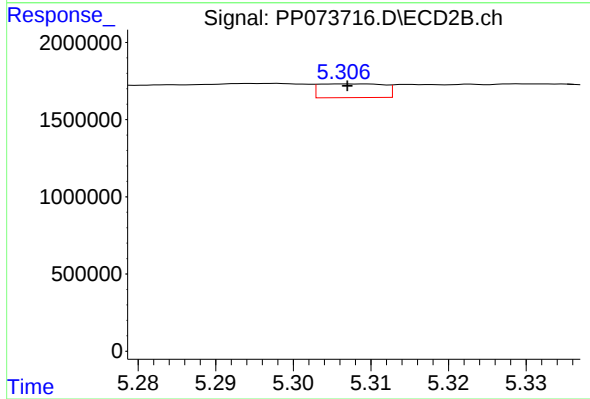


#7 AR-1016-5

R.T.: 5.307 min
Delta R.T.: 0.000 min
Response: 515548
Conc: 9.45 ng/ml

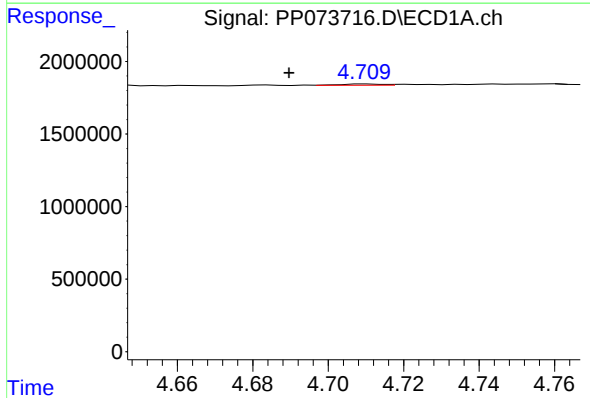


#8 AR-1221-1

R.T.: 4.710 min
Delta R.T.: 0.021 min
Response: 68123
Conc: 3.81 ng/ml

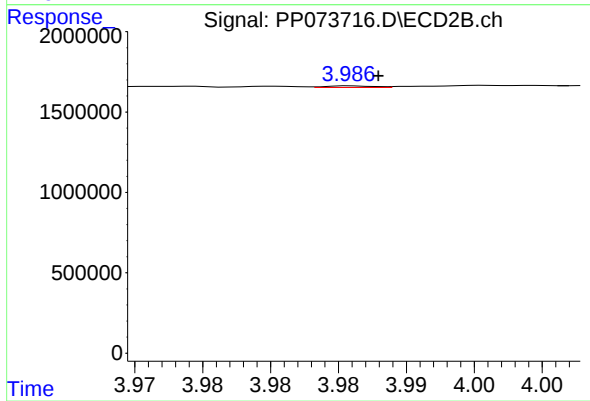

#8 AR-1221-1


R.T.: 3.986 min
Delta R.T.: -0.002 min
Response: 24582
Conc: 0.91 ng/ml

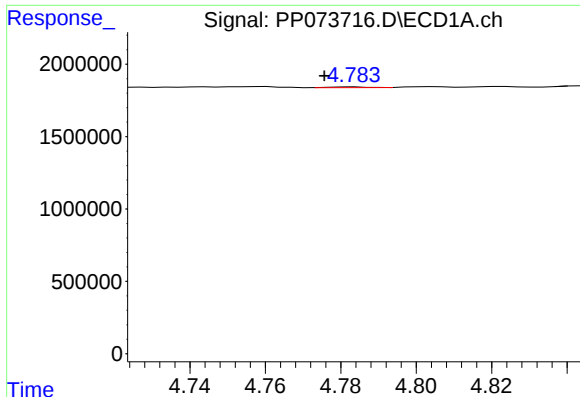

#9 AR-1221-2


R.T.: 4.784 min
Delta R.T.: 0.008 min
Response: 31498
Conc: 2.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

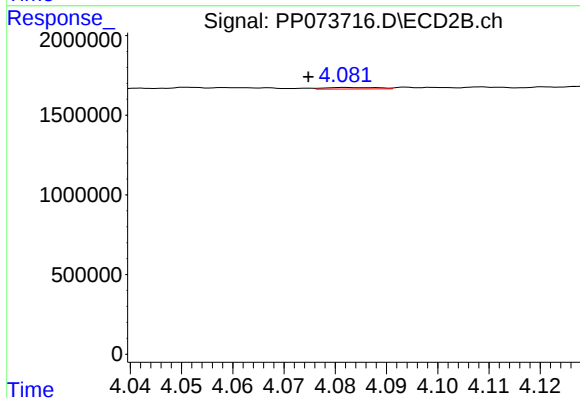


#9 AR-1221-2

R.T.: 4.082 min
Delta R.T.: 0.007 min
Response: 65574
Conc: 3.22 ng/ml

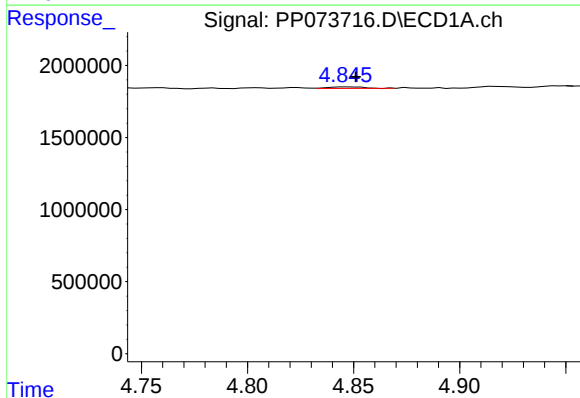


#10 AR-1221-3

R.T.: 4.847 min
Delta R.T.: -0.004 min
Response: 112350
Conc: 2.70 ng/ml

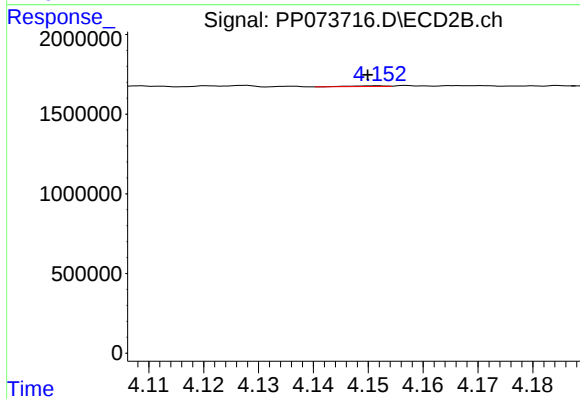

#10 AR-1221-3


R.T.: 4.151 min
Delta R.T.: 0.001 min
Response: 18366
Conc: 0.30 ng/ml

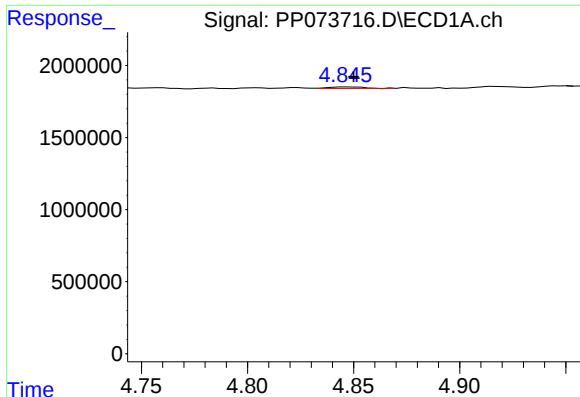

#11 AR-1232-1


R.T.: 4.847 min
Delta R.T.: -0.003 min
Response: 112350
Conc: 3.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

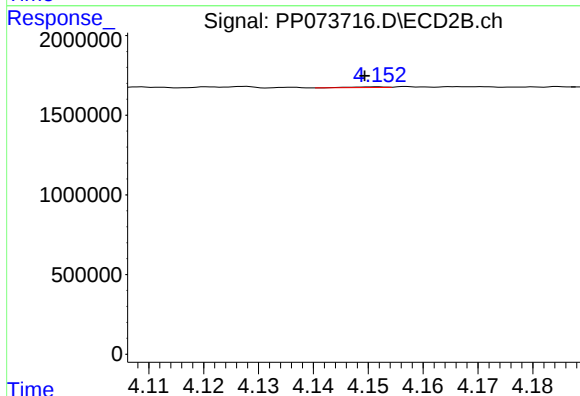


#11 AR-1232-1

R.T.: 4.151 min
Delta R.T.: 0.002 min
Response: 18366
Conc: 0.39 ng/ml

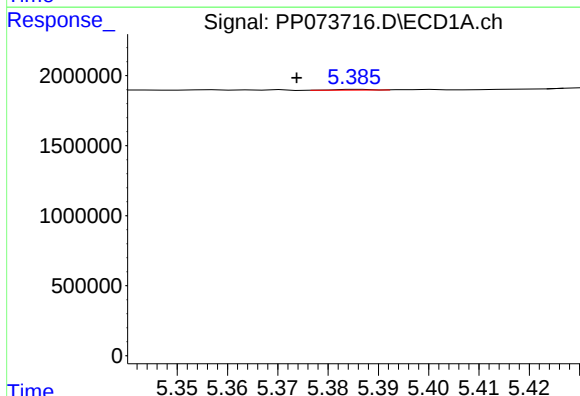


#12 AR-1232-2

R.T.: 5.386 min
Delta R.T.: 0.012 min
Response: 28185
Conc: 1.73 ng/ml

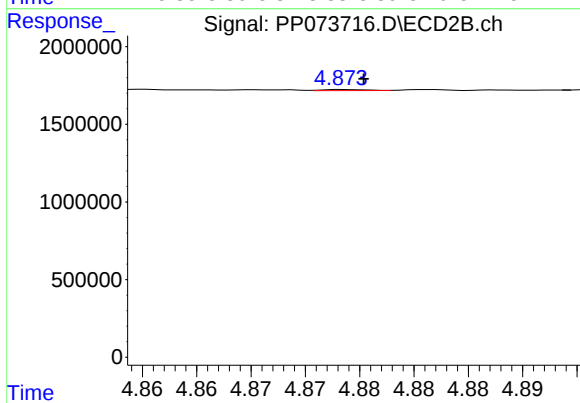

#12 AR-1232-2


R.T.: 4.874 min
Delta R.T.: -0.002 min
Response: 19033
Conc: 0.40 ng/ml

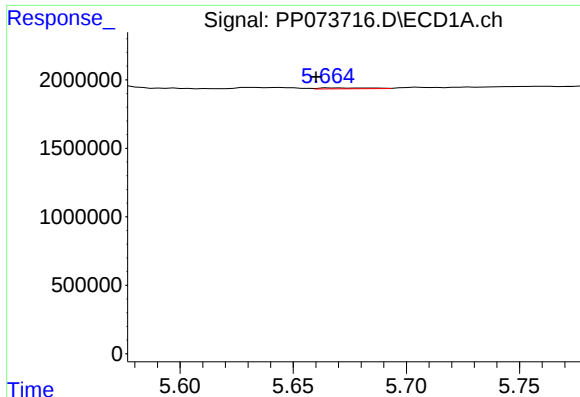

#13 AR-1232-3


R.T.: 5.666 min
Delta R.T.: 0.006 min
Response: 99986
Conc: 3.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

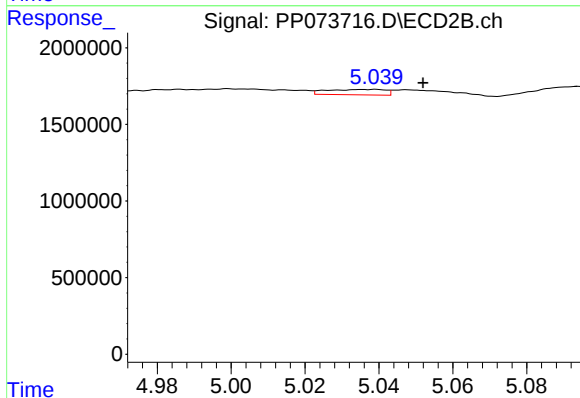


#13 AR-1232-3

R.T.: 5.039 min
Delta R.T.: -0.013 min
Response: 389099
Conc: 15.55 ng/ml

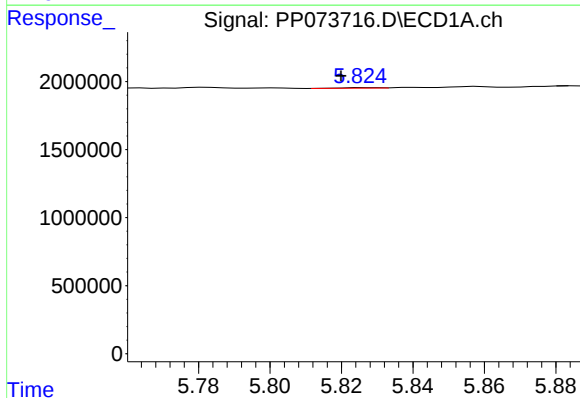


#14 AR-1232-4

R.T.: 5.826 min
Delta R.T.: 0.006 min
Response: 30356
Conc: 1.85 ng/ml

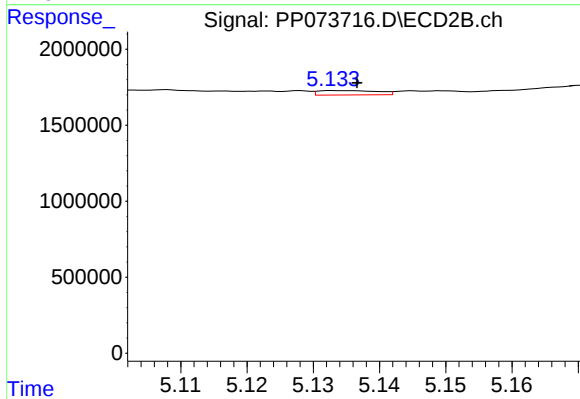

#14 AR-1232-4


R.T.: 5.133 min
Delta R.T.: -0.003 min
Response: 182504
Conc: 8.43 ng/ml

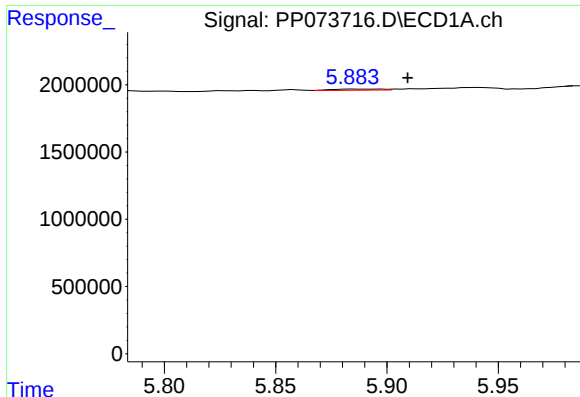

#15 AR-1232-5


R.T.: 5.885 min
Delta R.T.: -0.024 min
Response: 140209
Conc: 13.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

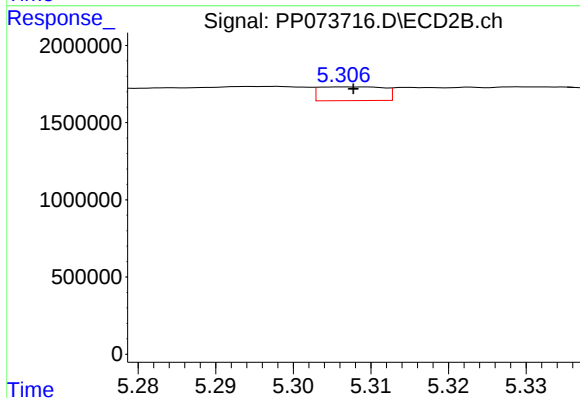


#15 AR-1232-5

R.T.: 5.307 min
Delta R.T.: -0.001 min
Response: 515548
Conc: 22.85 ng/ml

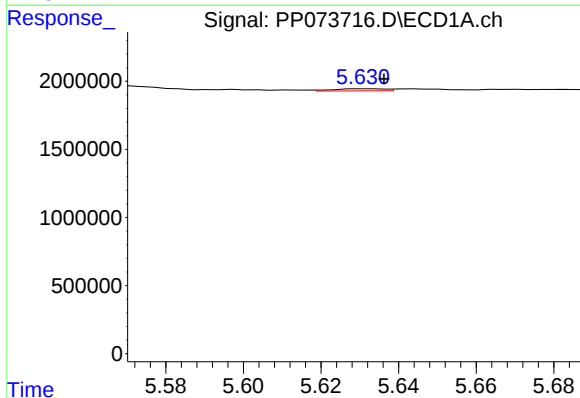


#16 AR-1242-1

R.T.: 5.632 min
Delta R.T.: -0.005 min
Response: 133819
Conc: 3.50 ng/ml

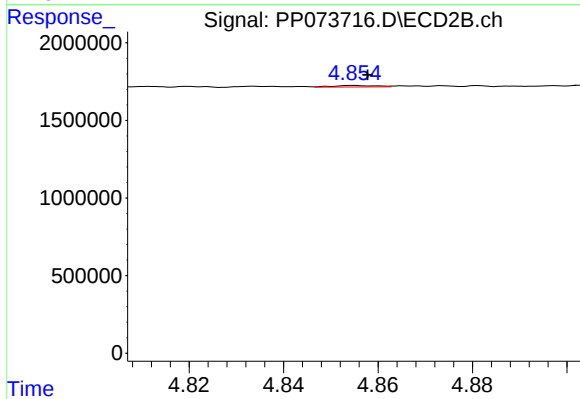

#16 AR-1242-1


R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 62673
Conc: 1.08 ng/ml

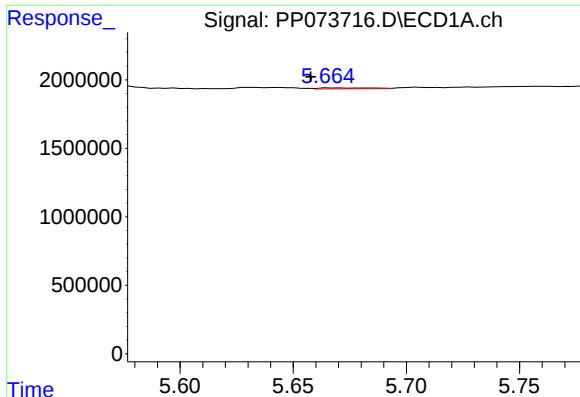

#17 AR-1242-2


R.T.: 5.666 min
Delta R.T.: 0.009 min
Response: 99986
Conc: 1.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

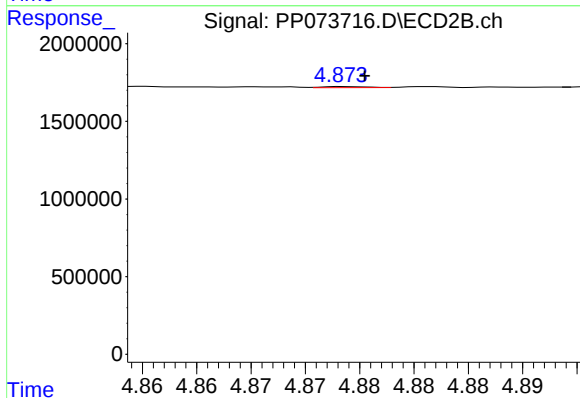


#17 AR-1242-2

R.T.: 4.874 min
Delta R.T.: -0.002 min
Response: 19033
Conc: 0.22 ng/ml

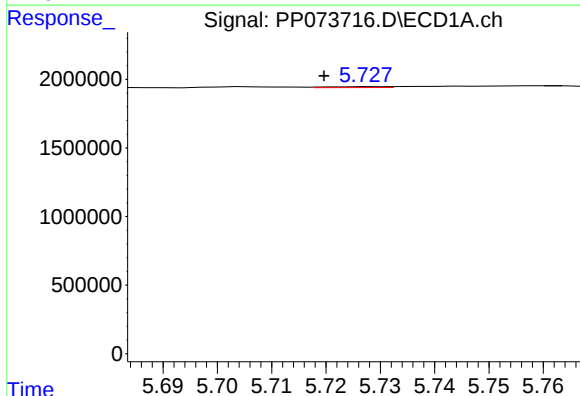


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: 0.009 min
Response: 49822
Conc: 1.36 ng/ml

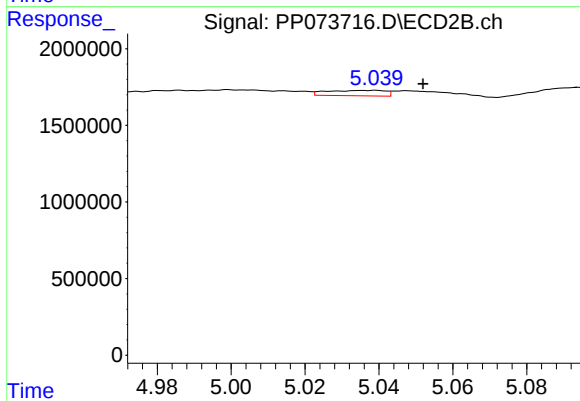

#18 AR-1242-3


R.T.: 5.039 min
Delta R.T.: -0.013 min
Response: 389099
Conc: 8.47 ng/ml

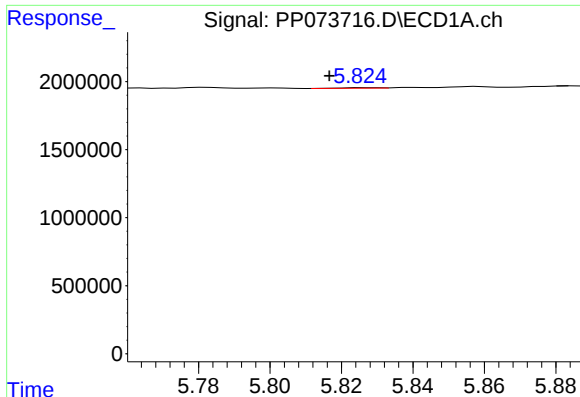

#19 AR-1242-4


R.T.: 5.826 min
Delta R.T.: 0.009 min
Response: 30356
Conc: 0.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

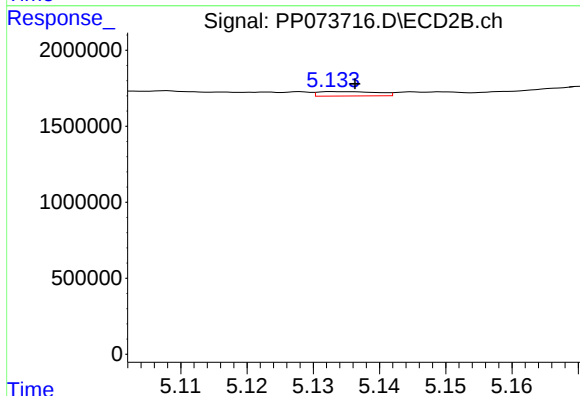


#19 AR-1242-4

R.T.: 5.133 min
Delta R.T.: -0.003 min
Response: 182504
Conc: 4.12 ng/ml

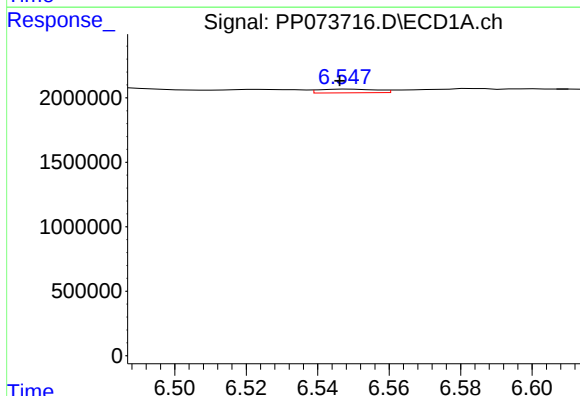


#20 AR-1242-5

R.T.: 6.549 min
Delta R.T.: 0.002 min
Response: 322114
Conc: 9.84 ng/ml

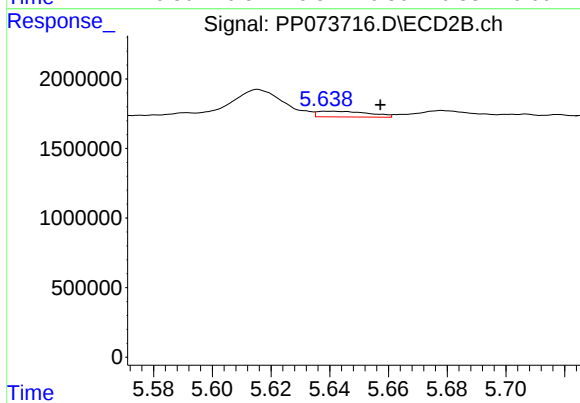

#20 AR-1242-5


R.T.: 5.641 min
Delta R.T.: -0.016 min
Response: 494248
Conc: 8.95 ng/ml

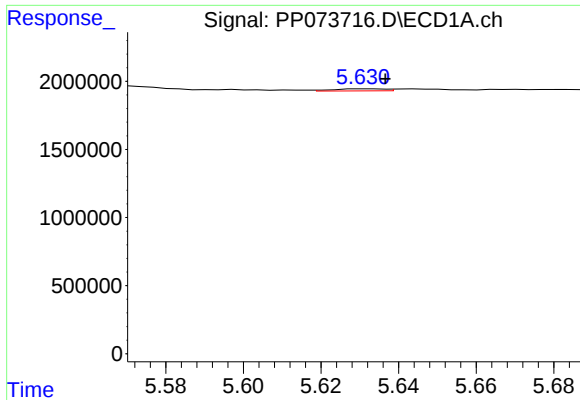

#21 AR-1248-1


R.T.: 5.632 min
Delta R.T.: -0.005 min
Response: 133819
Conc: 4.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

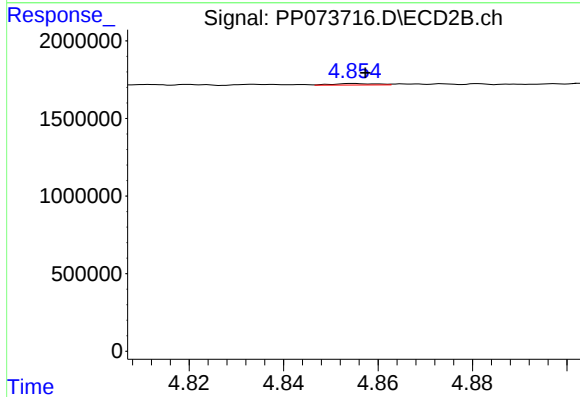


#21 AR-1248-1

R.T.: 4.855 min
Delta R.T.: -0.002 min
Response: 62673
Conc: 1.40 ng/ml

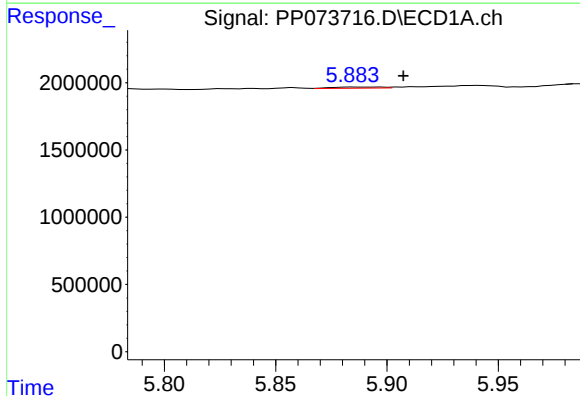


#22 AR-1248-2

R.T.: 5.885 min
Delta R.T.: -0.022 min
Response: 140209
Conc: 3.51 ng/ml

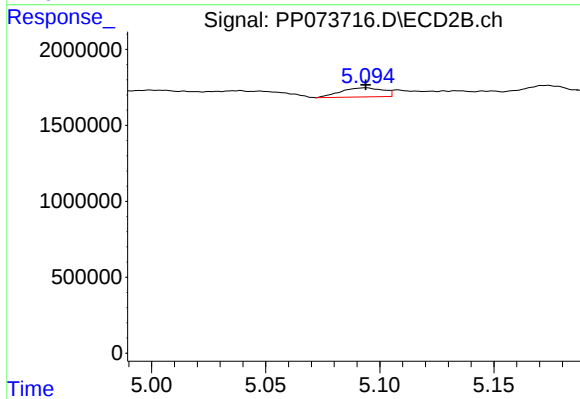

#22 AR-1248-2


R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 773614
Conc: 12.57 ng/ml

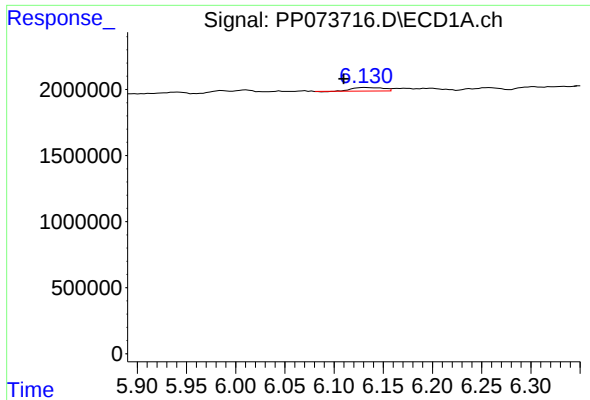

#23 AR-1248-3


R.T.: 6.131 min
Delta R.T.: 0.022 min
Response: 563373
Conc: 12.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

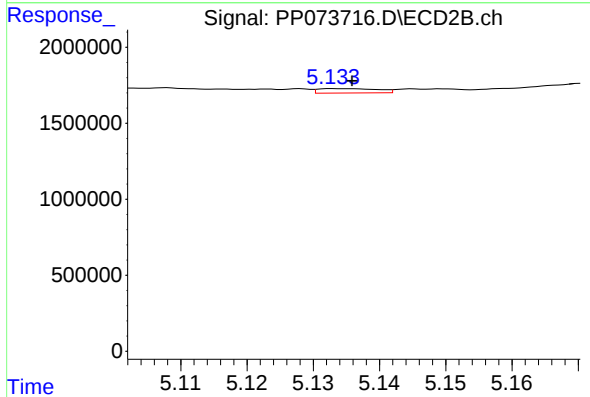


#23 AR-1248-3

R.T.: 5.133 min
Delta R.T.: -0.003 min
Response: 182504
Conc: 2.85 ng/ml

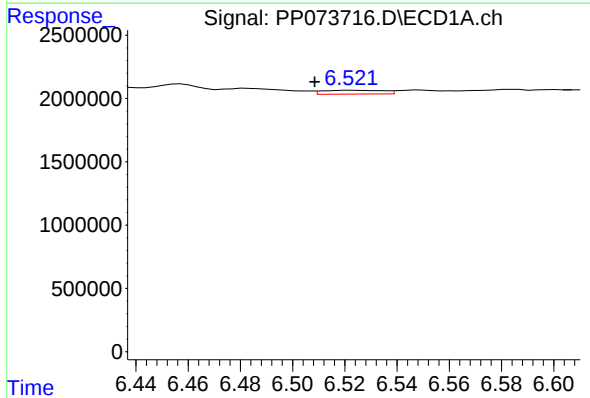


#24 AR-1248-4

R.T.: 6.523 min
Delta R.T.: 0.015 min
Response: 488311
Conc: 8.87 ng/ml

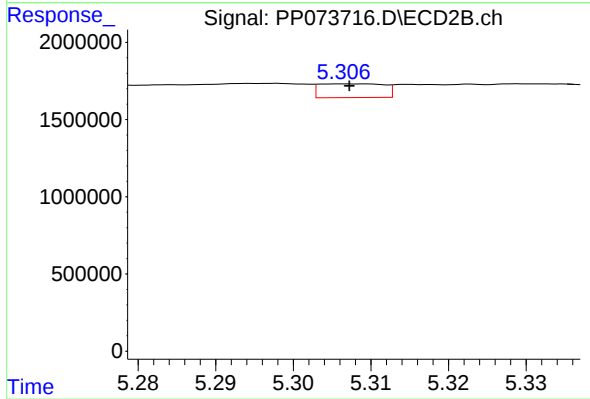

#24 AR-1248-4


R.T.: 5.307 min
Delta R.T.: 0.000 min
Response: 515548
Conc: 6.84 ng/ml

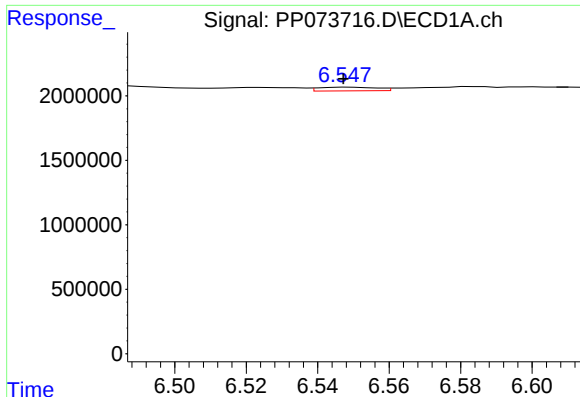

#25 AR-1248-5


R.T.: 6.549 min
Delta R.T.: 0.001 min
Response: 322114
Conc: 5.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

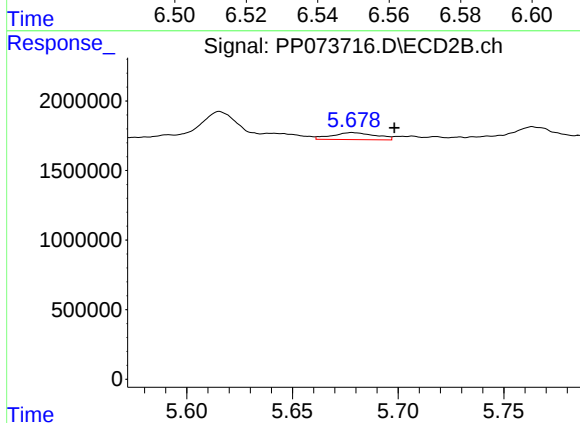


#25 AR-1248-5

R.T.: 5.678 min
Delta R.T.: -0.020 min
Response: 718081
Conc: 9.63 ng/ml

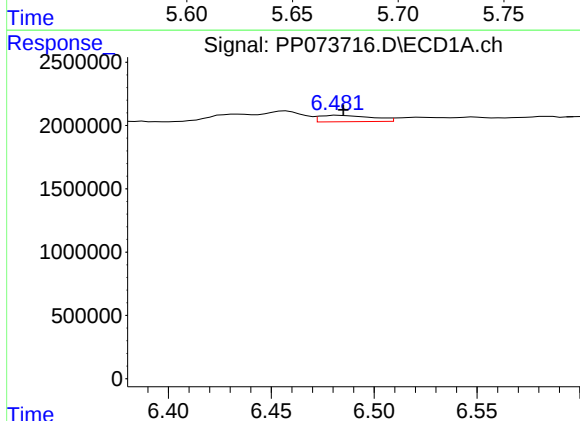


#26 AR-1254-1

R.T.: 6.482 min
Delta R.T.: -0.003 min
Response: 907943
Conc: 16.94 ng/ml

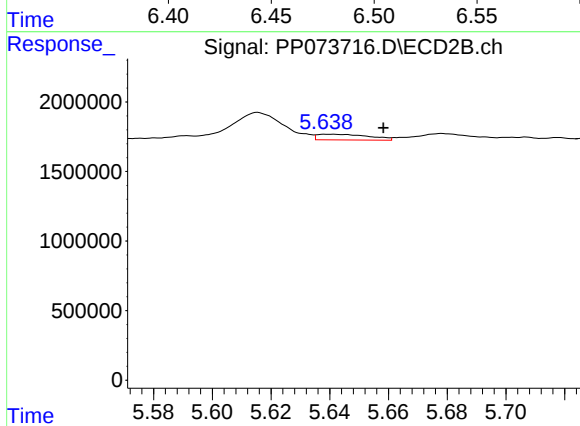

#26 AR-1254-1


R.T.: 5.641 min
Delta R.T.: -0.017 min
Response: 494248
Conc: 4.26 ng/ml

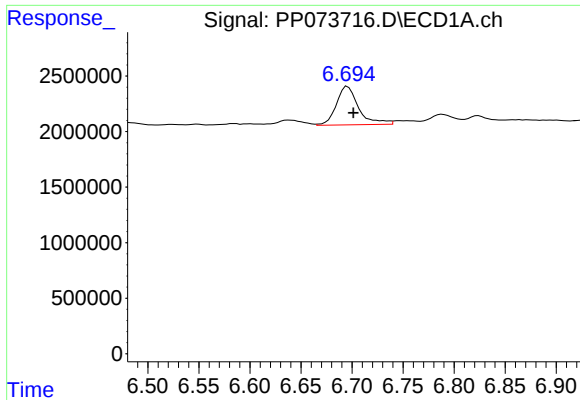

#27 AR-1254-2


R.T.: 6.696 min
Delta R.T.: -0.005 min
Response: 5280390
Conc: 63.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

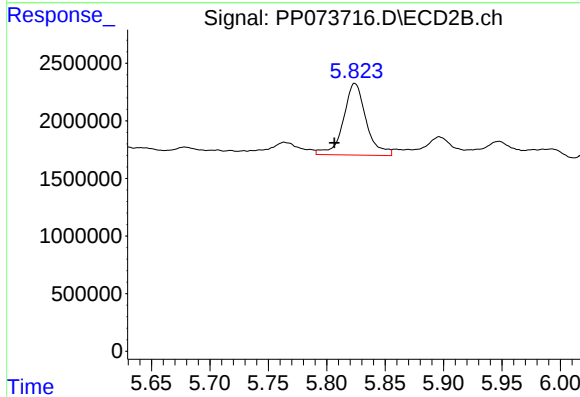


#27 AR-1254-2

R.T.: 5.824 min
Delta R.T.: 0.017 min
Response: 8445802
Conc: 83.93 ng/ml

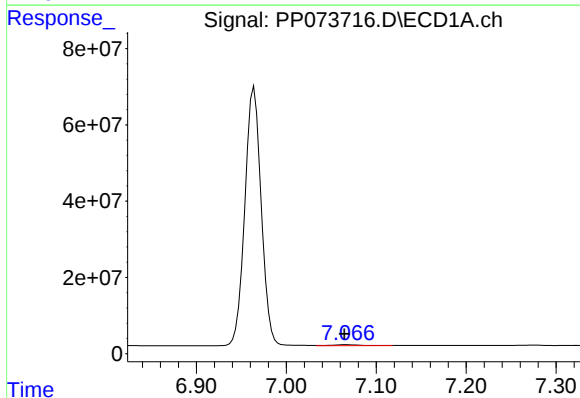


#28 AR-1254-3

R.T.: 7.067 min
Delta R.T.: 0.003 min
Response: 5792841
Conc: 65.58 ng/ml

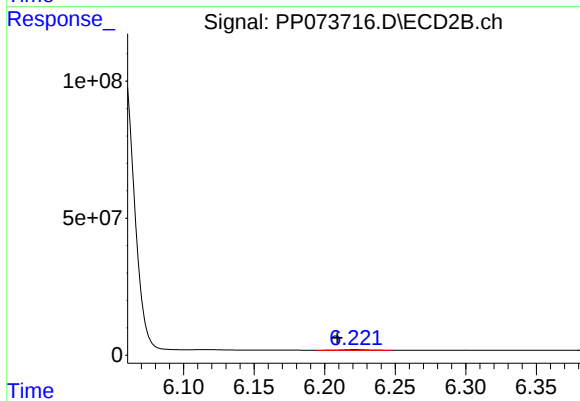

#28 AR-1254-3


R.T.: 6.221 min
Delta R.T.: 0.012 min
Response: 4411399
Conc: 28.56 ng/ml

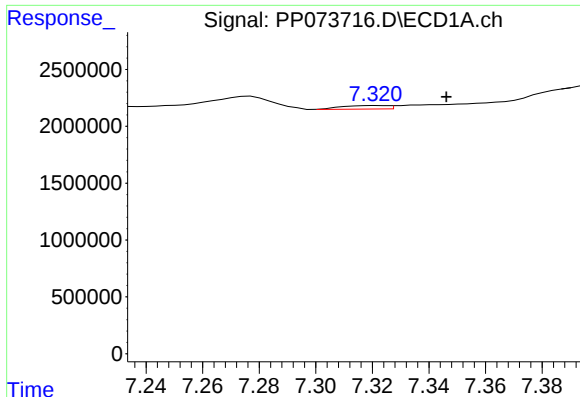

#29 AR-1254-4


R.T.: 7.322 min
Delta R.T.: -0.024 min
Response: 351637
Conc: 4.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

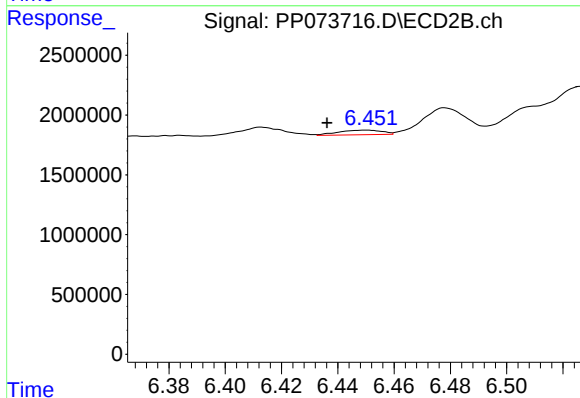


#29 AR-1254-4

R.T.: 6.451 min
Delta R.T.: 0.015 min
Response: 423225
Conc: 4.48 ng/ml

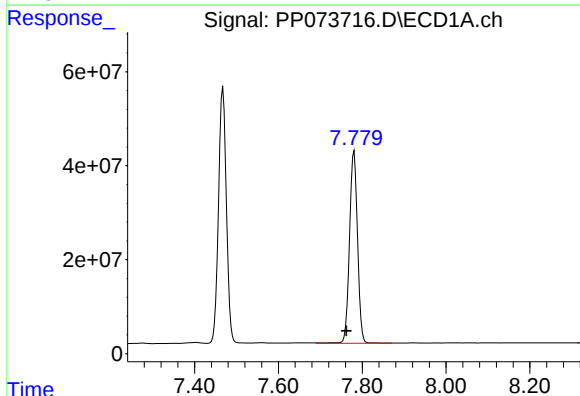


#30 AR-1254-5

R.T.: 7.781 min
Delta R.T.: 0.018 min
Response: 544079723
Conc: 7384.38 ng/ml

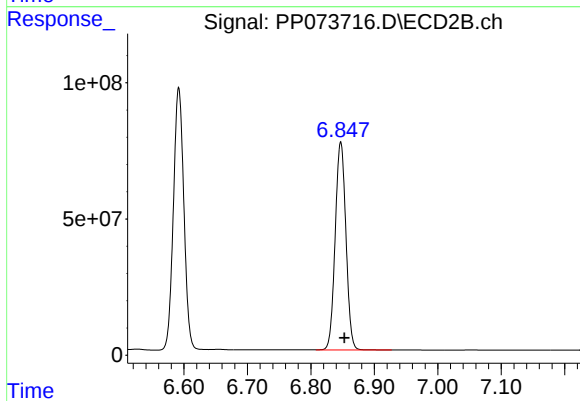

#30 AR-1254-5


R.T.: 6.847 min
Delta R.T.: -0.006 min
Response: 895157102
Conc: 6708.07 ng/ml

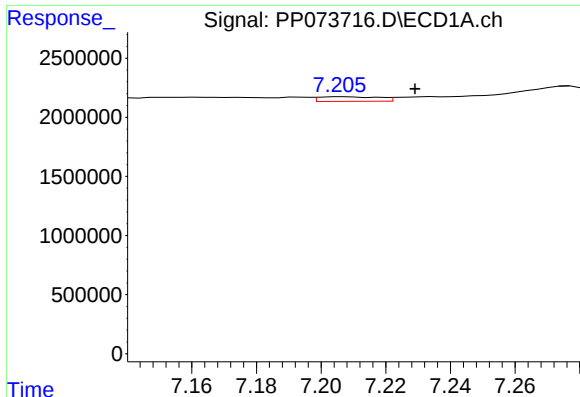

#31 AR-1260-1


R.T.: 7.206 min
Delta R.T.: -0.023 min
Response: 498081
Conc: 8.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

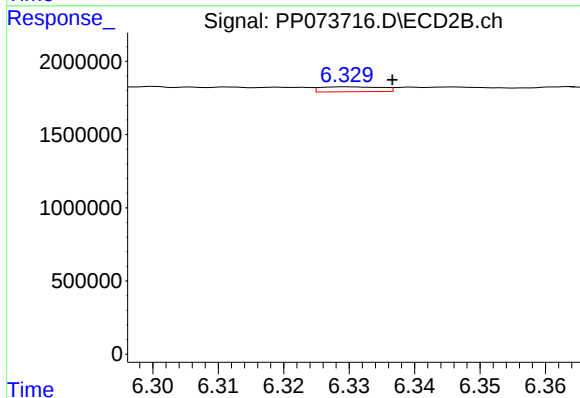


#31 AR-1260-1

R.T.: 6.330 min
Delta R.T.: -0.007 min
Response: 216337
Conc: 2.22 ng/ml

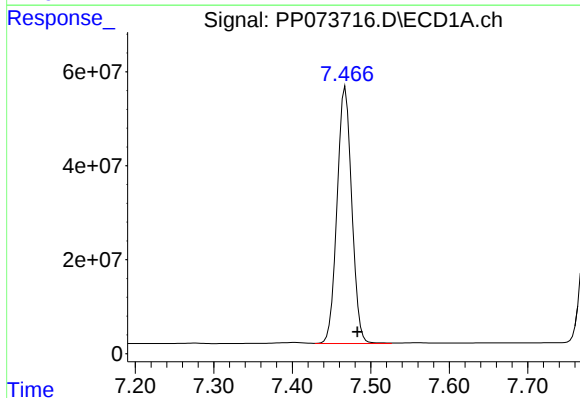


#32 AR-1260-2

R.T.: 7.468 min
Delta R.T.: -0.015 min
Response: 711745163
Conc: 7426.40 ng/ml

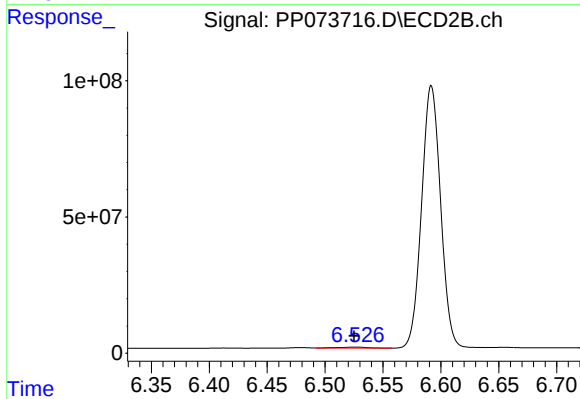

#32 AR-1260-2


R.T.: 6.526 min
Delta R.T.: 0.001 min
Response: 6773320
Conc: 55.14 ng/ml

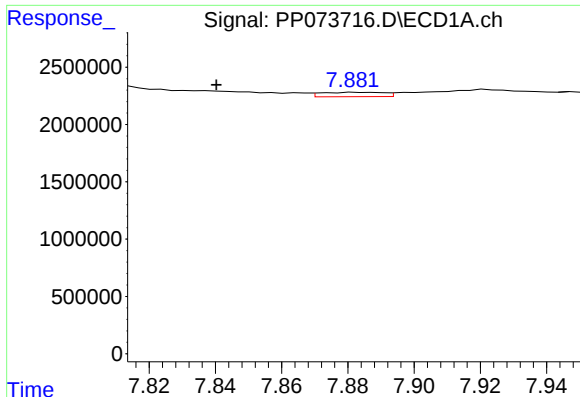

#33 AR-1260-3


R.T.: 7.882 min
Delta R.T.: 0.042 min
Response: 500111
Conc: 6.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

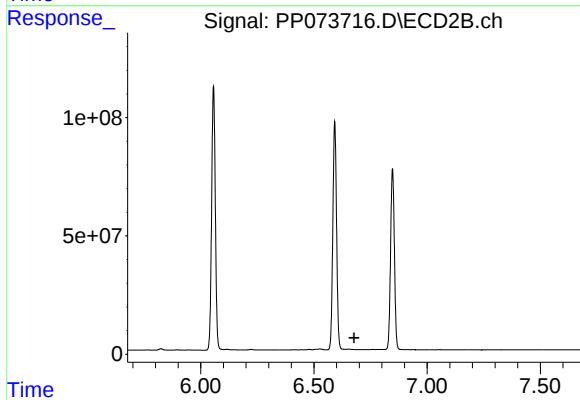


#33 AR-1260-3

R.T.: 6.656 min
Delta R.T.: -0.021 min
Response: -111519
Conc: N.D.

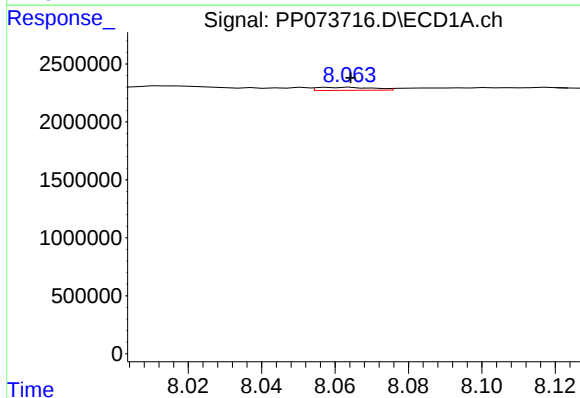


#34 AR-1260-4

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 280273
Conc: 4.29 ng/ml

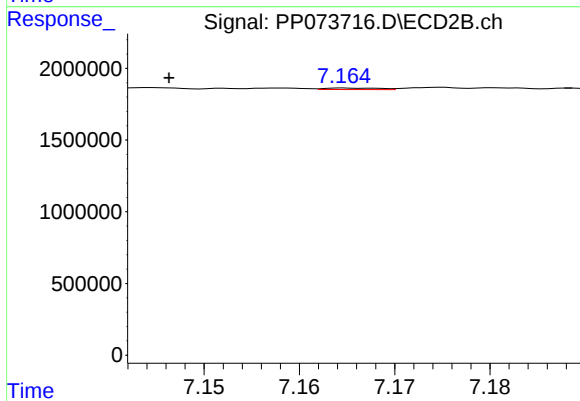

#34 AR-1260-4


R.T.: 7.165 min
Delta R.T.: 0.019 min
Response: 42150
Conc: 0.47 ng/ml

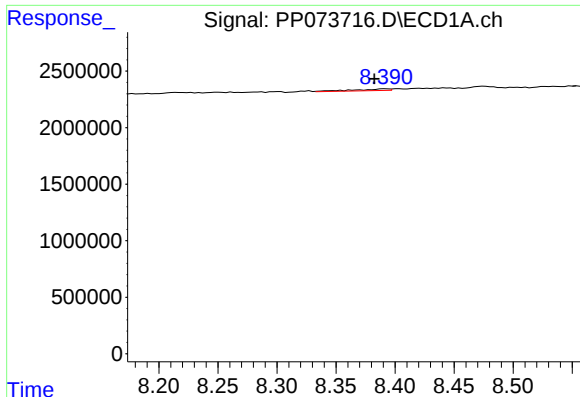

#35 AR-1260-5


R.T.: 8.391 min
Delta R.T.: 0.009 min
Response: 310856
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

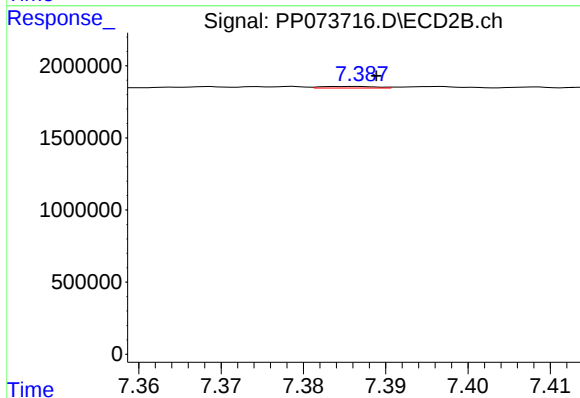


#35 AR-1260-5

R.T.: 7.387 min
Delta R.T.: -0.002 min
Response: 50371
Conc: 0.22 ng/ml

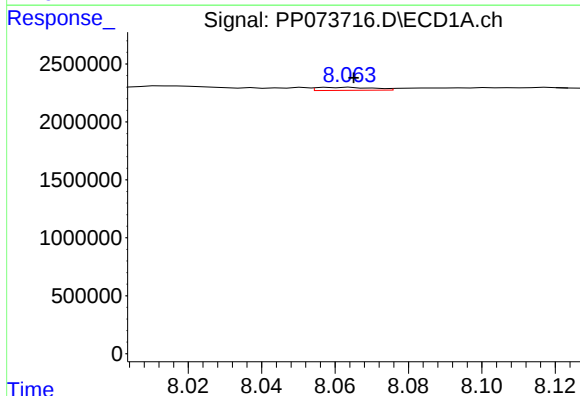


#36 AR-1262-1

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 280273
Conc: 3.22 ng/ml

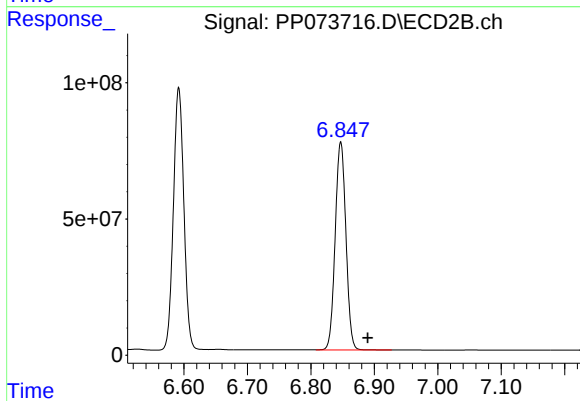

#36 AR-1262-1


R.T.: 6.847 min
Delta R.T.: -0.042 min
Response: 895157102
Conc: 6060.99 ng/ml

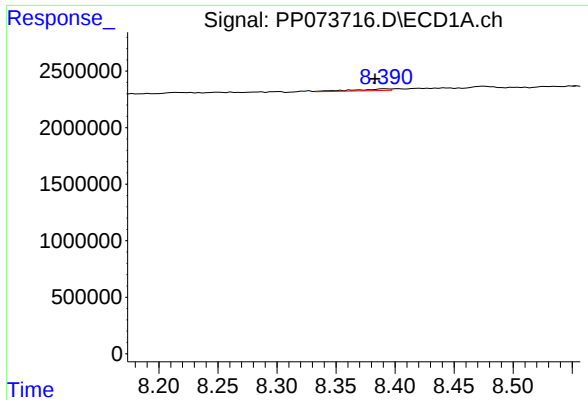

#37 AR-1262-2


R.T.: 8.391 min
Delta R.T.: 0.008 min
Response: 310856
Conc: 1.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

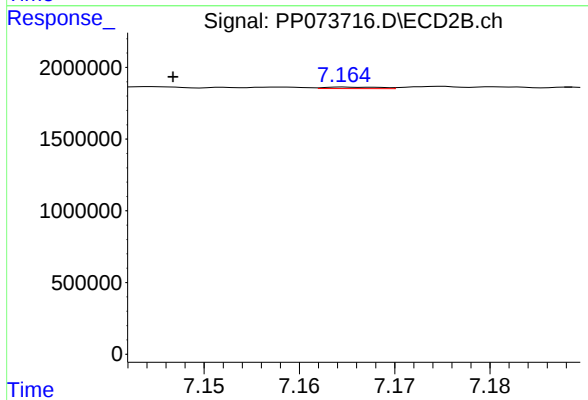


#37 AR-1262-2

R.T.: 7.165 min
Delta R.T.: 0.018 min
Response: 42150
Conc: 0.33 ng/ml

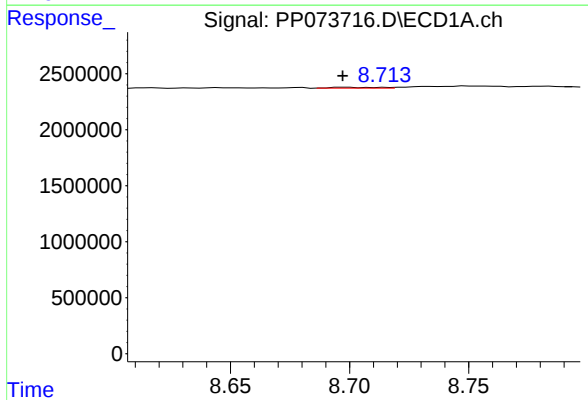


#38 AR-1262-3

R.T.: 8.698 min
Delta R.T.: 0.001 min
Response: 119382
Conc: 0.95 ng/ml

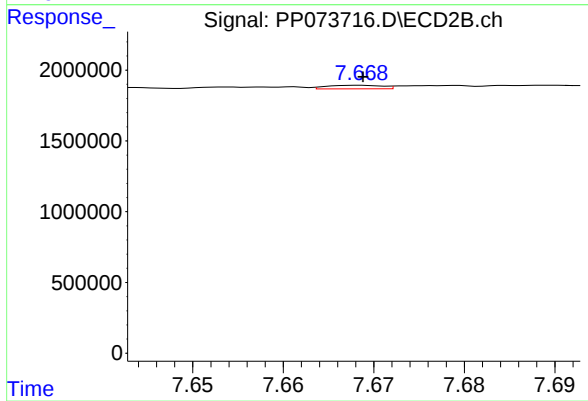

#38 AR-1262-3


R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 108384
Conc: 0.95 ng/ml

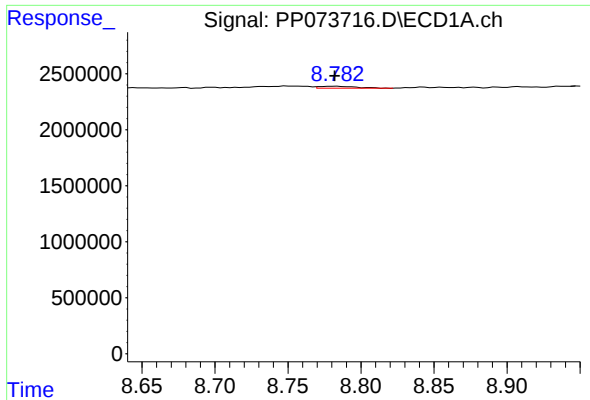

#39 AR-1262-4


R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 313718
Conc: 3.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

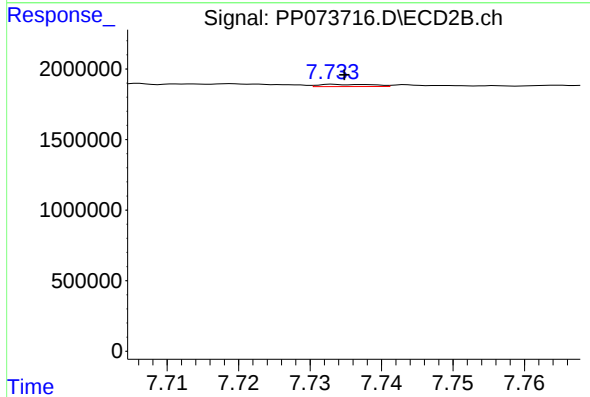


#39 AR-1262-4

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 82894
Conc: 0.45 ng/ml

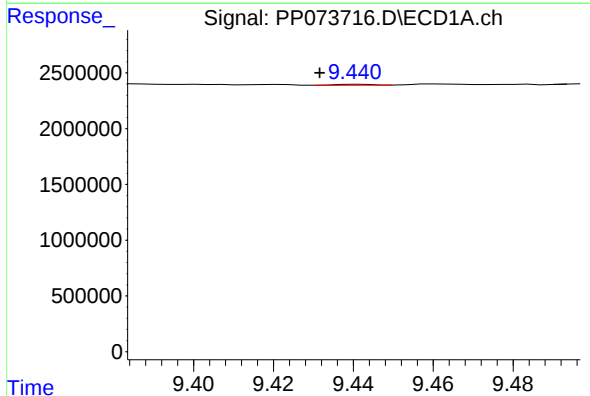


#40 AR-1262-5

R.T.: 9.441 min
Delta R.T.: 0.010 min
Response: 53829
Conc: 0.85 ng/ml

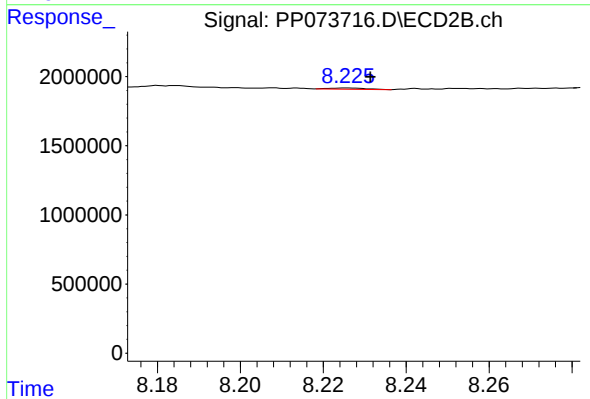

#40 AR-1262-5


R.T.: 8.226 min
Delta R.T.: -0.006 min
Response: 53127
Conc: 0.63 ng/ml

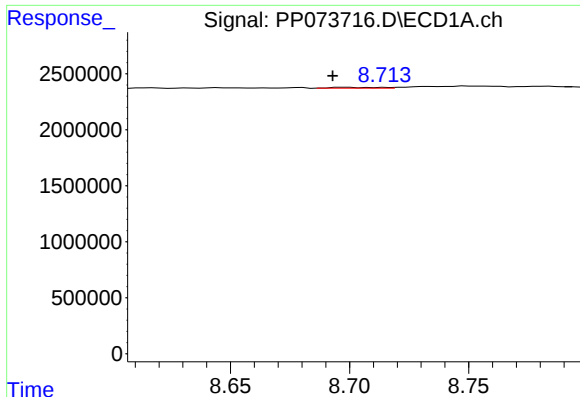

#41 AR-1268-1


R.T.: 8.698 min
Delta R.T.: 0.005 min
Response: 119382
Conc: 0.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

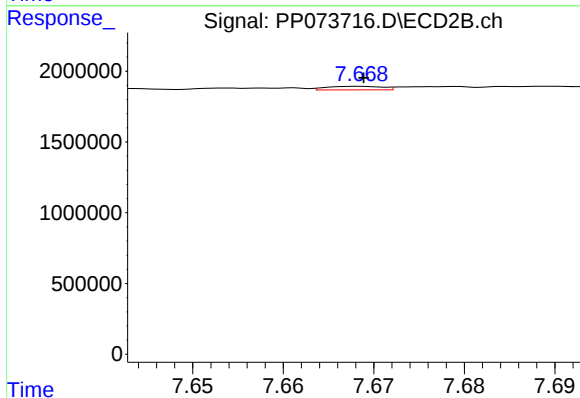


#41 AR-1268-1

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 108384
Conc: 0.35 ng/ml

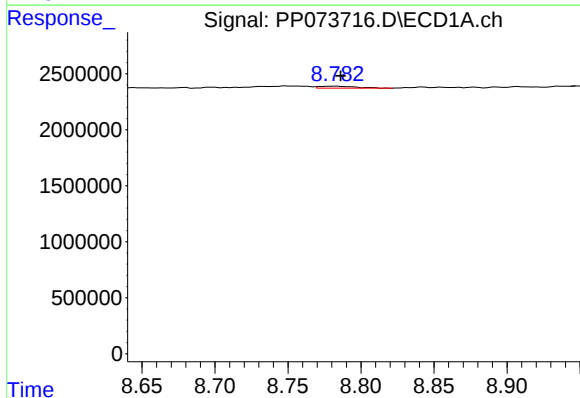


#42 AR-1268-2

R.T.: 8.782 min
Delta R.T.: -0.004 min
Response: 313718
Conc: 1.65 ng/ml

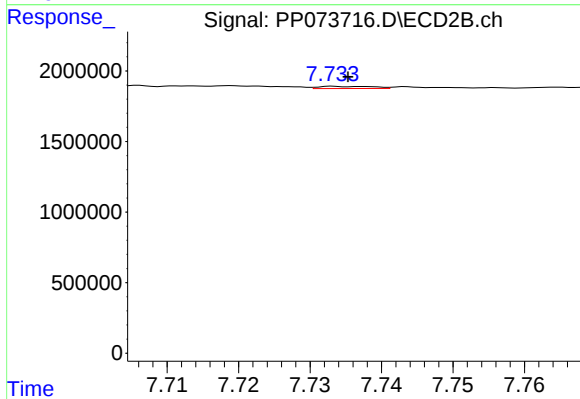

#42 AR-1268-2


R.T.: 7.733 min
Delta R.T.: -0.002 min
Response: 82894
Conc: 0.31 ng/ml

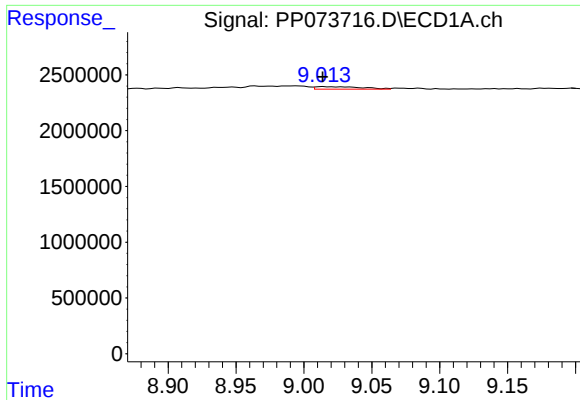

#43 AR-1268-3


R.T.: 9.014 min
Delta R.T.: 0.000 min
Response: 520908
Conc: 3.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

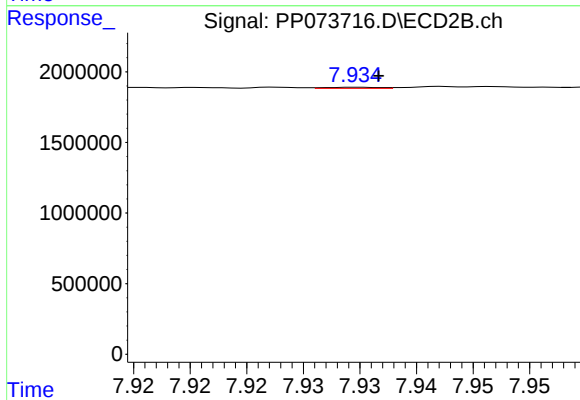


#43 AR-1268-3

R.T.: 7.935 min
Delta R.T.: -0.002 min
Response: 25667
Conc: 0.11 ng/ml

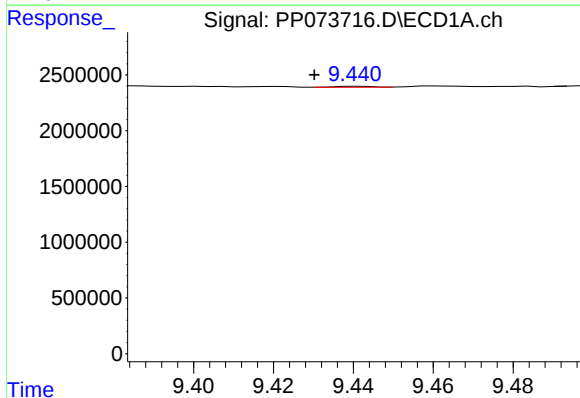


#44 AR-1268-4

R.T.: 9.441 min
Delta R.T.: 0.011 min
Response: 53829
Conc: 0.77 ng/ml

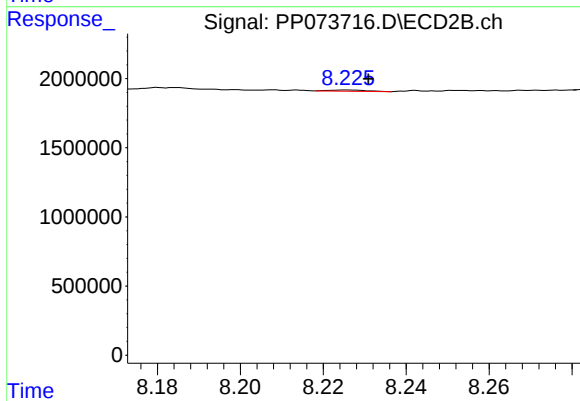

#44 AR-1268-4


R.T.: 8.226 min
Delta R.T.: -0.005 min
Response: 53127
Conc: 0.57 ng/ml

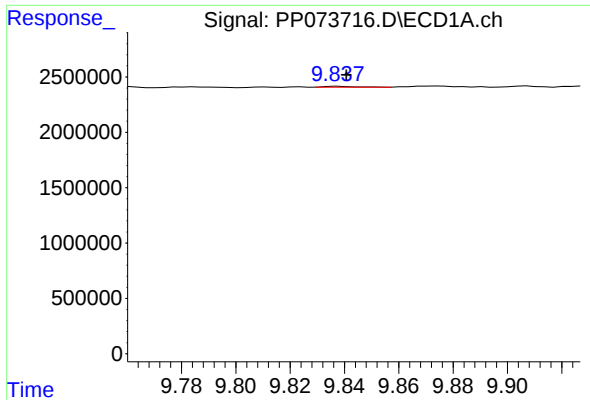

#45 AR-1268-5

R.T.: 9.838 min
Delta R.T.: -0.003 min
Response: 79045
Conc: 0.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOGUE

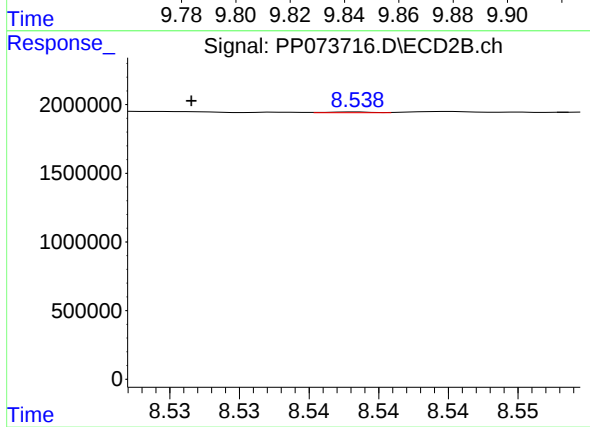

#45 AR-1268-5

R.T.: 8.538 min
Delta R.T.: 0.012 min
Response: 11574
Conc: 0.02 ng/ml