

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071225\
 Data File : PP073732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2025 18:21
 Operator : YP\AJ
 Sample : Q2565-04 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-25-0196

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/14/2025
 Supervised By :mohammad ahmed 07/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 22:52:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.778	1235571	1764852	0.902m	0.958
2) SA Decachlor...	10.175	8.777	1270698	1578204	1.165	1.193

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071225\
Data File : PP073732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2025 18:21
Operator : YP\AJ
Sample : Q2565-04 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-25-0196


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2025
Supervised By :mohammad ahmed 07/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 22:52:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

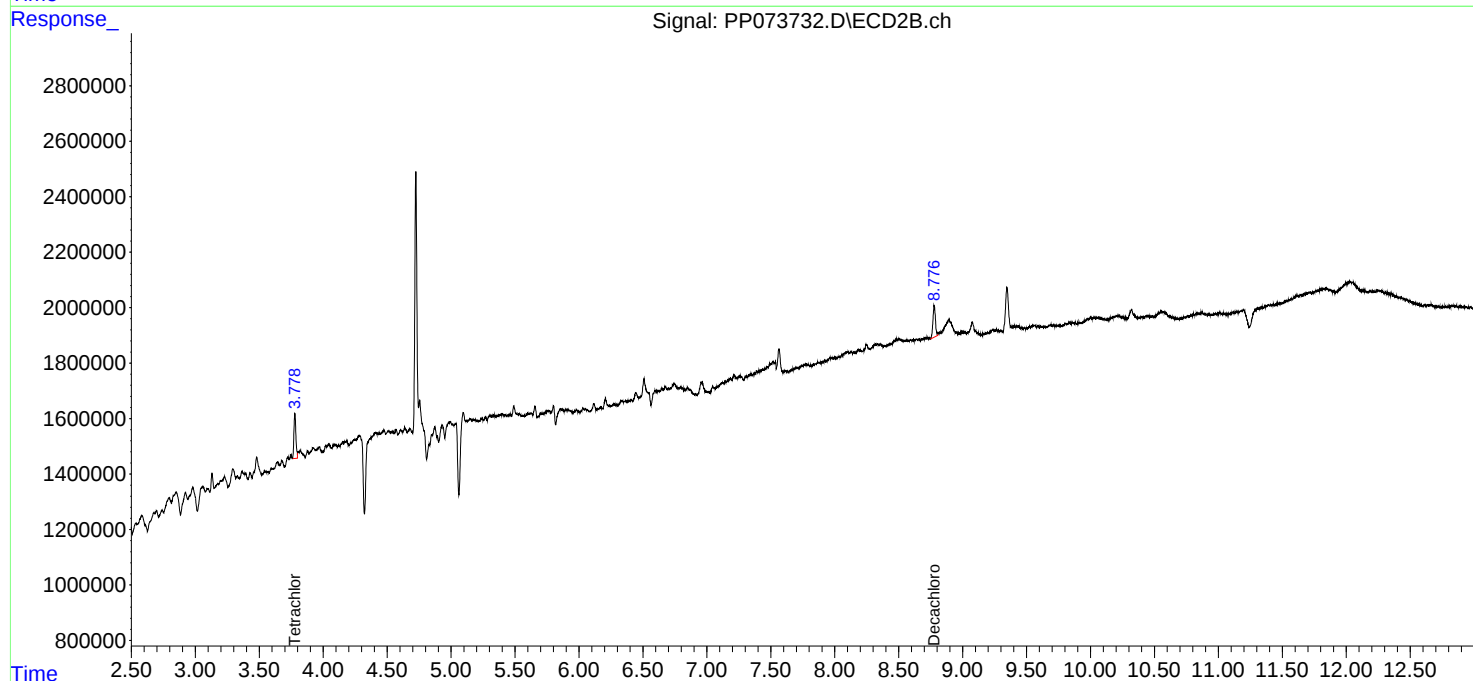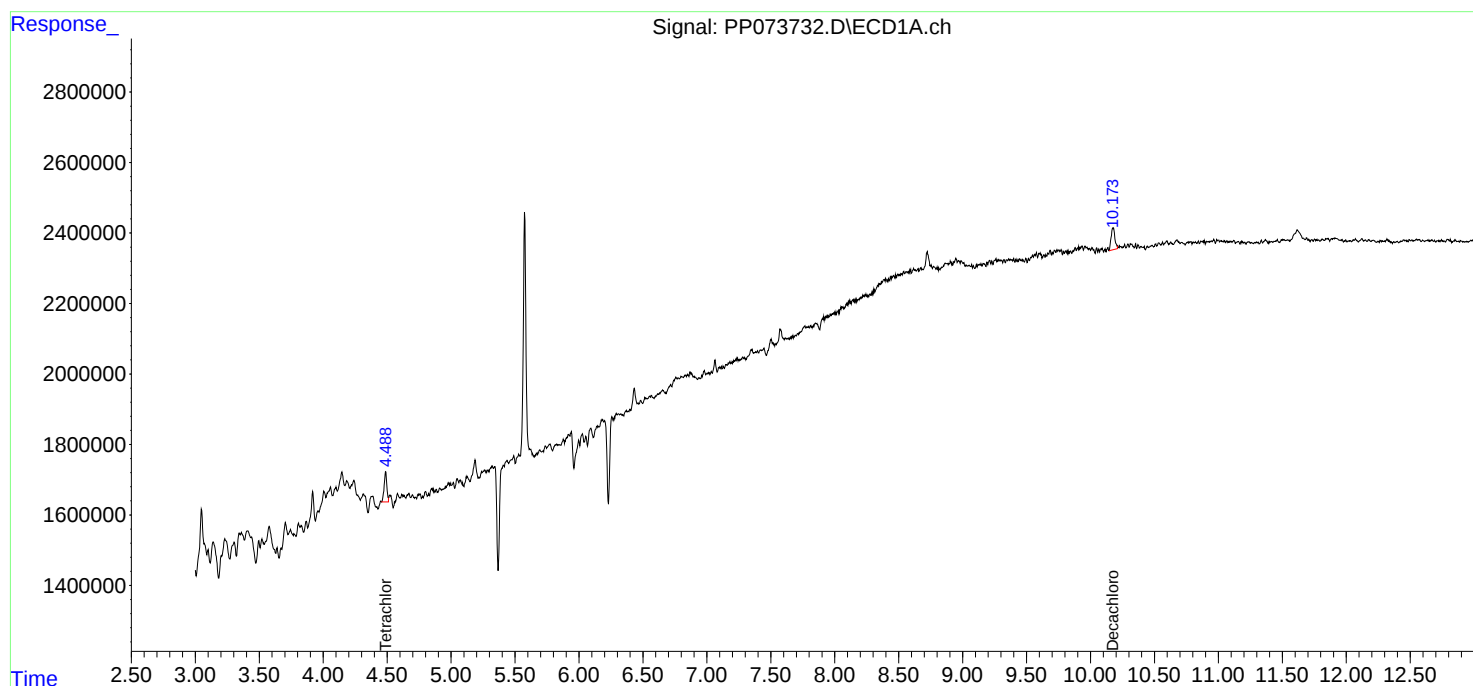

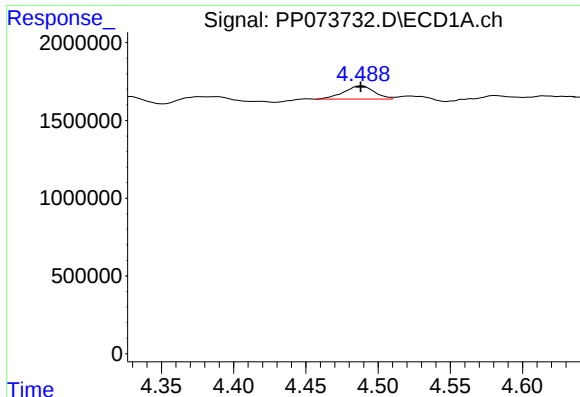


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 1235571
Conc: 0.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-25-0196


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2025
Supervised By :mohammad ahmed 07/15/2025

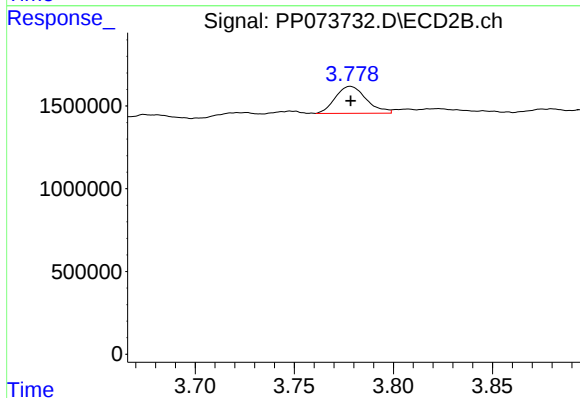


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: 0.000 min
Response: 1764852
Conc: 0.96 ng/ml

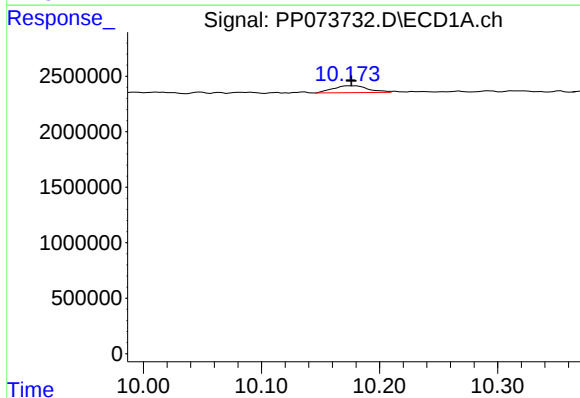

#2 Decachlorobiphenyl

R.T.: 10.175 min
Delta R.T.: -0.001 min
Response: 1270698
Conc: 1.16 ng/ml

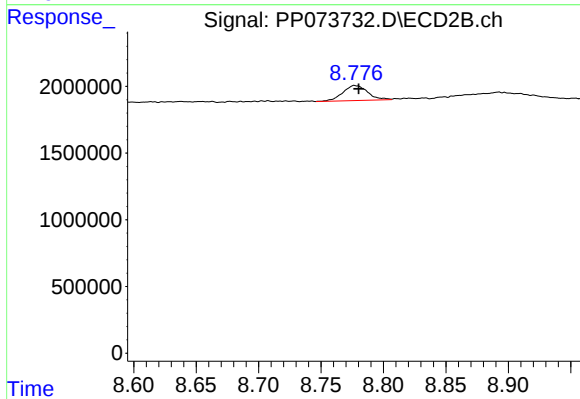

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: -0.003 min
Response: 1578204
Conc: 1.19 ng/ml