

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071321\
 Data File : PP037260.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jul 2021 12:46
 Operator : DD\AJ
 Sample : M3011-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

mohammad
 7/14/2021 12:22:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:13:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.955	3.946	955846	609931	21.031m	22.289
2) SA Decachlor...	10.985	9.237	989149	744505	21.487	26.747m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071321\
Data File : PP037260.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2021 12:46
Operator : DD\AJ
Sample : M3011-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

mohammad
7/14/2021 12:22:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:13:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

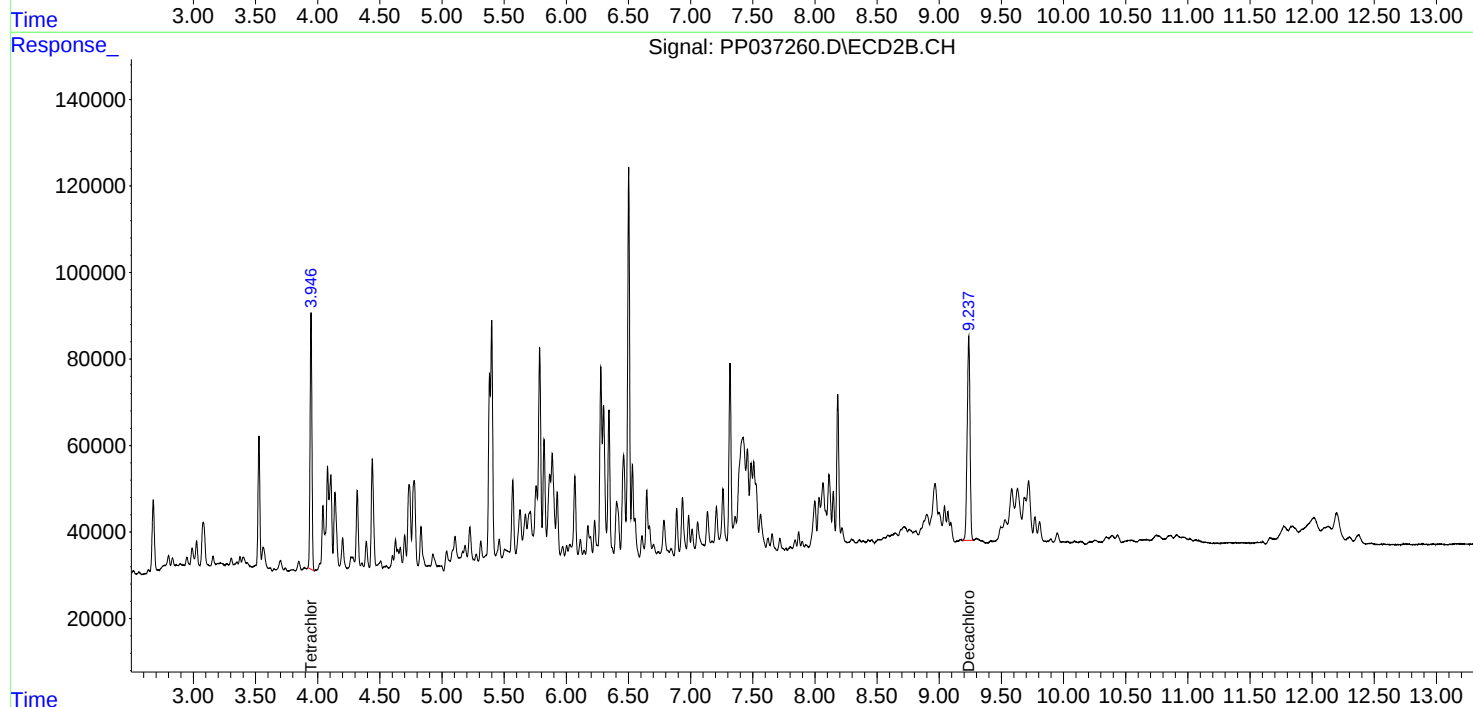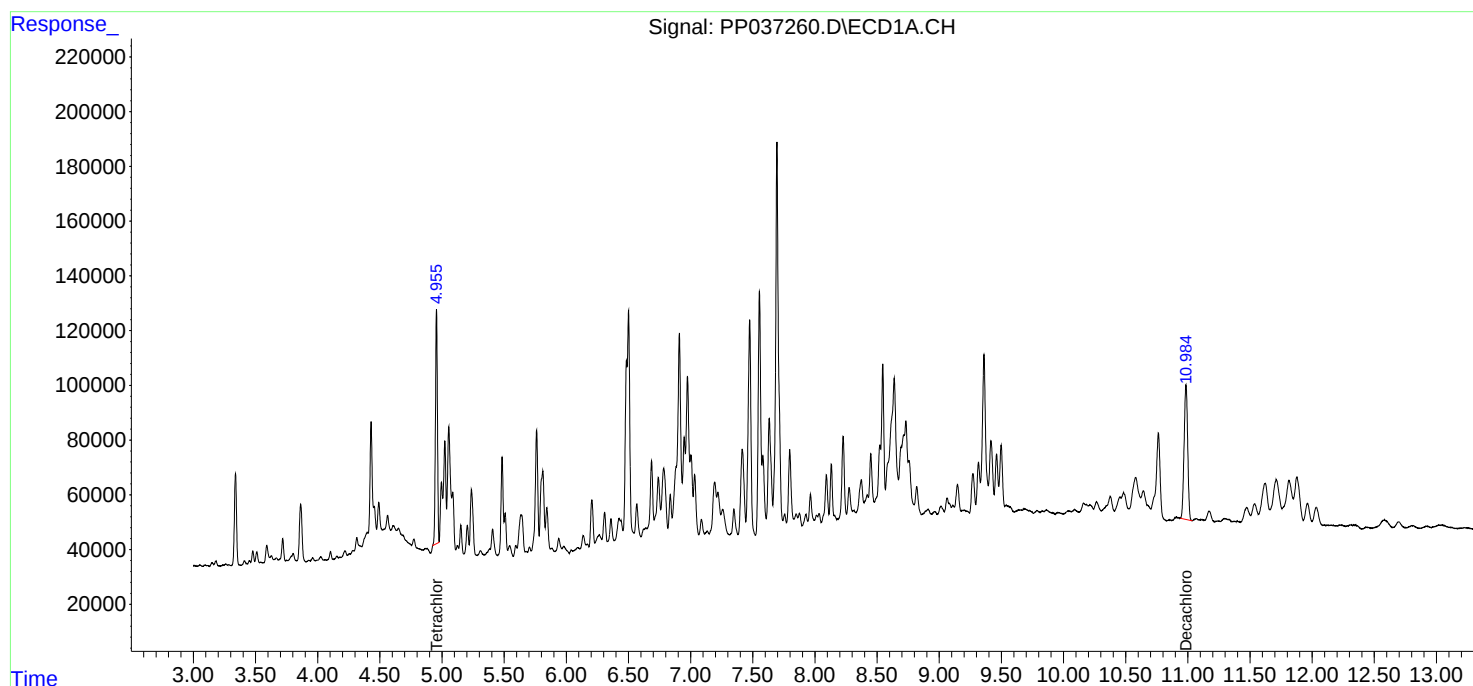

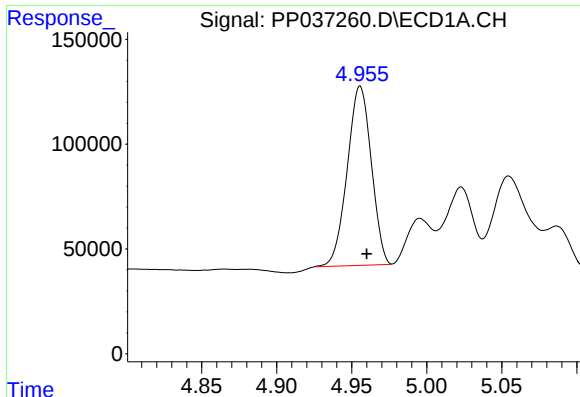

#1 Tetrachloro-m-xylene

R.T.: 4.955 min

Delta R.T.: -0.005 min


Response: 955846

Conc: 21.03 ng/ml m

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C

Manual Integrations
APPROVED

mohammad
7/14/2021 12:22:10 PM

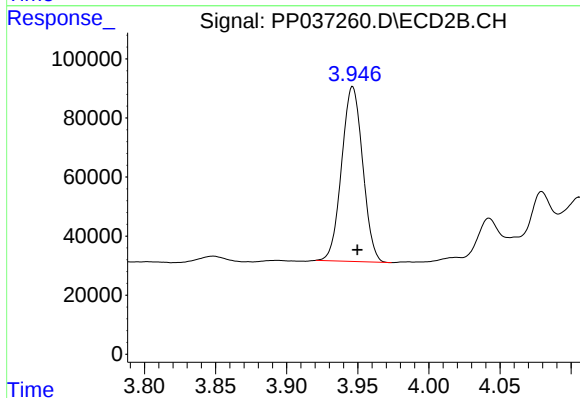


#1 Tetrachloro-m-xylene

R.T.: 3.946 min

Delta R.T.: -0.003 min

Response: 609931

Conc: 22.29 ng/ml

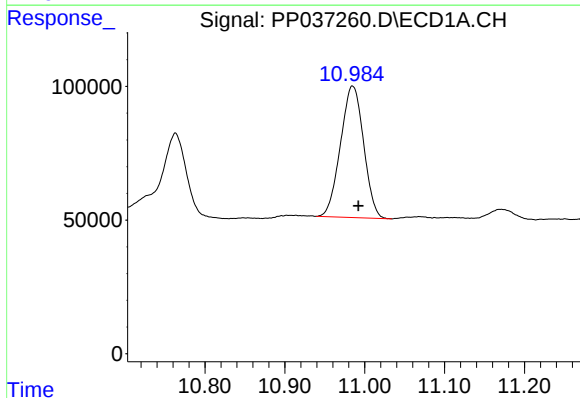


#2 Decachlorobiphenyl

R.T.: 10.985 min

Delta R.T.: -0.007 min

Response: 989149

Conc: 21.49 ng/ml

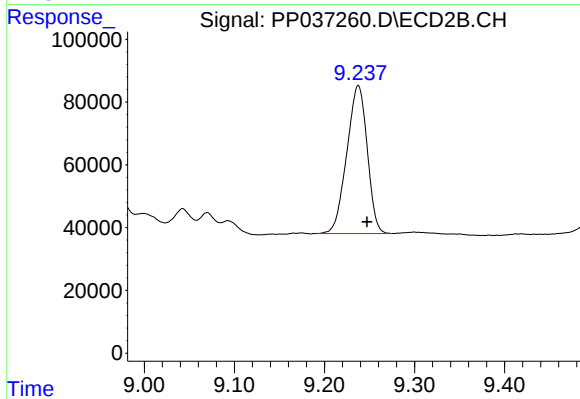

#2 Decachlorobiphenyl

R.T.: 9.237 min

Delta R.T.: -0.010 min

Response: 744505

Conc: 26.75 ng/ml m