

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071423\
 Data File : PP058731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 16:51
 Operator : YP\AJ
 Sample : 03614-02 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC280325-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 05:41:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jul 02 11:11:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.439	3.670	2425384	3088386	1.491	1.375
2) SA Decachlor...	10.248	8.724	2376443	3622737	2.019m	1.998

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071423\
Data File : PP058731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 16:51
Operator : YP\AJ
Sample : 03614-02 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC280325-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 05:41:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jul 02 11:11:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

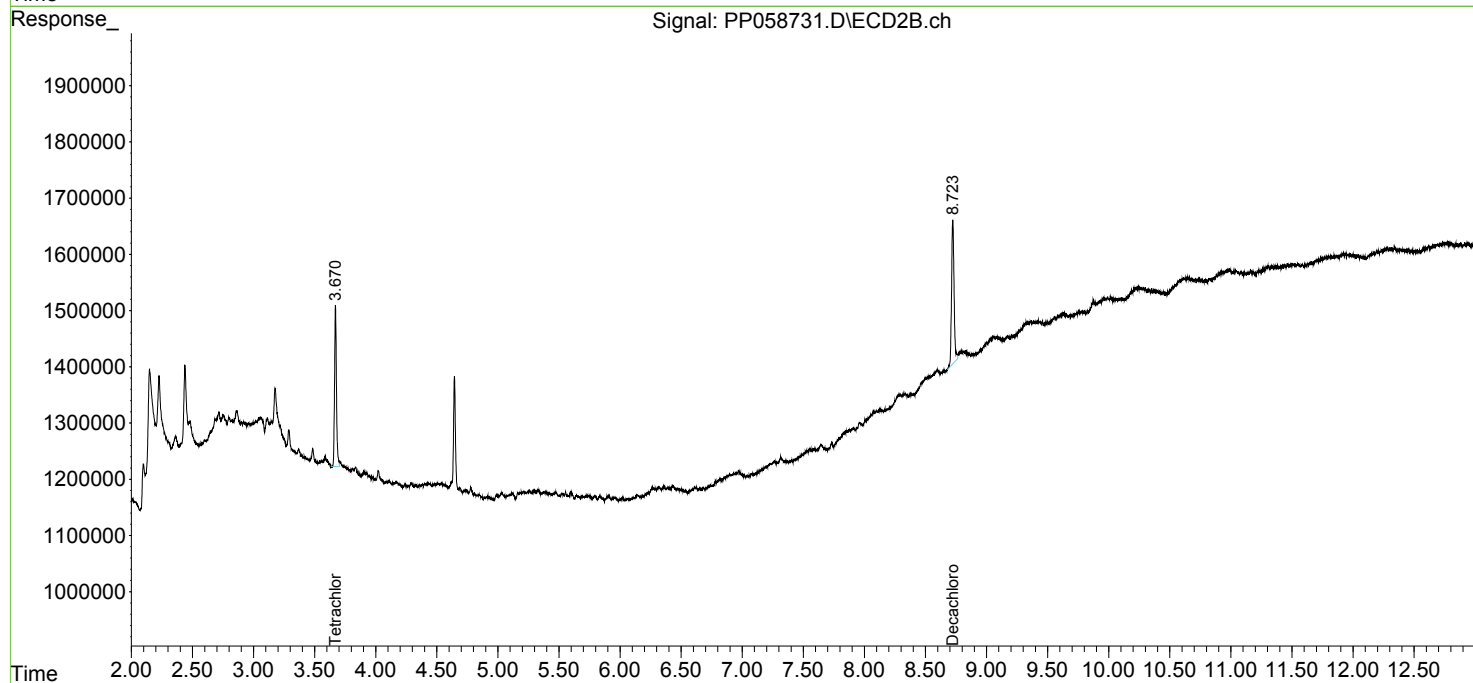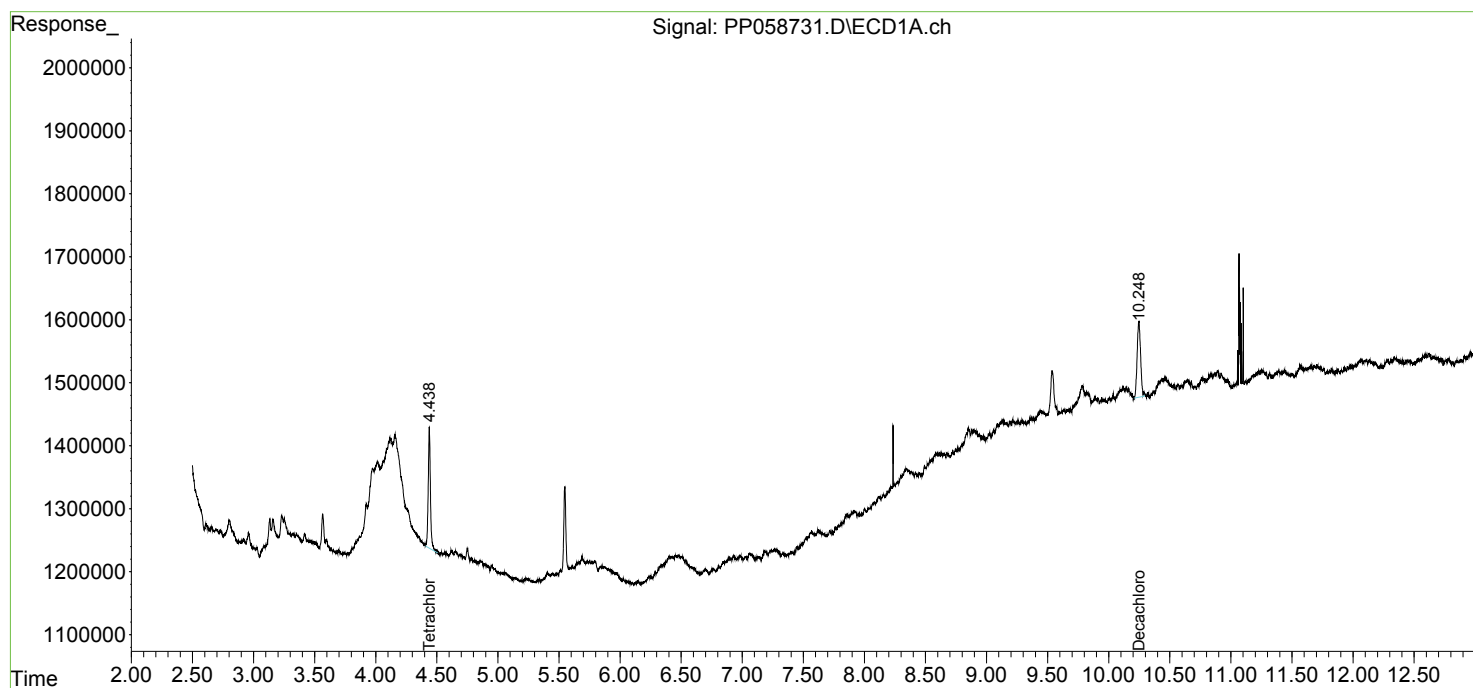

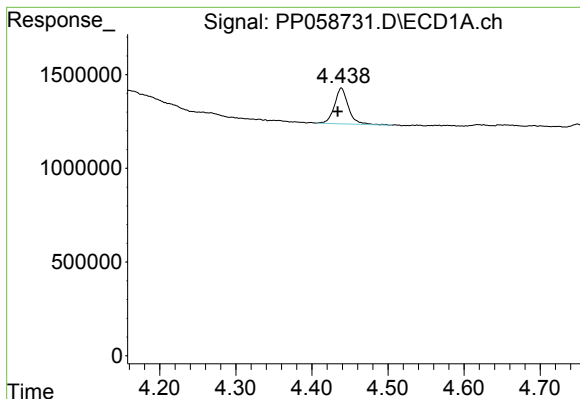

#1 Tetrachloro-m-xylene

R.T.: 4.439 min
Delta R.T.: 0.005 min
Response: 2425384
Conc: 1.49 ng/ml

Instrument :

ECD_P


ClientSampleId :

BC280325-1-2

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

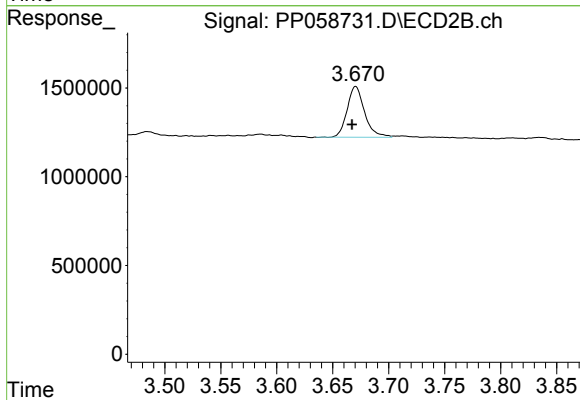


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.003 min
Response: 3088386
Conc: 1.37 ng/ml

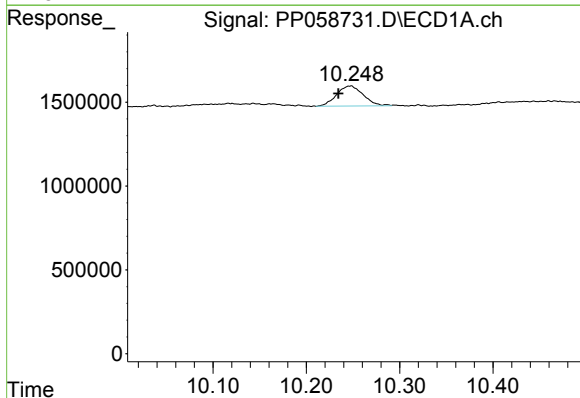

#2 Decachlorobiphenyl

R.T.: 10.248 min
Delta R.T.: 0.014 min
Response: 2376443
Conc: 2.02 ng/ml m

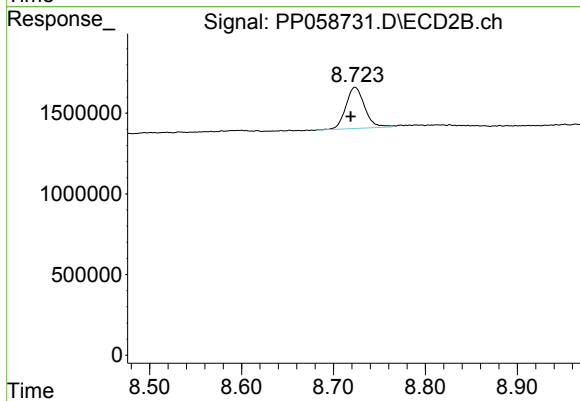

#2 Decachlorobiphenyl

R.T.: 8.724 min
Delta R.T.: 0.005 min
Response: 3622737
Conc: 2.00 ng/ml