

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071425\
 Data File : PP073765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2025 12:41
 Operator : YP\AJ
 Sample : Q2565-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-25-0192-0193

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/14/2025
 Supervised By :mohammad ahmed 07/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 14:55:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.487	3.780	17757576	23151176	12.966m	12.567
2) SA Decachlor...	10.172	8.778	11156240	13841072	10.225	10.461

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071425\
Data File : PP073765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2025 12:41
Operator : YP\AJ
Sample : Q2565-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-25-0192-0193


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2025
Supervised By :mohammad ahmed 07/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 14:55:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

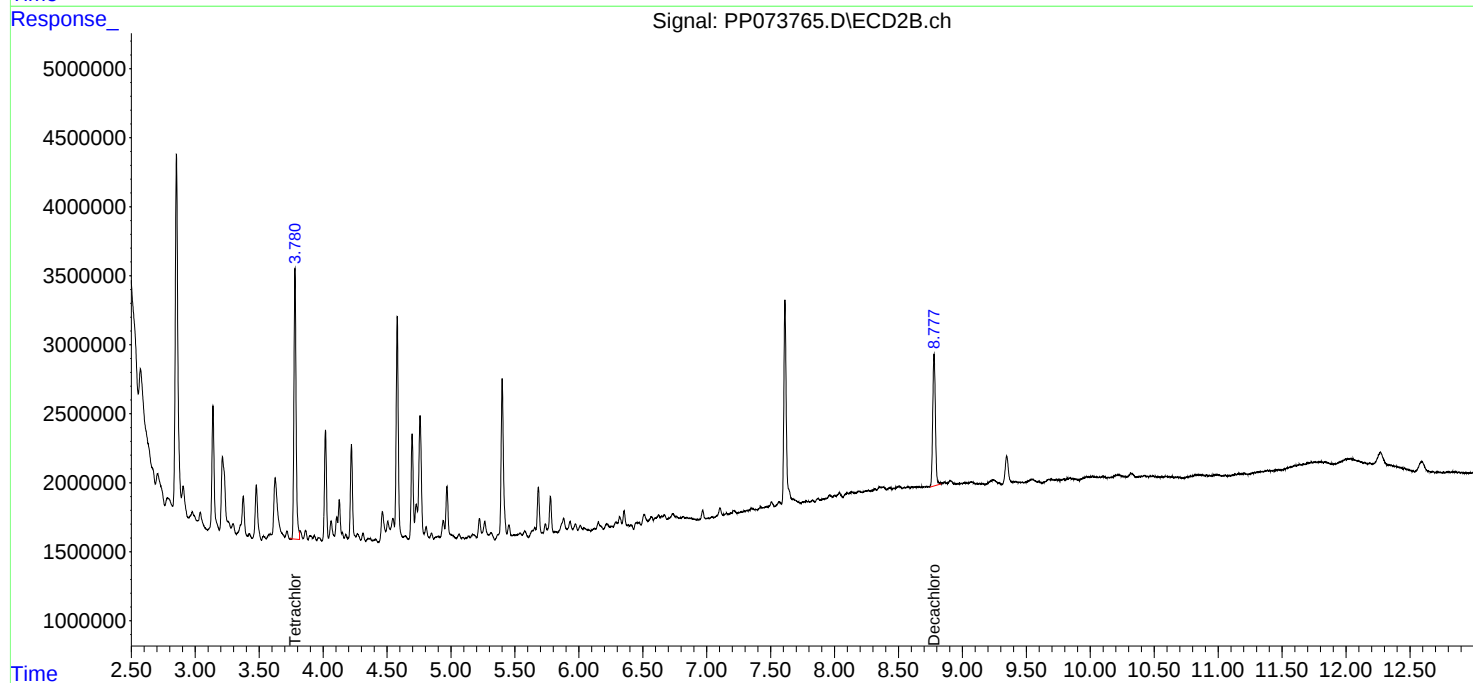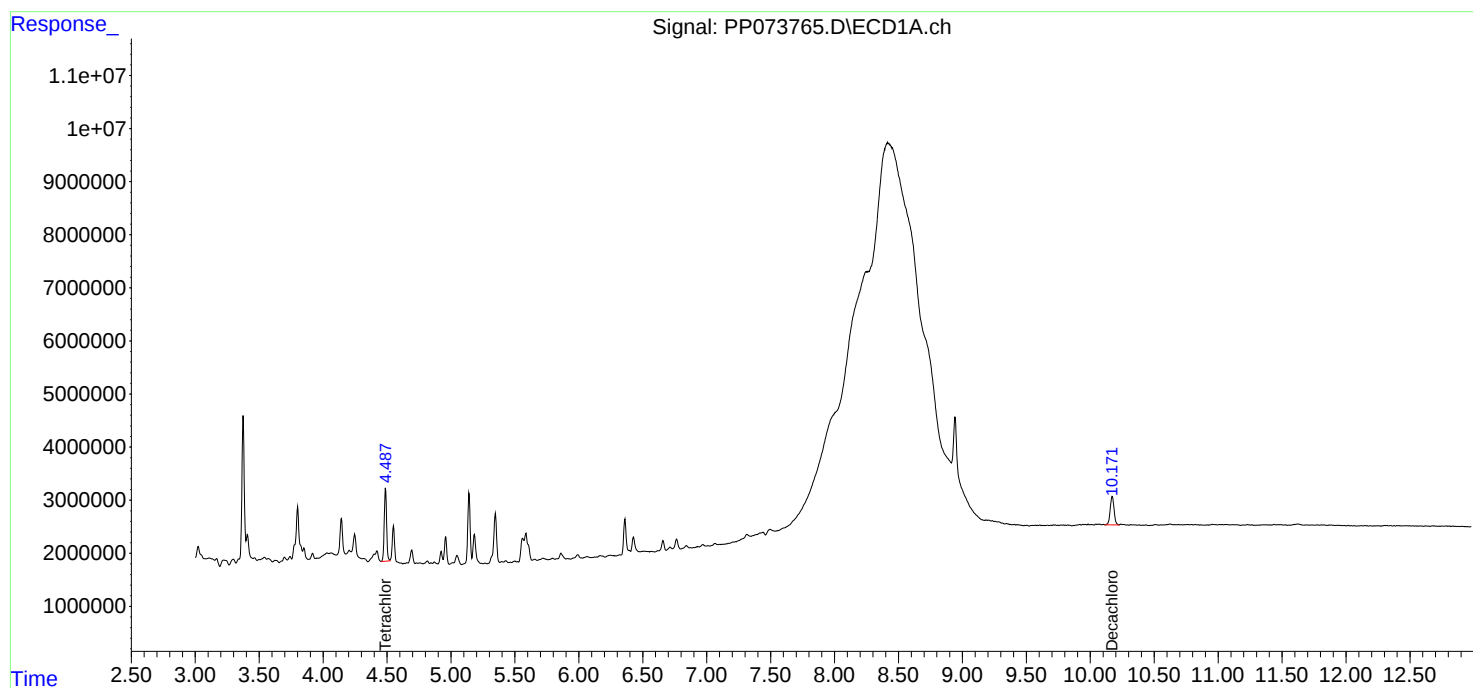

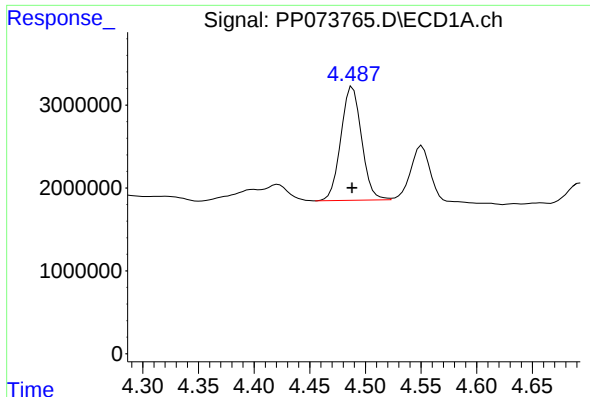


#1 Tetrachloro-m-xylene

R.T.: 4.487 min
Delta R.T.: 0.000 min
Response: 17757576
Conc: 12.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-25-0192-0193


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2025
Supervised By :mohammad ahmed 07/16/2025

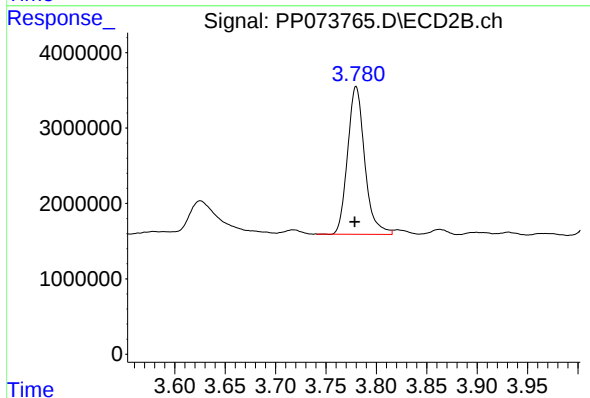


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: 0.002 min
Response: 23151176
Conc: 12.57 ng/ml

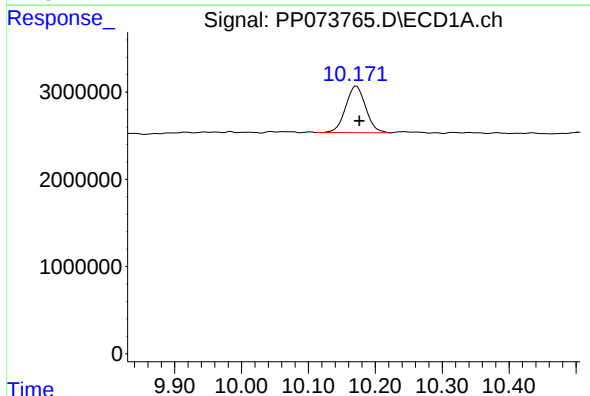

#2 Decachlorobiphenyl

R.T.: 10.172 min
Delta R.T.: -0.004 min
Response: 11156240
Conc: 10.23 ng/ml

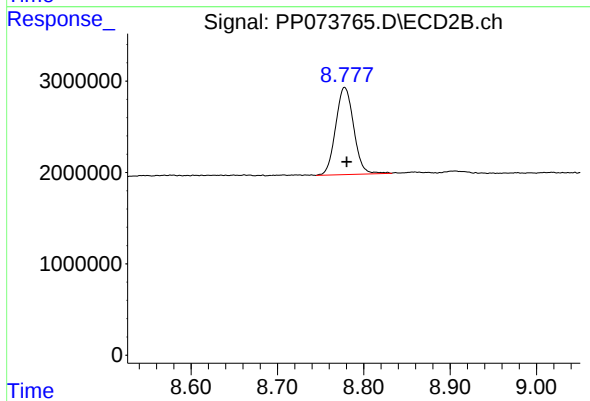

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.002 min
Response: 13841072
Conc: 10.46 ng/ml