

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071521\
 Data File : PP037303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2021 13:00
 Operator : DD\AJ
 Sample : PB137703BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 15:38:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.955	3.945	862081	498358	18.968	18.212
2)	SA Decachlor...	10.985	9.239	949392	527798	20.623	18.962
Target Compounds							
8)	L2 AR-1221-1	5.206	0.000	40190	0	75.777	N.D. #
9)	L2 AR-1221-2	5.308	0.000	11824	0	29.185	N.D. #
28)	L6 AR-1254-3	7.814	0.000	23211	0	7.529	N.D. #
34)	L7 AR-1260-4	8.815	0.000	6368	0	2.589	N.D. #
35)	L7 AR-1260-5	9.140f	0.000	1844	0	0.400	N.D. #
37)	L8 AR-1262-2	9.140f	0.000	1844	0	0.351	N.D. #
38)	L8 AR-1262-3	0.000	8.142f	0	26139	N.D.	18.566 #
41)	L9 AR-1268-1	0.000	8.142f	0	26139	N.D.	6.559 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071521\
Data File : PP037303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2021 13:00
Operator : DD\AJ
Sample : PB137703BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 15:38:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

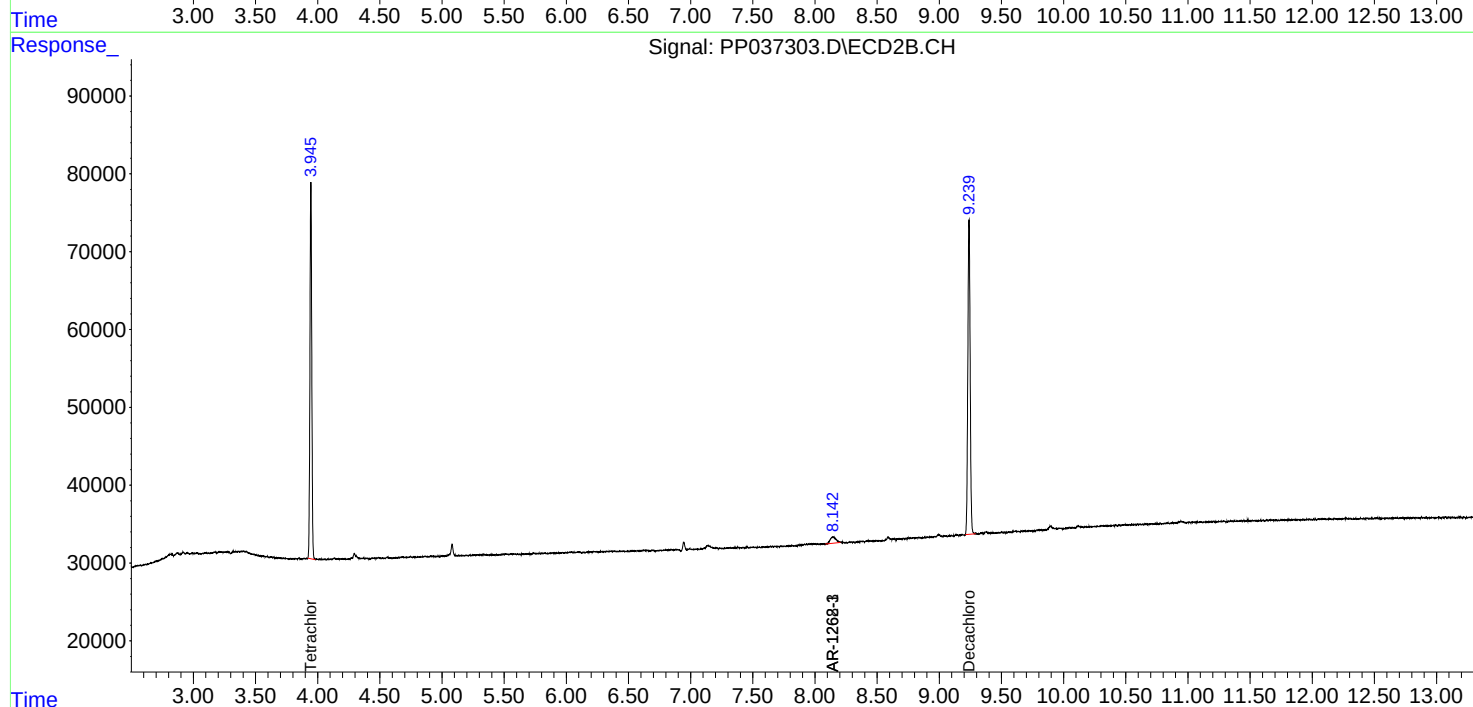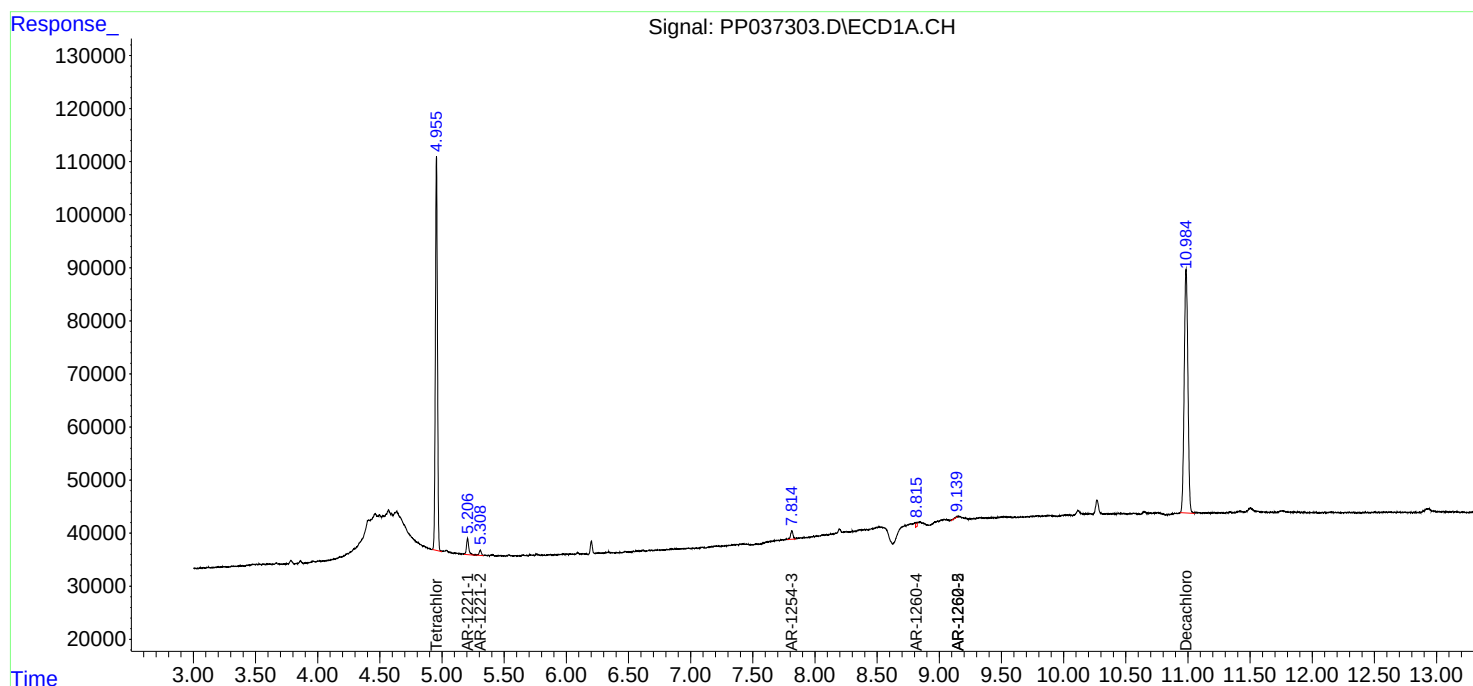


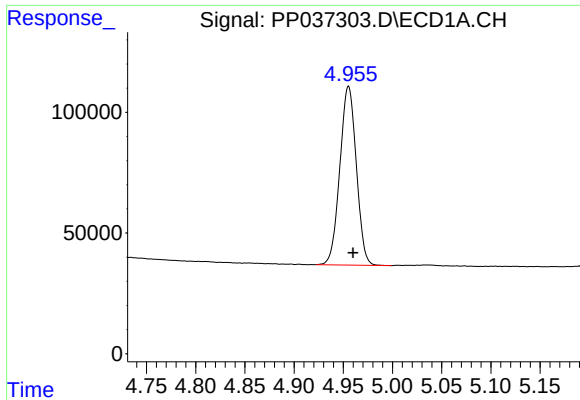

#1 Tetrachloro-m-xylene


R.T.: 4.955 min
Delta R.T.: -0.005 min
Response: 862081
Conc: 18.97 ng/ml

Instrument :
ECD_P
ClientSampleId :

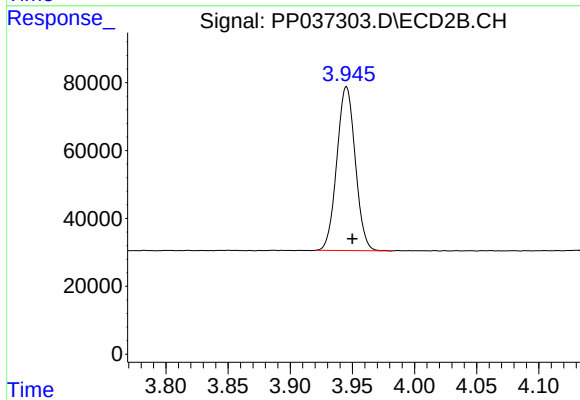


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: -0.005 min
Response: 498358
Conc: 18.21 ng/ml

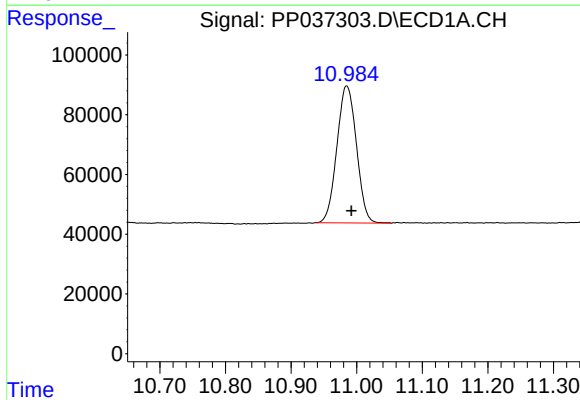


#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.008 min
Response: 949392
Conc: 20.62 ng/ml

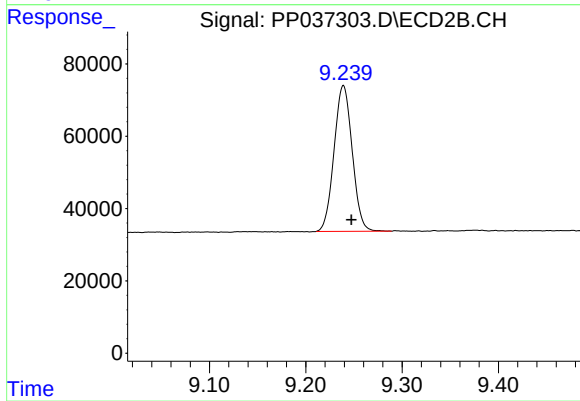

#2 Decachlorobiphenyl


R.T.: 9.239 min
Delta R.T.: -0.008 min
Response: 527798
Conc: 18.96 ng/ml

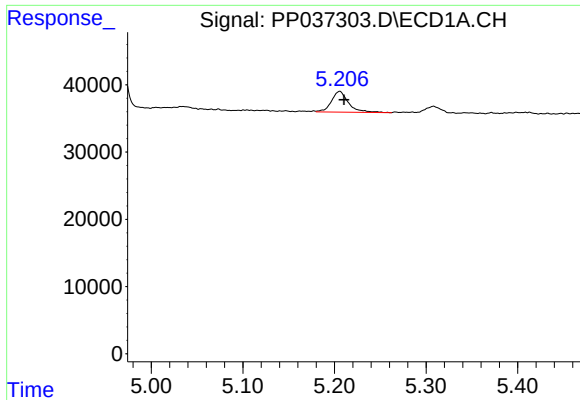

#8 AR-1221-1


R.T.: 5.206 min
Delta R.T.: -0.005 min
Response: 40190
Conc: 75.78 ng/ml

Instrument :
ECD_P
ClientSampleId :

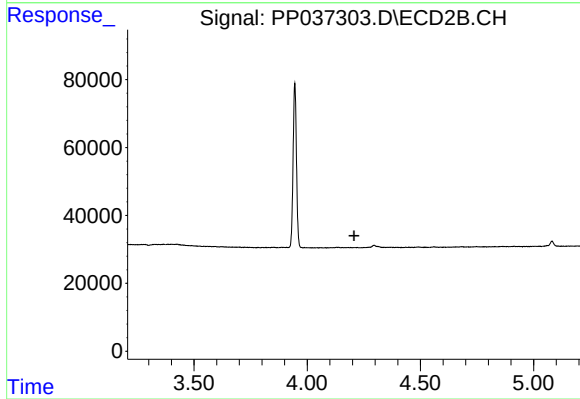


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

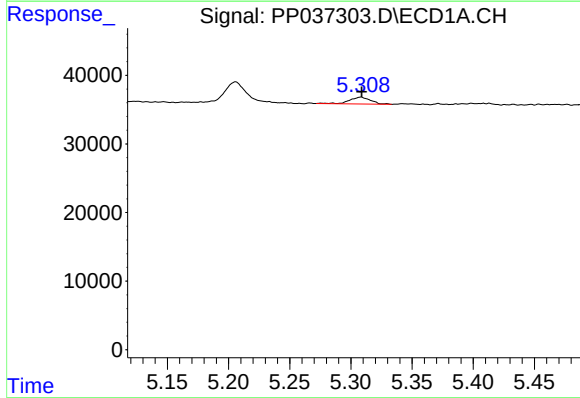


#9 AR-1221-2

R.T.: 5.308 min
Delta R.T.: 0.000 min
Response: 11824
Conc: 29.18 ng/ml

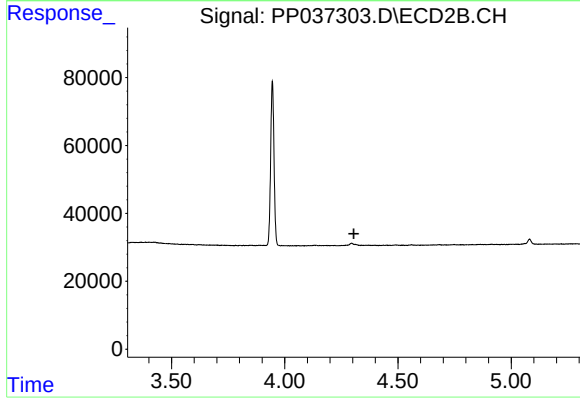

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

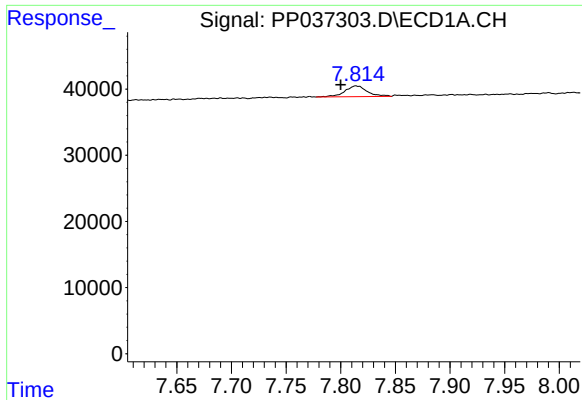

#28 AR-1254-3


R.T.: 7.814 min
Delta R.T.: 0.014 min
Response: 23211
Conc: 7.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

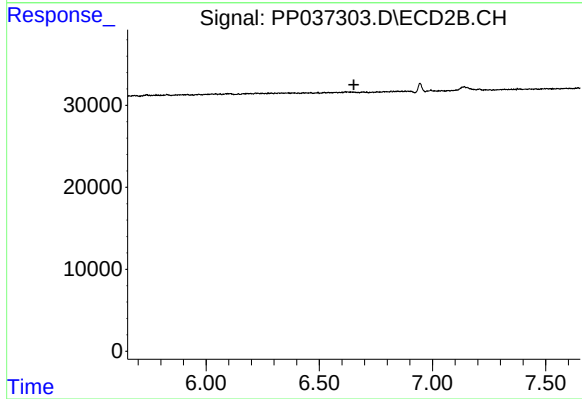


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.

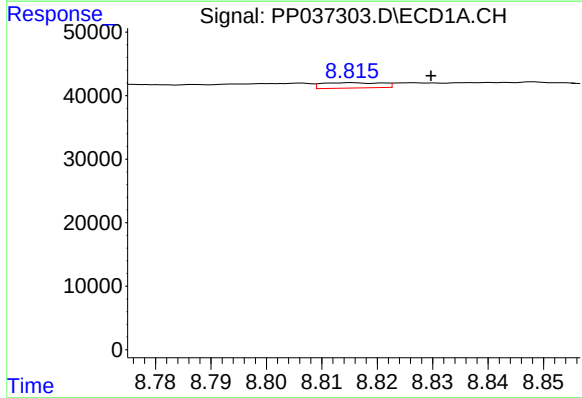


#34 AR-1260-4

R.T.: 8.815 min
Delta R.T.: -0.014 min
Response: 6368
Conc: 2.59 ng/ml

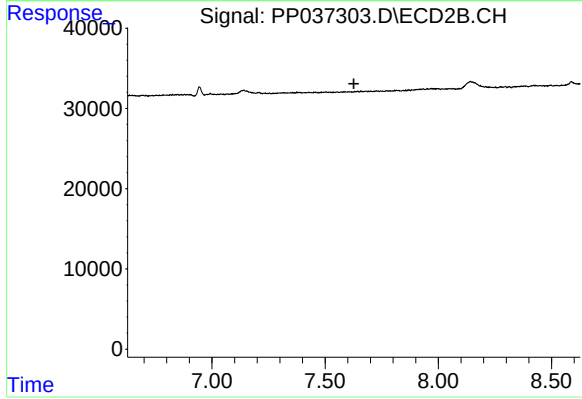

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.627 min
Response: 0
Conc: N.D.

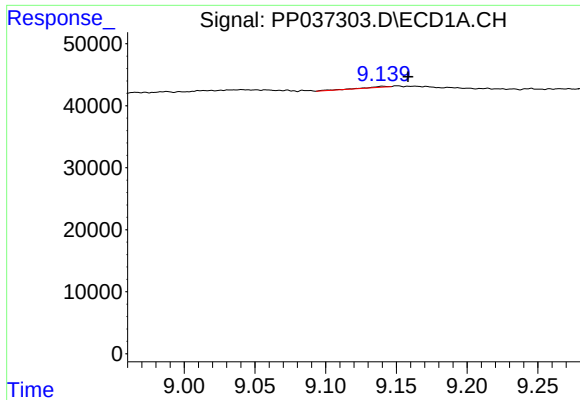

#35 AR-1260-5


R.T.: 9.140 min
Delta R.T.: -0.018 min
Response: 1844
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

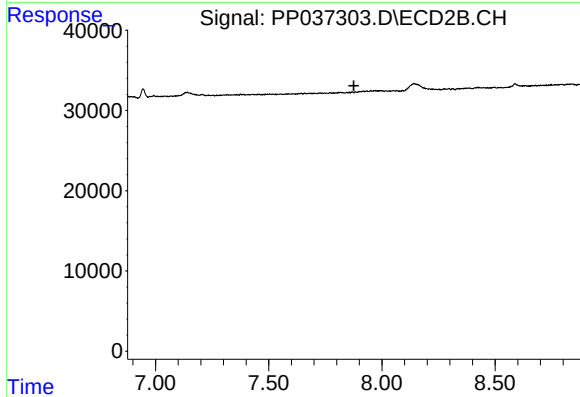


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.876 min
Response: 0
Conc: N.D.

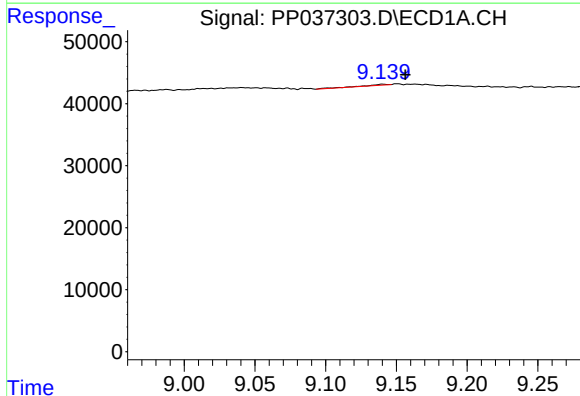


#37 AR-1262-2

R.T.: 9.140 min
Delta R.T.: -0.016 min
Response: 1844
Conc: 0.35 ng/ml

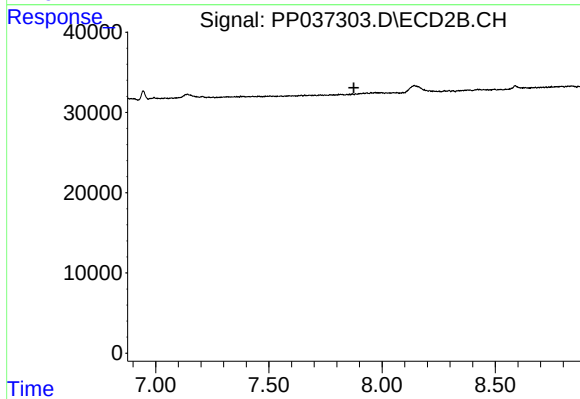

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.875 min
Response: 0
Conc: N.D.

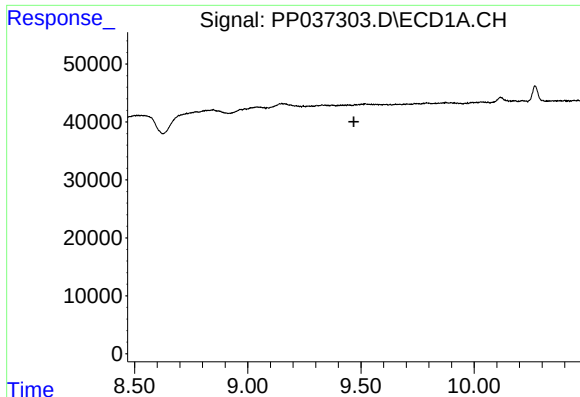

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

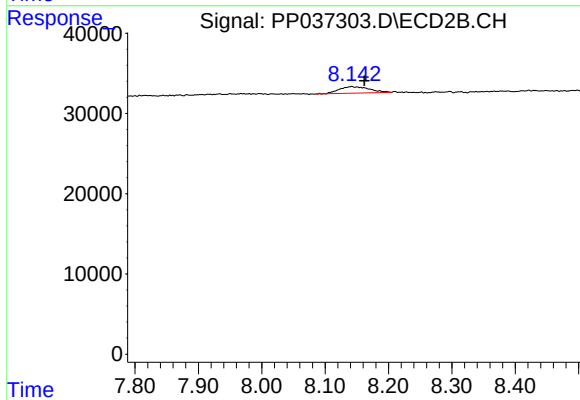


#38 AR-1262-3

R.T.: 8.142 min
Delta R.T.: -0.020 min
Response: 26139
Conc: 18.57 ng/ml

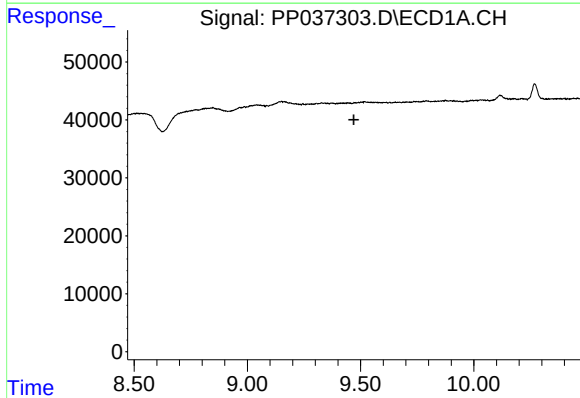

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.470 min
Response: 0
Conc: N.D.

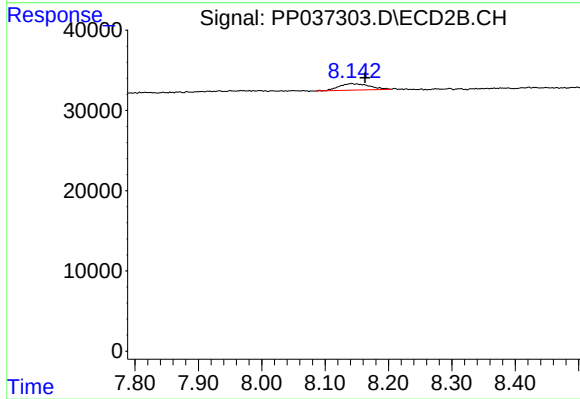

#41 AR-1268-1

R.T.: 8.142 min
Delta R.T.: -0.021 min
Response: 26139
Conc: 6.56 ng/ml