

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071525\
 Data File : PP073794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2025 10:38
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:42:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.520f	3.778	78582	21046	0.057	0.011 #
2)	SA Decachlor...	10.220	8.776	70670	106724	0.065	0.081
Target Compounds							
3)	L1 AR-1016-1	5.633	4.854	258495	78156	5.440	1.146 #
4)	L1 AR-1016-2	5.683	4.868	194905	86010	2.737	0.844 #
5)	L1 AR-1016-3	5.725	5.034	218229	141244	4.998	2.610 #
6)	L1 AR-1016-4	5.827	5.094	62005	598550	1.725	13.640 #
7)	L1 AR-1016-5	6.131	5.313	415341	141979	13.257	2.601 #
8)	L2 AR-1221-1	4.729f	3.994	62303	83230	3.487	3.077
9)	L2 AR-1221-2	4.765	4.082	148325	27313	10.983	1.341 #
10)	L2 AR-1221-3	4.839	4.149	192917	33886	4.637	0.551 #
11)	L3 AR-1232-1	4.839	4.149	192917	33886	5.909	0.727 #
12)	L3 AR-1232-2	5.380	4.868	34736	86010	2.137	1.805
13)	L3 AR-1232-3	5.683	5.034	194905	141244	5.907	5.643
14)	L3 AR-1232-4	5.827	5.139	62005	55503	3.770	2.563 #
15)	L3 AR-1232-5	5.895	5.313	180494	141979	17.076	6.292 #
16)	L4 AR-1242-1	5.633	4.854	258495	78156	6.769	1.353 #
17)	L4 AR-1242-2	5.633	4.868	258495	86010	4.317	0.995 #
18)	L4 AR-1242-3	5.725	5.034	218229	141244	5.959	3.074 #
19)	L4 AR-1242-4	5.808	5.139	87211	55503	2.714	1.254 #
20)	L4 AR-1242-5	6.555	5.643	391228	461889	11.951	8.361 #
21)	L5 AR-1248-1	5.633	4.854	258495	78156	8.374	1.741 #
22)	L5 AR-1248-2	5.895	5.094	180494	598550	4.521	9.727 #
23)	L5 AR-1248-3	6.131	5.139	415341	55503	9.353	0.866 #
24)	L5 AR-1248-4	6.513	5.313	143892	141979	2.612	1.884 #
25)	L5 AR-1248-5	6.555	5.680	391228	367729	7.273	4.930 #
26)	L6 AR-1254-1	6.463	5.673	1997980	205582	37.283	1.772 #
27)	L6 AR-1254-2	6.699	5.823	3564862	5427573	42.801	53.939 #
28)	L6 AR-1254-3	7.070	6.219	4031476	2279060	45.640	14.756 #
29)	L6 AR-1254-4	7.354	6.447	905399	481094	11.509	5.088 #
30)	L6 AR-1254-5	7.782	6.845	476.2E6	724.4E6	6463.496	5428.688
31)	L7 AR-1260-1	7.215	6.335	726355	39021	12.319	0.400 #
32)	L7 AR-1260-2	7.470	6.527	645.3E6	4405184	6733.078	35.862 #
34)	L7 AR-1260-4	8.065	7.131	61029	282547	0.935	3.160 #
35)	L7 AR-1260-5	8.411	7.376	354653	686371	2.351	3.054 #
36)	L8 AR-1262-1	8.065	6.932f	61029	81760	0.701	0.554
37)	L8 AR-1262-2	8.411	7.131	354653	282547	1.791	2.210
38)	L8 AR-1262-3	8.718	7.697	88955	335883	0.708	2.946 #
39)	L8 AR-1262-4	8.768	7.708	102663	130013	1.101	0.706 #
40)	L8 AR-1262-5	9.446	8.244	194024	41416	3.061	0.490 #
41)	L9 AR-1268-1	8.718	7.697	88955	335883	0.399	1.093 #
42)	L9 AR-1268-2	8.768	7.708	102663	130013	0.539	0.489

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071525\
 Data File : PP073794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2025 10:38
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:42:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	8.984	7.992f	243250	438111	1.469	1.942 #
44)	L9 AR-1268-4	9.446	8.244	194024	41416	2.790	0.445 #
45)	L9 AR-1268-5	9.849	8.559	130893	29683	0.284	0.048 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071525\
Data File : PP073794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2025 10:38
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:42:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

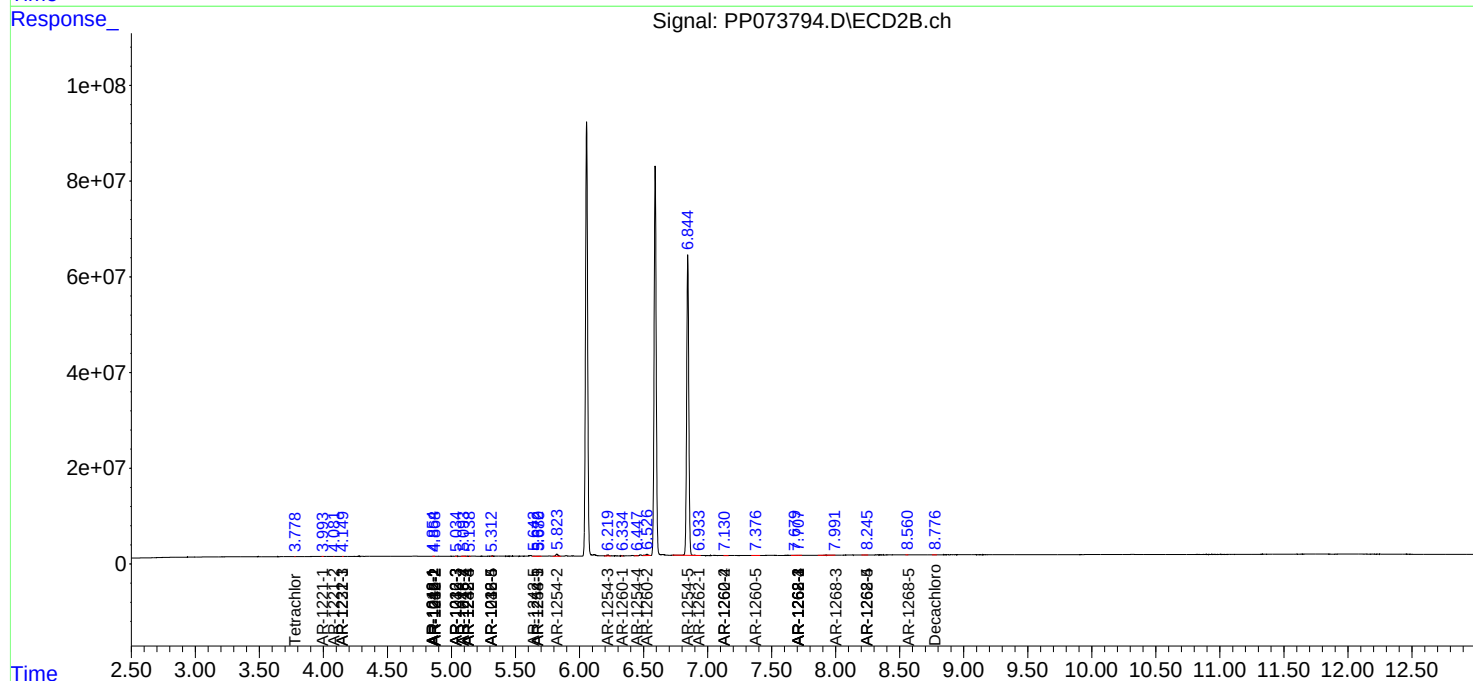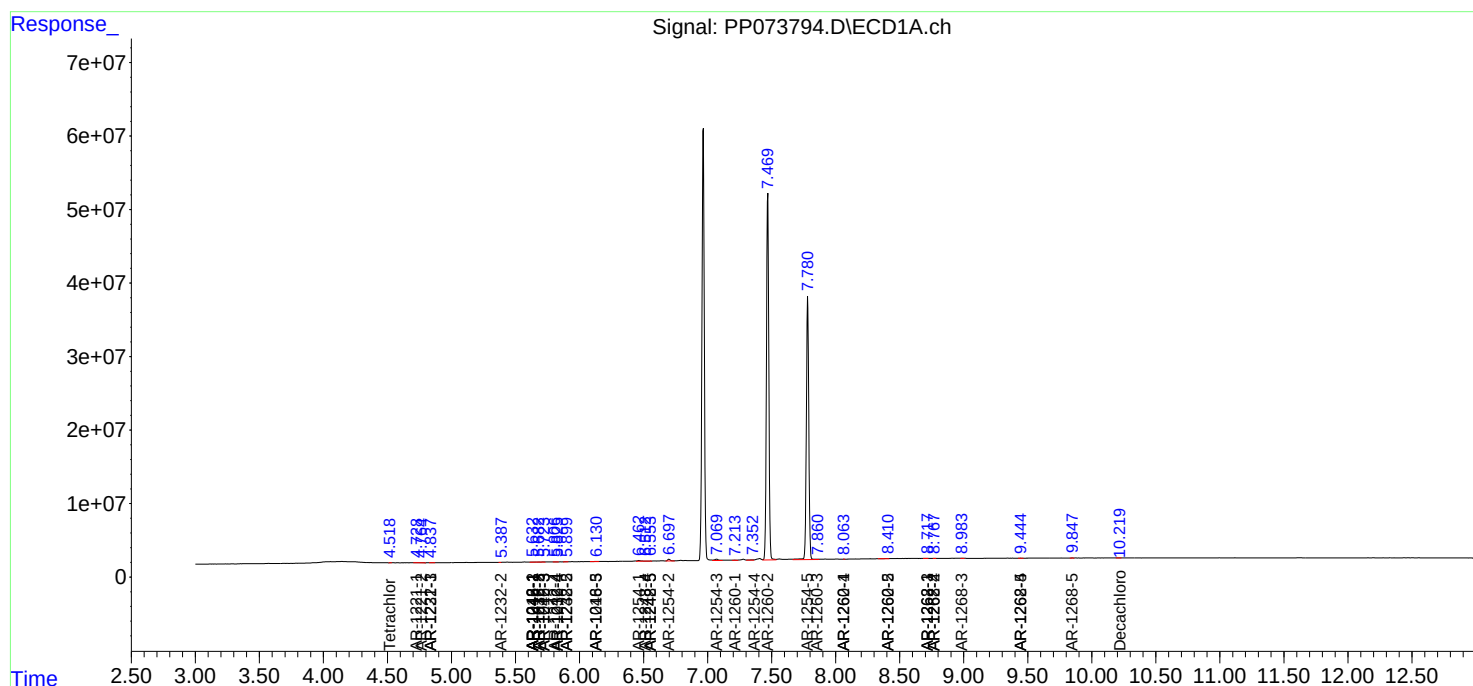


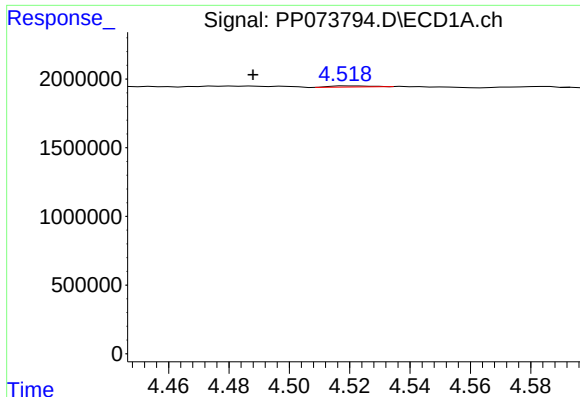

#1 Tetrachloro-m-xylene


R.T.: 4.520 min
Delta R.T.: 0.032 min
Response: 78582
Conc: 0.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

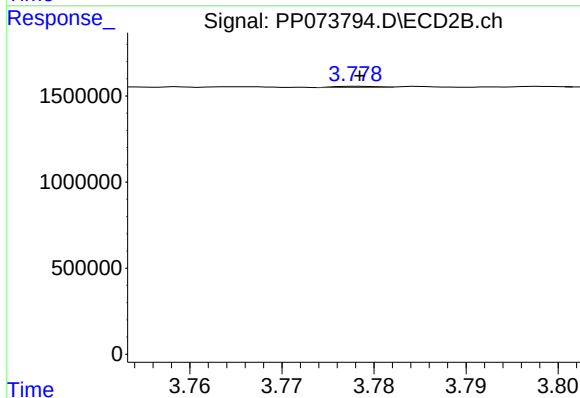


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: 0.000 min
Response: 21046
Conc: 0.01 ng/ml

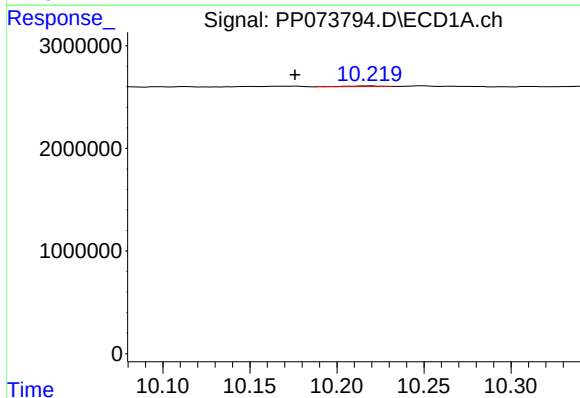


#2 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: 0.043 min
Response: 70670
Conc: 0.06 ng/ml

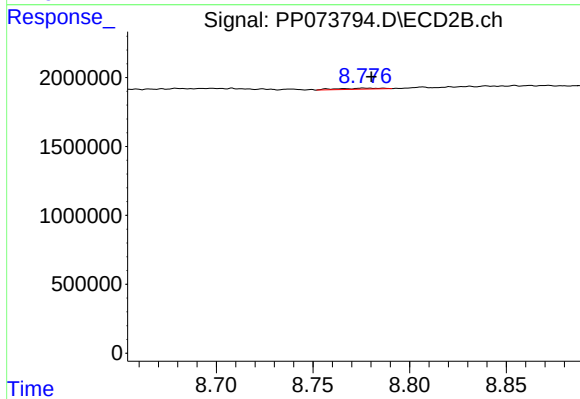

#2 Decachlorobiphenyl


R.T.: 8.776 min
Delta R.T.: -0.004 min
Response: 106724
Conc: 0.08 ng/ml

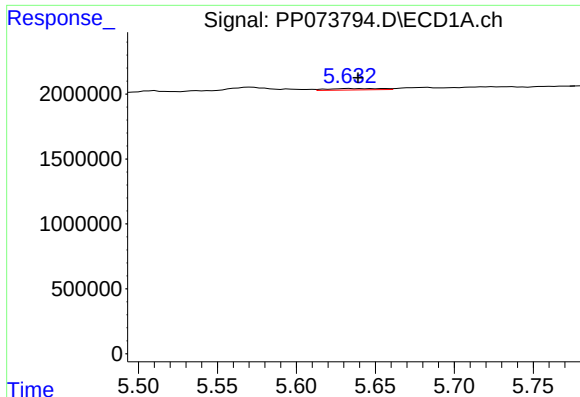

#3 AR-1016-1


R.T.: 5.633 min
Delta R.T.: -0.006 min
Response: 258495
Conc: 5.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

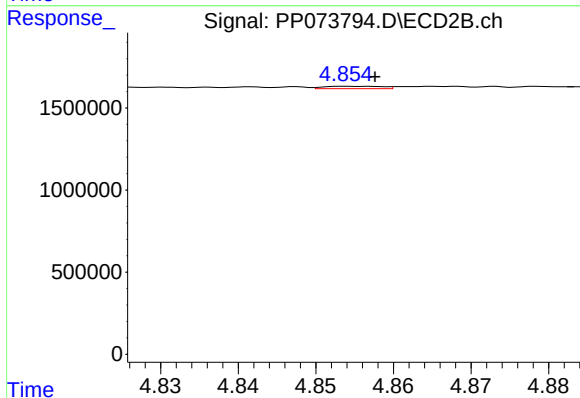


#3 AR-1016-1

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 78156
Conc: 1.15 ng/ml

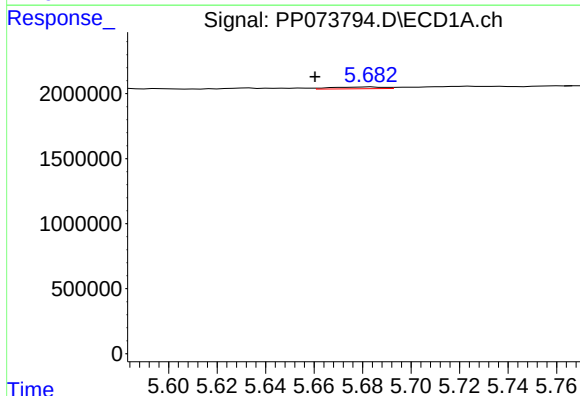


#4 AR-1016-2

R.T.: 5.683 min
Delta R.T.: 0.023 min
Response: 194905
Conc: 2.74 ng/ml

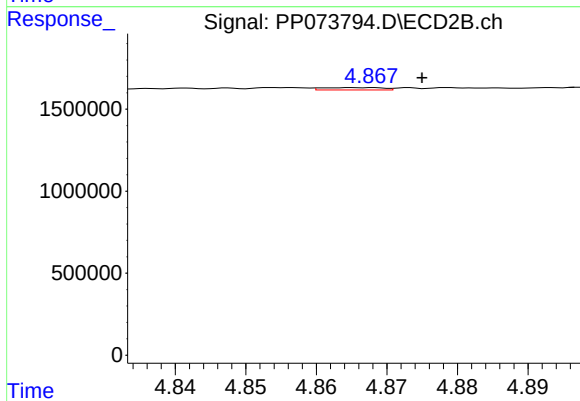

#4 AR-1016-2


R.T.: 4.868 min
Delta R.T.: -0.007 min
Response: 86010
Conc: 0.84 ng/ml

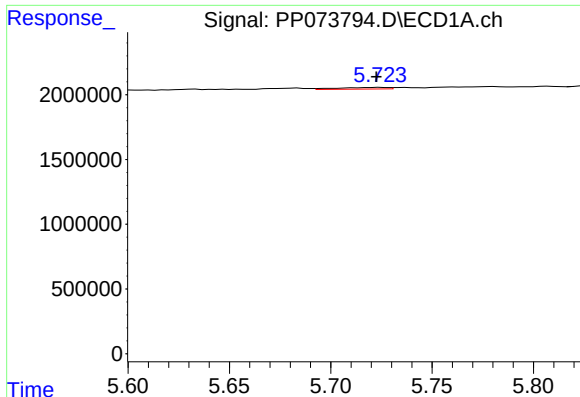

#5 AR-1016-3


R.T.: 5.725 min
Delta R.T.: 0.002 min
Response: 218229
Conc: 5.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

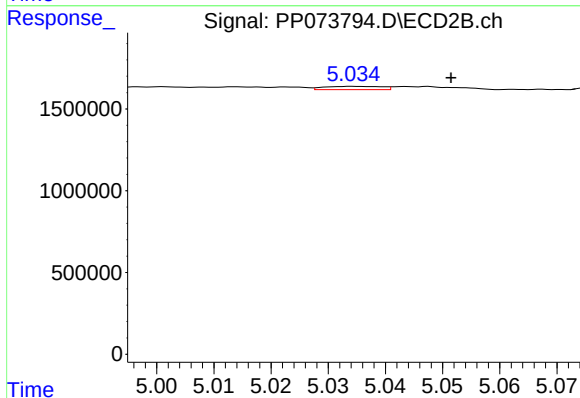


#5 AR-1016-3

R.T.: 5.034 min
Delta R.T.: -0.017 min
Response: 141244
Conc: 2.61 ng/ml

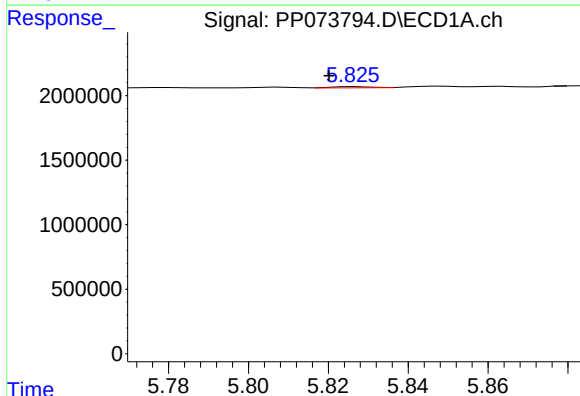


#6 AR-1016-4

R.T.: 5.827 min
Delta R.T.: 0.007 min
Response: 62005
Conc: 1.72 ng/ml

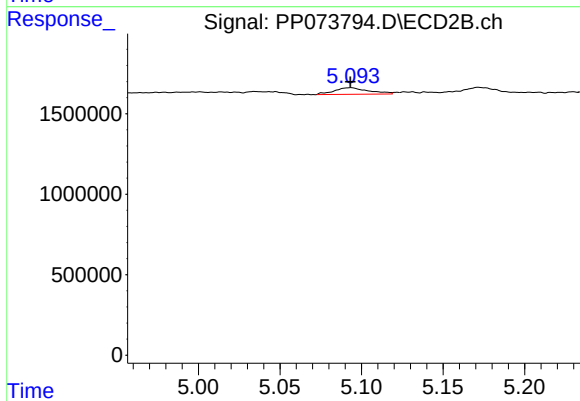

#6 AR-1016-4


R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 598550
Conc: 13.64 ng/ml

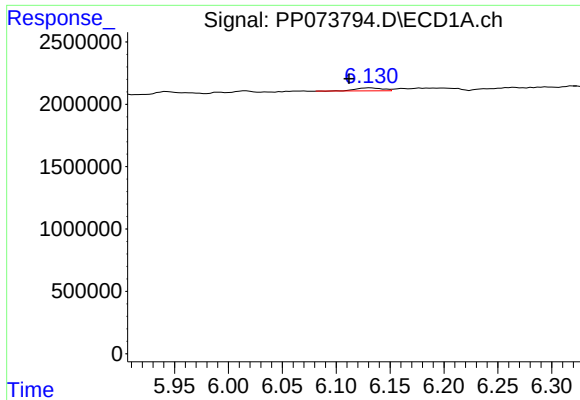

#7 AR-1016-5


R.T.: 6.131 min
Delta R.T.: 0.020 min
Response: 415341
Conc: 13.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

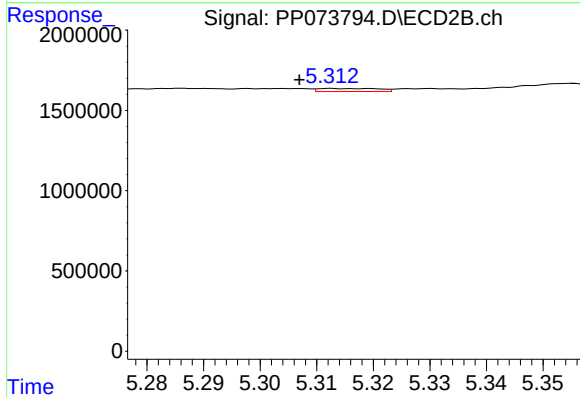


#7 AR-1016-5

R.T.: 5.313 min
Delta R.T.: 0.006 min
Response: 141979
Conc: 2.60 ng/ml

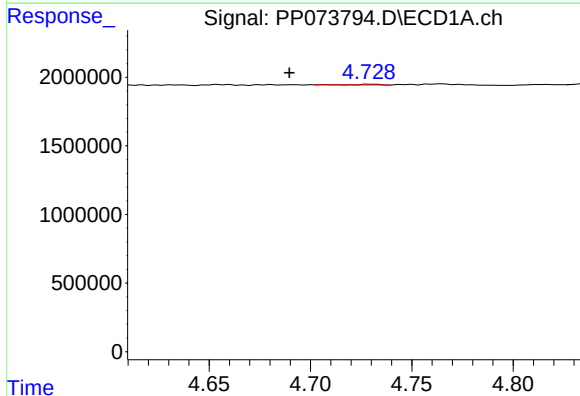


#8 AR-1221-1

R.T.: 4.729 min
Delta R.T.: 0.040 min
Response: 62303
Conc: 3.49 ng/ml

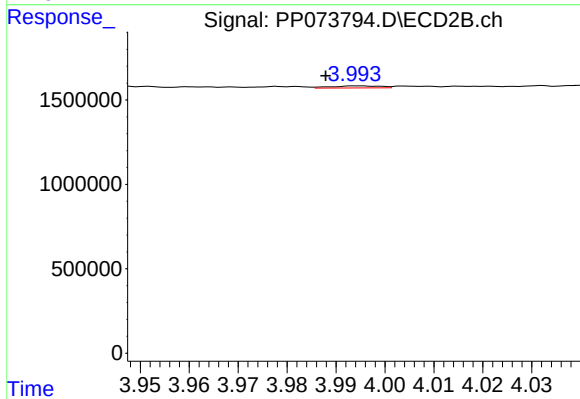

#8 AR-1221-1


R.T.: 3.994 min
Delta R.T.: 0.006 min
Response: 83230
Conc: 3.08 ng/ml

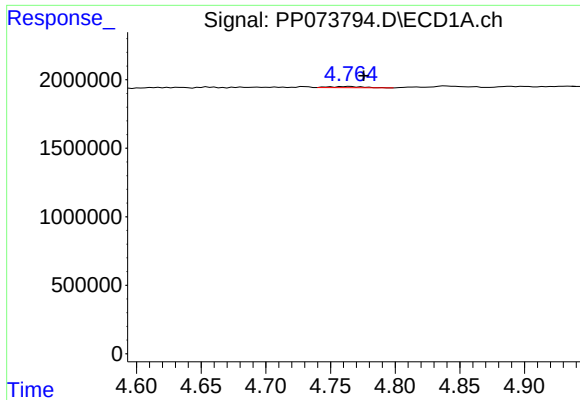

#9 AR-1221-2


R.T.: 4.765 min
Delta R.T.: -0.011 min
Response: 148325
Conc: 10.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

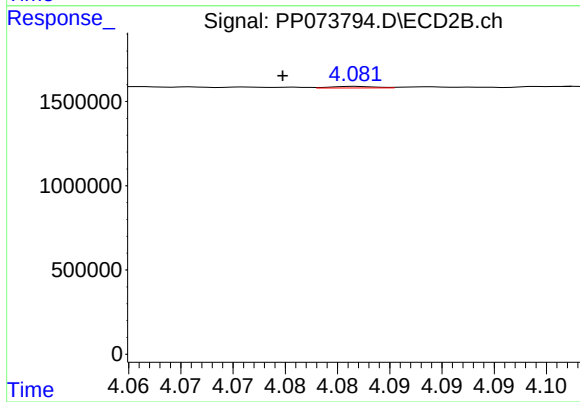


#9 AR-1221-2

R.T.: 4.082 min
Delta R.T.: 0.007 min
Response: 27313
Conc: 1.34 ng/ml

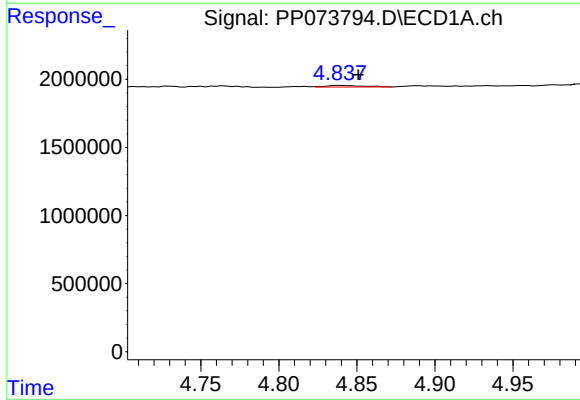


#10 AR-1221-3

R.T.: 4.839 min
Delta R.T.: -0.012 min
Response: 192917
Conc: 4.64 ng/ml

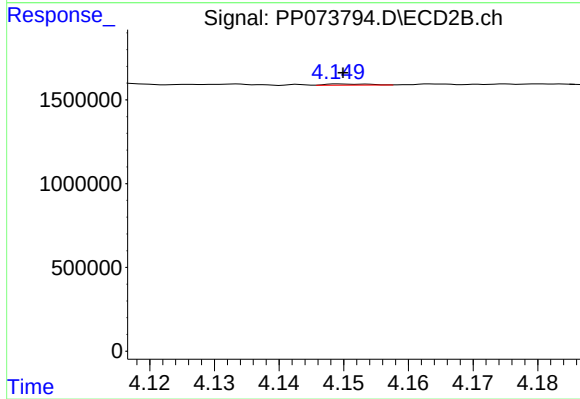

#10 AR-1221-3


R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 33886
Conc: 0.55 ng/ml

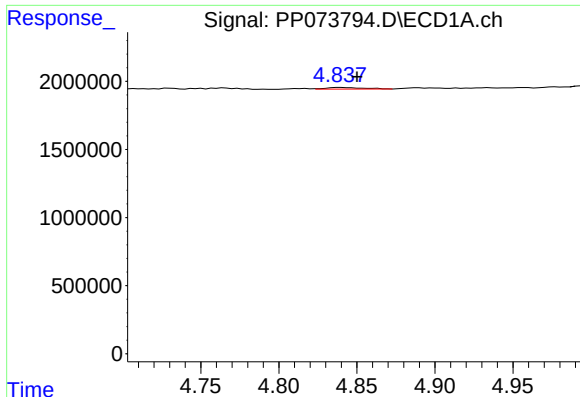

#11 AR-1232-1


R.T.: 4.839 min
Delta R.T.: -0.011 min
Response: 192917
Conc: 5.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

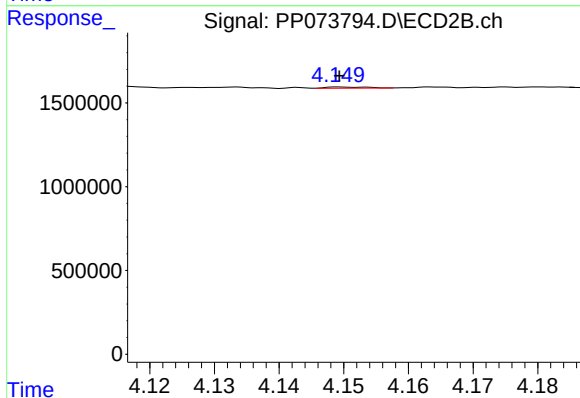


#11 AR-1232-1

R.T.: 4.149 min
Delta R.T.: 0.000 min
Response: 33886
Conc: 0.73 ng/ml

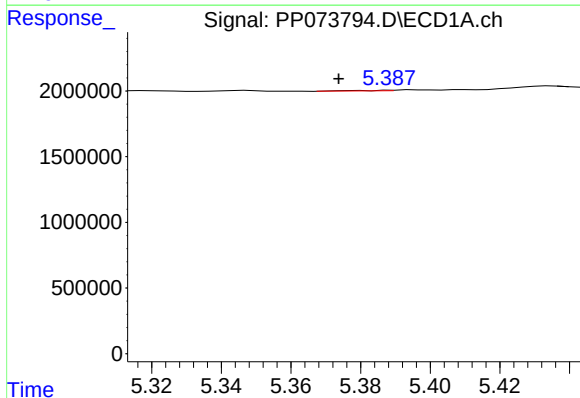


#12 AR-1232-2

R.T.: 5.380 min
Delta R.T.: 0.006 min
Response: 34736
Conc: 2.14 ng/ml

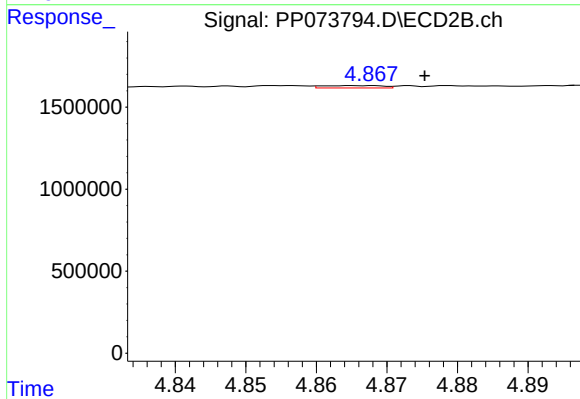

#12 AR-1232-2


R.T.: 4.868 min
Delta R.T.: -0.007 min
Response: 86010
Conc: 1.80 ng/ml

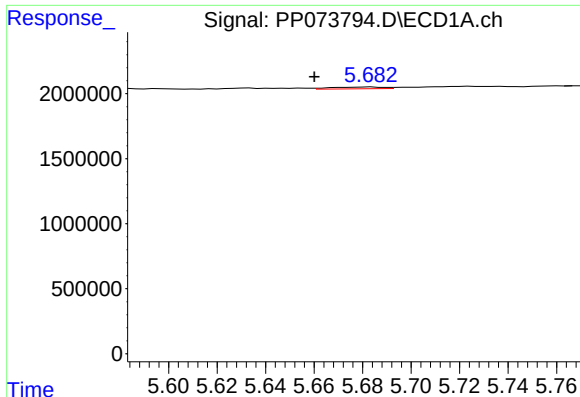

#13 AR-1232-3


R.T.: 5.683 min
Delta R.T.: 0.023 min
Response: 194905
Conc: 5.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

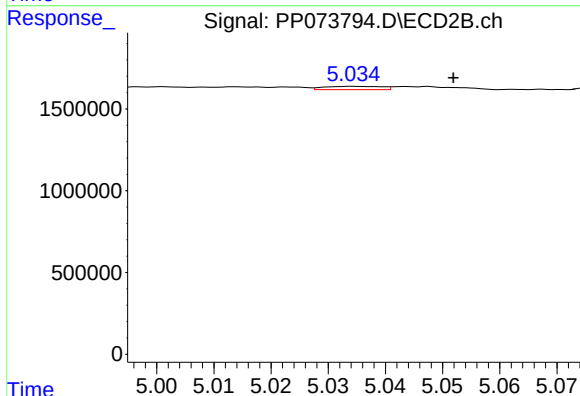


#13 AR-1232-3

R.T.: 5.034 min
Delta R.T.: -0.018 min
Response: 141244
Conc: 5.64 ng/ml

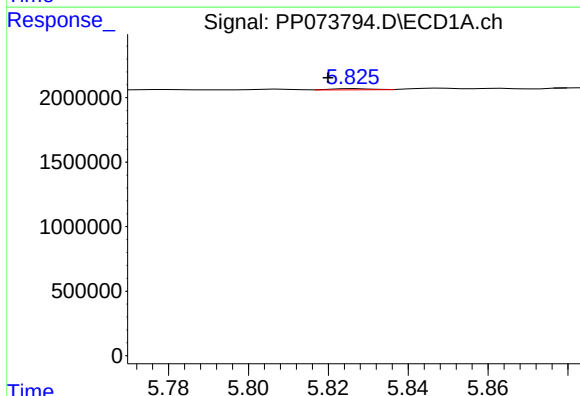


#14 AR-1232-4

R.T.: 5.827 min
Delta R.T.: 0.007 min
Response: 62005
Conc: 3.77 ng/ml

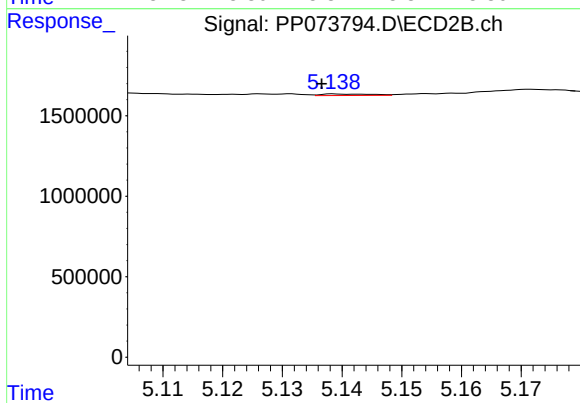

#14 AR-1232-4


R.T.: 5.139 min
Delta R.T.: 0.002 min
Response: 55503
Conc: 2.56 ng/ml

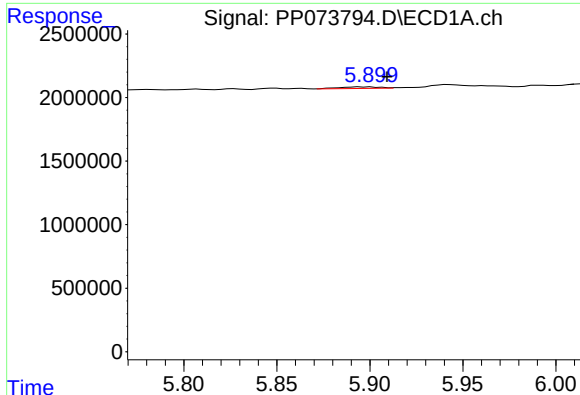

#15 AR-1232-5


R.T.: 5.895 min
Delta R.T.: -0.015 min
Response: 180494
Conc: 17.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

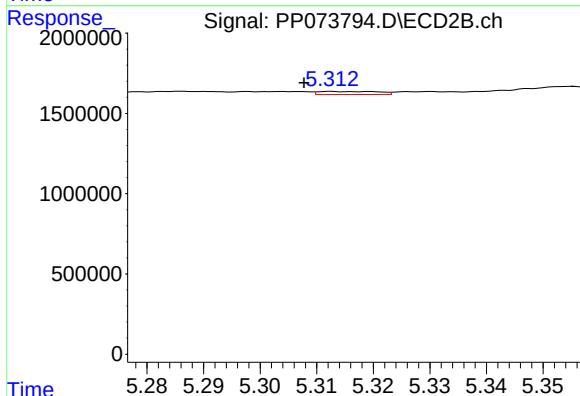


#15 AR-1232-5

R.T.: 5.313 min
Delta R.T.: 0.005 min
Response: 141979
Conc: 6.29 ng/ml

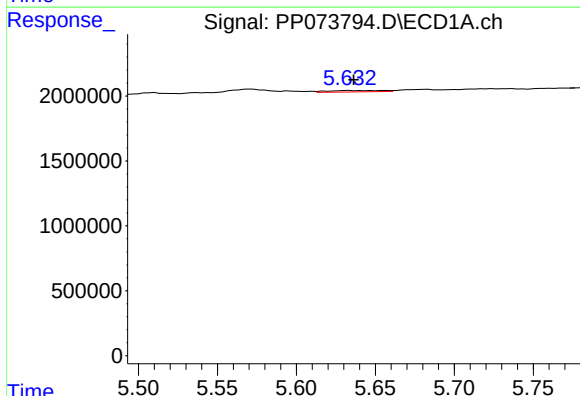


#16 AR-1242-1

R.T.: 5.633 min
Delta R.T.: -0.003 min
Response: 258495
Conc: 6.77 ng/ml

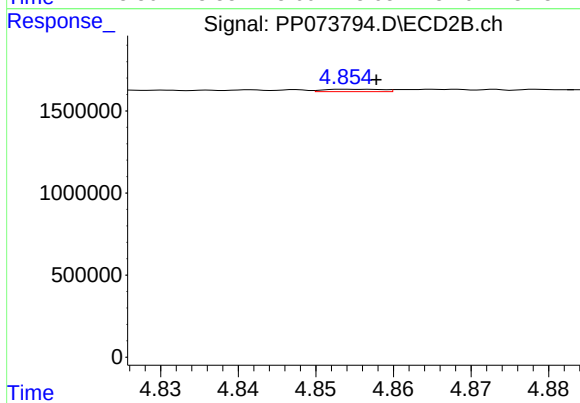

#16 AR-1242-1


R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 78156
Conc: 1.35 ng/ml

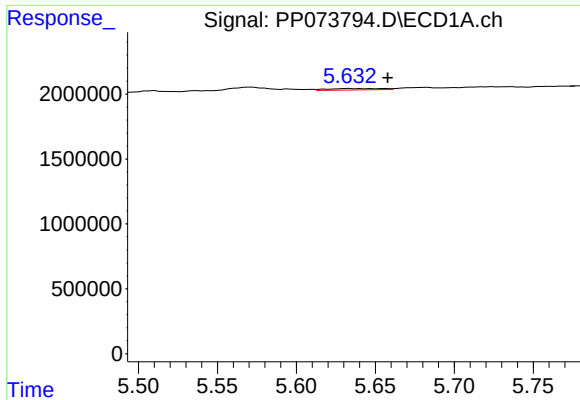

#17 AR-1242-2


R.T.: 5.633 min
Delta R.T.: -0.025 min
Response: 258495
Conc: 4.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

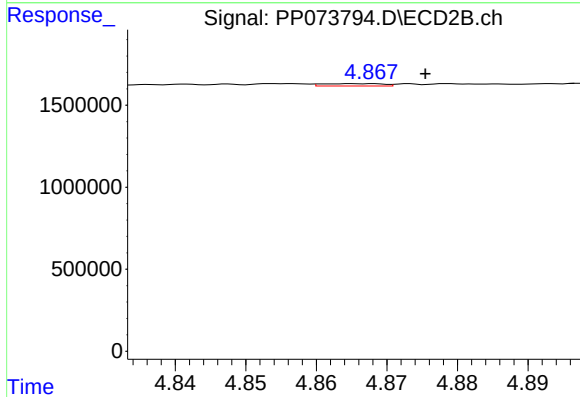


#17 AR-1242-2

R.T.: 4.868 min
Delta R.T.: -0.007 min
Response: 86010
Conc: 0.99 ng/ml

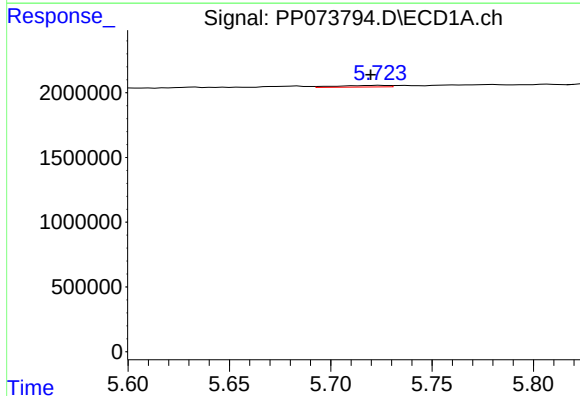


#18 AR-1242-3

R.T.: 5.725 min
Delta R.T.: 0.005 min
Response: 218229
Conc: 5.96 ng/ml

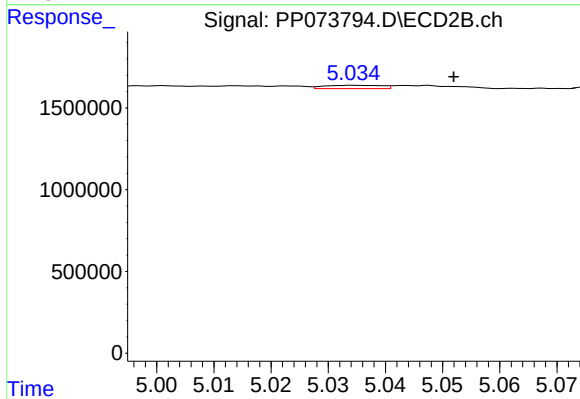

#18 AR-1242-3


R.T.: 5.034 min
Delta R.T.: -0.018 min
Response: 141244
Conc: 3.07 ng/ml

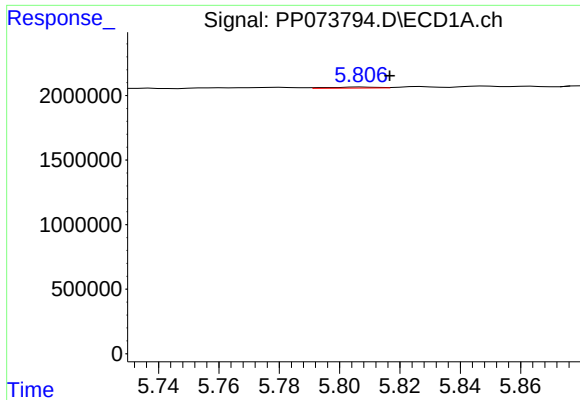

#19 AR-1242-4


R.T.: 5.808 min
Delta R.T.: -0.009 min
Response: 87211
Conc: 2.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

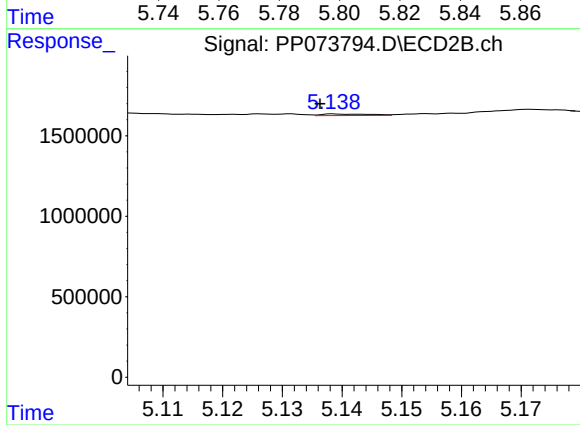


#19 AR-1242-4

R.T.: 5.139 min
Delta R.T.: 0.002 min
Response: 55503
Conc: 1.25 ng/ml

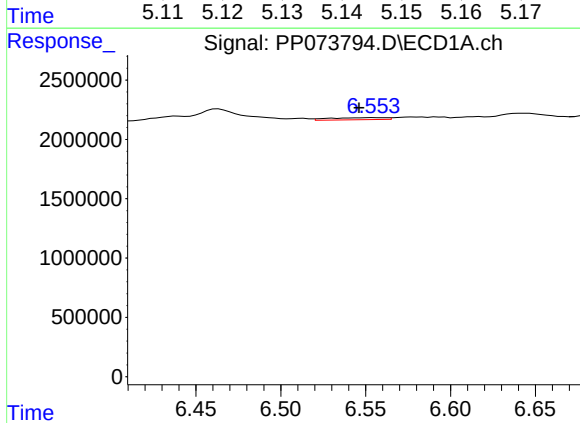


#20 AR-1242-5

R.T.: 6.555 min
Delta R.T.: 0.009 min
Response: 391228
Conc: 11.95 ng/ml

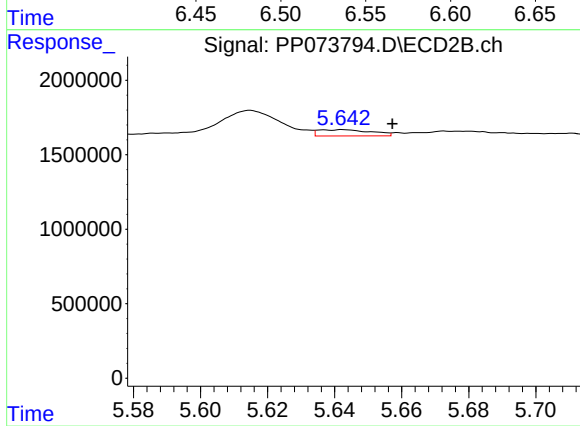

#20 AR-1242-5


R.T.: 5.643 min
Delta R.T.: -0.015 min
Response: 461889
Conc: 8.36 ng/ml

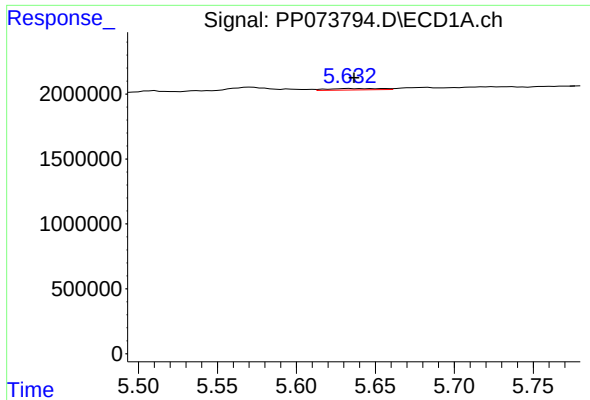

#21 AR-1248-1


R.T.: 5.633 min
Delta R.T.: -0.004 min
Response: 258495
Conc: 8.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

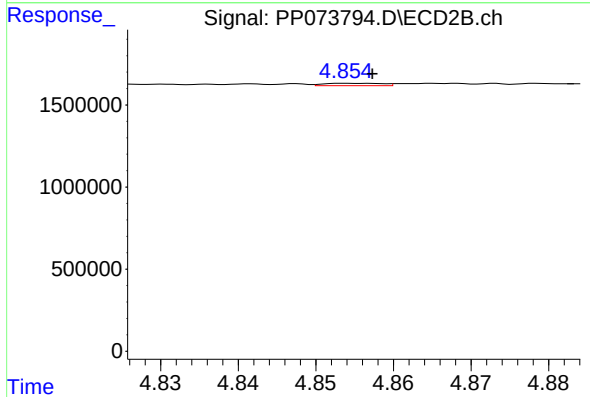


#21 AR-1248-1

R.T.: 4.854 min
Delta R.T.: -0.003 min
Response: 78156
Conc: 1.74 ng/ml

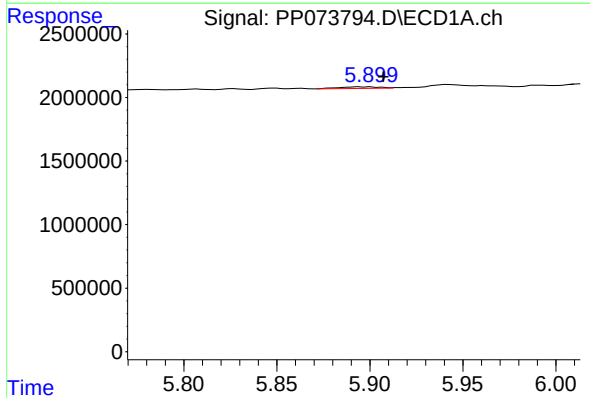


#22 AR-1248-2

R.T.: 5.895 min
Delta R.T.: -0.013 min
Response: 180494
Conc: 4.52 ng/ml

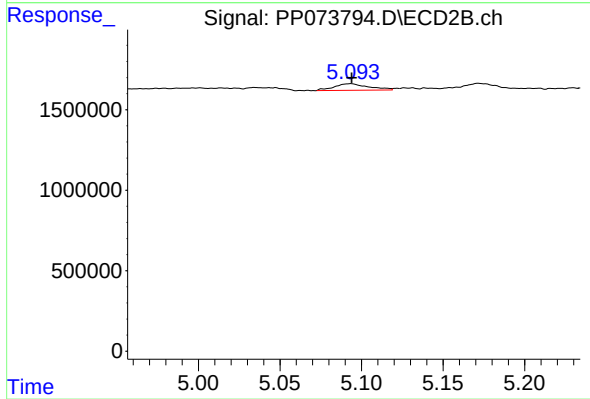

#22 AR-1248-2


R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 598550
Conc: 9.73 ng/ml

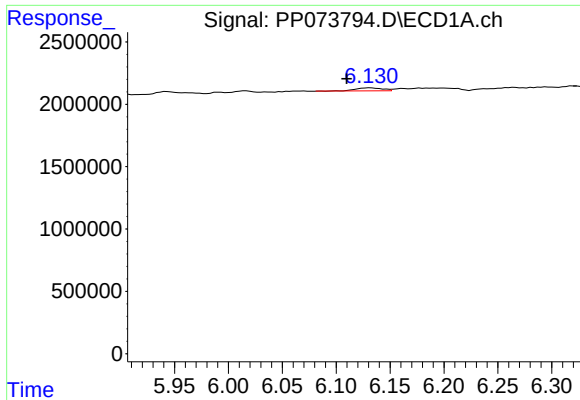

#23 AR-1248-3


R.T.: 6.131 min
Delta R.T.: 0.022 min
Response: 415341
Conc: 9.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

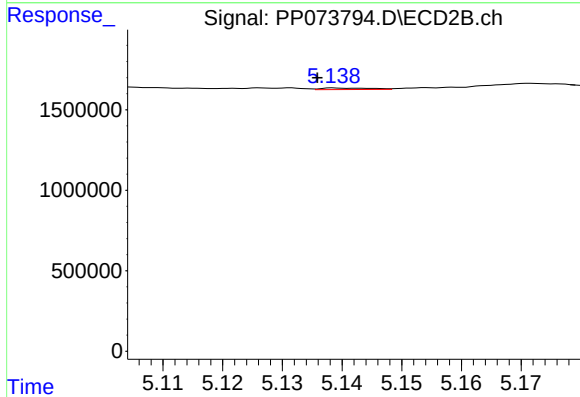


#23 AR-1248-3

R.T.: 5.139 min
Delta R.T.: 0.003 min
Response: 55503
Conc: 0.87 ng/ml

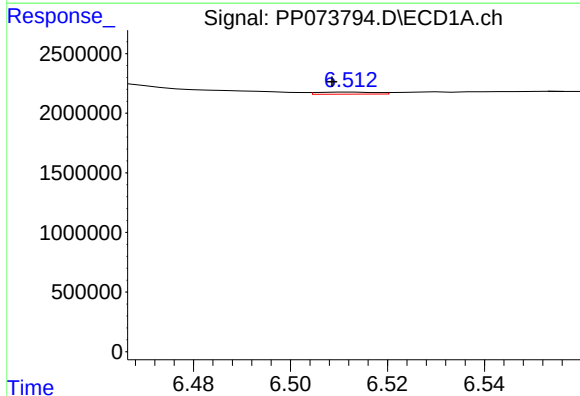


#24 AR-1248-4

R.T.: 6.513 min
Delta R.T.: 0.004 min
Response: 143892
Conc: 2.61 ng/ml

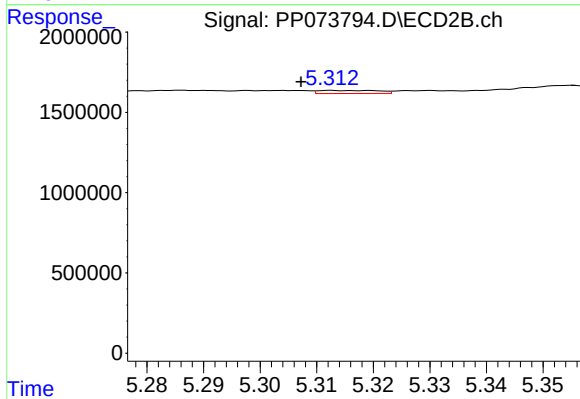

#24 AR-1248-4


R.T.: 5.313 min
Delta R.T.: 0.005 min
Response: 141979
Conc: 1.88 ng/ml

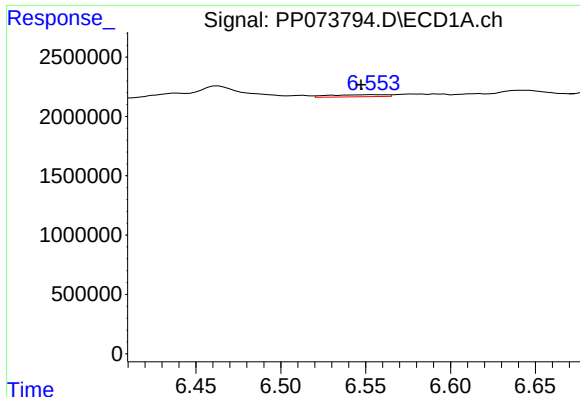

#25 AR-1248-5


R.T.: 6.555 min
Delta R.T.: 0.008 min
Response: 391228
Conc: 7.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

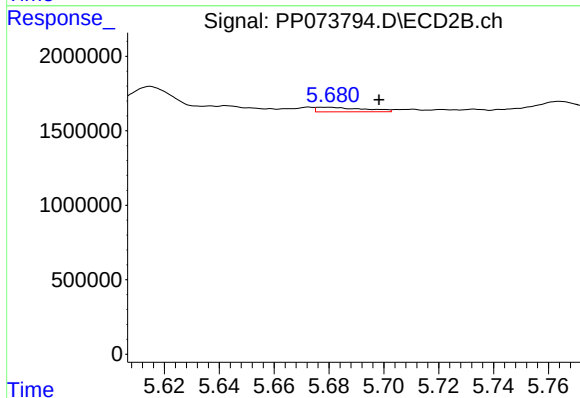


#25 AR-1248-5

R.T.: 5.680 min
Delta R.T.: -0.018 min
Response: 367729
Conc: 4.93 ng/ml

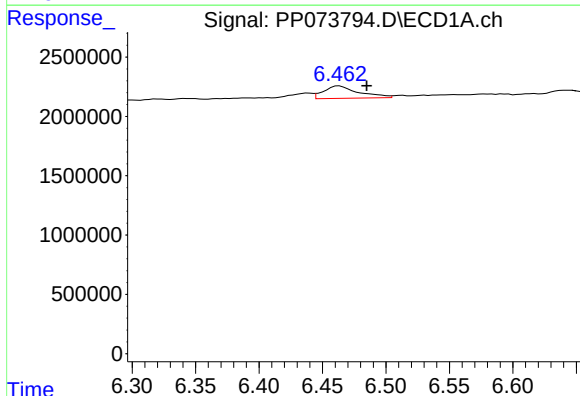


#26 AR-1254-1

R.T.: 6.463 min
Delta R.T.: -0.022 min
Response: 1997980
Conc: 37.28 ng/ml

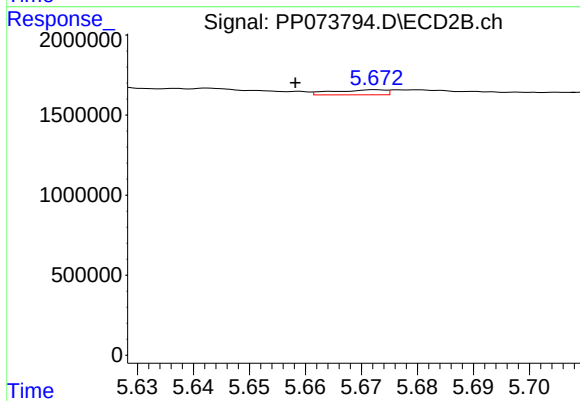

#26 AR-1254-1


R.T.: 5.673 min
Delta R.T.: 0.014 min
Response: 205582
Conc: 1.77 ng/ml

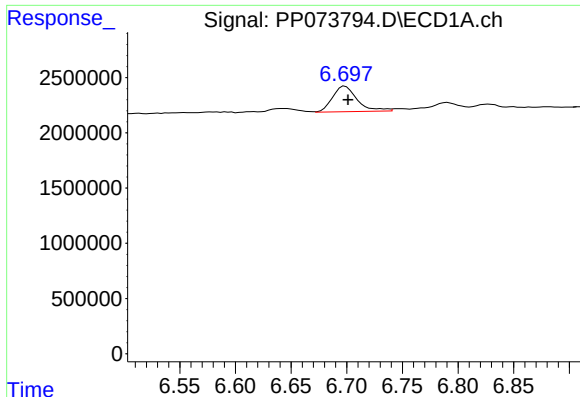

#27 AR-1254-2


R.T.: 6.699 min
Delta R.T.: -0.003 min
Response: 3564862
Conc: 42.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

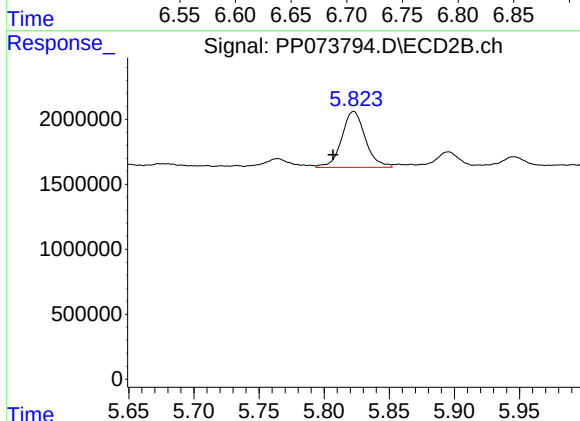


#27 AR-1254-2

R.T.: 5.823 min
Delta R.T.: 0.016 min
Response: 5427573
Conc: 53.94 ng/ml

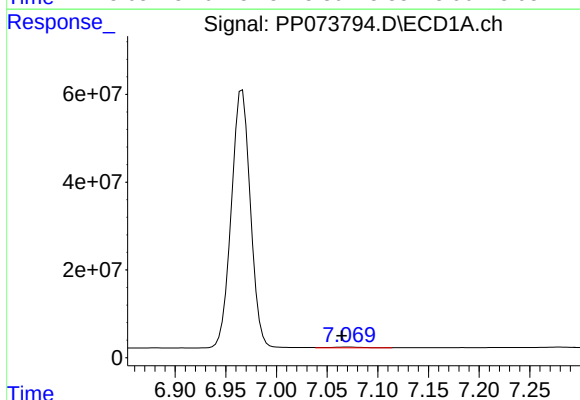


#28 AR-1254-3

R.T.: 7.070 min
Delta R.T.: 0.006 min
Response: 4031476
Conc: 45.64 ng/ml

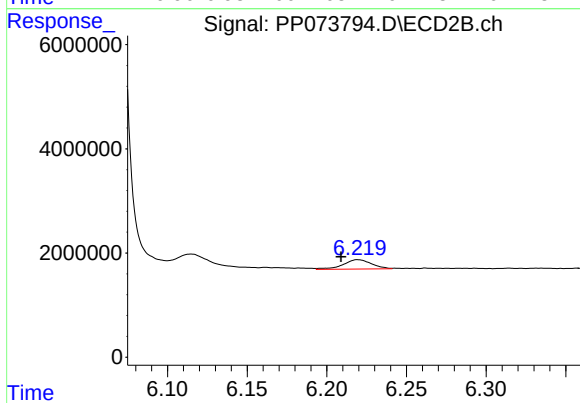

#28 AR-1254-3


R.T.: 6.219 min
Delta R.T.: 0.011 min
Response: 2279060
Conc: 14.76 ng/ml

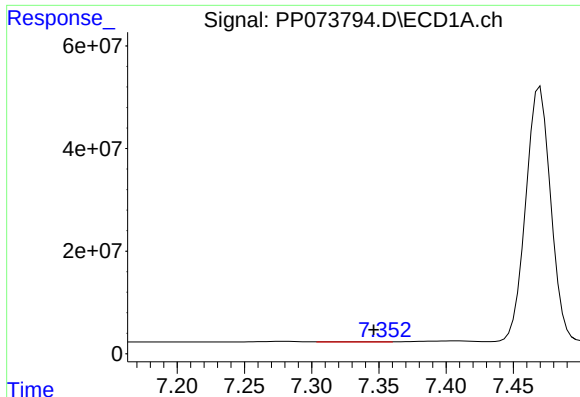

#29 AR-1254-4


R.T.: 7.354 min
Delta R.T.: 0.008 min
Response: 905399
Conc: 11.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

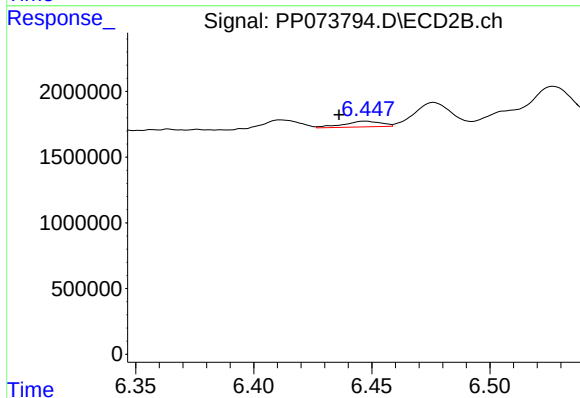


#29 AR-1254-4

R.T.: 6.447 min
Delta R.T.: 0.011 min
Response: 481094
Conc: 5.09 ng/ml

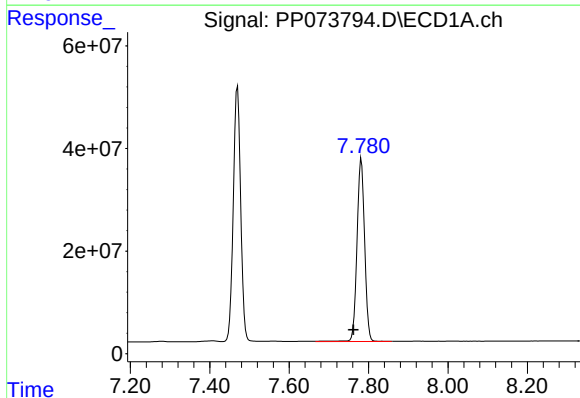


#30 AR-1254-5

R.T.: 7.782 min
Delta R.T.: 0.020 min
Response: 476229164
Conc: 6463.50 ng/ml

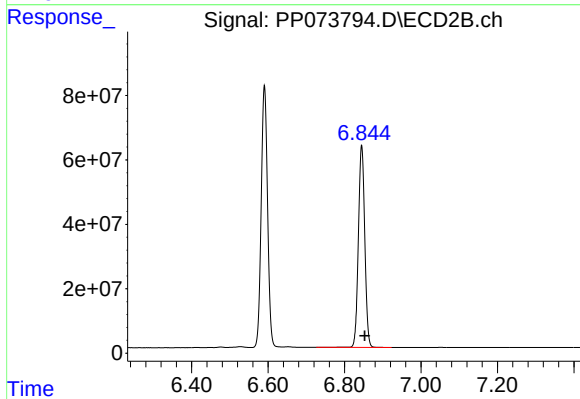

#30 AR-1254-5


R.T.: 6.845 min
Delta R.T.: -0.008 min
Response: 724430552
Conc: 5428.69 ng/ml

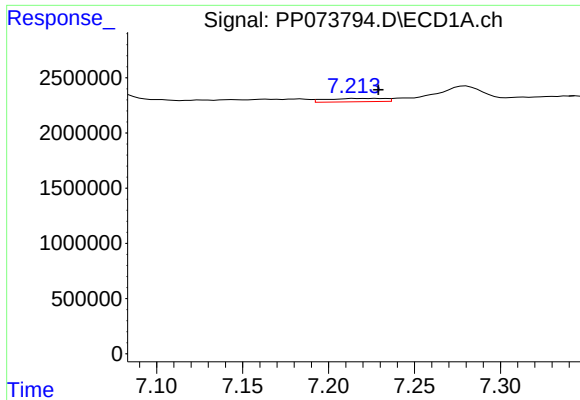

#31 AR-1260-1


R.T.: 7.215 min
Delta R.T.: -0.014 min
Response: 726355
Conc: 12.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

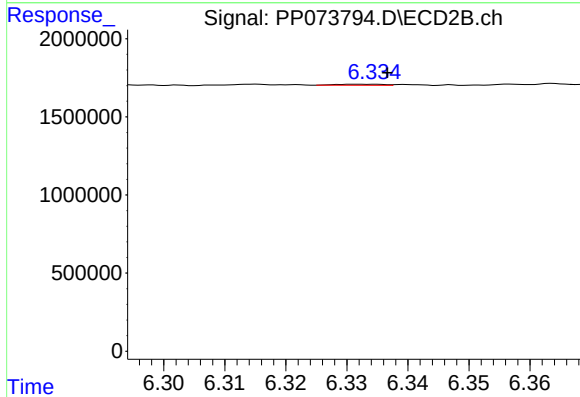


#31 AR-1260-1

R.T.: 6.335 min
Delta R.T.: -0.002 min
Response: 39021
Conc: 0.40 ng/ml

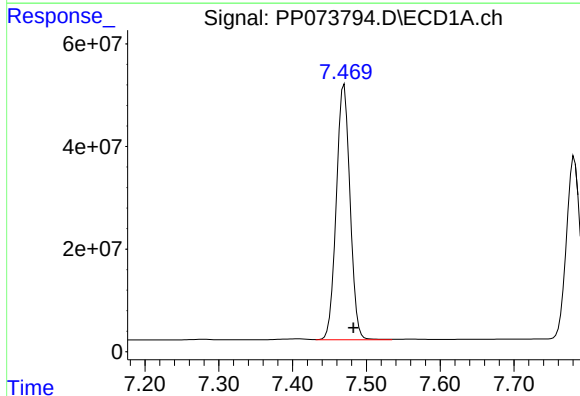


#32 AR-1260-2

R.T.: 7.470 min
Delta R.T.: -0.013 min
Response: 645297280
Conc: 6733.08 ng/ml

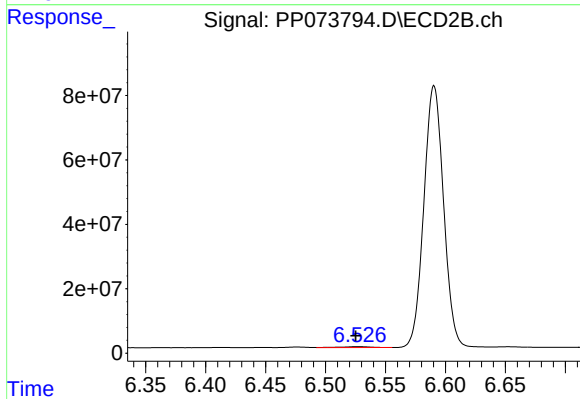

#32 AR-1260-2


R.T.: 6.527 min
Delta R.T.: 0.002 min
Response: 4405184
Conc: 35.86 ng/ml

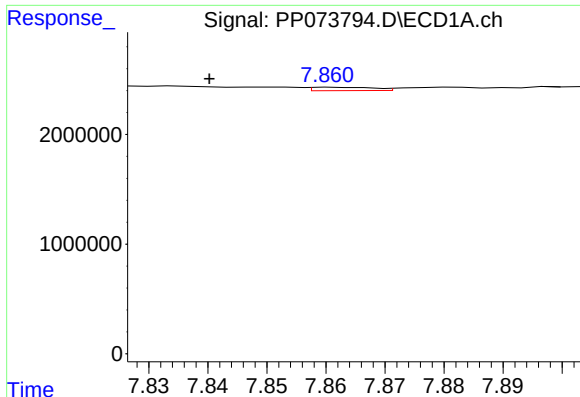

#33 AR-1260-3


R.T.: 7.861 min
Delta R.T.: 0.021 min
Response: 229722
Conc: 3.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

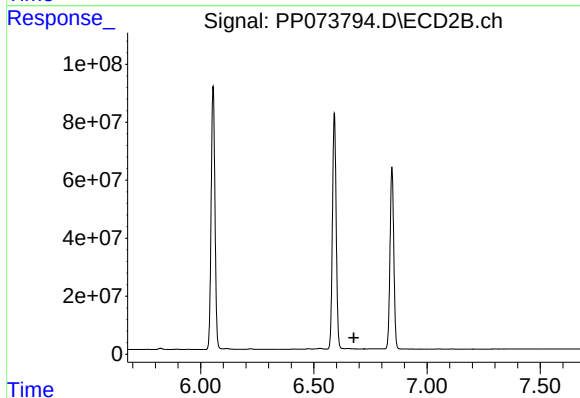


#33 AR-1260-3

R.T.: 6.652 min
Delta R.T.: -0.025 min
Response: -604182
Conc: N.D.

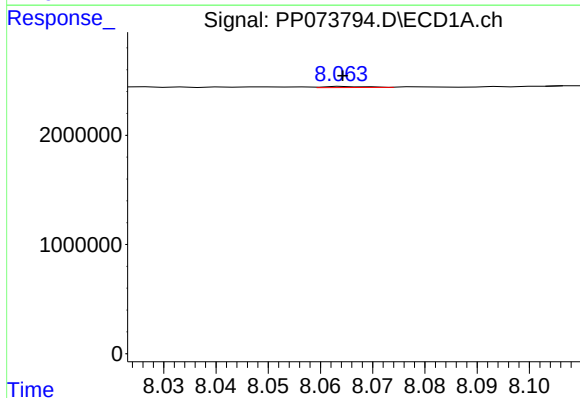


#34 AR-1260-4

R.T.: 8.065 min
Delta R.T.: 0.001 min
Response: 61029
Conc: 0.93 ng/ml

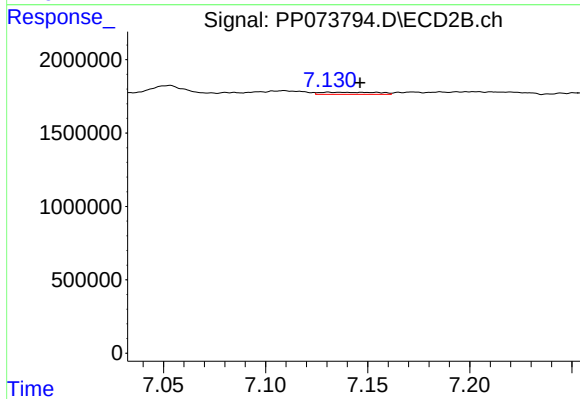

#34 AR-1260-4


R.T.: 7.131 min
Delta R.T.: -0.016 min
Response: 282547
Conc: 3.16 ng/ml

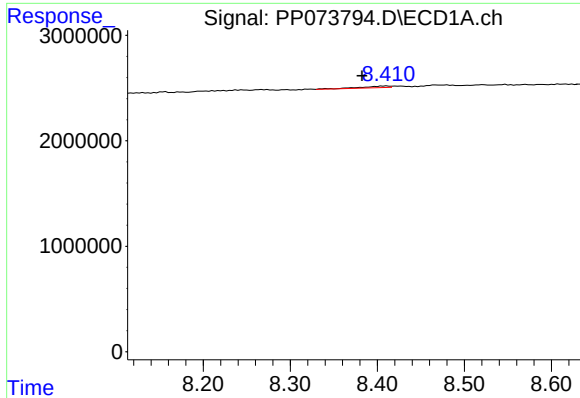

#35 AR-1260-5


R.T.: 8.411 min
Delta R.T.: 0.028 min
Response: 354653
Conc: 2.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

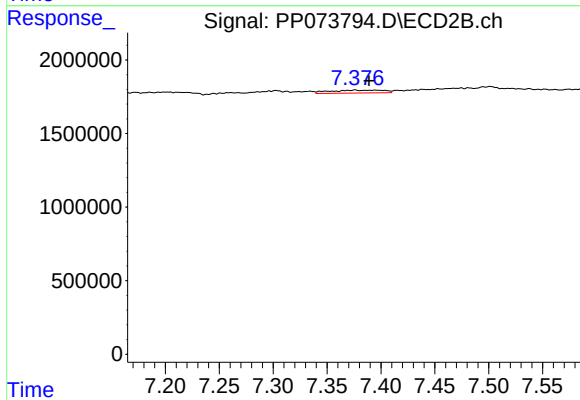


#35 AR-1260-5

R.T.: 7.376 min
Delta R.T.: -0.013 min
Response: 686371
Conc: 3.05 ng/ml

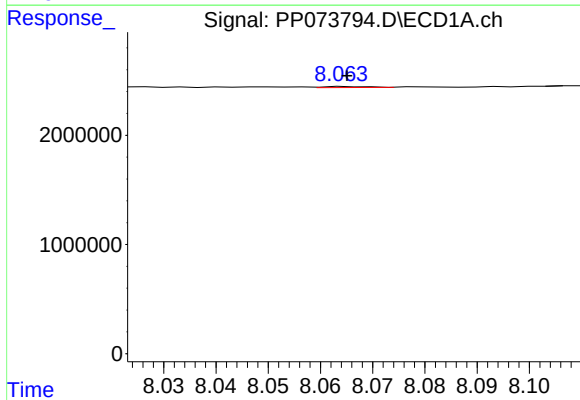


#36 AR-1262-1

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 61029
Conc: 0.70 ng/ml

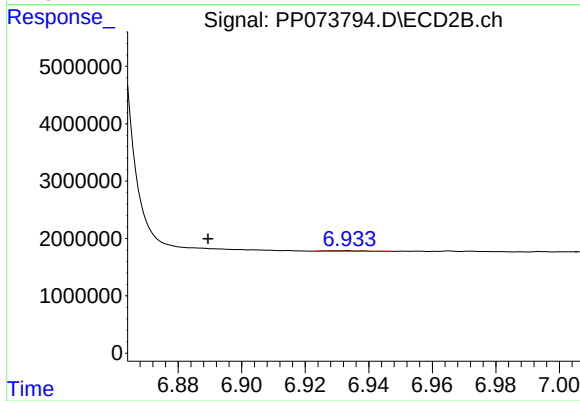

#36 AR-1262-1


R.T.: 6.932 min
Delta R.T.: 0.043 min
Response: 81760
Conc: 0.55 ng/ml

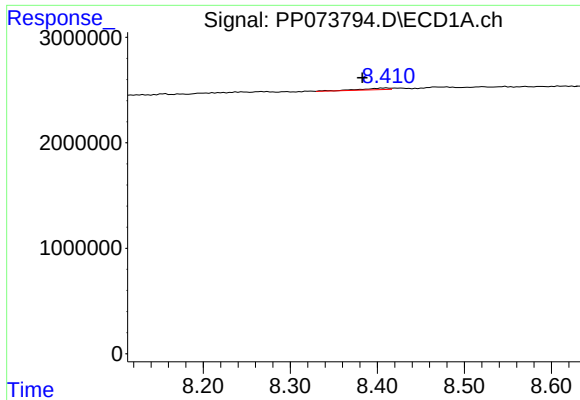

#37 AR-1262-2


R.T.: 8.411 min
Delta R.T.: 0.028 min
Response: 354653
Conc: 1.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

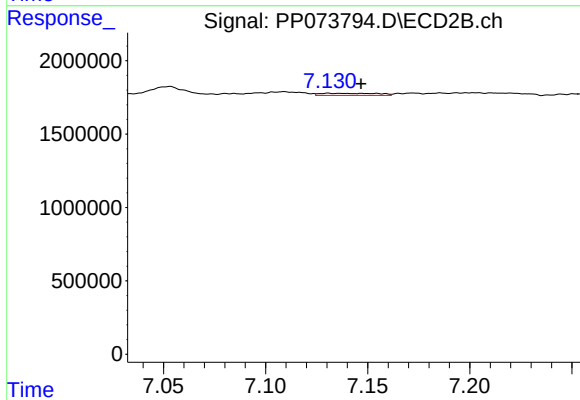


#37 AR-1262-2

R.T.: 7.131 min
Delta R.T.: -0.016 min
Response: 282547
Conc: 2.21 ng/ml

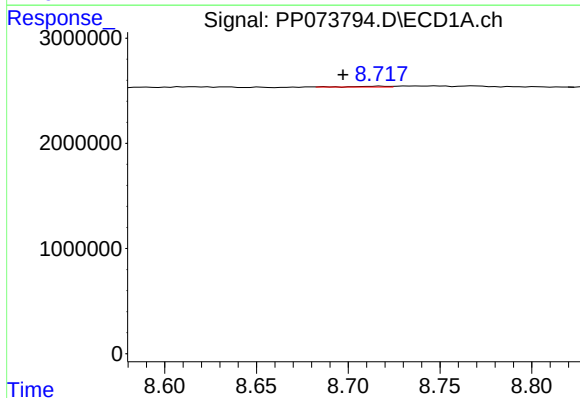


#38 AR-1262-3

R.T.: 8.718 min
Delta R.T.: 0.021 min
Response: 88955
Conc: 0.71 ng/ml

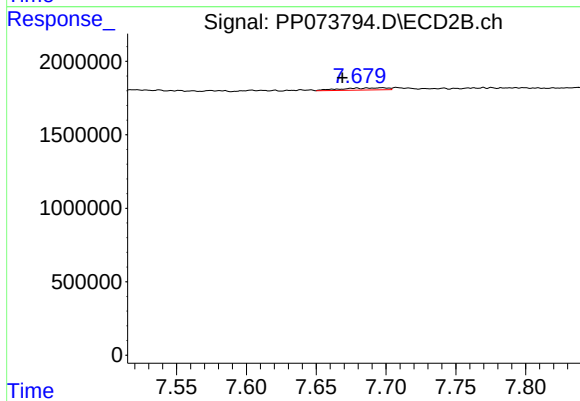

#38 AR-1262-3


R.T.: 7.697 min
Delta R.T.: 0.028 min
Response: 335883
Conc: 2.95 ng/ml

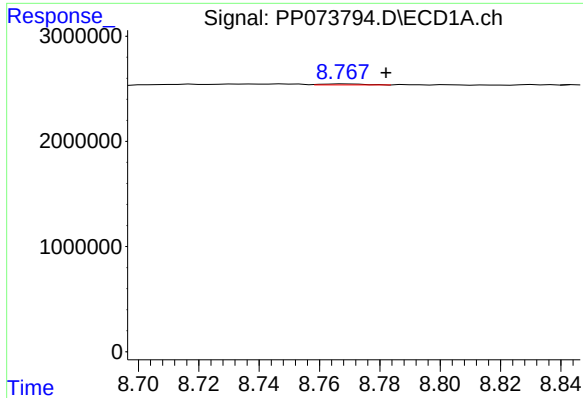

#39 AR-1262-4


R.T.: 8.768 min
Delta R.T.: -0.014 min
Response: 102663
Conc: 1.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

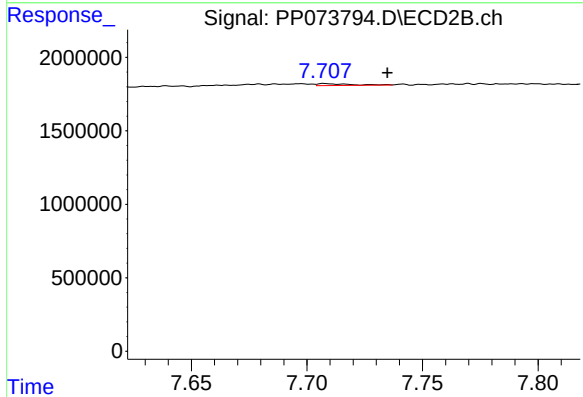


#39 AR-1262-4

R.T.: 7.708 min
Delta R.T.: -0.027 min
Response: 130013
Conc: 0.71 ng/ml

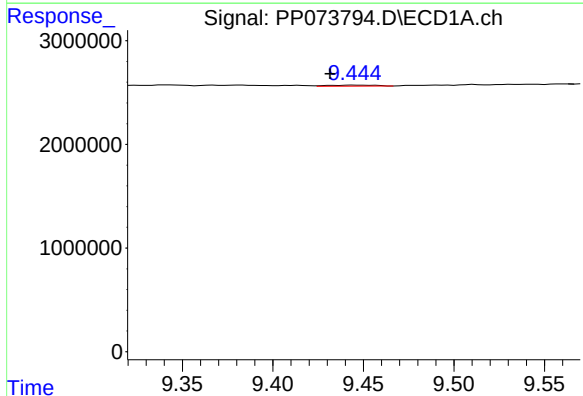


#40 AR-1262-5

R.T.: 9.446 min
Delta R.T.: 0.014 min
Response: 194024
Conc: 3.06 ng/ml

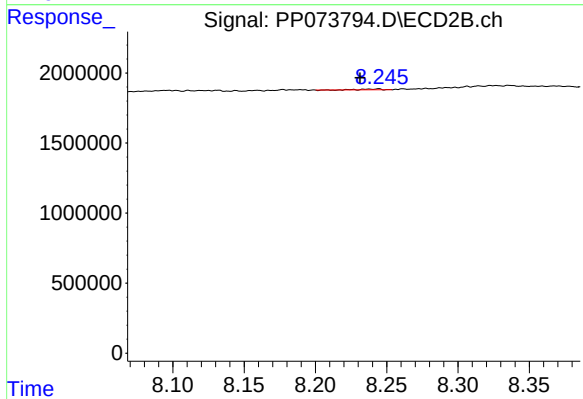

#40 AR-1262-5


R.T.: 8.244 min
Delta R.T.: 0.013 min
Response: 41416
Conc: 0.49 ng/ml

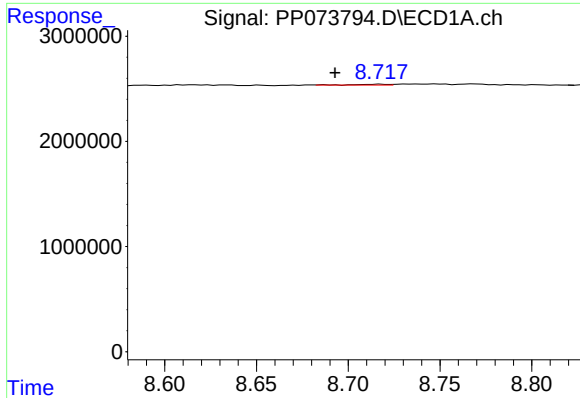

#41 AR-1268-1


R.T.: 8.718 min
Delta R.T.: 0.025 min
Response: 88955
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

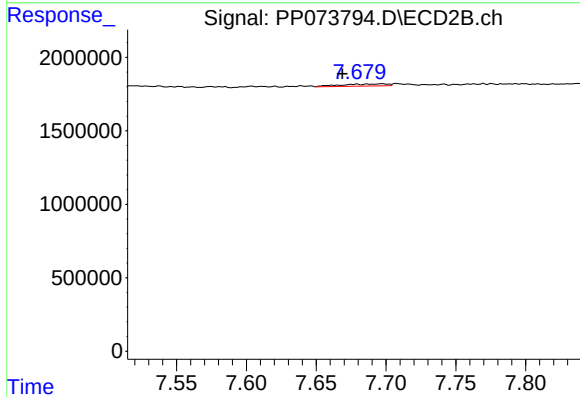


#41 AR-1268-1

R.T.: 7.697 min
Delta R.T.: 0.028 min
Response: 335883
Conc: 1.09 ng/ml

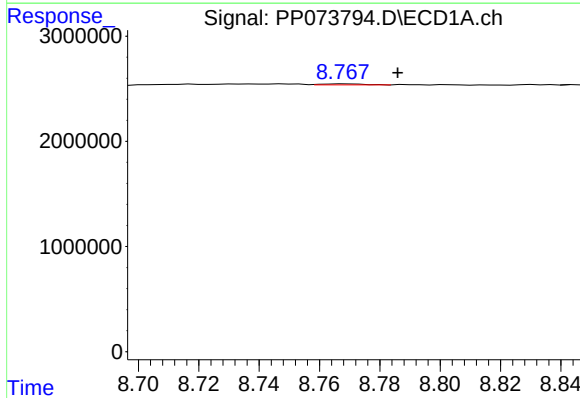


#42 AR-1268-2

R.T.: 8.768 min
Delta R.T.: -0.018 min
Response: 102663
Conc: 0.54 ng/ml

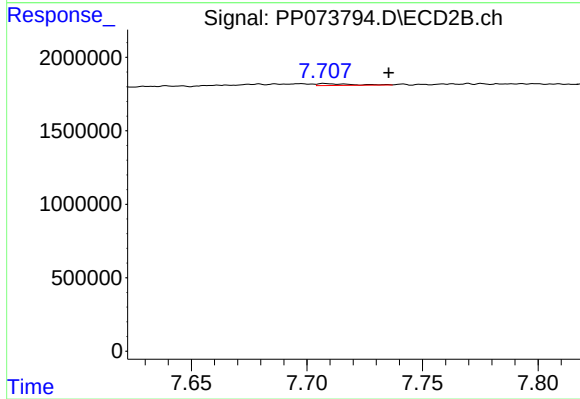

#42 AR-1268-2


R.T.: 7.708 min
Delta R.T.: -0.028 min
Response: 130013
Conc: 0.49 ng/ml

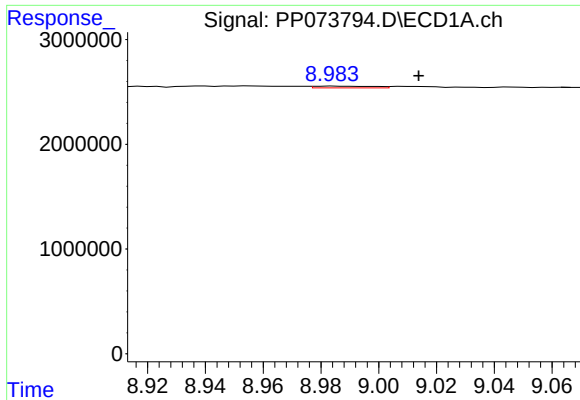

#43 AR-1268-3


R.T.: 8.984 min
Delta R.T.: -0.030 min
Response: 243250
Conc: 1.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

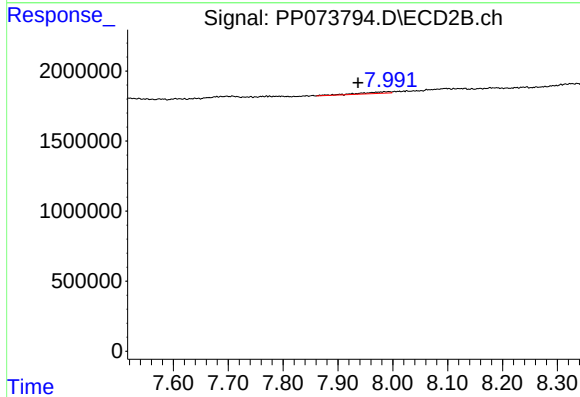


#43 AR-1268-3

R.T.: 7.992 min
Delta R.T.: 0.056 min
Response: 438111
Conc: 1.94 ng/ml

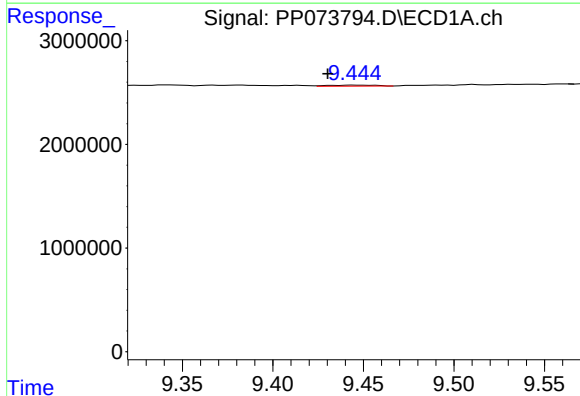


#44 AR-1268-4

R.T.: 9.446 min
Delta R.T.: 0.015 min
Response: 194024
Conc: 2.79 ng/ml

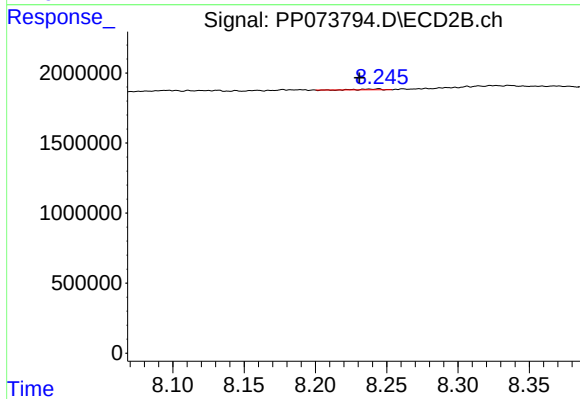

#44 AR-1268-4


R.T.: 8.244 min
Delta R.T.: 0.013 min
Response: 41416
Conc: 0.45 ng/ml

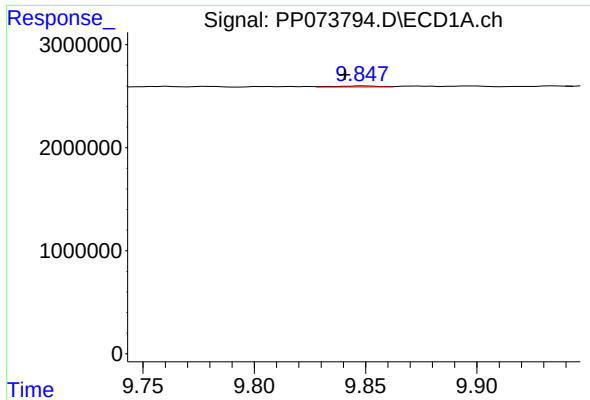

#45 AR-1268-5

R.T.: 9.849 min
Delta R.T.: 0.009 min
Response: 130893
Conc: 0.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

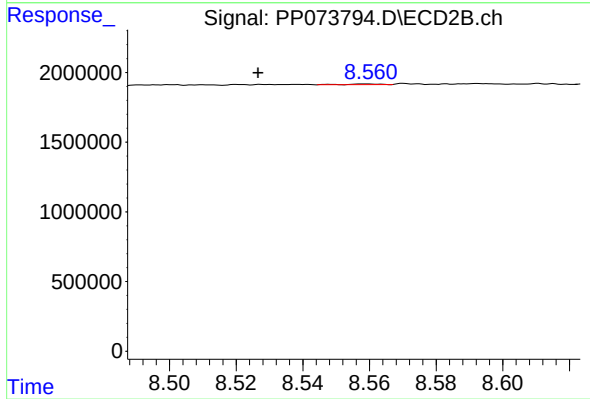

#45 AR-1268-5

R.T.: 8.559 min
Delta R.T.: 0.032 min
Response: 29683
Conc: 0.05 ng/ml