

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071525\
 Data File : PP073813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2025 18:35
 Operator : YP\AJ
 Sample : Q2507-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SU-04-7.3-2025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/16/2025
 Supervised By :mohammad ahmed 07/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:50:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 08 08:35:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.778	23368446	29086325	17.063	15.788
2) SA Decachlor...	10.170	8.776	16930465	21218020	15.518m	16.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP071525\
Data File : PP073813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2025 18:35
Operator : YP\AJ
Sample : Q2507-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SU-04-7.3-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/16/2025
Supervised By :mohammad ahmed 07/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:50:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 08 08:35:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

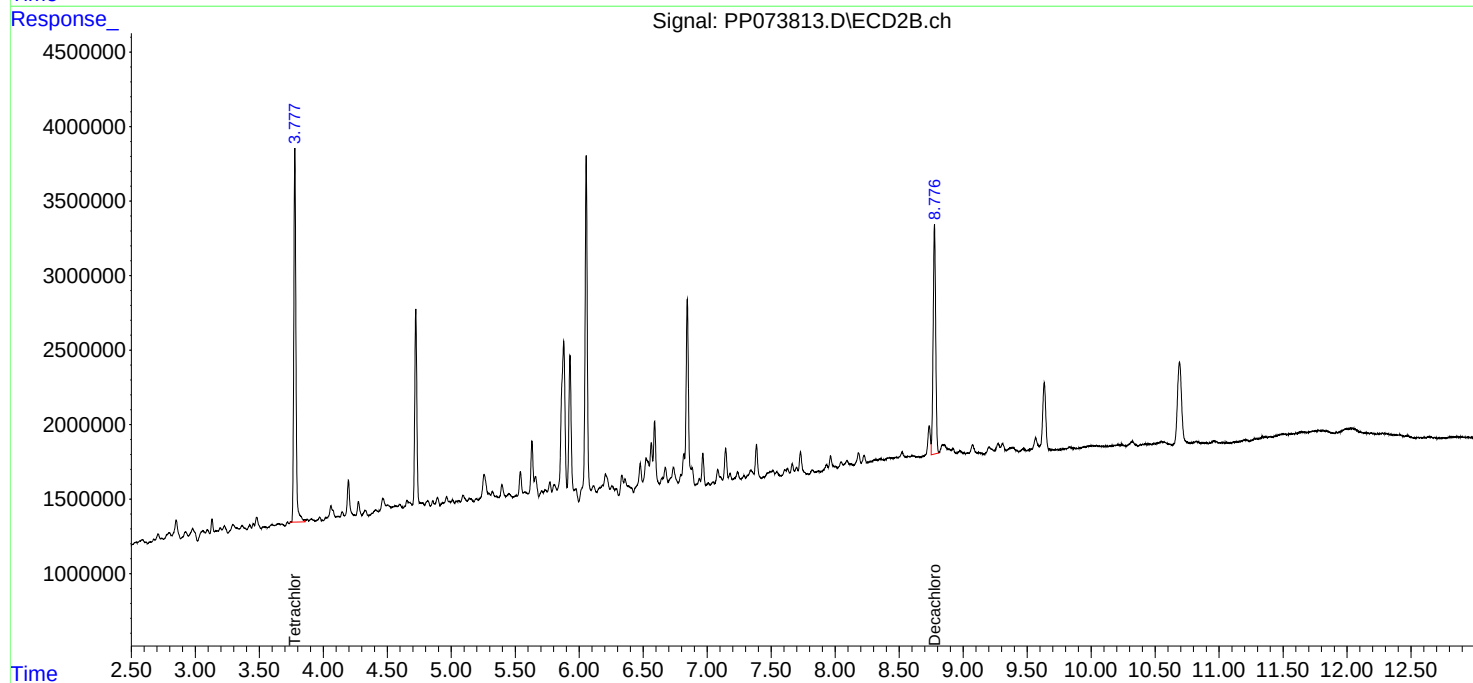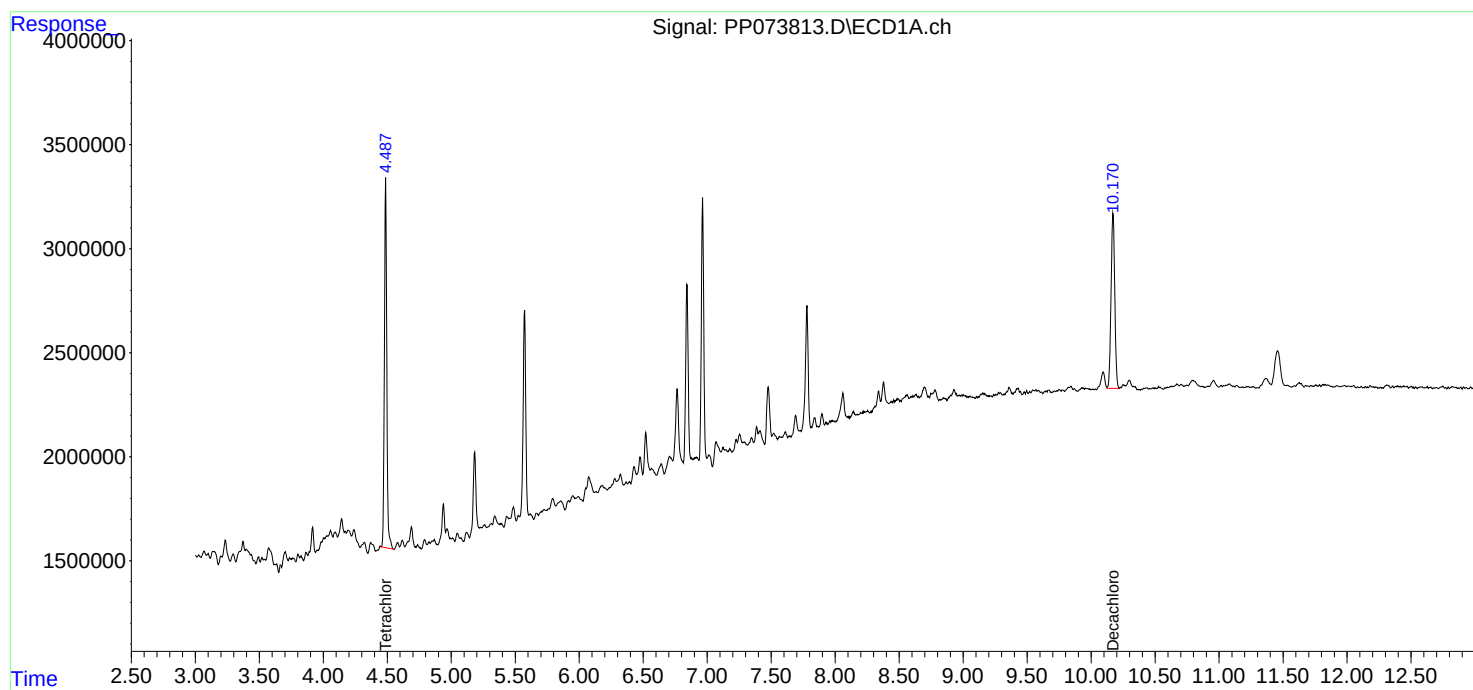

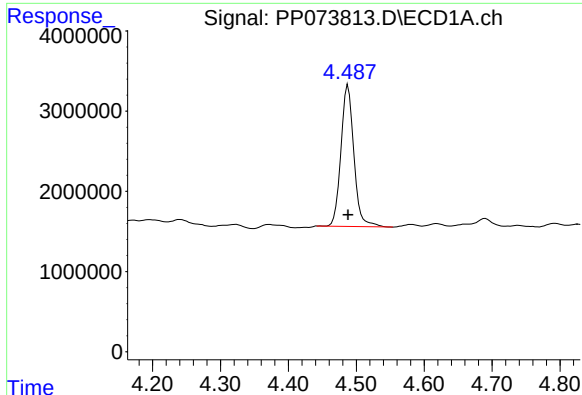


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 23368446
Conc: 17.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
SU-04-7.3-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/16/2025
Supervised By :mohammad ahmed 07/19/2025

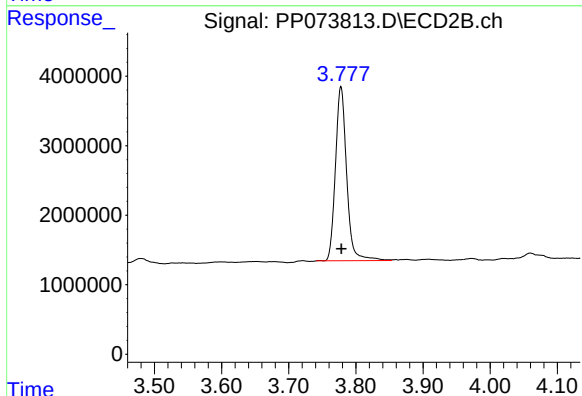


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: 0.000 min
Response: 29086325
Conc: 15.79 ng/ml

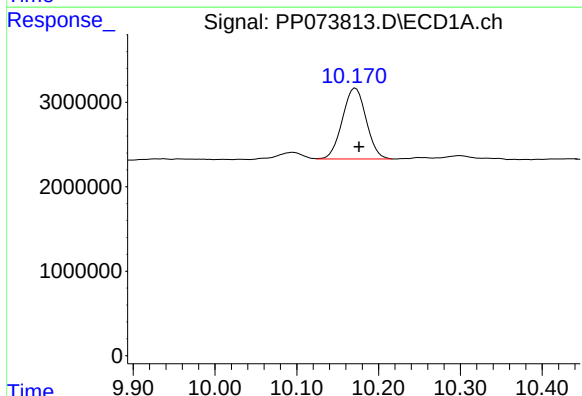

#2 Decachlorobiphenyl

R.T.: 10.170 min
Delta R.T.: -0.006 min
Response: 16930465
Conc: 15.52 ng/ml m

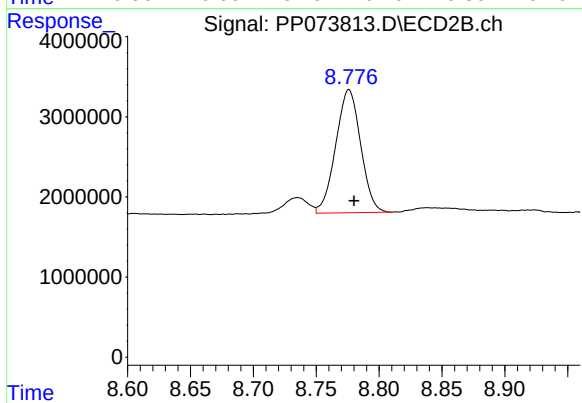

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: -0.004 min
Response: 21218020
Conc: 16.04 ng/ml